

January 13, 2017

Mr. Greg J. Lyssy
U.S. EPA, Region 6
1445 Ross Avenue (6SF-LT)
Dallas, TX 75202-2733

Subject: December 2016 Results of PFAS Sampling at Camp Stanley Storage Activity, Boerne, Texas
EPA Identification Number: TXD2210020739, US EPA Docket Number: RCRA-VI 002(h)99-H FY99

Dear Mr. Lyssy,

In December 2016, Camp Stanley Storage Activity (CSSA) collected groundwater samples from three on-post public water supply wells (CS-1, CS-10, CS-12) for analysis of Perfluoroalkyl Substances (PFAS). The results of these analyses have been received and validated by our Parsons chemists. We have prepared the enclosed CD with the following information for your review:

- EPA Lifetime Health Advisory Fact Sheet (recommends total PFAS concentration less than 70 parts per trillion [ppt]);
- Results Summary Table with comparisons to the EPA Health Advisory Level, and the Texas Risk Reduction Program (TRRP) Groundwater Protective Concentration Levels (PCLs) for Residential Groundwater;
- Data Validation Report; and
- Level 4 Analytical Package.

Three drinking water well samples, one duplicate sample (from CS-1), one trip blank, and one field blank were collected on December 6, 2016. None of the results exceeded either the TRRP Residential Groundwater PCLs or the EPA Health Advisory level:

- CS-1, CS-41 (CS-1 Duplicate), CS-12, and TB-1 had no PFAS detections, with the exception of low levels of PFTeA (M- and F-flagged). The validation report considers this a lab contaminant, since it was also associated with a method blank.
- CS-10 had detections of seven PFAS compounds (five of which are F-flagged). None of the individual concentrations exceeded TRRP Residential Groundwater PCLs. The PFAS total in this well is 31.16 ppt, which is significantly lower than the EPA Advisory Level of 70 ppt.
- The field blank (FB-1) had no PFAS detections.

We look forward to reviewing these results in further detail at our upcoming meeting with you in February 2017. In the meantime, if you have any specific questions please do not hesitate to contact me at 512.719.6087.

Sincerely,



W. Scott Pearson, P.G.

Enclosure

cc: Ms. Felicia Kraintz, CSSA Environmental Manager
Ms. Julie Burdey, Parsons
Ms. Brenda Shirley, Parsons

Overview

EPA has established health advisories for PFOA and PFOS based on the agency's assessment of the latest peer-reviewed science to provide drinking water system operators, and state, tribal and local officials who have the primary responsibility for overseeing these systems, with information on the health risks of these chemicals, so they can take the appropriate actions to protect their residents. EPA is committed to supporting states and public water systems as they determine the appropriate steps to reduce exposure to PFOA and PFOS in drinking water. As science on health effects of these chemicals evolves, EPA will continue to evaluate new evidence.

Background on PFOA and PFOS

PFOA and PFOS are fluorinated organic chemicals that are part of a larger group of chemicals referred to as perfluoroalkyl substances (PFASs). PFOA and PFOS have been the most extensively produced and studied of these chemicals. They have been used to make carpets, clothing, fabrics for furniture, paper packaging for food and other materials (e.g., cookware) that are resistant to water, grease or stains. They are also used for firefighting at airfields and in a number of industrial processes.

Because these chemicals have been used in an array of consumer products, most people have been exposed to them. Between 2000 and 2002, PFOS was voluntarily phased out of production in the U.S. by its primary manufacturer. In 2006, eight major companies voluntarily agreed to phase out their global production of PFOA and PFOA-related chemicals, although there are a limited number of ongoing uses. Scientists have found PFOA and PFOS in the blood of nearly all the people they tested, but these studies show that the levels of PFOA and PFOS in blood have been decreasing. While consumer products and food are a large source of exposure to these chemicals for most people, drinking water can be an additional source in the small percentage of communities where these chemicals have contaminated water supplies. Such contamination is typically localized and associated with a specific facility, for example, an industrial facility where these chemicals were produced or used to manufacture other products or an airfield at which they were used for firefighting.

EPA's 2016 Lifetime Health Advisories

EPA develops health advisories to provide information on contaminants that can cause human health effects and are known or anticipated to occur in drinking water. EPA's health advisories are non-enforceable and non-regulatory and provide technical information to states agencies and other public health officials on health effects, analytical methodologies, and treatment technologies associated with drinking water contamination. In 2009, EPA published provisional health advisories for PFOA and PFOS based on the evidence available at that time. The science has evolved since then and EPA is now replacing the 2009 provisional advisories with new, lifetime health advisories.

FACT SHEET

PFOA & PFOS Drinking Water Health Advisories

EPA's 2016 Lifetime Health Advisories, continued

To provide Americans, including the most sensitive populations, with a margin of protection from a lifetime of exposure to PFOA and PFOS from drinking water, EPA established the health advisory levels at 70 parts per trillion. When both PFOA and PFOS are found in drinking water, the combined concentrations of PFOA and PFOS should be compared with the 70 parts per trillion health advisory level. This health advisory level offers a margin of protection for all Americans throughout their life from adverse health effects resulting from exposure to PFOA and PFOS in drinking water.

How the Health Advisories were developed

EPA's health advisories are based on the best available peer-reviewed studies of the effects of PFOA and PFOS on laboratory animals (rats and mice) and were also informed by epidemiological studies of human populations that have been exposed to PFASs. These studies indicate that exposure to PFOA and PFOS over certain levels may result in adverse health effects, including developmental effects to fetuses during pregnancy or to breastfed infants (e.g., low birth weight, accelerated puberty, skeletal variations), cancer (e.g., testicular, kidney), liver effects (e.g., tissue damage), immune effects (e.g., antibody production and immunity), thyroid effects and other effects (e.g., cholesterol changes).

EPA's health advisory levels were calculated to offer a margin of protection against adverse health effects to the most sensitive populations: fetuses during pregnancy and breastfed infants. The health advisory levels are calculated based on the drinking water intake of lactating women, who drink more water than other people and can pass these chemicals along to nursing infants through breastmilk.

Recommended Actions for Drinking Water Systems

Steps to Assess Contamination

If water sampling results confirm that drinking water contains PFOA and PFOS at individual or combined concentrations greater than 70 parts per trillion, water systems should quickly undertake additional sampling to assess the level, scope and localized source of contamination to inform next steps

Steps to Inform

If water sampling results confirm that drinking water contains PFOA and PFOS at individual or combined concentrations greater than 70 parts per trillion, water systems should promptly notify their State drinking water safety agency (or with EPA in jurisdictions for which EPA is the primary drinking water safety agency) and consult with the relevant agency on the best approach to conduct additional sampling.

Drinking water systems and public health officials should also promptly provide consumers with information about the levels of PFOA and PFOS in their drinking water. This notice should include specific information on the risks to fetuses during pregnancy and breastfed and formula-fed infants from exposure to drinking water with an individual or combined concentration of PFOA and PFOS above EPA's health advisory level of 70 parts per trillion. In addition, the notification should include actions they are taking and identify options that consumers may consider to reduce risk such as seeking an alternative drinking water source, or in the case of parents of formula-fed infants, using formula that does not require adding water.

FACT SHEET

PFOA & PFOS Drinking Water Health Advisories

Recommended Actions for Drinking Water Systems, continued

Steps to Limit Exposure

A number of options are available to drinking water systems to lower concentrations of PFOA and PFOS in their drinking water supply. In some cases, drinking water systems can reduce concentrations of perfluoroalkyl substances, including PFOA and PFOS, by closing contaminated wells or changing rates of blending of water sources. Alternatively, public water systems can treat source water with activated carbon or high pressure membrane systems (e.g., reverse osmosis) to remove PFOA and PFOS from drinking water. These treatment systems are used by some public water systems today, but should be carefully designed and maintained to ensure that they are effective for treating PFOA and PFOS. In some communities, entities have provided bottled water to consumers while steps to reduce or remove PFOA or PFOS from drinking water or to establish a new water supply are completed.

Many home drinking water treatment units are certified by independent accredited third party organizations against American National Standards Institute (ANSI) standards to verify their contaminant removal claims. NSF International (NSF®) has developed a protocol for NSF/ANSI Standards 53 and 58 that establishes minimum requirements for materials, design and construction, and performance of point-of-use (POU) activated carbon drinking water treatment systems and reverse osmosis systems that are designed to reduce PFOA and PFOS in public water supplies. The protocol has been established to certify systems (e.g., home treatment systems) that meet the minimum requirements. The systems are evaluated for contaminant reduction by challenging them with an influent of $1.5 \pm 30\%$ $\mu\text{g}/\text{L}$ (total of both PFOA and PFOS) and must reduce this concentration by more than 95% to $0.07 \mu\text{g}/\text{L}$ or less (total of both PFOA and PFOS) throughout the manufacturer's stated life of the treatment system. Product certification to this protocol for testing home treatment systems verifies that devices effectively reduces PFOA and PFOS to acceptable levels.

Other Actions Relating to PFOA and PFOS

Between 2000 and 2002, PFOS was voluntarily phased out of production in the U.S. by its primary manufacturer, 3M. EPA also issued regulations to limit future manufacturing, including importation, of PFOS and its precursors, without first having EPA review the new use. A limited set of existing uses for PFOS (fire resistant aviation hydraulic fluids, photography and film products, photomicro lithography process to produce semiconductors, metal finishing and plating baths, component of an etchant) was excluded from these regulations because these uses were ongoing and alternatives were not available.

In 2006, EPA asked eight major companies to commit to working toward the elimination of their production and use of PFOA, and chemicals that degrade to PFOA, from emissions and products by the end of 2015. All eight companies have indicated that they have phased out PFOA, and chemicals that degrade to PFOA, from emissions and products by the end of 2015. Additionally, PFOA is included in EPA's proposed Toxic Substance Control Act's Significant New Use Rule (SNUR) issued in January 2015 which will ensure that EPA has an opportunity to review any efforts to reintroduce the chemical into the marketplace and take action, as necessary, to address potential concerns.

FACT SHEET

PFOA & PFOS Drinking Water Health Advisories

Other Actions Relating to PFOA and PFOS, continued

EPA has not established national primary drinking water regulations for PFOA and PFOS. EPA is evaluating PFOA and PFOS as drinking water contaminants in accordance with the process required by the Safe Drinking Water Act (SDWA). To regulate a contaminant under SDWA, EPA must find that it: (1) may have adverse health effects; (2) occurs frequently (or there is a substantial likelihood that it occurs frequently) at levels of public health concern; and (3) there is a meaningful opportunity for health risk reduction for people served by public water systems.

EPA included PFOA and PFOS among the list of contaminants that water systems are required to monitor under the third Unregulated Contaminant Monitoring Rule (UCMR 3) in 2012. Results of this monitoring effort are updated regularly and can be found on the publicly-available National Contaminant Occurrence Database (NCOD) (<https://www.epa.gov/dwucmr/occurrence-data-unregulated-contaminant-monitoring-rule#3>). In accordance with SDWA, EPA will consider the occurrence data from UCMR 3, along with the peer reviewed health effects assessments supporting the PFOA and PFOS Health Advisories, to make a regulatory determination on whether to initiate the process to develop a national primary drinking water regulation.

In addition, EPA plans to begin a separate effort to determine the range of PFAS for which an Integrated Risk Information System (IRIS) assessment is needed. The IRIS Program identifies and characterizes the health hazards of chemicals found in the environment. IRIS assessments inform the first two steps of the risk assessment process: hazard identification, and dose-response. As indicated in the 2015 IRIS Multi-Year Agenda, the IRIS Program will be working with other EPA offices to determine the range of PFAS compounds and the scope of assessment required to best meet Agency needs. More about this effort can be found at <https://www.epa.gov/iris/iris-agenda>.

Non-Drinking Water Exposure to PFOA and PFOS

These health advisories only apply to exposure scenarios involving drinking water. They are not appropriate for use, in identifying risk levels for ingestion of food sources, including: fish, meat produced from livestock that consumes contaminated water, or crops irrigated with contaminated water.

The health advisories are based on exposure from drinking water ingestion, not from skin contact or breathing. The advisory values are calculated based on drinking water consumption and household use of drinking water during food preparation (e.g., cooking or to prepare coffee, tea or soup). To develop the advisories, EPA considered non-drinking water sources of exposure to PFOA and PFOS, including: air, food, dust, and consumer products. In January 2016 the Food and Drug Administration amended its regulations to no longer allow PFOA and PFOS to be added in food packaging, which will likely decrease one source of non-drinking water exposure.

Where Can I Learn More?

- EPA's Drinking Water Health Advisories for PFOA and PFOS can be found at: <https://www.epa.gov/ground-water-and-drinking-water/drinking-water-health-advisories-pfoa-and-pfos>
- PFOA and PFOS data collected under EPA's Unregulated Contaminant Monitoring Rule are available: <https://www.epa.gov/dwucmr/occurrence-data-unregulated-contaminant-monitoring-rule>
- EPA's stewardship program for PFAS related to TSCA: <https://www.epa.gov/assessing-and-managing-chemicals-under-tsca/and-polyfluoroalkyl-substances-pfas-under-tsca>
- EPA's research activities on PFASs can be found at: <http://www.epa.gov/chemical-research/perfluorinated-chemical-pfc-research>
- The Agency for Toxic Substances and Disease Registry's Perfluorinated Chemicals and Your Health webpage at: <http://www.atsdr.cdc.gov/PFC/>



Camp Stanley Storage Activity
Polyfluoroalkyl Substances (PFAS) Sampling
Validated Results for Samples Collected December 6, 2016

SAMPLE ID:			TRRP GW _{ing} PCL [1]	EPA Lifetime Health Advisory Level[2]	CS-1		CS-41 (DUP of CS-1)		CS-10		CS-12		TB-1		FB-1	
DATE SAMPLED:					12/6/2016		12/6/2016		12/6/2016		12/6/2016		12/6/2016		12/6/2016	
LAB SAMPLE ID:					320-24118-6		320-24118-4		320-24118-3		320-24118-5		320-24118-1		320-24118-2	
Perfluorinated Hydrocarbons - E537M		CAS #	Units													
Perfluorobutanesulfonic acid (PFBS)	375-73-5	ng/L	34000		0.92	U	0.93	U	1.3	F	0.88	U	0.94	U	0.88	U
Perfluorobutanoic acid (PFBA)	375-22-4	ng/L	71000		0.46	U	0.46	U	0.51	F	0.44	U	0.47	U	0.44	U
Perfluorodecanesulfonic acid (PFDS)	335-77-3	ng/L	290		1.2	U	1.2	U	1.2	U	1.2	U	1.2	U	1.2	U
Perfluorodecanoic acid (PFDA)	335-76-2	ng/L	370		0.44	U	0.45	U	0.42	U	0.42	U	0.45	U	0.42	U
Perfluorododecanoic acid (PFDoA)	307-55-1	ng/L	290		0.58	U	0.59	U	0.56	U	0.56	U	0.60	U	0.56	U
Perfluoroheptanoic acid (PFHpA)	375-85-9	ng/L	560		0.80	U	0.81	U	0.77	U	0.77	U	0.82	U	0.77	U
Perfluorohexanesulfonic acid (PFHxS)	355-46-4	ng/L	93		0.87	U	0.88	U	10		0.83	U	0.89	U	0.83	U
Perfluorohexanoic acid (PFHxA)	307-24-4	ng/L	93		0.79	U	0.80	U	1.1	F	0.75	U	0.81	U	0.75	U
Perfluorononanoic acid (PFNA)	375-95-1	ng/L	290		0.65	U	0.66	U	0.63	U	0.63	U	0.67	U	0.63	U
Perfluorooctane Sulfonamide (FOSA)	754-91-6	ng/L	290		0.64	U	0.65	U	0.61	U	0.61	U	0.65	U	0.61	U
Perfluorooctanesulfonic acid (PFOS)	1763-23-1	ng/L	560		1.3	U	1.3	U	17		1.2	U	1.3	U	1.2	U
Perfluorooctanoic acid (PFOA)	335-67-1	ng/L	290		0.75	U	0.76	U	0.72	F	0.71	U	0.77	U	0.72	U
Perfluoropentanoic acid (PFPeA)	2706-90-3	ng/L	93		0.99	U	1.0	U	0.95	U	0.95	U	1.0	U	0.95	U
Perfluorotetradecanoic acid (PFTeA)	376-06-7	ng/L	290		0.75	M	0.51	M	0.53	F	0.72	F	0.54	F	0.38	U
Perfluorotridecanoic acid (PFTriA)	72629-94-8	ng/L	290		0.55	U	0.56	U	0.53	U	0.53	U	0.57	U	0.53	U
Perfluoroundecanoic acid (PFUnA)	2058-94-8	ng/L	290		0.75	U	0.76	U	0.72	U	0.71	U	0.77	U	0.72	U
Total Perfluorinated Hydrocarbons	--	ng/L		70	0.75		0.51		31.16		0.72		0.54		ND	

QA NOTES AND DATA QUALIFIERS:

(NU CODE) - Confirmed identification.

U - Analyte was not detected above the indicated Method Detection Limit (MDL).

F - Analyte was positively identified, but the quantitation is an estimation above the MDL and below the Reporting Limit (RL).

M - Concentration is estimated due to a matrix effect.

Detections are bolded.

ng/L - nanograms per liter.

ND - Not Detected.

NOTES:

[1] Residential Groundwater^{GW} PCL, TRRP Tier 1 Groundwater PCLs - Residential and Commercial/Industrial, March 4, 2016.

[2] USEPA Lifetime Health Advisory Level from the *EPA FACT SHEET PFOA & PFOS Drinking Water Health Advisories - November 2016 (EPA 800-F-16-003)*. To provide Americans, including the most sensitive populations, with a margin of protection from a life-time of exposure to PFOA and PFOS from drinking water, EPA established the health advisory levels at 70 parts per trillion (e.g., nanograms per liter [ng/L]). When both PFOA and PFOS are found in drinking water, the combined concentrations of PFOA and PFOS should be compared with the 70 parts per trillion health advisory level. This health advisory level offers a margin of protection for all Americans throughout their life from adverse health effects resulting from exposure to PFOA and PFOS in drinking water.

DATA VERIFICATION SUMMARY REPORT

for on-post samples collected from CAMP STANLEY STORAGE ACTIVITY

BOERNE, TEXAS

Data Verification by: Tammy Chang
Parsons - Austin

INTRODUCTION

The following data verification summary report covers three (3) groundwater samples and the associated field quality control (QC) samples collected from Camp Stanley Storage Activity (CSSA) on December 6th, 2016. The samples were assigned to the following Sample Delivery Group (SDG). All samples were analyzed for Texas Commission on Environmental Quality (TCEQ) listed 16 Perfluorinated Compounds (PFCs):

320-24118-1

The field QC samples associated with this SDG were one trip blank (TB) sample, one field blank (FB) sample, one set of parent/field duplicate (FD) samples, and one set of matrix spike/matrix spike duplicate (MS/MSD) samples.

All samples were collected by Parsons and analyzed by TestAmerica Laboratories, Inc. in West Sacramento, CA. following the procedures outlined in the Statement of Work, Department of Defense (DoD) Quality System Manual (QSM) version 5.0 and laboratory SOP No. WS-LC-0025, Rev. 1.9 issued on May 27, 2016 which has been approved by Department of Defense under the Environmental Laboratory Accreditation Program (ELAP) and US Environmental Protection Agency (EPA). Samples in this SDG were shipped to the laboratory in one cooler. Cooler was received by the laboratory at a temperature of 0.5°C, which was slightly below the 2-6°C range recommended by the CSSA QAPP.

EVALUATION CRITERIA

The data submitted by the laboratory has been reviewed and verified following the guidelines outlined in the CSSA QAPP, Version 1.0. Information reviewed in the data package included sample results; field and laboratory quality control samples; calibrations; case narratives; raw data; chain-of-custody (COC) forms, internal data package checklist, and the sample receipt checklist. The findings presented in this report are based on the reviewed information, and whether the procedures and technical requirements described in the lab SOP were followed and met. The Limits of Quantitation (LOQs) listed in the lab report equal to the Reporting Limits (RLs), Version 1.0 and the Detection Limits (DLs) listed in the lab report equal to Method Detection Limits (MDLs) in the CSSA QAPP.

All value between the LOQ and DL were flagged with “J” by lab and changed to “F” by Parsons date validator in order to keep the consistency of flagging in the CSSA database. All non-detects are associated with the MDL values.

PFCs

General

This data package consisted of three (3) groundwater samples, one (1) TB, one (1) FB, one (1) FD, and one (1) set of MS/MSD. All samples were collected on December 6, 2016 and analyzed for a TCEQ specified list of PFCs which included:

- Perfluorobutanoic acid (PFBA)
- Perfluoropentanoic acid (PFPeA)
- Perfluorohexanoic acid (PFHxA)
- Perfluoroheptanoic acid (PFHpA)
- Perfluorooctanoic acid (PFOA)
- Perfluorononanoic acid (PFNA)
- Perfluorodecanoic acid (PFDA)
- Perfluoroundecanoic acid (PFUnA)
- Perfluorododecanoic acid (PFDoA)
- Perfluorotridecanoic acid (PFTriA)
- Perfluorotetradecanoic acid (PFTeA)
- Perfluorobuanesulfonic acid (PFBS)
- Perfluorohexanesulfonic acid (PFHxS)
- Perfluorooctanesulfonic acid (PFOS)
- Perfluorodecanesulfonic acid (PFDS)
- Perfluorooctane Sulfonamide (FOSA)

The PFC analyses were performed using lab SOP which was modified from United States Environmental Protection Agency (USEPA) Method 537. The samples were analyzed in one preparation batch #142235 and one analysis batch #142379 under one initial calibration curve (ICAL) with the same instrument. All samples were analyzed following the procedures outlined in the lab SOP and were prepared and analyzed within the holding time required by the method. All analyses were performed undiluted.

Accuracy

Accuracy was evaluated using the percent recovery (%R) obtained from the laboratory control spike (LCS) sample, MS/MSD, and the surrogate spikes which were added to the sample as Isotope Dilution Compounds. Sample CS-1 was designated as the parent sample for the MS/MSD analyses.

The LCS has recoveries within the acceptance criteria.

For the surrogate, 13C8 PFTeA was recovered in all samples. Since the signal-to-noise ratio was greater than 10:1 for this surrogate in all samples, data quality was not affected. No flags were required.

The MS/MSD recoveries for Perfluorotetradecanoic acid (PFTeA) were outside control limits. The parent sample CS-1 and CS-41, field duplicate of CS-1 were flagged "M" for Perfluorotetradecanoic acid (PFTeA).

Precision

Precision was evaluated based on the relative percent difference (%RPD) of the parent and FD results, also with the MS/MSD results. Sample CS-41 is the FD of sample CS-1.

All %RPDs of the MS/MSD were compliant.

Since none of the target PFCs were detected above the reporting limits, the %RPD calculation was not-applicable.

Representativeness

Representativeness expresses the degree to which sample data accurately and precisely represents actual site conditions. Representativeness has been evaluated by:

- Comparing the COC procedures to those described in the CSSA QAPP;
- Comparing actual analytical procedures to those described in the lab SOP;
- Evaluating holding times; and
- Examining laboratory blank, field blank, and trip blank for cross contamination of samples during sample collection, cooler transportation and sample analysis.

All samples in this data package were analyzed following the COC and the analytical procedures described in the lab SOP. All samples were prepared and analyzed within the holding time (14 days) required by the method.

- All instrument performance check criteria were met.
- All initial calibration criteria were met for both sets of curves.
- All initial calibration verification (ICV) criteria were met. The ICV was prepared using a secondary source standard. All second source verification criteria were met.
- All continuing calibration verification (CCV) criteria were met.

There was one method blank associated with the PFC analyses in this SDG. PFTeA was detected <1/2 of RL in the method blank. This compound was also detected with similar concentration in all samples. It is considered as lab contaminant.

Completeness

Completeness has been evaluated in accordance with the CSSA QAPP. The number of usable results has been divided by the number of possible individual analyte results and expressed as a percentage to determine the completeness of the data set.

All PFC results for the samples in this SDG were considered usable. The completeness for this SDG is 100%, which meets the minimum acceptance criteria of 95%.

ANALYTICAL REPORT

Job Number: 320-24118-1

Job Description: Camp Stanley

For:

Parsons Corporation
8000 Centre Park Drive
Suite 200
Austin, TX 78754

Attention: Ms. Tammy Chang



Approved for release.
Linda C. Laver
Project Manager II
12/19/2016 12:09 PM

Linda C. Laver, Project Manager II
880 Riverside Parkway, West Sacramento, CA, 95605
(916)374-4362
linda.laver@testamericainc.com
12/19/2016

Table of Contents

Cover Title Page	1
Data Summaries	4
Definitions	4
Case Narrative	5
Detection Summary	7
Client Sample Results	8
Default Detection Limits	13
Isotope Dilution Summary	14
QC Sample Results	15
QC Association	19
Chronicle	20
Certification Summary	22
Method Summary	23
Sample Summary	24
Manual Integration Summary	25
Reagent Traceability	27
COAs	58
Organic Sample Data	388
LCMS	388
Method PFC DOD	388
Method PFC DOD QC Summary	389
Method PFC DOD Sample Data	395
Standards Data	446
Method PFC DOD ICAL Data	446
Method PFC DOD CCAL Data	531
Raw QC Data	571

Table of Contents

Method PFC DOD Blank Data	571
Method PFC DOD LCS/LCSD Data	580
Method PFC DOD MS/MSD Data	590
Method PFC DOD Run Logs	610
Method PFC DOD Prep Data	613
Shipping and Receiving Documents	624
Client Chain of Custody	625
Sample Receipt Checklist	626

Definitions/Glossary

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

Qualifiers

LCMS

Qualifier	Qualifier Description
Q	One or more quality control criteria failed.
U	Undetected at the Limit of Detection.
M	Manual integrated compound.
J	Estimated: The analyte was positively identified; the quantitation is an estimation
J	Estimated: The quantitation is an estimation due to discrepancies in meeting certain analyte-specific quality control criteria.

Glossary

Abbreviation	These commonly used abbreviations may or may not be present in this report.
α	Listed under the "D" column to designate that the result is reported on a dry weight basis
%R	Percent Recovery
CFL	Contains Free Liquid
CNF	Contains no Free Liquid
DER	Duplicate error ratio (normalized absolute difference)
Dil Fac	Dilution Factor
DL, RA, RE, IN	Indicates a Dilution, Re-analysis, Re-extraction, or additional Initial metals/anion analysis of the sample
DLC	Decision level concentration
MDA	Minimum detectable activity
EDL	Estimated Detection Limit
MDC	Minimum detectable concentration
MDL	Method Detection Limit
ML	Minimum Level (Dioxin)
NC	Not Calculated
ND	Not detected at the reporting limit (or MDL or EDL if shown)
PQL	Practical Quantitation Limit
QC	Quality Control
RER	Relative error ratio
RL	Reporting Limit or Requested Limit (Radiochemistry)
RPD	Relative Percent Difference, a measure of the relative difference between two points
TEF	Toxicity Equivalent Factor (Dioxin)
TEQ	Toxicity Equivalent Quotient (Dioxin)

CASE NARRATIVE
Client: Parsons Corporation
Project: Camp Stanley
Report Number: 320-24118-1

With the exceptions noted as flags or footnotes, standard analytical protocols were followed in the analysis of the samples and no problems were encountered or anomalies observed. In addition all laboratory quality control samples were within established control limits, with any exceptions noted below. Each sample was analyzed to achieve the lowest possible reporting limit within the constraints of the method. In some cases, due to interference or analytes present at high concentrations, samples were diluted. For diluted samples, the reporting limits are adjusted relative to the dilution required.

TestAmerica Sacramento attests to the validity of the laboratory data generated by TestAmerica facilities reported herein. All analyses performed by TestAmerica facilities were done using established laboratory SOPs that incorporate QA/QC procedures described in the applicable methods. TestAmerica's operations groups have reviewed the data for compliance with the laboratory QA/QC plan, and data have been found to be compliant with laboratory protocols unless otherwise noted below.

TestAmerica utilizes USEPA approved methods and DOD QSM, where applicable, in all analytical work. The samples presented in this report were analyzed for the parameter(s) listed on the analytical methods summary page in accordance with the method(s) indicated. A summary of QC data for these analyses is included at the back of the report.

All parameters for which TestAmerica Sacramento has certification were evaluated to the QSM specified reporting convention or to the client specified format if different from QSM. Parameters not certified under QSM, if any, were evaluated to the detection limit (DL) and include qualified results where applicable.

The sample(s) that contain constituents flagged with U are undetected when evaluated down to the detection limit (DL). The result associated with this flag is the limit of detection (LOD).

Calculations are performed before rounding to avoid round-off errors in calculated results.

All holding times were met and proper preservation noted for the methods performed on these samples, unless otherwise detailed in the individual sections below.

This laboratory report is confidential and is intended for the sole use of TestAmerica and its client.

LOQ = Limit of Quantitation (Reporting Limit)
LOD = Limit of Detection
DL = Detection Limit (Method Detection Limit)

Receipt

The samples were received on 12/7/2016 10:30 AM; the samples arrived in good condition, properly preserved and, where required, on ice. The temperature of the cooler at receipt was 0.2° C.

LCMS

Method(s) 537 (Modified): The first level standard from the initial calibration curve is used to evaluate the tune criteria. The instrument mass windows are set at +/- 0.5amu; therefore, detection of the analyte serves as verification that the assigned mass is within +/- 0.5amu of the true value, which meets the DoD/DOE QSM tune criterion.

Method(s) 537 (Modified): The Isotope Dilution Analyte (IDA) recovery for 13C8 FOSA in the following samples is below the method recommended limit: TB-1 (320-24118-1), CS-10 (320-24118-3), CS-41 (320-24118-4), CS-12 (320-24118-5), CS-1 (320-24118-6), CS-1 (320-24118-6[MS]), CS-1 (320-24118-6[MSD]) and (LCS 320-142235/2-A). Generally, data quality is not considered affected if the IDA signal-to-noise ratio is greater than 10:1, which is achieved for all IDA in the samples.

Method(s) 537 (Modified): Isotope Dilution Analyte (IDA) recoveries for 13C2 PFDA and 13C2 PFUnA are above the method recommended limit for the following sample: TB-1 (320-24118-1). Quantitation by isotope dilution generally precludes any adverse effect on data quality due to elevated IDA recoveries.

Method(s) 537 (Modified): Perfluorotetradecanoic acid (PFTeA) was detected in method blank (MB 320-142235/1-A) at a level that was above the detection limit (DL) but less than 1/2 the limit of quantitation (LOQ). The value should be considered an estimate, and has been "J" flagged. If the associated sample reported a result above the MDL and/or RL, the result has been flagged. PER QSM protocol, further action was not required.

Method(s) 537 (Modified): The matrix spike/matrix spike duplicate (MS/MSD) recoveries for Perfluorotetradecanoic acid (PFTeA) in preparation batch 320-142235 and analytical batch 320-142379 were outside control limits. Sample matrix interference and/or non-homogeneity are suspected because the associated laboratory control sample (LCS) recovery was within acceptance limits.

No additional analytical or quality issues were noted, other than those described above or in the Definitions/Glossary page.

Organic Prep

No analytical or quality issues were noted, other than those described in the Definitions/Glossary page.

Detection Summary

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

Client Sample ID: TB-1

Lab Sample ID: 320-24118-1

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorotetradecanoic acid (PFTeA)	0.54	J	2.6	0.41	ng/L	1		537 (Modified)	Total/NA

Client Sample ID: FB-1

Lab Sample ID: 320-24118-2

No Detections.

Client Sample ID: CS-10

Lab Sample ID: 320-24118-3

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorobutanoic acid (PFBA)	0.51	J	2.4	0.44	ng/L	1		537 (Modified)	Total/NA
Perfluorohexanoic acid (PFHxA)	1.1	J	2.4	0.76	ng/L	1		537 (Modified)	Total/NA
Perfluorooctanoic acid (PFOA)	0.72	J	2.4	0.72	ng/L	1		537 (Modified)	Total/NA
Perfluorotetradecanoic acid (PFTeA)	0.53	J	2.4	0.39	ng/L	1		537 (Modified)	Total/NA
Perfluorobutanesulfonic acid (PFBS)	1.3	J M	2.4	0.88	ng/L	1		537 (Modified)	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	10		2.4	0.84	ng/L	1		537 (Modified)	Total/NA
Perfluorooctanesulfonic acid (PFOS)	17		3.9	1.2	ng/L	1		537 (Modified)	Total/NA

Client Sample ID: CS-41

Lab Sample ID: 320-24118-4

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorotetradecanoic acid (PFTeA)	0.51	J	2.5	0.41	ng/L	1		537 (Modified)	Total/NA

Client Sample ID: CS-12

Lab Sample ID: 320-24118-5

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorotetradecanoic acid (PFTeA)	0.72	J	2.4	0.38	ng/L	1		537 (Modified)	Total/NA

Client Sample ID: CS-1

Lab Sample ID: 320-24118-6

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorotetradecanoic acid (PFTeA)	0.75	J	2.5	0.40	ng/L	1		537 (Modified)	Total/NA

This Detection Summary does not include radiochemical test results.

Client Sample Results

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

Client Sample ID: TB-1
Date Collected: 12/06/16 08:00
Date Received: 12/07/16 10:30

Lab Sample ID: 320-24118-1
Matrix: Water

Method: 537 (Modified) - Perfluorinated Hydrocarbons

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorobutanoic acid (PFBA)	1.0	U	2.6	0.47	ng/L		12/14/16 18:18	12/15/16 16:39	1
Perfluoropentanoic acid (PFPeA)	2.1	U	2.6	1.0	ng/L		12/14/16 18:18	12/15/16 16:39	1
Perfluorohexanoic acid (PFHxA)	2.1	U M	2.6	0.81	ng/L		12/14/16 18:18	12/15/16 16:39	1
Perfluoroheptanoic acid (PFHpA)	2.1	U	2.6	0.82	ng/L		12/14/16 18:18	12/15/16 16:39	1
Perfluorooctanoic acid (PFOA)	2.1	U	2.6	0.77	ng/L		12/14/16 18:18	12/15/16 16:39	1
Perfluorononanoic acid (PFNA)	2.1	U	2.6	0.67	ng/L		12/14/16 18:18	12/15/16 16:39	1
Perfluorodecanoic acid (PFDA)	1.0	U	2.6	0.45	ng/L		12/14/16 18:18	12/15/16 16:39	1
Perfluoroundecanoic acid (PFUnA)	2.1	U	2.6	0.77	ng/L		12/14/16 18:18	12/15/16 16:39	1
Perfluorododecanoic acid (PFDoA)	2.1	U	2.6	0.60	ng/L		12/14/16 18:18	12/15/16 16:39	1
Perfluorotridecanoic Acid (PFTriA)	2.1	U	2.6	0.57	ng/L		12/14/16 18:18	12/15/16 16:39	1
Perfluorotetradecanoic acid (PFTeA)	0.54	J	2.6	0.41	ng/L		12/14/16 18:18	12/15/16 16:39	1
Perfluorobutanesulfonic acid (PFBS)	2.1	U	2.6	0.94	ng/L		12/14/16 18:18	12/15/16 16:39	1
Perfluorohexanesulfonic acid (PFHxS)	2.1	U	2.6	0.89	ng/L		12/14/16 18:18	12/15/16 16:39	1
Perfluorooctanesulfonic acid (PFOS)	3.1	U	4.1	1.3	ng/L		12/14/16 18:18	12/15/16 16:39	1
Perfluorodecanesulfonic acid (PFDS)	3.1	U	4.1	1.2	ng/L		12/14/16 18:18	12/15/16 16:39	1
Perfluorooctane Sulfonamide (FOSA)	2.1	U	2.6	0.65	ng/L		12/14/16 18:18	12/15/16 16:39	1

Isotope Dilution	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C8 FOSA	14	Q	25 - 150				12/14/16 18:18	12/15/16 16:39	1
13C4 PFBA	131		25 - 150				12/14/16 18:18	12/15/16 16:39	1
13C2 PFHxA	133		25 - 150				12/14/16 18:18	12/15/16 16:39	1
13C4 PFOA	145		25 - 150				12/14/16 18:18	12/15/16 16:39	1
13C5 PFNA	142		25 - 150				12/14/16 18:18	12/15/16 16:39	1
13C2 PFDA	151	Q	25 - 150				12/14/16 18:18	12/15/16 16:39	1
13C2 PFUnA	153	Q	25 - 150				12/14/16 18:18	12/15/16 16:39	1
13C2 PFDoA	148		25 - 150				12/14/16 18:18	12/15/16 16:39	1
18O2 PFHxS	125		25 - 150				12/14/16 18:18	12/15/16 16:39	1
13C4 PFOS	131		25 - 150				12/14/16 18:18	12/15/16 16:39	1
13C4-PFHpA	142		25 - 150				12/14/16 18:18	12/15/16 16:39	1
13C5 PFPeA	141		25 - 150				12/14/16 18:18	12/15/16 16:39	1

Client Sample ID: FB-1
Date Collected: 12/06/16 09:22
Date Received: 12/07/16 10:30

Lab Sample ID: 320-24118-2
Matrix: Water

Method: 537 (Modified) - Perfluorinated Hydrocarbons

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorobutanoic acid (PFBA)	0.96	U	2.4	0.44	ng/L		12/14/16 18:18	12/15/16 16:46	1
Perfluoropentanoic acid (PFPeA)	1.9	U	2.4	0.95	ng/L		12/14/16 18:18	12/15/16 16:46	1
Perfluorohexanoic acid (PFHxA)	1.9	U	2.4	0.75	ng/L		12/14/16 18:18	12/15/16 16:46	1
Perfluoroheptanoic acid (PFHpA)	1.9	U	2.4	0.77	ng/L		12/14/16 18:18	12/15/16 16:46	1
Perfluorooctanoic acid (PFOA)	1.9	U	2.4	0.72	ng/L		12/14/16 18:18	12/15/16 16:46	1
Perfluorononanoic acid (PFNA)	1.9	U	2.4	0.63	ng/L		12/14/16 18:18	12/15/16 16:46	1
Perfluorodecanoic acid (PFDA)	0.96	U	2.4	0.42	ng/L		12/14/16 18:18	12/15/16 16:46	1
Perfluoroundecanoic acid (PFUnA)	1.9	U	2.4	0.72	ng/L		12/14/16 18:18	12/15/16 16:46	1
Perfluorododecanoic acid (PFDoA)	1.9	U	2.4	0.56	ng/L		12/14/16 18:18	12/15/16 16:46	1
Perfluorotridecanoic Acid (PFTriA)	1.9	U	2.4	0.53	ng/L		12/14/16 18:18	12/15/16 16:46	1
Perfluorotetradecanoic acid (PFTeA)	0.96	U	2.4	0.38	ng/L		12/14/16 18:18	12/15/16 16:46	1
Perfluorobutanesulfonic acid (PFBS)	1.9	U	2.4	0.88	ng/L		12/14/16 18:18	12/15/16 16:46	1

Client Sample Results

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

Client Sample ID: FB-1
Date Collected: 12/06/16 09:22
Date Received: 12/07/16 10:30

Lab Sample ID: 320-24118-2
Matrix: Water

Method: 537 (Modified) - Perfluorinated Hydrocarbons (Continued)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorohexanesulfonic acid (PFHxS)	1.9	U M	2.4	0.83	ng/L		12/14/16 18:18	12/15/16 16:46	1
Perfluorooctanesulfonic acid (PFOS)	2.9	U	3.8	1.2	ng/L		12/14/16 18:18	12/15/16 16:46	1
Perfluorodecanesulfonic acid (PFDS)	2.9	U	3.8	1.2	ng/L		12/14/16 18:18	12/15/16 16:46	1
Perfluorooctane Sulfonamide (FOSA)	1.9	U	2.4	0.61	ng/L		12/14/16 18:18	12/15/16 16:46	1
Isotope Dilution	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C8 FOSA	50		25 - 150				12/14/16 18:18	12/15/16 16:46	1
13C4 PFBA	131		25 - 150				12/14/16 18:18	12/15/16 16:46	1
13C2 PFHxA	130		25 - 150				12/14/16 18:18	12/15/16 16:46	1
13C4 PFOA	144		25 - 150				12/14/16 18:18	12/15/16 16:46	1
13C5 PFNA	140		25 - 150				12/14/16 18:18	12/15/16 16:46	1
13C2 PFDA	150		25 - 150				12/14/16 18:18	12/15/16 16:46	1
13C2 PFUnA	145		25 - 150				12/14/16 18:18	12/15/16 16:46	1
13C2 PFDoA	148		25 - 150				12/14/16 18:18	12/15/16 16:46	1
18O2 PFHxS	123		25 - 150				12/14/16 18:18	12/15/16 16:46	1
13C4 PFOS	128		25 - 150				12/14/16 18:18	12/15/16 16:46	1
13C4-PFHpA	139		25 - 150				12/14/16 18:18	12/15/16 16:46	1
13C5 PFPeA	140		25 - 150				12/14/16 18:18	12/15/16 16:46	1

Client Sample ID: CS-10
Date Collected: 12/06/16 10:40
Date Received: 12/07/16 10:30

Lab Sample ID: 320-24118-3
Matrix: Water

Method: 537 (Modified) - Perfluorinated Hydrocarbons

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorobutanoic acid (PFBA)	0.51	J	2.4	0.44	ng/L		12/14/16 18:18	12/15/16 16:54	1
Perfluoropentanoic acid (PFPeA)	1.9	U	2.4	0.95	ng/L		12/14/16 18:18	12/15/16 16:54	1
Perfluorohexanoic acid (PFHxA)	1.1	J	2.4	0.76	ng/L		12/14/16 18:18	12/15/16 16:54	1
Perfluoroheptanoic acid (PFHpA)	1.9	U M	2.4	0.77	ng/L		12/14/16 18:18	12/15/16 16:54	1
Perfluorooctanoic acid (PFOA)	0.72	J	2.4	0.72	ng/L		12/14/16 18:18	12/15/16 16:54	1
Perfluorononanoic acid (PFNA)	1.9	U	2.4	0.63	ng/L		12/14/16 18:18	12/15/16 16:54	1
Perfluorodecanoic acid (PFDA)	0.96	U	2.4	0.42	ng/L		12/14/16 18:18	12/15/16 16:54	1
Perfluoroundecanoic acid (PFUnA)	1.9	U	2.4	0.72	ng/L		12/14/16 18:18	12/15/16 16:54	1
Perfluorododecanoic acid (PFDoA)	1.9	U	2.4	0.56	ng/L		12/14/16 18:18	12/15/16 16:54	1
Perfluorotridecanoic Acid (PFTriA)	1.9	U	2.4	0.53	ng/L		12/14/16 18:18	12/15/16 16:54	1
Perfluorotetradecanoic acid (PFTeA)	0.53	J	2.4	0.39	ng/L		12/14/16 18:18	12/15/16 16:54	1
Perfluorobutanesulfonic acid (PFBS)	1.3	J M	2.4	0.88	ng/L		12/14/16 18:18	12/15/16 16:54	1
Perfluorohexanesulfonic acid (PFHxS)	10		2.4	0.84	ng/L		12/14/16 18:18	12/15/16 16:54	1
Perfluorooctanesulfonic acid (PFOS)	17		3.9	1.2	ng/L		12/14/16 18:18	12/15/16 16:54	1
Perfluorodecanesulfonic acid (PFDS)	2.9	U	3.9	1.2	ng/L		12/14/16 18:18	12/15/16 16:54	1
Perfluorooctane Sulfonamide (FOSA)	1.9	U	2.4	0.61	ng/L		12/14/16 18:18	12/15/16 16:54	1
Isotope Dilution	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C8 FOSA	4	Q	25 - 150				12/14/16 18:18	12/15/16 16:54	1
13C4 PFBA	103		25 - 150				12/14/16 18:18	12/15/16 16:54	1
13C2 PFHxA	105		25 - 150				12/14/16 18:18	12/15/16 16:54	1
13C4 PFOA	100		25 - 150				12/14/16 18:18	12/15/16 16:54	1
13C5 PFNA	79		25 - 150				12/14/16 18:18	12/15/16 16:54	1

Client Sample Results

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

Client Sample ID: CS-10
Date Collected: 12/06/16 10:40
Date Received: 12/07/16 10:30

Lab Sample ID: 320-24118-3
Matrix: Water

Method: 537 (Modified) - Perfluorinated Hydrocarbons (Continued)

<i>Isotope Dilution</i>	<i>%Recovery</i>	<i>Qualifier</i>	<i>Limits</i>	<i>Prepared</i>	<i>Analyzed</i>	<i>Dil Fac</i>
13C2 PFDA	73		25 - 150	12/14/16 18:18	12/15/16 16:54	1
13C2 PFUnA	77		25 - 150	12/14/16 18:18	12/15/16 16:54	1
13C2 PFDoA	99		25 - 150	12/14/16 18:18	12/15/16 16:54	1
18O2 PFHxS	123		25 - 150	12/14/16 18:18	12/15/16 16:54	1
13C4 PFOS	131		25 - 150	12/14/16 18:18	12/15/16 16:54	1
13C4-PFHpA	106		25 - 150	12/14/16 18:18	12/15/16 16:54	1
13C5 PFPeA	123		25 - 150	12/14/16 18:18	12/15/16 16:54	1

Client Sample ID: CS-41
Date Collected: 12/06/16 08:30
Date Received: 12/07/16 10:30

Lab Sample ID: 320-24118-4
Matrix: Water

Method: 537 (Modified) - Perfluorinated Hydrocarbons

<i>Analyte</i>	<i>Result</i>	<i>Qualifier</i>	<i>LOQ</i>	<i>DL</i>	<i>Unit</i>	<i>D</i>	<i>Prepared</i>	<i>Analyzed</i>	<i>Dil Fac</i>
Perfluorobutanoic acid (PFBA)	1.0	U	2.5	0.46	ng/L		12/14/16 18:18	12/15/16 17:01	1
Perfluoropentanoic acid (PFPeA)	2.0	U	2.5	1.0	ng/L		12/14/16 18:18	12/15/16 17:01	1
Perfluorohexanoic acid (PFHxA)	2.0	U	2.5	0.80	ng/L		12/14/16 18:18	12/15/16 17:01	1
Perfluoroheptanoic acid (PFHpA)	2.0	U	2.5	0.81	ng/L		12/14/16 18:18	12/15/16 17:01	1
Perfluorooctanoic acid (PFOA)	2.0	U	2.5	0.76	ng/L		12/14/16 18:18	12/15/16 17:01	1
Perfluorononanoic acid (PFNA)	2.0	U	2.5	0.66	ng/L		12/14/16 18:18	12/15/16 17:01	1
Perfluorodecanoic acid (PFDA)	1.0	U	2.5	0.45	ng/L		12/14/16 18:18	12/15/16 17:01	1
Perfluoroundecanoic acid (PFUnA)	2.0	U	2.5	0.76	ng/L		12/14/16 18:18	12/15/16 17:01	1
Perfluorododecanoic acid (PFDoA)	2.0	U	2.5	0.59	ng/L		12/14/16 18:18	12/15/16 17:01	1
Perfluorotridecanoic Acid (PFTriA)	2.0	U	2.5	0.56	ng/L		12/14/16 18:18	12/15/16 17:01	1
Perfluorotetradecanoic acid (PFTeA)	0.51	J	2.5	0.41	ng/L		12/14/16 18:18	12/15/16 17:01	1
Perfluorobutanesulfonic acid (PFBS)	2.0	U	2.5	0.93	ng/L		12/14/16 18:18	12/15/16 17:01	1
Perfluorohexanesulfonic acid (PFHxS)	2.0	U M	2.5	0.88	ng/L		12/14/16 18:18	12/15/16 17:01	1
Perfluorooctanesulfonic acid (PFOS)	3.0	U	4.1	1.3	ng/L		12/14/16 18:18	12/15/16 17:01	1
Perfluorodecanesulfonic acid (PFDS)	3.0	U	4.1	1.2	ng/L		12/14/16 18:18	12/15/16 17:01	1
Perfluorooctane Sulfonamide (FOSA)	2.0	U	2.5	0.65	ng/L		12/14/16 18:18	12/15/16 17:01	1

<i>Isotope Dilution</i>	<i>%Recovery</i>	<i>Qualifier</i>	<i>Limits</i>	<i>Prepared</i>	<i>Analyzed</i>	<i>Dil Fac</i>
13C8 FOSA	3	Q	25 - 150	12/14/16 18:18	12/15/16 17:01	1
13C4 PFBA	86		25 - 150	12/14/16 18:18	12/15/16 17:01	1
13C2 PFHxA	87		25 - 150	12/14/16 18:18	12/15/16 17:01	1
13C4 PFOA	82		25 - 150	12/14/16 18:18	12/15/16 17:01	1
13C5 PFNA	63		25 - 150	12/14/16 18:18	12/15/16 17:01	1
13C2 PFDA	55		25 - 150	12/14/16 18:18	12/15/16 17:01	1
13C2 PFUnA	62		25 - 150	12/14/16 18:18	12/15/16 17:01	1
13C2 PFDoA	80		25 - 150	12/14/16 18:18	12/15/16 17:01	1
18O2 PFHxS	101		25 - 150	12/14/16 18:18	12/15/16 17:01	1
13C4 PFOS	104		25 - 150	12/14/16 18:18	12/15/16 17:01	1
13C4-PFHpA	90		25 - 150	12/14/16 18:18	12/15/16 17:01	1
13C5 PFPeA	101		25 - 150	12/14/16 18:18	12/15/16 17:01	1

Client Sample Results

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

Client Sample ID: CS-12
Date Collected: 12/06/16 10:00
Date Received: 12/07/16 10:30

Lab Sample ID: 320-24118-5
Matrix: Water

Method: 537 (Modified) - Perfluorinated Hydrocarbons

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorobutanoic acid (PFBA)	0.96	U	2.4	0.44	ng/L		12/14/16 18:18	12/15/16 17:09	1
Perfluoropentanoic acid (PFPeA)	1.9	U	2.4	0.95	ng/L		12/14/16 18:18	12/15/16 17:09	1
Perfluorohexanoic acid (PFHxA)	1.9	U	2.4	0.75	ng/L		12/14/16 18:18	12/15/16 17:09	1
Perfluoroheptanoic acid (PFHpA)	1.9	U	2.4	0.77	ng/L		12/14/16 18:18	12/15/16 17:09	1
Perfluorooctanoic acid (PFOA)	1.9	U	2.4	0.71	ng/L		12/14/16 18:18	12/15/16 17:09	1
Perfluorononanoic acid (PFNA)	1.9	U	2.4	0.63	ng/L		12/14/16 18:18	12/15/16 17:09	1
Perfluorodecanoic acid (PFDA)	0.96	U	2.4	0.42	ng/L		12/14/16 18:18	12/15/16 17:09	1
Perfluoroundecanoic acid (PFUnA)	1.9	U	2.4	0.71	ng/L		12/14/16 18:18	12/15/16 17:09	1
Perfluorododecanoic acid (PFDoA)	1.9	U	2.4	0.56	ng/L		12/14/16 18:18	12/15/16 17:09	1
Perfluorotridecanoic Acid (PFTriA)	1.9	U	2.4	0.53	ng/L		12/14/16 18:18	12/15/16 17:09	1
Perfluorotetradecanoic acid (PFTeA)	0.72	J	2.4	0.38	ng/L		12/14/16 18:18	12/15/16 17:09	1
Perfluorobutanesulfonic acid (PFBS)	1.9	U	2.4	0.88	ng/L		12/14/16 18:18	12/15/16 17:09	1
Perfluorohexanesulfonic acid (PFHxS)	1.9	U	2.4	0.83	ng/L		12/14/16 18:18	12/15/16 17:09	1
Perfluorooctanesulfonic acid (PFOS)	2.9	U	3.8	1.2	ng/L		12/14/16 18:18	12/15/16 17:09	1
Perfluorodecanesulfonic acid (PFDS)	2.9	U	3.8	1.2	ng/L		12/14/16 18:18	12/15/16 17:09	1
Perfluorooctane Sulfonamide (FOSA)	1.9	U	2.4	0.61	ng/L		12/14/16 18:18	12/15/16 17:09	1
Isotope Dilution	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C8 FOSA	4	Q	25 - 150				12/14/16 18:18	12/15/16 17:09	1
13C4 PFBA	84		25 - 150				12/14/16 18:18	12/15/16 17:09	1
13C2 PFHxA	83		25 - 150				12/14/16 18:18	12/15/16 17:09	1
13C4 PFOA	79		25 - 150				12/14/16 18:18	12/15/16 17:09	1
13C5 PFNA	62		25 - 150				12/14/16 18:18	12/15/16 17:09	1
13C2 PFDA	59		25 - 150				12/14/16 18:18	12/15/16 17:09	1
13C2 PFUnA	64		25 - 150				12/14/16 18:18	12/15/16 17:09	1
13C2 PFDoA	80		25 - 150				12/14/16 18:18	12/15/16 17:09	1
18O2 PFHxS	101		25 - 150				12/14/16 18:18	12/15/16 17:09	1
13C4 PFOS	104		25 - 150				12/14/16 18:18	12/15/16 17:09	1
13C4-PFHpA	85		25 - 150				12/14/16 18:18	12/15/16 17:09	1
13C5 PFPeA	93		25 - 150				12/14/16 18:18	12/15/16 17:09	1

Client Sample ID: CS-1
Date Collected: 12/06/16 09:17
Date Received: 12/07/16 10:30

Lab Sample ID: 320-24118-6
Matrix: Water

Method: 537 (Modified) - Perfluorinated Hydrocarbons

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorobutanoic acid (PFBA)	1.0	U	2.5	0.46	ng/L		12/14/16 18:18	12/15/16 17:16	1
Perfluoropentanoic acid (PFPeA)	2.0	U	2.5	0.99	ng/L		12/14/16 18:18	12/15/16 17:16	1
Perfluorohexanoic acid (PFHxA)	2.0	U	2.5	0.79	ng/L		12/14/16 18:18	12/15/16 17:16	1
Perfluoroheptanoic acid (PFHpA)	2.0	U	2.5	0.80	ng/L		12/14/16 18:18	12/15/16 17:16	1
Perfluorooctanoic acid (PFOA)	2.0	U	2.5	0.75	ng/L		12/14/16 18:18	12/15/16 17:16	1
Perfluorononanoic acid (PFNA)	2.0	U	2.5	0.65	ng/L		12/14/16 18:18	12/15/16 17:16	1
Perfluorodecanoic acid (PFDA)	1.0	U	2.5	0.44	ng/L		12/14/16 18:18	12/15/16 17:16	1
Perfluoroundecanoic acid (PFUnA)	2.0	U	2.5	0.75	ng/L		12/14/16 18:18	12/15/16 17:16	1
Perfluorododecanoic acid (PFDoA)	2.0	U	2.5	0.58	ng/L		12/14/16 18:18	12/15/16 17:16	1
Perfluorotridecanoic Acid (PFTriA)	2.0	U	2.5	0.55	ng/L		12/14/16 18:18	12/15/16 17:16	1
Perfluorotetradecanoic acid (PFTeA)	0.75	J	2.5	0.40	ng/L		12/14/16 18:18	12/15/16 17:16	1
Perfluorobutanesulfonic acid (PFBS)	2.0	U	2.5	0.92	ng/L		12/14/16 18:18	12/15/16 17:16	1

TestAmerica Sacramento

Client Sample Results

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

Client Sample ID: CS-1

Lab Sample ID: 320-24118-6

Date Collected: 12/06/16 09:17

Matrix: Water

Date Received: 12/07/16 10:30

Method: 537 (Modified) - Perfluorinated Hydrocarbons (Continued)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorohexanesulfonic acid (PFHxS)	2.0	U	2.5	0.87	ng/L		12/14/16 18:18	12/15/16 17:16	1
Perfluorooctanesulfonic acid (PFOS)	3.0	U	4.0	1.3	ng/L		12/14/16 18:18	12/15/16 17:16	1
Perfluorodecanesulfonic acid (PFDS)	3.0	U	4.0	1.2	ng/L		12/14/16 18:18	12/15/16 17:16	1
Perfluorooctane Sulfonamide (FOSA)	2.0	U	2.5	0.64	ng/L		12/14/16 18:18	12/15/16 17:16	1
Isotope Dilution	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C8 FOSA	5	Q	25 - 150				12/14/16 18:18	12/15/16 17:16	1
13C4 PFBA	94		25 - 150				12/14/16 18:18	12/15/16 17:16	1
13C2 PFHxA	95		25 - 150				12/14/16 18:18	12/15/16 17:16	1
13C4 PFOA	81		25 - 150				12/14/16 18:18	12/15/16 17:16	1
13C5 PFNA	54		25 - 150				12/14/16 18:18	12/15/16 17:16	1
13C2 PFDA	48		25 - 150				12/14/16 18:18	12/15/16 17:16	1
13C2 PFUnA	63		25 - 150				12/14/16 18:18	12/15/16 17:16	1
13C2 PFDoA	84		25 - 150				12/14/16 18:18	12/15/16 17:16	1
18O2 PFHxS	122		25 - 150				12/14/16 18:18	12/15/16 17:16	1
13C4 PFOS	129		25 - 150				12/14/16 18:18	12/15/16 17:16	1
13C4-PFHpA	94		25 - 150				12/14/16 18:18	12/15/16 17:16	1
13C5 PFPeA	117		25 - 150				12/14/16 18:18	12/15/16 17:16	1

Default Detection Limits

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

Method: 537 (Modified) - Perfluorinated Hydrocarbons Prep: 3535

Analyte	LOQ	DL	Units	Method
Perfluorobutanesulfonic acid (PFBS)	2.5	0.92	ng/L	537 (Modified)
Perfluorobutanoic acid (PFBA)	2.5	0.46	ng/L	537 (Modified)
Perfluorodecanesulfonic acid (PFDS)	4.0	1.2	ng/L	537 (Modified)
Perfluorodecanoic acid (PFDA)	2.5	0.44	ng/L	537 (Modified)
Perfluorododecanoic acid (PFDoA)	2.5	0.58	ng/L	537 (Modified)
Perfluoroheptanoic acid (PFHpA)	2.5	0.80	ng/L	537 (Modified)
Perfluorohexanesulfonic acid (PFHxS)	2.5	0.87	ng/L	537 (Modified)
Perfluorohexanoic acid (PFHxA)	2.5	0.79	ng/L	537 (Modified)
Perfluorononanoic acid (PFNA)	2.5	0.65	ng/L	537 (Modified)
Perfluorooctane Sulfonamide (FOSA)	2.5	0.64	ng/L	537 (Modified)
Perfluorooctanesulfonic acid (PFOS)	4.0	1.3	ng/L	537 (Modified)
Perfluorooctanoic acid (PFOA)	2.5	0.75	ng/L	537 (Modified)
Perfluoropentanoic acid (PFPeA)	2.5	0.99	ng/L	537 (Modified)
Perfluorotetradecanoic acid (PFTeA)	2.5	0.40	ng/L	537 (Modified)
Perfluorotridecanoic Acid (PFTriA)	2.5	0.55	ng/L	537 (Modified)
Perfluoroundecanoic acid (PFUnA)	2.5	0.75	ng/L	537 (Modified)

Isotope Dilution Summary

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

Method: 537 (Modified) - Perfluorinated Hydrocarbons

Matrix: Water

Prep Type: Total/NA

		Percent Isotope Dilution Recovery (Acceptance Limits)							
Lab Sample ID	Client Sample ID	3C8 FOS/ (25-150)	3C4 PFB/ (25-150)	3C2 PFHx (25-150)	3C4 PFO/ (25-150)	3C5 PFN/ (25-150)	3C2 PFD/ (25-150)	3C2 PFUn (25-150)	3C2 PFDo (25-150)
320-24118-1	TB-1	14 Q	131	133	145	142	151 Q	153 Q	148
320-24118-2	FB-1	50	131	130	144	140	150	145	148
320-24118-3	CS-10	4 Q	103	105	100	79	73	77	99
320-24118-4	CS-41	3 Q	86	87	82	63	55	62	80
320-24118-5	CS-12	4 Q	84	83	79	62	59	64	80
320-24118-6	CS-1	5 Q	94	95	81	54	48	63	84
320-24118-6 MS	CS-1	6 Q	93	102	101	82	82	92	110
320-24118-6 MSD	CS-1	4 Q	95	101	97	76	83	87	99
LCS 320-142235/2-A	Lab Control Sample	13 Q	105	103	110	111	122	116	112
MB 320-142235/1-A	Method Blank	39	118	118	128	125	136	135	129

		Percent Isotope Dilution Recovery (Acceptance Limits)			
Lab Sample ID	Client Sample ID	3O2 PFHx (25-150)	3C4 PFO (25-150)	3C4-PFHp (25-150)	3C5 PFPe (25-150)
320-24118-1	TB-1	125	131	142	141
320-24118-2	FB-1	123	128	139	140
320-24118-3	CS-10	123	131	106	123
320-24118-4	CS-41	101	104	90	101
320-24118-5	CS-12	101	104	85	93
320-24118-6	CS-1	122	129	94	117
320-24118-6 MS	CS-1	123	125	107	117
320-24118-6 MSD	CS-1	118	125	105	115
LCS 320-142235/2-A	Lab Control Sample	100	101	110	107
MB 320-142235/1-A	Method Blank	111	115	127	126

Surrogate Legend

- 13C8 FOSA = 13C8 FOSA
- 13C4 PFBA = 13C4 PFBA
- 13C2 PFHxA = 13C2 PFHxA
- 13C4 PFOA = 13C4 PFOA
- 13C5 PFNA = 13C5 PFNA
- 13C2 PFDA = 13C2 PFDA
- 13C2 PFUnA = 13C2 PFUnA
- 13C2 PFDoA = 13C2 PFDoA
- 18O2 PFHxS = 18O2 PFHxS
- 13C4 PFOS = 13C4 PFOS
- 13C4-PFHpA = 13C4-PFHpA
- 13C5 PFPeA = 13C5 PFPeA

QC Sample Results

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

Method: 537 (Modified) - Perfluorinated Hydrocarbons

Lab Sample ID: MB 320-142235/1-A
Matrix: Water
Analysis Batch: 142379

Client Sample ID: Method Blank
Prep Type: Total/NA
Prep Batch: 142235

Analyte	MB	MB	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
	Result	Qualifier							
Perfluorobutanoic acid (PFBA)	1.0	U	2.5	0.46	ng/L		12/14/16 18:18	12/15/16 16:24	1
Perfluoropentanoic acid (PFPeA)	2.0	U	2.5	0.99	ng/L		12/14/16 18:18	12/15/16 16:24	1
Perfluorohexanoic acid (PFHxA)	2.0	U	2.5	0.79	ng/L		12/14/16 18:18	12/15/16 16:24	1
Perfluoroheptanoic acid (PFHpA)	2.0	U	2.5	0.80	ng/L		12/14/16 18:18	12/15/16 16:24	1
Perfluorooctanoic acid (PFOA)	2.0	U	2.5	0.75	ng/L		12/14/16 18:18	12/15/16 16:24	1
Perfluorononanoic acid (PFNA)	2.0	U	2.5	0.65	ng/L		12/14/16 18:18	12/15/16 16:24	1
Perfluorodecanoic acid (PFDA)	1.0	U	2.5	0.44	ng/L		12/14/16 18:18	12/15/16 16:24	1
Perfluoroundecanoic acid (PFUnA)	2.0	U	2.5	0.75	ng/L		12/14/16 18:18	12/15/16 16:24	1
Perfluorododecanoic acid (PFDoA)	2.0	U	2.5	0.58	ng/L		12/14/16 18:18	12/15/16 16:24	1
Perfluorotridecanoic Acid (PFTriA)	2.0	U	2.5	0.55	ng/L		12/14/16 18:18	12/15/16 16:24	1
Perfluorotetradecanoic acid (PFTeA)	0.559	J	2.5	0.40	ng/L		12/14/16 18:18	12/15/16 16:24	1
Perfluorobutanesulfonic acid (PFBS)	2.0	U	2.5	0.92	ng/L		12/14/16 18:18	12/15/16 16:24	1
Perfluorohexanesulfonic acid (PFHxS)	2.0	U	2.5	0.87	ng/L		12/14/16 18:18	12/15/16 16:24	1
Perfluorooctanesulfonic acid (PFOS)	3.0	U	4.0	1.3	ng/L		12/14/16 18:18	12/15/16 16:24	1
Perfluorodecanesulfonic acid (PFDS)	3.0	U	4.0	1.2	ng/L		12/14/16 18:18	12/15/16 16:24	1
Perfluorooctane Sulfonamide (FOSA)	2.0	U	2.5	0.64	ng/L		12/14/16 18:18	12/15/16 16:24	1

Isotope Dilution	MB	MB	Limits	Prepared	Analyzed	Dil Fac
	%Recovery	Qualifier				
13C8 FOSA	39		25 - 150	12/14/16 18:18	12/15/16 16:24	1
13C4 PFBA	118		25 - 150	12/14/16 18:18	12/15/16 16:24	1
13C2 PFHxA	118		25 - 150	12/14/16 18:18	12/15/16 16:24	1
13C4 PFOA	128		25 - 150	12/14/16 18:18	12/15/16 16:24	1
13C5 PFNA	125		25 - 150	12/14/16 18:18	12/15/16 16:24	1
13C2 PFDA	136		25 - 150	12/14/16 18:18	12/15/16 16:24	1
13C2 PFUnA	135		25 - 150	12/14/16 18:18	12/15/16 16:24	1
13C2 PFDoA	129		25 - 150	12/14/16 18:18	12/15/16 16:24	1
18O2 PFHxS	111		25 - 150	12/14/16 18:18	12/15/16 16:24	1
13C4 PFOS	115		25 - 150	12/14/16 18:18	12/15/16 16:24	1
13C4-PFHpA	127		25 - 150	12/14/16 18:18	12/15/16 16:24	1
13C5 PFPeA	126		25 - 150	12/14/16 18:18	12/15/16 16:24	1

Lab Sample ID: LCS 320-142235/2-A
Matrix: Water
Analysis Batch: 142379

Client Sample ID: Lab Control Sample
Prep Type: Total/NA
Prep Batch: 142235

Analyte	Spike Added	LCS	LCS	Unit	D	%Rec	Limits
		Result	Qualifier				
Perfluorobutanoic acid (PFBA)	40.0	41.3		ng/L		103	60 - 140
Perfluoropentanoic acid (PFPeA)	40.0	40.6		ng/L		101	60 - 140
Perfluorohexanoic acid (PFHxA)	40.0	38.6		ng/L		97	60 - 140
Perfluoroheptanoic acid (PFHpA)	40.0	37.8		ng/L		95	60 - 140
Perfluorooctanoic acid (PFOA)	40.0	39.8		ng/L		99	60 - 140
Perfluorononanoic acid (PFNA)	40.0	38.5	M	ng/L		96	60 - 140
Perfluorodecanoic acid (PFDA)	40.0	37.7		ng/L		94	60 - 140
Perfluoroundecanoic acid (PFUnA)	40.0	38.1		ng/L		95	60 - 140
Perfluorododecanoic acid (PFDoA)	40.0	38.5		ng/L		96	60 - 140
Perfluorotridecanoic Acid (PFTriA)	40.0	41.4		ng/L		103	50 - 150

TestAmerica Sacramento

QC Sample Results

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

Method: 537 (Modified) - Perfluorinated Hydrocarbons (Continued)

Lab Sample ID: LCS 320-142235/2-A

Matrix: Water

Analysis Batch: 142379

Client Sample ID: Lab Control Sample

Prep Type: Total/NA

Prep Batch: 142235

Analyte	Spike Added	LCS Result	LCS Qualifier	Unit	D	%Rec	Limits
Perfluorotetradecanoic acid (PFTeA)	40.0	43.7		ng/L		109	50 - 150
Perfluorobutanesulfonic acid (PFBS)	35.4	39.8		ng/L		113	50 - 150
Perfluorohexanesulfonic acid (PFHxS)	36.4	34.7		ng/L		95	60 - 140
Perfluorooctanesulfonic acid (PFOS)	37.1	37.5		ng/L		101	60 - 140
Perfluorodecanesulfonic acid (PFDS)	38.6	38.2		ng/L		99	50 - 150
Perfluorooctane Sulfonamide (FOSA)	40.0	38.3		ng/L		96	60 - 140

Isotope Dilution	LCS %Recovery	LCS Qualifier	Limits
13C8 FOSA	13	Q	25 - 150
13C4 PFBA	105		25 - 150
13C2 PFHxA	103		25 - 150
13C4 PFOA	110		25 - 150
13C5 PFNA	111		25 - 150
13C2 PFDA	122		25 - 150
13C2 PFUnA	116		25 - 150
13C2 PFDoA	112		25 - 150
18O2 PFHxS	100		25 - 150
13C4 PFOS	101		25 - 150
13C4-PFHpA	110		25 - 150
13C5 PFPeA	107		25 - 150

Lab Sample ID: 320-24118-6 MS

Matrix: Water

Analysis Batch: 142379

Client Sample ID: CS-1

Prep Type: Total/NA

Prep Batch: 142235

Analyte	Sample Result	Sample Qualifier	Spike Added	MS Result	MS Qualifier	Unit	D	%Rec	Limits
Perfluorobutanoic acid (PFBA)	1.0	U	38.3	40.3		ng/L		105	60 - 140
Perfluoropentanoic acid (PFPeA)	2.0	U	38.3	38.5		ng/L		100	60 - 140
Perfluorohexanoic acid (PFHxA)	2.0	U	38.3	37.3		ng/L		97	60 - 140
Perfluoroheptanoic acid (PFHpA)	2.0	U	38.3	37.4		ng/L		98	60 - 140
Perfluorooctanoic acid (PFOA)	2.0	U	38.3	38.1		ng/L		99	60 - 140
Perfluorononanoic acid (PFNA)	2.0	U	38.3	37.4		ng/L		98	60 - 140
Perfluorodecanoic acid (PFDA)	1.0	U	38.3	36.8		ng/L		96	60 - 140
Perfluoroundecanoic acid (PFUnA)	2.0	U	38.3	37.7		ng/L		98	60 - 140
Perfluorododecanoic acid (PFDoA)	2.0	U	38.3	37.6		ng/L		98	60 - 140
Perfluorotridecanoic Acid (PFTriA)	2.0	U	38.3	52.7		ng/L		138	50 - 150
Perfluorotetradecanoic acid (PFTeA)	0.75	J J	38.3	58.5	J	ng/L		151	50 - 150
Perfluorobutanesulfonic acid (PFBS)	2.0	U	33.9	39.2		ng/L		116	50 - 150
Perfluorohexanesulfonic acid (PFHxS)	2.0	U	34.9	34.1		ng/L		98	60 - 140

TestAmerica Sacramento

QC Sample Results

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

Method: 537 (Modified) - Perfluorinated Hydrocarbons (Continued)

Lab Sample ID: 320-24118-6 MS

Matrix: Water

Analysis Batch: 142379

Client Sample ID: CS-1

Prep Type: Total/NA

Prep Batch: 142235

Analyte	Sample Result	Sample Qualifier	Spike Added	MS Result	MS Qualifier	Unit	D	%Rec	Limits
Perfluorooctanesulfonic acid (PFOS)	3.0	U	35.6	37.8		ng/L		106	60 - 140
Perfluorodecanesulfonic acid (PFDS)	3.0	U	37.0	37.7		ng/L		102	50 - 150
Perfluorooctane Sulfonamide (FOSA)	2.0	U	38.3	37.6		ng/L		98	60 - 140
Isotope Dilution	MS %Recovery	MS Qualifier	Limits						
13C8 FOSA	6	Q	25 - 150						
13C4 PFBA	93		25 - 150						
13C2 PFHxA	102		25 - 150						
13C4 PFOA	101		25 - 150						
13C5 PFNA	82		25 - 150						
13C2 PFDA	82		25 - 150						
13C2 PFUnA	92		25 - 150						
13C2 PFDoA	110		25 - 150						
18O2 PFHxS	123		25 - 150						
13C4 PFOS	125		25 - 150						
13C4-PFHpA	107		25 - 150						
13C5 PFPeA	117		25 - 150						

Lab Sample ID: 320-24118-6 MSD

Matrix: Water

Analysis Batch: 142602

Client Sample ID: CS-1

Prep Type: Total/NA

Prep Batch: 142235

Analyte	Sample Result	Sample Qualifier	Spike Added	MSD Result	MSD Qualifier	Unit	D	%Rec	Limits	RPD	Limit
Perfluorobutanoic acid (PFBA)	1.0	U	39.1	41.1		ng/L		105	60 - 140	2	30
Perfluoropentanoic acid (PFPeA)	2.0	U	39.1	39.3		ng/L		101	60 - 140	2	30
Perfluorohexanoic acid (PFHxA)	2.0	U	39.1	38.1		ng/L		97	60 - 140	2	30
Perfluoroheptanoic acid (PFHpA)	2.0	U	39.1	38.2		ng/L		98	60 - 140	2	30
Perfluorooctanoic acid (PFOA)	2.0	U	39.1	39.0		ng/L		100	60 - 140	2	30
Perfluorononanoic acid (PFNA)	2.0	U	39.1	37.6		ng/L		96	60 - 140	1	30
Perfluorodecanoic acid (PFDA)	1.0	U	39.1	36.4		ng/L		93	60 - 140	1	30
Perfluoroundecanoic acid (PFUnA)	2.0	U	39.1	38.3		ng/L		98	60 - 140	2	30
Perfluorododecanoic acid (PFDoA)	2.0	U	39.1	38.8		ng/L		99	60 - 140	3	30
Perfluorotridecanoic Acid (PFTriA)	2.0	U	39.1	51.3		ng/L		131	50 - 150	3	30
Perfluorotetradecanoic acid (PFTeA)	0.75	J J	39.1	68.0	J	ng/L		172	50 - 150	15	30
Perfluorobutanesulfonic acid (PFBS)	2.0	U	34.6	42.3		ng/L		122	50 - 150	8	30
Perfluorohexanesulfonic acid (PFHxS)	2.0	U	35.6	35.7		ng/L		100	60 - 140	5	30
Perfluorooctanesulfonic acid (PFOS)	3.0	U	36.3	37.1		ng/L		102	60 - 140	2	30
Perfluorodecanesulfonic acid (PFDS)	3.0	U	37.7	37.2		ng/L		99	50 - 150	1	30
Perfluorooctane Sulfonamide (FOSA)	2.0	U	39.1	36.9		ng/L		94	60 - 140	2	30

TestAmerica Sacramento

QC Sample Results

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

<i>Isotope Dilution</i>	<i>MSD MSD</i>		<i>Limits</i>
	<i>%Recovery</i>	<i>Qualifier</i>	
<i>13C8 FOSA</i>	4	Q	25 - 150
<i>13C4 PFBA</i>	95		25 - 150
<i>13C2 PFHxA</i>	101		25 - 150
<i>13C4 PFOA</i>	97		25 - 150
<i>13C5 PFNA</i>	76		25 - 150
<i>13C2 PFDA</i>	83		25 - 150
<i>13C2 PFUnA</i>	87		25 - 150
<i>13C2 PFDoA</i>	99		25 - 150
<i>18O2 PFHxS</i>	118		25 - 150
<i>13C4 PFOS</i>	125		25 - 150
<i>13C4-PFHpA</i>	105		25 - 150
<i>13C5 PFPeA</i>	115		25 - 150

QC Association Summary

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

LCMS

Prep Batch: 142235

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-24118-1	TB-1	Total/NA	Water	3535	
320-24118-2	FB-1	Total/NA	Water	3535	
320-24118-3	CS-10	Total/NA	Water	3535	
320-24118-4	CS-41	Total/NA	Water	3535	
320-24118-5	CS-12	Total/NA	Water	3535	
320-24118-6	CS-1	Total/NA	Water	3535	
MB 320-142235/1-A	Method Blank	Total/NA	Water	3535	
LCS 320-142235/2-A	Lab Control Sample	Total/NA	Water	3535	
320-24118-6 MS	CS-1	Total/NA	Water	3535	
320-24118-6 MSD	CS-1	Total/NA	Water	3535	

Analysis Batch: 142379

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-24118-1	TB-1	Total/NA	Water	537 (Modified)	142235
320-24118-2	FB-1	Total/NA	Water	537 (Modified)	142235
320-24118-3	CS-10	Total/NA	Water	537 (Modified)	142235
320-24118-4	CS-41	Total/NA	Water	537 (Modified)	142235
320-24118-5	CS-12	Total/NA	Water	537 (Modified)	142235
320-24118-6	CS-1	Total/NA	Water	537 (Modified)	142235
MB 320-142235/1-A	Method Blank	Total/NA	Water	537 (Modified)	142235
LCS 320-142235/2-A	Lab Control Sample	Total/NA	Water	537 (Modified)	142235
320-24118-6 MS	CS-1	Total/NA	Water	537 (Modified)	142235

Analysis Batch: 142602

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-24118-6 MSD	CS-1	Total/NA	Water	537 (Modified)	142235

Lab Chronicle

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

Client Sample ID: TB-1

Date Collected: 12/06/16 08:00

Date Received: 12/07/16 10:30

Lab Sample ID: 320-24118-1

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	3535			142235	12/14/16 18:18	VPM	TAL SAC
Total/NA	Analysis	537 (Modified)		1	142379	12/15/16 16:39	SBC	TAL SAC

Client Sample ID: FB-1

Date Collected: 12/06/16 09:22

Date Received: 12/07/16 10:30

Lab Sample ID: 320-24118-2

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	3535			142235	12/14/16 18:18	VPM	TAL SAC
Total/NA	Analysis	537 (Modified)		1	142379	12/15/16 16:46	SBC	TAL SAC

Client Sample ID: CS-10

Date Collected: 12/06/16 10:40

Date Received: 12/07/16 10:30

Lab Sample ID: 320-24118-3

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	3535			142235	12/14/16 18:18	VPM	TAL SAC
Total/NA	Analysis	537 (Modified)		1	142379	12/15/16 16:54	SBC	TAL SAC

Client Sample ID: CS-41

Date Collected: 12/06/16 08:30

Date Received: 12/07/16 10:30

Lab Sample ID: 320-24118-4

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	3535			142235	12/14/16 18:18	VPM	TAL SAC
Total/NA	Analysis	537 (Modified)		1	142379	12/15/16 17:01	SBC	TAL SAC

Client Sample ID: CS-12

Date Collected: 12/06/16 10:00

Date Received: 12/07/16 10:30

Lab Sample ID: 320-24118-5

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	3535			142235	12/14/16 18:18	VPM	TAL SAC
Total/NA	Analysis	537 (Modified)		1	142379	12/15/16 17:09	SBC	TAL SAC

Client Sample ID: CS-1

Date Collected: 12/06/16 09:17

Date Received: 12/07/16 10:30

Lab Sample ID: 320-24118-6

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	3535			142235	12/14/16 18:18	VPM	TAL SAC
Total/NA	Analysis	537 (Modified)		1	142379	12/15/16 17:16	SBC	TAL SAC

TestAmerica Sacramento

Lab Chronicle

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

Laboratory References:

TAL SAC = TestAmerica Sacramento, 880 Riverside Parkway, West Sacramento, CA 95605, TEL (916)373-5600

Certification Summary

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

Laboratory: TestAmerica Sacramento

All certifications held by this laboratory are listed. Not all certifications are applicable to this report.

Authority	Program	EPA Region	Certification ID	Expiration Date
A2LA	DoD ELAP		2928-01	01-31-17
Alaska (UST)	State Program	10	UST-055	12-18-17
Arizona	State Program	9	AZ0708	08-11-17
Arkansas DEQ	State Program	6	88-0691	06-17-17
California	State Program	9	2897	01-31-18
Colorado	State Program	8	CA00044	08-31-17
Connecticut	State Program	1	PH-0691	06-30-17
Florida	NELAP	4	E87570	06-30-17
Hawaii	State Program	9	N/A	01-31-17
Illinois	NELAP	5	200060	03-17-17
Kansas	NELAP	7	E-10375	10-31-17
Louisiana	NELAP	6	30612	06-30-17
Maine	State Program	1	CA0004	04-18-18
Michigan	State Program	5	9947	01-31-18
New Jersey	NELAP	2	CA005	06-30-17
New York	NELAP	2	11666	04-01-17
Oregon	NELAP	10	4040	01-29-17
Pennsylvania	NELAP	3	68-01272	03-31-17
Texas	NELAP	6	T104704399	07-31-17
US Fish & Wildlife	Federal		LE148388-0	10-31-17
USDA	Federal		P330-11-00436	12-30-17
USEPA UCMR	Federal	1	CA00044	11-06-18
Utah	NELAP	8	CA00044	02-28-17
Virginia	NELAP	3	460278	03-14-17
Washington	State Program	10	C581	05-05-17
West Virginia (DW)	State Program	3	9930C	12-31-16
Wyoming	State Program	8	8TMS-L	01-29-17

Method Summary

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

Method	Method Description	Protocol	Laboratory
537 (Modified)	Perfluorinated Hydrocarbons	EPA	TAL SAC

Protocol References:

EPA = US Environmental Protection Agency

Laboratory References:

TAL SAC = TestAmerica Sacramento, 880 Riverside Parkway, West Sacramento, CA 95605, TEL (916)373-5600

Sample Summary

Client: Parsons Corporation
Project/Site: Camp Stanley

TestAmerica Job ID: 320-24118-1

Lab Sample ID	Client Sample ID	Matrix	Collected	Received
320-24118-1	TB-1	Water	12/06/16 08:00	12/07/16 10:30
320-24118-2	FB-1	Water	12/06/16 09:22	12/07/16 10:30
320-24118-3	CS-10	Water	12/06/16 10:40	12/07/16 10:30
320-24118-4	CS-41	Water	12/06/16 08:30	12/07/16 10:30
320-24118-5	CS-12	Water	12/06/16 10:00	12/07/16 10:30
320-24118-6	CS-1	Water	12/06/16 09:17	12/07/16 10:30

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 142379

Lab Sample ID: IC 320-142379/4 Client Sample ID: _____

Date Analyzed: 12/15/16 12:29 Lab File ID: 15DEC2016B_004.d GC Column: Acquity ID: 2.1(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluoroheptanoic acid (PFHpA)	2.43	Assign Peak	chandrase nas	12/15/16 13:48
Perfluorohexanesulfonic acid (PFHxS)	2.44	Assign Peak	chandrase nas	12/15/16 13:48
Perfluorooctanesulfonic acid (PFOS)	3.15	Assign Peak	chandrase nas	12/15/16 13:48
Perfluorododecanoic acid (PFDoA)	4.14	Incomplete Integration	chandrase nas	12/15/16 13:48

Lab Sample ID: IC 320-142379/5 Client Sample ID: _____

Date Analyzed: 12/15/16 12:36 Lab File ID: 15DEC2016B_005.d GC Column: Acquity ID: 2.1(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	3.15	Assign Peak	chandrase nas	12/15/16 13:50

Lab Sample ID: LCS 320-142235/2-A Client Sample ID: _____

Date Analyzed: 12/15/16 16:31 Lab File ID: 15DEC2016B_030.d GC Column: Acquity ID: 2.1(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorononanoic acid (PFNA)	3.31	Incomplete Integration	chandrase nas	12/16/16 09:38

Lab Sample ID: 320-24118-1 Client Sample ID: TB-1

Date Analyzed: 12/15/16 16:39 Lab File ID: 15DEC2016B_031.d GC Column: Acquity ID: 2.1(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorohexanoic acid (PFHxA)	2.23	Incomplete Integration	chandrase nas	12/16/16 09:39

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 142379

Lab Sample ID: 320-24118-2 Client Sample ID: FB-1

Date Analyzed: 12/15/16 16:46 Lab File ID: 15DEC2016B_032.d GC Column: Acquity ID: 2.1(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorohexanesulfonic acid (PFHxS)	2.61	Assign Peak	chandrase nas	12/16/16 09:39

Lab Sample ID: 320-24118-3 Client Sample ID: CS-10

Date Analyzed: 12/15/16 16:54 Lab File ID: 15DEC2016B_033.d GC Column: Acquity ID: 2.1(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorobutanesulfonic acid (PFBS)	1.97	Incomplete Integration	chandrase nas	12/16/16 09:41
Perfluoroheptanoic acid (PFHpA)	2.58	Assign Peak	chandrase nas	12/16/16 09:41

Lab Sample ID: 320-24118-4 Client Sample ID: CS-41

Date Analyzed: 12/15/16 17:01 Lab File ID: 15DEC2016B_034.d GC Column: Acquity ID: 2.1(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorohexanesulfonic acid (PFHxS)	2.60	Assign Peak	chandrase nas	12/16/16 09:42

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
LCMPFCSU_00047	06/14/17	12/14/16	Methanol, Lot Baker 144541	50000 uL	LCM2PFHxDA_00008	1000 uL	13C2-PFHxDA	1 ug/mL
					LCM2PFTeDA_00007	1000 uL	13C2-PFTeDA	1 ug/mL
					LCM4PFHPA_00007	1000 uL	13C4-PFHpA	1 ug/mL
					LCM5PFPEA_00008	1000 uL	13C5 PFPeA	1 ug/mL
					LCM8FOSA_00011	1000 uL	13C8 FOSA	1 ug/mL
					LCMPFBA_00008	1000 uL	13C4 PFBA	1 ug/mL
					LCMPFDA_00011	1000 uL	13C2 PFDA	1 ug/mL
					LCMPFDoA_00008	1000 uL	13C2 PFDoA	1 ug/mL
					LCMPFHxA_00012	1000 uL	13C2 PFHxA	1 ug/mL
					LCMPFHxS_00008	1000 uL	1802 PFHxS	0.946 ug/mL
					LCMPFNA_00008	1000 uL	13C5 PFNA	1 ug/mL
					LCMPFOA_00012	1000 uL	13C4 PFOA	1 ug/mL
					LCMPFOS_00017	1000 uL	13C4 PFOS	0.956 ug/mL
LCMPFUDa_00009	1000 uL	13C2 PFUnA	1 ug/mL					
.LCM2PFHxDA_00008	01/07/21	Wellington Laboratories, Lot M2PFHxDA1112			(Purchased Reagent)	13C2-PFHxDA	50 ug/mL	
.LCM2PFTeDA_00007	12/07/20	Wellington Laboratories, Lot M2PFTeDA1115			(Purchased Reagent)	13C2-PFTeDA	50 ug/mL	
.LCM4PFHPA_00007	05/27/21	Wellington Laboratories, Lot M4PFHpa0516			(Purchased Reagent)	13C4-PFHpa	50 ug/mL	
.LCM5PFPEA_00008	05/22/20	Wellington Laboratories, Lot M5PFPeA0515			(Purchased Reagent)	13C5 PFPeA	50 ug/mL	
.LCM8FOSA_00011	12/22/17	Wellington Laboratories, Lot M8FOSA1215I			(Purchased Reagent)	13C8 FOSA	50 ug/mL	
.LCMPFBA_00008	05/24/21	Wellington Laboratories, Lot MPFBA0516			(Purchased Reagent)	13C4 PFBA	50 ug/mL	
.LCMPFDA_00011	08/19/20	Wellington Laboratories, Lot MPFDA0815			(Purchased Reagent)	13C2 PFDA	50 ug/mL	
.LCMPFDoA_00008	04/08/21	Wellington Laboratories, Lot MPFDoA0416			(Purchased Reagent)	13C2 PFDoA	50 ug/mL	
.LCMPFHxA_00012	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)	13C2 PFHxA	50 ug/mL	
.LCMPFHxS_00008	10/23/20	Wellington Laboratories, Lot MPFHxS1015			(Purchased Reagent)	1802 PFHxS	47.3 ug/mL	
.LCMPFNA_00008	04/13/19	Wellington Laboratories, Lot MPFNA0414			(Purchased Reagent)	13C5 PFNA	50 ug/mL	
.LCMPFOA_00012	01/22/21	Wellington Laboratories, Lot MPFOA0116			(Purchased Reagent)	13C4 PFOA	50 ug/mL	
.LCMPFOS_00017	08/03/21	Wellington Laboratories, Lot MPFOS0816			(Purchased Reagent)	13C4 PFOS	47.8 ug/mL	
.LCMPFUDa_00009	02/12/21	Wellington Laboratories, Lot MPFUDa0216			(Purchased Reagent)	13C2 PFUnA	50 ug/mL	
LCPPFC-L1_00022	05/15/17	12/15/16	MeOH/H2O, Lot 90285	5 mL	LCMPFCSU_00047	250 uL	13C2-PFHxDA	50 ng/mL
							13C2-PFTeDA	50 ng/mL
							13C4-PFHpA	50 ng/mL
							13C5 PFPeA	50 ng/mL
							13C8 FOSA	50 ng/mL
							13C4 PFBA	50 ng/mL
							13C2 PFDA	50 ng/mL
							13C2 PFDoA	50 ng/mL
							13C2 PFHxA	50 ng/mL
							1802 PFHxS	47.3 ng/mL
							13C5 PFNA	50 ng/mL
							13C4 PFOA	50 ng/mL
							13C4 PFOS	47.8 ng/mL
					13C2 PFUnA	50 ng/mL		
					LCPFCSP_00071	25 uL	Perfluorobutanoic acid (PFBA)	0.5 ng/mL
		Perfluorobutanesulfonic acid (PFBS)	0.442 ng/mL					
		Perfluorodecanoic acid (PFDA)	0.5 ng/mL					

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration	
					Reagent ID	Volume Added			
							Perfluorododecanoic acid (PFDoA)	0.5 ng/mL	
							Perfluorodecanesulfonic acid (PFDS)	0.482 ng/mL	
							Perfluoroheptanoic acid (PFHpA)	0.5 ng/mL	
							Perfluoroheptanesulfonic Acid (PFHxA)	0.476 ng/mL	
							Perfluorohexanoic acid (PFHxA)	0.5 ng/mL	
							Perfluorohexadecanoic acid	0.5 ng/mL	
							Perfluorohexanesulfonic acid (PFHxS)	0.455 ng/mL	
							Perfluorononanoic acid (PFNA)	0.5 ng/mL	
							Perfluorooctanoic acid (PFOA)	0.5 ng/mL	
							Perfluorooctadecanoic acid	0.5 ng/mL	
							Perfluorooctanesulfonic acid (PFOS)	0.464 ng/mL	
							Perfluorooctane Sulfonamide (FOSA)	0.5 ng/mL	
							Perfluoropentanoic acid (PFPeA)	0.5 ng/mL	
							Perfluorotetradecanoic acid (PFTeA)	0.5 ng/mL	
							Perfluorotridecanoic Acid (PFTriA)	0.5 ng/mL	
							Perfluoroundecanoic acid (PFUnA)	0.5 ng/mL	
.LCMPFCSU_00047	06/14/17	12/14/16	Methanol, Lot Baker 144541	50000 uL	LCM2PFHxDA_00008	1000 uL	13C2-PFHxDA	1 ug/mL	
					LCM2PFTeDA_00007	1000 uL	13C2-PFTeDA	1 ug/mL	
					LCM4PFHPA_00007	1000 uL	13C4-PFHpA	1 ug/mL	
					LCM5PFPEA_00008	1000 uL	13C5 PFPeA	1 ug/mL	
					LCM8FOSA_00011	1000 uL	13C8 FOSA	1 ug/mL	
					LCMPFBA_00008	1000 uL	13C4 PFBA	1 ug/mL	
					LCMPFDA_00011	1000 uL	13C2 PFDA	1 ug/mL	
					LCMPFDoA_00008	1000 uL	13C2 PFDoA	1 ug/mL	
					LCMPFHxA_00012	1000 uL	13C2 PFHxA	1 ug/mL	
					LCMPFHxS_00008	1000 uL	1802 PFHxS	0.946 ug/mL	
					LCMPFNA_00008	1000 uL	13C5 PFNA	1 ug/mL	
					LCMPFOA_00012	1000 uL	13C4 PFOA	1 ug/mL	
					LCMPFOS_00017	1000 uL	13C4 PFOS	0.956 ug/mL	
					LCMPFUdA_00009	1000 uL	13C2 PFUnA	1 ug/mL	
..LCM2PFHxDA_00008	01/07/21		Wellington Laboratories, Lot M2PFHxDA1112				(Purchased Reagent)	13C2-PFHxDA	50 ug/mL
..LCM2PFTeDA_00007	12/07/20		Wellington Laboratories, Lot M2PFTeDA1115				(Purchased Reagent)	13C2-PFTeDA	50 ug/mL
..LCM4PFHPA_00007	05/27/21		Wellington Laboratories, Lot M4PFHpA0516				(Purchased Reagent)	13C4-PFHpA	50 ug/mL
..LCM5PFPEA_00008	05/22/20		Wellington Laboratories, Lot M5PFPeA0515				(Purchased Reagent)	13C5 PFPeA	50 ug/mL
..LCM8FOSA_00011	12/22/17		Wellington Laboratories, Lot M8FOSA1215I				(Purchased Reagent)	13C8 FOSA	50 ug/mL
..LCMPFBA_00008	05/24/21		Wellington Laboratories, Lot MPFBA0516				(Purchased Reagent)	13C4 PFBA	50 ug/mL
..LCMPFDA_00011	08/19/20		Wellington Laboratories, Lot MPFDA0815				(Purchased Reagent)	13C2 PFDA	50 ug/mL
..LCMPFDoA_00008	04/08/21		Wellington Laboratories, Lot MPFDoA0416				(Purchased Reagent)	13C2 PFDoA	50 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
..LCMPFHxA_00012	04/08/21		Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)	13C2 PFHxA	50 ug/mL
..LCMPFHxS_00008	10/23/20		Wellington Laboratories, Lot MPFHxS1015			(Purchased Reagent)	18O2 PFHxS	47.3 ug/mL
..LCMPFNA_00008	04/13/19		Wellington Laboratories, Lot MPFNA0414			(Purchased Reagent)	13C5 PFNA	50 ug/mL
..LCMPFOA_00012	01/22/21		Wellington Laboratories, Lot MPFOA0116			(Purchased Reagent)	13C4 PFOA	50 ug/mL
..LCMPFOS_00017	08/03/21		Wellington Laboratories, Lot MPFOS0816			(Purchased Reagent)	13C4 PFOS	47.8 ug/mL
..LCMPFUDa_00009	02/12/21		Wellington Laboratories, Lot MPFUDa0216			(Purchased Reagent)	13C2 PFUnA	50 ug/mL
.LCPFCSP_00071	05/15/17	11/10/16	Methanol, Lot 090285	10000 uL	LCPFCSP_00070	2000 uL	Perfluorobutanoic acid (PFBA)	0.1 ug/mL
							Perfluorobutanesulfonic acid (PFBS)	0.0884 ug/mL
							Perfluorodecanoic acid (PFDA)	0.1 ug/mL
							Perfluorododecanoic acid (PFDoA)	0.1 ug/mL
							Perfluorodecanesulfonic acid (PFDS)	0.0964 ug/mL
							Perfluoroheptanoic acid (PFHpA)	0.1 ug/mL
							Perfluoroheptanesulfonic Acid	0.0952 ug/mL
							Perfluorohexanoic acid (PFHxA)	0.1 ug/mL
							Perfluorohexadecanoic acid	0.1 ug/mL
							Perfluorohexanesulfonic acid (PFHxS)	0.091 ug/mL
							Perfluorononanoic acid (PFNA)	0.1 ug/mL
							Perfluorooctanoic acid (PFOA)	0.1 ug/mL
							Perfluorooctadecanoic acid	0.1 ug/mL
							Perfluorooctanesulfonic acid (PFOS)	0.0928 ug/mL
							Perfluorooctane Sulfonamide (FOSA)	0.1 ug/mL
							Perfluoropentanoic acid (PFPeA)	0.1 ug/mL
							Perfluorotetradecanoic acid (PFTeA)	0.1 ug/mL
							Perfluorotridecanoic Acid (PFTriA)	0.1 ug/mL
							Perfluoroundecanoic acid (PFUnA)	0.1 ug/mL
..LCPFCSP_00070	05/15/17	11/15/16	Methanol, Lot 090285	10000 uL	LCPFBA_00005	100 uL	Perfluorobutanoic acid (PFBA)	0.5 ug/mL
					LCPFBS_00005	100 uL	Perfluorobutanesulfonic acid (PFBS)	0.442 ug/mL
					LCPFDA_00005	100 uL	Perfluorodecanoic acid (PFDA)	0.5 ug/mL
					LCPFDoA_00005	100 uL	Perfluorododecanoic acid (PFDoA)	0.5 ug/mL
					LCPFDS_00006	100 uL	Perfluorodecanesulfonic acid (PFDS)	0.482 ug/mL
					LCPFHpA_00005	100 uL	Perfluoroheptanoic acid (PFHpA)	0.5 ug/mL
					LCPFHpS_00009	100 uL	Perfluoroheptanesulfonic Acid	0.476 ug/mL
					LCPFHxA_00004	100 uL	Perfluorohexanoic acid (PFHxA)	0.5 ug/mL
					LCPFHxDA_00006	100 uL	Perfluorohexadecanoic acid	0.5 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LCPFHxS-br_00002	100 uL	Perfluorohexanesulfonic acid (PFHxS)	0.455 ug/mL
					LCPFNA_00005	100 uL	Perfluorononanoic acid (PFNA)	0.5 ug/mL
					LCPFDA_00006	100 uL	Perfluorooctanoic acid (PFOA)	0.5 ug/mL
					LCPFODA_00005	100 uL	Perfluorooctadecanoic acid	0.5 ug/mL
					LCPFOS-br_00002	100 uL	Perfluorooctanesulfonic acid (PFOS)	0.464 ug/mL
					LCPFOSA_00006	100 uL	Perfluorooctane Sulfonamide (FOSA)	0.5 ug/mL
					LCPPeA_00005	100 uL	Perfluoropentanoic acid (PFPeA)	0.5 ug/mL
					LCPFTEda_00004	100 uL	Perfluorotetradecanoic acid (PFTEa)	0.5 ug/mL
					LCPFTrDA_00004	100 uL	Perfluorotridecanoic Acid (PFTriA)	0.5 ug/mL
					LCPFUDA_00005	100 uL	Perfluoroundecanoic acid (PFUnA)	0.5 ug/mL
...LCPFBA_00005	05/27/21	Wellington Laboratories, Lot PFBA0516			(Purchased Reagent)		Perfluorobutanoic acid (PFBA)	50 ug/mL
...LCPFBS_00005	03/15/21	Wellington Laboratories, Lot LPFBS0316			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	44.2 ug/mL
...LCPFDA_00005	07/02/20	Wellington Laboratories, Lot PFDA0615			(Purchased Reagent)		Perfluorodecanoic acid (PFDA)	50 ug/mL
...LCPFDoA_00005	01/30/20	Wellington Laboratories, Lot PFDoA0115			(Purchased Reagent)		Perfluorododecanoic acid (PFDoA)	50 ug/mL
...LCPFDS_00006	05/24/21	Wellington Laboratories, Lot LPFDS0516			(Purchased Reagent)		Perfluorodecanesulfonic acid (PFDS)	48.2 ug/mL
...LCPFHpa_00005	01/22/21	Wellington Laboratories, Lot PFHpA0116			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	50 ug/mL
...LCPFHps_00009	11/06/20	Wellington Laboratories, Lot LPFHpS1115			(Purchased Reagent)		Perfluoroheptanesulfonic Acid (PFHpA)	47.6 ug/mL
...LCPFHxA_00004	12/22/20	Wellington Laboratories, Lot PFHxA1215			(Purchased Reagent)		Perfluorohexanoic acid (PFHxA)	50 ug/mL
...LCPFHxDA_00006	05/25/21	Wellington Laboratories, Lot PFHxDA0516			(Purchased Reagent)		Perfluorohexadecanoic acid	50 ug/mL
...LCPFHxS-br_00002	07/03/20	Wellington Laboratories, Lot brPFHxSK0615			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	45.5 ug/mL
...LCPFNA_00005	10/23/20	Wellington Laboratories, Lot PFNA1015			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	50 ug/mL
...LCPFOA_00006	11/06/20	Wellington Laboratories, Lot PFOA1115			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	50 ug/mL
...LCPFODA_00005	01/30/20	Wellington Laboratories, Lot PFODA0115			(Purchased Reagent)		Perfluorooctadecanoic acid	50 ug/mL
...LCPFOS-br_00002	10/14/20	Wellington Laboratories, Lot brPFOSK1015			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	46.4 ug/mL
...LCPFOSA_00006	09/02/17	Wellington Laboratories, Lot FOSA0815I			(Purchased Reagent)		Perfluorooctane Sulfonamide (FOSA)	50 ug/mL
...LCPPeA_00005	01/30/20	Wellington Laboratories, Lot PFPeA0115			(Purchased Reagent)		Perfluoropentanoic acid (PFPeA)	50 ug/mL
...LCPFTEda_00004	12/09/20	Wellington Laboratories, Lot PFTeDA1215			(Purchased Reagent)		Perfluorotetradecanoic acid (PFTEa)	50 ug/mL
...LCPFTrDA_00004	12/10/18	Wellington Laboratories, Lot PFTTrDA1213			(Purchased Reagent)		Perfluorotridecanoic Acid (PFTriA)	50 ug/mL
...LCPFUDA_00005	08/19/20	Wellington Laboratories, Lot PFUDA0815			(Purchased Reagent)		Perfluoroundecanoic acid (PFUnA)	50 ug/mL
LCPFC-L2_00023	05/15/17	12/15/16	MeOH/H2O, Lot 090285	5 mL	LCMPFCSU_00047	250 uL	13C2-PFHxDA 13C2-PFTEda	50 ng/mL 50 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration		
					Reagent ID	Volume Added				
							13C4-PFHpA	50 ng/mL		
							13C5 PFPeA	50 ng/mL		
							13C8 FOSA	50 ng/mL		
							13C4 PFBA	50 ng/mL		
							13C2 PFDA	50 ng/mL		
							13C2 PFDoA	50 ng/mL		
							13C2 PFHxA	50 ng/mL		
							1802 PFHxS	47.3 ng/mL		
							13C5 PFNA	50 ng/mL		
							13C4 PFOA	50 ng/mL		
							13C4 PFOS	47.8 ng/mL		
							13C2 PFUnA	50 ng/mL		
							LCPFCSU_00071	50 uL	Perfluorobutanoic acid (PFBA)	1 ng/mL
									Perfluorobutanesulfonic acid (PFBS)	0.884 ng/mL
							Perfluorodecanoic acid (PFDA)	1 ng/mL		
							Perfluorododecanoic acid (PFDoA)	1 ng/mL		
							Perfluorodecanesulfonic acid (PFDS)	0.964 ng/mL		
							Perfluoroheptanoic acid (PFHpA)	1 ng/mL		
							Perfluoroheptanesulfonic Acid	0.952 ng/mL		
							Perfluorohexanoic acid (PFHxA)	1 ng/mL		
							Perfluorohexadecanoic acid	1 ng/mL		
							Perfluorohexanesulfonic acid (PFHxS)	0.91 ng/mL		
							Perfluorononanoic acid (PFNA)	1 ng/mL		
							Perfluorooctanoic acid (PFOA)	1 ng/mL		
							Perfluorooctadecanoic acid	1 ng/mL		
							Perfluorooctanesulfonic acid (PFOS)	0.928 ng/mL		
		Perfluorooctane Sulfonamide (FOSA)	1 ng/mL							
		Perfluoropentanoic acid (PFPeA)	1 ng/mL							
		Perfluorotetradecanoic acid (PFTeA)	1 ng/mL							
		Perfluorotridecanoic Acid (PFTriA)	1 ng/mL							
		Perfluoroundecanoic acid (PFUnA)	1 ng/mL							
.LCMPFCSU_00047	06/14/17	12/14/16	Methanol, Lot Baker 144541	50000 uL	LCM2PFHxDA_00008	1000 uL	13C2-PFHxDA	1 ug/mL		
					LCM2PFTeDA_00007	1000 uL	13C2-PFTeDA	1 ug/mL		
					LCM4PFHPA_00007	1000 uL	13C4-PFHpA	1 ug/mL		
					LCM5PFPEA_00008	1000 uL	13C5 PFPeA	1 ug/mL		
					LCM8FOSA_00011	1000 uL	13C8 FOSA	1 ug/mL		
					LCMPFBA_00008	1000 uL	13C4 PFBA	1 ug/mL		

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LCMPFDA 00011	1000 uL	13C2 PFDA	1 ug/mL
					LCMPFDoA 00008	1000 uL	13C2 PFDoA	1 ug/mL
					LCMPFHxA 00012	1000 uL	13C2 PFHxA	1 ug/mL
					LCMPFHxS 00008	1000 uL	18O2 PFHxS	0.946 ug/mL
					LCMPFNA 00008	1000 uL	13C5 PFNA	1 ug/mL
					LCMPFOA 00012	1000 uL	13C4 PFOA	1 ug/mL
					LCMPFOS 00017	1000 uL	13C4 PFOS	0.956 ug/mL
					LCMPFUDa 00009	1000 uL	13C2 PFUnA	1 ug/mL
..LCM2PFHxDA 00008	01/07/21		Wellington Laboratories, Lot M2PFHxDA1112		(Purchased Reagent)		13C2-PFHxDA	50 ug/mL
..LCM2PFTeDA 00007	12/07/20		Wellington Laboratories, Lot M2PFTeDA1115		(Purchased Reagent)		13C2-PFTeDA	50 ug/mL
..LCM4PFHPA 00007	05/27/21		Wellington Laboratories, Lot M4PFHPA0516		(Purchased Reagent)		13C4-PFHpa	50 ug/mL
..LCM5PFPEA 00008	05/22/20		Wellington Laboratories, Lot M5PFPeA0515		(Purchased Reagent)		13C5 PFPeA	50 ug/mL
..LCM8FOSA 00011	12/22/17		Wellington Laboratories, Lot M8FOSA1215I		(Purchased Reagent)		13C8 FOSA	50 ug/mL
..LCMPFBA 00008	05/24/21		Wellington Laboratories, Lot MPFBA0516		(Purchased Reagent)		13C4 PFBA	50 ug/mL
..LCMPFDA 00011	08/19/20		Wellington Laboratories, Lot MPFDA0815		(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFDoA 00008	04/08/21		Wellington Laboratories, Lot MPFDoA0416		(Purchased Reagent)		13C2 PFDoA	50 ug/mL
..LCMPFHxA 00012	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL
..LCMPFHxS 00008	10/23/20		Wellington Laboratories, Lot MPFHxS1015		(Purchased Reagent)		18O2 PFHxS	47.3 ug/mL
..LCMPFNA 00008	04/13/19		Wellington Laboratories, Lot MPFNA0414		(Purchased Reagent)		13C5 PFNA	50 ug/mL
..LCMPFOA 00012	01/22/21		Wellington Laboratories, Lot MPFOA0116		(Purchased Reagent)		13C4 PFOA	50 ug/mL
..LCMPFOS 00017	08/03/21		Wellington Laboratories, Lot MPFOS0816		(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
..LCMPFUDa 00009	02/12/21		Wellington Laboratories, Lot MPFUDa0216		(Purchased Reagent)		13C2 PFUnA	50 ug/mL
.LCPFCSP_00071	05/15/17	11/10/16	Methanol, Lot 090285	10000 uL	LCPFCSP_00070	2000 uL	Perfluorobutanoic acid (PFBA)	0.1 ug/mL
							Perfluorobutanesulfonic acid (PFBS)	0.0884 ug/mL
							Perfluorodecanoic acid (PFDA)	0.1 ug/mL
							Perfluorododecanoic acid (PFDoA)	0.1 ug/mL
							Perfluorodecanesulfonic acid (PFDS)	0.0964 ug/mL
							Perfluoroheptanoic acid (PFHpA)	0.1 ug/mL
							Perfluoroheptanesulfonic Acid	0.0952 ug/mL
							Perfluorohexanoic acid (PFHxA)	0.1 ug/mL
							Perfluorohexadecanoic acid	0.1 ug/mL
							Perfluorohexanesulfonic acid (PFHxS)	0.091 ug/mL
							Perfluorononanoic acid (PFNA)	0.1 ug/mL
							Perfluorooctanoic acid (PFOA)	0.1 ug/mL
							Perfluorooctadecanoic acid	0.1 ug/mL
							Perfluorooctanesulfonic acid (PFOS)	0.0928 ug/mL
							Perfluorooctane Sulfonamide (FOSA)	0.1 ug/mL
							Perfluoropentanoic acid (PFPeA)	0.1 ug/mL
							Perfluorotetradecanoic acid (PFTeA)	0.1 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Perfluorotridecanoic Acid (PFTriA)	0.1 ug/mL
							Perfluoroundecanoic acid (PFUnA)	0.1 ug/mL
..LCPFCSP_00070	05/15/17	11/15/16	Methanol, Lot 090285	10000 uL	LCPFBA_00005	100 uL	Perfluorobutanoic acid (PFBA)	0.5 ug/mL
					LCPFBS_00005	100 uL	Perfluorobutanesulfonic acid (PFBS)	0.442 ug/mL
					LCPFDA_00005	100 uL	Perfluorodecanoic acid (PFDA)	0.5 ug/mL
					LCPFDoA_00005	100 uL	Perfluorododecanoic acid (PFDoA)	0.5 ug/mL
					LCPFDS_00006	100 uL	Perfluorodecanesulfonic acid (PFDS)	0.482 ug/mL
					LCPFHpA_00005	100 uL	Perfluoroheptanoic acid (PFHpA)	0.5 ug/mL
					LCPFHpS_00009	100 uL	Perfluoroheptanesulfonic Acid	0.476 ug/mL
					LCPFHxA_00004	100 uL	Perfluorohexanoic acid (PFHxA)	0.5 ug/mL
					LCPFHxDA_00006	100 uL	Perfluorohexadecanoic acid	0.5 ug/mL
					LCPFHxS-br_00002	100 uL	Perfluorohexanesulfonic acid (PFHxS)	0.455 ug/mL
					LCPFNA_00005	100 uL	Perfluorononanoic acid (PFNA)	0.5 ug/mL
					LCPFOA_00006	100 uL	Perfluorooctanoic acid (PFOA)	0.5 ug/mL
					LCPFODA_00005	100 uL	Perfluorooctadecanoic acid	0.5 ug/mL
					LCPFOS-br_00002	100 uL	Perfluorooctanesulfonic acid (PFOS)	0.464 ug/mL
					LCPFOSA_00006	100 uL	Perfluorooctane Sulfonamide (FOSA)	0.5 ug/mL
					LCPFPeA_00005	100 uL	Perfluoropentanoic acid (PFPeA)	0.5 ug/mL
					LCPFTeDA_00004	100 uL	Perfluorotetradecanoic acid (PFTeA)	0.5 ug/mL
					LCPFTrDA_00004	100 uL	Perfluorotridecanoic Acid (PFTriA)	0.5 ug/mL
					LCPFUdA_00005	100 uL	Perfluoroundecanoic acid (PFUnA)	0.5 ug/mL
...LCPFBA_00005	05/27/21		Wellington Laboratories, Lot PFBA0516		(Purchased Reagent)		Perfluorobutanoic acid (PFBA)	50 ug/mL
...LCPFBS_00005	03/15/21		Wellington Laboratories, Lot LPFBS0316		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	44.2 ug/mL
...LCPFDA_00005	07/02/20		Wellington Laboratories, Lot PFDA0615		(Purchased Reagent)		Perfluorodecanoic acid (PFDA)	50 ug/mL
...LCPFDoA_00005	01/30/20		Wellington Laboratories, Lot PFDoA0115		(Purchased Reagent)		Perfluorododecanoic acid (PFDoA)	50 ug/mL
...LCPFDS_00006	05/24/21		Wellington Laboratories, Lot LPFDS0516		(Purchased Reagent)		Perfluorodecanesulfonic acid (PFDS)	48.2 ug/mL
...LCPFHpA_00005	01/22/21		Wellington Laboratories, Lot PFHpA0116		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	50 ug/mL
...LCPFHpS_00009	11/06/20		Wellington Laboratories, Lot LPFHpS1115		(Purchased Reagent)		Perfluoroheptanesulfonic Acid	47.6 ug/mL
...LCPFHxA_00004	12/22/20		Wellington Laboratories, Lot PFHxA1215		(Purchased Reagent)		Perfluorohexanoic acid (PFHxA)	50 ug/mL
...LCPFHxDA_00006	05/25/21		Wellington Laboratories, Lot PFHxDA0516		(Purchased Reagent)		Perfluorohexadecanoic acid	50 ug/mL
...LCPFHxS-br_00002	07/03/20		Wellington Laboratories, Lot brPFHxSK0615		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	45.5 ug/mL
...LCPFNA_00005	10/23/20		Wellington Laboratories, Lot PFNA1015		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	50 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
...LCPFOA_00006	11/06/20		Wellington Laboratories, Lot PFOA1115		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	50 ug/mL
...LCPFODA_00005	01/30/20		Wellington Laboratories, Lot PFODA0115		(Purchased Reagent)		Perfluorooctadecanoic acid	50 ug/mL
...LCPFOS-br_00002	10/14/20		Wellington Laboratories, Lot brPFOSK1015		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	46.4 ug/mL
...LCPFOSA_00006	09/02/17		Wellington Laboratories, Lot FOSA0815I		(Purchased Reagent)		Perfluorooctane Sulfonamide (FOSA)	50 ug/mL
...LCPFPeA_00005	01/30/20		Wellington Laboratories, Lot PFPeA0115		(Purchased Reagent)		Perfluoropentanoic acid (PFPeA)	50 ug/mL
...LCPFTeDA_00004	12/09/20		Wellington Laboratories, Lot PFTeDA1215		(Purchased Reagent)		Perfluorotetradecanoic acid (PFTeA)	50 ug/mL
...LCPFTrDA_00004	12/10/18		Wellington Laboratories, Lot PFTrDA1213		(Purchased Reagent)		Perfluorotridecanoic Acid (PFTriA)	50 ug/mL
...LCPFUdA_00005	08/19/20		Wellington Laboratories, Lot PFUdA0815		(Purchased Reagent)		Perfluoroundecanoic acid (PFUnA)	50 ug/mL
LCPFC-L3_00020	05/15/17	12/15/16	MeOH/H2O, Lot 090285	5 mL	LCMPFCSU_00047	250 uL	13C2-PFHxDA	50 ng/mL
							13C2-PFTeDA	50 ng/mL
							13C4-PFHpA	50 ng/mL
							13C5 PFPeA	50 ng/mL
							13C8 FOSA	50 ng/mL
							13C4 PFBA	50 ng/mL
							13C2 PFDA	50 ng/mL
							13C2 PFDoA	50 ng/mL
							13C2 PFHxA	50 ng/mL
							18O2 PFHxS	47.3 ng/mL
							13C5 PFNA	50 ng/mL
							13C4 PFOA	50 ng/mL
							13C4 PFOS	47.8 ng/mL
							13C2 PFUnA	50 ng/mL
					LCPFCSP_00071	250 uL	Perfluorobutanoic acid (PFBA)	5 ng/mL
							Perfluorobutanesulfonic acid (PFBS)	4.42 ng/mL
							Perfluorodecanoic acid (PFDA)	5 ng/mL
							Perfluorododecanoic acid (PFDoA)	5 ng/mL
							Perfluorodecanesulfonic acid (PFDS)	4.82 ng/mL
							Perfluoroheptanoic acid (PFHpA)	5 ng/mL
							Perfluoroheptanesulfonic Acid	4.76 ng/mL
							Perfluorohexanoic acid (PFHxA)	5 ng/mL
							Perfluorohexadecanoic acid	5 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	4.55 ng/mL
							Perfluorononanoic acid (PFNA)	5 ng/mL
							Perfluorooctanoic acid (PFOA)	5 ng/mL
Perfluorooctadecanoic acid	5 ng/mL							
Perfluorooctanesulfonic acid (PFOS)	4.64 ng/mL							

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Perfluorooctane Sulfonamide (FOSA)	5 ng/mL
							Perfluoropentanoic acid (PFPeA)	5 ng/mL
							Perfluorotetradecanoic acid (PFTeA)	5 ng/mL
							Perfluorotridecanoic Acid (PFTriA)	5 ng/mL
							Perfluoroundecanoic acid (PFUnA)	5 ng/mL
.LCMPFCSU_00047	06/14/17	12/14/16	Methanol, Lot Baker 144541	50000 uL	LCM2PFHxDA_00008	1000 uL	13C2-PFHxDA	1 ug/mL
					LCM2PFTeDA_00007	1000 uL	13C2-PFTeDA	1 ug/mL
					LCM4PFHPA_00007	1000 uL	13C4-PFHpa	1 ug/mL
					LCM5PFPEA_00008	1000 uL	13C5 PFPeA	1 ug/mL
					LCM8FOSA_00011	1000 uL	13C8 FOSA	1 ug/mL
					LCMPFBA_00008	1000 uL	13C4 PFBA	1 ug/mL
					LCMPFDA_00011	1000 uL	13C2 PFDA	1 ug/mL
					LCMPFDoA_00008	1000 uL	13C2 PFDoA	1 ug/mL
					LCMPFHxA_00012	1000 uL	13C2 PFHxA	1 ug/mL
					LCMPFHxS_00008	1000 uL	18O2 PFHxS	0.946 ug/mL
					LCMPFNA_00008	1000 uL	13C5 PFNA	1 ug/mL
					LCMPFOA_00012	1000 uL	13C4 PFOA	1 ug/mL
					LCMPFOS_00017	1000 uL	13C4 PFOS	0.956 ug/mL
					LCMPFUDa_00009	1000 uL	13C2 PFUnA	1 ug/mL
..LCM2PFHxDA_00008	01/07/21	Wellington Laboratories, Lot M2PFHxDA1112			(Purchased Reagent)		13C2-PFHxDA	50 ug/mL
..LCM2PFTeDA_00007	12/07/20	Wellington Laboratories, Lot M2PFTeDA1115			(Purchased Reagent)		13C2-PFTeDA	50 ug/mL
..LCM4PFHPA_00007	05/27/21	Wellington Laboratories, Lot M4PFHpA0516			(Purchased Reagent)		13C4-PFHpa	50 ug/mL
..LCM5PFPEA_00008	05/22/20	Wellington Laboratories, Lot M5PFPeA0515			(Purchased Reagent)		13C5 PFPeA	50 ug/mL
..LCM8FOSA_00011	12/22/17	Wellington Laboratories, Lot M8FOSA1215I			(Purchased Reagent)		13C8 FOSA	50 ug/mL
..LCMPFBA_00008	05/24/21	Wellington Laboratories, Lot MPFBA0516			(Purchased Reagent)		13C4 PFBA	50 ug/mL
..LCMPFDA_00011	08/19/20	Wellington Laboratories, Lot MPFDA0815			(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFDoA_00008	04/08/21	Wellington Laboratories, Lot MPFDoA0416			(Purchased Reagent)		13C2 PFDoA	50 ug/mL
..LCMPFHxA_00012	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)		13C2 PFHxA	50 ug/mL
..LCMPFHxS_00008	10/23/20	Wellington Laboratories, Lot MPFHxS1015			(Purchased Reagent)		18O2 PFHxS	47.3 ug/mL
..LCMPFNA_00008	04/13/19	Wellington Laboratories, Lot MPFNA0414			(Purchased Reagent)		13C5 PFNA	50 ug/mL
..LCMPFOA_00012	01/22/21	Wellington Laboratories, Lot MPFOA0116			(Purchased Reagent)		13C4 PFOA	50 ug/mL
..LCMPFOS_00017	08/03/21	Wellington Laboratories, Lot MPFOS0816			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
..LCMPFUDa_00009	02/12/21	Wellington Laboratories, Lot MPFUDa0216			(Purchased Reagent)		13C2 PFUnA	50 ug/mL
.LCPFCSP_00071	05/15/17	11/10/16	Methanol, Lot 090285	10000 uL	LCPFCSP_00070	2000 uL	Perfluorobutanoic acid (PFBA)	0.1 ug/mL
							Perfluorobutanesulfonic acid (PFBS)	0.0884 ug/mL
							Perfluorodecanoic acid (PFDA)	0.1 ug/mL
							Perfluorododecanoic acid (PFDoA)	0.1 ug/mL
							Perfluorodecanesulfonic acid (PFDS)	0.0964 ug/mL
							Perfluoroheptanoic acid (PFHpA)	0.1 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Perfluoroheptanesulfonic Acid	0.0952 ug/mL
							Perfluorohexanoic acid (PFHxA)	0.1 ug/mL
							Perfluorohexadecanoic acid	0.1 ug/mL
							Perfluorohexanesulfonic acid (PFHxS)	0.091 ug/mL
							Perfluorononanoic acid (PFNA)	0.1 ug/mL
							Perfluorooctanoic acid (PFOA)	0.1 ug/mL
							Perfluorooctadecanoic acid	0.1 ug/mL
							Perfluorooctanesulfonic acid (PFOS)	0.0928 ug/mL
							Perfluorooctane Sulfonamide (FOSA)	0.1 ug/mL
							Perfluoropentanoic acid (PFPeA)	0.1 ug/mL
							Perfluorotetradecanoic acid (PFTeA)	0.1 ug/mL
							Perfluorotridecanoic Acid (PFTriA)	0.1 ug/mL
							Perfluoroundecanoic acid (PFUnA)	0.1 ug/mL
..LCPFCSP_00070	05/15/17	11/15/16	Methanol, Lot 090285	10000 uL	LCPFBA_00005	100 uL	Perfluorobutanoic acid (PFBA)	0.5 ug/mL
					LCPFBS_00005	100 uL	Perfluorobutanesulfonic acid (PFBS)	0.442 ug/mL
					LCPFDA_00005	100 uL	Perfluorodecanoic acid (PFDA)	0.5 ug/mL
					LCPFDoA_00005	100 uL	Perfluorododecanoic acid (PFDoA)	0.5 ug/mL
					LCPFDS_00006	100 uL	Perfluorodecanesulfonic acid (PFDS)	0.482 ug/mL
					LCPFHpA_00005	100 uL	Perfluoroheptanoic acid (PFHpA)	0.5 ug/mL
					LCPFHpS_00009	100 uL	Perfluoroheptanesulfonic Acid	0.476 ug/mL
					LCPFHxA_00004	100 uL	Perfluorohexanoic acid (PFHxA)	0.5 ug/mL
					LCPFHxDA_00006	100 uL	Perfluorohexadecanoic acid	0.5 ug/mL
					LCPFHxS-br_00002	100 uL	Perfluorohexanesulfonic acid (PFHxS)	0.455 ug/mL
					LCPFNA_00005	100 uL	Perfluorononanoic acid (PFNA)	0.5 ug/mL
					LCPFOA_00006	100 uL	Perfluorooctanoic acid (PFOA)	0.5 ug/mL
					LCPFODA_00005	100 uL	Perfluorooctadecanoic acid	0.5 ug/mL
					LCPFOS-br_00002	100 uL	Perfluorooctanesulfonic acid (PFOS)	0.464 ug/mL
					LCPFOSA_00006	100 uL	Perfluorooctane Sulfonamide (FOSA)	0.5 ug/mL
					LCPFPeA_00005	100 uL	Perfluoropentanoic acid (PFPeA)	0.5 ug/mL
					LCPFTeDA_00004	100 uL	Perfluorotetradecanoic acid (PFTeA)	0.5 ug/mL
					LCPFTriDA_00004	100 uL	Perfluorotridecanoic Acid (PFTriA)	0.5 ug/mL
					LCPFUdA_00005	100 uL	Perfluoroundecanoic acid (PFUnA)	0.5 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration		
					Reagent ID	Volume Added				
...LCPFBFA_00005	05/27/21		Wellington Laboratories, Lot PFBA0516		(Purchased Reagent)		Perfluorobutanoic acid (PFBA)	50 ug/mL		
...LCPFBFS_00005	03/15/21		Wellington Laboratories, Lot LPPBFS0316		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	44.2 ug/mL		
...LCPFDA_00005	07/02/20		Wellington Laboratories, Lot PFDA0615		(Purchased Reagent)		Perfluorodecanoic acid (PFDA)	50 ug/mL		
...LCPFDoA_00005	01/30/20		Wellington Laboratories, Lot PFDoA0115		(Purchased Reagent)		Perfluorododecanoic acid (PFDoA)	50 ug/mL		
...LCPFDS_00006	05/24/21		Wellington Laboratories, Lot LPPFDS0516		(Purchased Reagent)		Perfluorodecanesulfonic acid (PFDS)	48.2 ug/mL		
...LCPFHpA_00005	01/22/21		Wellington Laboratories, Lot PFHpA0116		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	50 ug/mL		
...LCPFHpS_00009	11/06/20		Wellington Laboratories, Lot LPPFHpS1115		(Purchased Reagent)		Perfluoroheptanesulfonic Acid	47.6 ug/mL		
...LCPFHxA_00004	12/22/20		Wellington Laboratories, Lot PFHxA1215		(Purchased Reagent)		Perfluorohexanoic acid (PFHxA)	50 ug/mL		
...LCPFHxDA_00006	05/25/21		Wellington Laboratories, Lot PFHxDA0516		(Purchased Reagent)		Perfluorohexadecanoic acid	50 ug/mL		
...LCPFHxS-br_00002	07/03/20		Wellington Laboratories, Lot brPFHxSK0615		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	45.5 ug/mL		
...LCPFNA_00005	10/23/20		Wellington Laboratories, Lot PFNA1015		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	50 ug/mL		
...LCPFOA_00006	11/06/20		Wellington Laboratories, Lot PFOA1115		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	50 ug/mL		
...LCPFOA_00005	01/30/20		Wellington Laboratories, Lot PFOA0115		(Purchased Reagent)		Perfluorooctadecanoic acid	50 ug/mL		
...LCPFOS-br_00002	10/14/20		Wellington Laboratories, Lot brPFOSK1015		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	46.4 ug/mL		
...LCPFOSA_00006	09/02/17		Wellington Laboratories, Lot FOSA0815I		(Purchased Reagent)		Perfluorooctane Sulfonamide (FOSA)	50 ug/mL		
...LCPFPeA_00005	01/30/20		Wellington Laboratories, Lot PFPeA0115		(Purchased Reagent)		Perfluoropentanoic acid (PFPeA)	50 ug/mL		
...LCPFTeDA_00004	12/09/20		Wellington Laboratories, Lot PFTeDA1215		(Purchased Reagent)		Perfluorotetradecanoic acid (PFTeA)	50 ug/mL		
...LCPFTrDA_00004	12/10/18		Wellington Laboratories, Lot PFTrDA1213		(Purchased Reagent)		Perfluorotridecanoic Acid (PFTrA)	50 ug/mL		
...LCPFUdA_00005	08/19/20		Wellington Laboratories, Lot PFUdA0815		(Purchased Reagent)		Perfluoroundecanoic acid (PFUnA)	50 ug/mL		
LCPFC-L4_00024	06/14/17	12/15/16	MeOH/H2O, Lot 090285	5 mL	LCMPFCSU_00047	250 uL	13C2-PFHxDA	50 ng/mL		
							13C2-PFTeDA	50 ng/mL		
							13C4-PFHpA	50 ng/mL		
							13C5 PFPeA	50 ng/mL		
							13C8 FOSA	50 ng/mL		
							13C4 PFBA	50 ng/mL		
							13C2 PFDA	50 ng/mL		
							13C2 PFDoA	50 ng/mL		
							13C2 PFHxA	50 ng/mL		
							18O2 PFHxS	47.3 ng/mL		
							13C5 PFNA	50 ng/mL		
							13C4 PFOA	50 ng/mL		
							13C4 PFOS	47.8 ng/mL		
							13C2 PFUnA	50 ng/mL		
							LCPFCSP_00074	100 uL	Perfluorobutanoic acid (PFBA)	20 ng/mL
									Perfluorobutanesulfonic acid (PFBS)	17.68 ng/mL
		Perfluorodecanoic acid (PFDA)	20 ng/mL							

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration	
					Reagent ID	Volume Added			
							Perfluorododecanoic acid (PFDoA)	20 ng/mL	
							Perfluorodecanesulfonic acid (PFDS)	19.28 ng/mL	
							Perfluoroheptanoic acid (PFHpA)	20 ng/mL	
							Perfluoroheptanesulfonic Acid (PFHxA)	19.04 ng/mL	
							Perfluorohexanoic acid (PFHxA)	20 ng/mL	
							Perfluorohexadecanoic acid	20 ng/mL	
							Perfluorohexanesulfonic acid (PFHxS)	18.2 ng/mL	
							Perfluorononanoic acid (PFNA)	20 ng/mL	
							Perfluorooctanoic acid (PFOA)	20 ng/mL	
							Perfluorooctadecanoic acid	20 ng/mL	
							Perfluorooctanesulfonic acid (PFOS)	18.56 ng/mL	
							Perfluorooctane Sulfonamide (FOSA)	20 ng/mL	
							Perfluoropentanoic acid (PFPeA)	20 ng/mL	
							Perfluorotetradecanoic acid (PFTeA)	20 ng/mL	
							Perfluorotridecanoic Acid (PFTriA)	20 ng/mL	
							Perfluoroundecanoic acid (PFUnA)	20 ng/mL	
.LCMPFCSU_00047	06/14/17	12/14/16	Methanol, Lot Baker 144541	50000 uL	LCM2PFHxDA_00008	1000 uL	13C2-PFHxDA	1 ug/mL	
					LCM2PFTeDA_00007	1000 uL	13C2-PFTeDA	1 ug/mL	
					LCM4PFHHPA_00007	1000 uL	13C4-PFHHPA	1 ug/mL	
					LCM5PFPEA_00008	1000 uL	13C5 PFPeA	1 ug/mL	
					LCM8FOSA_00011	1000 uL	13C8 FOSA	1 ug/mL	
					LCMPFBA_00008	1000 uL	13C4 PFBA	1 ug/mL	
					LCMPFDA_00011	1000 uL	13C2 PFDA	1 ug/mL	
					LCMPFDoA_00008	1000 uL	13C2 PFDoA	1 ug/mL	
					LCMPFHxA_00012	1000 uL	13C2 PFHxA	1 ug/mL	
					LCMPFHxS_00008	1000 uL	1802 PFHxS	0.946 ug/mL	
					LCMPFNA_00008	1000 uL	13C5 PFNA	1 ug/mL	
					LCMPFOA_00012	1000 uL	13C4 PFOA	1 ug/mL	
					LCMPFOS_00017	1000 uL	13C4 PFOS	0.956 ug/mL	
					LCMPFUdA_00009	1000 uL	13C2 PFUnA	1 ug/mL	
..LCM2PFHxDA_00008	01/07/21		Wellington Laboratories, Lot M2PFHxDA1112				(Purchased Reagent)	13C2-PFHxDA	50 ug/mL
..LCM2PFTeDA_00007	12/07/20		Wellington Laboratories, Lot M2PFTeDA1115				(Purchased Reagent)	13C2-PFTeDA	50 ug/mL
..LCM4PFHHPA_00007	05/27/21		Wellington Laboratories, Lot M4PFHHPA0516				(Purchased Reagent)	13C4-PFHHPA	50 ug/mL
..LCM5PFPEA_00008	05/22/20		Wellington Laboratories, Lot M5PFPeA0515				(Purchased Reagent)	13C5 PFPeA	50 ug/mL
..LCM8FOSA_00011	12/22/17		Wellington Laboratories, Lot M8FOSA1215I				(Purchased Reagent)	13C8 FOSA	50 ug/mL
..LCMPFBA_00008	05/24/21		Wellington Laboratories, Lot MPFBA0516				(Purchased Reagent)	13C4 PFBA	50 ug/mL
..LCMPFDA_00011	08/19/20		Wellington Laboratories, Lot MPFDA0815				(Purchased Reagent)	13C2 PFDA	50 ug/mL
..LCMPFDoA_00008	04/08/21		Wellington Laboratories, Lot MPFDoA0416				(Purchased Reagent)	13C2 PFDoA	50 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
..LCMPFHxA 00012	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL
..LCMPFHxS 00008	10/23/20		Wellington Laboratories, Lot MPFHxS1015		(Purchased Reagent)		18O2 PFHxS	47.3 ug/mL
..LCMPFNA 00008	04/13/19		Wellington Laboratories, Lot MPFNA0414		(Purchased Reagent)		13C5 PFNA	50 ug/mL
..LCMPFOA 00012	01/22/21		Wellington Laboratories, Lot MPFOA0116		(Purchased Reagent)		13C4 PFOA	50 ug/mL
..LCMPFOS 00017	08/03/21		Wellington Laboratories, Lot MPFOS0816		(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
..LCMPFUDa 00009	02/12/21		Wellington Laboratories, Lot MPFUDa0216		(Purchased Reagent)		13C2 PFUnA	50 ug/mL
.LCPFCSP_00074	06/14/17	12/14/16	Methanol, Lot 090285	10000 uL	LCPFBA_00005	200 uL	Perfluorobutanoic acid (PFBA)	1 ug/mL
					LCPFBS_00005	200 uL	Perfluorobutanesulfonic acid (PFBS)	0.884 ug/mL
					LCPFDA_00005	200 uL	Perfluorodecanoic acid (PFDA)	1 ug/mL
					LCPFDoA_00005	200 uL	Perfluorododecanoic acid (PFDoA)	1 ug/mL
					LCPFDS_00006	200 uL	Perfluorodecanesulfonic acid (PFDS)	0.964 ug/mL
					LCPFHpA_00006	200 uL	Perfluoroheptanoic acid (PFHpA)	1 ug/mL
					LCPFHpS_00009	200 uL	Perfluoroheptanesulfonic Acid	0.952 ug/mL
					LCPFHxA_00005	200 uL	Perfluorohexanoic acid (PFHxA)	1 ug/mL
					LCPFHxDA_00006	200 uL	Perfluorohexadecanoic acid	1 ug/mL
					LCPFHxS-br_00002	200 uL	Perfluorohexanesulfonic acid (PFHxS)	0.91 ug/mL
					LCPFNA_00006	200 uL	Perfluorononanoic acid (PFNA)	1 ug/mL
					LCPFOA_00006	200 uL	Perfluorooctanoic acid (PFOA)	1 ug/mL
					LCPFODA_00006	200 uL	Perfluorooctadecanoic acid	1 ug/mL
					LCPFOS-br_00002	200 uL	Perfluorooctanesulfonic acid (PFOS)	0.928 ug/mL
					LCPFOSA_00008	200 uL	Perfluorooctane Sulfonamide (FOSA)	1 ug/mL
					LCPFPeA_00005	200 uL	Perfluoropentanoic acid (PFPeA)	1 ug/mL
					LCPFTeDA_00005	200 uL	Perfluorotetradecanoic acid (PFTeA)	1 ug/mL
					LCPFTriDA_00005	200 uL	Perfluorotridecanoic Acid (PFTriA)	1 ug/mL
					LCPFUdA_00005	200 uL	Perfluoroundecanoic acid (PFUnA)	1 ug/mL
..LCPFBA 00005	05/27/21		Wellington Laboratories, Lot PFBA0516		(Purchased Reagent)		Perfluorobutanoic acid (PFBA)	50 ug/mL
..LCPFBS_00005	03/15/21		Wellington Laboratories, Lot LPFBS0316		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	44.2 ug/mL
..LCPFDA_00005	07/02/20		Wellington Laboratories, Lot PFDA0615		(Purchased Reagent)		Perfluorodecanoic acid (PFDA)	50 ug/mL
..LCPFDoA_00005	01/30/20		Wellington Laboratories, Lot PFDoA0115		(Purchased Reagent)		Perfluorododecanoic acid (PFDoA)	50 ug/mL
..LCPFDS_00006	05/24/21		Wellington Laboratories, Lot LPFDS0516		(Purchased Reagent)		Perfluorodecanesulfonic acid (PFDS)	48.2 ug/mL
..LCPFHpA_00006	01/22/21		Wellington Laboratories, Lot PFHpA0116		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	50 ug/mL
..LCPFHpS_00009	11/06/20		Wellington Laboratories, Lot LPFHpS1115		(Purchased Reagent)		Perfluoroheptanesulfonic Acid	47.6 ug/mL
..LCPFHxA_00005	12/22/20		Wellington Laboratories, Lot PFHxA1215		(Purchased Reagent)		Perfluorohexanoic acid (PFHxA)	50 ug/mL
..LCPFHxDA_00006	05/25/21		Wellington Laboratories, Lot PFHxDA0516		(Purchased Reagent)		Perfluorohexadecanoic acid	50 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
..LCPFHxS-br_00002	07/03/20	Wellington Laboratories, Lot brPFHxSK0615			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	45.5 ug/mL
..LCPFNA_00006	10/23/20	Wellington Laboratories, Lot PFNA1015			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	50 ug/mL
..LCPFOA_00006	11/06/20	Wellington Laboratories, Lot PFOA1115			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	50 ug/mL
..LCPFODA_00006	04/29/21	Wellington Laboratories, Lot PFODA0416			(Purchased Reagent)		Perfluorooctadecanoic acid	50 ug/mL
..LCPFOS-br_00002	10/14/20	Wellington Laboratories, Lot brPFOSK1015			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	46.4 ug/mL
..LCPFOSA_00008	09/02/17	Wellington Laboratories, Lot FOSA0815I			(Purchased Reagent)		Perfluorooctane Sulfonamide (FOSA)	50 ug/mL
..LCPFPeA_00005	01/30/20	Wellington Laboratories, Lot PFPeA0115			(Purchased Reagent)		Perfluoropentanoic acid (PFPeA)	50 ug/mL
..LCPFTeDA_00005	12/09/20	Wellington Laboratories, Lot PFTeDA1215			(Purchased Reagent)		Perfluorotetradecanoic acid (PFTeA)	50 ug/mL
..LCPFTrDA_00005	02/12/21	Wellington Laboratories, Lot PFTrDA0216			(Purchased Reagent)		Perfluorotridecanoic Acid (PFTriA)	50 ug/mL
..LCPFUdA_00005	08/19/20	Wellington Laboratories, Lot PFUdA0815			(Purchased Reagent)		Perfluoroundecanoic acid (PFUnA)	50 ug/mL
LCPFC-L5_00022	06/14/17	12/15/16	MeOH/H2O, Lot 090285	5 mL	LCPFCSU_00047	250 uL	13C2-PFHxDA	50 ng/mL
							13C2-PFTeDA	50 ng/mL
							13C4-PFHpA	50 ng/mL
							13C5 PFPeA	50 ng/mL
							13C8 FOSA	50 ng/mL
							13C4 PFBA	50 ng/mL
							13C2 PFDA	50 ng/mL
							13C2 PFDoA	50 ng/mL
							13C2 PFHxA	50 ng/mL
							18O2 PFHxS	47.3 ng/mL
							13C5 PFNA	50 ng/mL
							13C4 PFOA	50 ng/mL
							13C4 PFOS	47.8 ng/mL
							13C2 PFUnA	50 ng/mL
							LCPFCSP_00074	250 uL
					Perfluorobutanesulfonic acid (PFBS)	44.2 ng/mL		
					Perfluorodecanoic acid (PFDA)	50 ng/mL		
					Perfluorododecanoic acid (PFDoA)	50 ng/mL		
					Perfluorodecanesulfonic acid (PFDS)	48.2 ng/mL		
					Perfluoroheptanoic acid (PFHpA)	50 ng/mL		
					Perfluoroheptanesulfonic Acid (PFHpA)	47.6 ng/mL		
					Perfluorohexanoic acid (PFHxA)	50 ng/mL		
					Perfluorohexadecanoic acid	50 ng/mL		
Perfluorohexanesulfonic acid (PFHxS)	45.5 ng/mL							
Perfluorononanoic acid (PFNA)	50 ng/mL							
Perfluorooctanoic acid (PFOA)	50 ng/mL							
Perfluorooctadecanoic acid	50 ng/mL							

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Perfluorooctanesulfonic acid (PFOS)	46.4 ng/mL
							Perfluorooctane Sulfonamide (FOSA)	50 ng/mL
							Perfluoropentanoic acid (PFPeA)	50 ng/mL
							Perfluorotetradecanoic acid (PFTeA)	50 ng/mL
							Perfluorotridecanoic Acid (PFTriA)	50 ng/mL
							Perfluoroundecanoic acid (PFUnA)	50 ng/mL
.LCMPFCSU_00047	06/14/17	12/14/16	Methanol, Lot Baker 144541	50000 uL	LCM2PFHxDA_00008	1000 uL	13C2-PFHxDA	1 ug/mL
					LCM2PFTeDA_00007	1000 uL	13C2-PFTeDA	1 ug/mL
					LCM4PFHFA_00007	1000 uL	13C4-PFHFA	1 ug/mL
					LCM5PFPEA_00008	1000 uL	13C5 PFPeA	1 ug/mL
					LCM8FOSA_00011	1000 uL	13C8 FOSA	1 ug/mL
					LCMPFBA_00008	1000 uL	13C4 PFBA	1 ug/mL
					LCMPFDA_00011	1000 uL	13C2 PFDA	1 ug/mL
					LCMPFDoA_00008	1000 uL	13C2 PFDoA	1 ug/mL
					LCMPFHxA_00012	1000 uL	13C2 PFHxA	1 ug/mL
					LCMPFHxS_00008	1000 uL	18O2 PFHxS	0.946 ug/mL
					LCMPFNA_00008	1000 uL	13C5 PFNA	1 ug/mL
					LCMPFOA_00012	1000 uL	13C4 PFOA	1 ug/mL
					LCMPFOS_00017	1000 uL	13C4 PFOS	0.956 ug/mL
					LCMPFUdA_00009	1000 uL	13C2 PFUnA	1 ug/mL
..LCM2PFHxDA_00008	01/07/21		Wellington Laboratories, Lot M2PFHxDA1112		(Purchased Reagent)		13C2-PFHxDA	50 ug/mL
..LCM2PFTeDA_00007	12/07/20		Wellington Laboratories, Lot M2PFTeDA1115		(Purchased Reagent)		13C2-PFTeDA	50 ug/mL
..LCM4PFHFA_00007	05/27/21		Wellington Laboratories, Lot M4PFHFA0516		(Purchased Reagent)		13C4-PFHFA	50 ug/mL
..LCM5PFPEA_00008	05/22/20		Wellington Laboratories, Lot M5PFPeA0515		(Purchased Reagent)		13C5 PFPeA	50 ug/mL
..LCM8FOSA_00011	12/22/17		Wellington Laboratories, Lot M8FOSA1215I		(Purchased Reagent)		13C8 FOSA	50 ug/mL
..LCMPFBA_00008	05/24/21		Wellington Laboratories, Lot MPFBA0516		(Purchased Reagent)		13C4 PFBA	50 ug/mL
..LCMPFDA_00011	08/19/20		Wellington Laboratories, Lot MPFDA0815		(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFDoA_00008	04/08/21		Wellington Laboratories, Lot MPFDoA0416		(Purchased Reagent)		13C2 PFDoA	50 ug/mL
..LCMPFHxA_00012	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL
..LCMPFHxS_00008	10/23/20		Wellington Laboratories, Lot MPFHxS1015		(Purchased Reagent)		18O2 PFHxS	47.3 ug/mL
..LCMPFNA_00008	04/13/19		Wellington Laboratories, Lot MPFNA0414		(Purchased Reagent)		13C5 PFNA	50 ug/mL
..LCMPFOA_00012	01/22/21		Wellington Laboratories, Lot MPFOA0116		(Purchased Reagent)		13C4 PFOA	50 ug/mL
..LCMPFOS_00017	08/03/21		Wellington Laboratories, Lot MPFOS0816		(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
..LCMPFUdA_00009	02/12/21		Wellington Laboratories, Lot MPFUdA0216		(Purchased Reagent)		13C2 PFUnA	50 ug/mL
.LCPFCSP_00074	06/14/17	12/14/16	Methanol, Lot 090285	10000 uL	LCPFBA_00005	200 uL	Perfluorobutanoic acid (PFBA)	1 ug/mL
					LCPFBS_00005	200 uL	Perfluorobutanesulfonic acid (PFBS)	0.884 ug/mL
					LCPFDA_00005	200 uL	Perfluorodecanoic acid (PFDA)	1 ug/mL
					LCPFDoA_00005	200 uL	Perfluorododecanoic acid (PFDoA)	1 ug/mL
					LCPFDS_00006	200 uL	Perfluorodecanesulfonic acid (PFDS)	0.964 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LCPFHpA_00006	200 uL	Perfluoroheptanoic acid (PFHpA)	1 ug/mL
					LCPFHps_00009	200 uL	Perfluoroheptanesulfonic Acid	0.952 ug/mL
					LCPFHxA_00005	200 uL	Perfluorohexanoic acid (PFHxA)	1 ug/mL
					LCPFHxDA_00006	200 uL	Perfluorohexadecanoic acid	1 ug/mL
					LCPFHxS-br_00002	200 uL	Perfluorohexanesulfonic acid (PFHxS)	0.91 ug/mL
					LCPFNA_00006	200 uL	Perfluorononanoic acid (PFNA)	1 ug/mL
					LCPFOA_00006	200 uL	Perfluorooctanoic acid (PFOA)	1 ug/mL
					LCPFODA_00006	200 uL	Perfluorooctadecanoic acid	1 ug/mL
					LCPFOS-br_00002	200 uL	Perfluorooctanesulfonic acid (PFOS)	0.928 ug/mL
					LCPFOSA_00008	200 uL	Perfluorooctane Sulfonamide (FOSA)	1 ug/mL
					LCPFPeA_00005	200 uL	Perfluoropentanoic acid (PFPeA)	1 ug/mL
					LCPFTeDA_00005	200 uL	Perfluorotetradecanoic acid (PFTeA)	1 ug/mL
					LCPFTrDA_00005	200 uL	Perfluorotridecanoic Acid (PFTriA)	1 ug/mL
					LCPFUdA_00005	200 uL	Perfluoroundecanoic acid (PFUnA)	1 ug/mL
..LCPFBA_00005	05/27/21	Wellington Laboratories, Lot PFBA0516			(Purchased Reagent)		Perfluorobutanoic acid (PFBA)	50 ug/mL
..LCPFBS_00005	03/15/21	Wellington Laboratories, Lot LPFBS0316			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	44.2 ug/mL
..LCPFDA_00005	07/02/20	Wellington Laboratories, Lot PFDA0615			(Purchased Reagent)		Perfluorodecanoic acid (PFDA)	50 ug/mL
..LCPFDoA_00005	01/30/20	Wellington Laboratories, Lot PFDoA0115			(Purchased Reagent)		Perfluorododecanoic acid (PFDoA)	50 ug/mL
..LCPFDS_00006	05/24/21	Wellington Laboratories, Lot LPFDS0516			(Purchased Reagent)		Perfluorodecanesulfonic acid (PFDS)	48.2 ug/mL
..LCPFHpA_00006	01/22/21	Wellington Laboratories, Lot PFHpA0116			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	50 ug/mL
..LCPFHps_00009	11/06/20	Wellington Laboratories, Lot LPFHps1115			(Purchased Reagent)		Perfluoroheptanesulfonic Acid	47.6 ug/mL
..LCPFHxA_00005	12/22/20	Wellington Laboratories, Lot PFHxA1215			(Purchased Reagent)		Perfluorohexanoic acid (PFHxA)	50 ug/mL
..LCPFHxDA_00006	05/25/21	Wellington Laboratories, Lot PFHxDA0516			(Purchased Reagent)		Perfluorohexadecanoic acid	50 ug/mL
..LCPFHxS-br_00002	07/03/20	Wellington Laboratories, Lot brPFHxSK0615			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	45.5 ug/mL
..LCPFNA_00006	10/23/20	Wellington Laboratories, Lot PFNA1015			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	50 ug/mL
..LCPFOA_00006	11/06/20	Wellington Laboratories, Lot PFOA1115			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	50 ug/mL
..LCPFODA_00006	04/29/21	Wellington Laboratories, Lot PFODA0416			(Purchased Reagent)		Perfluorooctadecanoic acid	50 ug/mL
..LCPFOS-br_00002	10/14/20	Wellington Laboratories, Lot brPFOSK1015			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	46.4 ug/mL
..LCPFOSA_00008	09/02/17	Wellington Laboratories, Lot FOSA0815I			(Purchased Reagent)		Perfluorooctane Sulfonamide (FOSA)	50 ug/mL
..LCPFPeA_00005	01/30/20	Wellington Laboratories, Lot PFPeA0115			(Purchased Reagent)		Perfluoropentanoic acid (PFPeA)	50 ug/mL
..LCPFTeDA_00005	12/09/20	Wellington Laboratories, Lot PFTeDA1215			(Purchased Reagent)		Perfluorotetradecanoic acid (PFTeA)	50 ug/mL
..LCPFTrDA_00005	02/12/21	Wellington Laboratories, Lot PFTTrDA0216			(Purchased Reagent)		Perfluorotridecanoic Acid (PFTriA)	50 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
..LCPFUdA_00005	08/19/20		Wellington Laboratories, Lot PFUdA0815			(Purchased Reagent)	Perfluoroundecanoic acid (PFUnA)	50 ug/mL
LCPFC-L6_00020	12/28/16	12/15/16	MeOH/H2O, Lot 090285	5 mL	LCMPFCSU_00047	250 uL	13C2-PFHxDA	50 ng/mL
							13C2-PFTeDA	50 ng/mL
							13C4-PFHpA	50 ng/mL
							13C5 PFPeA	50 ng/mL
							13C8 FOSA	50 ng/mL
							13C4 PFBA	50 ng/mL
							13C2 PFDA	50 ng/mL
							13C2 PFDoA	50 ng/mL
							13C2 PFHxA	50 ng/mL
							18O2 PFHxS	47.3 ng/mL
							13C5 PFNA	50 ng/mL
							13C4 PFOA	50 ng/mL
							13C4 PFOS	47.8 ng/mL
							13C2 PFUnA	50 ng/mL
							LCPFCSP_00074	1000 uL
					Perfluorobutanesulfonic acid (PFBS)	176.8 ng/mL		
					Perfluorodecanoic acid (PFDA)	200 ng/mL		
					Perfluorododecanoic acid (PFDoA)	200 ng/mL		
					Perfluorodecanesulfonic acid (PFDS)	192.8 ng/mL		
					Perfluoroheptanoic acid (PFHpA)	200 ng/mL		
					Perfluoroheptanesulfonic Acid (PFHpA)	190.4 ng/mL		
					Perfluoroheptanoic acid (PFHxA)	200 ng/mL		
					Perfluorohexadecanoic acid	200 ng/mL		
					Perfluorohexanesulfonic acid (PFHxS)	182 ng/mL		
					Perfluorononanoic acid (PFNA)	200 ng/mL		
					Perfluorooctanoic acid (PFOA)	200 ng/mL		
					Perfluorooctadecanoic acid	200 ng/mL		
Perfluorooctanesulfonic acid (PFOS)	185.6 ng/mL							
Perfluorooctane Sulfonamide (FOSA)	200 ng/mL							
Perfluoropentanoic acid (PFPeA)	200 ng/mL							
Perfluorotetradecanoic acid (PFTeA)	200 ng/mL							
Perfluorotridecanoic Acid (PFTriA)	200 ng/mL							
Perfluoroundecanoic acid (PFUnA)	200 ng/mL							
.LCMPFCSU_00047	06/14/17	12/14/16	Methanol, Lot Baker 144541	50000 uL	LCM2PFHxDA_00008	1000 uL	13C2-PFHxDA	1 ug/mL
					LCM2PFTeDA_00007	1000 uL	13C2-PFTeDA	1 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LCM4PFHPA_00007	1000 uL	13C4-PFHpA	1 ug/mL
					LCM5PFPEA_00008	1000 uL	13C5 PFPeA	1 ug/mL
					LCM8FOSA_00011	1000 uL	13C8 FOSA	1 ug/mL
					LCMPFBA_00008	1000 uL	13C4 PFBA	1 ug/mL
					LCMPFDA_00011	1000 uL	13C2 PFDA	1 ug/mL
					LCMPFDoA_00008	1000 uL	13C2 PFDoA	1 ug/mL
					LCMPFHxA_00012	1000 uL	13C2 PFHxA	1 ug/mL
					LCMPFHxS_00008	1000 uL	1802 PFHxS	0.946 ug/mL
					LCMPFNA_00008	1000 uL	13C5 PFNA	1 ug/mL
					LCMPFOA_00012	1000 uL	13C4 PFOA	1 ug/mL
					LCMPFOS_00017	1000 uL	13C4 PFOS	0.956 ug/mL
					LCMPFUDa_00009	1000 uL	13C2 PFUnA	1 ug/mL
..LCM2PFHxDA_00008	01/07/21		Wellington Laboratories, Lot M2PFHxDA1112		(Purchased Reagent)		13C2-PFHxDA	50 ug/mL
..LCM2PFTEDA_00007	12/07/20		Wellington Laboratories, Lot M2PFTEDA1115		(Purchased Reagent)		13C2-PFTEDA	50 ug/mL
..LCM4PFHPA_00007	05/27/21		Wellington Laboratories, Lot M4PFHPA0516		(Purchased Reagent)		13C4-PFHpA	50 ug/mL
..LCM5PFPEA_00008	05/22/20		Wellington Laboratories, Lot M5PFPeA0515		(Purchased Reagent)		13C5 PFPeA	50 ug/mL
..LCM8FOSA_00011	12/22/17		Wellington Laboratories, Lot M8FOSA1215I		(Purchased Reagent)		13C8 FOSA	50 ug/mL
..LCMPFBA_00008	05/24/21		Wellington Laboratories, Lot MPFBA0516		(Purchased Reagent)		13C4 PFBA	50 ug/mL
..LCMPFDA_00011	08/19/20		Wellington Laboratories, Lot MPFDA0815		(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFDoA_00008	04/08/21		Wellington Laboratories, Lot MPFDoA0416		(Purchased Reagent)		13C2 PFDoA	50 ug/mL
..LCMPFHxA_00012	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL
..LCMPFHxS_00008	10/23/20		Wellington Laboratories, Lot MPFHxS1015		(Purchased Reagent)		1802 PFHxS	47.3 ug/mL
..LCMPFNA_00008	04/13/19		Wellington Laboratories, Lot MPFNA0414		(Purchased Reagent)		13C5 PFNA	50 ug/mL
..LCMPFOA_00012	01/22/21		Wellington Laboratories, Lot MPFOA0116		(Purchased Reagent)		13C4 PFOA	50 ug/mL
..LCMPFOS_00017	08/03/21		Wellington Laboratories, Lot MPFOS0816		(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
..LCMPFUDa_00009	02/12/21		Wellington Laboratories, Lot MPFUDa0216		(Purchased Reagent)		13C2 PFUnA	50 ug/mL
.LCPFCSP_00074	06/14/17	12/14/16	Methanol, Lot 090285	10000 uL	LCPFBA_00005	200 uL	Perfluorobutanoic acid (PFBA)	1 ug/mL
					LCPFBS_00005	200 uL	Perfluorobutanesulfonic acid (PFBS)	0.884 ug/mL
					LCPFDA_00005	200 uL	Perfluorodecanoic acid (PFDA)	1 ug/mL
					LCPFDoA_00005	200 uL	Perfluorododecanoic acid (PFDoA)	1 ug/mL
					LCPFDS_00006	200 uL	Perfluorodecanesulfonic acid (PFDS)	0.964 ug/mL
					LCPFHpA_00006	200 uL	Perfluoroheptanoic acid (PFHpA)	1 ug/mL
					LCPFHpS_00009	200 uL	Perfluoroheptanesulfonic Acid	0.952 ug/mL
					LCPFHxA_00005	200 uL	Perfluorohexanoic acid (PFHxA)	1 ug/mL
					LCPFHxDA_00006	200 uL	Perfluorohexadecanoic acid	1 ug/mL
					LCPFHxS-br_00002	200 uL	Perfluorohexanesulfonic acid (PFHxS)	0.91 ug/mL
					LCPFNA_00006	200 uL	Perfluorononanoic acid (PFNA)	1 ug/mL
					LCPFOA_00006	200 uL	Perfluorooctanoic acid (PFOA)	1 ug/mL
					LCPFODA_00006	200 uL	Perfluorooctadecanoic acid	1 ug/mL
					LCPFOS-br_00002	200 uL	Perfluorooctanesulfonic acid (PFOS)	0.928 ug/mL
					LCPFOSA_00008	200 uL	Perfluorooctane Sulfonamide (FOSA)	1 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LCPFPeA_00005	200 uL	Perfluoropentanoic acid (PFPeA)	1 ug/mL
					LCPFTeDA_00005	200 uL	Perfluorotetradecanoic acid (PFTeA)	1 ug/mL
					LCPFTrDA_00005	200 uL	Perfluorotridecanoic Acid (PFTriA)	1 ug/mL
					LCPFUDA_00005	200 uL	Perfluoroundecanoic acid (PFUnA)	1 ug/mL
..LCPFBA_00005	05/27/21		Wellington Laboratories, Lot PFBA0516		(Purchased Reagent)		Perfluorobutanoic acid (PFBA)	50 ug/mL
..LCPFBS_00005	03/15/21		Wellington Laboratories, Lot LPFBS0316		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	44.2 ug/mL
..LCPFDA_00005	07/02/20		Wellington Laboratories, Lot PFDA0615		(Purchased Reagent)		Perfluorodecanoic acid (PFDA)	50 ug/mL
..LCPFDoA_00005	01/30/20		Wellington Laboratories, Lot PFDoA0115		(Purchased Reagent)		Perfluorododecanoic acid (PFDoA)	50 ug/mL
..LCPFDS_00006	05/24/21		Wellington Laboratories, Lot LPFDS0516		(Purchased Reagent)		Perfluorodecanesulfonic acid (PFDS)	48.2 ug/mL
..LCPFHpA_00006	01/22/21		Wellington Laboratories, Lot PFHpA0116		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	50 ug/mL
..LCPFHpS_00009	11/06/20		Wellington Laboratories, Lot LPFHpS1115		(Purchased Reagent)		Perfluoroheptanesulfonic Acid	47.6 ug/mL
..LCPFHxA_00005	12/22/20		Wellington Laboratories, Lot PFHxA1215		(Purchased Reagent)		Perfluorohexanoic acid (PFHxA)	50 ug/mL
..LCPFHxDA_00006	05/25/21		Wellington Laboratories, Lot PFHxDA0516		(Purchased Reagent)		Perfluorohexadecanoic acid	50 ug/mL
..LCPFHxS-br_00002	07/03/20		Wellington Laboratories, Lot brPFHxSK0615		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	45.5 ug/mL
..LCPFNA_00006	10/23/20		Wellington Laboratories, Lot PFNA1015		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	50 ug/mL
..LCPFOA_00006	11/06/20		Wellington Laboratories, Lot PFOA1115		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	50 ug/mL
..LCPFODA_00006	04/29/21		Wellington Laboratories, Lot PFODA0416		(Purchased Reagent)		Perfluorooctadecanoic acid	50 ug/mL
..LCPFOS-br_00002	10/14/20		Wellington Laboratories, Lot brPFOSK1015		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	46.4 ug/mL
..LCPFOSA_00008	09/02/17		Wellington Laboratories, Lot FOSA0815I		(Purchased Reagent)		Perfluorooctane Sulfonamide (FOSA)	50 ug/mL
..LCPFPeA_00005	01/30/20		Wellington Laboratories, Lot PFPeA0115		(Purchased Reagent)		Perfluoropentanoic acid (PFPeA)	50 ug/mL
..LCPFTeDA_00005	12/09/20		Wellington Laboratories, Lot PFTeDA1215		(Purchased Reagent)		Perfluorotetradecanoic acid (PFTeA)	50 ug/mL
..LCPFTrDA_00005	02/12/21		Wellington Laboratories, Lot PFTTrDA0216		(Purchased Reagent)		Perfluorotridecanoic Acid (PFTriA)	50 ug/mL
..LCPFUDA_00005	08/19/20		Wellington Laboratories, Lot PFUDA0815		(Purchased Reagent)		Perfluoroundecanoic acid (PFUnA)	50 ug/mL
LCPFC2-L1_00002	01/08/17	07/20/16	MeOH/H2O, Lot 104453	5 mL	LCMPFC2SU_00005	250 uL	d-N-EtFOSA-M	50 ng/mL
							d-N-MeFOSA-M	50 ng/mL
							d3-NMeFOSAA	50 ng/mL
							d5-NEtFOSAA	50 ng/mL
							M2-6:2FTS	47.5 ng/mL
							M2-8:2FTS	47.9 ng/mL
					LCPFC2SP_00014	25 uL	Sodium 1H, 1H, 2H, 2H-perfluorooctane sulfonate (6:2)	0.474 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Sodium 1H, 1H, 2H, 2H-perfluorooctane sulfonate (8:2)	0.479 ng/mL
							N-ethylperfluoro-1-octanesulfonamide	0.5 ng/mL
							N-ethyl perfluorooctane sulfonamidoacetic acid	0.5 ng/mL
							MeFOSA	0.5 ng/mL
							N-methyl perfluorooctane sulfonamidoacetic acid	0.5 ng/mL
.LCMPFC2SU_00005	01/08/17	07/08/16	Methanol, Lot 104453	10000 uL	LCd-NEtFOSA-M_00001	200 uL	d-N-EtFOSA-M	1 ug/mL
					LCd-NMeFOSA-M_00001	200 uL	d-N-MeFOSA-M	1 ug/mL
					LCd3-NMeFOSAA_00001	200 uL	d3-NMeFOSAA	1 ug/mL
					LCd5-NEtFOSAA_00001	200 uL	d5-NEtFOSAA	1 ug/mL
					LCM2-6:FtS_00001	200 uL	M2-6:2FtS	0.95 ug/mL
					LCM2-8:2FtS_00001	200 uL	M2-8:2FtS	0.958 ug/mL
..LCd-NEtFOSA-M_00001	03/10/19		WELLINGTON, Lot dNEtFOSA0314M			(Purchased Reagent)	d-N-EtFOSA-M	50 ug/mL
..LCd-NMeFOSA-M_00001	01/28/19		WELLINGTON, Lot dNMeFOSA0114M			(Purchased Reagent)	d-N-MeFOSA-M	50 ug/mL
..LCd3-NMeFOSAA_00001	01/31/18		WELLINGTON, Lot d3NMeFOSAA0113			(Purchased Reagent)	d3-NMeFOSAA	50 ug/mL
..LCd5-NEtFOSAA_00001	05/08/20		WELLINGTON, Lot d5NEtFOSAA0515			(Purchased Reagent)	d5-NEtFOSAA	50 ug/mL
..LCM2-6:FtS_00001	07/15/17		WELLINGTON, Lot M262FtS0714			(Purchased Reagent)	M2-6:2FtS	47.5 ug/mL
..LCM2-8:2FtS_00001	04/13/17		WELLINGTON, Lot M282FtS0414			(Purchased Reagent)	M2-8:2FtS	47.9 ug/mL
.LCPFC2SP_00014	01/20/17	07/20/16	Methanol, Lot 104453	5000 uL	LCPFC2SP_00013	500 uL	Sodium 1H, 1H, 2H, 2H-perfluorooctane sulfonate (6:2)	0.0948 ug/mL
							Sodium 1H, 1H, 2H, 2H-perfluorooctane sulfonate (8:2)	0.0958 ug/mL
							N-ethylperfluoro-1-octanesulfonamide	0.1 ug/mL
							N-ethyl perfluorooctane sulfonamidoacetic acid	0.1 ug/mL
							MeFOSA	0.1 ug/mL
							N-methyl perfluorooctane sulfonamidoacetic acid	0.1 ug/mL
..LCPFC2SP_00013	01/20/17	07/20/16	Methanol, Lot 104453	10000 uL	LC6:2FtS_00001	200 uL	Sodium 1H, 1H, 2H, 2H-perfluorooctane sulfonate (6:2)	0.948 ug/mL
					LC8:2FtS_00001	200 uL	Sodium 1H, 1H, 2H, 2H-perfluorooctane sulfonate (8:2)	0.958 ug/mL
					LCN-EtFOSA-M_00002	200 uL	N-ethylperfluoro-1-octanesulfonamide	1 ug/mL
					LCN-EtFOSAA_00001	200 uL	N-ethyl perfluorooctane sulfonamidoacetic acid	1 ug/mL
					LCN-MeFOSA-M_00001	200 uL	MeFOSA	1 ug/mL
					LCN-MeFOSAA_00001	200 uL	N-methyl perfluorooctane sulfonamidoacetic acid	1 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
...LC6:2FTS_00001	10/03/17		WELLINGTON, Lot 62FTS1014		(Purchased Reagent)		Sodium 1H, 1H, 2H, 2H-perfluorooctane sulfonate (6:2)	47.4 ug/mL
...LC8:2FTS_00001	10/03/17		WELLINGTON, Lot 82FTS1014		(Purchased Reagent)		Sodium 1H, 1H, 2H, 2H-perfluorooctane sulfonate (8:2)	47.9 ug/mL
...LCN-EtFOSA-M_00002	07/14/19		WELLINGTON, Lot NETFOSA0714M		(Purchased Reagent)		N-ethylperfluoro-1-octanesulfo namide	50 ug/mL
...LCN-EtFOSAA_00001	01/29/18		WELLINGTON, Lot NETFOSAA0113		(Purchased Reagent)		N-ethyl perfluorooctane sulfonamidoacetic acid	50 ug/mL
...LCN-MeFOSA-M_00001	07/15/19		WELLINGTON, Lot NMeFOSA0714M		(Purchased Reagent)		MeFOSA	50 ug/mL
...LCN-MeFOSAA_00001	12/09/19		WELLINGTON, Lot NMeFOSAA1214		(Purchased Reagent)		N-methyl perfluorooctane sulfonamidoacetic acid	50 ug/mL
LCPFC2-L2_00002	01/08/17	07/20/16	MeOH/H2O, Lot 104453	5 mL	LCMPFC2SU_00005	250 uL	d-N-EtFOSA-M	50 ng/mL
							d-N-MeFOSA-M	50 ng/mL
							d3-NMeFOSAA	50 ng/mL
							d5-NEtFOSAA	50 ng/mL
							M2-6:2FTS	47.5 ng/mL
					M2-8:2FTS	47.9 ng/mL		
					LCPFC2SP_00014	50 uL	Sodium 1H, 1H, 2H, 2H-perfluorooctane sulfonate (6:2)	0.948 ng/mL
							Sodium 1H, 1H, 2H, 2H-perfluorooctane sulfonate (8:2)	0.958 ng/mL
							N-ethylperfluoro-1-octanesulfo namide	1 ng/mL
							N-ethyl perfluorooctane sulfonamidoacetic acid	1 ng/mL
MeFOSA	1 ng/mL							
N-methyl perfluorooctane sulfonamidoacetic acid	1 ng/mL							
.LCMPFC2SU_00005	01/08/17	07/08/16	Methanol, Lot 104453	10000 uL	LCd-NEtFOSA-M_00001	200 uL	d-N-EtFOSA-M	1 ug/mL
					LCd-NMeFOSA-M_00001	200 uL	d-N-MeFOSA-M	1 ug/mL
					LCd3-NMeFOSAA_00001	200 uL	d3-NMeFOSAA	1 ug/mL
					LCd5-NEtFOSAA_00001	200 uL	d5-NEtFOSAA	1 ug/mL
					LCM2-6:Fts_00001	200 uL	M2-6:2Fts	0.95 ug/mL
					LCM2-8:2Fts_00001	200 uL	M2-8:2Fts	0.958 ug/mL
..LCd-NEtFOSA-M_00001	03/10/19		WELLINGTON, Lot dNetFOSA0314M		(Purchased Reagent)		d-N-EtFOSA-M	50 ug/mL
..LCd-NMeFOSA-M_00001	01/28/19		WELLINGTON, Lot dNMeFOSA0114M		(Purchased Reagent)		d-N-MeFOSA-M	50 ug/mL
..LCd3-NMeFOSAA_00001	01/31/18		WELLINGTON, Lot d3NMeFOSAA0113		(Purchased Reagent)		d3-NMeFOSAA	50 ug/mL
..LCd5-NEtFOSAA_00001	05/08/20		WELLINGTON, Lot d5NetFOSAA0515		(Purchased Reagent)		d5-NEtFOSAA	50 ug/mL
..LCM2-6:Fts_00001	07/15/17		WELLINGTON, Lot M262Fts0714		(Purchased Reagent)		M2-6:2Fts	47.5 ug/mL
..LCM2-8:2Fts_00001	04/13/17		WELLINGTON, Lot M282Fts0414		(Purchased Reagent)		M2-8:2Fts	47.9 ug/mL
.LCPFC2SP_00014	01/20/17	07/20/16	Methanol, Lot 104453	5000 uL	LCPFC2SP_00013	500 uL	Sodium 1H, 1H, 2H, 2H-perfluorooctane sulfonate (6:2)	0.0948 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (8:2)	0.0958 ug/mL
							N-ethylperfluoro-1-octanesulfonamide	0.1 ug/mL
							N-ethyl perfluorooctane sulfonamidoacetic acid	0.1 ug/mL
							MeFOSA	0.1 ug/mL
							N-methyl perfluorooctane sulfonamidoacetic acid	0.1 ug/mL
..LCPFC2SP_00013	01/20/17	07/20/16	Methanol, Lot 104453	10000 uL	LC6:2FTS_00001	200 uL	Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (6:2)	0.948 ug/mL
					LC8:2FTS_00001	200 uL	Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (8:2)	0.958 ug/mL
					LCN-EtFOSA-M_00002	200 uL	N-ethylperfluoro-1-octanesulfonamide	1 ug/mL
					LCN-EtFOSAA_00001	200 uL	N-ethyl perfluorooctane sulfonamidoacetic acid	1 ug/mL
					LCN-MeFOSA-M_00001	200 uL	MeFOSA	1 ug/mL
					LCN-MeFOSAA_00001	200 uL	N-methyl perfluorooctane sulfonamidoacetic acid	1 ug/mL
...LC6:2FTS_00001	10/03/17		WELLINGTON, Lot 62FTS1014		(Purchased Reagent)		Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (6:2)	47.4 ug/mL
...LC8:2FTS_00001	10/03/17		WELLINGTON, Lot 82FTS1014		(Purchased Reagent)		Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (8:2)	47.9 ug/mL
...LCN-EtFOSA-M_00002	07/14/19		WELLINGTON, Lot NETFOSA0714M		(Purchased Reagent)		N-ethylperfluoro-1-octanesulfonamide	50 ug/mL
...LCN-EtFOSAA_00001	01/29/18		WELLINGTON, Lot NETFOSAA0113		(Purchased Reagent)		N-ethyl perfluorooctane sulfonamidoacetic acid	50 ug/mL
...LCN-MeFOSA-M_00001	07/15/19		WELLINGTON, Lot NMeFOSA0714M		(Purchased Reagent)		MeFOSA	50 ug/mL
...LCN-MeFOSAA_00001	12/09/19		WELLINGTON, Lot NMeFOSAA1214		(Purchased Reagent)		N-methyl perfluorooctane sulfonamidoacetic acid	50 ug/mL
LCPFC2-L3_00002	01/08/17	07/20/16	MeOH/H2O, Lot 104453	5 mL	LCMPFC2SU_00005	250 uL	d-N-EtFOSA-M	50 ng/mL
							d-N-MeFOSA-M	50 ng/mL
							d3-NMeFOSAA	50 ng/mL
							d5-NETFOSAA	50 ng/mL
							M2-6:2FTS	47.5 ng/mL
							M2-8:2FTS	47.9 ng/mL
					LCPFC2SP_00014	250 uL	Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (6:2)	4.74 ng/mL
							Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (8:2)	4.79 ng/mL
							N-ethylperfluoro-1-octanesulfonamide	5 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							N-ethyl perfluorooctane sulfonamidoacetic acid	5 ng/mL
							MeFOSA	5 ng/mL
							N-methyl perfluorooctane sulfonamidoacetic acid	5 ng/mL
.LCMPFC2SU_00005	01/08/17	07/08/16	Methanol, Lot 104453	10000 uL	LCd-NETfOSA-M 00001	200 uL	d-N-EtFOSA-M	1 ug/mL
					LCd-NMeFOSA-M 00001	200 uL	d-N-MeFOSA-M	1 ug/mL
					LCd3-NMeFOSAA 00001	200 uL	d3-NMeFOSAA	1 ug/mL
					LCd5-NETfOSAA 00001	200 uL	d5-NETfOSAA	1 ug/mL
					LCM2-6:FtS 00001	200 uL	M2-6:2FtS	0.95 ug/mL
					LCM2-8:2FtS 00001	200 uL	M2-8:2FtS	0.958 ug/mL
..LCd-NETfOSA-M 00001	03/10/19		WELLINGTON, Lot dNetFOSA0314M		(Purchased Reagent)		d-N-EtFOSA-M	50 ug/mL
..LCd-NMeFOSA-M 00001	01/28/19		WELLINGTON, Lot dNMeFOSA0114M		(Purchased Reagent)		d-N-MeFOSA-M	50 ug/mL
..LCd3-NMeFOSAA 00001	01/31/18		WELLINGTON, Lot d3NMeFOSAA0113		(Purchased Reagent)		d3-NMeFOSAA	50 ug/mL
..LCd5-NETfOSAA 00001	05/08/20		WELLINGTON, Lot d5NETfOSAA0515		(Purchased Reagent)		d5-NETfOSAA	50 ug/mL
..LCM2-6:FtS 00001	07/15/17		WELLINGTON, Lot M262FtS0714		(Purchased Reagent)		M2-6:2FtS	47.5 ug/mL
..LCM2-8:2FtS 00001	04/13/17		WELLINGTON, Lot M282FtS0414		(Purchased Reagent)		M2-8:2FtS	47.9 ug/mL
.LCPFC2SP_00014	01/20/17	07/20/16	Methanol, Lot 104453	5000 uL	LCPFC2SP_00013	500 uL	Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (6:2)	0.0948 ug/mL
							Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (8:2)	0.0958 ug/mL
							N-ethylperfluoro-1-octanesulfoamide	0.1 ug/mL
							N-ethyl perfluorooctane sulfonamidoacetic acid	0.1 ug/mL
							MeFOSA	0.1 ug/mL
							N-methyl perfluorooctane sulfonamidoacetic acid	0.1 ug/mL
..LCPFC2SP_00013	01/20/17	07/20/16	Methanol, Lot 104453	10000 uL	LC6:2FtS_00001	200 uL	Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (6:2)	0.948 ug/mL
					LC8:2FtS_00001	200 uL	Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (8:2)	0.958 ug/mL
					LCN-EtFOSA-M_00002	200 uL	N-ethylperfluoro-1-octanesulfoamide	1 ug/mL
					LCN-EtFOSAA_00001	200 uL	N-ethyl perfluorooctane sulfonamidoacetic acid	1 ug/mL
					LCN-MeFOSA-M 00001	200 uL	MeFOSA	1 ug/mL
					LCN-MeFOSAA_00001	200 uL	N-methyl perfluorooctane sulfonamidoacetic acid	1 ug/mL
...LC6:2FtS_00001	10/03/17		WELLINGTON, Lot 62FtS1014		(Purchased Reagent)		Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (6:2)	47.4 ug/mL
...LC8:2FtS_00001	10/03/17		WELLINGTON, Lot 82FtS1014		(Purchased Reagent)		Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (8:2)	47.9 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
...LCN-EtFOSA-M_00002	07/14/19		WELLINGTON, Lot NETFOSA0714M		(Purchased Reagent)		N-ethylperfluoro-1-octanesulfo namide	50 ug/mL
...LCN-EtFOSAA_00001	01/29/18		WELLINGTON, Lot NETFOSAA0113		(Purchased Reagent)		N-ethyl perfluorooctane sulfonamidoacetic acid	50 ug/mL
...LCN-MeFOSA-M_00001	07/15/19		WELLINGTON, Lot NMeFOSA0714M		(Purchased Reagent)		MeFOSA	50 ug/mL
...LCN-MeFOSAA_00001	12/09/19		WELLINGTON, Lot NMeFOSAA1214		(Purchased Reagent)		N-methyl perfluorooctane sulfonamidoacetic acid	50 ug/mL
LCPFC2-L4_00003	02/26/17	09/22/16	MeOH/H2O, Lot 104453	5 mL	LCMPFC2SU_00008	250 uL	d-N-EtFOSA-M	50 ng/mL
							d-N-MeFOSA-M	50 ng/mL
							d3-NMeFOSAA	50 ng/mL
							d5-NETFOSAA	50 ng/mL
							M2-6:2FTS	47.5 ng/mL
					LCPFC2SP_00017	200 uL	Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (6:2)	18.96 ng/mL
							Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (8:2)	19.16 ng/mL
							N-ethylperfluoro-1-octanesulfo namide	20 ng/mL
							N-ethyl perfluorooctane sulfonamidoacetic acid	20 ng/mL
							MeFOSA	20 ng/mL
.LCMPFC2SU_00008	02/26/17	08/26/16	Methanol, Lot 104453	10000 uL	LCd-NEtFOSA-M_00002	200 uL	d-N-EtFOSA-M	1 ug/mL
					LCd-NMeFOSA-M_00002	200 uL	d-N-MeFOSA-M	1 ug/mL
					LCd3-NMeFOSAA_00002	200 uL	d3-NMeFOSAA	1 ug/mL
					LCd5-NETFOSAA_00002	200 uL	d5-NETFOSAA	1 ug/mL
					LCM2-6:Fts_00002	200 uL	M2-6:2FTS	0.95 ug/mL
					LCM2-8:2Fts_00002	200 uL	M2-8:2FTS	0.958 ug/mL
..LCd-NEtFOSA-M_00002	03/10/19		WELLINGTON, Lot dNEtFOSA0314M		(Purchased Reagent)		d-N-EtFOSA-M	50 ug/mL
..LCd-NMeFOSA-M_00002	06/10/21		WELLINGTON, Lot dNMeFOSA0616M		(Purchased Reagent)		d-N-MeFOSA-M	50 ug/mL
..LCd3-NMeFOSAA_00002	01/20/21		WELLINGTON, Lot d3NMeFOSAA0116		(Purchased Reagent)		d3-NMeFOSAA	50 ug/mL
..LCd5-NETFOSAA_00002	12/07/20		WELLINGTON, Lot d5NETFOSAA1115		(Purchased Reagent)		d5-NETFOSAA	50 ug/mL
..LCM2-6:Fts_00002	01/08/21		WELLINGTON, Lot M262Fts0116		(Purchased Reagent)		M2-6:2Fts	47.5 ug/mL
..LCM2-8:2Fts_00002	01/08/21		WELLINGTON, Lot M282Fts0116		(Purchased Reagent)		M2-8:2Fts	47.9 ug/mL
.LCPFC2SP_00017	03/02/17	09/02/16	Methanol, Lot 104453	10000 uL	LC6:2Fts_00002	100 uL	Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (6:2)	0.474 ug/mL
					LC8:2Fts_00002	100 uL	Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (8:2)	0.479 ug/mL
					LCN-EtFOSA-M_00003	100 uL	N-ethylperfluoro-1-octanesulfo namide	0.5 ug/mL
					LCN-EtFOSAA_00002	100 uL	N-ethyl perfluorooctane sulfonamidoacetic acid	0.5 ug/mL
					LCN-MeFOSA-M_00002	100 uL	MeFOSA	0.5 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LCN-MeFOSAA_00003	100 uL	N-methyl perfluorooctane sulfonamidoacetic acid	0.5 ug/mL
..LC6:2FTS_00002	06/25/21		WELLINGTON, Lot 62FTS0616		(Purchased Reagent)		Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (6:2)	47.4 ug/mL
..LC8:2FTS_00002	10/23/20		WELLINGTON, Lot 82FTS1015		(Purchased Reagent)		Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (8:2)	47.9 ug/mL
..LCN-EtFOSA-M_00003	05/24/21		WELLINGTON, Lot NETFOSA0516M		(Purchased Reagent)		N-ethylperfluoro-1-octanesulfo namide	50 ug/mL
..LCN-EtFOSAA_00002	01/20/21		WELLINGTON, Lot NETFOSAA0116		(Purchased Reagent)		N-ethyl perfluorooctane sulfonamidoacetic acid	50 ug/mL
..LCN-MeFOSA-M_00002	05/24/21		WELLINGTON, Lot NMeFOSA0714M		(Purchased Reagent)		MeFOSA	50 ug/mL
..LCN-MeFOSAA_00003	01/20/21		WELLINGTON, Lot NMeFOSAA0116		(Purchased Reagent)		N-methyl perfluorooctane sulfonamidoacetic acid	50 ug/mL
LCPFC2-L5_00002	01/08/17	07/20/16	MeOH/H2O, Lot 104453	5 mL	LCMPFC2SU_00005	250 uL	d-N-EtFOSA-M	50 ng/mL
							d-N-MeFOSA-M	50 ng/mL
							d3-NMeFOSAA	50 ng/mL
							d5-NETFOSAA	50 ng/mL
							M2-6:2FTS	47.5 ng/mL
					M2-8:2FTS	47.9 ng/mL		
					LCPFC2SP_00013	250 uL	Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (6:2)	47.4 ng/mL
							Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (8:2)	47.9 ng/mL
							N-ethylperfluoro-1-octanesulfo namide	50 ng/mL
							N-ethyl perfluorooctane sulfonamidoacetic acid	50 ng/mL
MeFOSA	50 ng/mL							
N-methyl perfluorooctane sulfonamidoacetic acid	50 ng/mL							
.LCMPFC2SU_00005	01/08/17	07/08/16	Methanol, Lot 104453	10000 uL	LCd-NETFOSA-M_00001	200 uL	d-N-EtFOSA-M	1 ug/mL
							LCd-NMeFOSA-M_00001	1 ug/mL
							LCd3-NMeFOSAA_00001	1 ug/mL
							LCd5-NETFOSAA_00001	1 ug/mL
							LCM2-6:FOSAA_00001	0.95 ug/mL
							LCM2-8:2FTS_00001	0.958 ug/mL
..LCd-NETFOSA-M_00001	03/10/19		WELLINGTON, Lot dNETFOSA0314M		(Purchased Reagent)		d-N-EtFOSA-M	50 ug/mL
..LCd-NMeFOSA-M_00001	01/28/19		WELLINGTON, Lot dNMeFOSA0114M		(Purchased Reagent)		d-N-MeFOSA-M	50 ug/mL
..LCd3-NMeFOSAA_00001	01/31/18		WELLINGTON, Lot d3NMeFOSAA0113		(Purchased Reagent)		d3-NMeFOSAA	50 ug/mL
..LCd5-NETFOSAA_00001	05/08/20		WELLINGTON, Lot d5NETFOSAA0515		(Purchased Reagent)		d5-NETFOSAA	50 ug/mL
..LCM2-6:FOSAA_00001	07/15/17		WELLINGTON, Lot M262FTS0714		(Purchased Reagent)		M2-6:2FTS	47.5 ug/mL
..LCM2-8:2FTS_00001	04/13/17		WELLINGTON, Lot M282FTS0414		(Purchased Reagent)		M2-8:2FTS	47.9 ug/mL
.LCPFC2SP_00013	01/20/17	07/20/16	Methanol, Lot 104453	10000 uL	LC6:2FTS_00001	200 uL	Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (6:2)	0.948 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LC8:2FTS_00001	200 uL	Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (8:2)	0.958 ug/mL
					LCN-EtFOSA-M_00002	200 uL	N-ethylperfluoro-1-octanesulfonamide	1 ug/mL
					LCN-EtFOSAA_00001	200 uL	N-ethyl perfluorooctane sulfonamidoacetic acid	1 ug/mL
					LCN-MeFOSA-M_00001	200 uL	MeFOSA	1 ug/mL
					LCN-MeFOSAA_00001	200 uL	N-methyl perfluorooctane sulfonamidoacetic acid	1 ug/mL
..LC6:2FTS_00001	10/03/17		WELLINGTON, Lot 62FTS1014		(Purchased Reagent)		Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (6:2)	47.4 ug/mL
..LC8:2FTS_00001	10/03/17		WELLINGTON, Lot 82FTS1014		(Purchased Reagent)		Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (8:2)	47.9 ug/mL
..LCN-EtFOSA-M_00002	07/14/19		WELLINGTON, Lot NETFOSA0714M		(Purchased Reagent)		N-ethylperfluoro-1-octanesulfonamide	50 ug/mL
..LCN-EtFOSAA_00001	01/29/18		WELLINGTON, Lot NETFOSAA0113		(Purchased Reagent)		N-ethyl perfluorooctane sulfonamidoacetic acid	50 ug/mL
..LCN-MeFOSA-M_00001	07/15/19		WELLINGTON, Lot NMeFOSA0714M		(Purchased Reagent)		MeFOSA	50 ug/mL
..LCN-MeFOSAA_00001	12/09/19		WELLINGTON, Lot NMeFOSAA1214		(Purchased Reagent)		N-methyl perfluorooctane sulfonamidoacetic acid	50 ug/mL
LCPPFC2-L6_00002	01/08/17	07/20/16	MeOH/H2O, Lot 104453	5 mL	LCMPFC2SU_00005	250 uL	d-N-EtFOSA-M	50 ng/mL
							d-N-MeFOSA-M	50 ng/mL
							d3-NMeFOSAA	50 ng/mL
							d5-NETFOSAA	50 ng/mL
							M2-6:2FTS	47.5 ng/mL
							M2-8:2FTS	47.9 ng/mL
					LCPPFC2SP_00013	1000 uL	Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (6:2)	189.6 ng/mL
							Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (8:2)	191.6 ng/mL
							N-ethylperfluoro-1-octanesulfonamide	200 ng/mL
							N-ethyl perfluorooctane sulfonamidoacetic acid	200 ng/mL
						MeFOSA	200 ng/mL	
						N-methyl perfluorooctane sulfonamidoacetic acid	200 ng/mL	
.LCMPFC2SU_00005	01/08/17	07/08/16	Methanol, Lot 104453	10000 uL	LCd-NETFOSA-M_00001	200 uL	d-N-EtFOSA-M	1 ug/mL
					LCd-NMeFOSA-M_00001	200 uL	d-N-MeFOSA-M	1 ug/mL
					LCd3-NMeFOSAA_00001	200 uL	d3-NMeFOSAA	1 ug/mL
					LCd5-NETFOSAA_00001	200 uL	d5-NETFOSAA	1 ug/mL
					LCM2-6:FTS_00001	200 uL	M2-6:2FTS	0.95 ug/mL
					LCM2-8:2FTS_00001	200 uL	M2-8:2FTS	0.958 ug/mL
..LCd-NETFOSA-M_00001	03/10/19		WELLINGTON, Lot dNETFOSA0314M		(Purchased Reagent)		d-N-EtFOSA-M	50 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
..LCd-NMeFOSA-M_00001	01/28/19		WELLINGTON, Lot dNMeFOSA0114M			(Purchased Reagent)	d-N-MeFOSA-M	50 ug/mL
..LCd3-NMeFOSAA_00001	01/31/18		WELLINGTON, Lot d3NMeFOSAA0113			(Purchased Reagent)	d3-NMeFOSAA	50 ug/mL
..LCd5-NEtFOSAA_00001	05/08/20		WELLINGTON, Lot d5NEtFOSAA0515			(Purchased Reagent)	d5-NEtFOSAA	50 ug/mL
..LCM2-6:FtS_00001	07/15/17		WELLINGTON, Lot M262FtS0714			(Purchased Reagent)	M2-6:2FtS	47.5 ug/mL
..LCM2-8:2FtS_00001	04/13/17		WELLINGTON, Lot M282FtS0414			(Purchased Reagent)	M2-8:2FtS	47.9 ug/mL
.LCPFC2SP_00013	01/20/17	07/20/16	Methanol, Lot 104453	10000 uL	LC6:2FtS_00001	200 uL	Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (6:2)	0.948 ug/mL
					LC8:2FtS_00001	200 uL	Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (8:2)	0.958 ug/mL
					LCN-EtFOSA-M_00002	200 uL	N-ethylperfluoro-1-octanesulfo namide	1 ug/mL
					LCN-EtFOSAA_00001	200 uL	N-ethyl perfluorooctane sulfonamidoacetic acid	1 ug/mL
					LCN-MeFOSA-M_00001	200 uL	MeFOSA	1 ug/mL
					LCN-MeFOSAA_00001	200 uL	N-methyl perfluorooctane sulfonamidoacetic acid	1 ug/mL
..LC6:2FtS_00001	10/03/17		WELLINGTON, Lot 62FtS1014			(Purchased Reagent)	Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (6:2)	47.4 ug/mL
..LC8:2FtS_00001	10/03/17		WELLINGTON, Lot 82FtS1014			(Purchased Reagent)	Sodium 1H,1H,2H,2H-perfluorooctane sulfonate (8:2)	47.9 ug/mL
..LCN-EtFOSA-M_00002	07/14/19		WELLINGTON, Lot NEtFOSA0714M			(Purchased Reagent)	N-ethylperfluoro-1-octanesulfo namide	50 ug/mL
..LCN-EtFOSAA_00001	01/29/18		WELLINGTON, Lot NEtFOSAA0113			(Purchased Reagent)	N-ethyl perfluorooctane sulfonamidoacetic acid	50 ug/mL
..LCN-MeFOSA-M_00001	07/15/19		WELLINGTON, Lot NMeFOSA0714M			(Purchased Reagent)	MeFOSA	50 ug/mL
..LCN-MeFOSAA_00001	12/09/19		WELLINGTON, Lot NMeFOSAA1214			(Purchased Reagent)	N-methyl perfluorooctane sulfonamidoacetic acid	50 ug/mL
LCPFCIC_00020	03/01/17	12/01/16	MeOH/H2O, Lot 09285	5 mL	LCMPFCSU_00046	250 uL	13C2-PFHxDA	50 ng/mL
							13C2-PFtEDA	50 ng/mL
							13C4-PFHpA	50 ng/mL
							13C5 PFPeA	50 ng/mL
							13C8 FOSA	50 ng/mL
							13C4 PFBA	50 ng/mL
							13C2 PFDA	50 ng/mL
							13C2 PFDoA	50 ng/mL
							13C2 PFHxA	50 ng/mL
							18O2 PFHxS	47.3 ng/mL
							13C5 PFNA	50 ng/mL
							13C4 PFOA	50 ng/mL
							13C4 PFOS	47.8 ng/mL
							13C2 PFUnA	50 ng/mL
							LCPFACMXB_00007	125 uL
							Perfluorobutanoic acid (PFBA)	50 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Perfluorodecanesulfonic acid (PFDS)	48.25 ng/mL
							Perfluorodecanoic acid (PFDA)	50 ng/mL
							Perfluorododecanoic acid (PFDoA)	50 ng/mL
							Perfluoroheptanoic acid (PFHpA)	50 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	47.25 ng/mL
							Perfluorohexanoic acid (PFHxA)	50 ng/mL
							Perfluorononanoic acid (PFNA)	50 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	47.75 ng/mL
							Perfluorooctanoic acid (PFOA)	50 ng/mL
							Perfluoropentanoic acid (PFPeA)	50 ng/mL
							Perfluorotetradecanoic acid (PFTeA)	50 ng/mL
							Perfluorotridecanoic Acid (PFTriA)	50 ng/mL
							Perfluoroundecanoic acid (PFUnA)	50 ng/mL
					LCPFC3IM_00005	250 uL	Perfluorooctane Sulfonamide (FOSA)	50 ng/mL
.LCMPFCSU_00046	03/01/17	11/03/16	Methanol, Lot Baker 144541	50000 uL	LCM2PFHxDA_00008	1000 uL	13C2-PFHxDA	1 ug/mL
					LCM2PFTeDA_00007	1000 uL	13C2-PFTeDA	1 ug/mL
					LCM4PFHPA_00007	1000 uL	13C4-PFHpa	1 ug/mL
					LCM5PFPEA_00008	1000 uL	13C5 PFPeA	1 ug/mL
					LCM8FOSA_00011	1000 uL	13C8 FOSA	1 ug/mL
					LCMPFBA_00008	1000 uL	13C4 PFBA	1 ug/mL
					LCMPFDA_00011	1000 uL	13C2 PFDA	1 ug/mL
					LCMPFDoA_00008	1000 uL	13C2 PFDoA	1 ug/mL
					LCMPFHxA_00012	1000 uL	13C2 PFHxA	1 ug/mL
					LCMPFHxS_00008	1000 uL	1802 PFHxS	0.946 ug/mL
					LCMPFNA_00008	1000 uL	13C5 PFNA	1 ug/mL
					LCMPFOA_00012	1000 uL	13C4 PFOA	1 ug/mL
					LCMPFOS_00017	1000 uL	13C4 PFOS	0.956 ug/mL
					LCMPFUnA_00009	1000 uL	13C2 PFUnA	1 ug/mL
..LCM2PFHxDA_00008	01/07/21		Wellington Laboratories, Lot M2PFHxDA1112		(Purchased Reagent)		13C2-PFHxDA	50 ug/mL
..LCM2PFTeDA_00007	12/07/20		Wellington Laboratories, Lot M2PFTeDA1115		(Purchased Reagent)		13C2-PFTeDA	50 ug/mL
..LCM4PFHPA_00007	05/27/21		Wellington Laboratories, Lot M4PFHPA0516		(Purchased Reagent)		13C4-PFHpa	50 ug/mL
..LCM5PFPEA_00008	05/22/20		Wellington Laboratories, Lot M5PFPeA0515		(Purchased Reagent)		13C5 PFPeA	50 ug/mL
..LCM8FOSA_00011	12/22/17		Wellington Laboratories, Lot M8FOSA1215I		(Purchased Reagent)		13C8 FOSA	50 ug/mL
..LCMPFBA_00008	05/24/21		Wellington Laboratories, Lot MPFBA0516		(Purchased Reagent)		13C4 PFBA	50 ug/mL
..LCMPFDA_00011	08/19/20		Wellington Laboratories, Lot MPFDA0815		(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFDoA_00008	04/08/21		Wellington Laboratories, Lot MPFDoA0416		(Purchased Reagent)		13C2 PFDoA	50 ug/mL
..LCMPFHxA_00012	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL
..LCMPFHxS_00008	10/23/20		Wellington Laboratories, Lot MPFHxS1015		(Purchased Reagent)		1802 PFHxS	47.3 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
..LCMPFNA_00008	04/13/19		Wellington Laboratories, Lot MPFNA0414		(Purchased Reagent)		13C5 PFNA	50 ug/mL
..LCMPFOA_00012	01/22/21		Wellington Laboratories, Lot MPFOA0116		(Purchased Reagent)		13C4 PFOA	50 ug/mL
..LCMPFOS_00017	08/03/21		Wellington Laboratories, Lot MPFOS0816		(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
..LCMPFUDa_00009	02/12/21		Wellington Laboratories, Lot MPFUDa0216		(Purchased Reagent)		13C2 PFUnA	50 ug/mL
.LCPFACMXB_00007	11/06/20		Wellington Laboratories, Lot PFACMXB1115		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1.77 ug/mL
							Perfluorobutanoic acid (PFBA)	2 ug/mL
							Perfluorodecanesulfonic acid (PFDS)	1.93 ug/mL
							Perfluorodecanoic acid (PFDA)	2 ug/mL
							Perfluorododecanoic acid (PFDoA)	2 ug/mL
							Perfluoroheptanoic acid (PFHpA)	2 ug/mL
							Perfluorohexanesulfonic acid (PFHxS)	1.89 ug/mL
							Perfluorohexanoic acid (PFHxA)	2 ug/mL
							Perfluorononanoic acid (PFNA)	2 ug/mL
							Perfluorooctanesulfonic acid (PFOS)	1.91 ug/mL
							Perfluorooctanoic acid (PFOA)	2 ug/mL
							Perfluoropentanoic acid (PFPeA)	2 ug/mL
							Perfluorotetradecanoic acid (PFTeA)	2 ug/mL
							Perfluorotridecanoic Acid (PFTriA)	2 ug/mL
							Perfluoroundecanoic acid (PFUnA)	2 ug/mL
.LCPFC3IM_00005	06/01/17	12/01/16	Methanol, Lot 090285	5 mL	LCPFOSA_00008	0.1 mL	Perfluorooctane Sulfonamide (FOSA)	1000 ng/mL
..LCPFOSA_00008	09/02/17		Wellington Laboratories, Lot FOSA0815I		(Purchased Reagent)		Perfluorooctane Sulfonamide (FOSA)	50 ug/mL
LCPFCSP_00075	06/14/17	12/14/16	Methanol, Lot 090285	10000 uL	LCPFCSP_00074	5000 uL	Perfluorobutanoic acid (PFBA)	0.5 ug/mL
							Perfluorobutane Sulfonate	0.442 ug/mL
							Perfluorobutanesulfonic acid (PFBS)	0.442 ug/mL
							Perfluorodecanoic acid (PFDA)	0.5 ug/mL
							Perfluorododecanoic acid (PFDoA)	0.5 ug/mL
							Perfluorodecane Sulfonate	0.482 ug/mL
							Perfluorodecanesulfonic acid (PFDS)	0.482 ug/mL
							Perfluoroheptanoic acid (PFHpA)	0.5 ug/mL
							Perfluoroheptane Sulfonate	0.476 ug/mL
							Perfluoroheptanesulfonic Acid	0.476 ug/mL
							Perfluorohexanoic acid (PFHxA)	0.5 ug/mL
							Perfluorohexadecanoic acid	0.5 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Perfluorohexane Sulfonate	0.455 ug/mL
							Perfluorohexanesulfonic acid (PFHxS)	0.455 ug/mL
							Perfluorononanoic acid (PFNA)	0.5 ug/mL
							Perfluorooctanoic acid (PFOA)	0.5 ug/mL
							Perfluorooctadecanoic acid	0.5 ug/mL
							Perfluorooctanesulfonic acid (PFOS)	0.464 ug/mL
							Perfluorooctane Sulfonamide (FOSA)	0.5 ug/mL
							Perfluoropentanoic acid (PFPeA)	0.5 ug/mL
							Perfluorotetradecanoic acid (PFTeA)	0.5 ug/mL
							Perfluorotridecanoic Acid (PFTriA)	0.5 ug/mL
							Perfluoroundecanoic acid (PFUnA)	0.5 ug/mL
.LCPFCSP_00074	06/14/17	12/14/16	Methanol, Lot 090285	10000 uL	LCPFBA_00005	200 uL	Perfluorobutanoic acid (PFBA)	1 ug/mL
					LCPFBS_00005	200 uL	Perfluorobutane Sulfonate	0.884 ug/mL
							Perfluorobutanesulfonic acid (PFBS)	0.884 ug/mL
					LCPFDA_00005	200 uL	Perfluorodecanoic acid (PFDA)	1 ug/mL
					LCPFDoA_00005	200 uL	Perfluorododecanoic acid (PFDoA)	1 ug/mL
					LCPFDS_00006	200 uL	Perfluorodecane Sulfonate	0.964 ug/mL
							Perfluorodecanesulfonic acid (PFDS)	0.964 ug/mL
					LCPFHpA_00006	200 uL	Perfluoroheptanoic acid (PFHpA)	1 ug/mL
					LCPFHpS_00009	200 uL	Perfluoroheptane Sulfonate	0.952 ug/mL
							Perfluoroheptanesulfonic Acid	0.952 ug/mL
					LCPFHxA_00005	200 uL	Perfluorohexanoic acid (PFHxA)	1 ug/mL
					LCPFHxDA_00006	200 uL	Perfluorohexadecanoic acid	1 ug/mL
					LCPFHxS-br_00002	200 uL	Perfluorohexane Sulfonate	0.91 ug/mL
							Perfluorohexanesulfonic acid (PFHxS)	0.91 ug/mL
					LCPFNA_00006	200 uL	Perfluorononanoic acid (PFNA)	1 ug/mL
					LCPFOA_00006	200 uL	Perfluorooctanoic acid (PFOA)	1 ug/mL
					LCPFODA_00006	200 uL	Perfluorooctadecanoic acid	1 ug/mL
					LCPFOS-br_00002	200 uL	Perfluorooctanesulfonic acid (PFOS)	0.928 ug/mL
					LCPFOSA_00008	200 uL	Perfluorooctane Sulfonamide (FOSA)	1 ug/mL
					LCPFPeA_00005	200 uL	Perfluoropentanoic acid (PFPeA)	1 ug/mL
					LCPFTeDA_00005	200 uL	Perfluorotetradecanoic acid (PFTeA)	1 ug/mL
					LCPFTriDA_00005	200 uL	Perfluorotridecanoic Acid (PFTriA)	1 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LCPFUdA_00005	200 uL	Perfluoroundecanoic acid (PFUnA)	1 ug/mL
..LCPFBA_00005	05/27/21		Wellington Laboratories, Lot PFBA0516		(Purchased Reagent)		Perfluorobutanoic acid (PFBA)	50 ug/mL
..LCPFBS_00005	03/15/21		Wellington Laboratories, Lot LPFBS0316		(Purchased Reagent)		Perfluorobutane Sulfonate	44.2 ug/mL
							Perfluorobutanesulfonic acid (PFBS)	44.2 ug/mL
..LCPFDA_00005	07/02/20		Wellington Laboratories, Lot PFDA0615		(Purchased Reagent)		Perfluorodecanoic acid (PFDA)	50 ug/mL
..LCPFDoA_00005	01/30/20		Wellington Laboratories, Lot PFDoA0115		(Purchased Reagent)		Perfluorododecanoic acid (PFDoA)	50 ug/mL
..LCPFDS_00006	05/24/21		Wellington Laboratories, Lot LPFDS0516		(Purchased Reagent)		Perfluorodecane Sulfonate	48.2 ug/mL
							Perfluorodecanesulfonic acid (PFDS)	48.2 ug/mL
..LCPFHpA_00006	01/22/21		Wellington Laboratories, Lot PFHpA0116		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	50 ug/mL
..LCPFHpS_00009	11/06/20		Wellington Laboratories, Lot LPFHpS1115		(Purchased Reagent)		Perfluoroheptane Sulfonate	47.6 ug/mL
							Perfluoroheptanesulfonic Acid	47.6 ug/mL
..LCPFHxA_00005	12/22/20		Wellington Laboratories, Lot PFHxA1215		(Purchased Reagent)		Perfluorohexanoic acid (PFHxA)	50 ug/mL
..LCPFHxDA_00006	05/25/21		Wellington Laboratories, Lot PFHxDA0516		(Purchased Reagent)		Perfluorohexadecanoic acid	50 ug/mL
..LCPFHxS-br_00002	07/03/20		Wellington Laboratories, Lot brPFHxSK0615		(Purchased Reagent)		Perfluorohexane Sulfonate	45.5 ug/mL
							Perfluorohexanesulfonic acid (PFHxS)	45.5 ug/mL
..LCPFNA_00006	10/23/20		Wellington Laboratories, Lot PFNA1015		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	50 ug/mL
..LCPFOA_00006	11/06/20		Wellington Laboratories, Lot PFOA1115		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	50 ug/mL
..LCPFODA_00006	04/29/21		Wellington Laboratories, Lot PFODA0416		(Purchased Reagent)		Perfluorooctadecanoic acid	50 ug/mL
..LCPFOS-br_00002	10/14/20		Wellington Laboratories, Lot brPFOSK1015		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	46.4 ug/mL
..LCPFOSA_00008	09/02/17		Wellington Laboratories, Lot FOSA0815I		(Purchased Reagent)		Perfluorooctane Sulfonamide (FOSA)	50 ug/mL
..LCPFPeA_00005	01/30/20		Wellington Laboratories, Lot PFPeA0115		(Purchased Reagent)		Perfluoropentanoic acid (PFPeA)	50 ug/mL
..LCPFTeDA_00005	12/09/20		Wellington Laboratories, Lot PFTeDA1215		(Purchased Reagent)		Perfluorotetradecanoic acid (PFTeA)	50 ug/mL
..LCPFTrDA_00005	02/12/21		Wellington Laboratories, Lot PFTrDA0216		(Purchased Reagent)		Perfluorotridecanoic Acid (PFTriA)	50 ug/mL
..LCPFUdA_00005	08/19/20		Wellington Laboratories, Lot PFUdA0815		(Purchased Reagent)		Perfluoroundecanoic acid (PFUnA)	50 ug/mL

Reagent

LC6:2FTS_00001

r: 7hclis ev
S: 7hclis sw




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: 6:2FTS **LOT NUMBER:** 62FTS1014
COMPOUND: Sodium 1H,1H,2H,2H-perfluorooctane sulfonate

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: $C_8H_4F_{13}SO_3Na$ **MOLECULAR WEIGHT:** 450.15
CONCENTRATION: $50.0 \pm 2.5 \mu\text{g/ml}$ (Na salt) **SOLVENT(S):** Methanol
 $47.4 \pm 2.4 \mu\text{g/ml}$ (6:2FTS anion)
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 10/03/2014
EXPIRY DATE: (mm/dd/yyyy) 10/03/2017
RECOMMENDED STORAGE: Refrigerate ampoule

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 03/27/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: 6:2FTS; LC/MS Data (TIC and Mass Spectrum)

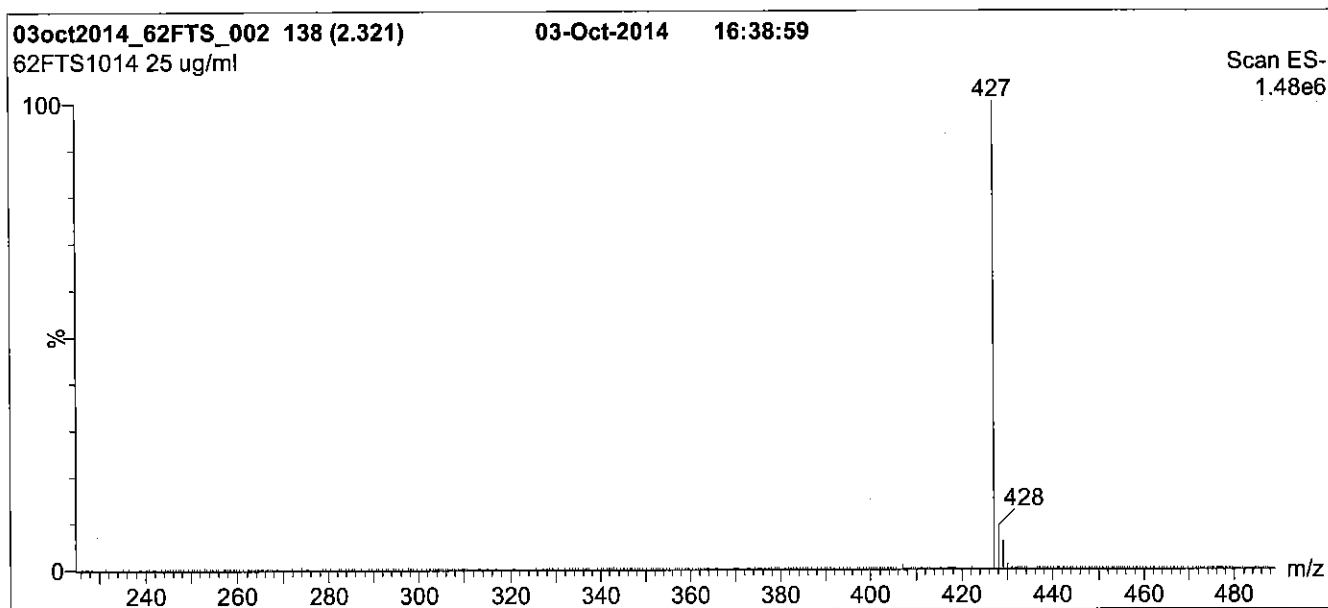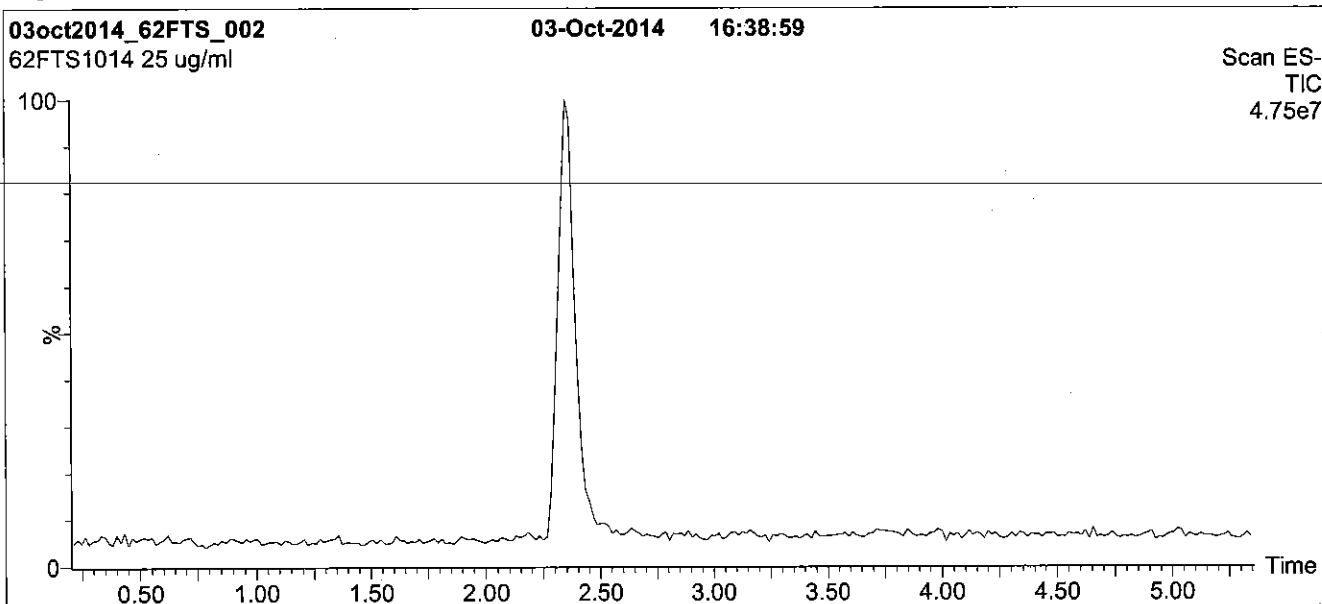

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 55% (80:20 MeOH:ACN) / 45% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 2 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 30.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: 6:2FTS; LC/MS/MS Data (Selected MRM Transitions)

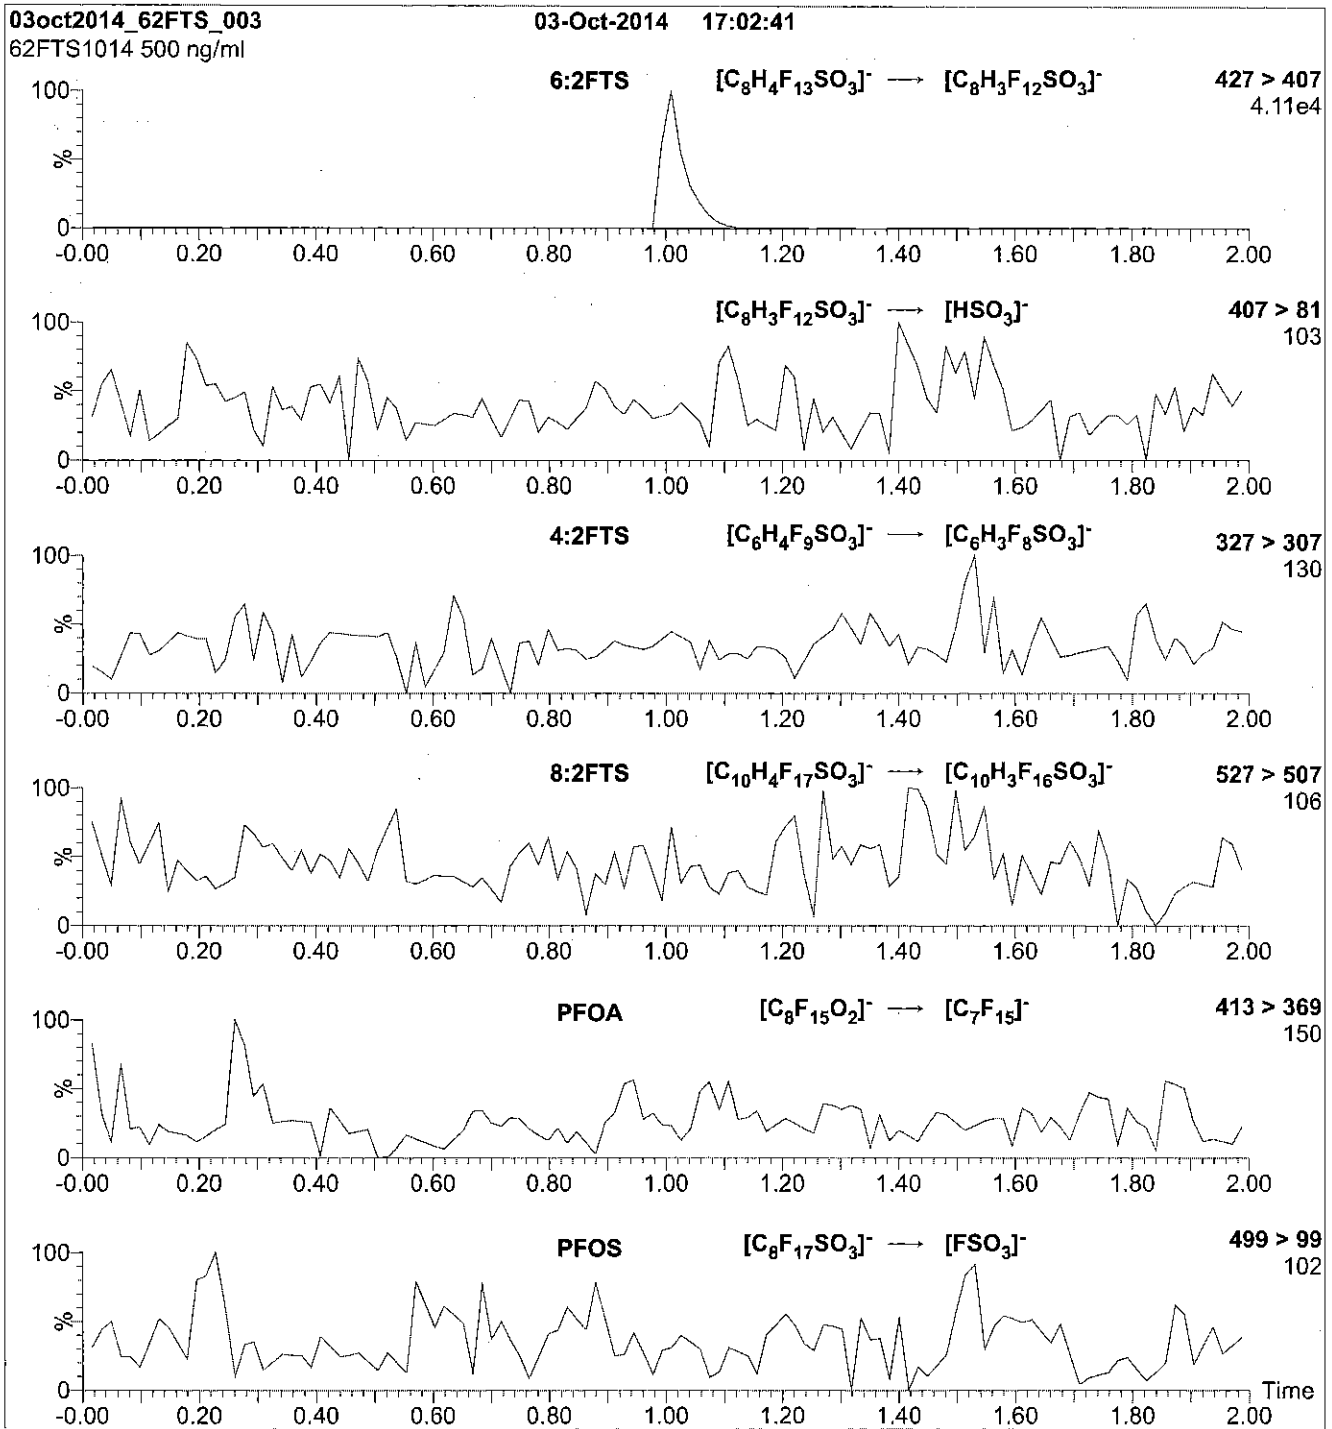

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml 6:2FTS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.50e-3
Collision Energy (eV) = 25

Reagent

LC6:2FTS_00002

R: 8/23/16 SBC



715544
ID: LC6:2FTS_00002
Exp: 06/25/21 Prod: SBC
6:2FTS




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: 6:2FTS **LOT NUMBER:** 62FTS0616
COMPOUND: Sodium 1H,1H,2H,2H-perfluorooctane sulfonate

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA:	C ₈ H ₄ F ₁₃ SO ₃ Na	MOLECULAR WEIGHT:	450.15
CONCENTRATION:	50.0 ± 2.5 µg/ml (Na salt)	SOLVENT(S):	Methanol
	47.4 ± 2.4 µg/ml (6:2FTS anion)		
CHEMICAL PURITY:	>98%		
LAST TESTED: (mm/dd/yyyy)	06/25/2016		
EXPIRY DATE: (mm/dd/yyyy)	06/25/2021		
RECOMMENDED STORAGE:	Refrigerate ampoule		

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim

Date: 06/29/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • Info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: 6:2FTS; LC/MS Data (TIC and Mass Spectrum)

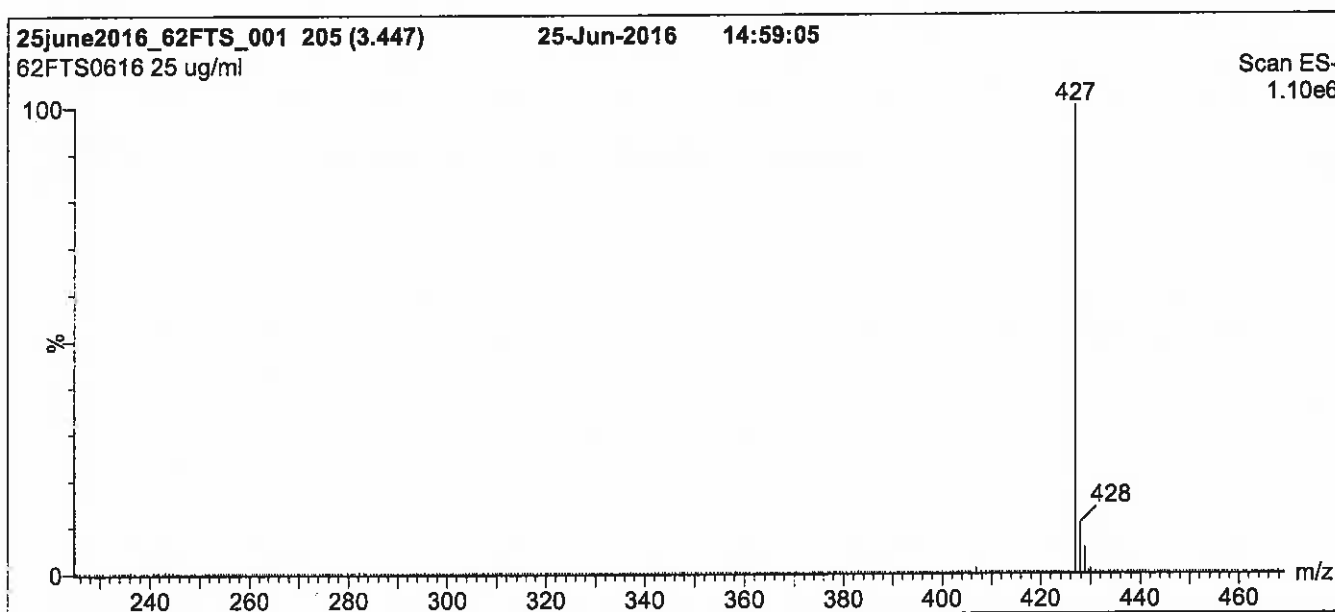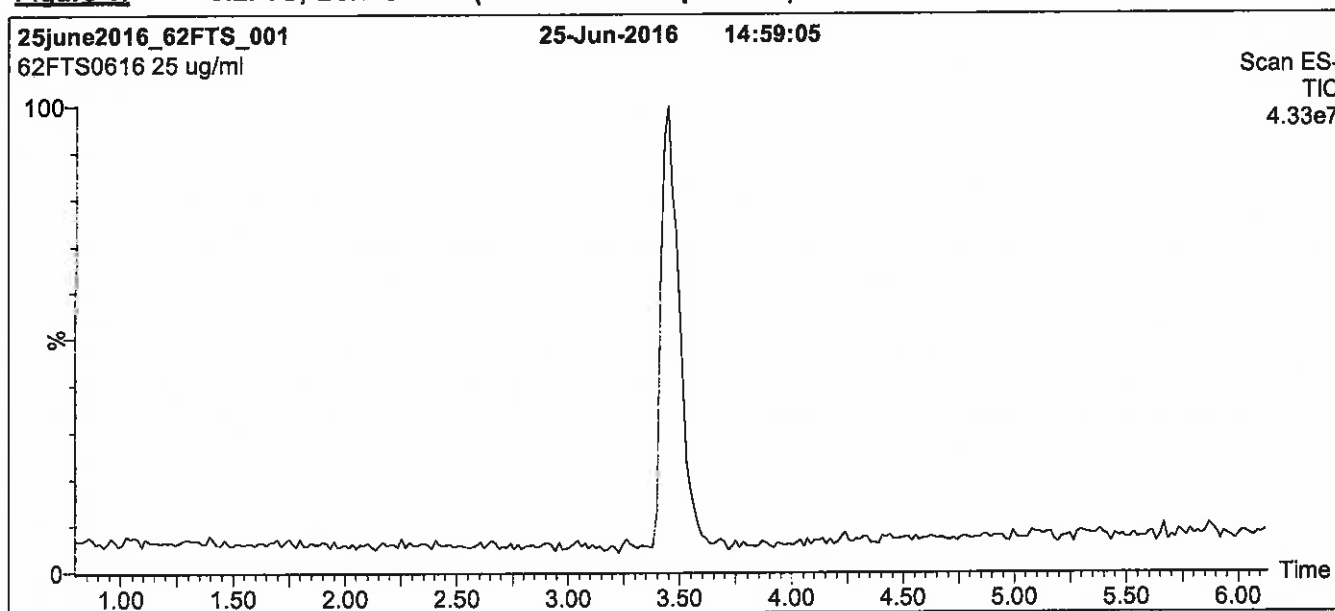

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 30.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: 6:2FTS; LC/MS/MS Data (Selected MRM Transitions)

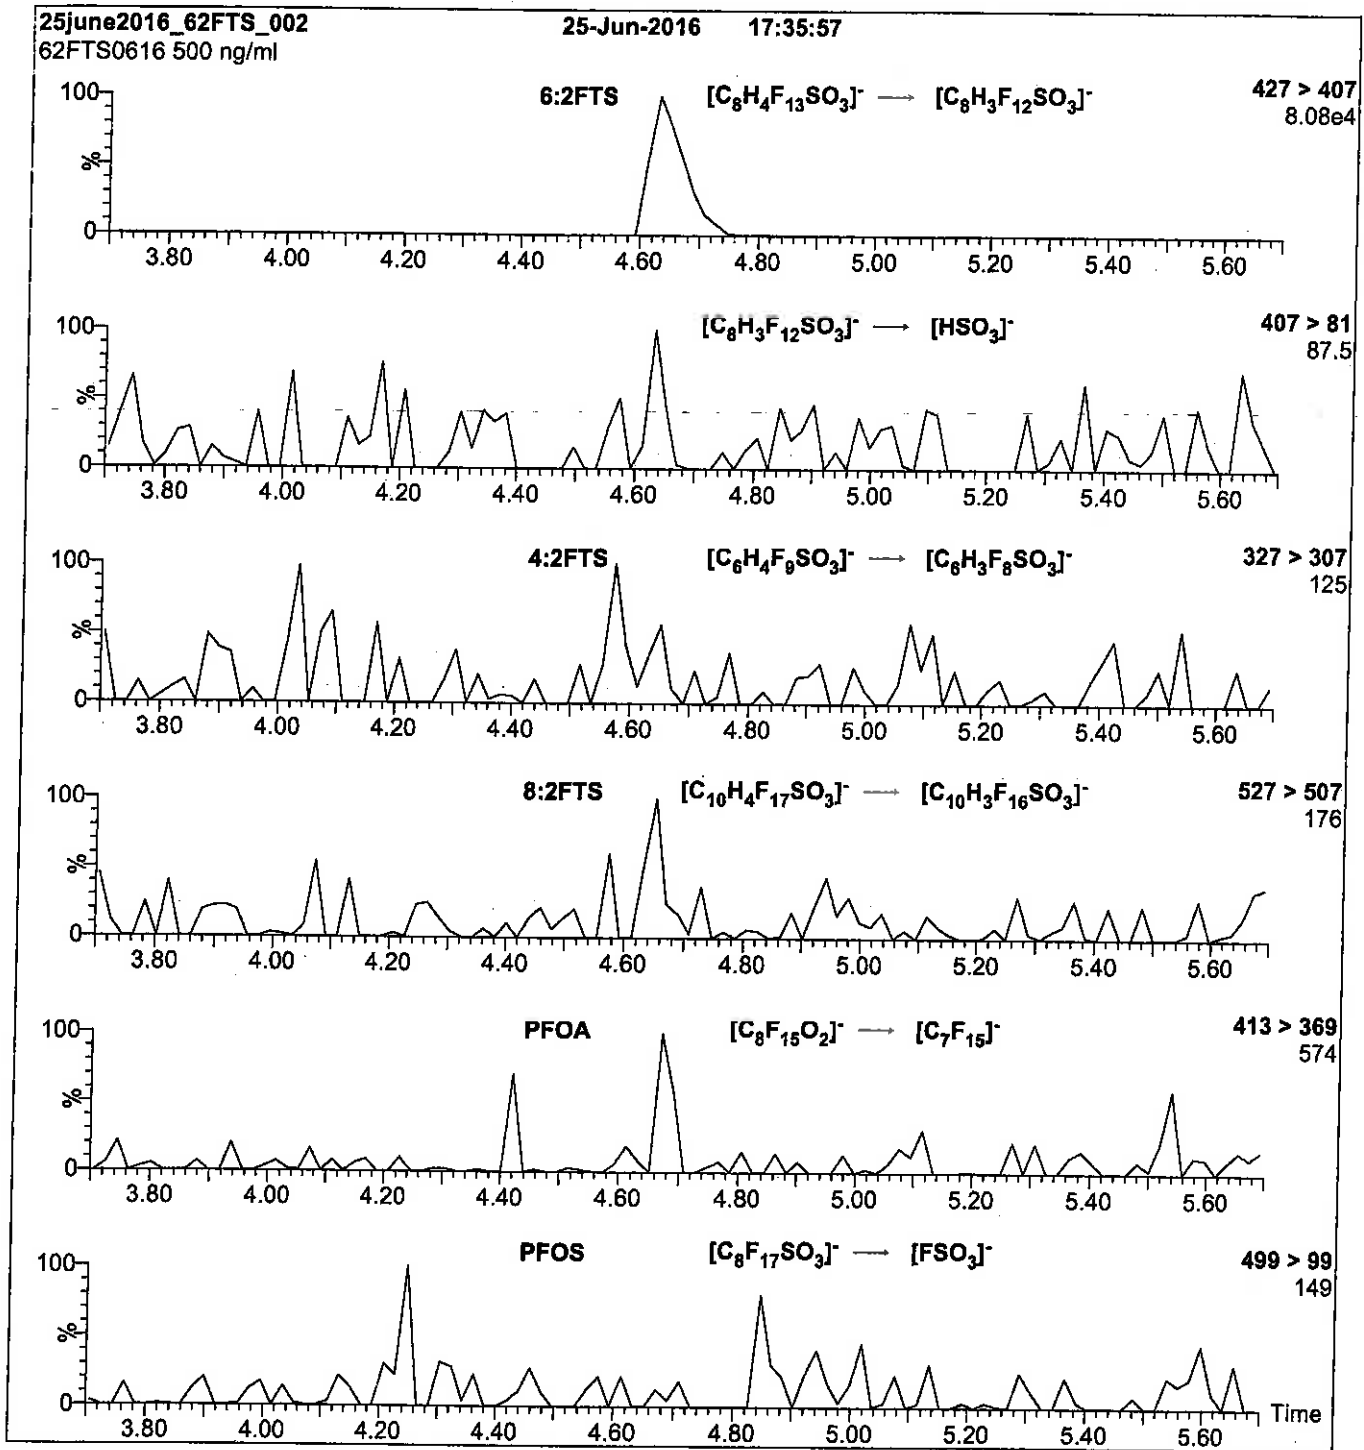

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml 6:2FTS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.46e-3
Collision Energy (eV) = 25

Reagent

LC8 : 2FTS _ 00001

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: 8:2FTS; LC/MS Data (TIC and Mass Spectrum)

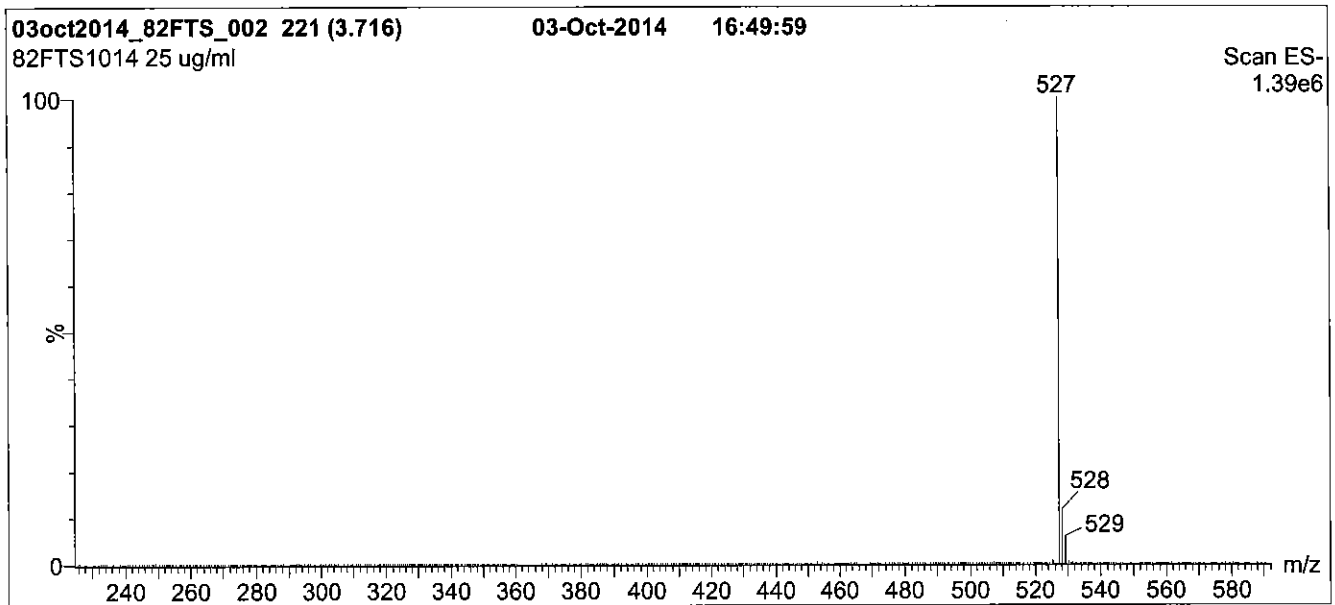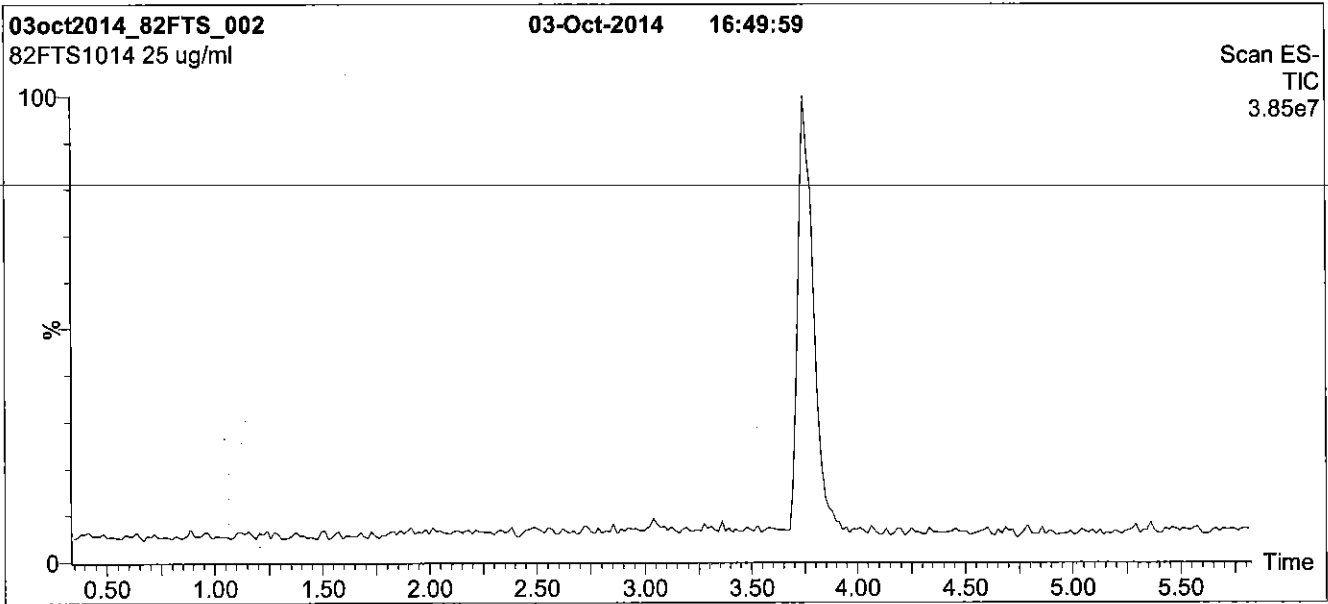

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 55% (80:20 MeOH:ACN) / 45% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 2 min.
Return to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 30.00
Cone Gas Flow (l/hr) = 100
Desolvation Gas Flow (l/hr) = 750

Figure 2: 8:2FTS; LC/MS/MS Data (Selected MRM Transitions)

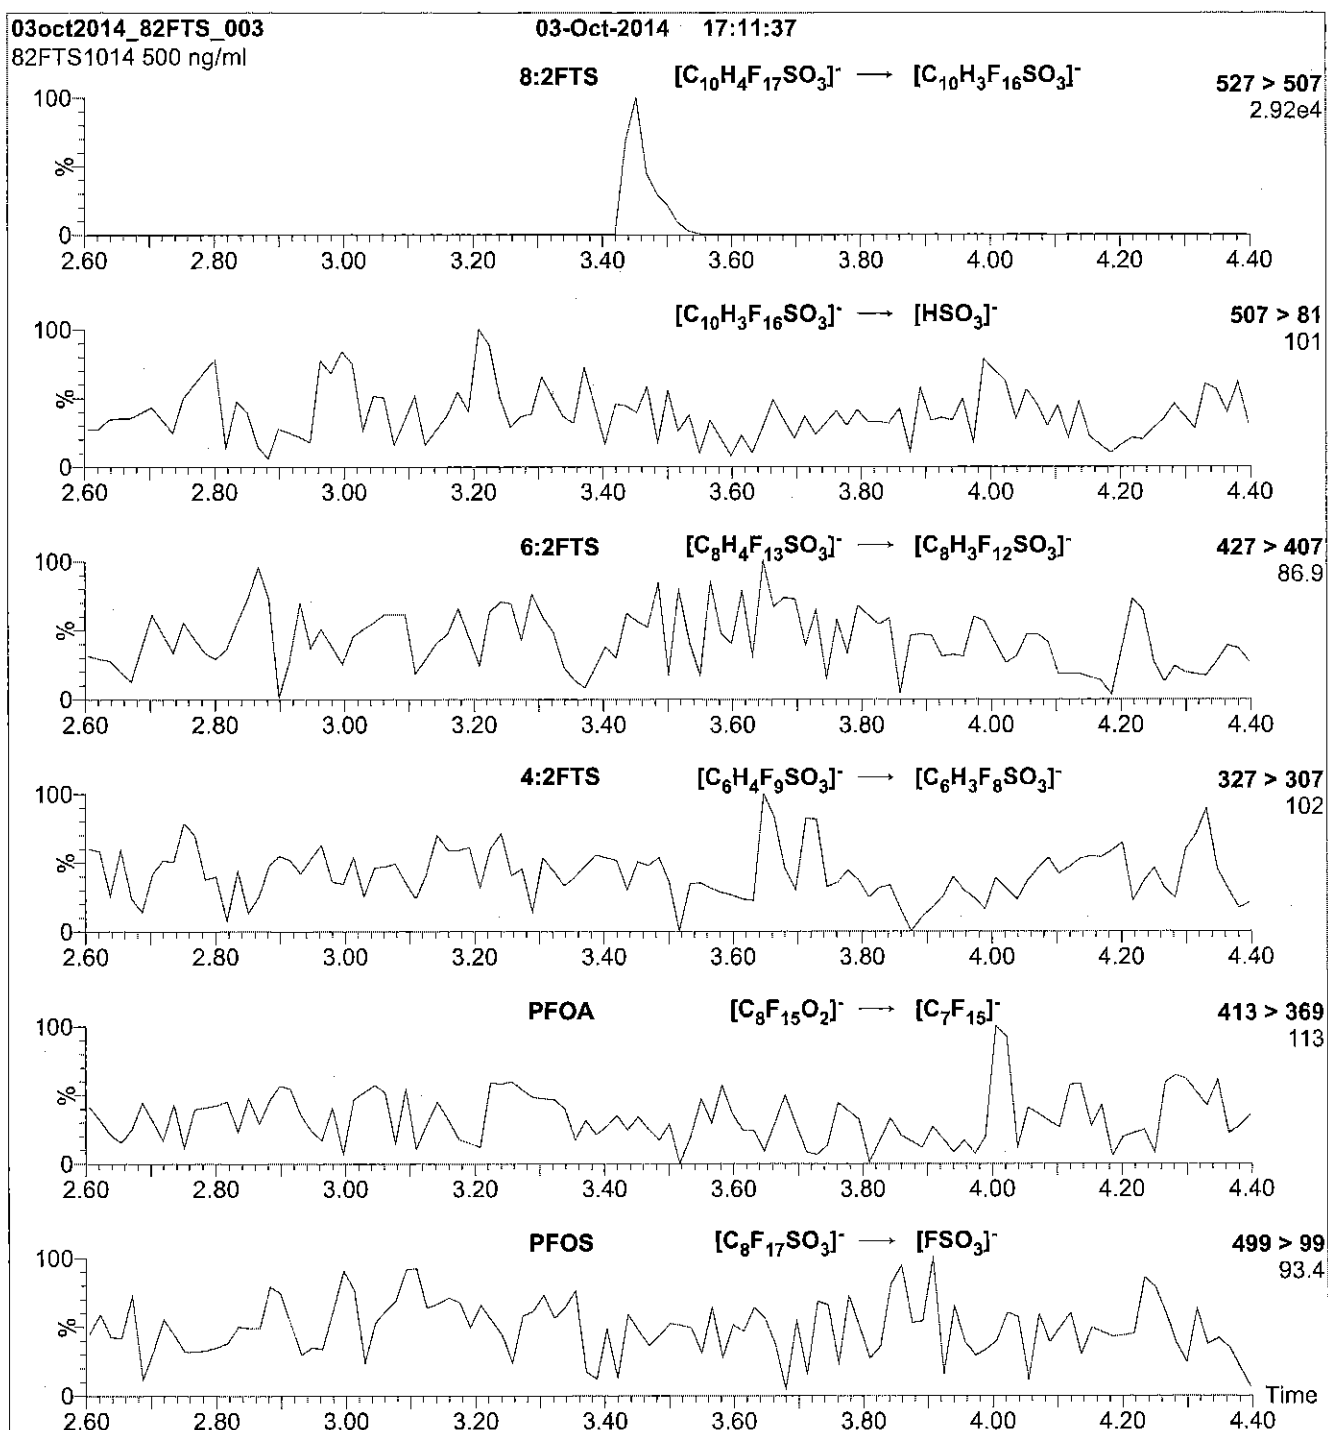

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml 8:2FTS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.50e-3
Collision Energy (eV) = 30

Reagent

LC8 : 2FTS _ 00002

R: 8/23/16 SBC

715545
ID: LC8:2FTS_00002
Exp: 10/23/20 Prod: SBC
8:2FTS




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: 8:2FTS **LOT NUMBER:** 82FTS1015
COMPOUND: Sodium 1H,1H,2H,2H-perfluorodecane sulfonate

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: C₁₀H₄F₁₇SO₃Na **MOLECULAR WEIGHT:** 550.16
CONCENTRATION: 50.0 ± 2.5 µg/ml (Na salt) **SOLVENT(S):** Methanol
47.9 ± 2.4 µg/ml (8:2FTS anion)
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 10/23/2015
EXPIRY DATE: (mm/dd/yyyy) 10/23/2020
RECOMMENDED STORAGE: Refrigerate ampoule


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

See page 2 for further details.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 10/27/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: 8:2FTS; LC/MS Data (TIC and Mass Spectrum)

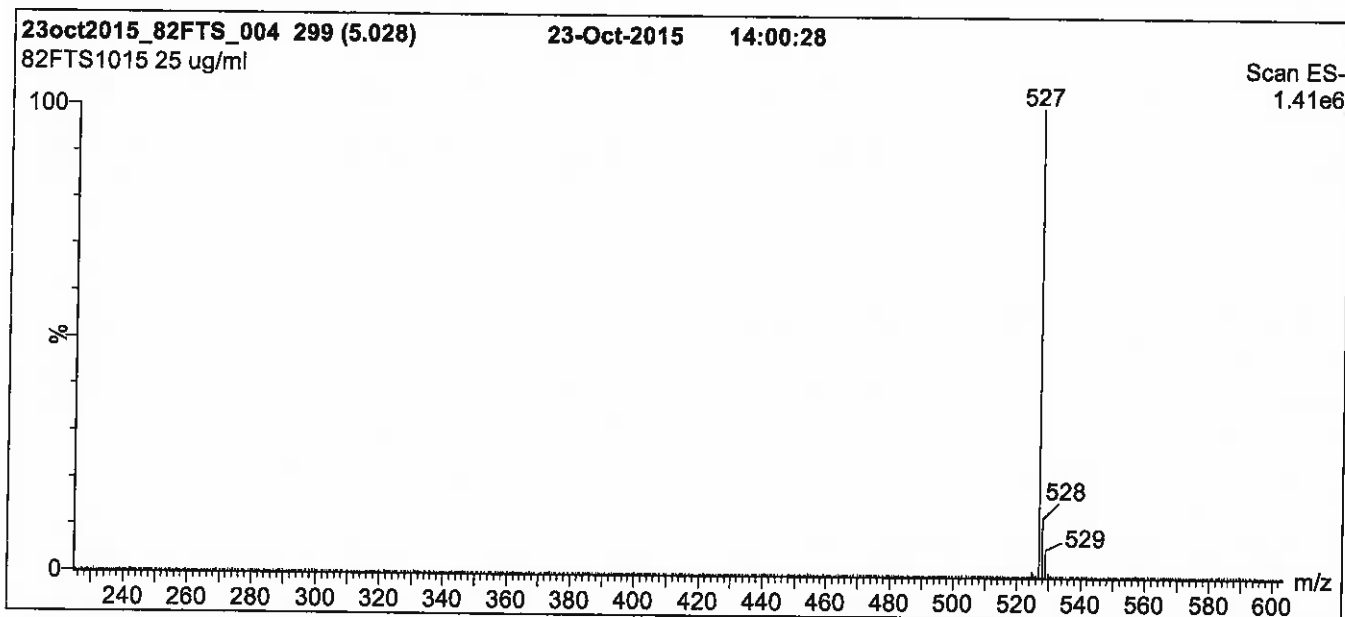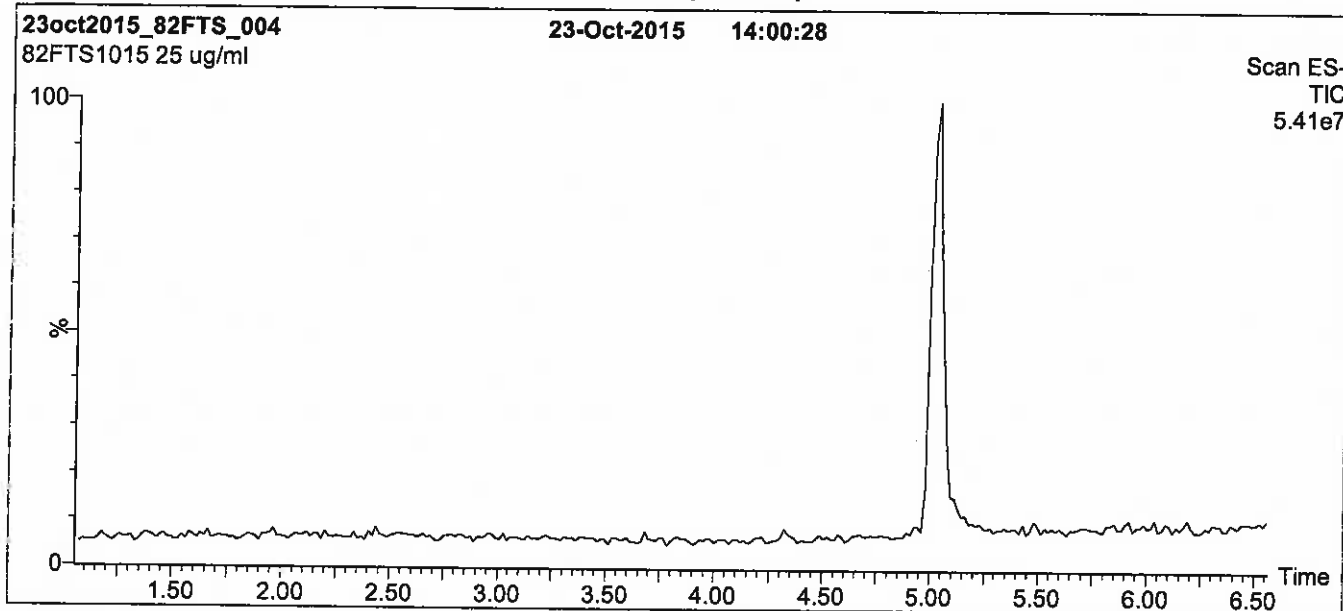

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 50% (80:20 MeOH:ACN) / 50% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 2 min.
 Return to Initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 30.00
 Cone Gas Flow (l/hr) = 100
 Desolvation Gas Flow (l/hr) = 750

Figure 2: 8:2FTS; LC/MS/MS Data (Selected MRM Transitions)

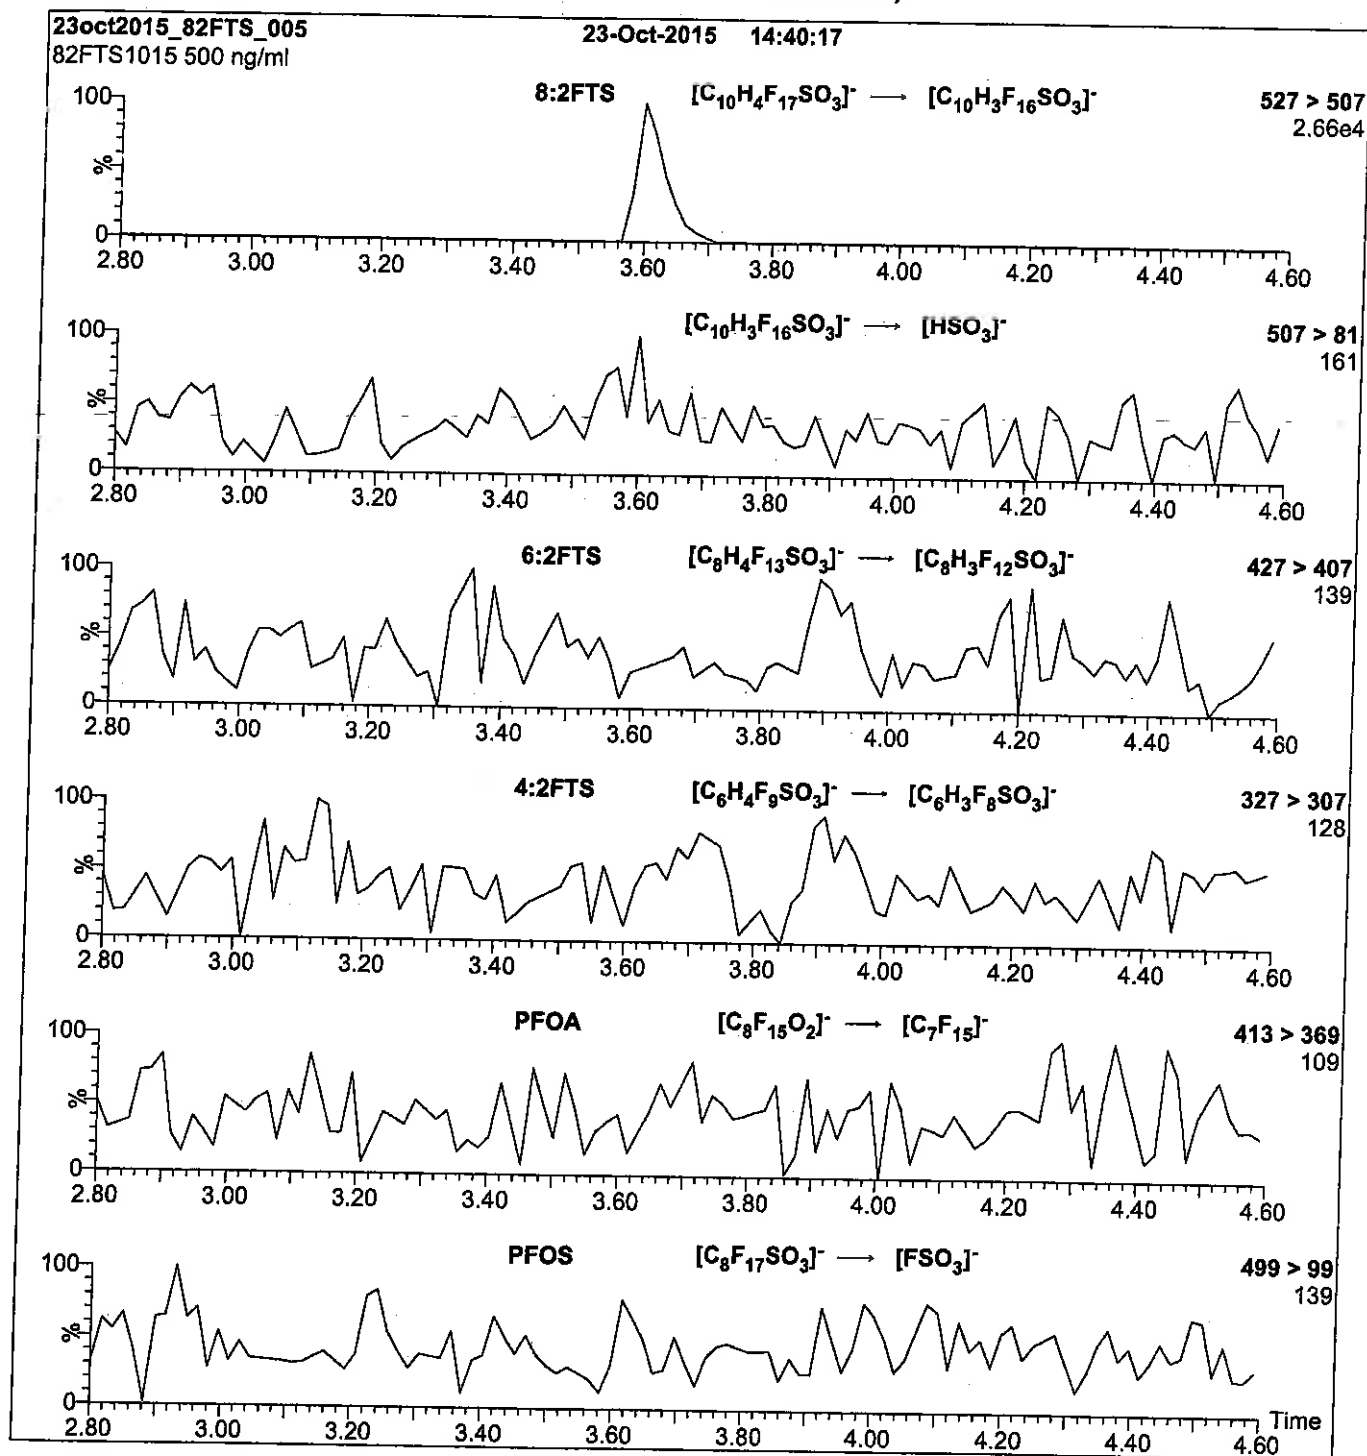

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml 8:2FTS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.28e-3
Collision Energy (eV) = 30

Reagent

LCd-NEtFOSA-M_00001

C: 7/16/15 8/



WELLINGTON LABORATORIES


CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: d-N-EtFOSA-M
COMPOUND: N-ethyl-d₅-perfluoro-1-octanesulfonamide

LOT NUMBER: dNEtFOSA0314M

STRUCTURE:

CAS #: Not available



MOLECULAR FORMULA: C₁₀D₅HF₁₇NO₂S
CONCENTRATION: 50 ± 2.5 µg/ml
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 03/10/2014
EXPIRY DATE: (mm/dd/yyyy) 03/10/2019
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

MOLECULAR WEIGHT: 532.23
SOLVENT(S): Methanol
ISOTOPIC PURITY: ≥98% ²H₅

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim

Date: 04/01/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: d-N-EtFOSA-M; LC/MS Data (TIC and Mass Spectrum)

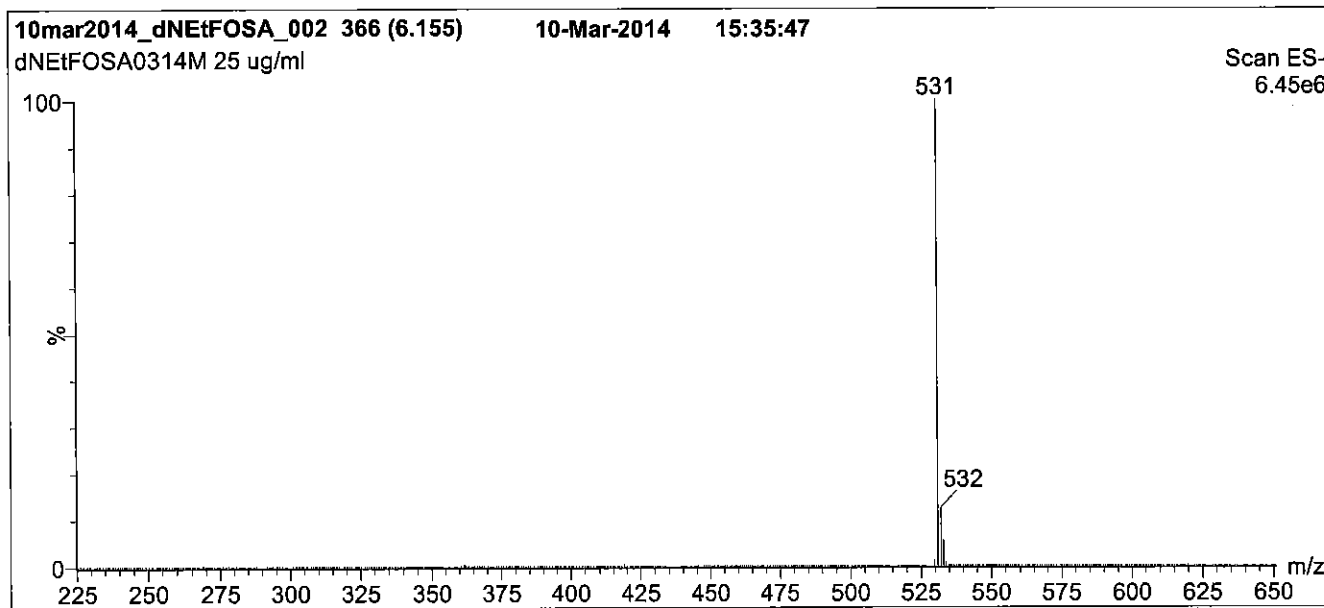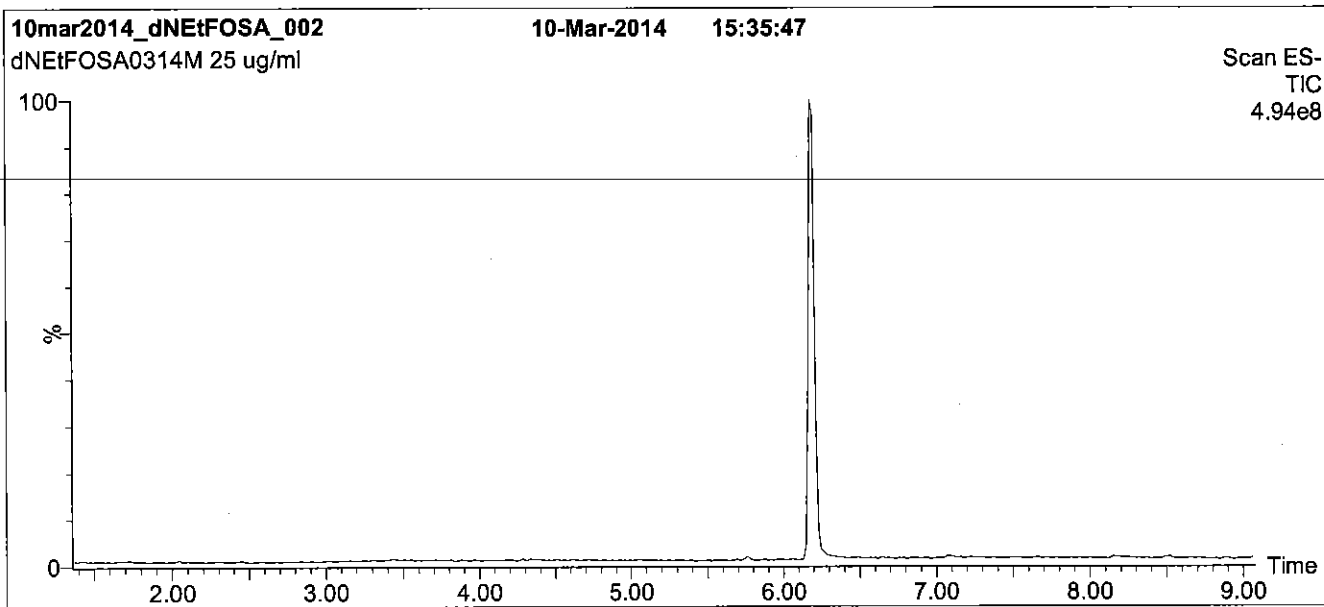

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 40% H₂O / 60% (80:20 MeOH:ACN)
 (both with 10mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 950 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 40.00
 Cone Gas Flow (l/hr) = 100
 Desolvation Gas Flow (l/hr) = 750

Figure 2: d-N-EtFOSA-M; LC/MS/MS Data (Selected MRM Transitions)

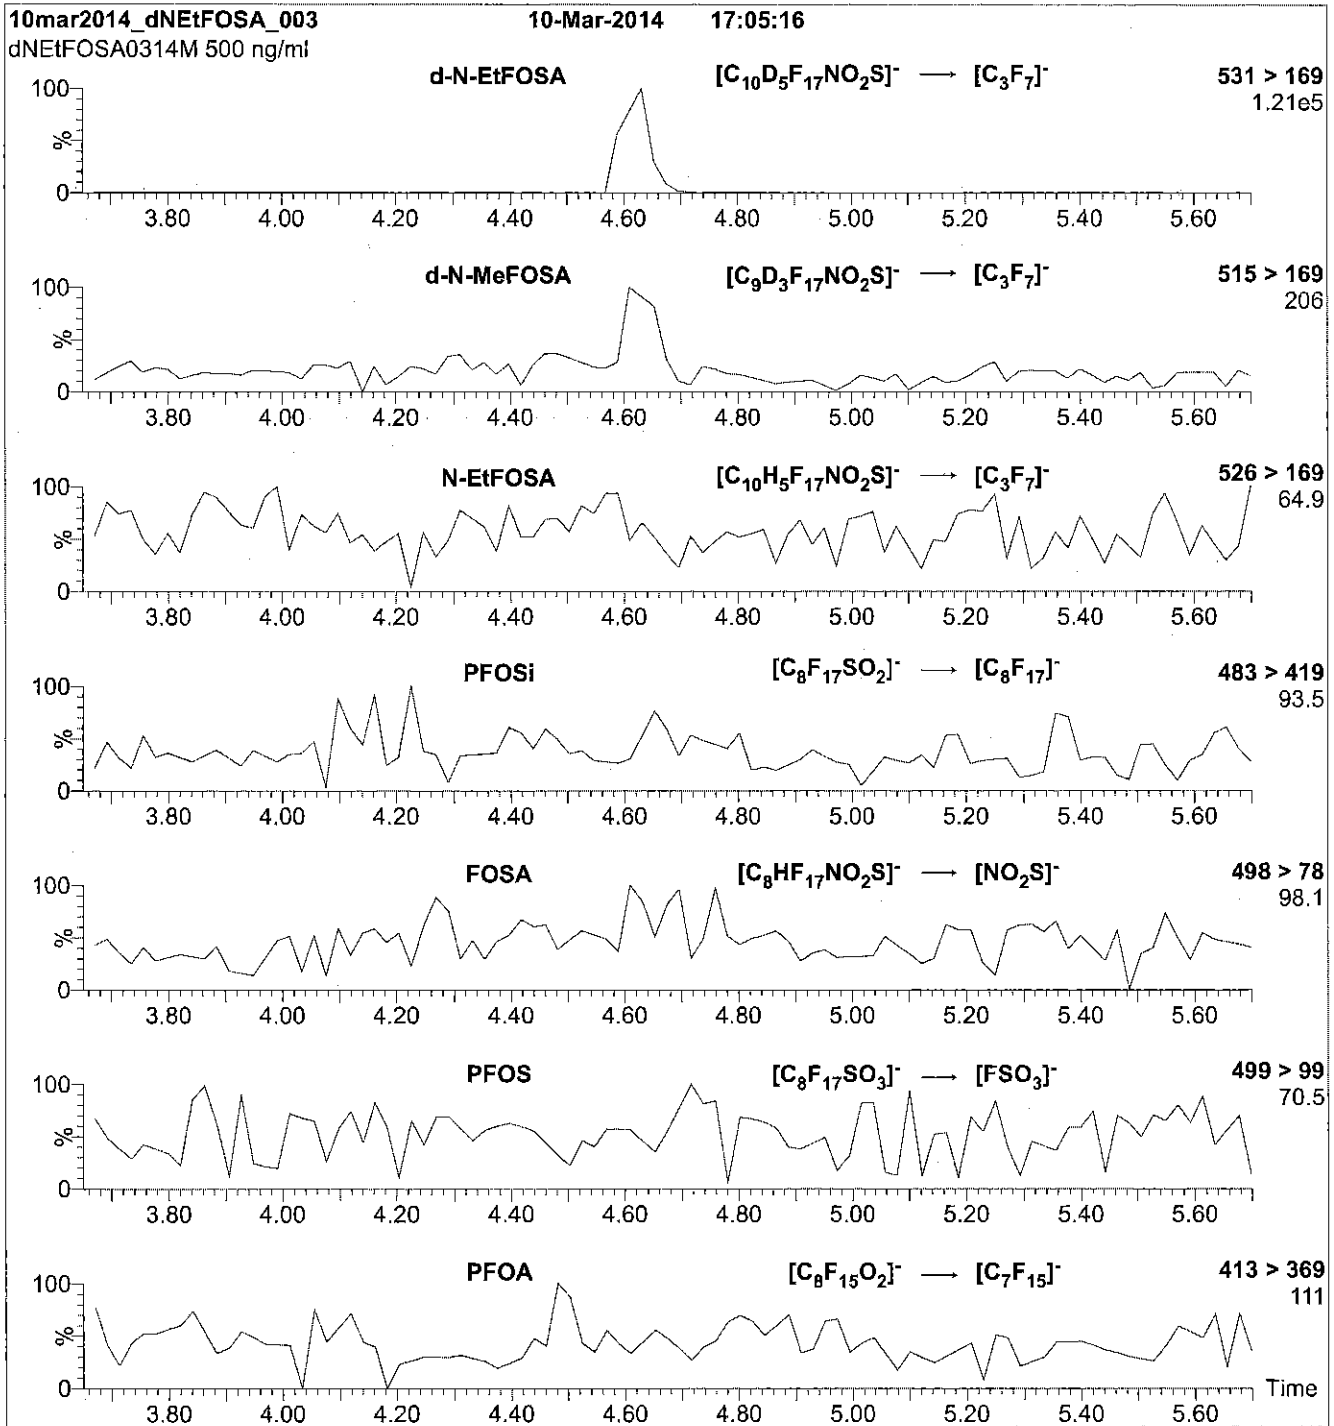

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml d-N-EtFOSA-M)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.43e-3
Collision Energy (eV) = 25

Reagent

LCd-NEtFOSA-M_00002

R-7/6/16 CAW



671571
ID: LCd-NEtFOSA-M_00002
Exp: 03/10/19 Pipd: CBW
d-N-EtFOSA-M




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: d-N-EtFOSA-M **LOT NUMBER:** dNEtFOSA0314M
COMPOUND: N-ethyl-d₅-perfluoro-1-octanesulfonamide

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: C₁₀D₅HF₁₇NO₂S **MOLECULAR WEIGHT:** 532.23
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Methanol
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥98% ²H₅
LAST TESTED: (mm/dd/yyyy) 03/10/2014
EXPIRY DATE: (mm/dd/yyyy) 03/10/2019
RECOMMENDED STORAGE: Store ampoule in a cool, dark place


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:  **Date:** 04/01/2015
B.G. Chittim (mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at Info@well-labs.com

Figure 1: d-N-EtFOSA-M; LC/MS Data (TIC and Mass Spectrum)

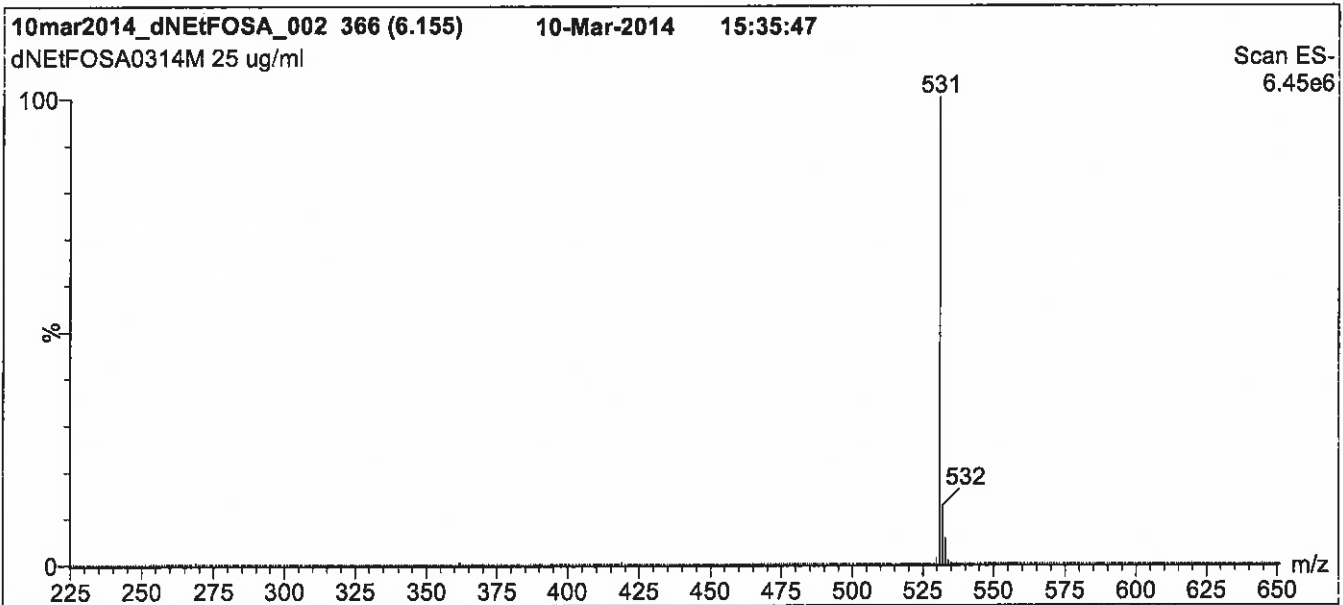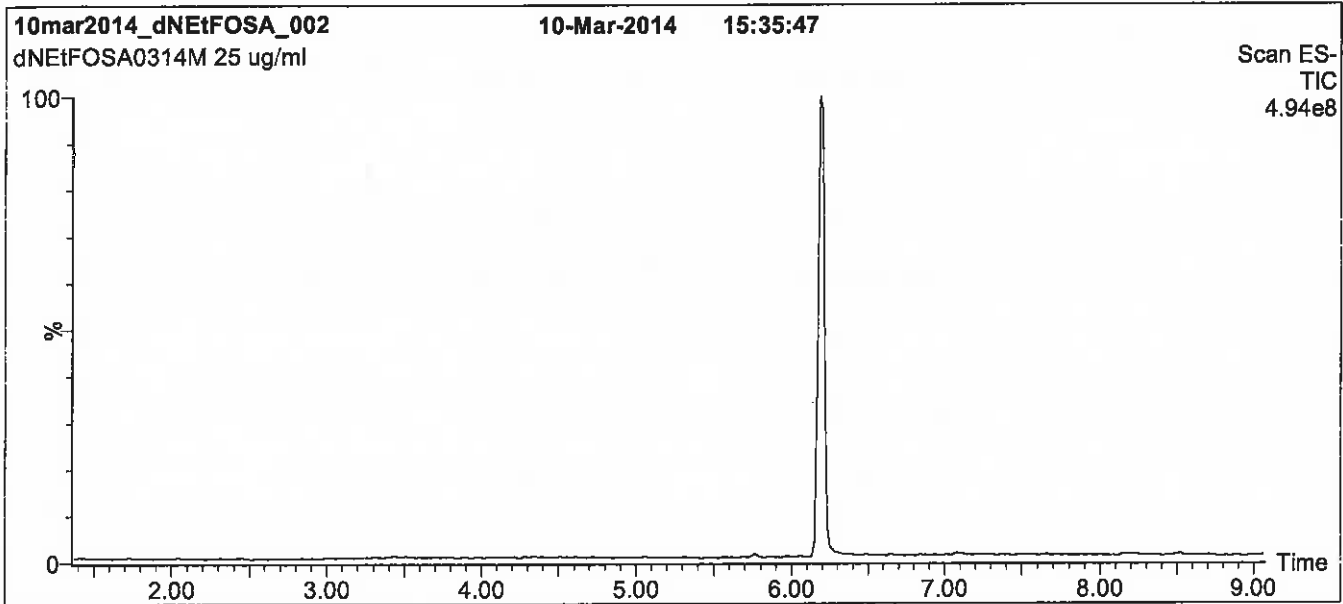

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μm, 2.1 x 100 mm

Mobile phase: Gracient
 Start: 40% H₂O / 60% (80:20 MeOH:ACN)
 (both with 10mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μl/min

MS Parameters

Experiment: Full Scan (225 - 950 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 40.00
 Cone Gas Flow (l/hr) = 100
 Desolvation Gas Flow (l/hr) = 750

Figure 2: d-N-EtFOSA-M; LC/MS/MS Data (Selected MRM Transitions)

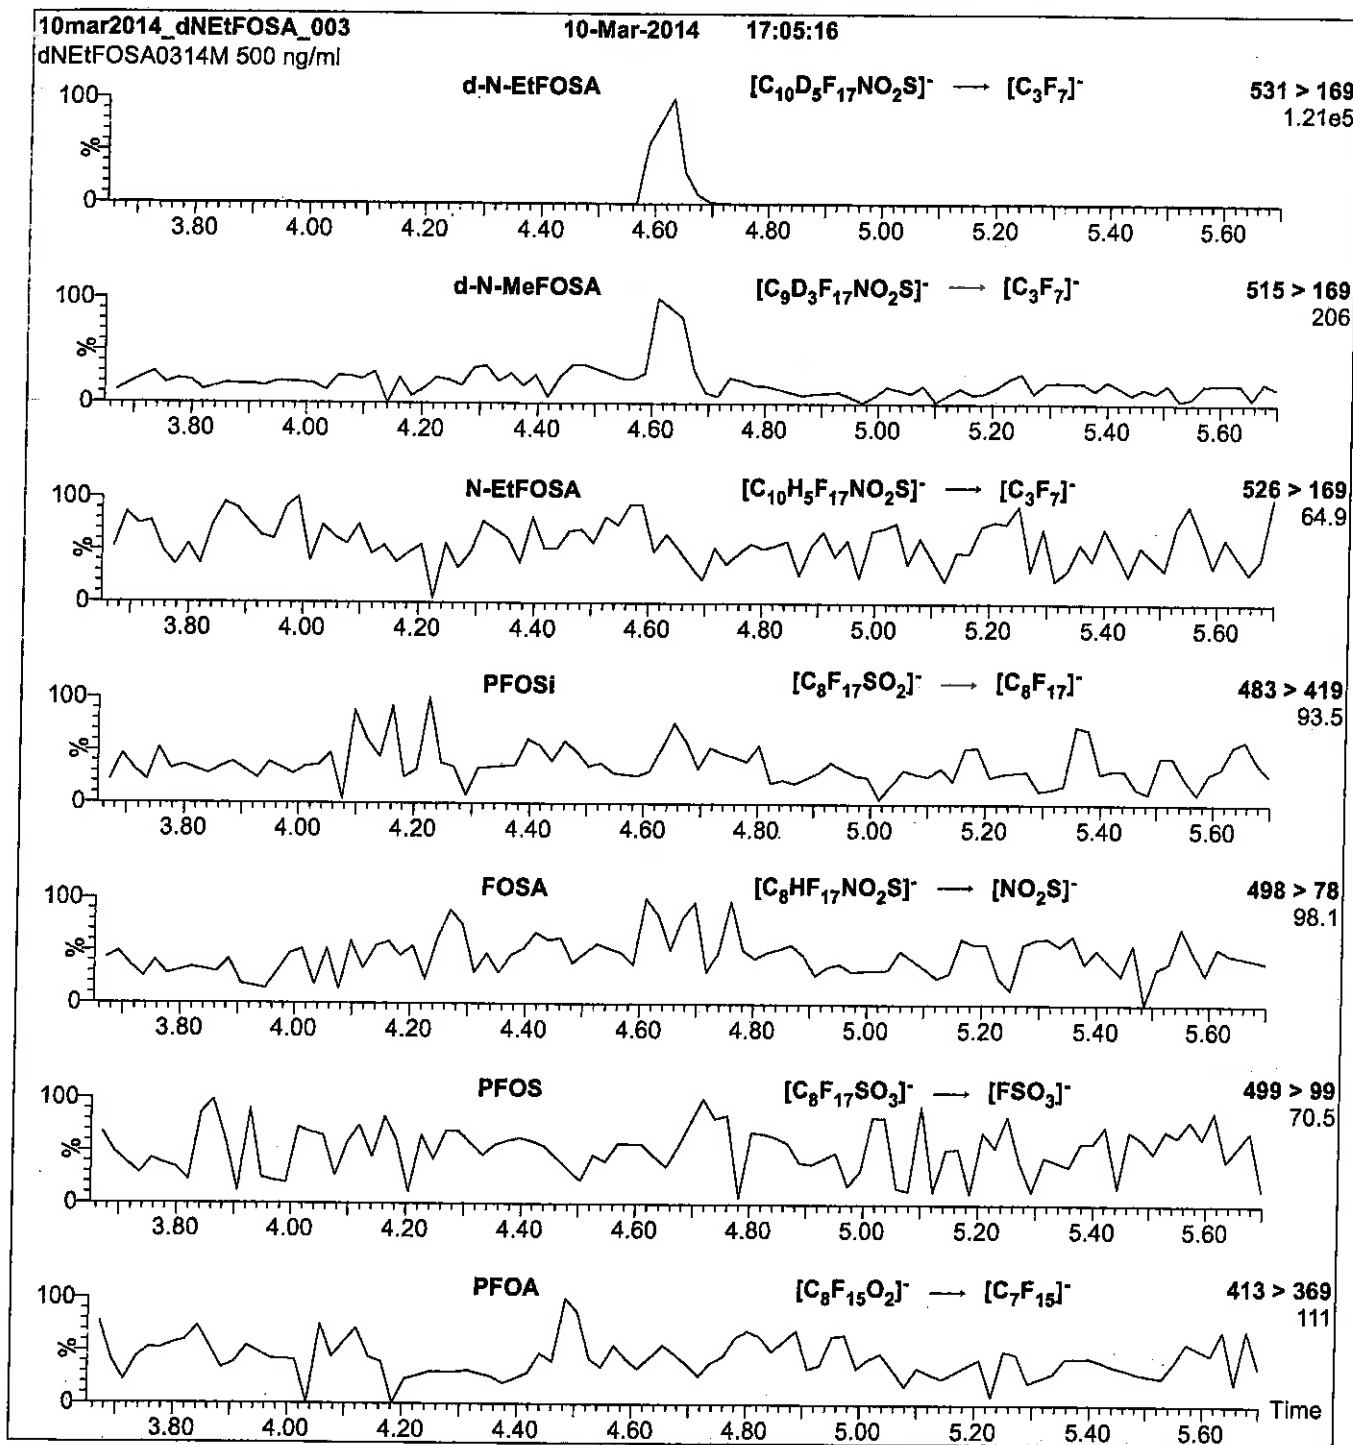

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml d-N-EtFOSA-M)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.43e-3
Collision Energy (eV) = 25

Reagent

LCd-NMeFOSA-M_00001

r: 7/16/15 SKW



WELLINGTON LABORATORIES


CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: d-N-MeFOSA-M
COMPOUND: N-methyl-d₃-perfluoro-1-octanesulfonamide

LOT NUMBER: dNMeFOSA0114M

STRUCTURE:

CAS #: Not available

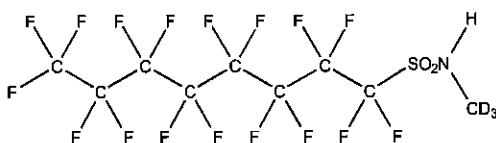

MOLECULAR FORMULA: C₉D₃HF₁₇NO₂S
CONCENTRATION: 50 ± 2.5 µg/ml
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 01/28/2014
EXPIRY DATE: (mm/dd/yyyy) 01/28/2019
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

MOLECULAR WEIGHT: 516.19
SOLVENT(S): Methanol
ISOTOPIC PURITY: ≥98% ²H₃


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim

Date: 04/01/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: d-N-MeFOSA-M; LC/MS Data (TIC and Mass Spectrum)

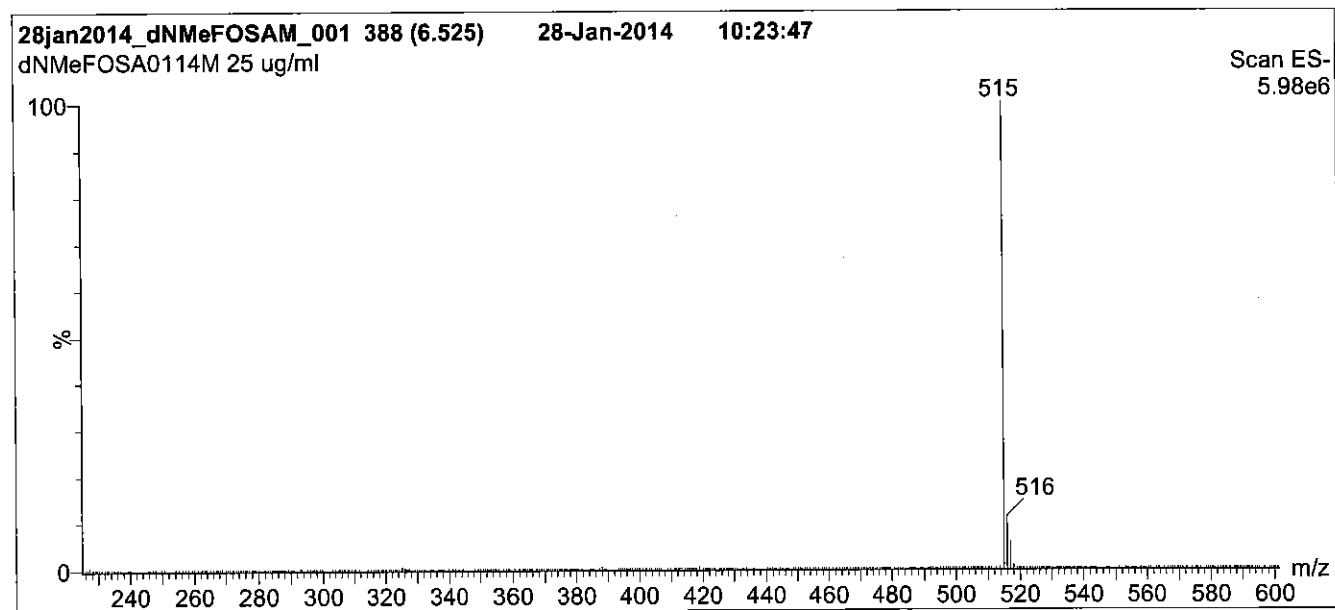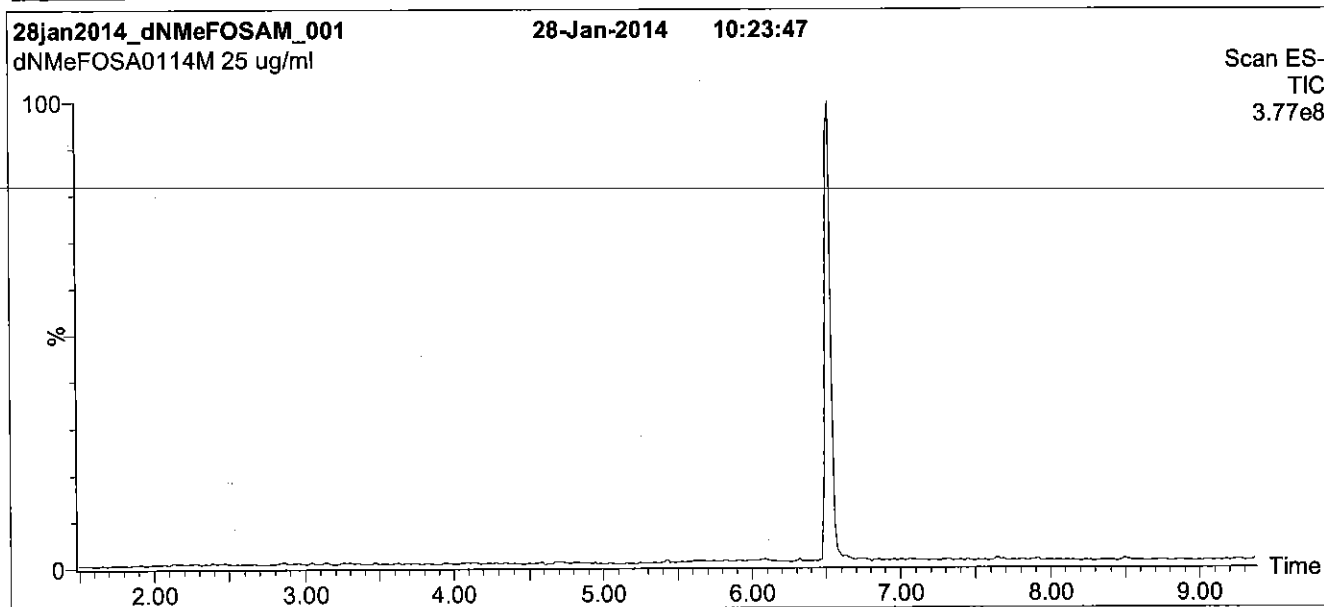

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 50% H₂O / 50% (80:20 MeOH:ACN)
 (both with 10mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for
 1.5 min. Return to initial conditions over 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.50
 Cone Voltage (V) = 40.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: d-N-MeFOSA-M; LC/MS/MS Data (Selected MRM Transitions)

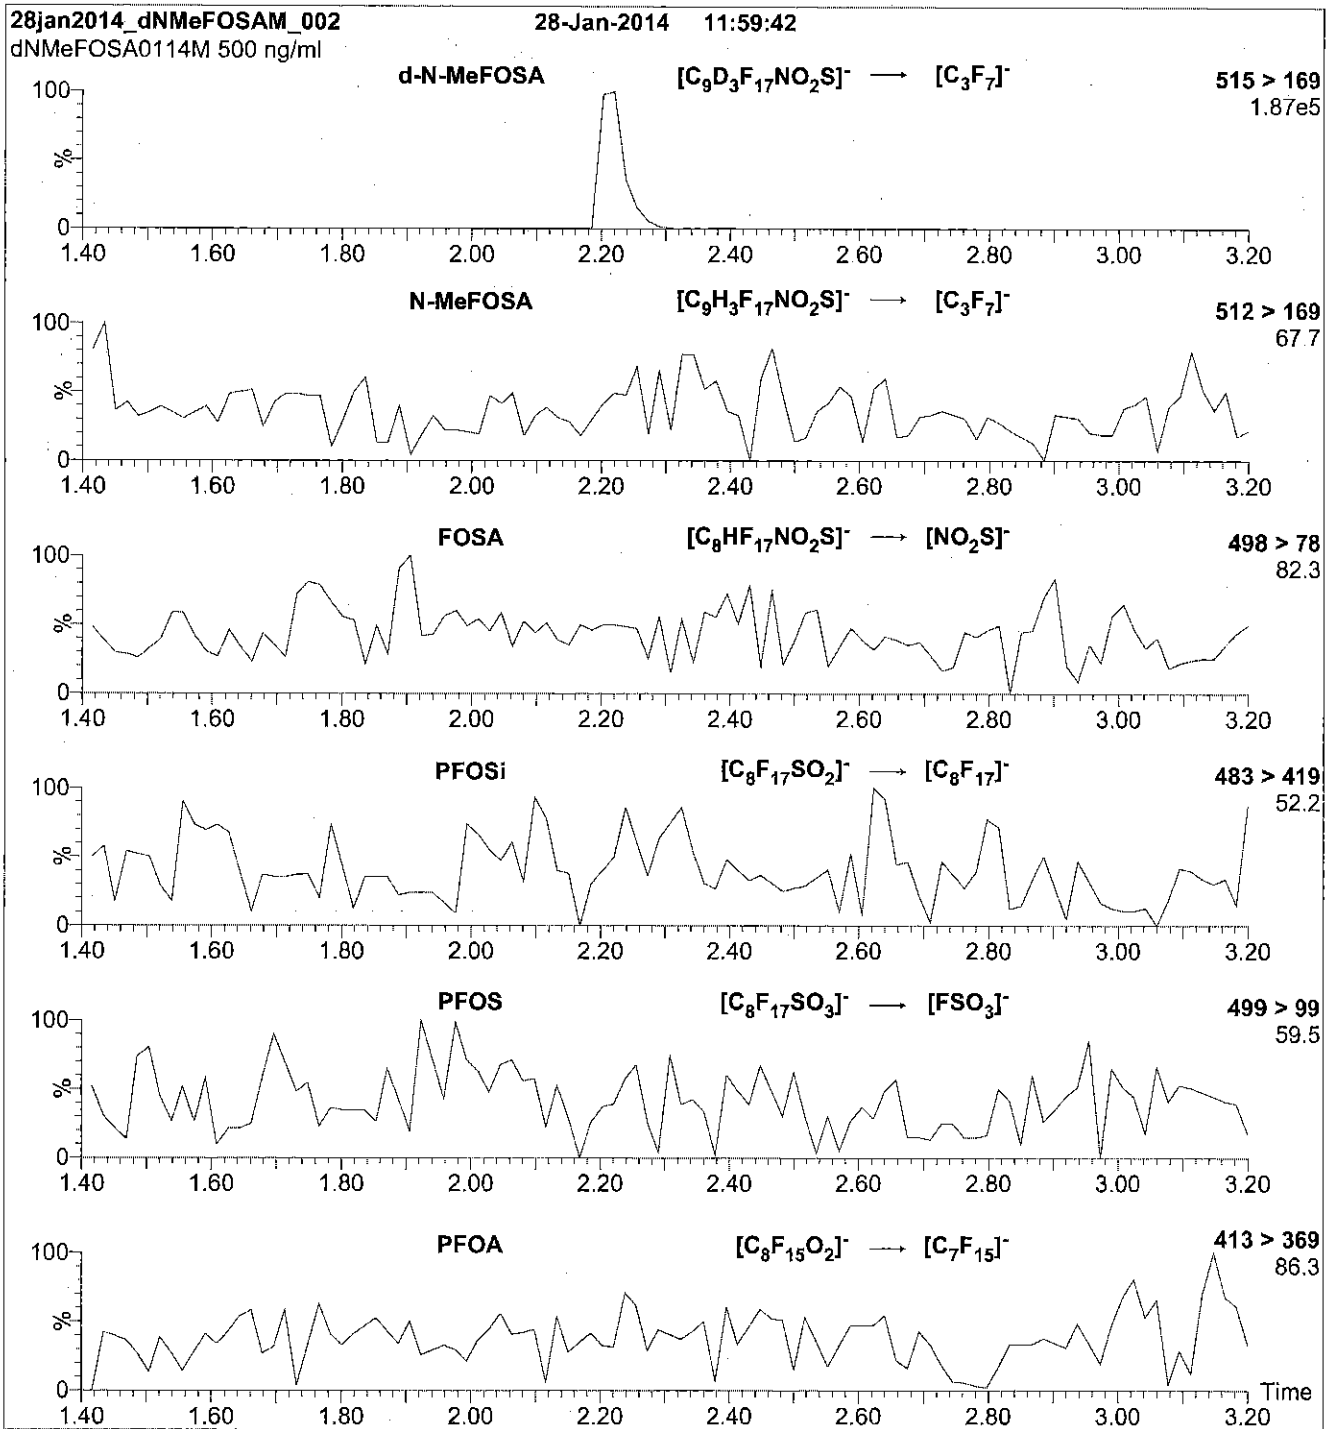

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml d-N-MeFOSA-M)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.50e-3
Collision Energy (eV) = 30

Reagent

LCd-NMeFOSA-M_00002



671625

ID: LCd-NMeFOSA-M_00002

Exp: 06/10/21 Prep: CBW

d-N-MeFOSA-M




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: d-N-MeFOSA-M **LOT NUMBER:** dNMeFOSA0616M
COMPOUND: N-methyl-d₃-perfluoro-1-octanesulfonamide

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: C₉D₃HF₁₇NO₂S
CONCENTRATION: 50 ± 2.5 µg/ml
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 06/10/2016
EXPIRY DATE: (mm/dd/yyyy) 06/10/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

MOLECULAR WEIGHT: 516.19
SOLVENT(S): Methanol
ISOTOPIC PURITY: ≥98% ²H₃

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)

Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

See page 2 for further details.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 

B.G. Chittim

Date: 06/16/2016

(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
 519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: d-N-MeFOSA-M; LC/MS Data (TIC and Mass Spectrum)

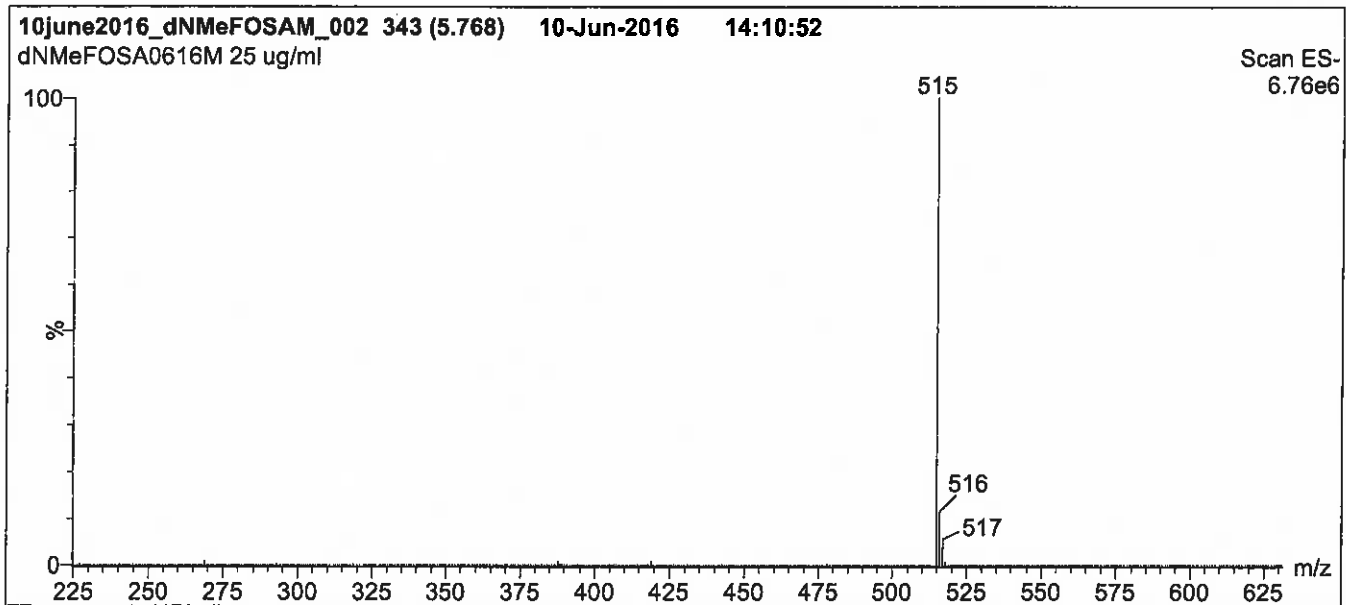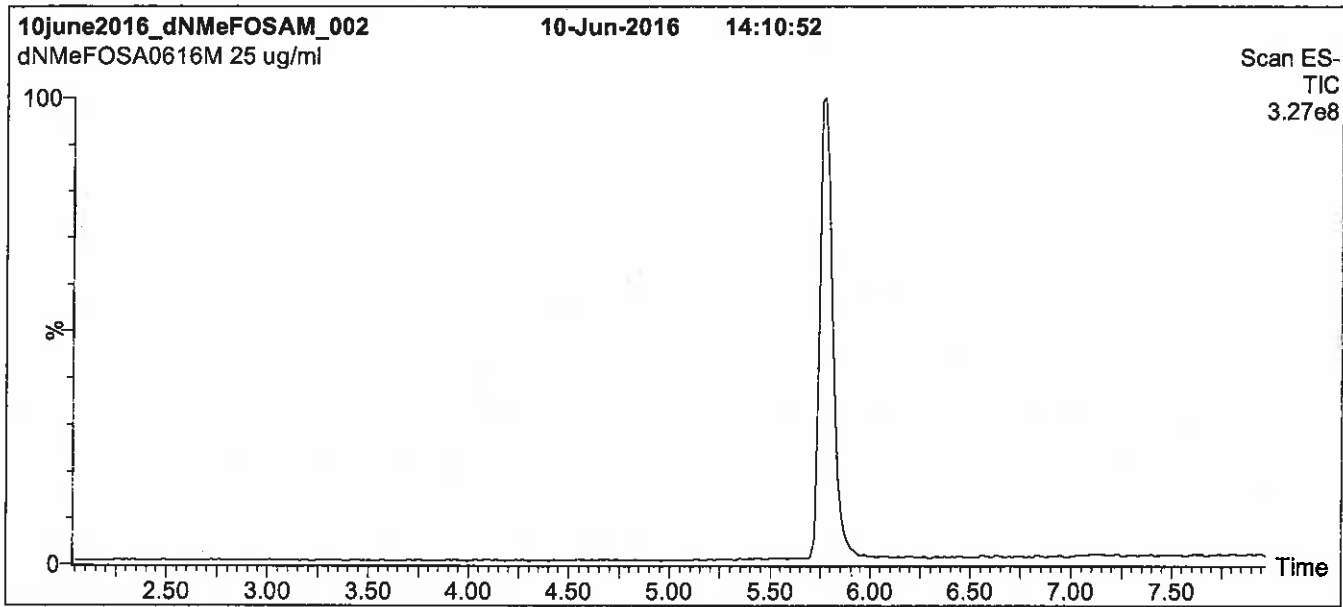

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 40% H₂O / 60% (80:20 MeOH:ACN)
 (both with 10mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.50
 Cone Voltage (V) = 40.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: d-N-MeFOSA-M; LC/MS/MS Data (Selected MRM Transitions)

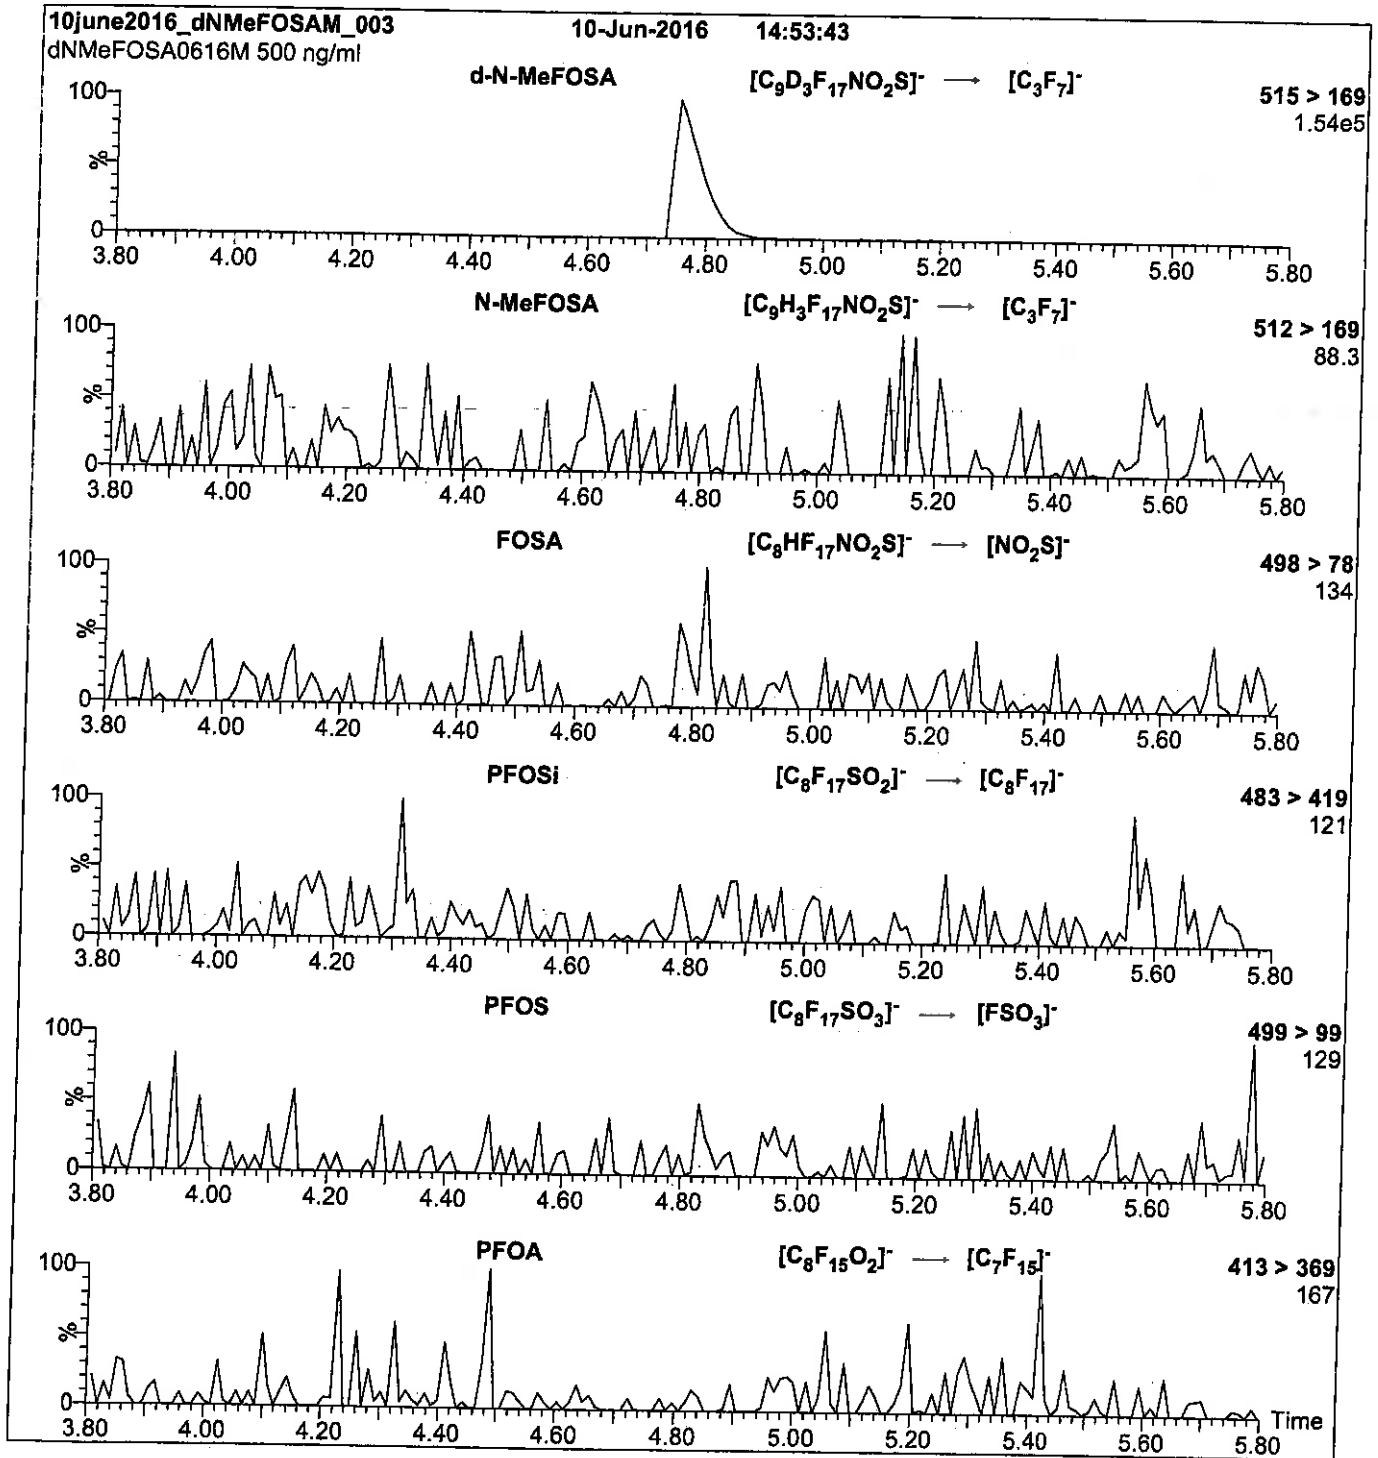

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml d-N-MeFOSA-M)

Mobile phase: isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.39e-3
Collision Energy (eV) = 25

Reagent

LCd3-NMeFOSAA_00001




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: d3-N-MeFOSAA **LOT NUMBER:** d3NMeFOSAA0113
COMPOUND: N-methyl-d3-perfluoro-1-octanesulfonamidoacetic acid

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: C₁₁D₃H₃F₁₇NO₄S
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 574.23
SOLVENT(S): Methanol
 Water (<1%)

CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 01/31/2013
EXPIRY DATE: (mm/dd/yyyy) 01/31/2018
RECOMMENDED STORAGE: Refrigerate ampoule

ISOTOPIC PURITY: ≥98% ²H₃


DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
 Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent the conversion of the acetic acid moiety to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
 B.G. Chittim **Date:** 04/06/2015
 (mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
 519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: d3-N-MeFOSAA; LC/MS Data (TIC and Mass Spectrum)

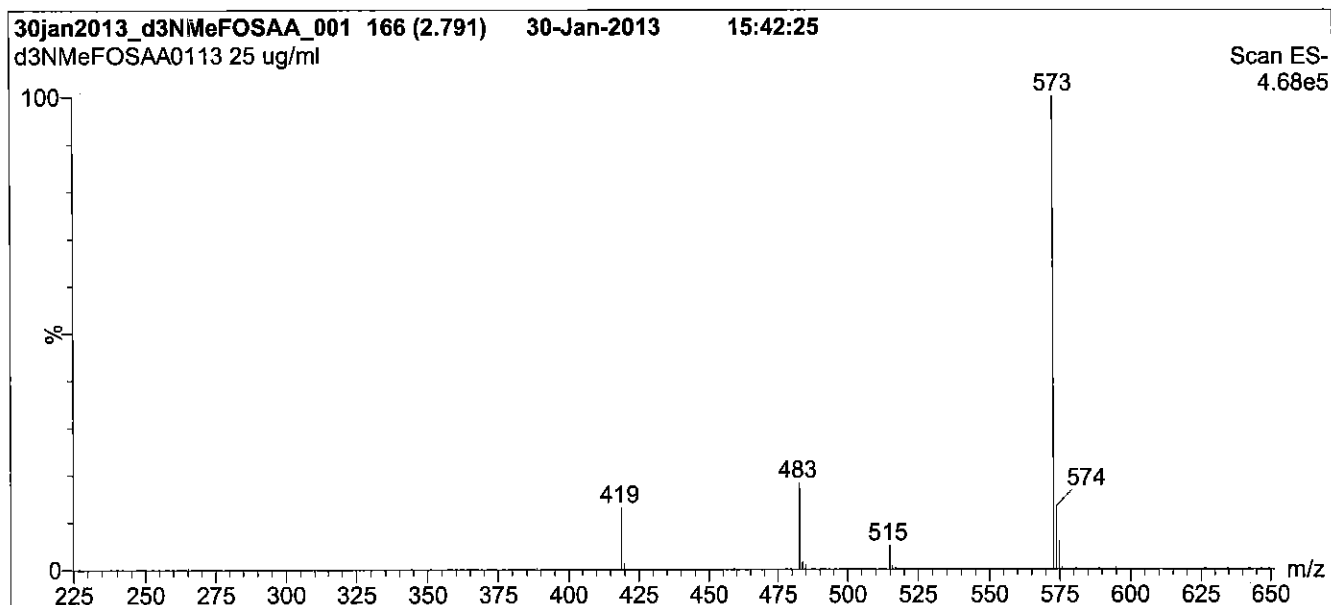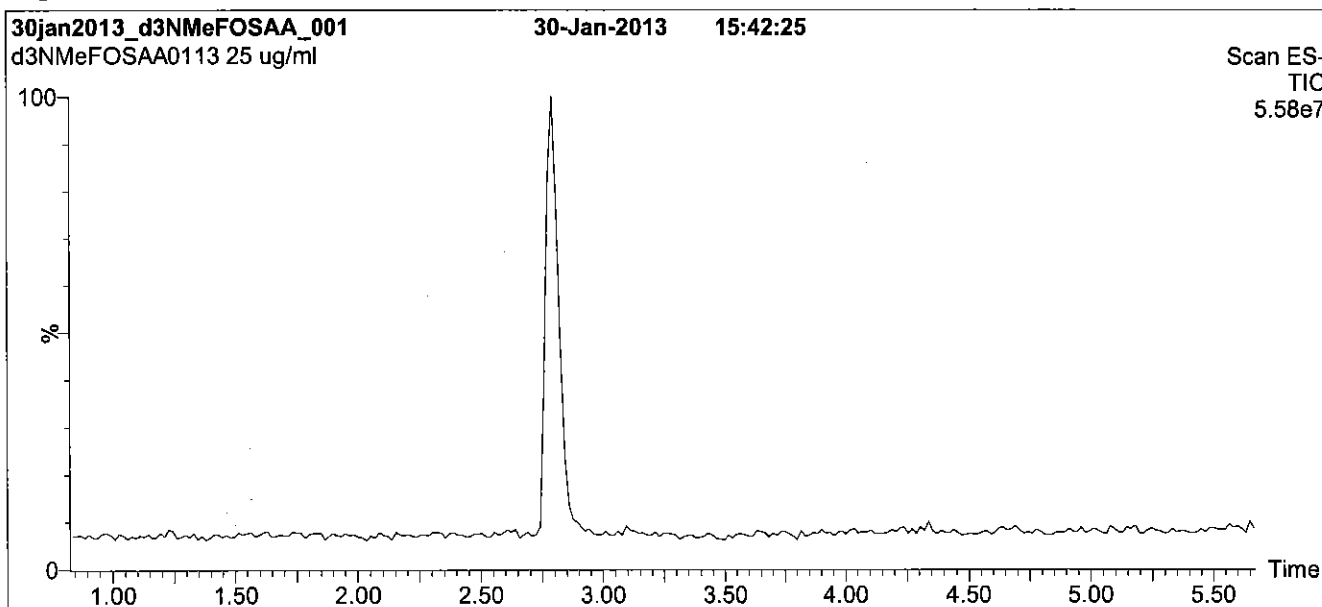

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 65% (80:20 MeOH:ACN) / 35% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 35.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: d3-N-MeFOSAA; LC/MS/MS Data (Selected MRM Transitions)

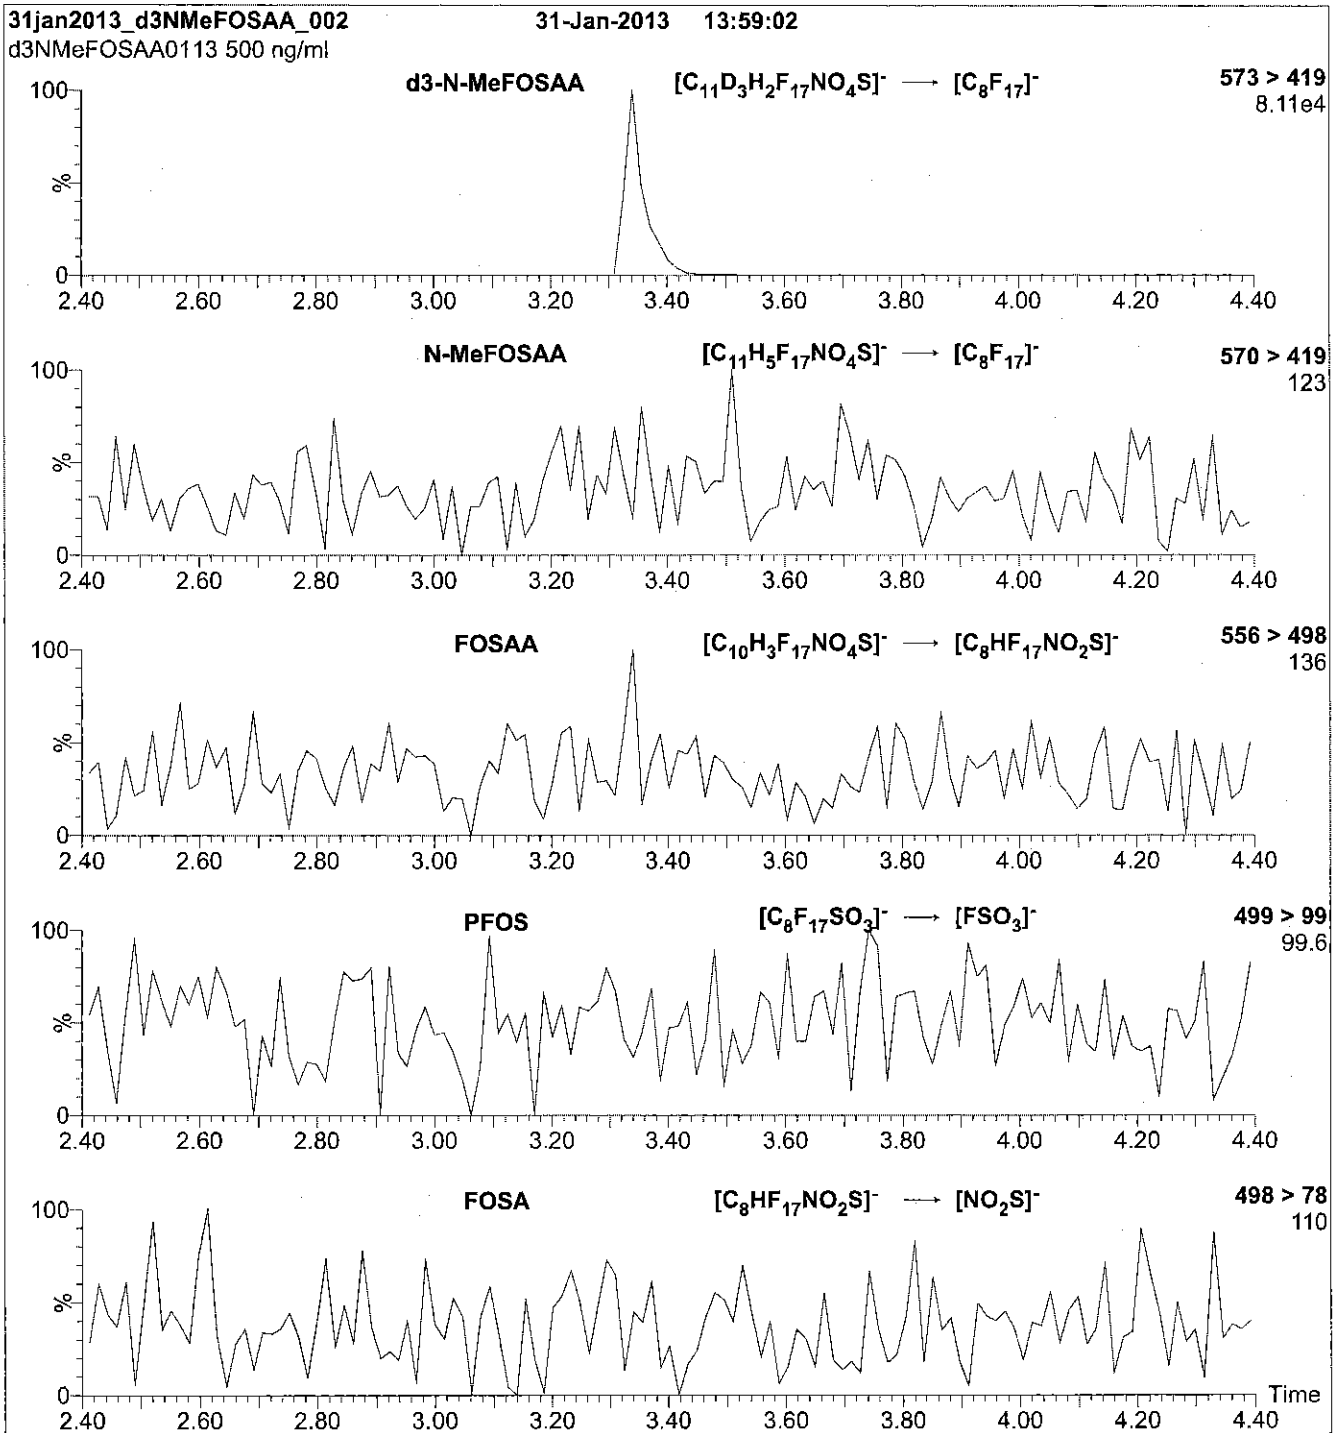

Conditions for Figure 2:

Injection: Direct loop injection
 10 μ l (500 ng/ml d3-N-MeFOSAA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.31e-3
 Collision Energy (eV) = 25

Reagent

LCd3-NMeFOSAA_00002

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: d3-N-MeFOSAA; LC/MS Data (TIC and Mass Spectrum)

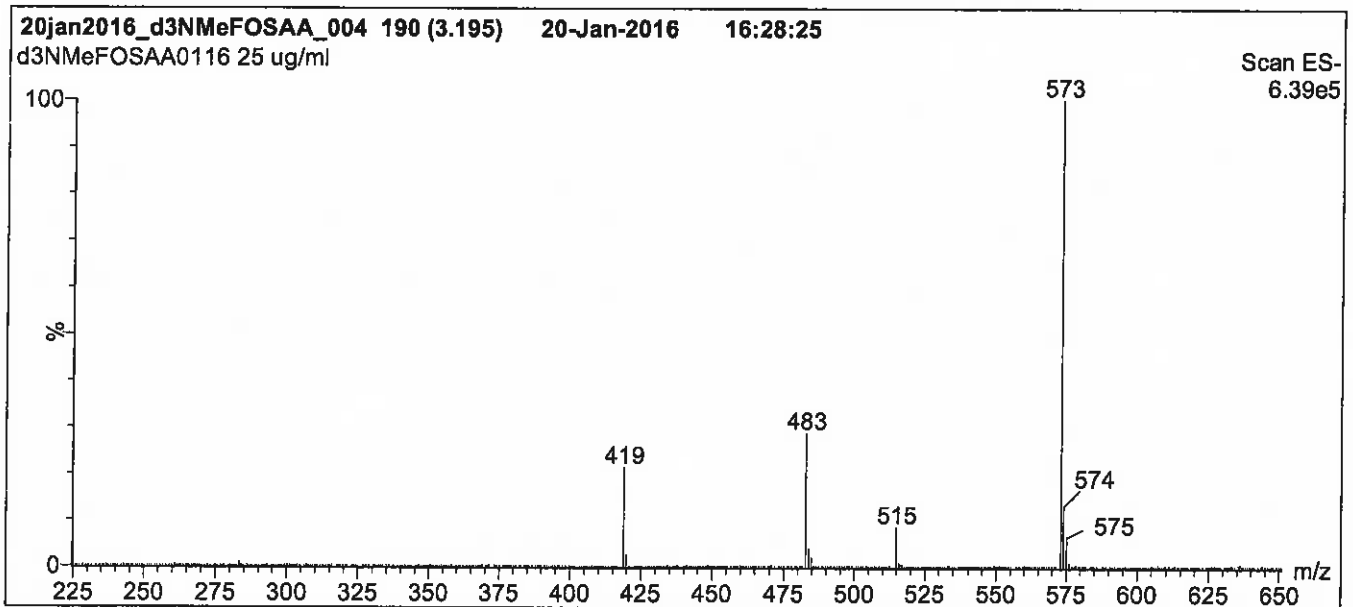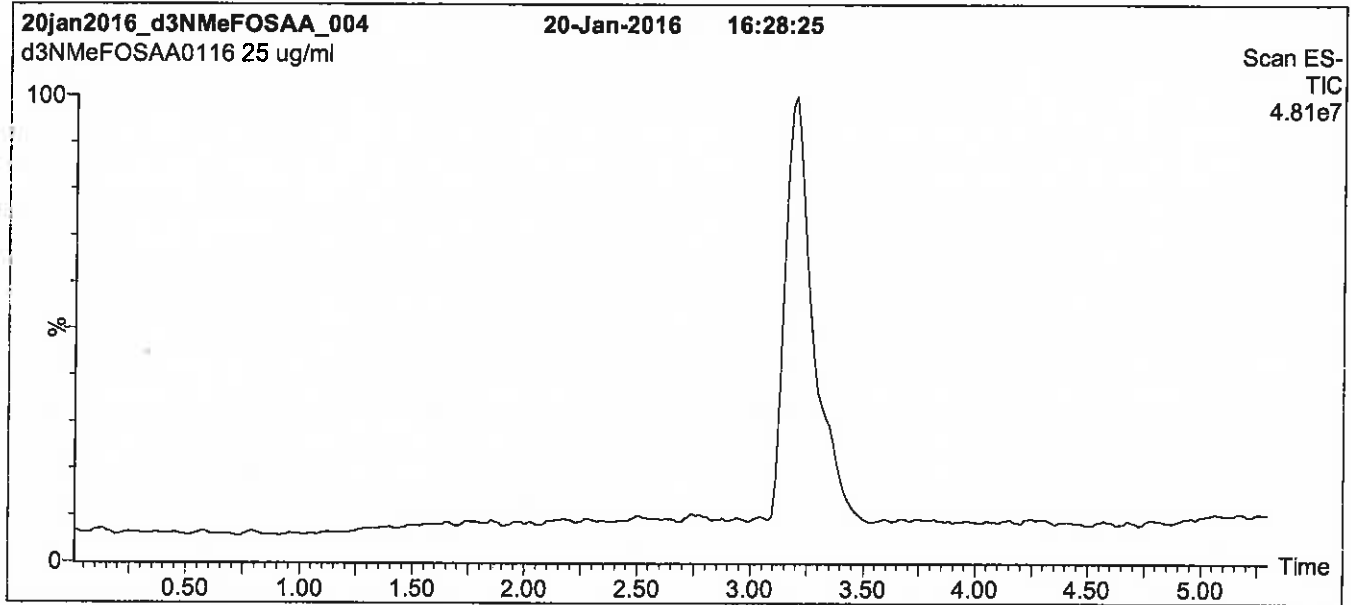

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 60% (80:20 MeOH:ACN) / 40% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 35.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: d3-N-MeFOSAA; LC/MS/MS Data (Selected MRM Transitions)

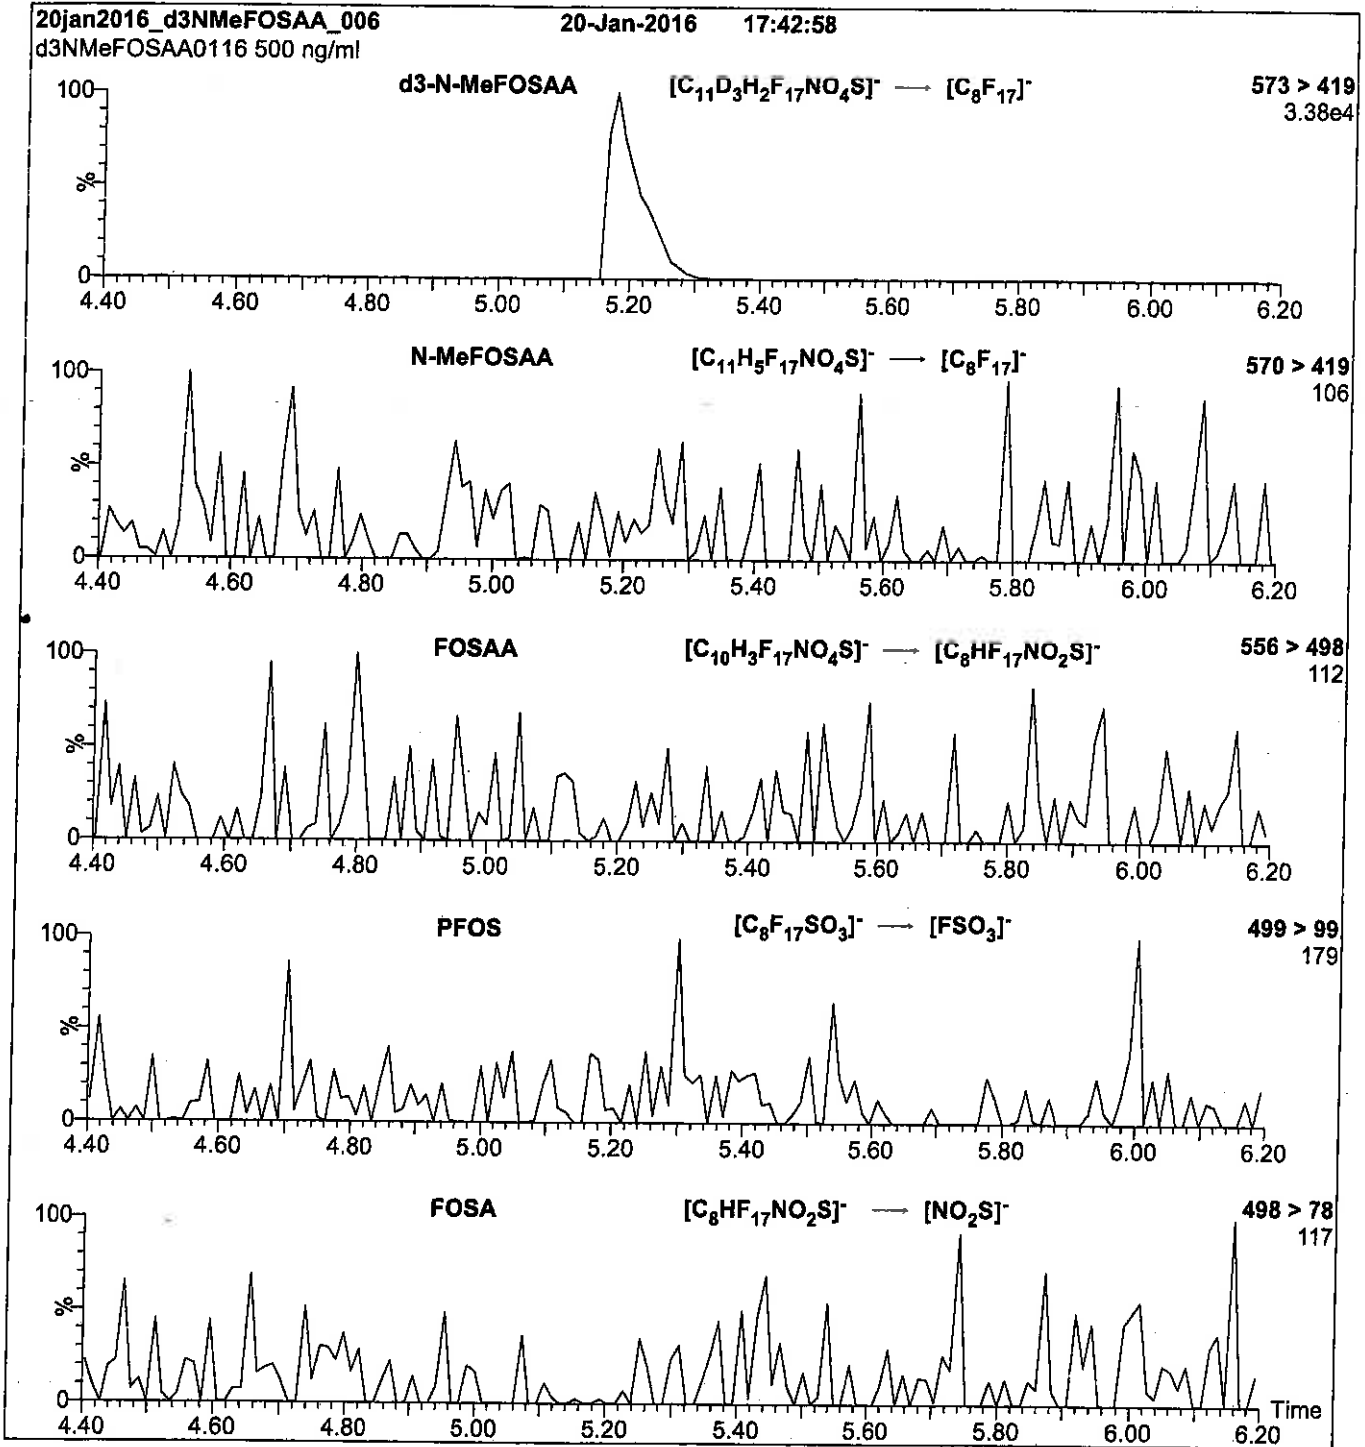

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml d3-N-MeFOSAA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.66e-3
Collision Energy (eV) = 25

Reagent

LCd5-NEtFOSAA_00001




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: d5-N-EtFOSAA **LOT NUMBER:** d5NEtFOSAA0515
COMPOUND: N-ethyl-d5-perfluoro-1-octanesulfonamidoacetic acid

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: C₁₂D₅H₃F₁₇NO₄S
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 590.27
SOLVENT(S): Methanol
 Water (<1%)

CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 05/08/2015
EXPIRY DATE: (mm/dd/yyyy) 05/08/2020
RECOMMENDED STORAGE: Refrigerate ampoule

ISOTOPIC PURITY: ≥98% ²H₅


DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
 Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent the conversion of the acetic acid moiety to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
 B.G. Chittim **Date:** 05/11/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
 519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: d5-N-EtFOSAA; LC/MS Data (TIC and Mass Spectrum)

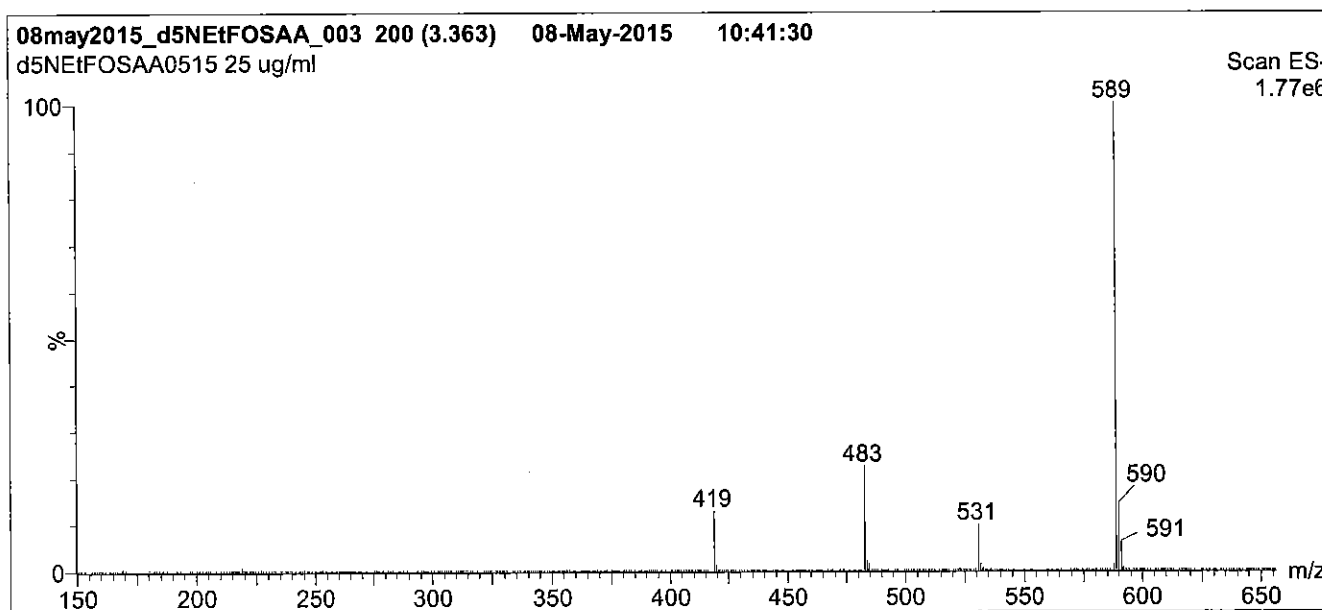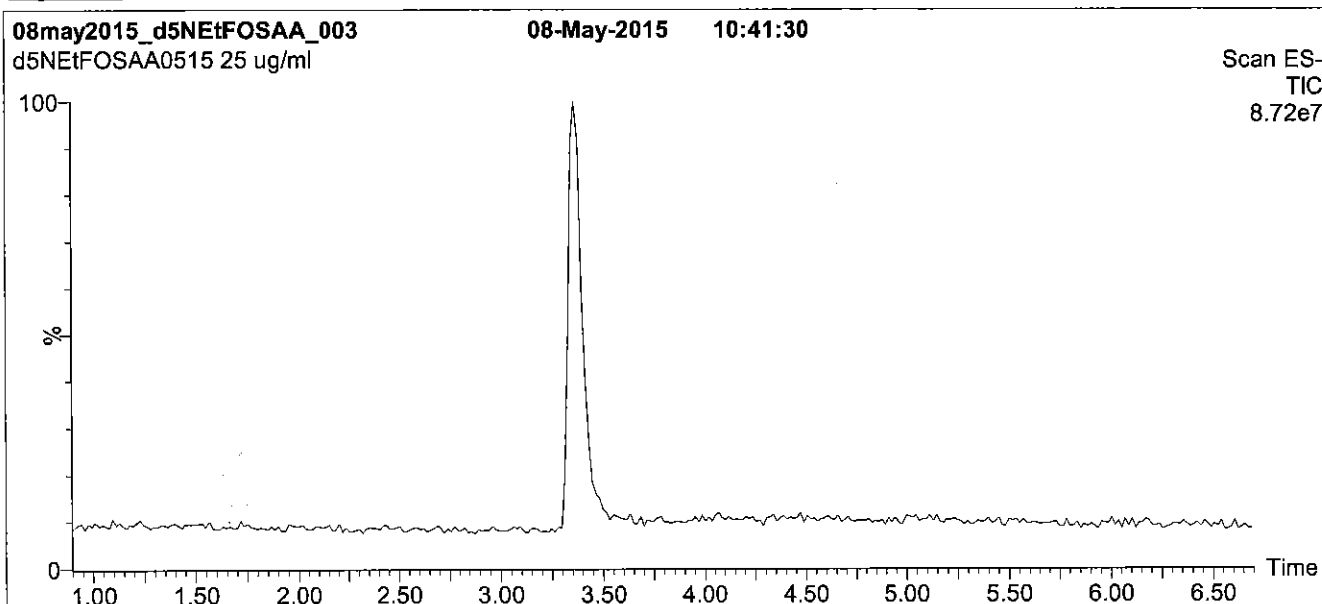

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 65% (80:20 MeOH:ACN) / 35% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 2 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 35.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: d5-N-EtFOSAA; LC/MS/MS Data (Selected MRM Transitions)

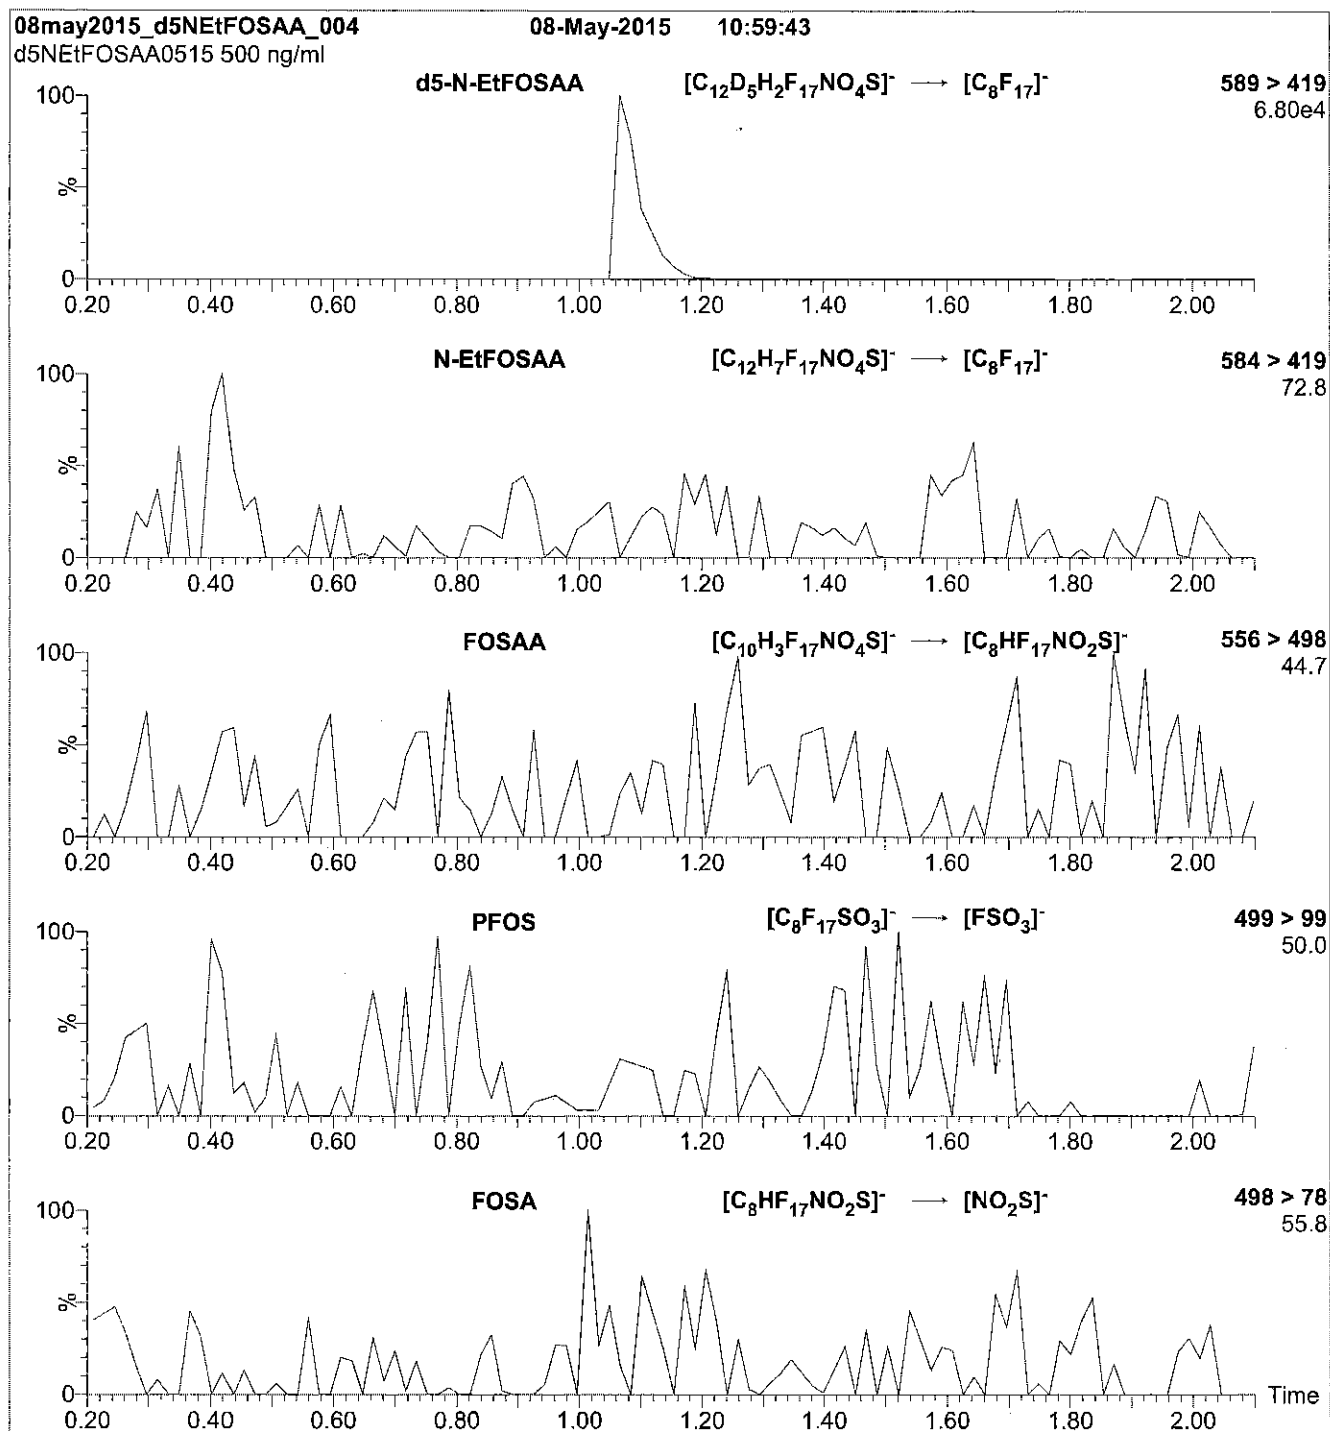

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml d5-N-EtFOSAA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.24e-3
Collision Energy (eV) = 25

Reagent

LCd5-NEtFOSAA_00002

R: 7/6/16 CBW



671603
ID: LCd5-NEtFOSAA_00002
Exp: 12/07/20 Prep: CBW
d5-N-EtFOSAA




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: d5-N-EtFOSAA **LOT NUMBER:** d5NEtFOSAA1115
COMPOUND: N-ethyl-d5-perfluoro-1-octanesulfonamidoacetic acid

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: C₁₂D₅H₃F₁₇NO₄S

CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 590.27

SOLVENT(S): Methanol

Water (<1%)

CHEMICAL PURITY: >98%

ISOTOPIC PURITY: ≥98% ²H₆

LAST TESTED: (mm/dd/yyyy) 12/07/2015

EXPIRY DATE: (mm/dd/yyyy) 12/07/2020

RECOMMENDED STORAGE: Refrigerate ampoule

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)

Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent the conversion of the acetic acid moiety to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim

Date: 12/07/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: d5-N-EtFOSAA; LC/MS Data (TIC and Mass Spectrum)

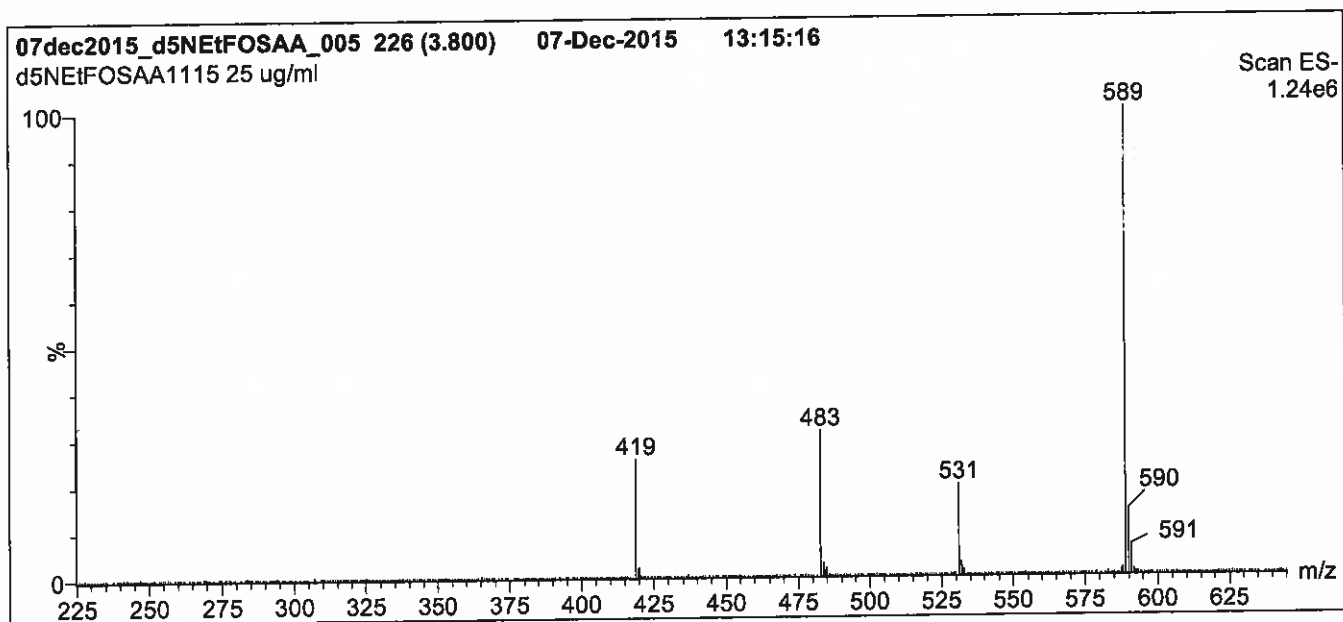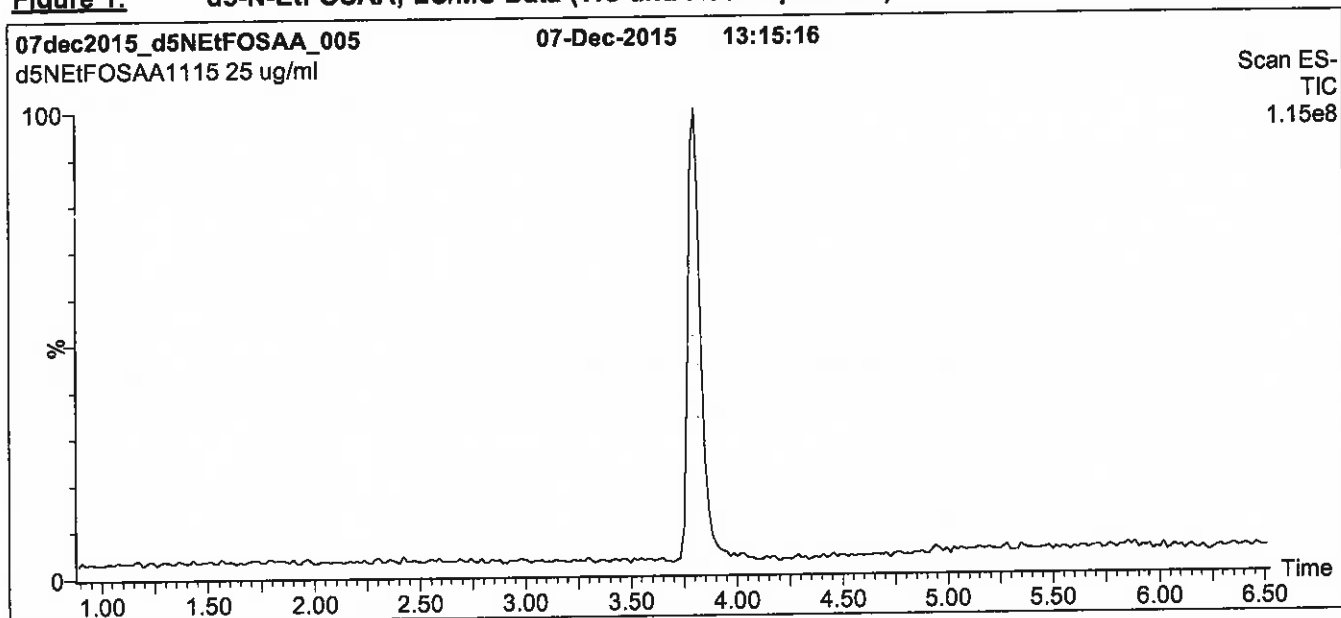

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 65% (80:20 MeOH:ACN) / 35% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 2 min.
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 35.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: d5-N-EtFOSAA; LC/MS/MS Data (Selected MRM Transitions)

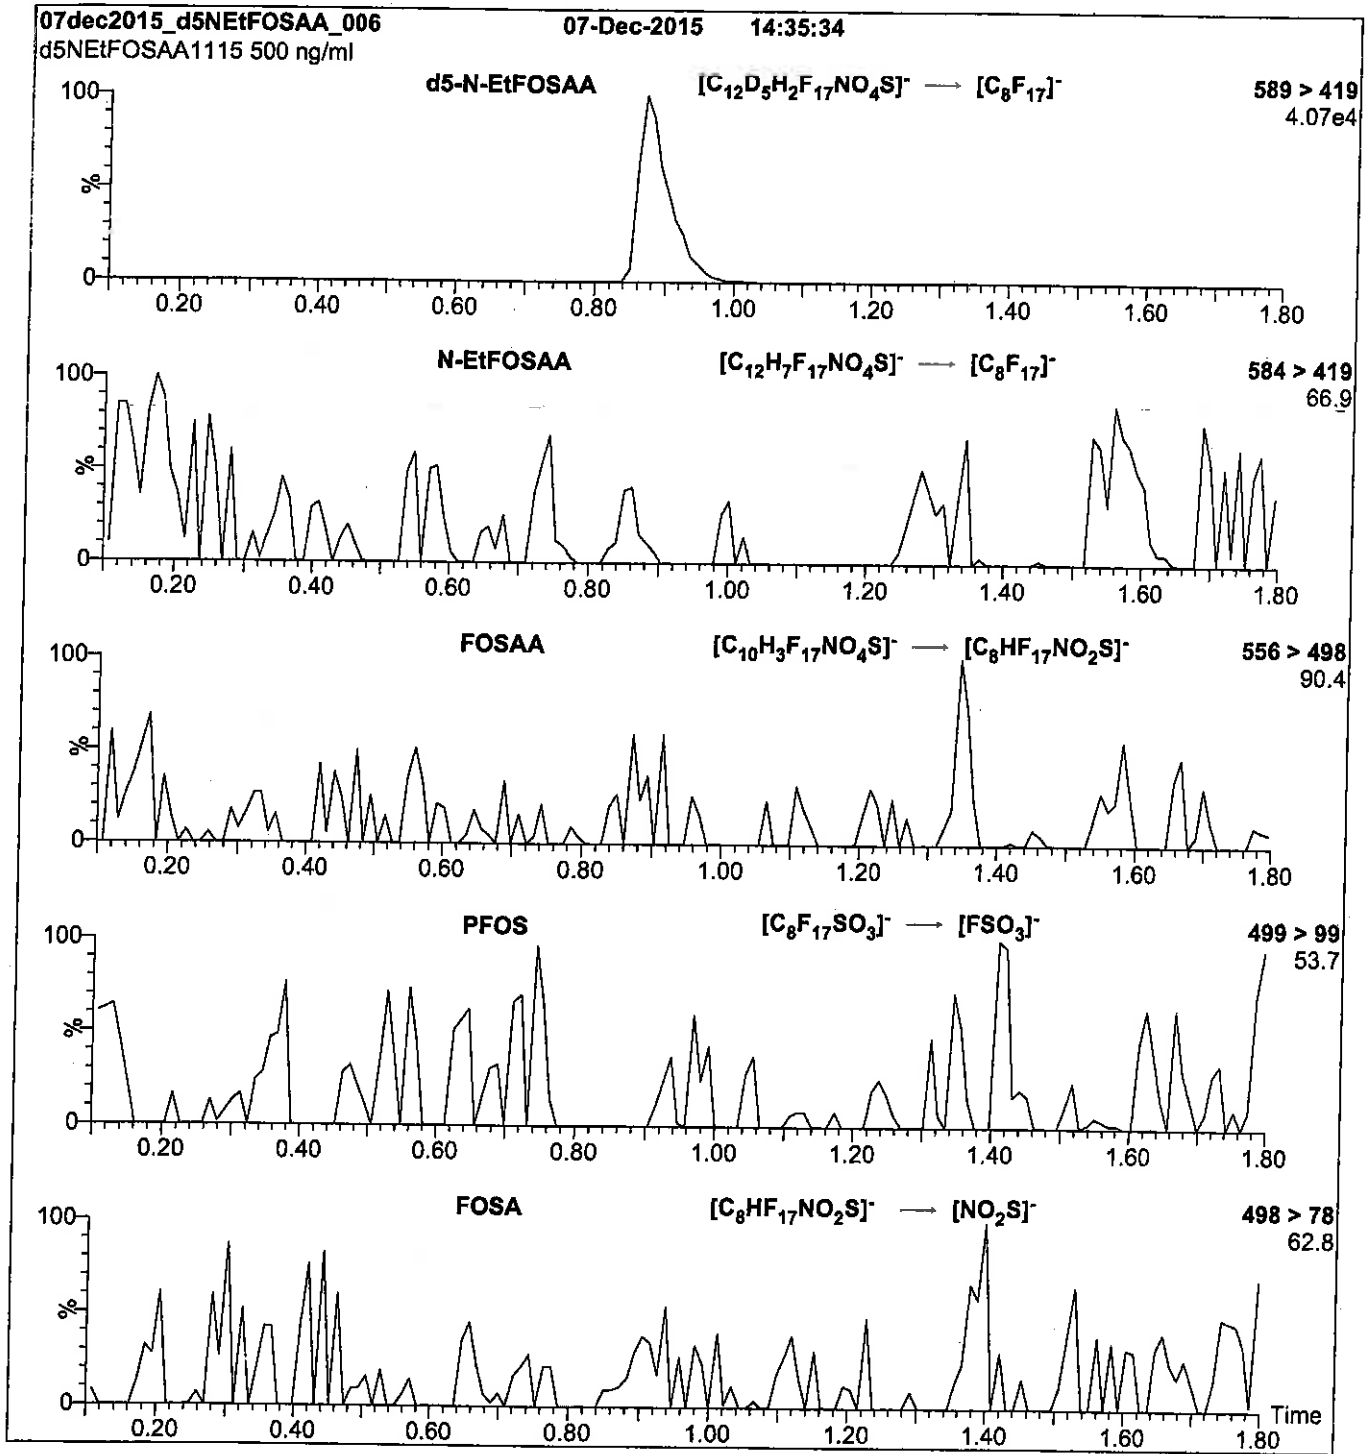

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml d5-N-EtFOSAA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.43e-3
Collision Energy (eV) = 25

Reagent

LCM2-6:FTS_00001

R: 7/16/15 SW
S: 7/20/15 SW




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: M2-6:2FTS **LOT NUMBER:** M262FTS0714
COMPOUND: Sodium 1H,1H,2H,2H-perfluoro-[1,2-¹³C₂]octane sulfonate

STRUCTURE: **CAS #:** Not available

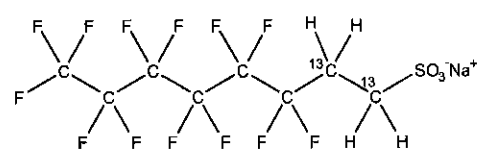

MOLECULAR FORMULA: ¹³C₂¹²C₆H₄F₁₃SO₃Na **MOLECULAR WEIGHT:** 452.13
CONCENTRATION: 50.0 ± 2.5 µg/ml (Na salt) **SOLVENT(S):** Methanol
47.5 ± 2.4 µg/ml (M2-6:2FTS anion)
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥99% ¹³C
LAST TESTED: (mm/dd/yyyy) 07/15/2014 (1,2-¹³C₂)
EXPIRY DATE: (mm/dd/yyyy) 07/15/2017
RECOMMENDED STORAGE: Refrigerate ampoule


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- The native 6:2FTS contains 4.22% of ³⁴S (due to natural isotopic abundance) therefore both native 6:2FTS and M2-6:2FTS will produce signals in the m/z 429 to m/z 409 channel during SRM analysis. We recommend using the m/z 429 to m/z 81 transition to monitor for M2-6:2FTS during quantitative analysis as it will be free of any native contribution (see Figure 2).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 03/27/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: M2-6:2FTS; LC/MS Data (TIC and Mass Spectrum)

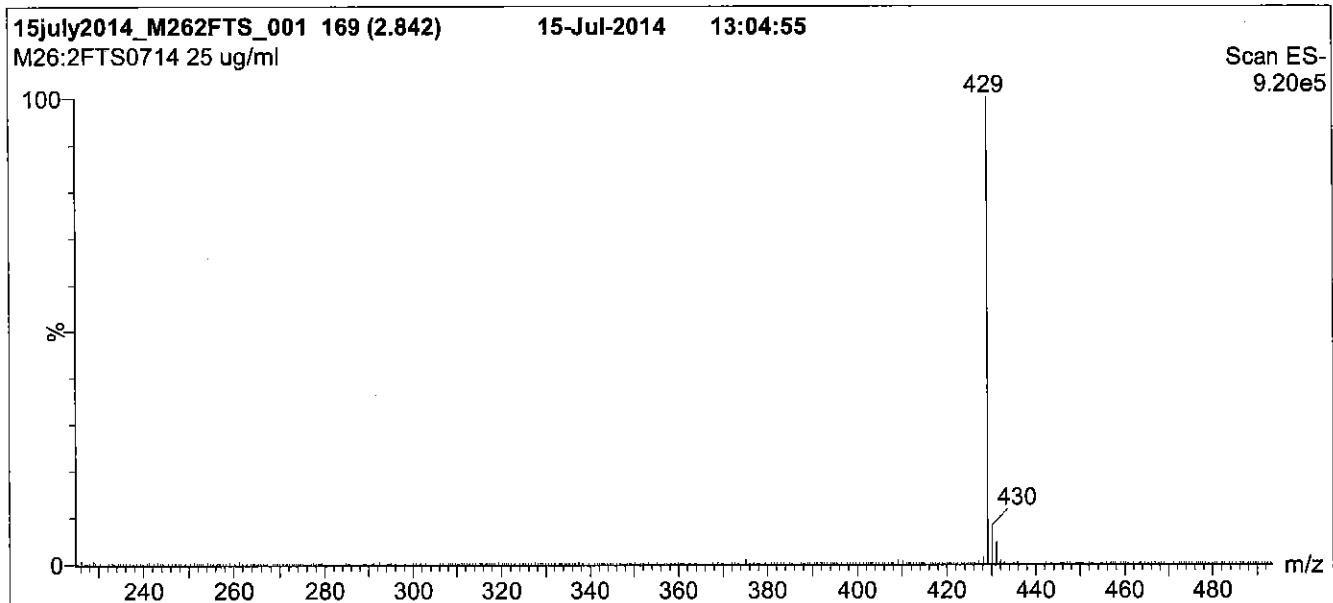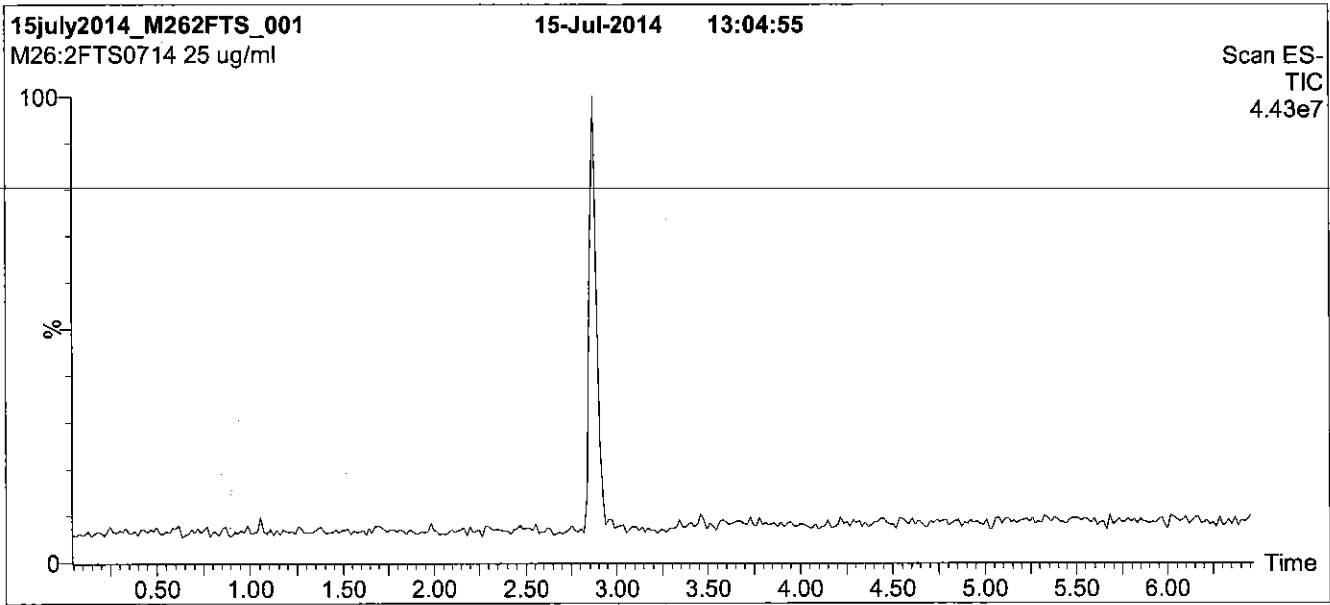

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 55% (80:20 MeOH:ACN) / 45% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min
and hold for 2 min before returning
to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 950 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 30.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: M2-6:2FTS; LC/MS/MS Data (Selected MRM Transitions)

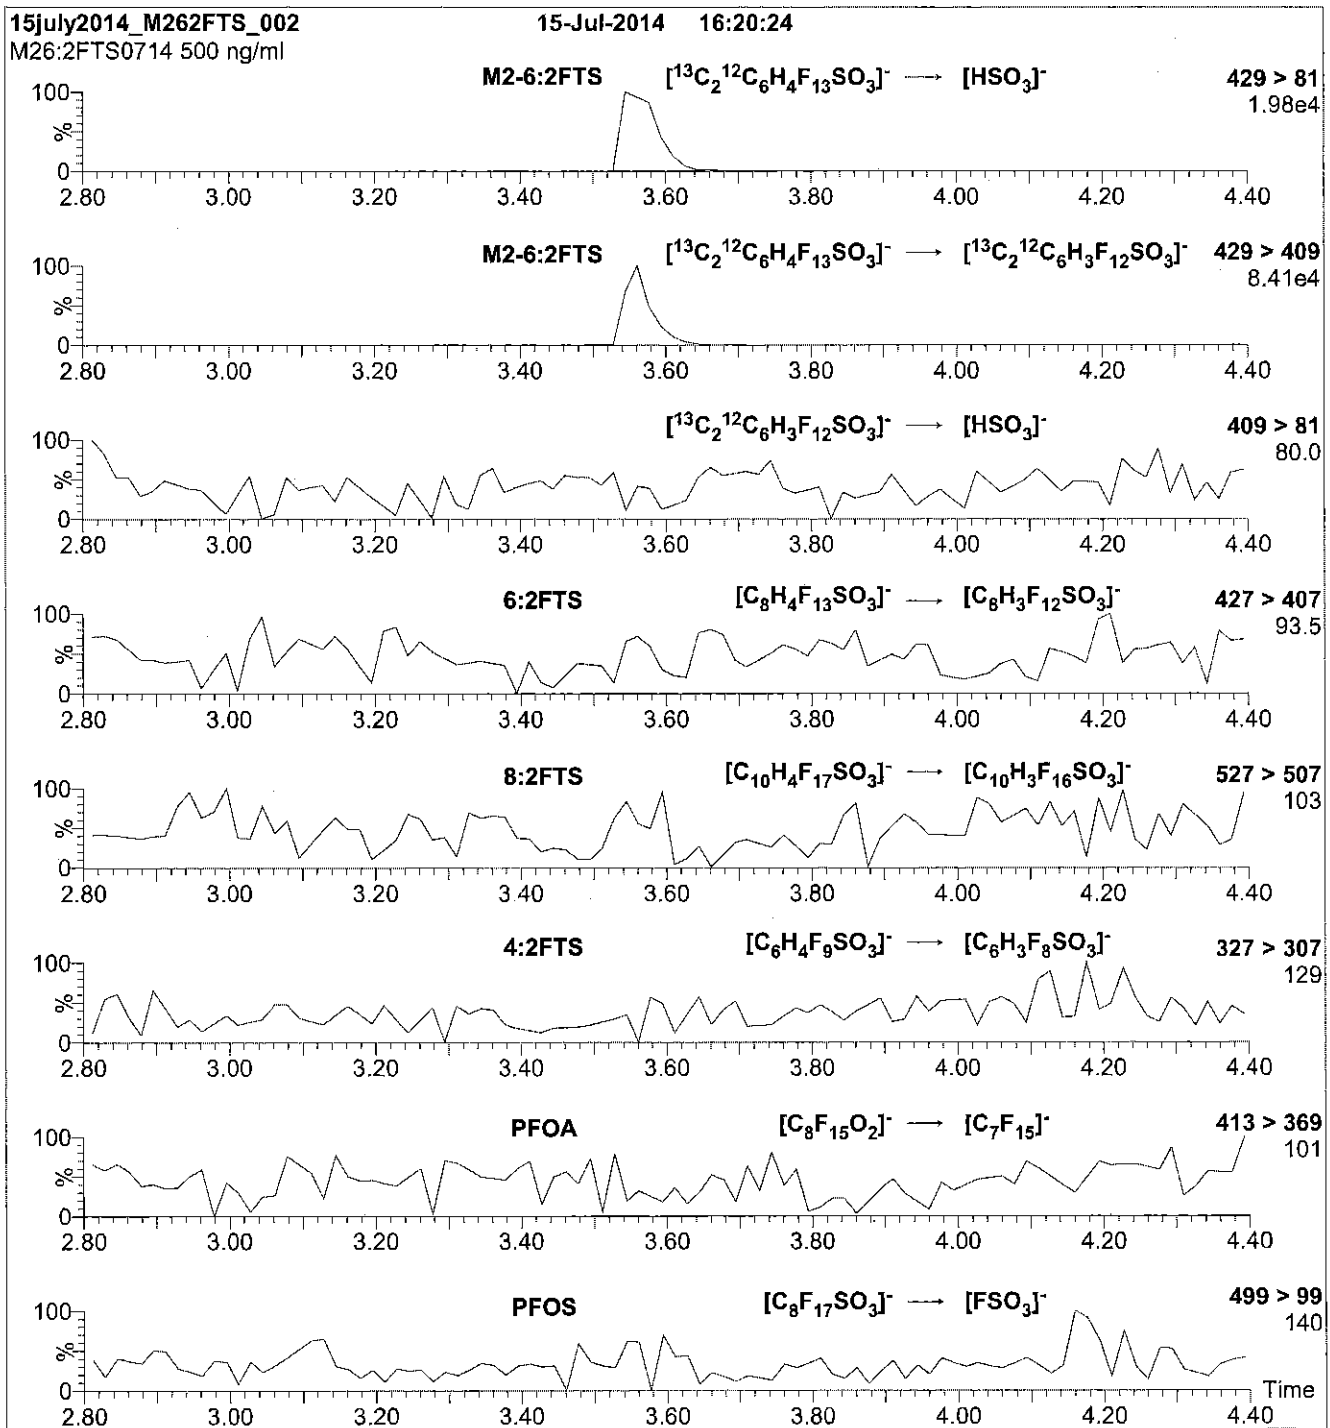

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml M2-6:2FTS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.43e-3
Collision Energy (eV) = 25

Reagent

LCM2-6: FTS_00002

R: 7/6/16 CSW

671575
ID: LCM2-6:F2S_00002
Exp: 01/08/21 Prod: CSW
M2-6:2F2S




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: M2-6:2F2S **LOT NUMBER:** M262F2S0116
COMPOUND: Sodium 1H,1H,2H,2H-perfluoro-[1,2-¹³C₂]octane sulfonate

STRUCTURE: **CAS #:** Not available

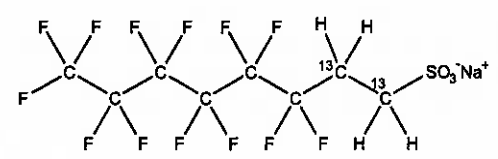

MOLECULAR FORMULA: ¹³C₂¹²C₆H₄F₁₃SO₃Na **MOLECULAR WEIGHT:** 452.13
CONCENTRATION: 50.0 ± 2.5 µg/ml (Na salt) **SOLVENT(S):** Methanol
47.5 ± 2.4 µg/ml (M2-6:2F2S anion)
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥99% ¹³C
LAST TESTED: (mm/dd/yyyy) 01/08/2016 (1,2-¹³C₂)
EXPIRY DATE: (mm/dd/yyyy) 01/08/2021
RECOMMENDED STORAGE: Refrigerate ampoule


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- The native 6:2F2S contains 4.22% of ³⁴S (due to natural isotopic abundance) therefore both native 6:2F2S and M2-6:2F2S will produce signals in the m/z 429 to m/z 409 channel during SRM analysis. We recommend using the m/z 429 to m/z 81 transition to monitor for M2-6:2F2S during quantitative analysis as it will be free of any native contribution (see Figure 2).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 01/11/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to International interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



****For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com****

Figure 1: M2-6:2FTS; LC/MS Data (TIC and Mass Spectrum)

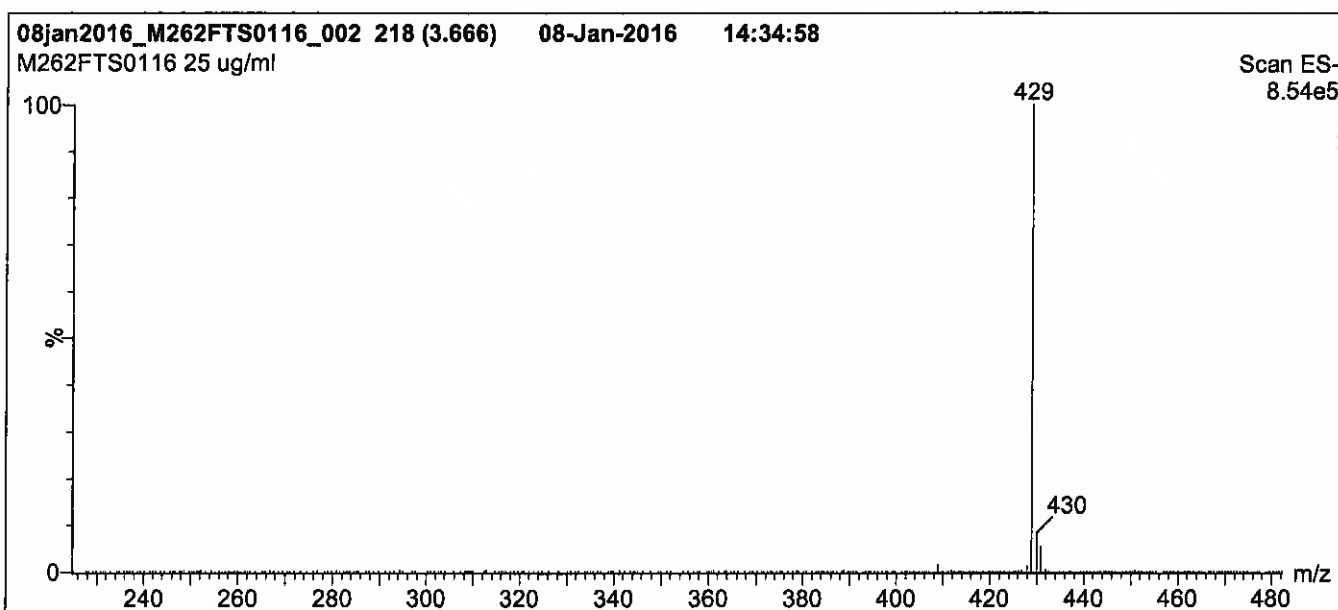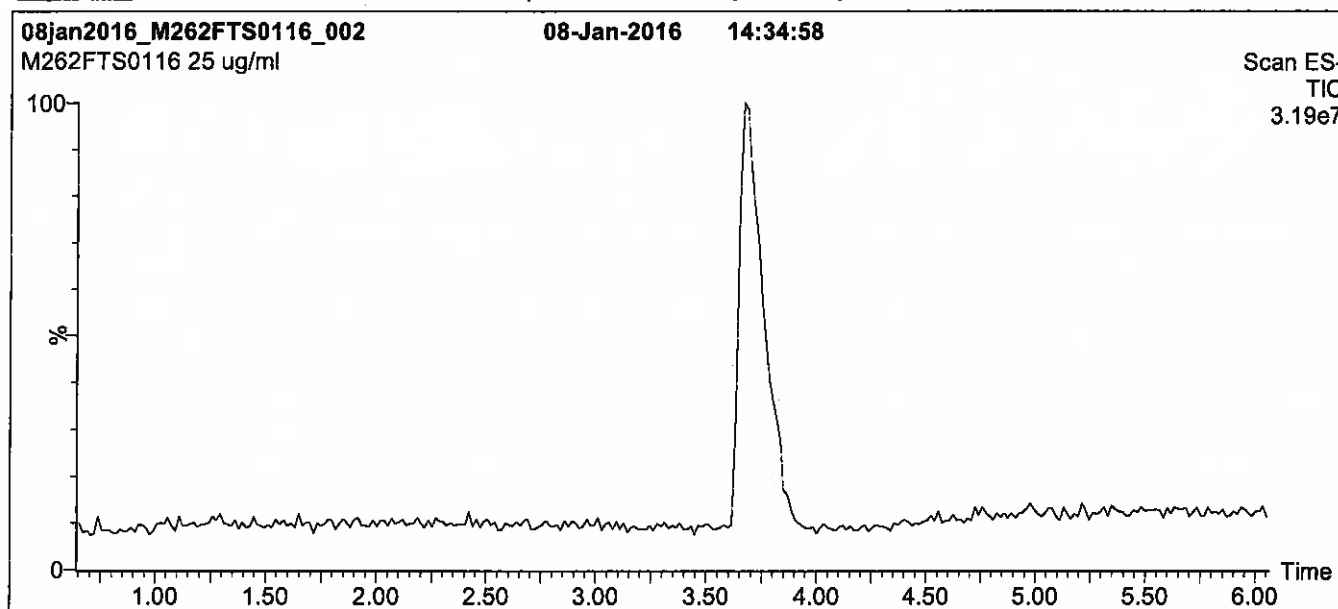

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min
and hold for 2 min before returning
to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 30.00
Cone Gas Flow (l/hr) = 100
Desolvation Gas Flow (l/hr) = 750

Figure 2: M2-6:2FTS; LC/MS/MS Data (Selected MRM Transitions)

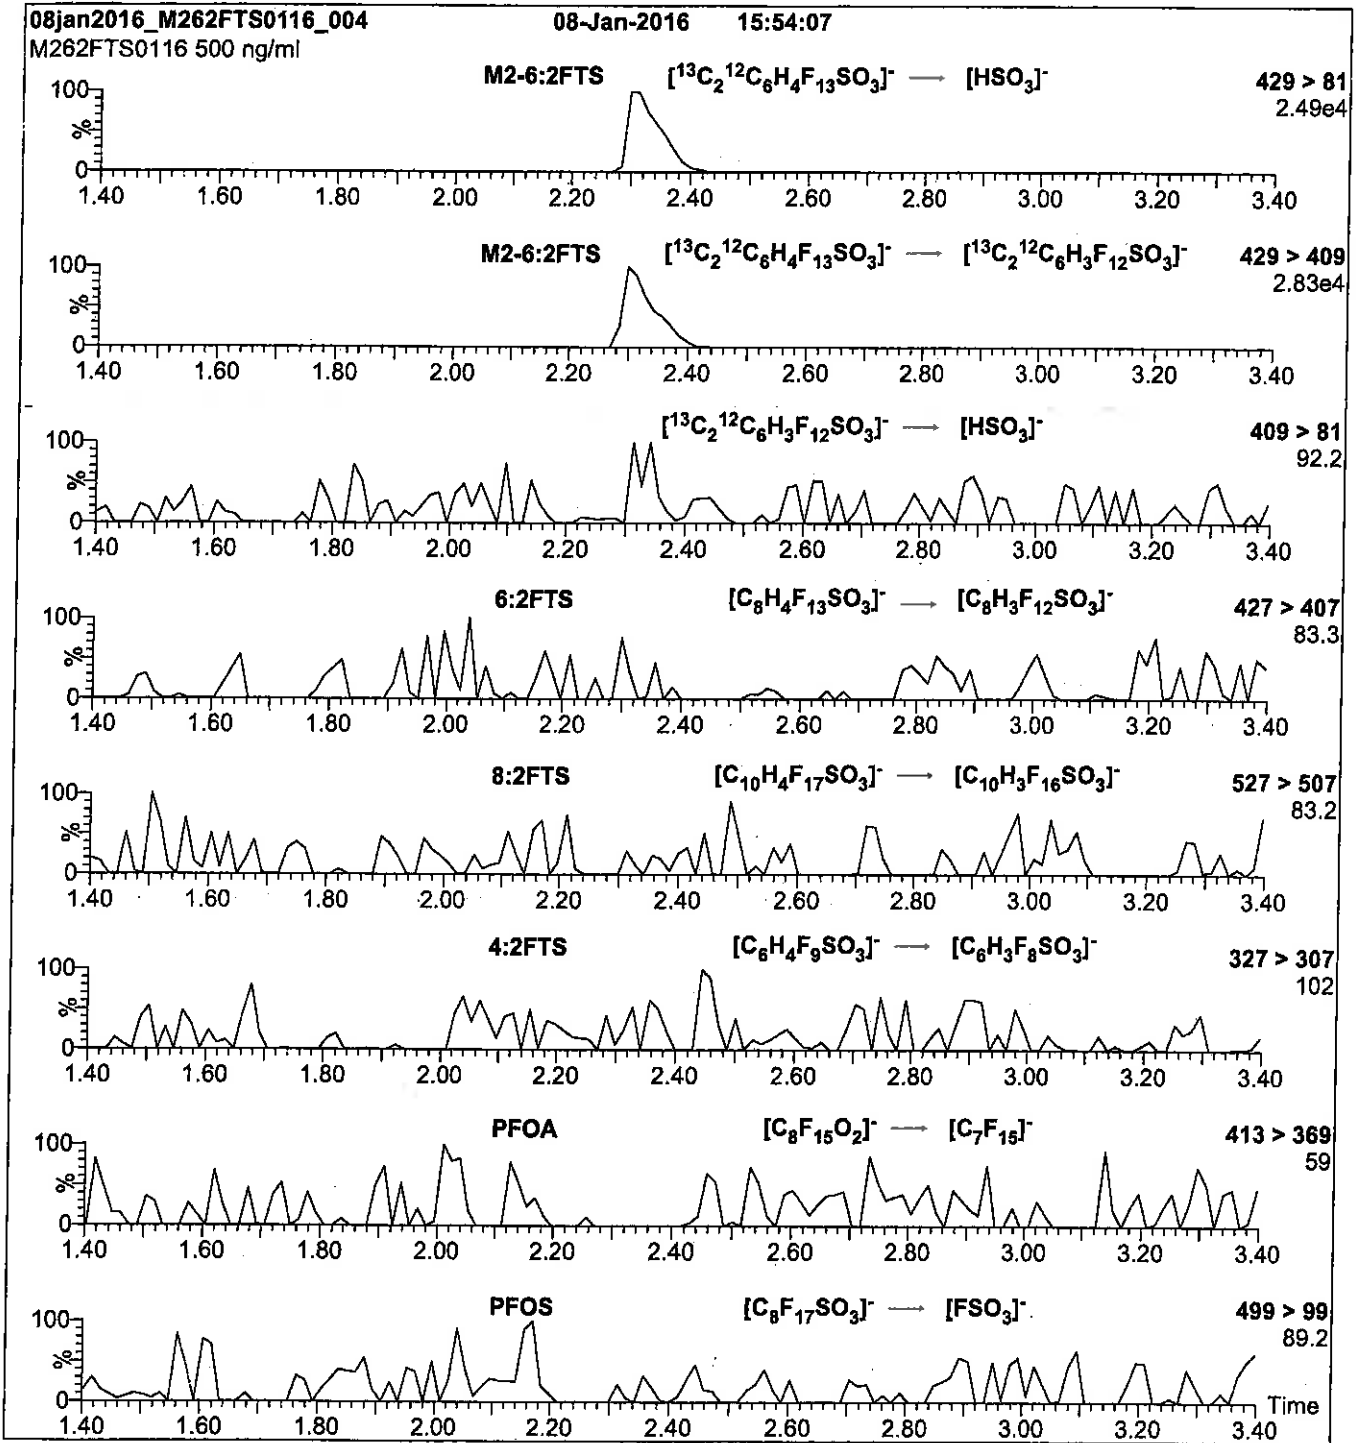

Conditions for Figure 2:

Injection: Direct loop injection
10 µl (500 ng/ml M2-6:2FTS)

MS Parameters

Collision Gas (mbar) = 3.28e-3
Collision Energy (eV) = 25

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 µl/min

Reagent

LCM2-8:2FTS_00001

r: 7/16/15 ✓
s: 7/22/15 STV




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: M2-8:2FTS **LOT NUMBER:** M282FTS0414
COMPOUND: Sodium 1H,1H,2H,2H-perfluoro-[1,2-¹³C₂]decane sulfonate

STRUCTURE: **CAS #:** Not available

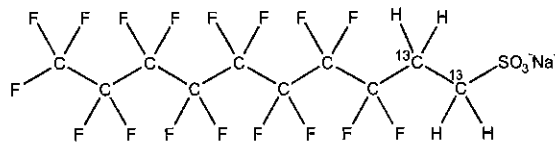

MOLECULAR FORMULA: ¹³C₂¹²C₈H₄F₁₇SO₃Na **MOLECULAR WEIGHT:** 552.15
CONCENTRATION: 50.0 ± 2.5 µg/ml (Na salt) **SOLVENT(S):** Methanol
47.9 ± 2.4 µg/ml (M2-8:2FTS anion)
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥99% ¹³C
LAST TESTED: (mm/dd/yyyy) 04/13/2014 (1,2-¹³C₂)
EXPIRY DATE: (mm/dd/yyyy) 04/13/2017
RECOMMENDED STORAGE: Refrigerate ampoule


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- The native 8:2FTS contains 4.22% of ³⁴S (due to natural isotopic abundance) therefore both native 8:2FTS and M2-8:2FTS will produce signals in the m/z 529 to m/z 509 channel during SRM analysis. We recommend using the m/z 529 to m/z 81 transition to monitor for M2-8:2FTS during quantitative analysis as it will be free of any native contribution (see Figure 2).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 03/27/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: M2-8:2FTS; LC/MS Data (TIC and Mass Spectrum)

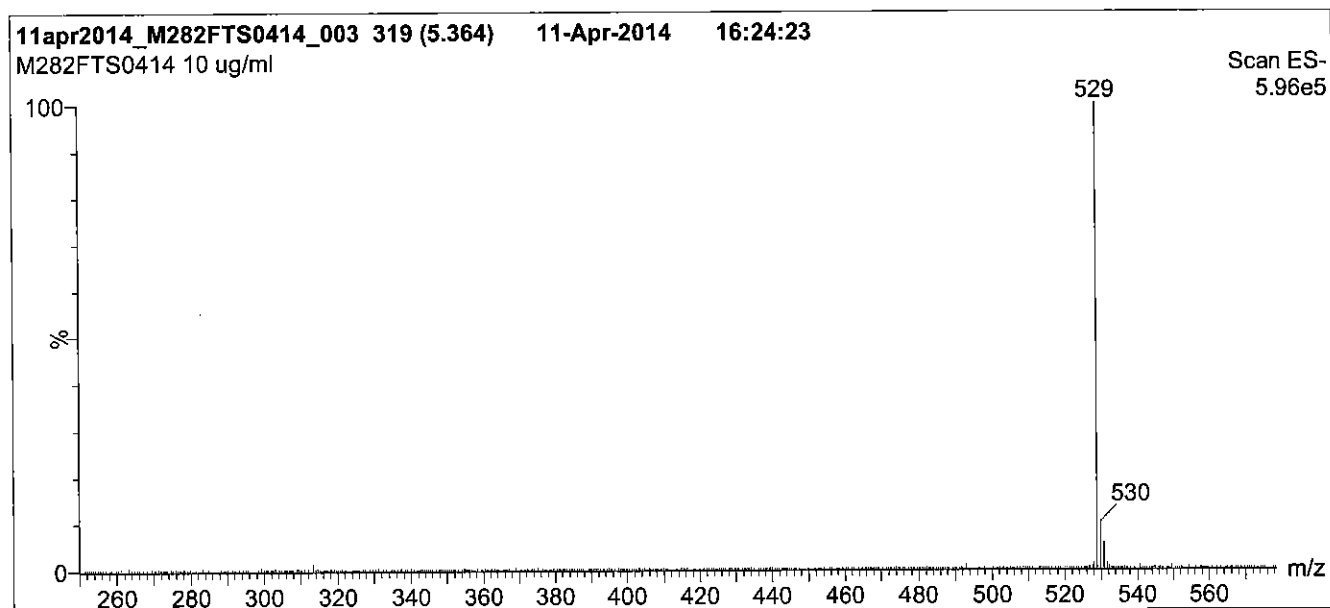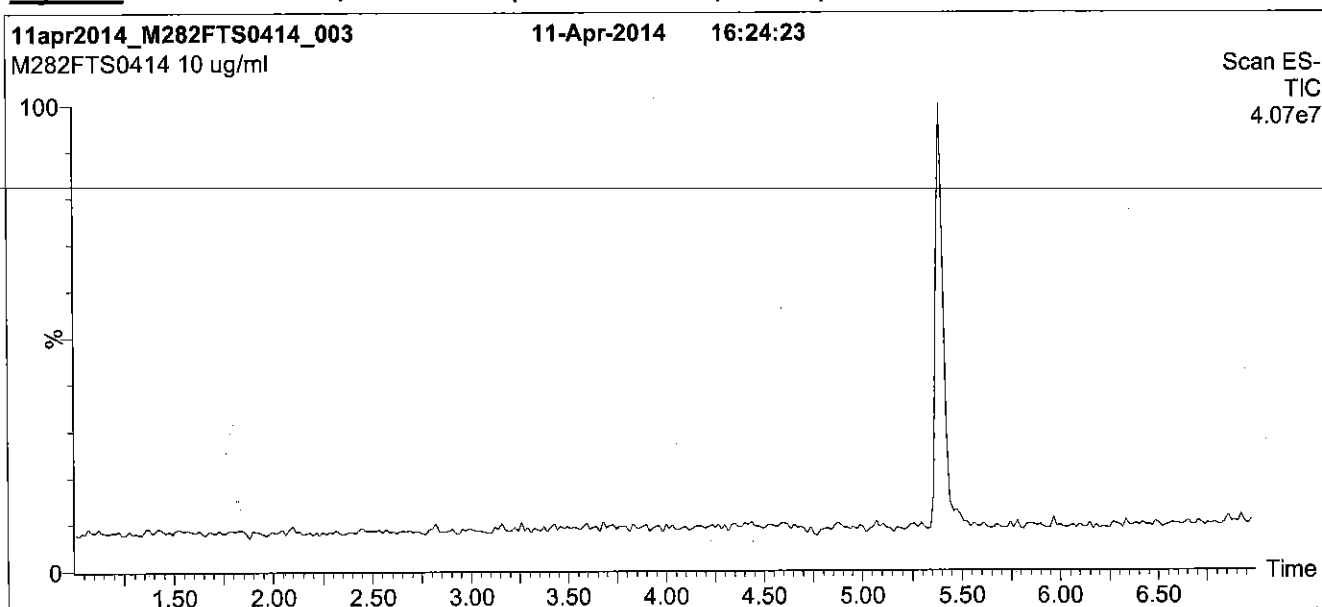

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min
and hold for 2 min before returning
to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (250 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 30.00
Cone Gas Flow (l/hr) = 100
Desolvation Gas Flow (l/hr) = 750

Figure 2: M2-8:2FTS; LC/MS/MS Data (Selected MRM Transitions)

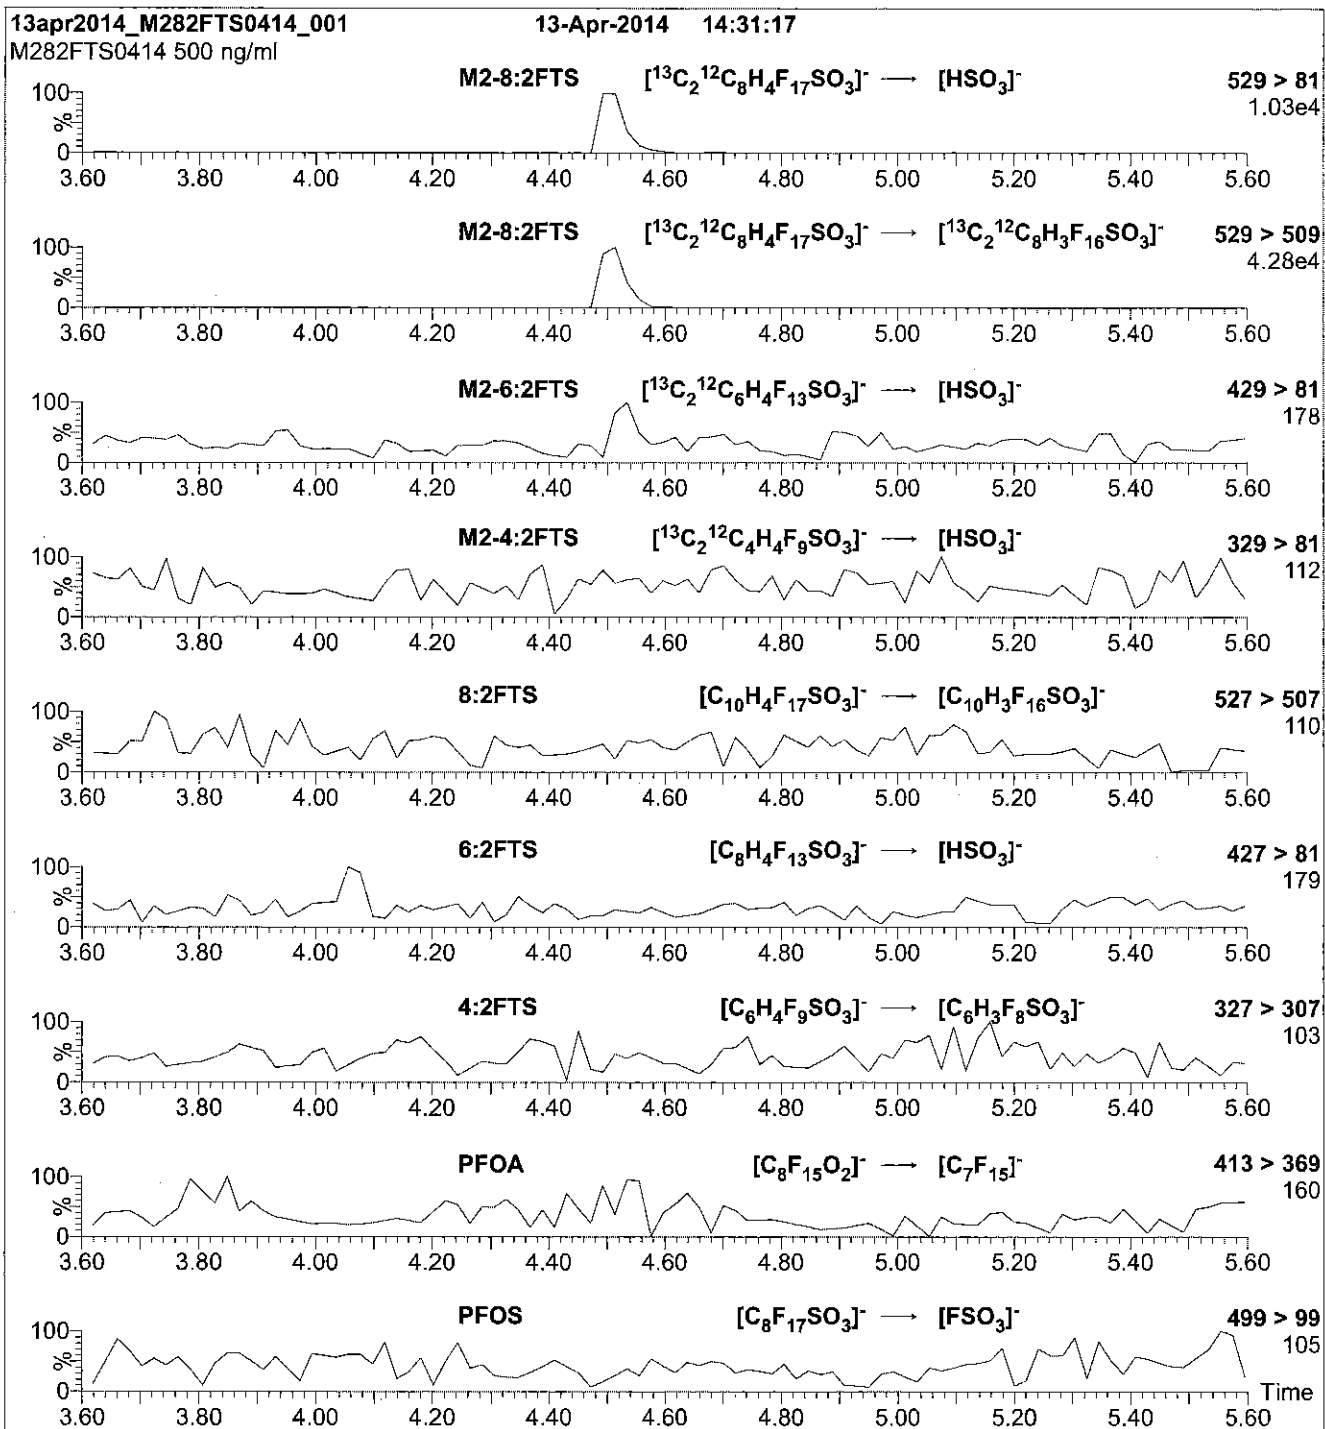

Conditions for Figure 2:

Injection: Direct loop injection
 10 µl (500 ng/ml M2-8:2FTS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)

Flow: 300 µl/min

MS Parameters

Collision Gas (mbar) = 3.24e-3
 Collision Energy (eV) = 25

Reagent

LCM2-8:2FTS_00002

R: 7/6/16 CBW



671602
ID: LCM2-8:2FTS_00002
Exp: 01/08/21 Prod: CBW
M2-8:2FTS




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: M2-8:2FTS **LOT NUMBER:** M282FTS0116
COMPOUND: Sodium 1H,1H,2H,2H-perfluoro-[1,2-¹³C₂]decane sulfonate

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: ¹³C₂¹²C₈H₄F₁₇SO₃Na **MOLECULAR WEIGHT:** 552.15
CONCENTRATION: 50.0 ± 2.5 µg/ml (Na salt) **SOLVENT(S):** Methanol
47.9 ± 2.4 µg/ml (M2-8:2FTS anion)
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥99% ¹³C
LAST TESTED: (mm/dd/yyyy) 01/08/2016 (1,2-¹³C₂)
EXPIRY DATE: (mm/dd/yyyy) 01/08/2021
RECOMMENDED STORAGE: Refrigerate ampoule

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- The native 8:2FTS contains 4.22% of ³⁴S (due to natural isotopic abundance) therefore both native 8:2FTS and M2-8:2FTS will produce signals in the m/z 529 to m/z 509 channel during SRM analysis. We recommend using the m/z 529 to m/z 81 transition to monitor for M2-8:2FTS during quantitative analysis as it will be free of any native contribution (see Figure 2).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 01/18/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: M2-8:2FTS; LC/MS Data (TIC and Mass Spectrum)

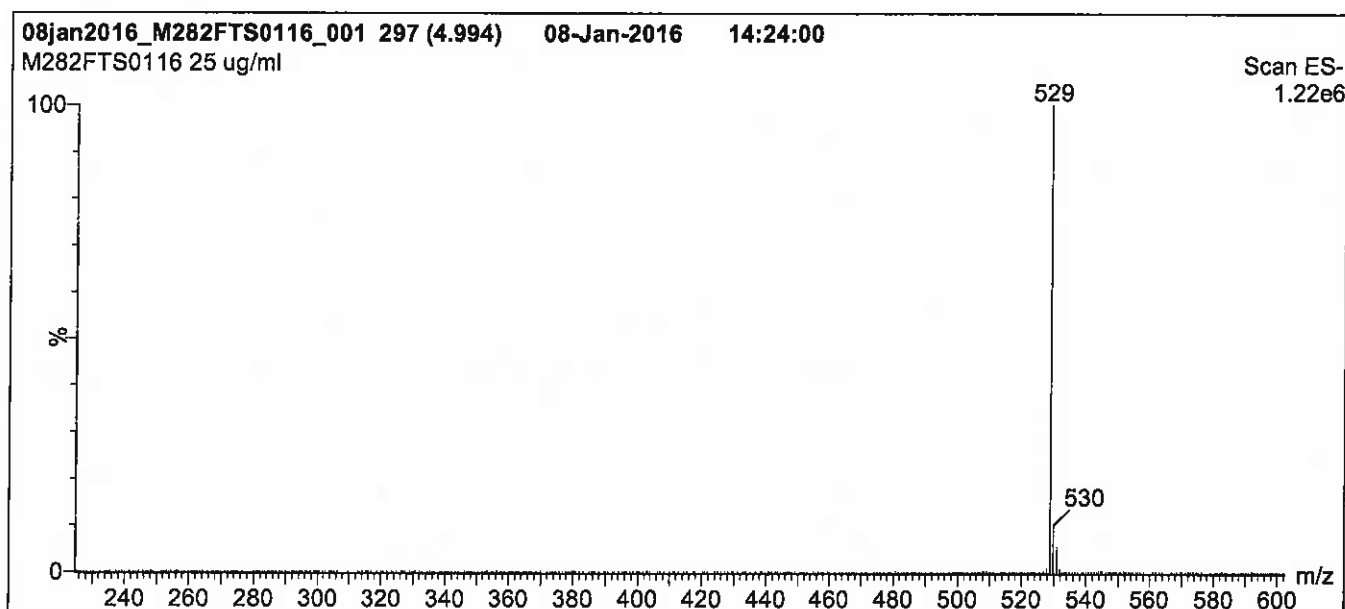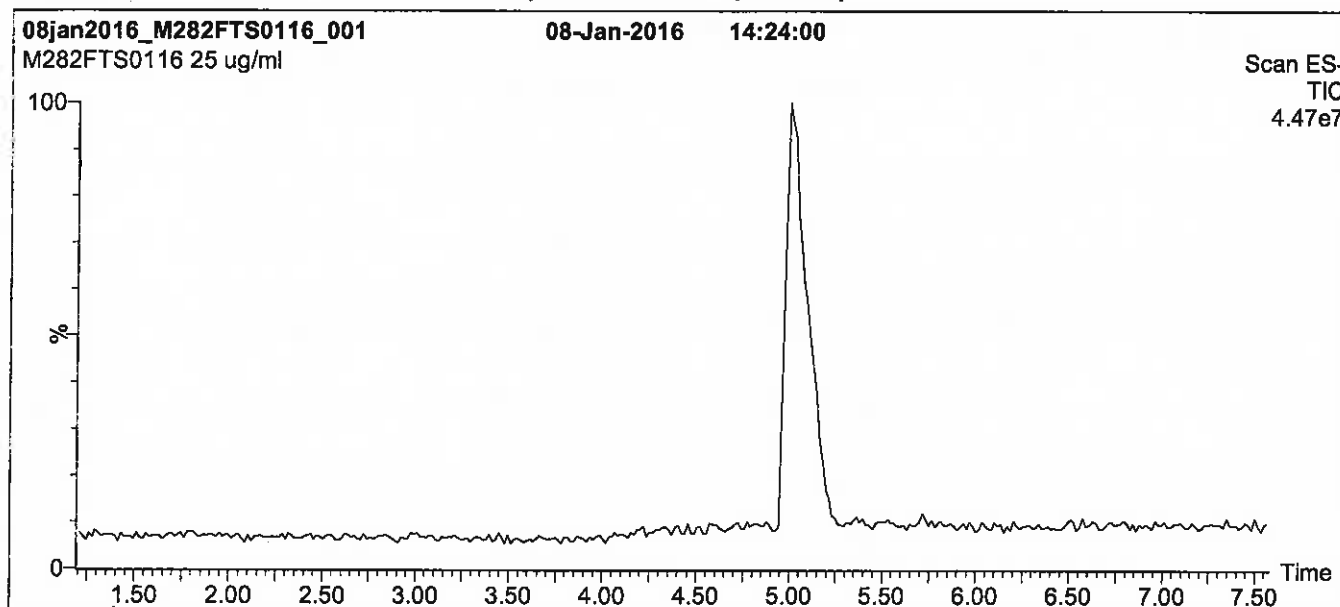

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min
and hold for 2 min before returning
to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 30.00
Cone Gas Flow (l/hr) = 100
Desolvation Gas Flow (l/hr) = 750

Figure 2: M2-8:2FTS; LC/MS/MS Data (Selected MRM Transitions)

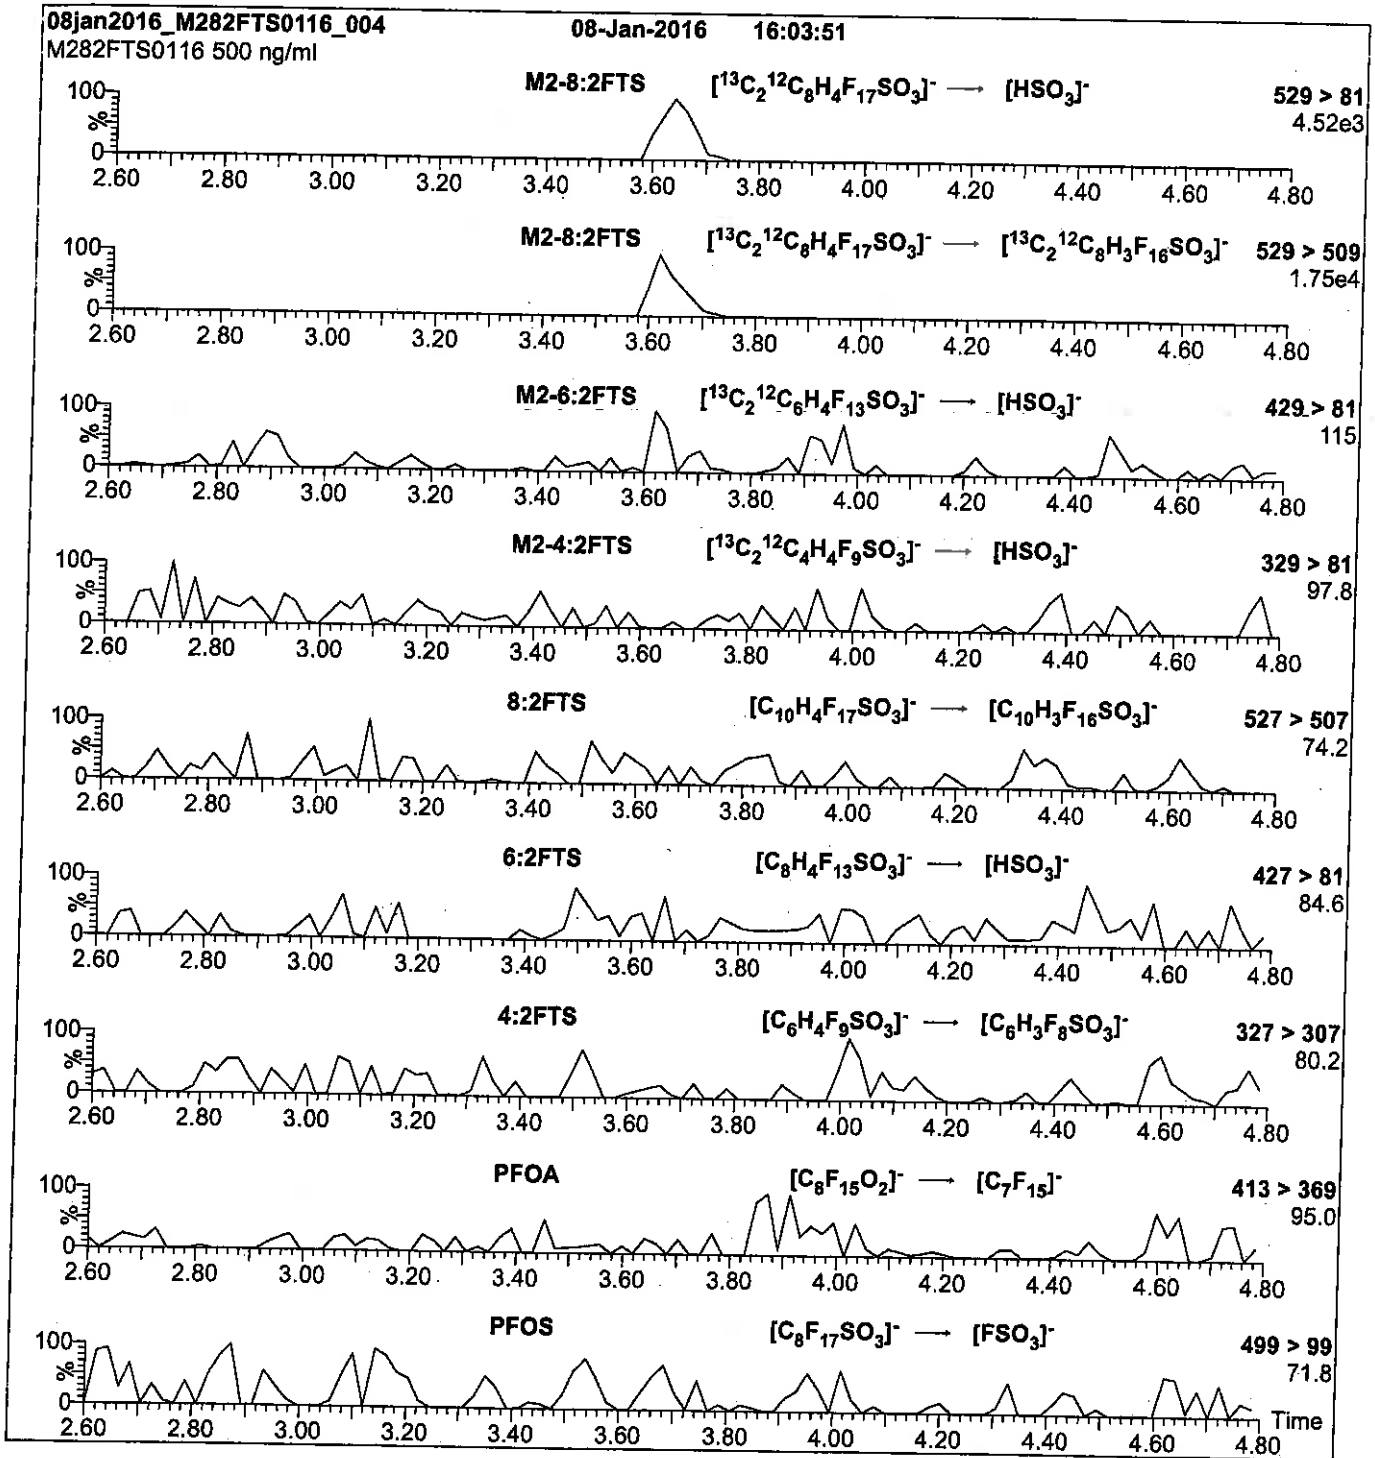

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml M2-8:2FTS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = $3.20\text{e-}3$
Collision Energy (eV) = 30

Reagent

LCM2PFHxDA_00008

R: SBC 9/22/16

739512
ID: LCM2PFHxDA_00008
Exp: 01/07/21 Prod: SBC
13C2-PFHxDA at 50ug/mL




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: M2PFHxDA **LOT NUMBER:** M2PFHxDA1112
COMPOUND: Perfluoro-n-[1,2-¹³C₂]hexadecanoic acid

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA:	¹³ C ₂ ¹² C ₁₄ HF ₃₁ O ₂	MOLECULAR WEIGHT:	816.11
CONCENTRATION:	50 ± 2.5 µg/ml	SOLVENT(S):	Methanol Water (<1%)
CHEMICAL PURITY:	>98%	ISOTOPIC PURITY:	≥99% ¹³ C (1,2- ¹³ C ₂)
LAST TESTED: (mm/dd/yyyy)	01/07/2016		
EXPIRY DATE: (mm/dd/yyyy)	01/07/2021		
RECOMMENDED STORAGE:	Store ampoule in a cool, dark place		


DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains ~ 0.3% of native perfluoro-n-hexadecanoic acid.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:  **Date:** 01/11/2016
B.G. Chittim (mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: M2PFHxDA; LC/MS Data (TIC and Mass Spectrum)

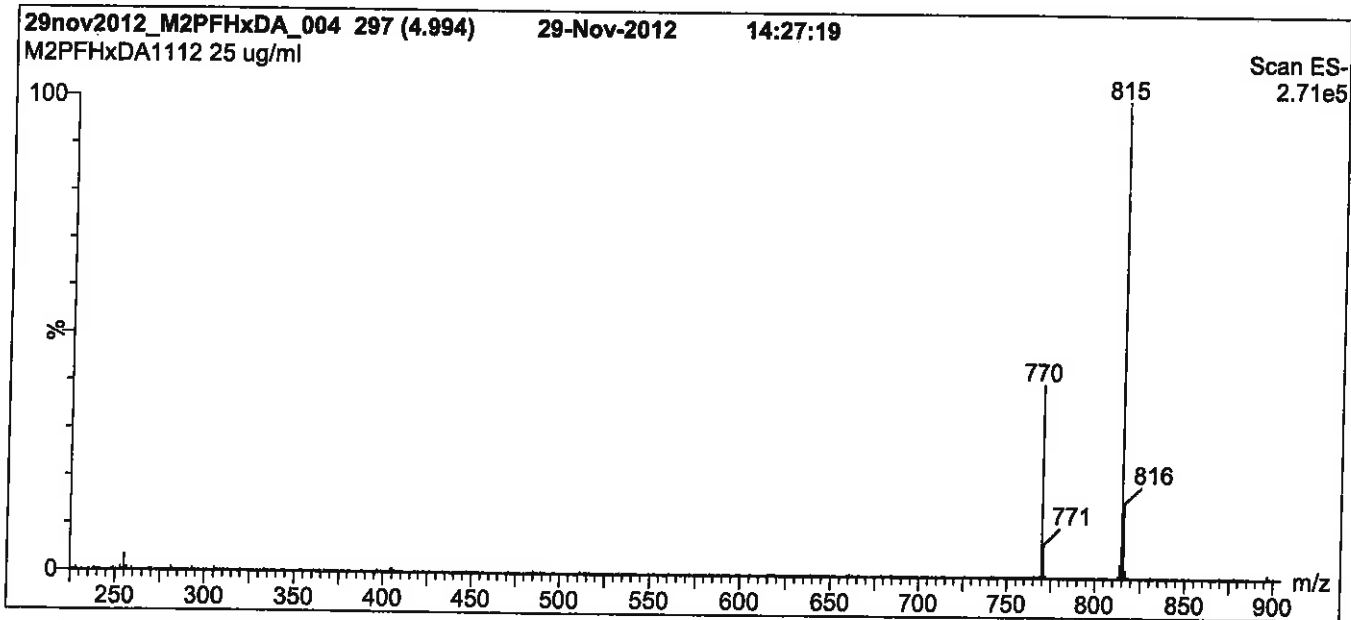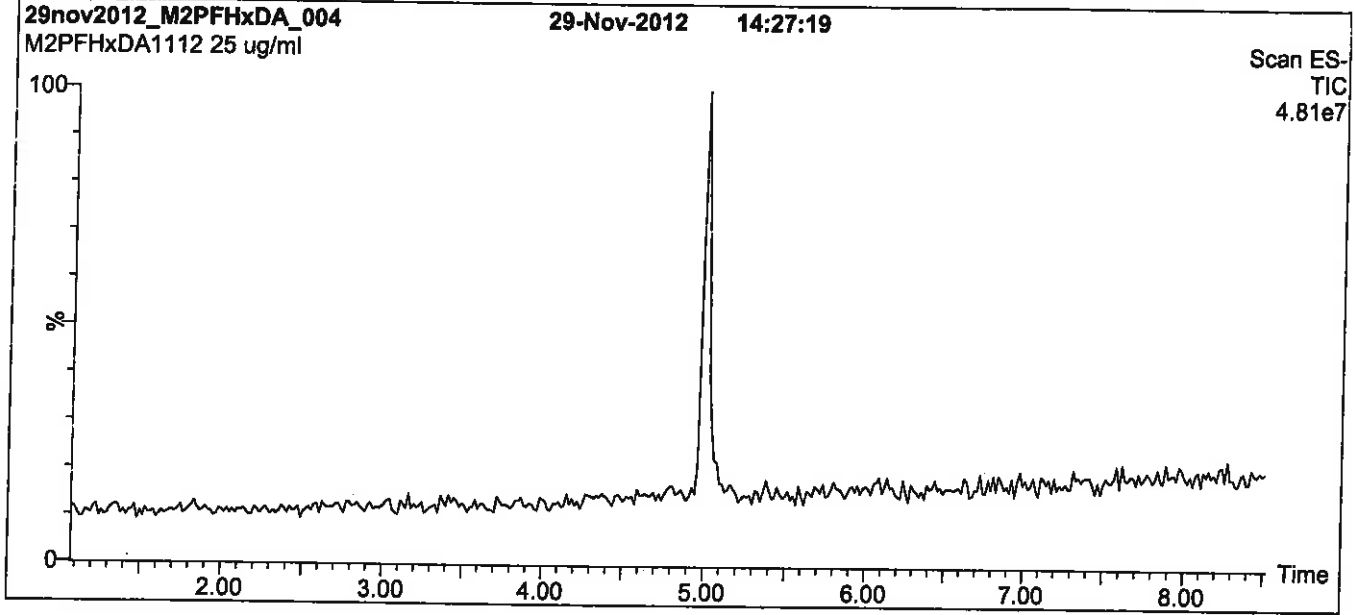

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm


Mobile phase: Gradient
Start: 60% (80:20 MeOH:ACN) / 40% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 100% organic over 7 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min

Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 1200 amu)
Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 25.00
Cone Gas Flow (l/hr) = 60
Desolvation Gas Flow (l/hr) = 750

Figure 2: M2PFHxDA; LC/MS/MS Data (Selected MRM Transitions)

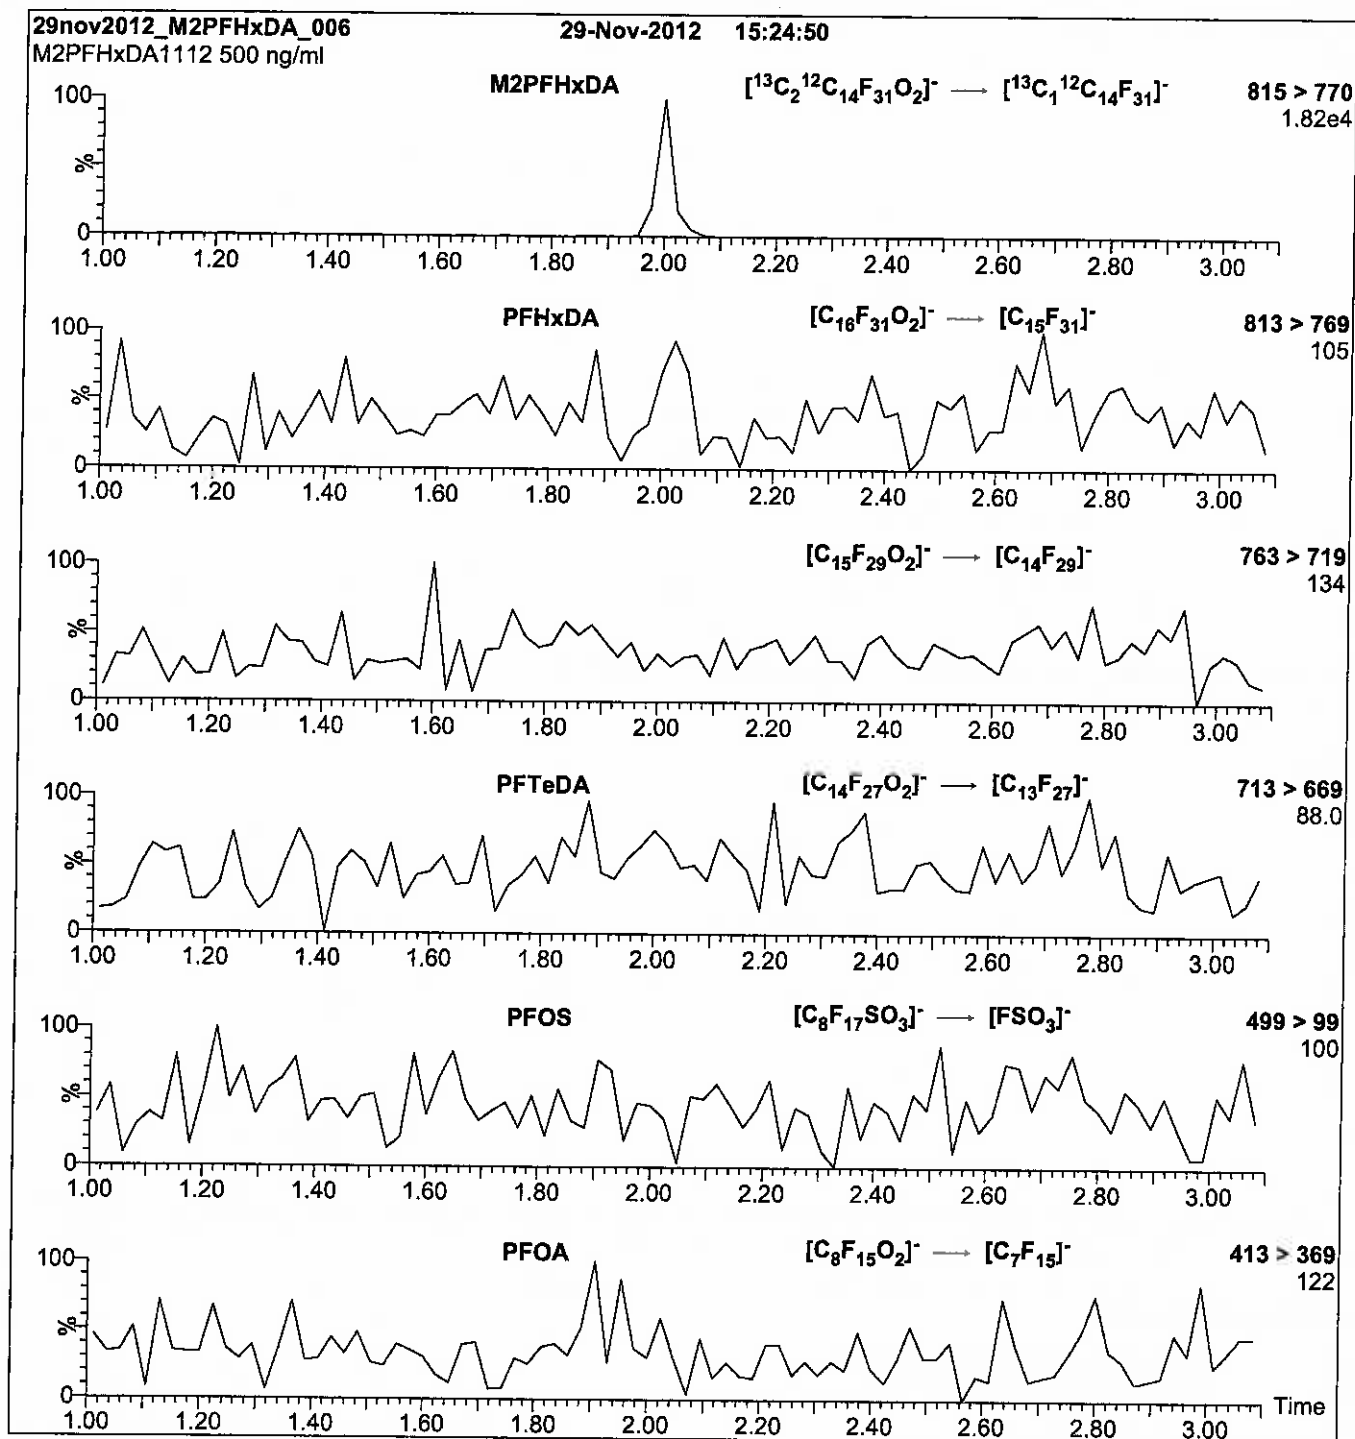

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml M2PFHxDA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.39e-3
Collision Energy (eV) = 15

Reagent

LCM2PFTeDA_00007

Scanned 10/14/16 R: Soc 9/22/16

739563
ID: LCM2PFTeDA_00007
Exp: 12/07/20 Prod: SBC
13C2-PFTeDA at 50ug/mL




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: M2PFTeDA **LOT NUMBER:** M2PFTeDA1115
COMPOUND: Perfluoro-n-[1,2-¹³C₂]tetradecanoic acid

STRUCTURE: **CAS #:** Not available

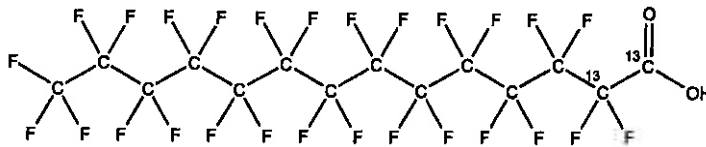

MOLECULAR FORMULA: ¹³C₂¹²C₁₂HF₂₇O₂ **MOLECULAR WEIGHT:** 716.10
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Methanol
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥99% ¹³C
LAST TESTED: (mm/dd/yyyy) 12/07/2015 (1,2-¹³C₂)
EXPIRY DATE: (mm/dd/yyyy) 12/07/2020
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: B.G. Chittim Date: 12/08/2015
B.G. Chittim (mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • Info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: M2PFTeDA; LC/MS Data (TIC and Mass Spectrum)

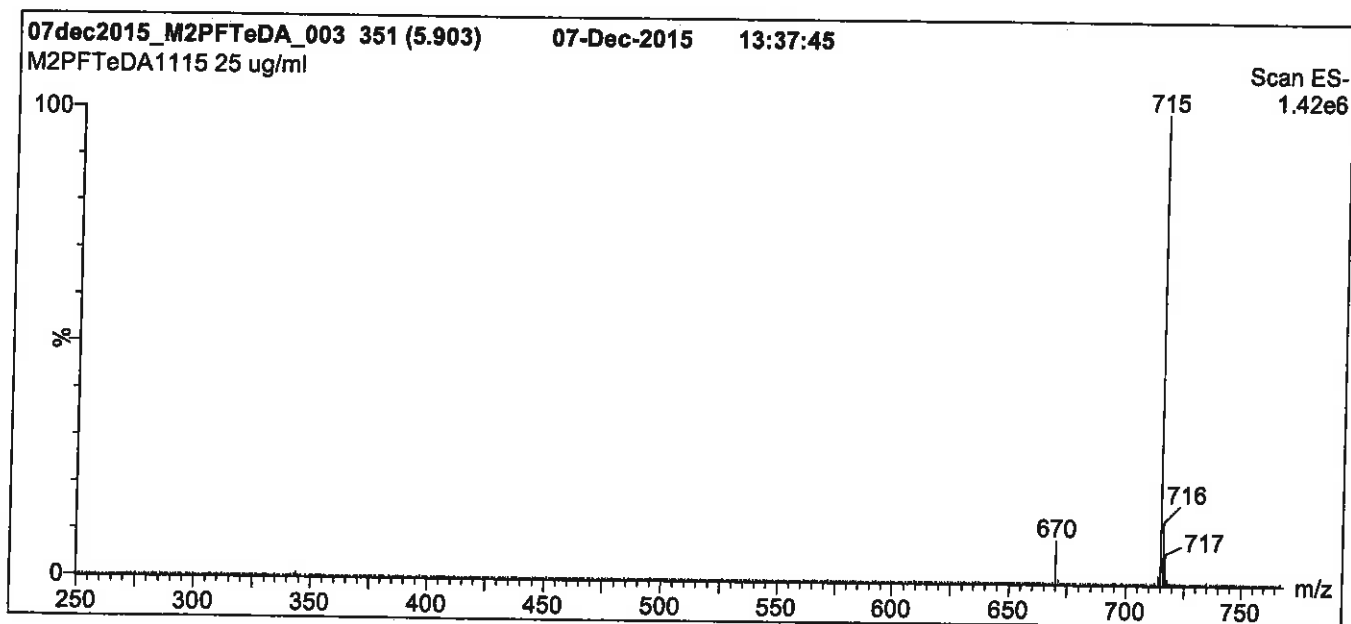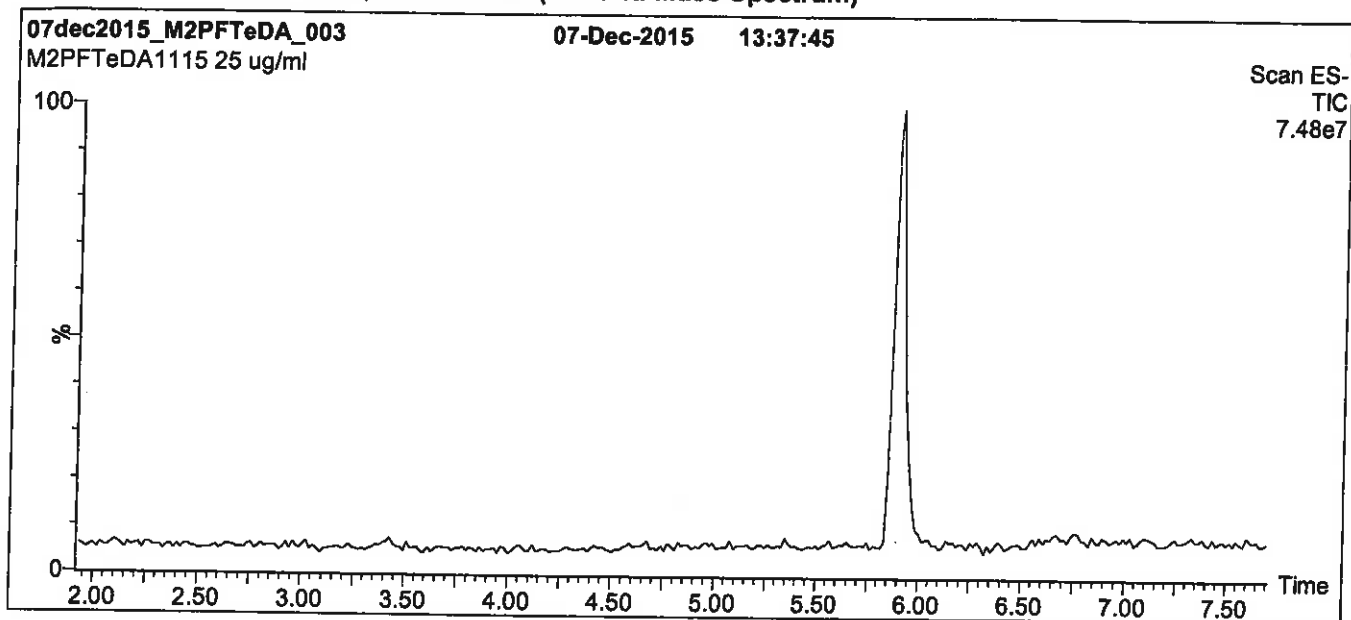

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 65% (80:20 MeOH:ACN) / 35% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 2 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (250 - 1250 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 60
Desolvation Gas Flow (l/hr) = 750

Figure 2: M2PFTeDA; LC/MS/MS Data (Selected MRM Transitions)

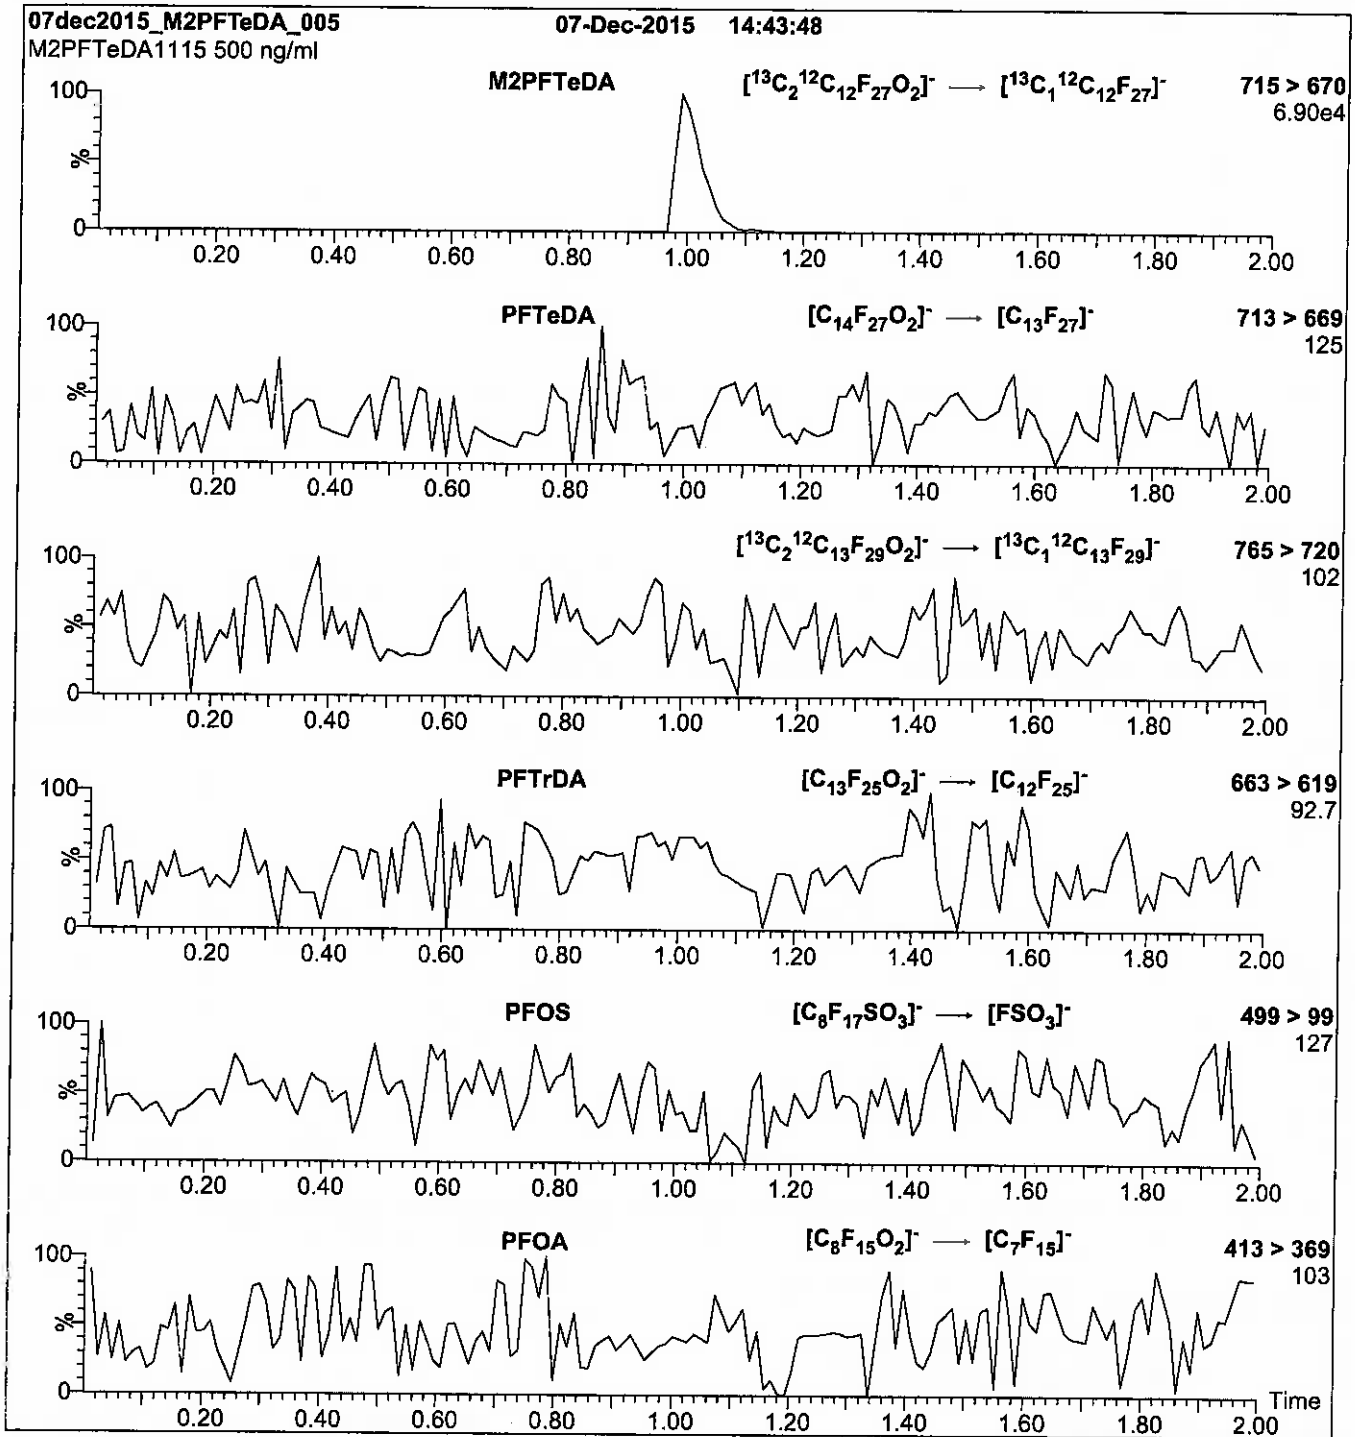

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml M2PFTeDA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.28e-3
Collision Energy (eV) = 14

Reagent

LCM4PFHPA_00007

f: SBC a/22/16

739567
ID: LCM4PFHPA_00007
Exp: 05/27/21 Prpd: SBC
13C4-Perfluoroheptanoic a




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

Scanned 10/14/16 SK

PRODUCT CODE: M4PFHpA **LOT NUMBER:** M4PFHpA0516
COMPOUND: Perfluoro-n-[1,2,3,4-¹³C₄]heptanoic acid

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: ¹³C₄¹²C₃HF₁₃O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 368.03
SOLVENT(S): Methanol
Water (<1%)
ISOTOPIC PURITY: ≥99%¹³C
(1,2,3,4-¹³C₄)

CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 05/27/2016
EXPIRY DATE: (mm/dd/yyyy) 05/27/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 07/05/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: M4PFHpA; LC/MS Data (TIC and Mass Spectrum)

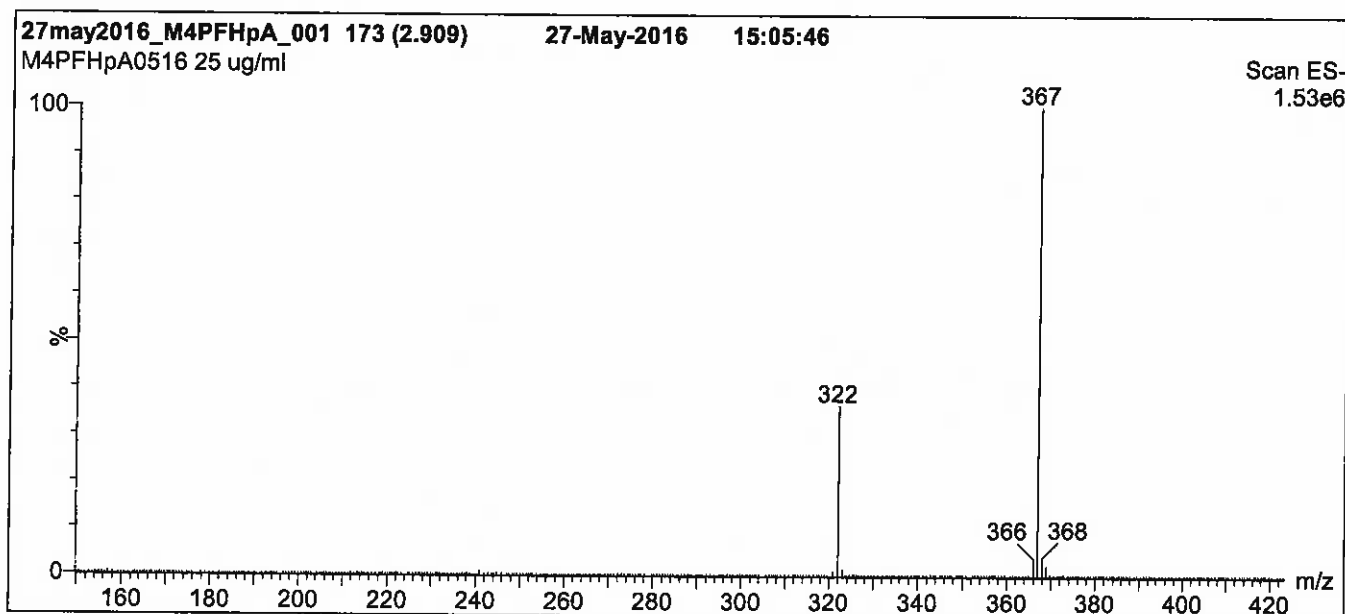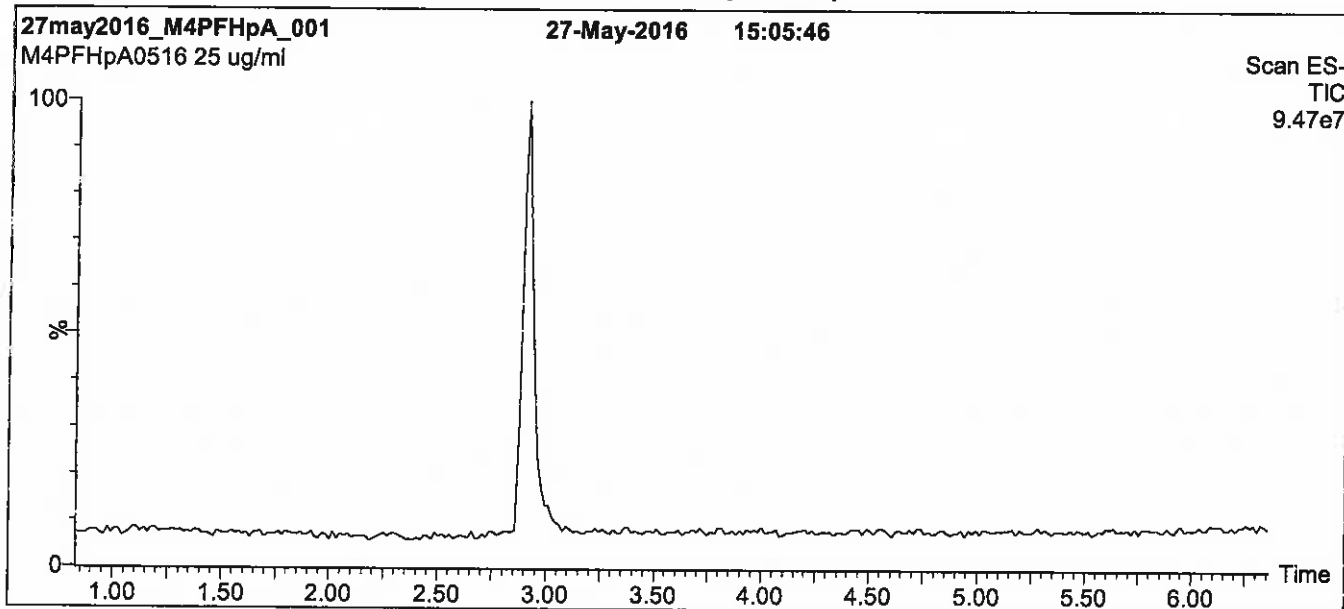

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7.5 min and hold for 1.5 min before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: M4PFHpA; LC/MS/MS Data (Selected MRM Transitions)

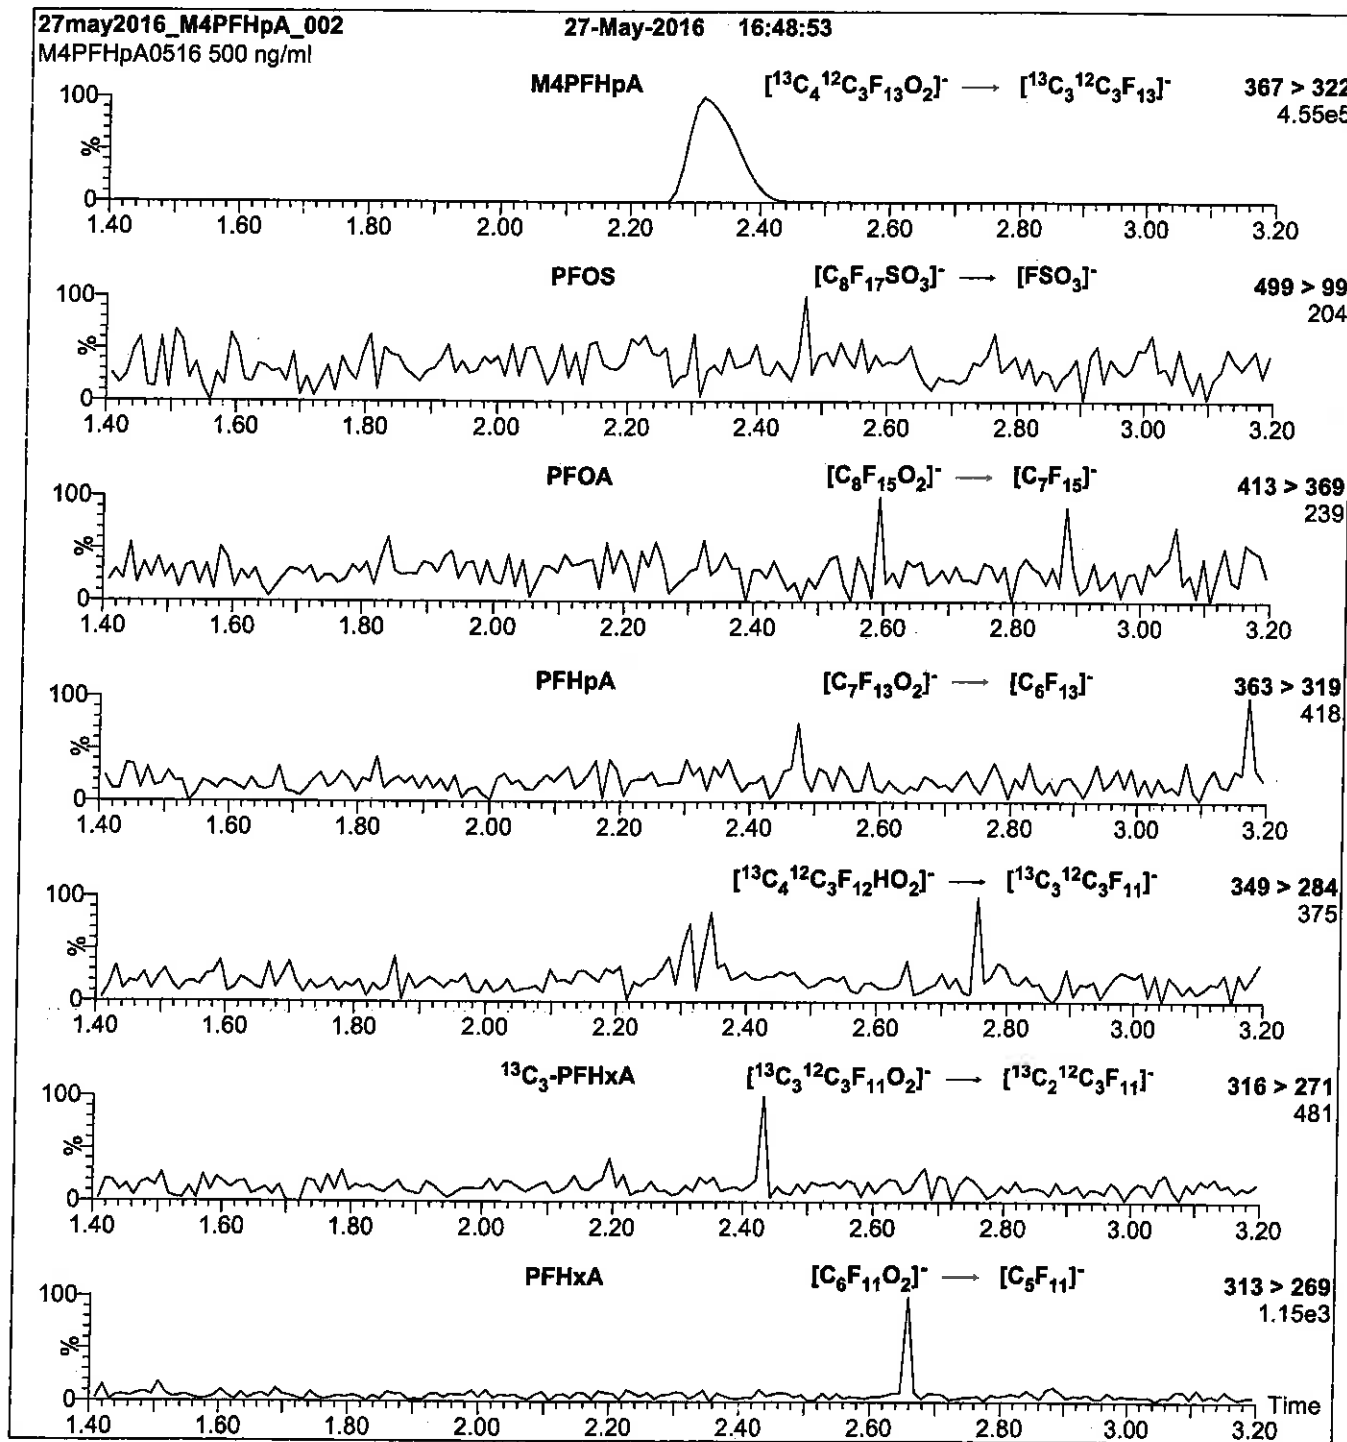

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml M4PFHpA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.35e-3
Collision Energy (eV) = 11

Reagent

LCM5PFPEA_00008

R: 8BC 9/22/16



739590
ID: LCM5PFPEA_00008
Exp: 05/22/20 Prpt: SAC
13C5-Perfluoropentanoic a




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

Scanned 10/14/16 LR

PRODUCT CODE: M5PFPeA **LOT NUMBER:** M5PFPeA0515
COMPOUND: Perfluoro-n-[¹³C₅]pentanoic acid

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: ¹³C₅HF₉O₂ **MOLECULAR WEIGHT:** 269.01
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Methanol
Water (<1%)
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥99% ¹³C
(¹³C₅)
LAST TESTED: (mm/dd/yyyy) 05/22/2015
EXPIRY DATE: (mm/dd/yyyy) 05/22/2020
RECOMMENDED STORAGE: Store ampoule in a cool, dark place


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains < 0.1% of perfluoro-n-pentanoic acid.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:  **Date:** 05/25/2015
B.G. Chittim (mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: M5PFPeA; LC/MS Data (TIC and Mass Spectrum)

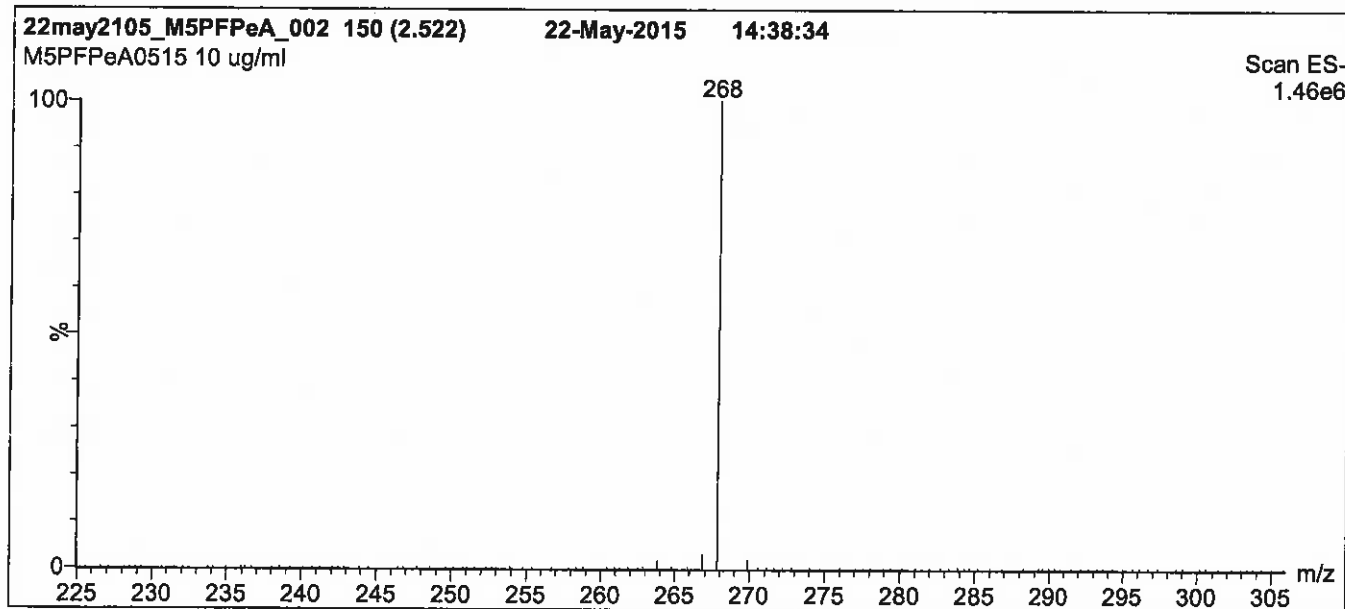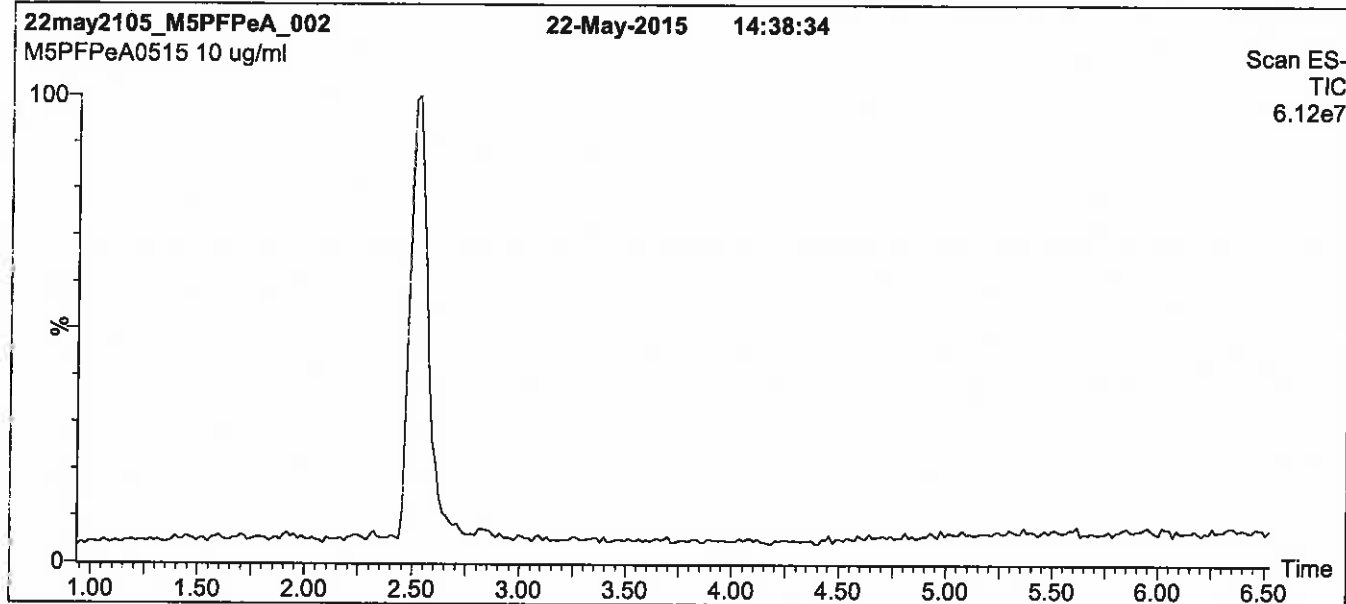

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 40% (80:20 MeOH:ACN) / 60% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for
 1.5 min before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.00
 Cone Voltage (V) = 15.00
 Cone Gas Flow (l/hr) = 60
 Desolvation Gas Flow (l/hr) = 750

Figure 2: M5PFPeA; LC/MS/MS Data (Selected MRM Transitions)

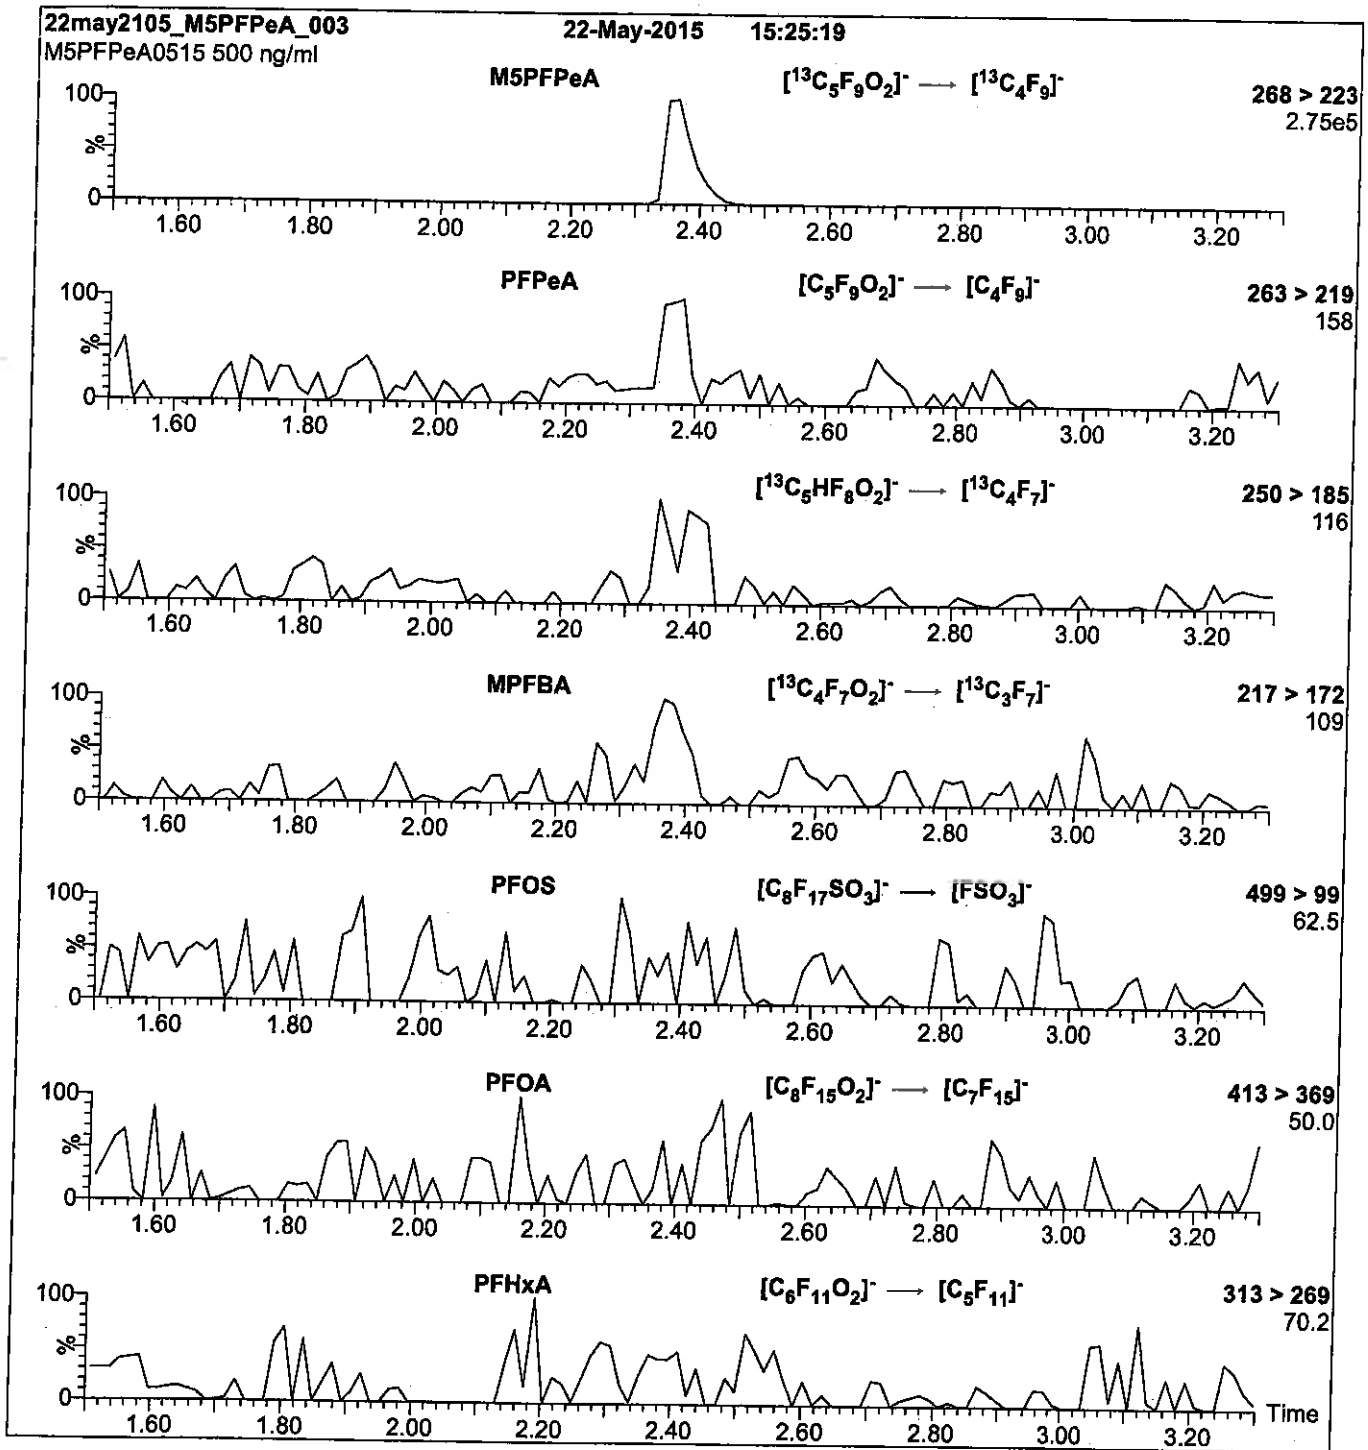

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml M5PFPeA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.35e-3
Collision Energy (eV) = 9

Reagent

LCM8FOSA_00011

R: SBC
Scanned 10/14/16
9/22/16



739615
ID: LCM8FOSA_00011
Exp: 12/22/17 Prod: SBC
13C8-Perfluorooctanesulfo




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: M8FOSA-I **LOT NUMBER:** M8FOSA1215I
COMPOUND: Perfluoro-1-[¹³C₈]octanesulfonamide

STRUCTURE: **CAS #:** Not available

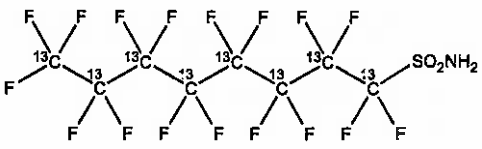

MOLECULAR FORMULA: ¹³C₈H₂F₁₇NO₂S **MOLECULAR WEIGHT:** 507.09
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Isopropanol
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥99% ¹³C
LAST TESTED: (mm/dd/yyyy) 12/22/2015 (¹³C₈)
EXPIRY DATE: (mm/dd/yyyy) 12/22/2017
RECOMMENDED STORAGE: Refrigerate ampoule

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:  **Date:** 01/14/2016
B.G. Chittim (mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: M8FOSA-I; LC/MS Data (TIC and Mass Spectrum)

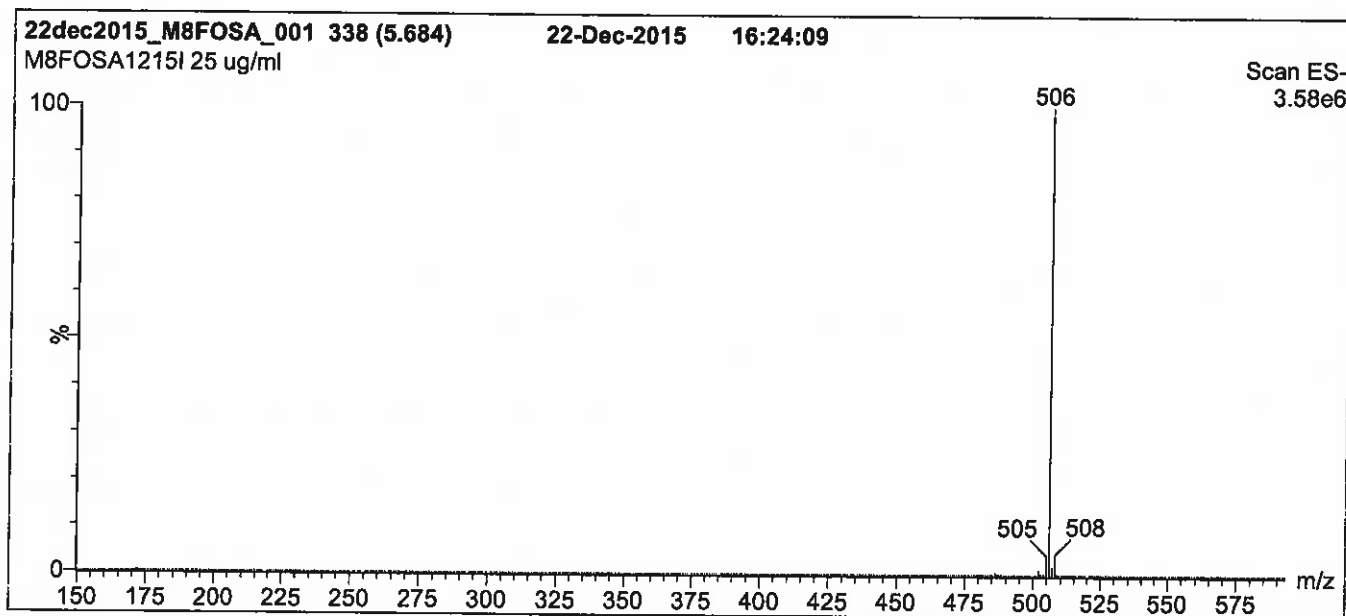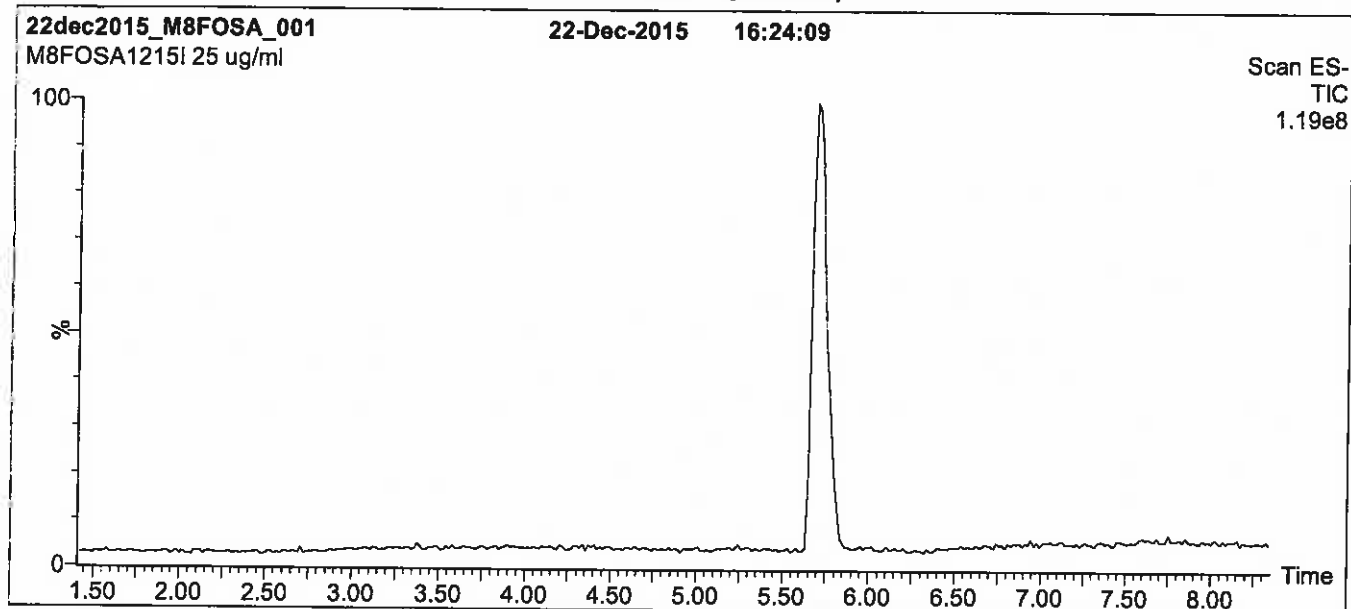

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient

Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 2 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 2.50
Cone Voltage (V) = 40.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: M8FOSA-I; LC/MS/MS Data (Selected MRM Transitions)

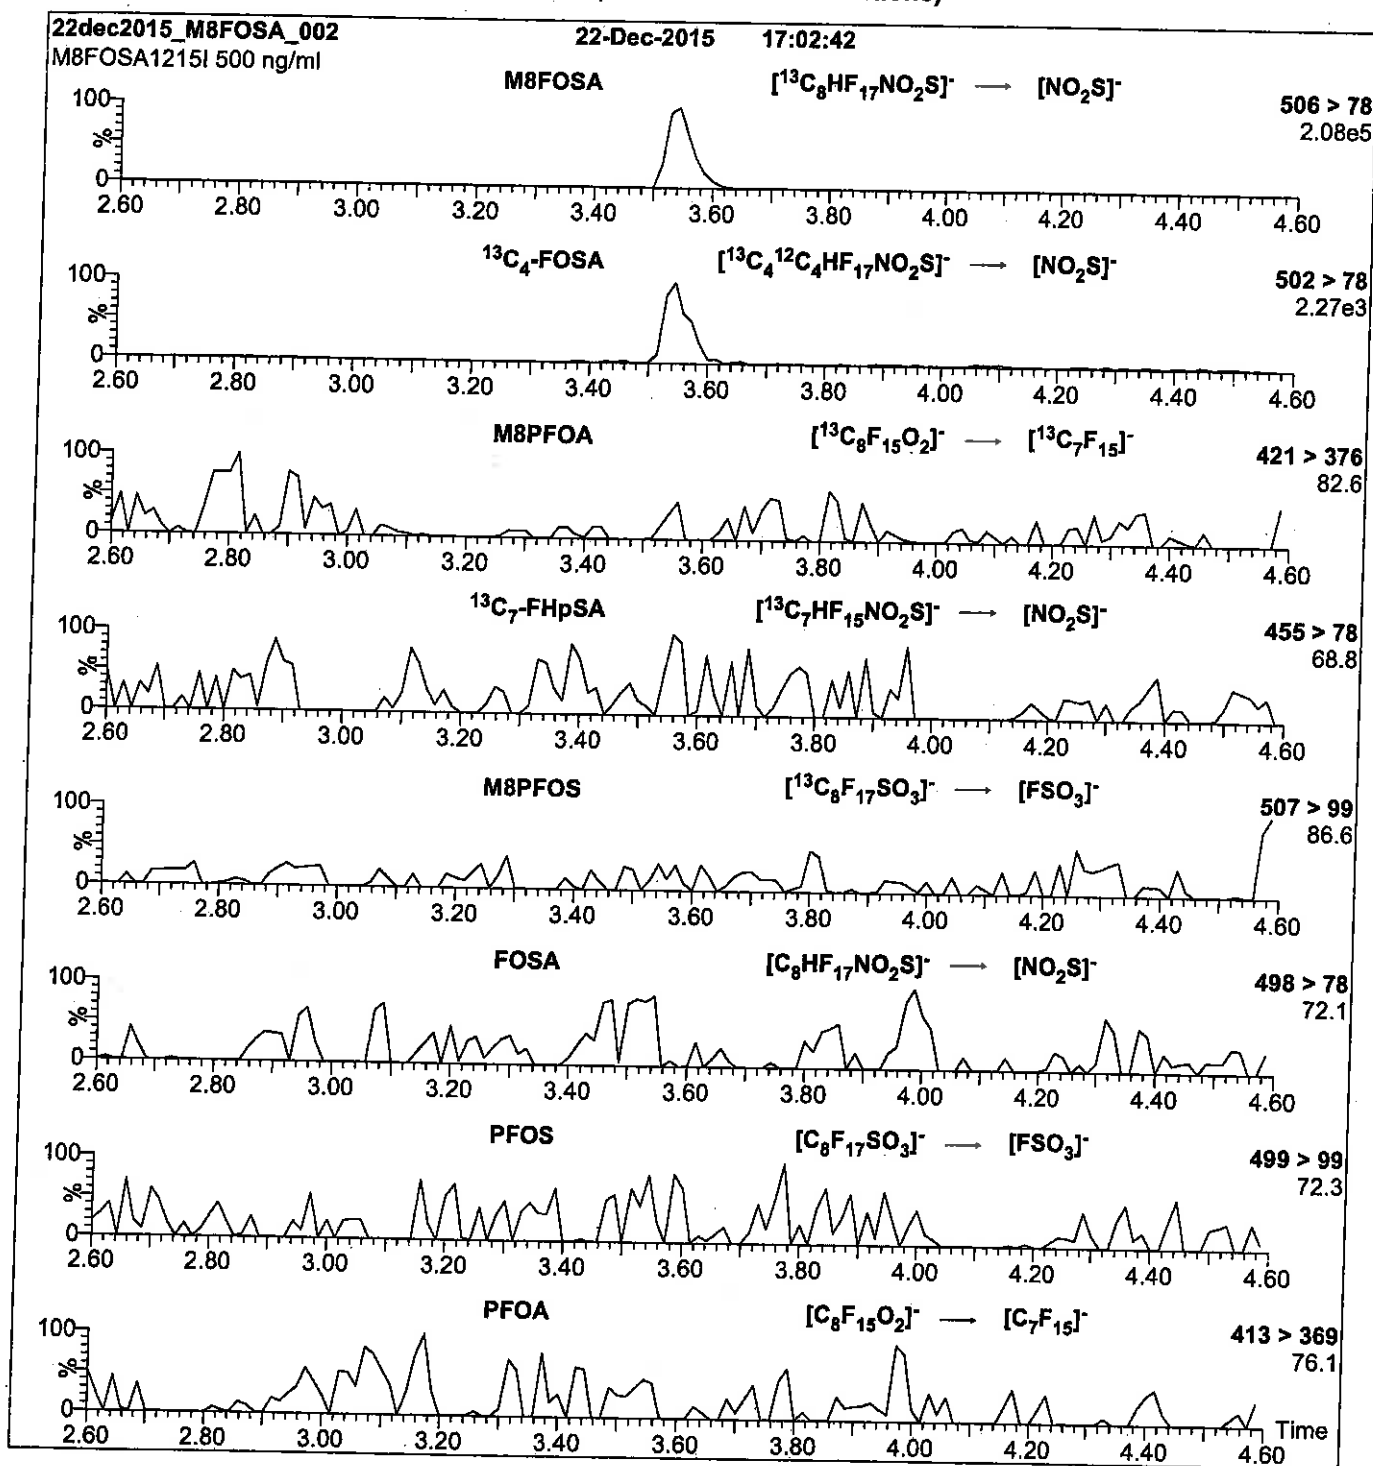

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml M8FOSA-I)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.39e-3
Collision Energy (eV) = 30

Reagent

LCMPFBA_00008

R: 8BC 9/22/16



739593

ID: LCMFBA_00008

Exp: 05/24/21 Prep: SEC

¹³C4-Perfluorobutanoic ac




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

Scanned 10/14/16 SP

PRODUCT CODE: MPFBA **LOT NUMBER:** MPFBA0516
COMPOUND: Perfluoro-n-[1,2,3,4-¹³C₄]butanoic acid

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: ¹³C₄HF₇O₂ **MOLECULAR WEIGHT:** 218.01
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Methanol
Water (<1%)
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥99%¹³C
(1,2,3,4-¹³C₄)
LAST TESTED: (mm/dd/yyyy) 05/24/2016
EXPIRY DATE: (mm/dd/yyyy) 05/24/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:  **Date:** 05/30/2016
B.G. Chittim (mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFBA; LC/MS Data (TIC and Mass Spectrum)

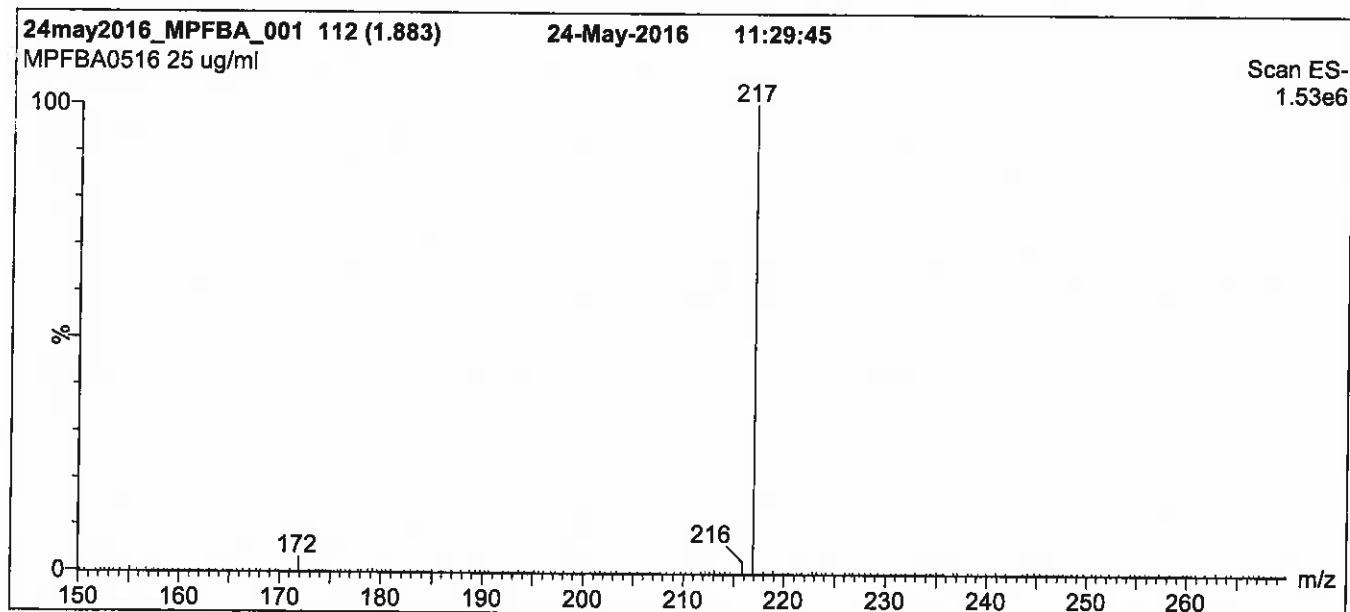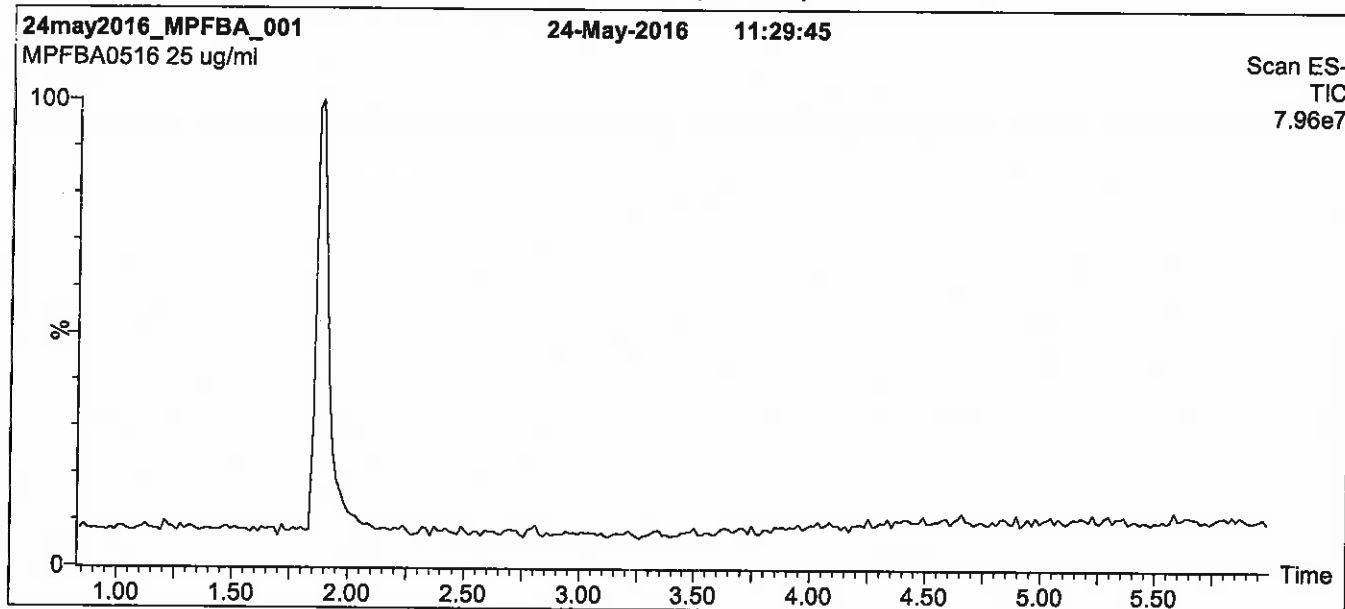

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 30% (80:20 MeOH:ACN) / 70% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 10.00
 Cone Gas Flow (l/hr) = 100
 Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFBA; LC/MS/MS Data (Selected MRM Transitions)

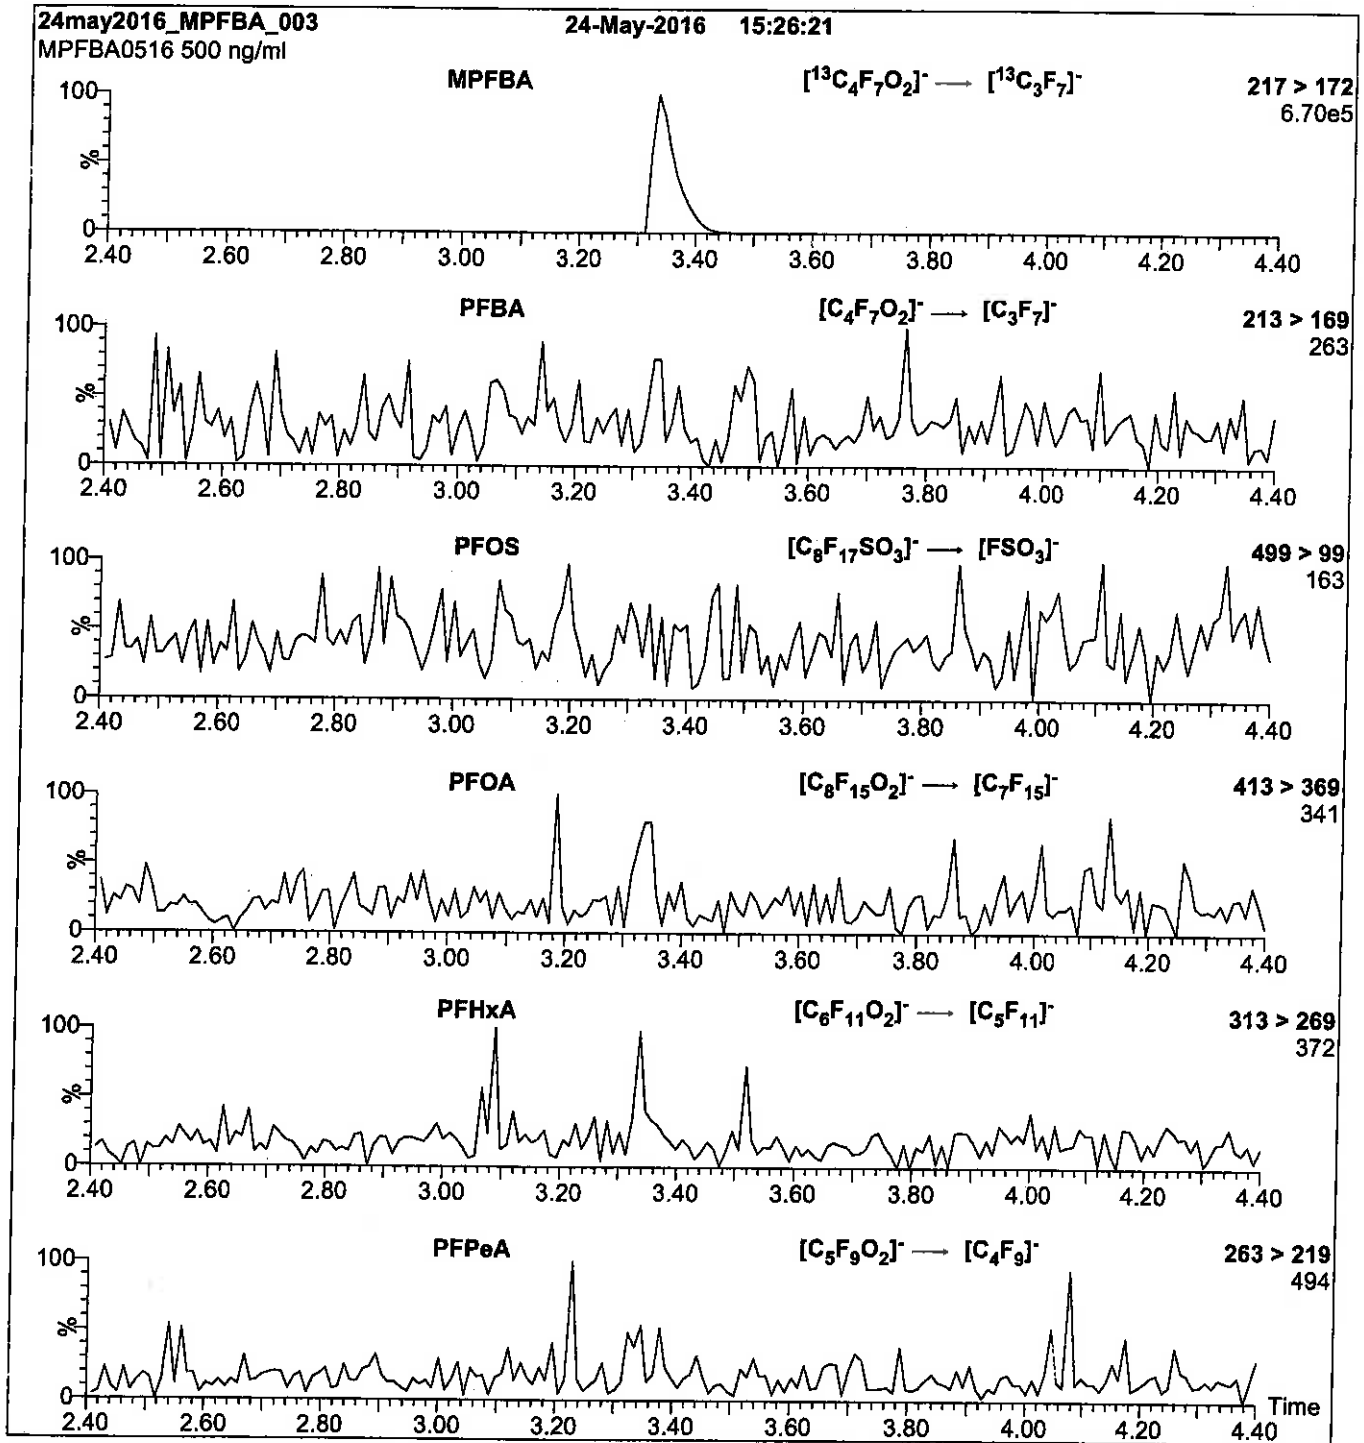

Conditions for Figure 2:

Injection: Direct loop Injection
10 μl (500 ng/ml MPFBA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.50e-3
Collision Energy (eV) = 10

Reagent

LCMPFDA_00011

Scanned 10/14/16 R: SBC 9/22/16

739609
ID: LCMFDA_00011
Exp: 08/19/20 Prep: SBC
13C2-Perfluorodecanoic a




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFDA **LOT NUMBER:** MPFDA0815
COMPOUND: Perfluoro-n-[1,2-¹³C₂]decanoic acid

STRUCTURE: **CAS #:** Not available

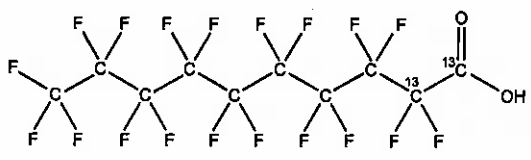

MOLECULAR FORMULA: ¹³C₂¹²C₈HF₁₈O₂ **MOLECULAR WEIGHT:** 516.07
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Methanol
Water (<1%)
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥99% ¹³C
(1,2-¹³C₂)
LAST TESTED: (mm/dd/yyyy) 08/19/2015
EXPIRY DATE: (mm/dd/yyyy) 08/19/2020
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains < 0.1% of ¹³C₁-PFNA.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: B.G. Chittim Date: 08/21/2015
B.G. Chittim (mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFDA; LC/MS Data (TIC and Mass Spectrum)

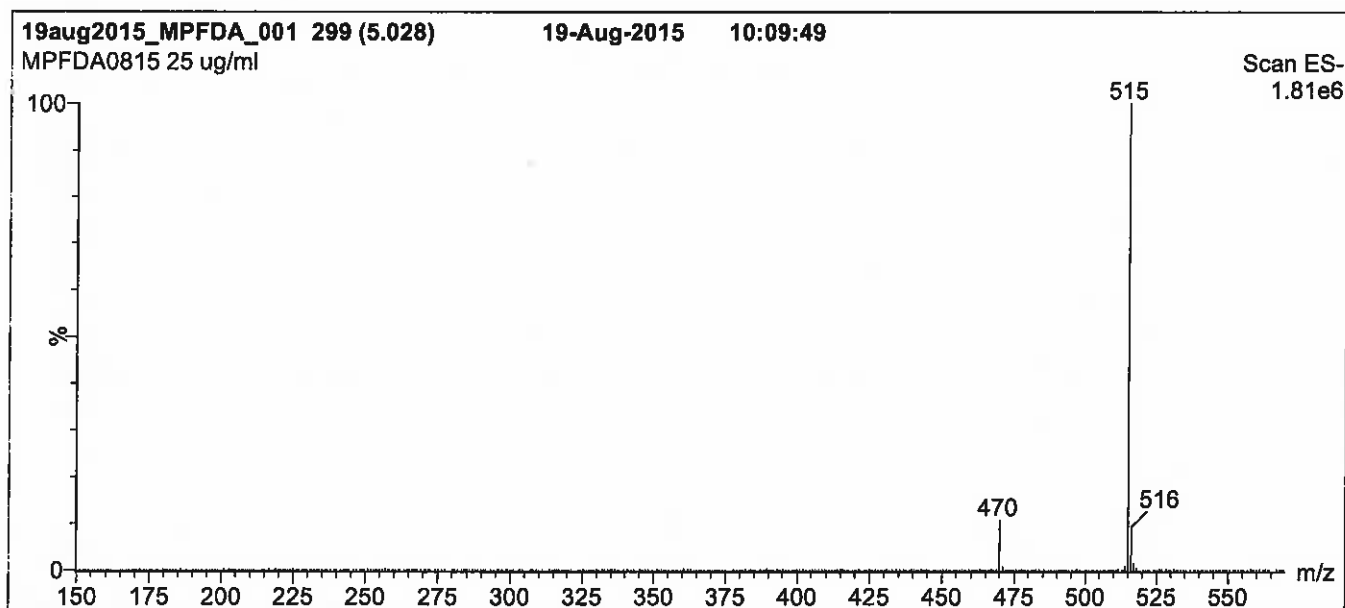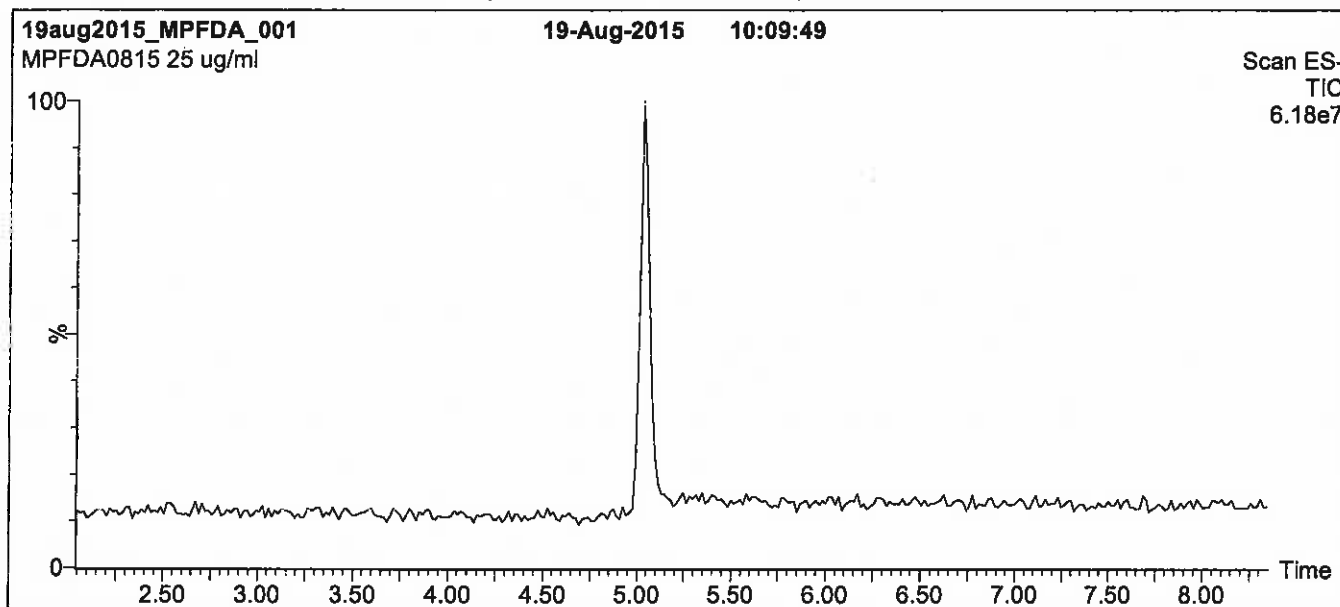

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm
Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 2 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFDA; LC/MS/MS Data (Selected MRM Transitions)

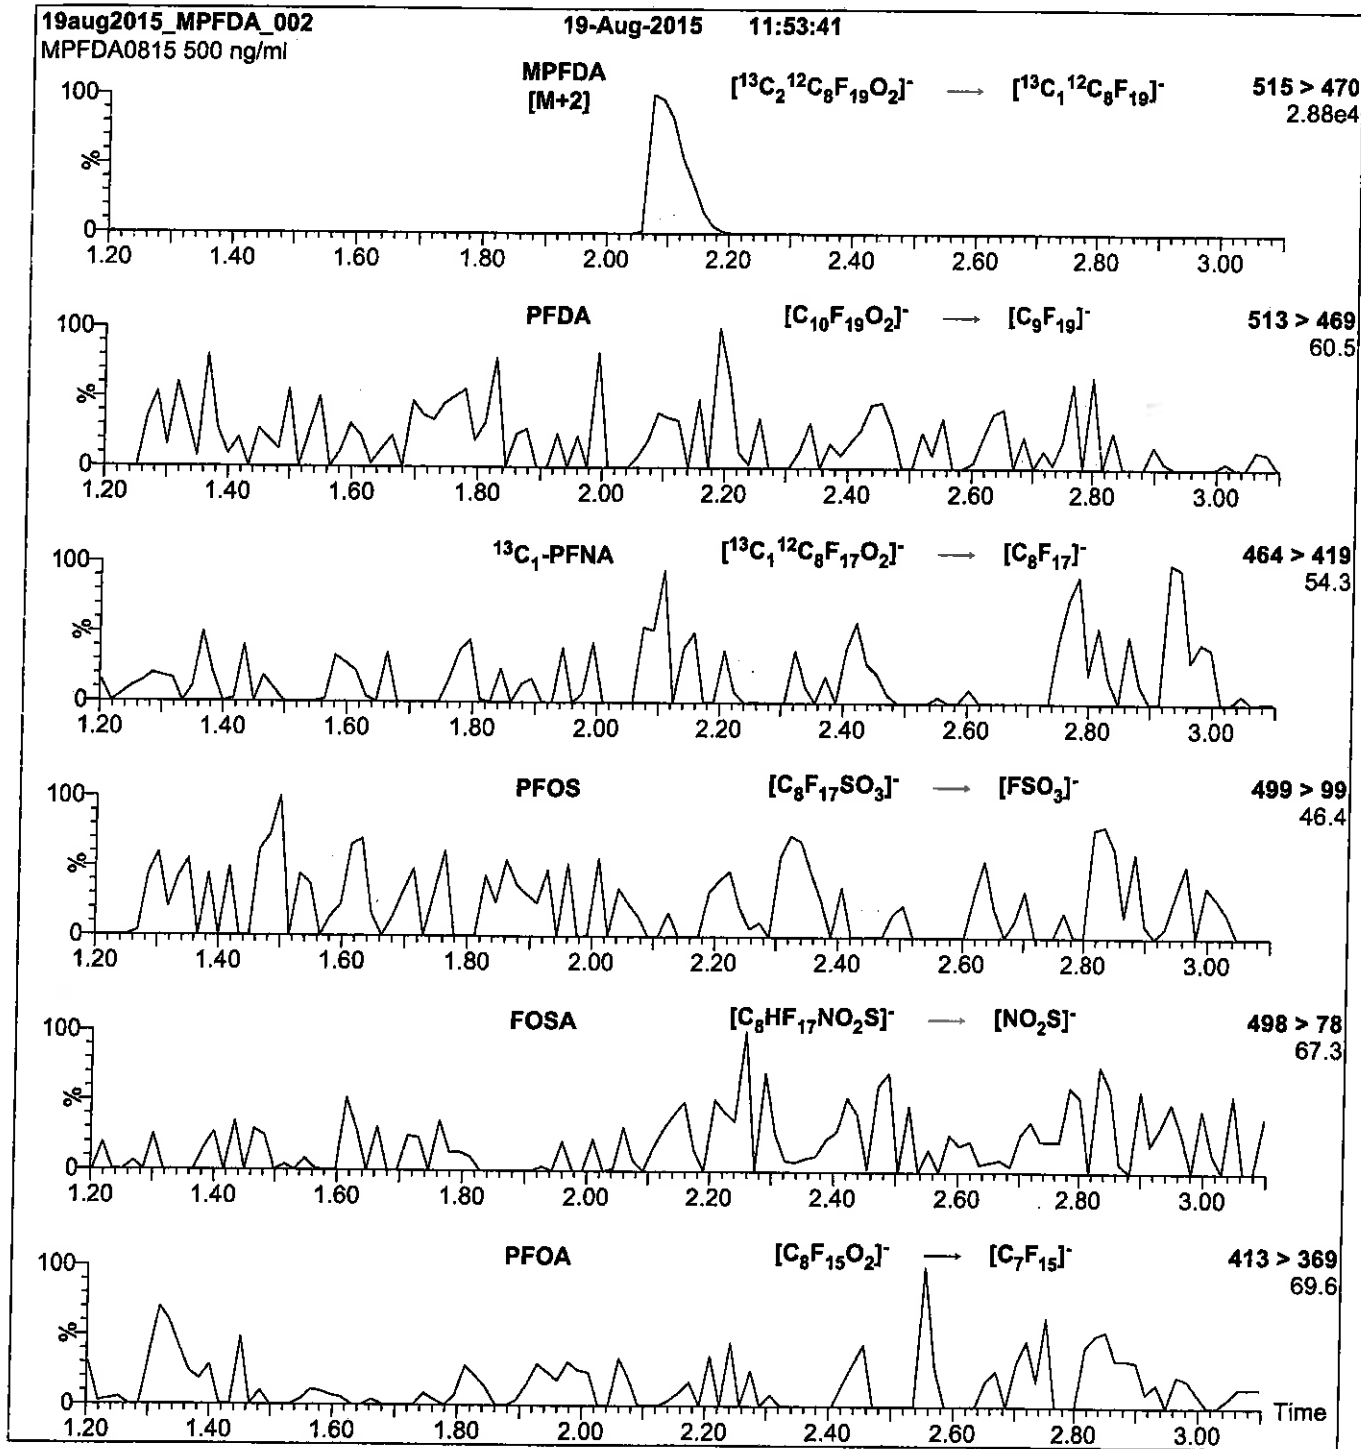

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml MPFDA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.35e-3
Collision Energy (eV) = 13

Reagent

LCMPFD_oA_00008

R: 882 9/22/16



739598
ID: LCMFDoA_00008
Exp: 04/08/21 Prod: SBC
13C2-Perfluorododecanoic




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

Scanned 10/14/16 SR

PRODUCT CODE: MPFDoA **LOT NUMBER:** MPFDoA0416
COMPOUND: Perfluoro-n-[1,2-¹³C₂]dodecanoic acid

STRUCTURE: **CAS #:** Not available

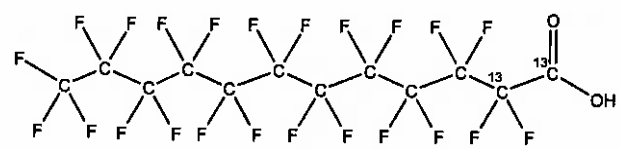

MOLECULAR FORMULA: ¹³C₂¹²C₁₀HF₂₃O₂ **MOLECULAR WEIGHT:** 616.08
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Methanol
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥99% ¹³C
LAST TESTED: (mm/dd/yyyy) 04/08/2016 (1,2-¹³C₂)
EXPIRY DATE: (mm/dd/yyyy) 04/08/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 04/15/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • Info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFDoA; LC/MS Data (TIC and Mass Spectrum)

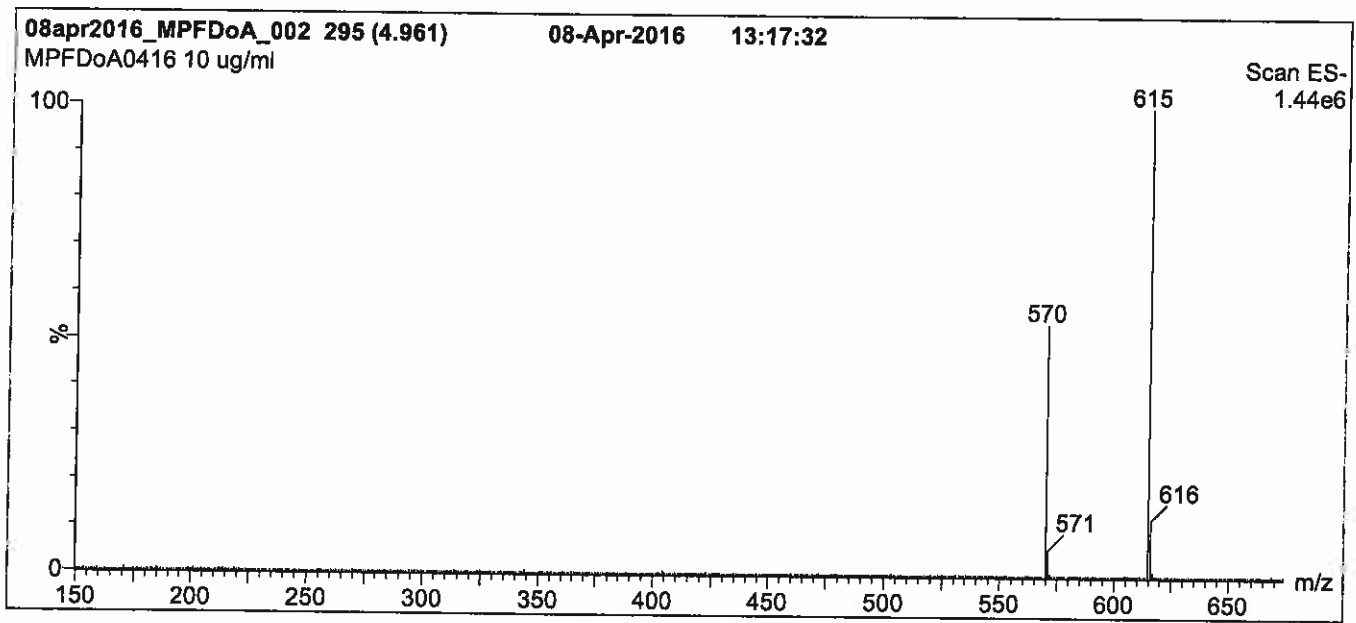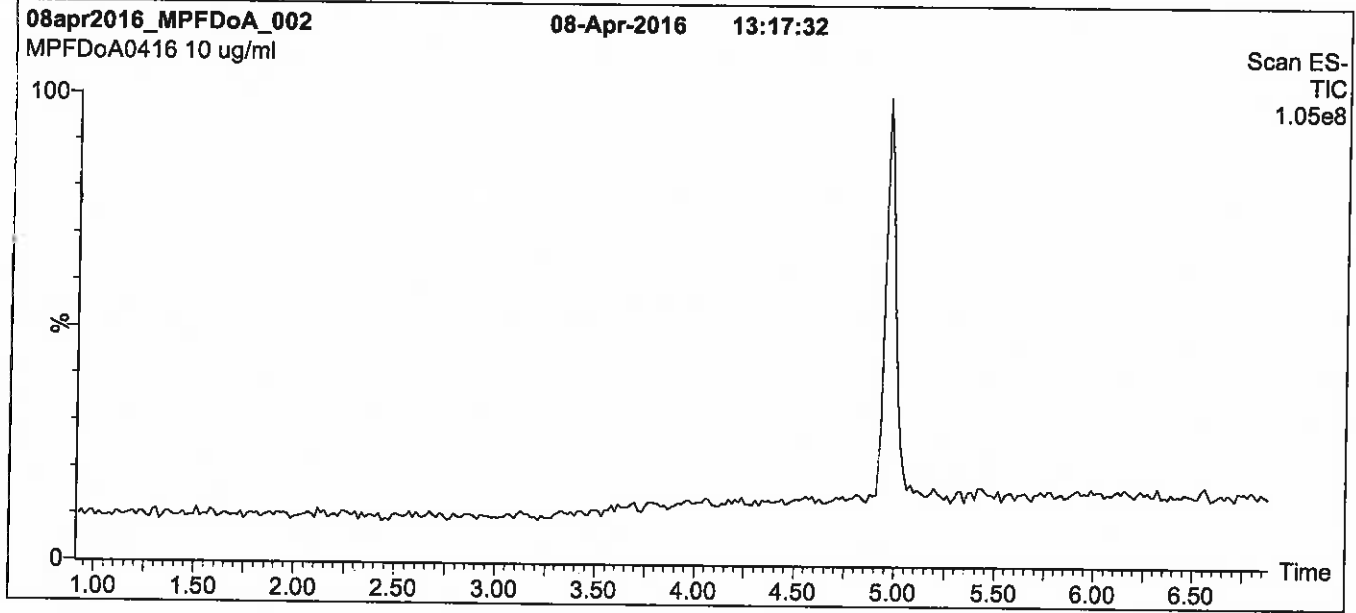

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 60% (80:20 MeOH:ACN) / 40% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.00
 Cone Voltage (V) = 20.00
 Cone Gas Flow (l/hr) = 100
 Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFDoA; LC/MS/MS Data (Selected MRM Transitions)

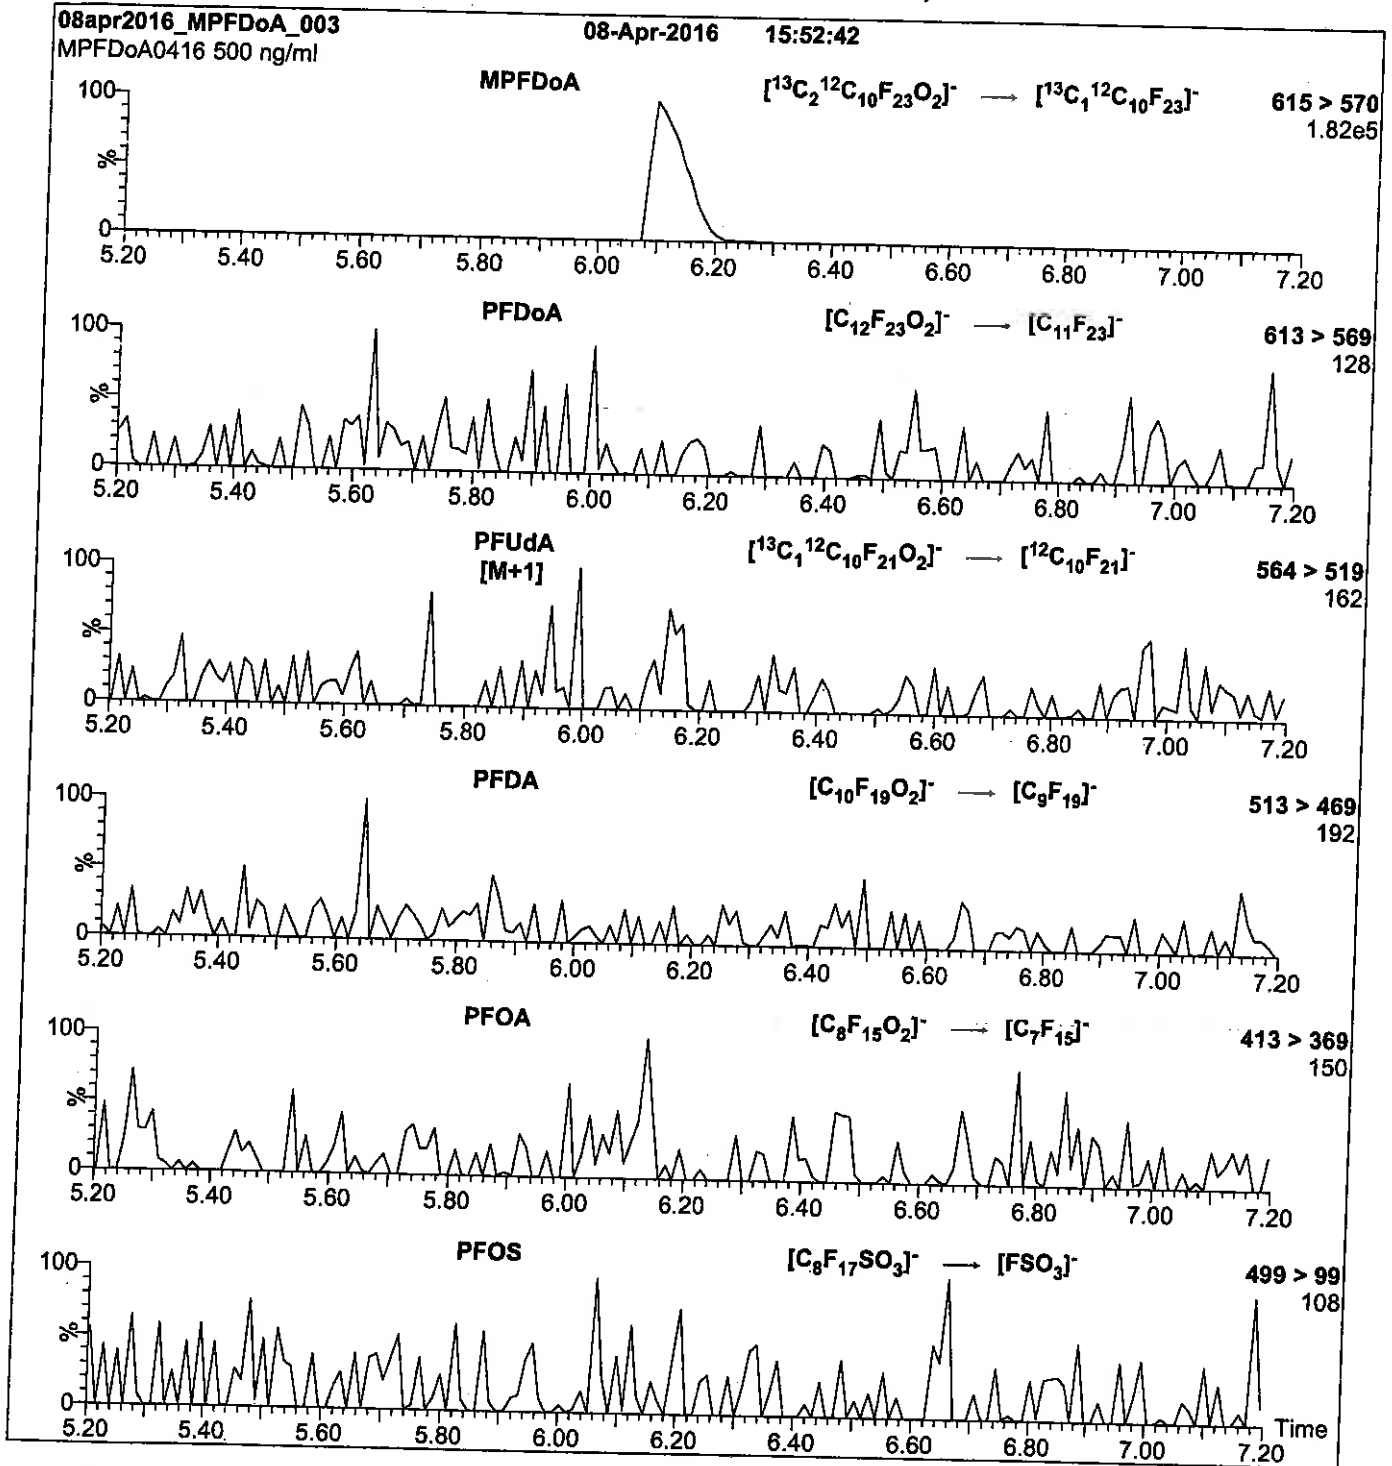

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml MPFDoA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.24e-3
Collision Energy (eV) = 13

Reagent

LCMPFHxA_00012

Scanned 10/11/16 R: SBC 9/22/16

739612
ID: LCMPFHxA_00012
Exp: 04/08/21 Prpd: SBC
13C2-Perfluorohexanoic ac



WELLINGTON LABORATORIES


CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFHxA
COMPOUND: Perfluoro-n-[1,2-¹³C₂]hexanoic acid

LOT NUMBER: MPFHxA0416

STRUCTURE:

CAS #: Not available

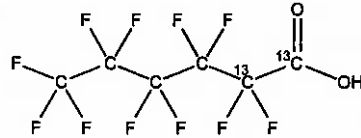

MOLECULAR FORMULA: ¹³C₂¹²C₄HF₁₁O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 316.04
SOLVENT(S): Methanol
Water (<1%)

CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 04/08/2016
EXPIRY DATE: (mm/dd/yyyy) 04/08/2021

ISOTOPIC PURITY: ≥99%¹³C
(1,2-¹³C₂)

RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains < 0.1% of perfluoro-n-hexanoic acid and ~ 0.3% of perfluoro-n-octanoic acid.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim
Date: 04/29/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFHxA; LC/MS Data (TIC and Mass Spectrum)

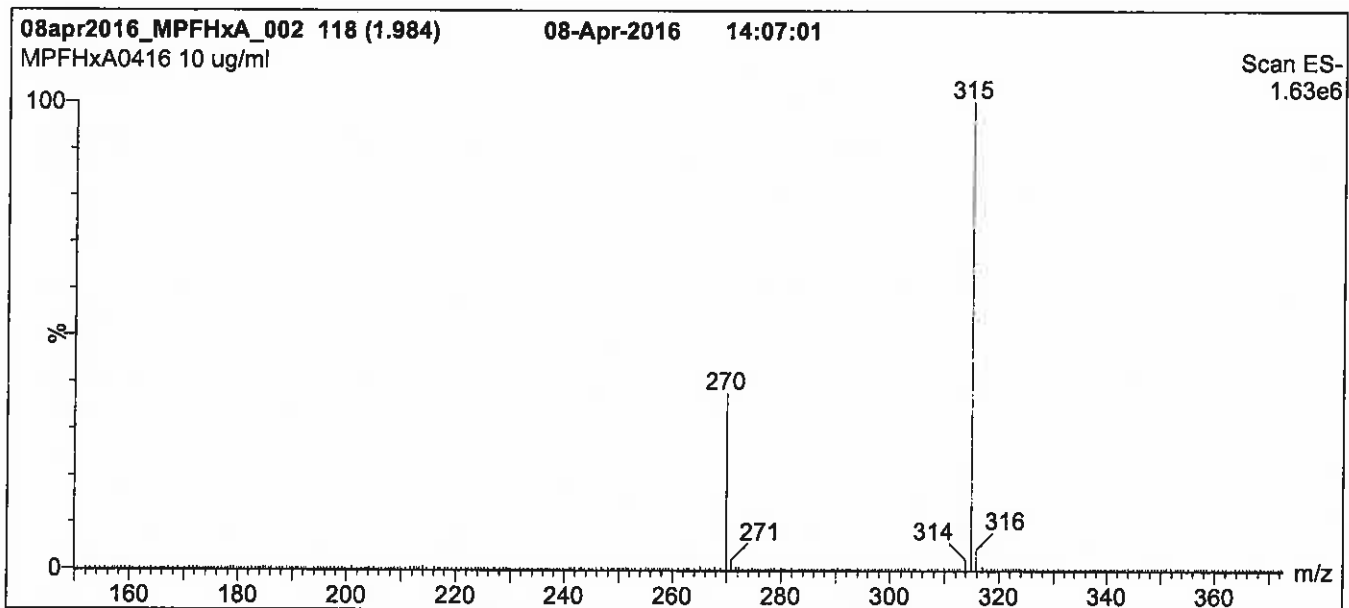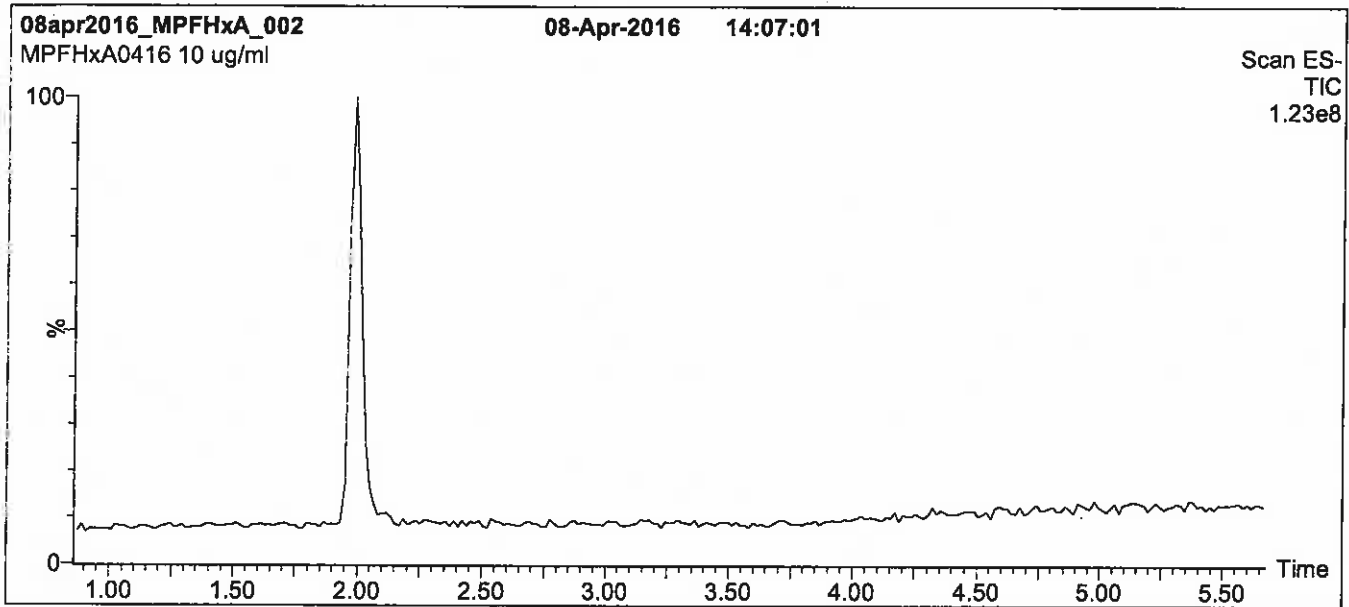

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm


Mobile phase: Gradient
 Start: 50% (80:20 MeOH:ACN) / 50% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7.5 min and hold for 1.5 min
 before returning to initial conditions over 0.5 min.
 Time: 10 min

Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)
 Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.00
 Cone Voltage (V) = 15.00
 Cone Gas Flow (l/hr) = 100
 Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFHxA; LC/MS/MS Data (Selected MRM Transitions)

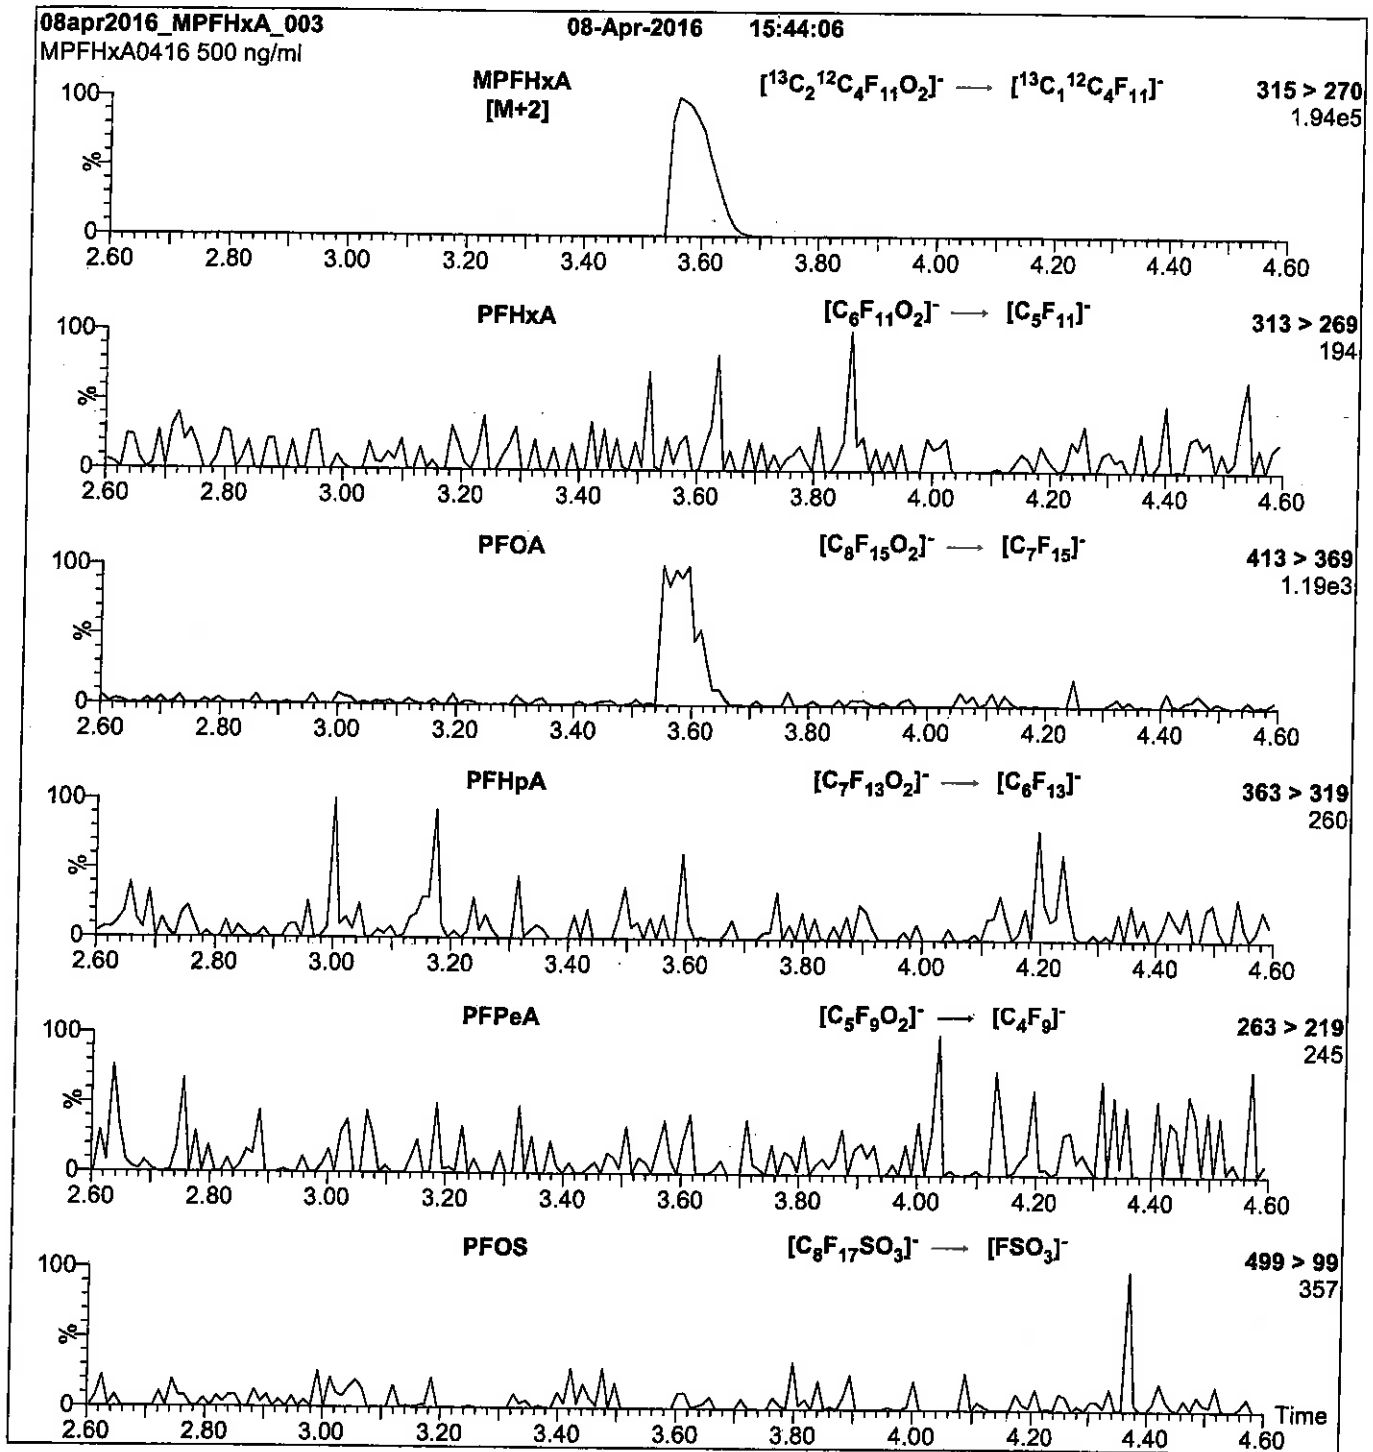

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml MPFHxA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.39e-3
Collision Energy (eV) = 10

Reagent

LCMPFHXS_00008

R: 800 9/22/16



739601

ID: LCMPFHxS_00008

Exp: 10/23/20 Prod: SBC

18O2-Perfluorohexanesulfo



WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION


Scanned 10/14/16 SK

PRODUCT CODE: MPFHxS
COMPOUND: Sodium perfluoro-1-hexane[¹⁸O₂]sulfonate

LOT NUMBER: MPFHxS1015

STRUCTURE:

CAS #: Not available



MOLECULAR FORMULA: C₆F₁₃S¹⁸O₂¹⁶ONa
CONCENTRATION: 50.0 ± 2.5 µg/ml (Na salt)
47.3 ± 2.4 µg/ml (MPFHxS anion)
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 10/23/2015
EXPIRY DATE: (mm/dd/yyyy) 10/23/2020
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

MOLECULAR WEIGHT: 426.10
SOLVENT(S): Methanol
ISOTOPIC PURITY: >94% (¹⁸O₂)


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- The response factor for MPFHxS (C₆F₁₃S¹⁸O₂¹⁶O) has been observed to be up to 10% lower than for PFHxS (C₆F₁₃S¹⁶O₃) when both compounds are injected together. This difference may vary between instruments.
- Due to the isotopic purity of the starting material (¹⁸O₂ >94%), MPFHxS contains ~ 0.3% of PFHxS. This value agrees with the theoretical percent relative abundance that is expected based on the stated isotopic purity.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim
Date: 10/28/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFHxS; LC/MS Data (TIC and Mass Spectrum)

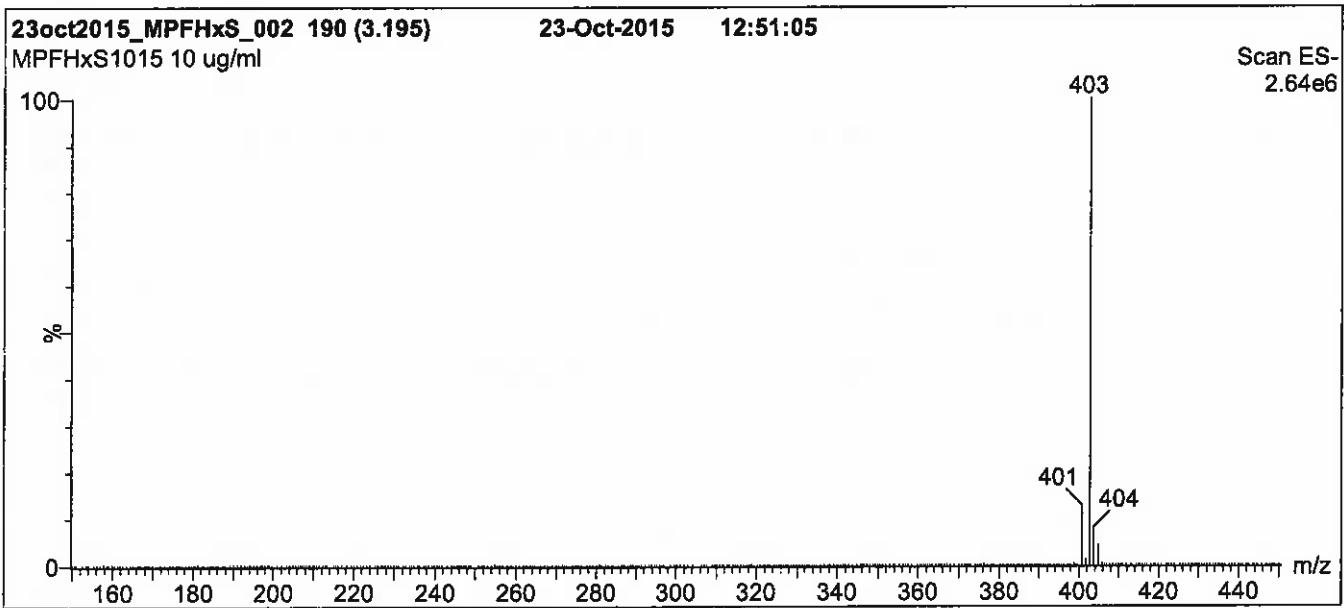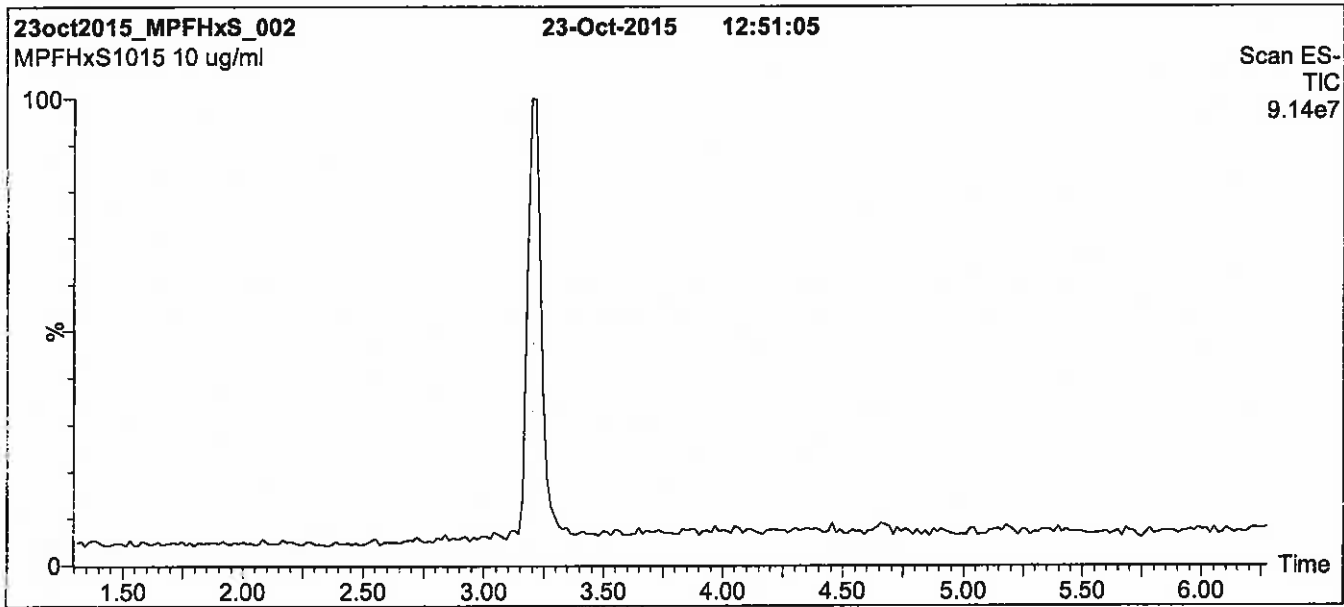

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 2 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 50.00
Cone Gas Flow (l/hr) = 60
Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFHxS; LC/MS/MS Data (Selected MRM Transitions)

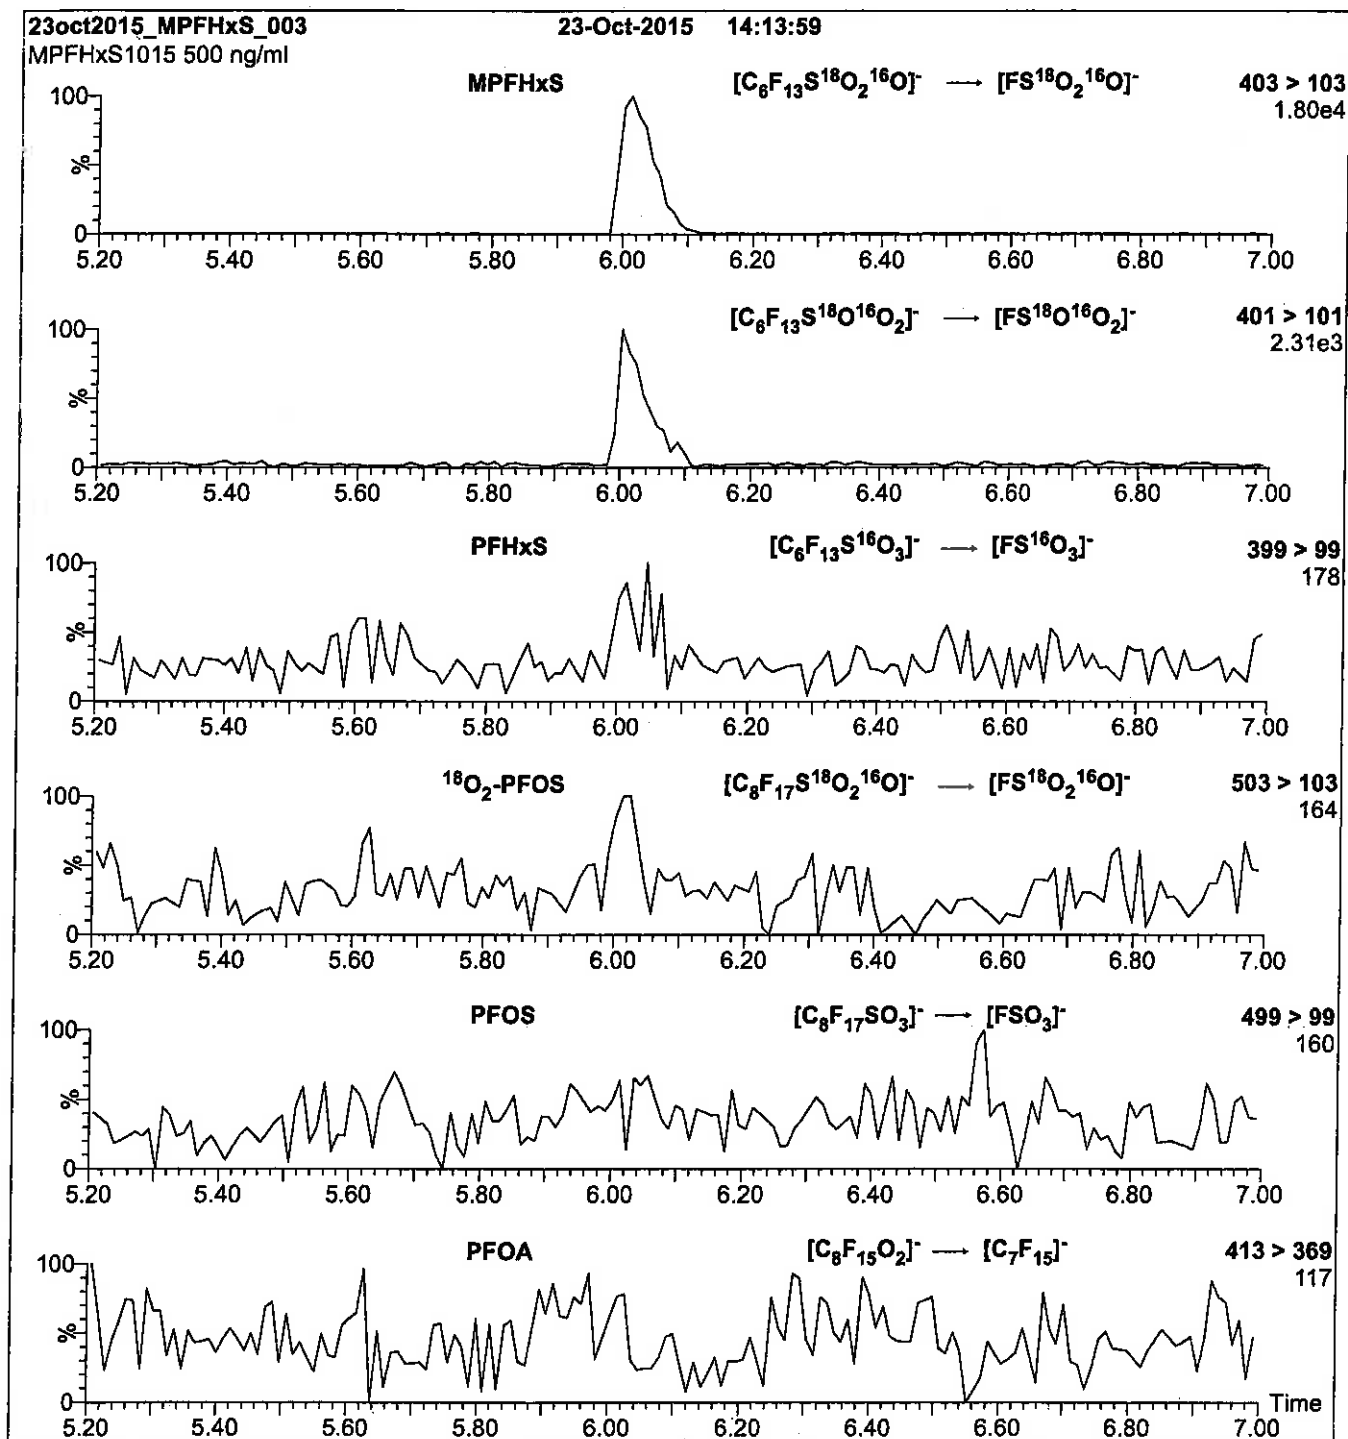

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml MPFHxS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.35e-3
Collision Energy (eV) = 30

Reagent

LCMPFNA_00008

Scanned 10/14/16 R: SBC 9/22/16



739637
ID: LCM:PFNA_0008
Exp: 04/13/19 Pppl: SBC
13C5-Perfluoronoic aci




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFNA **LOT NUMBER:** MPFNA0414
COMPOUND: Perfluoro-n-[1,2,3,4,5-¹³C₅]nonanoic acid

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: ¹³C₅¹²C₄HF₁₇O₂ **MOLECULAR WEIGHT:** 469.04
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Methanol
Water (<1%)
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥99%¹³C
(1,2,3,4,5-¹³C₅)
LAST TESTED: (mm/dd/yyyy) 04/13/2014
EXPIRY DATE: (mm/dd/yyyy) 04/13/2019
RECOMMENDED STORAGE: Store ampoule in a cool, dark place


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 04/01/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFNA; LC/MS Data (TIC and Mass Spectrum)

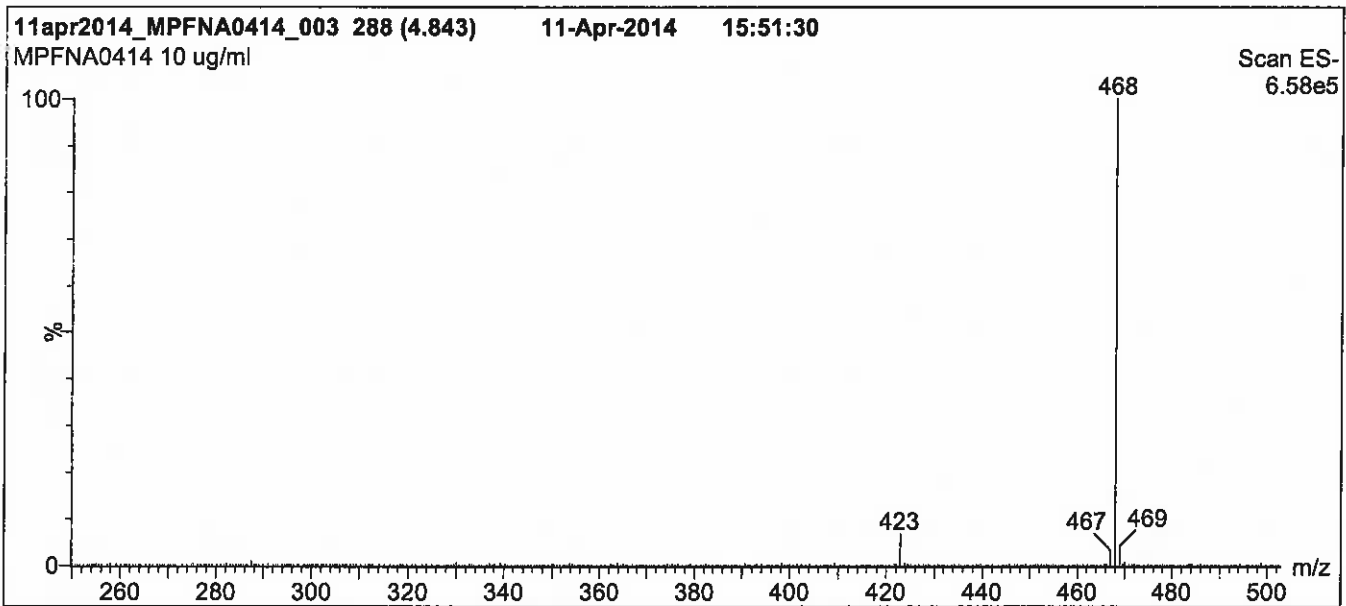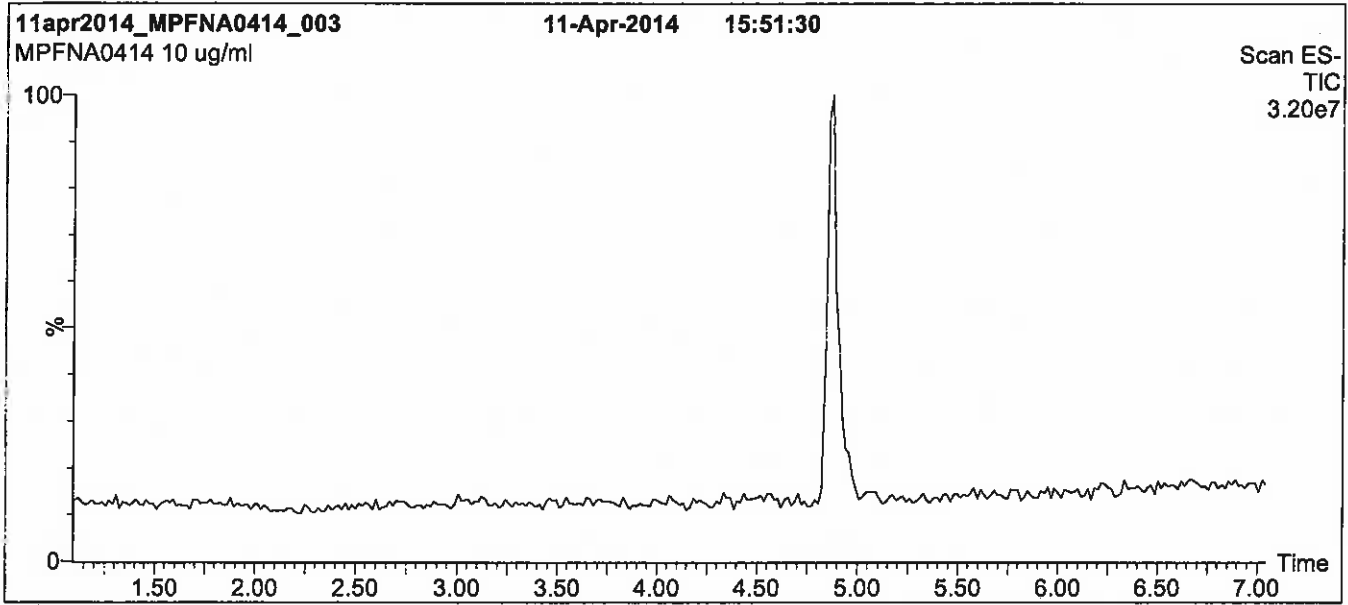

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 50% (80:20 MeOH:ACN) / 50% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 2 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (250 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.00
 Cone Voltage (V) = 15.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFNA; LC/MS/MS Data (Selected MRM Transitions)

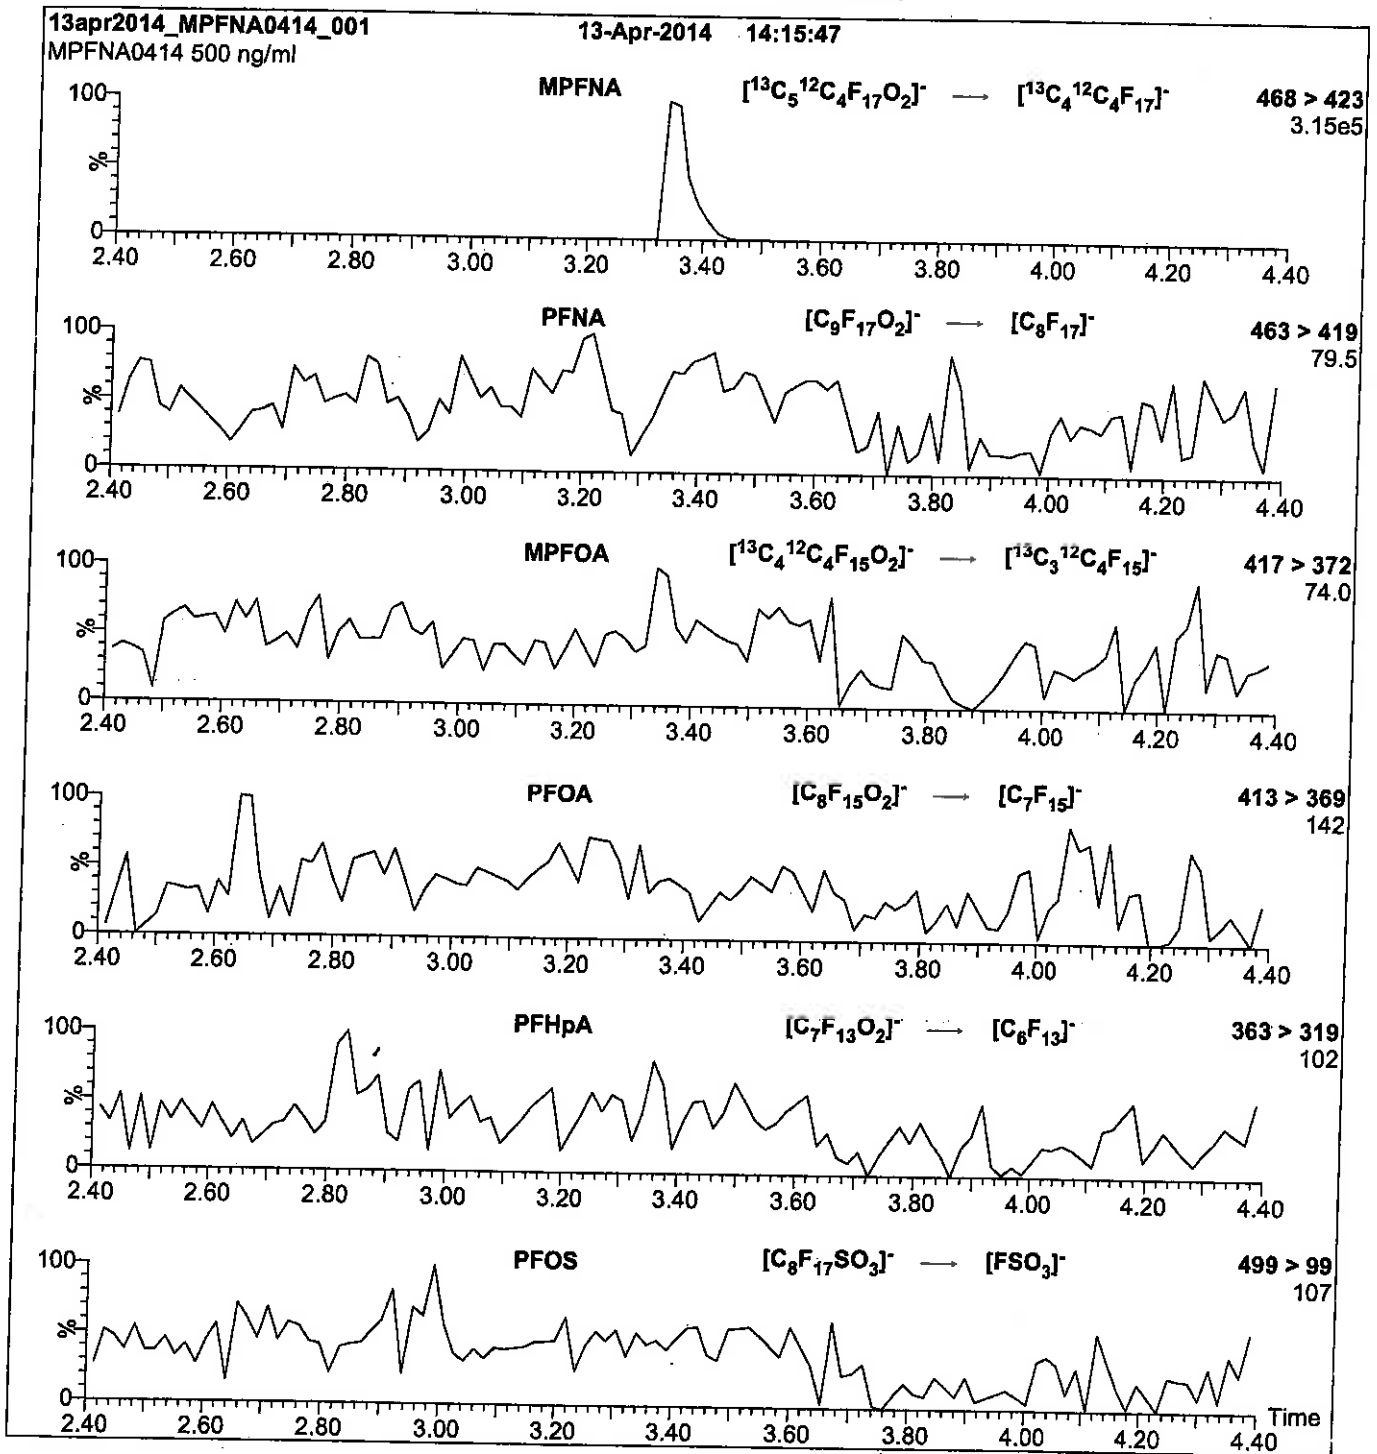

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml MPFNA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.28e-3
Collision Energy (eV) = 11

Reagent

LCMPFOA_00012

R: SBC 9/22/16



738683
ID: LCMFOA_00012
Exp: 01/22/21 Prep: SBC
13C4-Perfluorooctanoic ac




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFOA
COMPOUND: Perfluoro-n-[1,2,3,4-¹³C₄]octanoic acid

LOT NUMBER: MPFOA0116

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: ¹³C₄¹²C₄HF₁₅O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 418.04
SOLVENT(S): Methanol
Water (<1%)
ISOTOPIC PURITY: ≥99% ¹³C
(1,2,3,4-¹³C₄)

CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 01/22/2016
EXPIRY DATE: (mm/dd/yyyy) 01/22/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains ~ 0.1% of native perfluoro-n-octanoic acid (PFOA).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim
Date: 02/01/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.


QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 2: MPFOA; LC/MS/MS Data (Selected MRM Transitions)

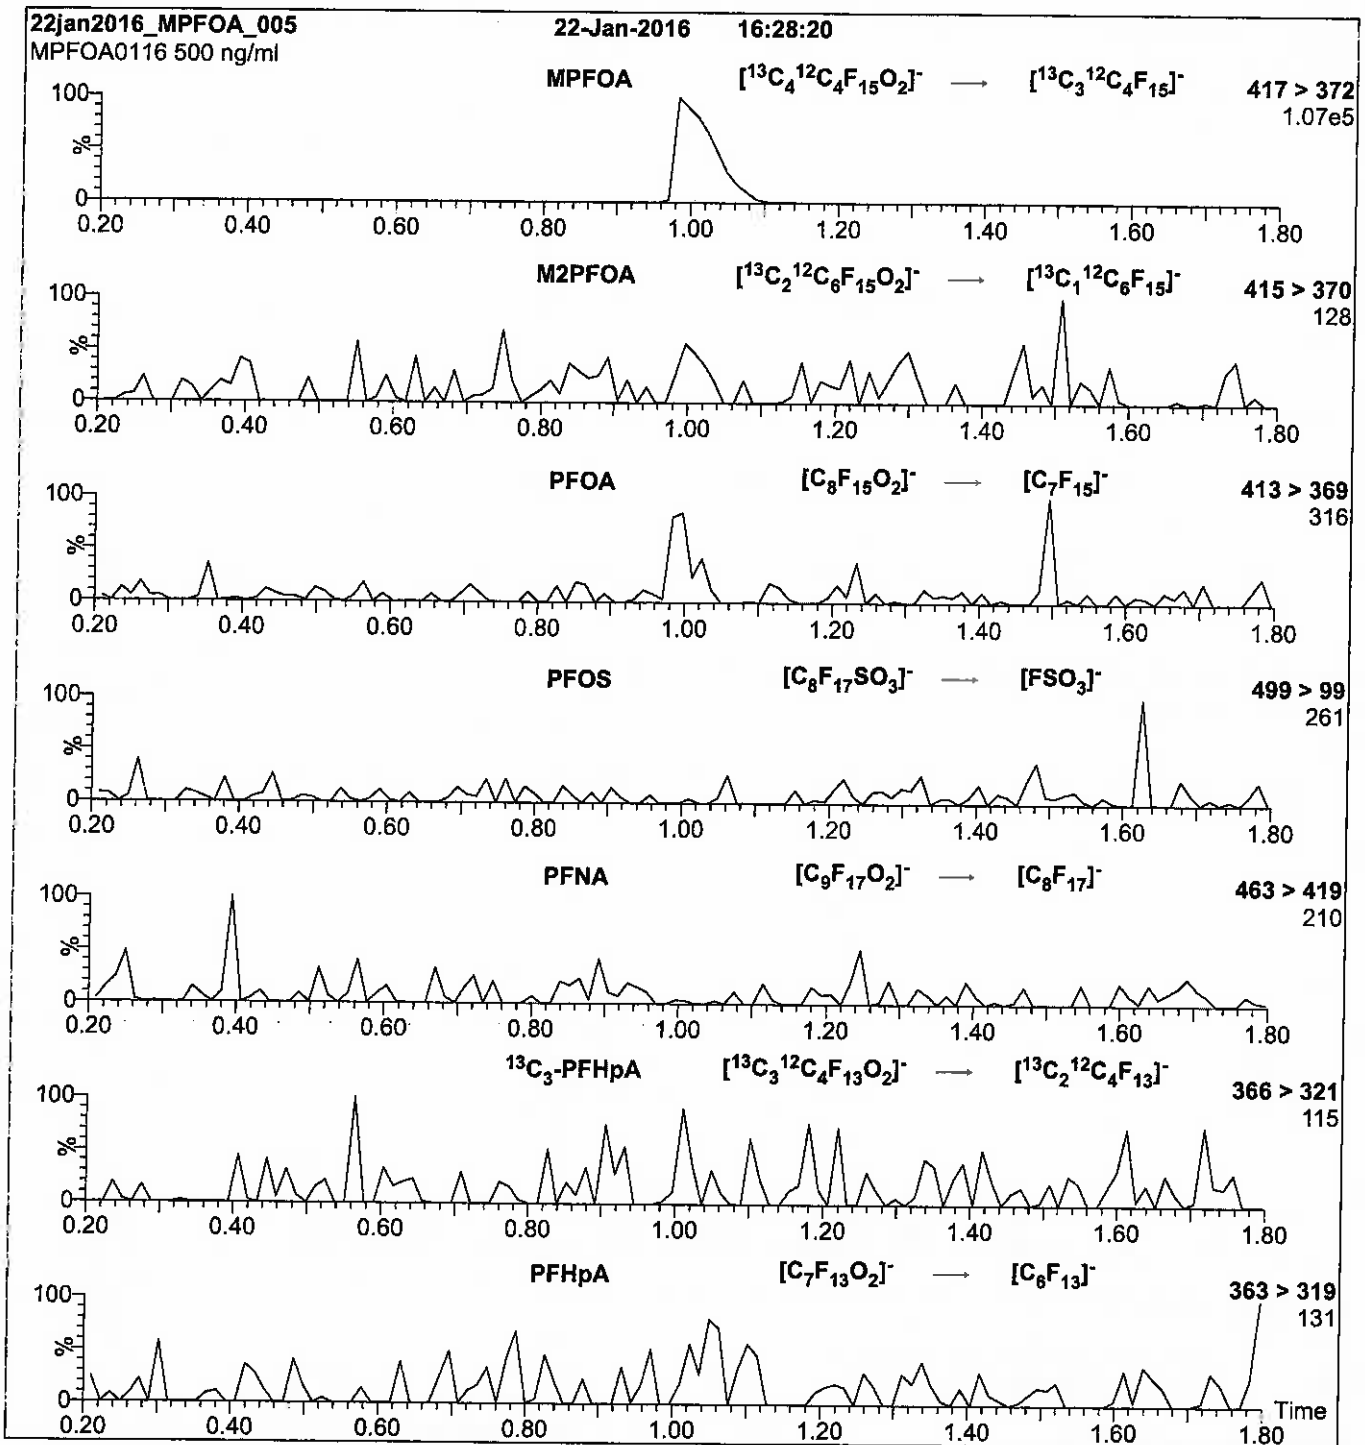

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml MPFOA)


Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.58e-3
Collision Energy (eV) = 10

Figure 2: MPFOA; LC/MS/MS Data (Selected MRM Transitions)

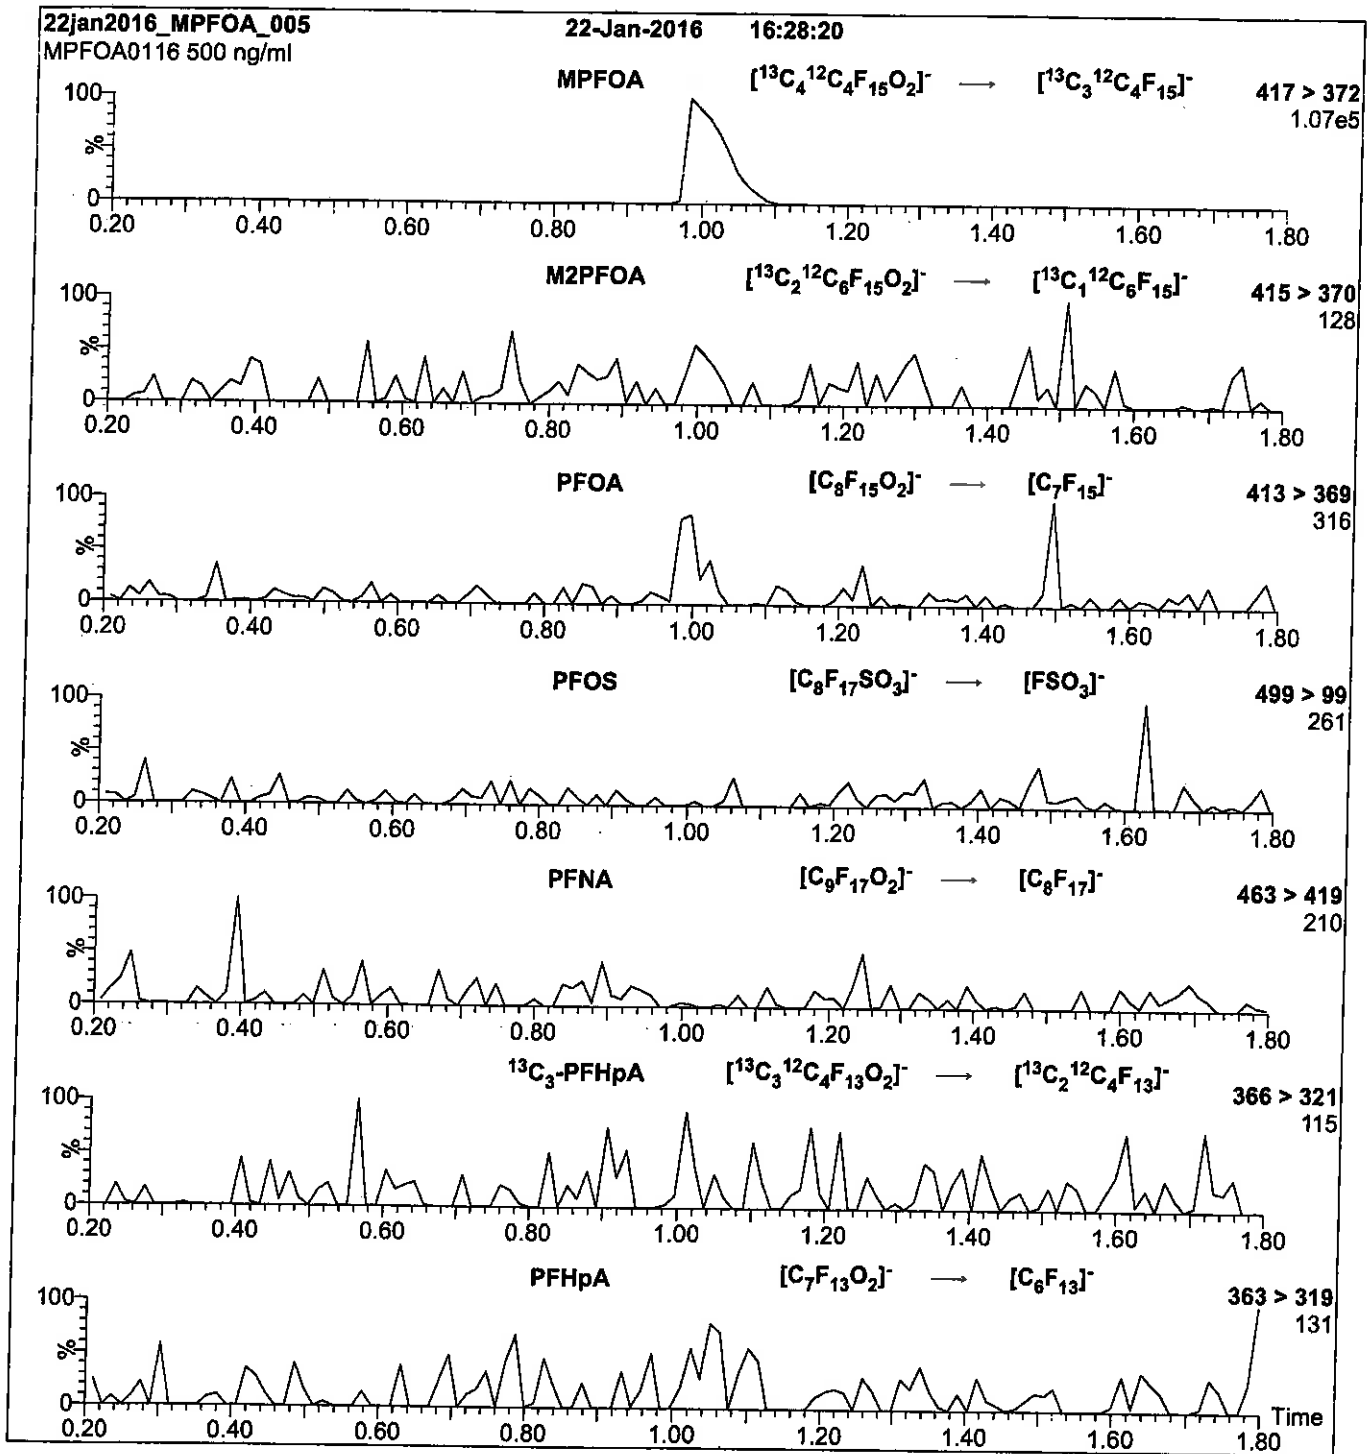

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml MPFOA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.58e-3
Collision Energy (eV) = 10

Reagent

LCMPFOS_00017

R: 9/9/16 802

728309
ID: LCMPPFOS_00017
Exp: 08/03/21 Prpd: SBC
13C4-Perfluorooctanesulfo




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFOS **LOT NUMBER:** MPFOS0816
COMPOUND: Sodium perfluoro-1-[1,2,3,4-¹³C₄]octanesulfonate

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA:	¹³ C ₄ ¹² C ₄ F ₁₇ SO ₃ Na	MOLECULAR WEIGHT:	526.08
CONCENTRATION:	50.0 ± 2.5 µg/ml (Na salt) 47.8 ± 2.4 µg/ml (MPFOS anion)	SOLVENT(S):	Methanol
CHEMICAL PURITY:	>98%	ISOTOPIC PURITY:	≥99% ¹³ C (1,2,3,4- ¹³ C ₄)
LAST TESTED: (mm/dd/yyyy)	08/03/2016		
EXPIRY DATE: (mm/dd/yyyy)	08/03/2021		
RECOMMENDED STORAGE:	Store ampoule in a cool, dark place		


DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains ~ 0.8% Sodium perfluoro-1-[1,2,3-¹³C₃]heptanesulfonate.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 08/05/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFOS; LC/MS Data (TIC and Mass Spectrum)

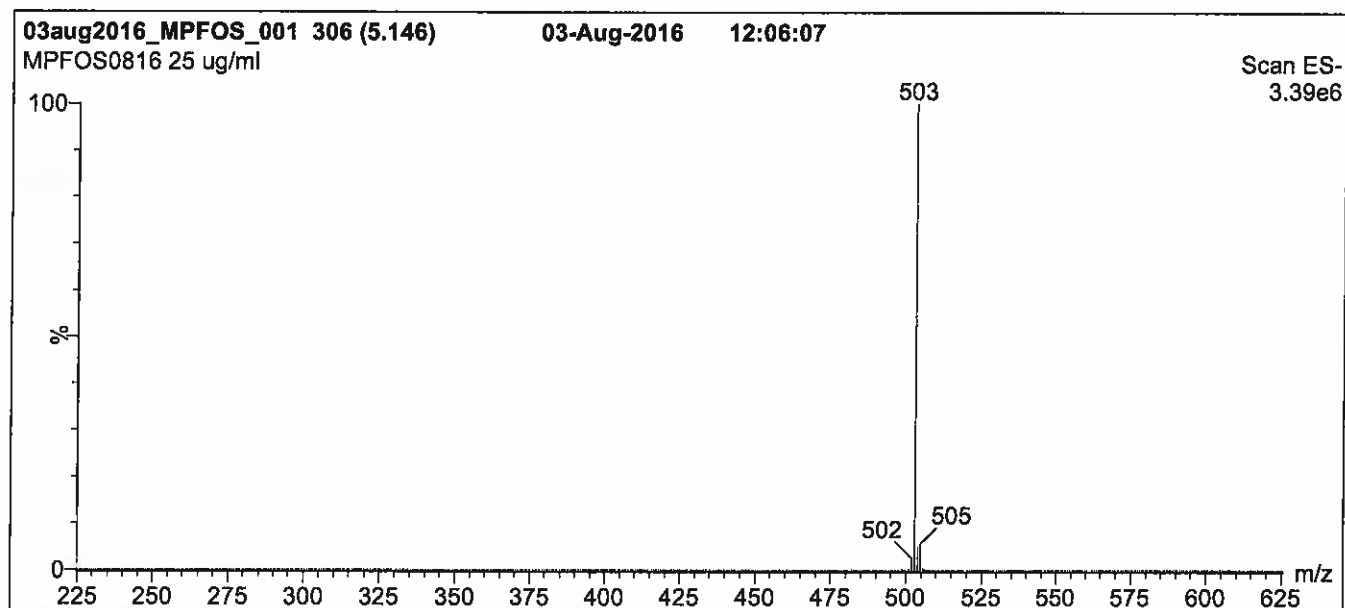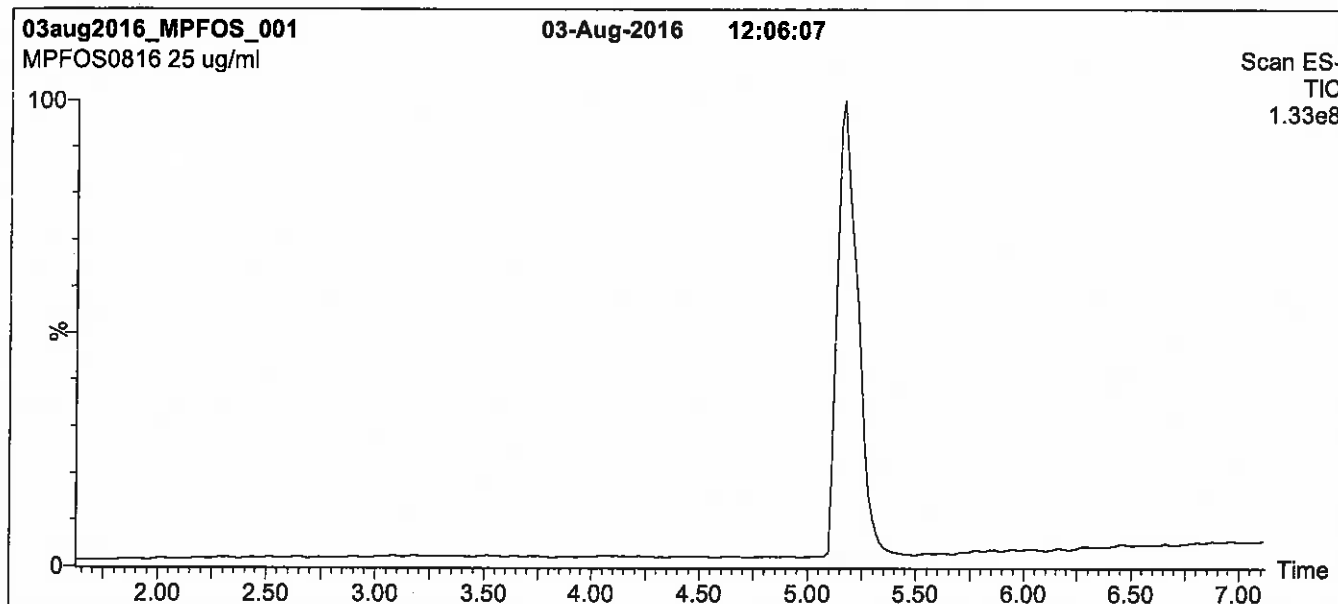

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 45% (80:20 MeOH:ACN) / 55% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 60.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFOS; LC/MS/MS Data (Selected MRM Transitions)

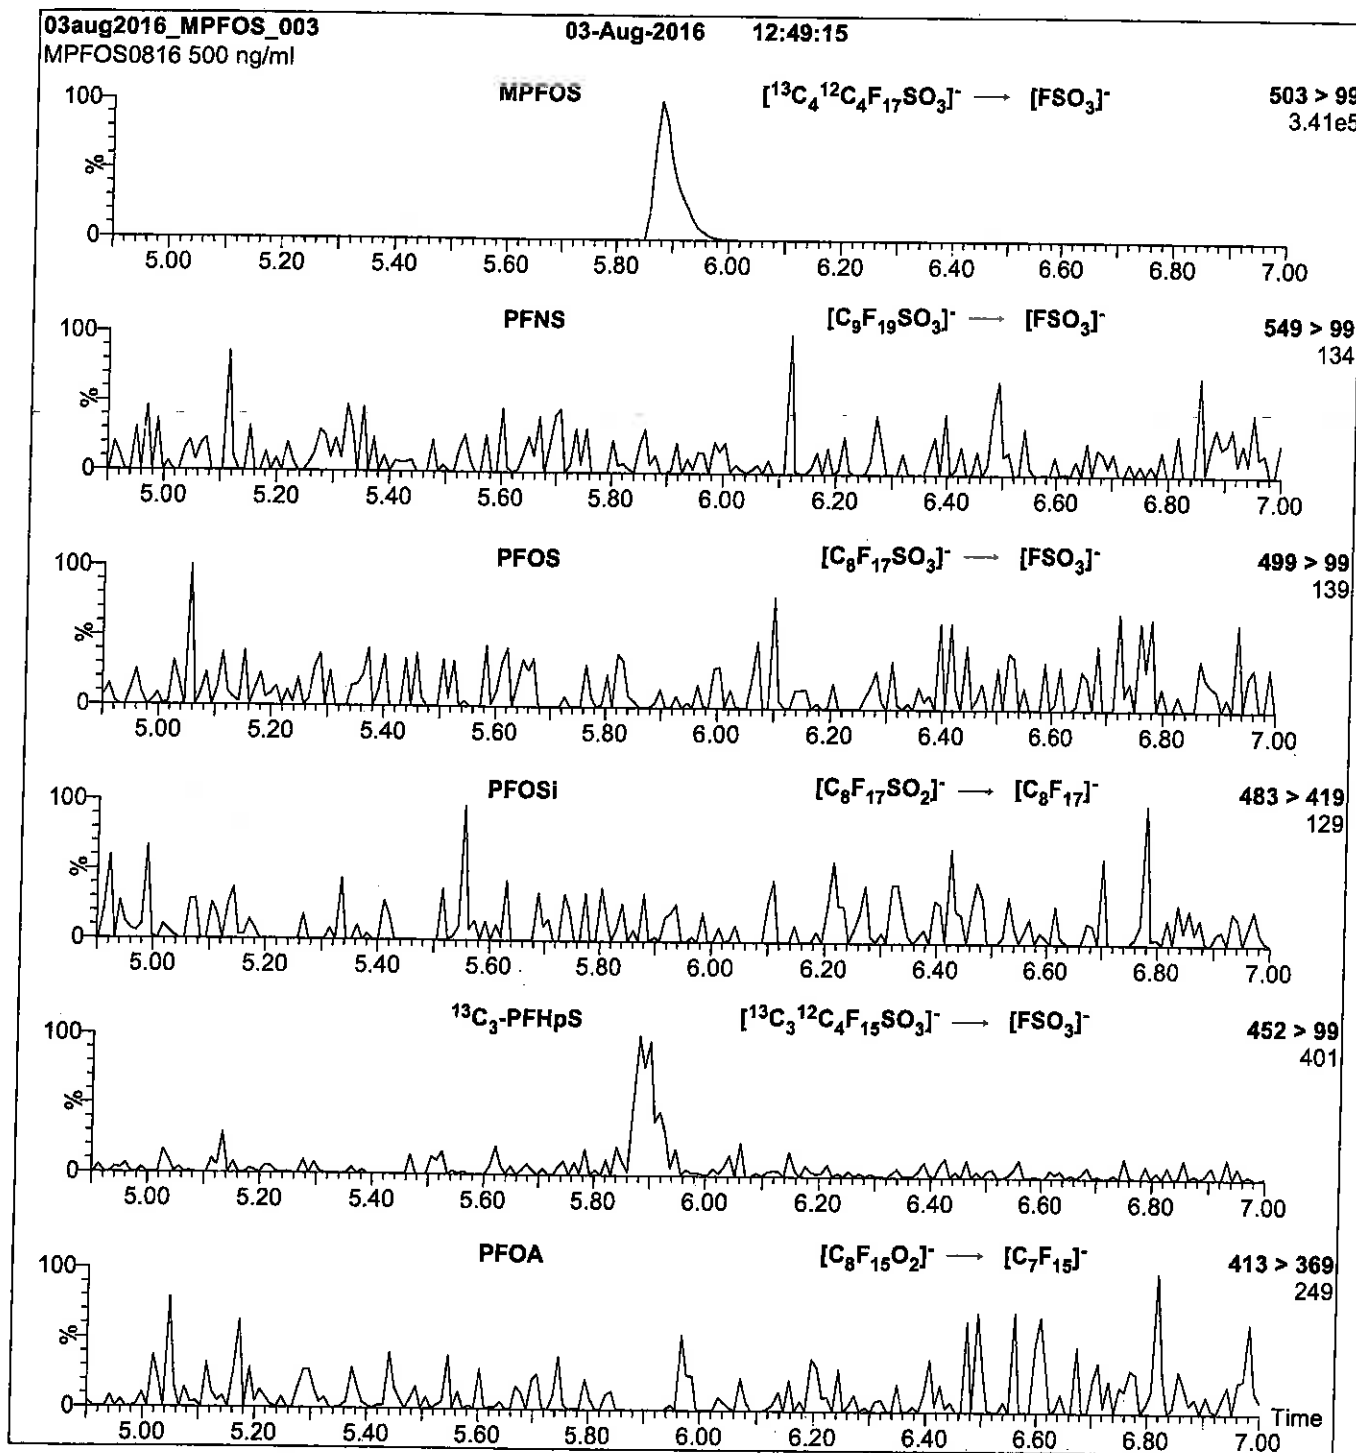

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml MPFOS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.46e-3
Collision Energy (eV) = 40

Reagent

LCMPFUdA_00009

R: SBC 9/22/16

739604
ID: LCMPFUdA_00009
Exp: 02/12/21 Prod: SBC
13C2-Perfluoroundecanoic




WELLINGTON
LABORATORIES

CERTIFICATE OF ANALYSIS
DOCUMENTATION

Scanned 10/14/16 SRC

PRODUCT CODE: MPFUdA **LOT NUMBER:** MPFUdA0216
COMPOUND: Perfluoro-n-[1,2-¹³C₂]undecanoic acid
STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: ¹³C₂¹²C₉HF₂₁O₂ **MOLECULAR WEIGHT:** 566.08
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Methanol
Water (<1%)
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥99% ¹³C
(1,2-¹³C₂)
LAST TESTED: (mm/dd/yyyy) 02/12/2016
EXPIRY DATE: (mm/dd/yyyy) 02/12/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Presence of 1-¹³C₁-PFUdA (~1%; see Figure 2), 2-¹³C₁-PFUdA (~1%), and PFUdA (~0.2%; see Figure 2) are due to the isotopic purity of the ¹³C-precursor.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 02/24/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFUdA; LC/MS Data (TIC and Mass Spectrum)

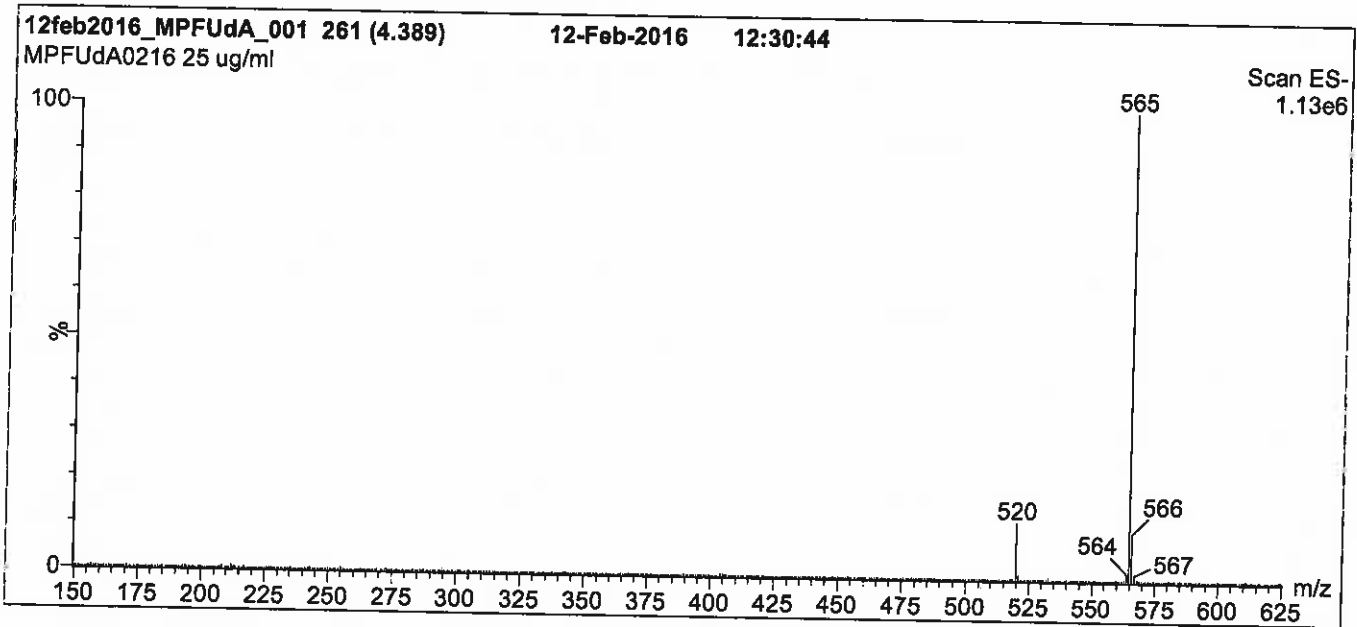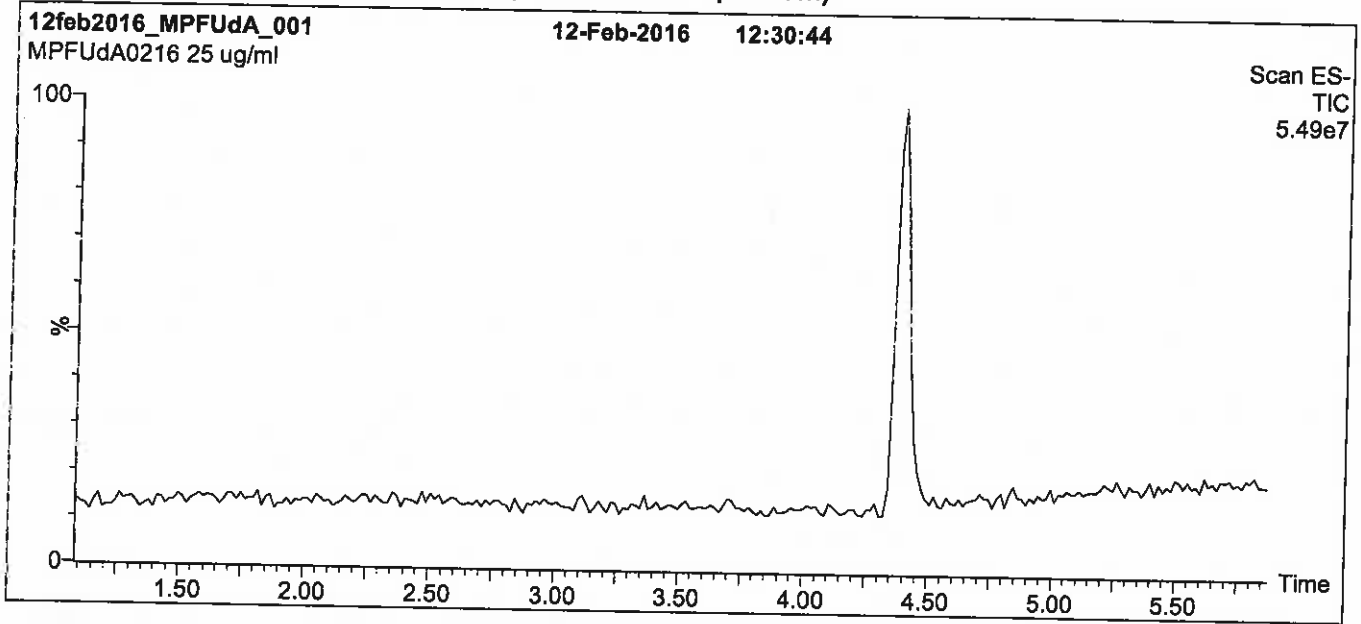

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 60% (80:20 MeOH:ACN) / 40% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for
 1.5 min before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 15.00
 Cone Gas Flow (l/hr) = 65
 Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFUdA; LC/MS/MS Data (Selected MRM Transitions)

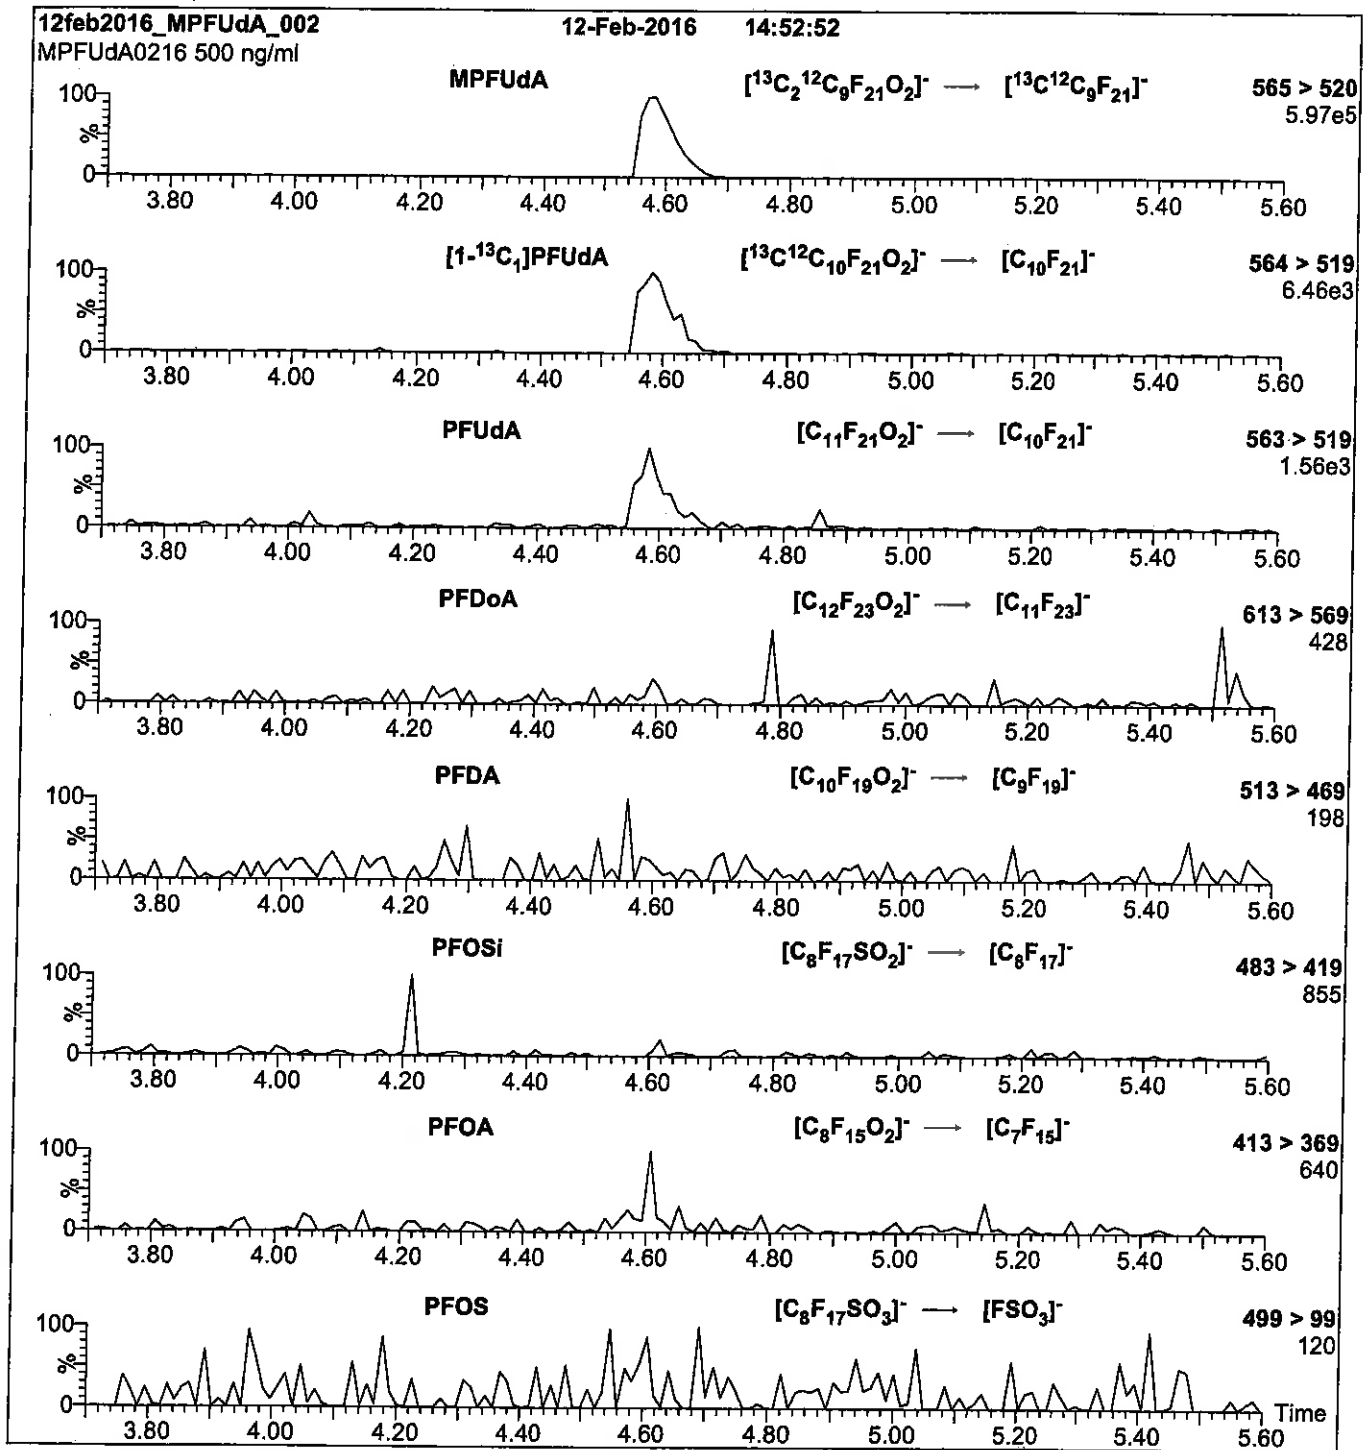

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml MPFUdA)

Mobile phase: Isocratic 80% MeOH / 20% H_2O

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.35e-3
Collision Energy (eV) = 11

Reagent

LCN-EtFOSA-M_00002

P: 7/16/15 SW



WELLINGTON LABORATORIES


CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: N-EtFOSA-M
COMPOUND: N-ethylperfluoro-1-octanesulfonamide

LOT NUMBER: NEIFOSA0714M

STRUCTURE:

CAS #: 4151-50-2

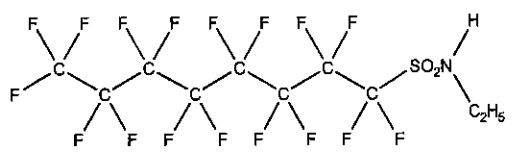

MOLECULAR FORMULA: C₁₀H₆F₁₇NO₂S
CONCENTRATION: 50 ± 2.5 µg/ml
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 07/14/2014
EXPIRY DATE: (mm/dd/yyyy) 07/14/2019
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

MOLECULAR WEIGHT: 527.20
SOLVENT(S): Methanol


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim

Date: 04/01/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: N-EtFOSA-M; LC/MS Data (TIC and Mass Spectrum)

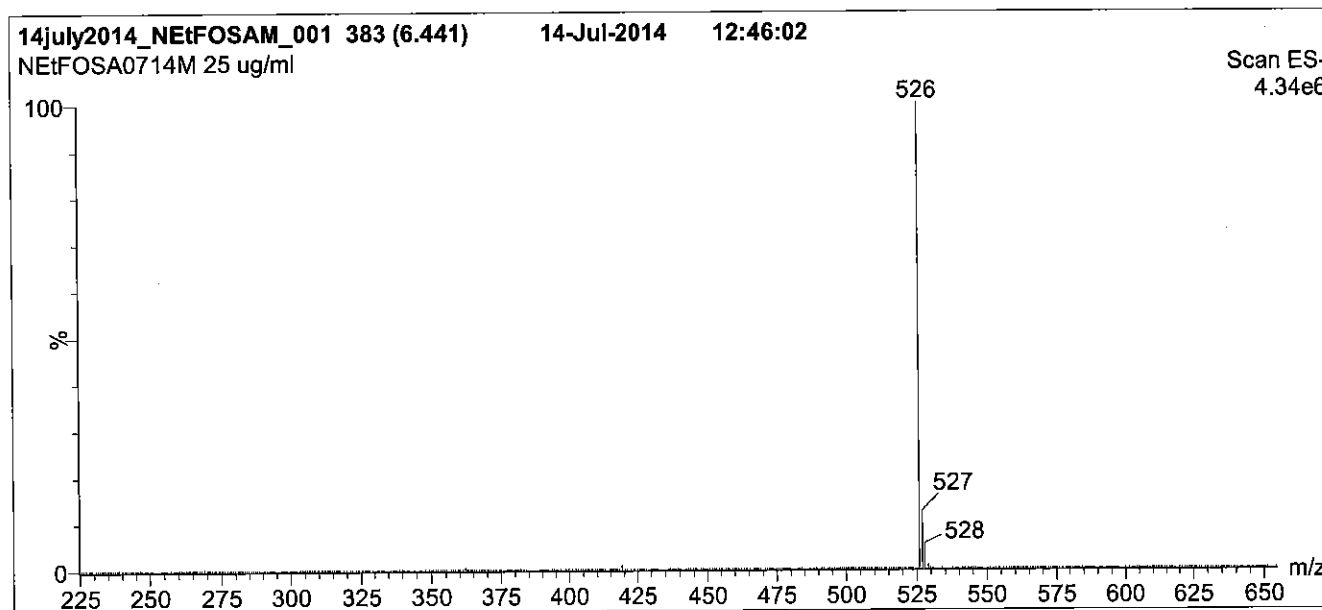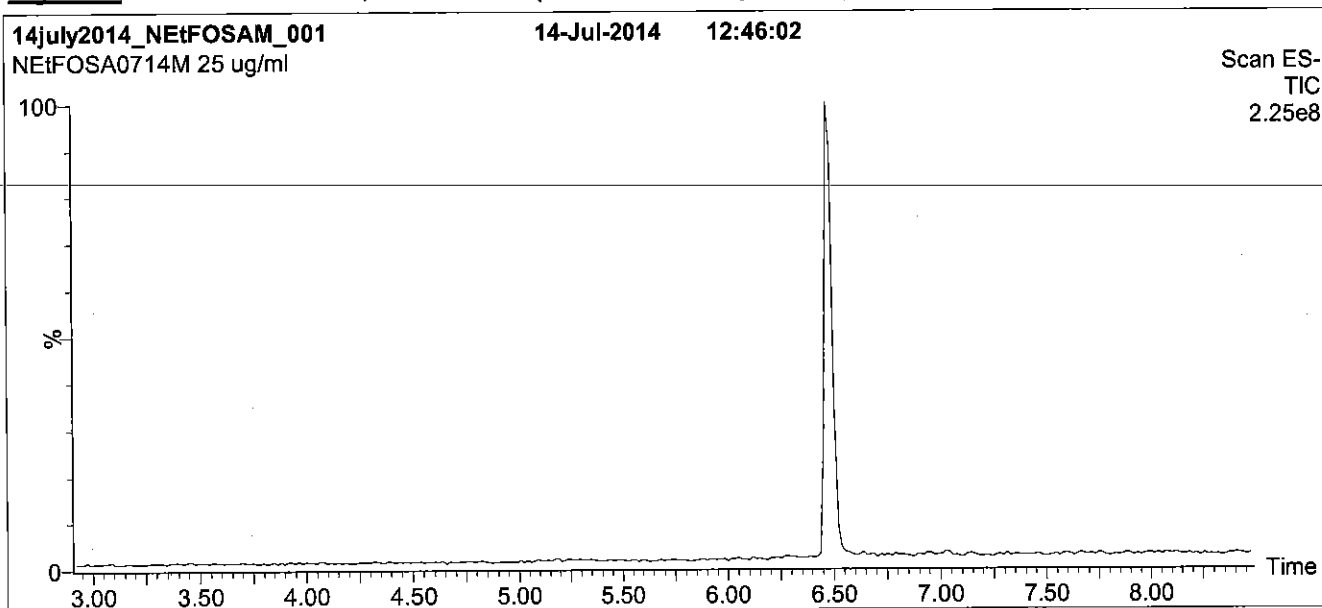

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 45% H₂O / 55% (80:20 MeOH:ACN)
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 2 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 950 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.50
 Cone Voltage (V) = 40.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: N-EtFOSA-M; LC/MS/MS Data (Selected MRM Transitions)

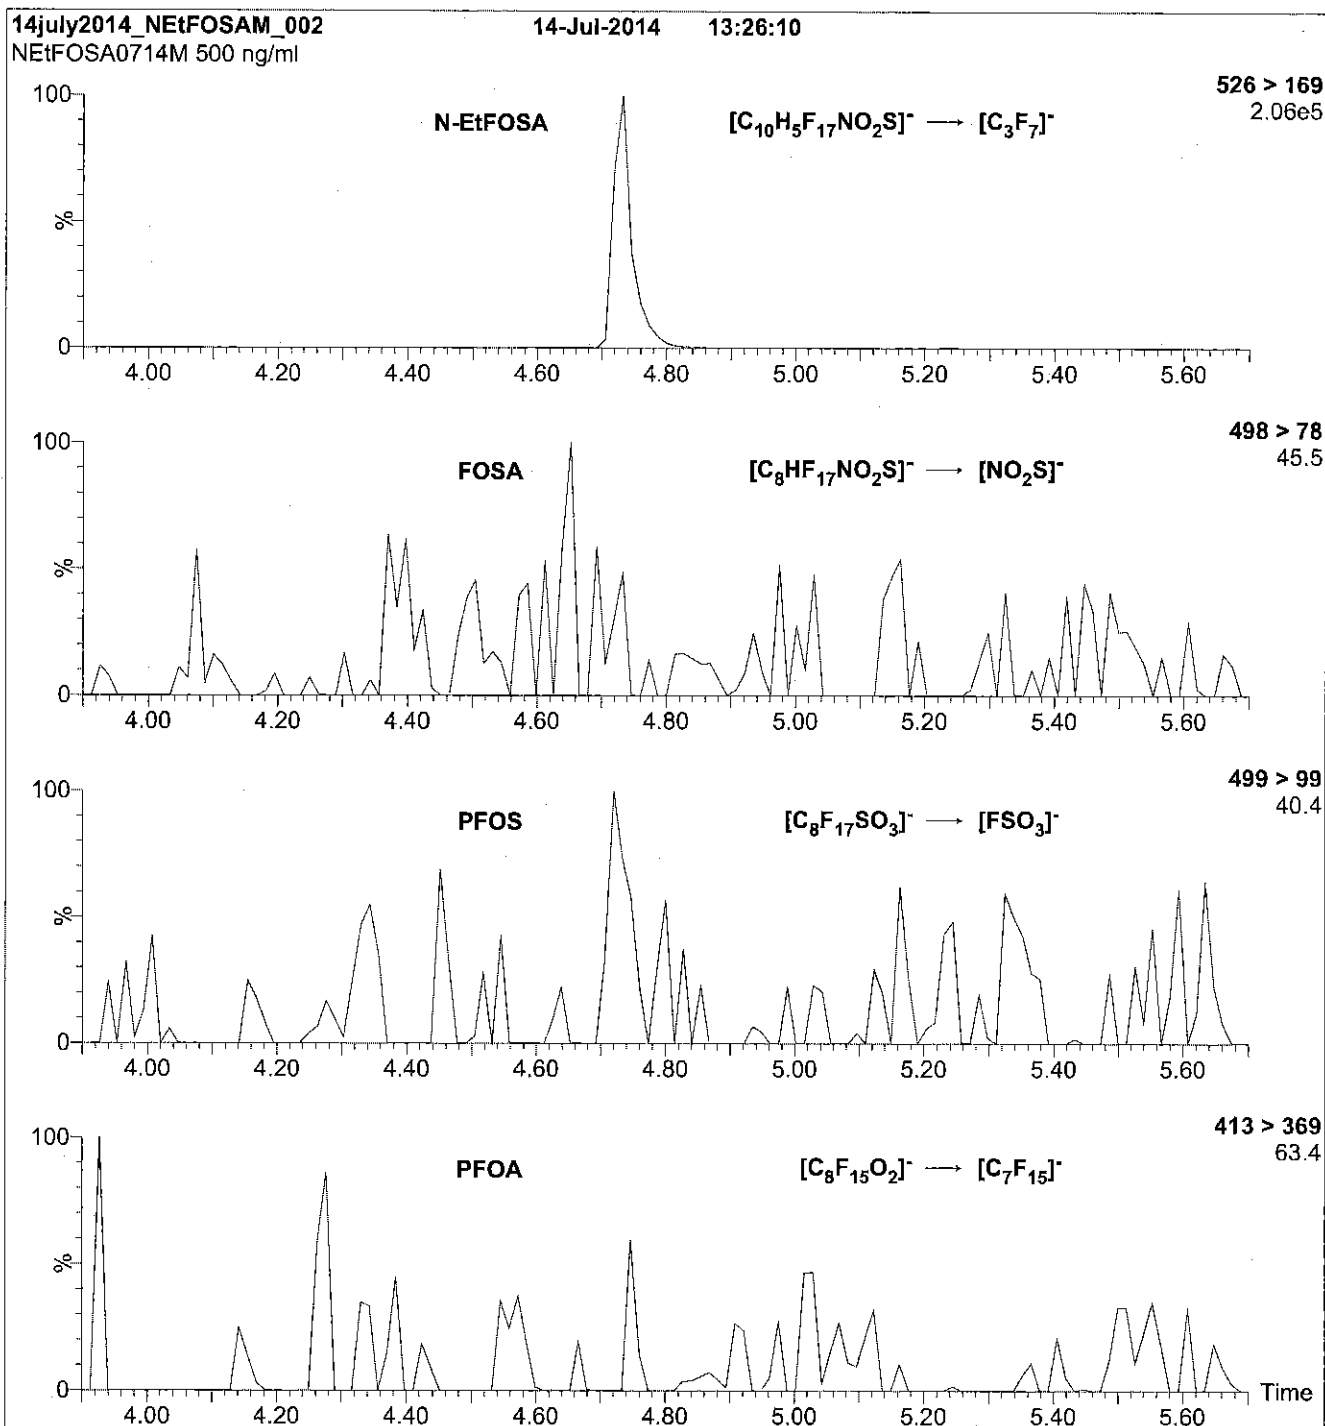

Conditions for Figure 2:

Injection: Direct loop injection
 10 μ l (500 ng/ml N-EtFOSA-M)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.50e-3
 Collision Energy (eV) = 30

Reagent

LCN-EtFOSA-M_00003

R: 8/23/16 SBC



715563
ID: LCN-EtFOSA-M_00003
Exp: 05/24/21 Prpt: SBC
N-EtFOSA-M




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: N-EtFOSA-M **LOT NUMBER:** NEtFOSA0516M
COMPOUND: N-ethylperfluoro-1-octanesulfonamide

STRUCTURE: **CAS #:** 4151-50-2



MOLECULAR FORMULA: C₁₀H₈F₁₇NO₂S **MOLECULAR WEIGHT:** 527.20
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Methanol
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 05/24/2016
EXPIRY DATE: (mm/dd/yyyy) 05/24/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:

B.G. Chittim

Date: 05/27/2016

(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: N-EtFOSA-M; LC/MS Data (TIC and Mass Spectrum)

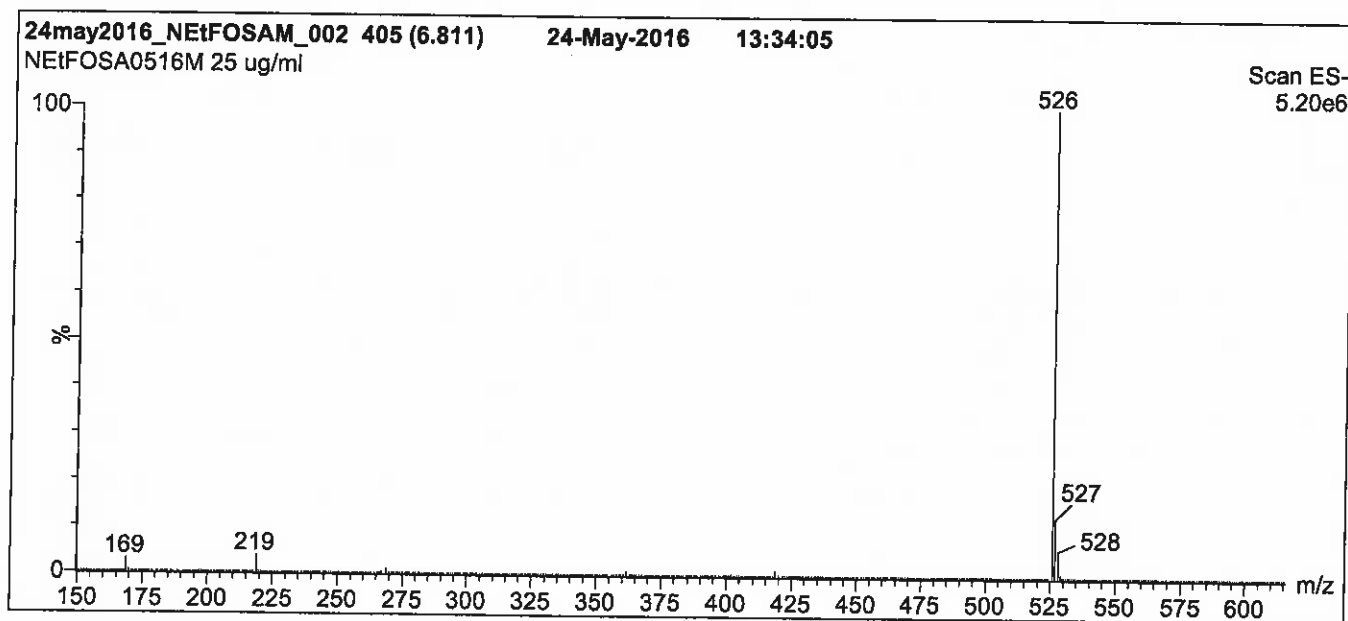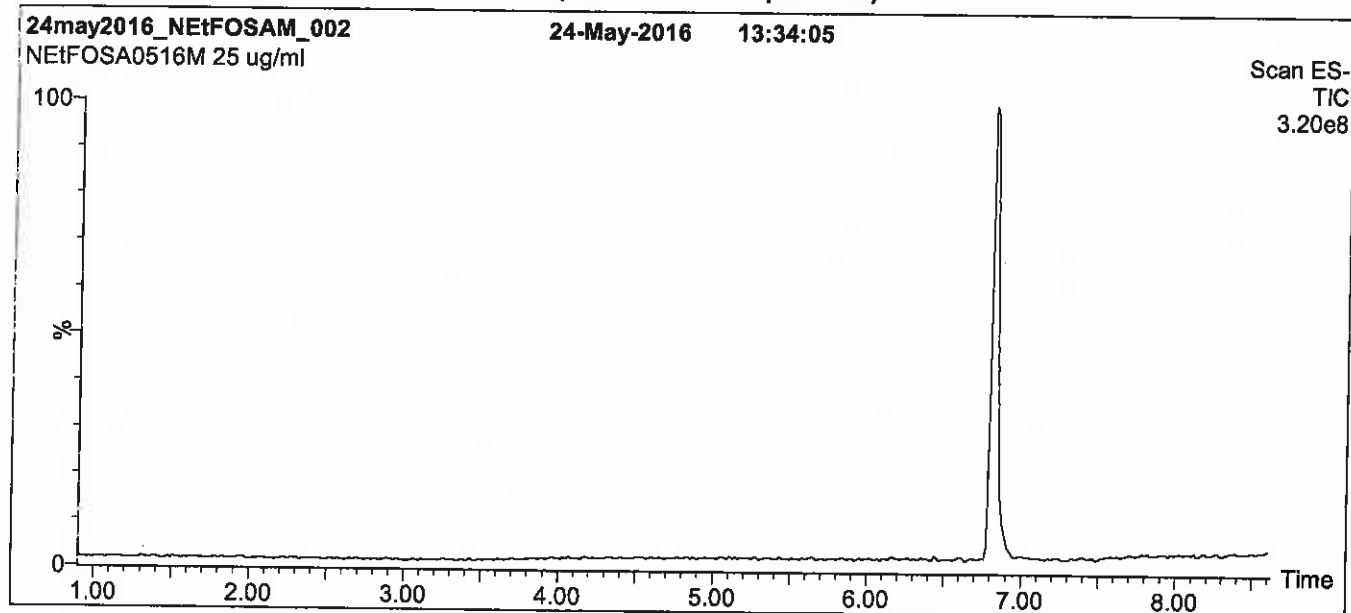

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 45% H₂O / 55% (80:20 MeOH:ACN)
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7.5 min and hold for 1.5 min before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 2.50
Cone Voltage (V) = 40.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: N-EtFOSA-M; LC/MS/MS Data (Selected MRM Transitions)

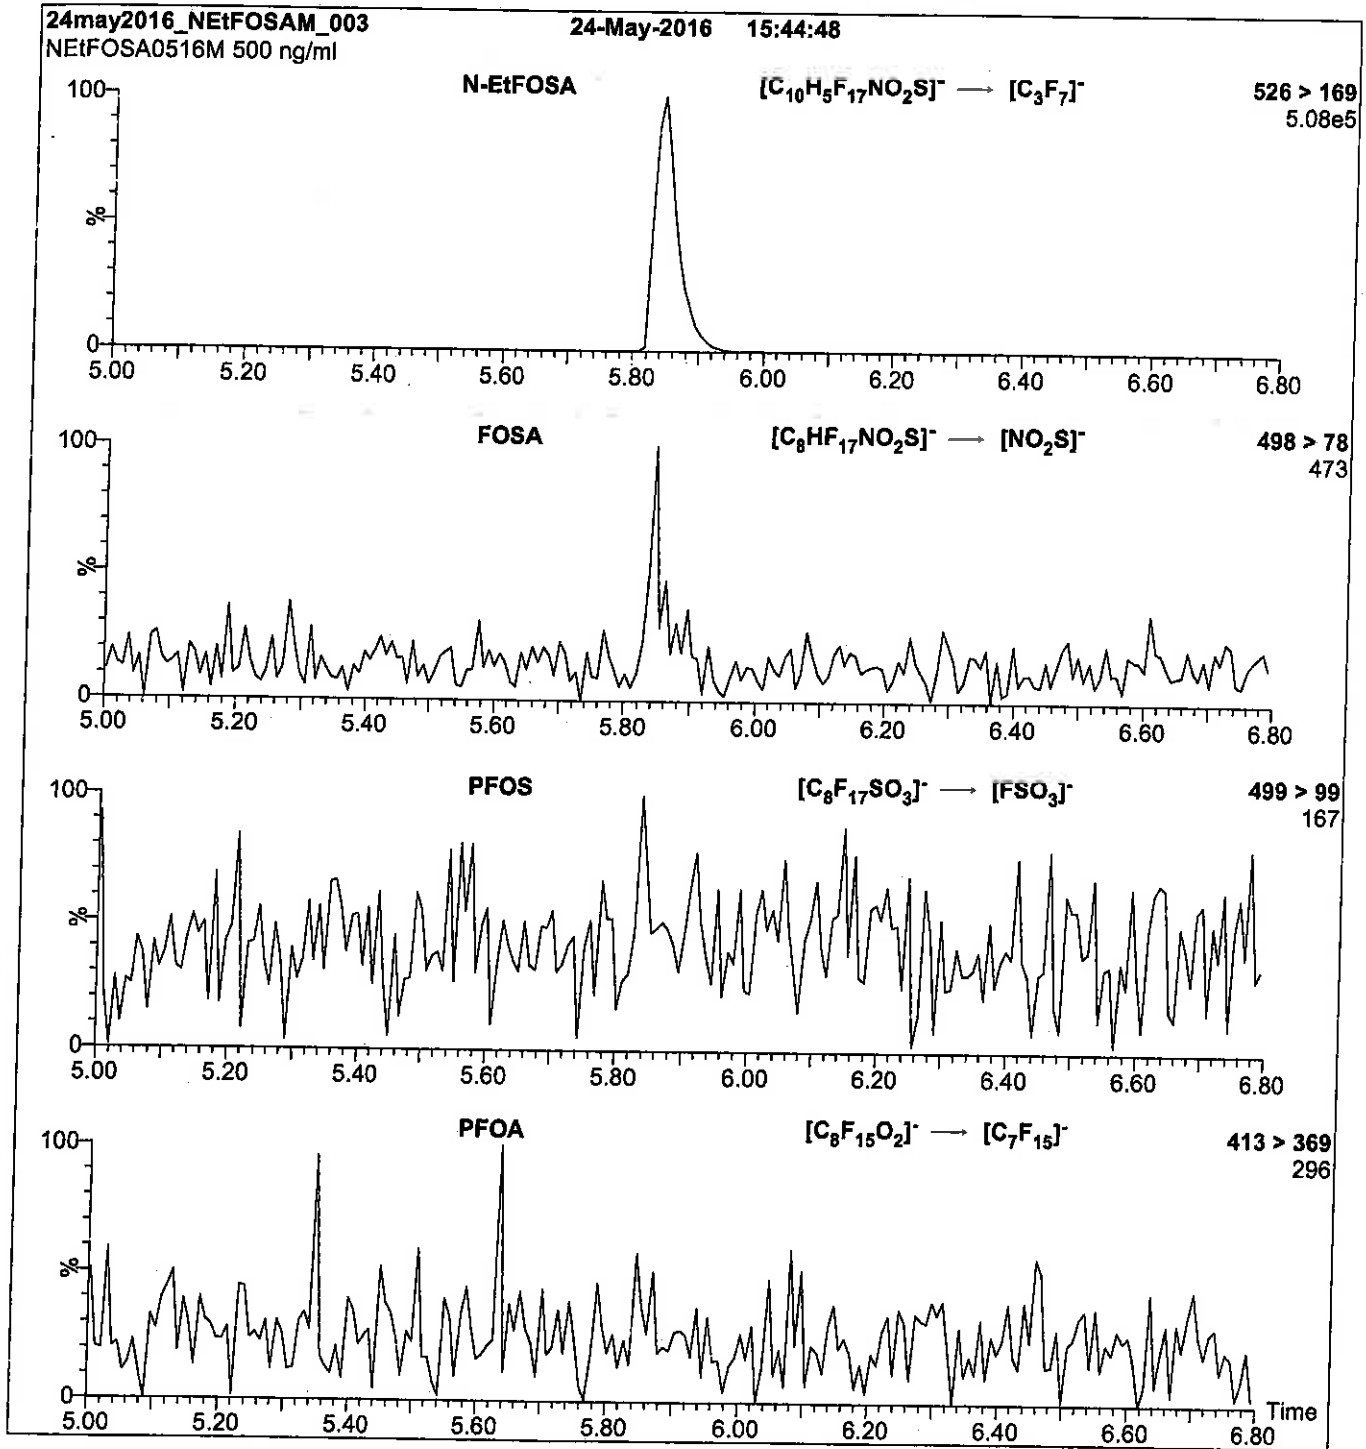

Conditions for Figure 2:

Injection: Direct loop injection
 10 μ l (500 ng/ml N-EtFOSA-M)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)


Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.54e-3
 Collision Energy (eV) = 30

Reagent

LCN-ETFOSAA_00001




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: N-EtFOSAA **LOT NUMBER:** NEtFOSAA0113
COMPOUND: N-ethylperfluoro-1-octanesulfonamidoacetic acid

STRUCTURE: **CAS #:** 2991-50-6

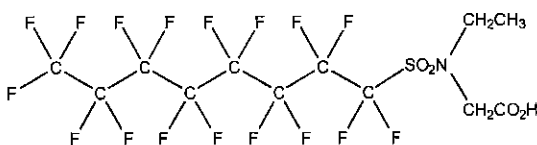

MOLECULAR FORMULA: C₁₂H₈F₁₇NO₄S
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 585.23
SOLVENT(S): Methanol
 Water (<1%)

CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 01/29/2013
EXPIRY DATE: (mm/dd/yyyy) 01/29/2018
RECOMMENDED STORAGE: Refrigerate ampoule

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
 Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent the conversion of the acetic acid moiety to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:


 B.G. Chittim

Date: 04/06/2015
 (mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
 519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: N-EtFOSAA; LC/MS Data (TIC and Mass Spectrum)

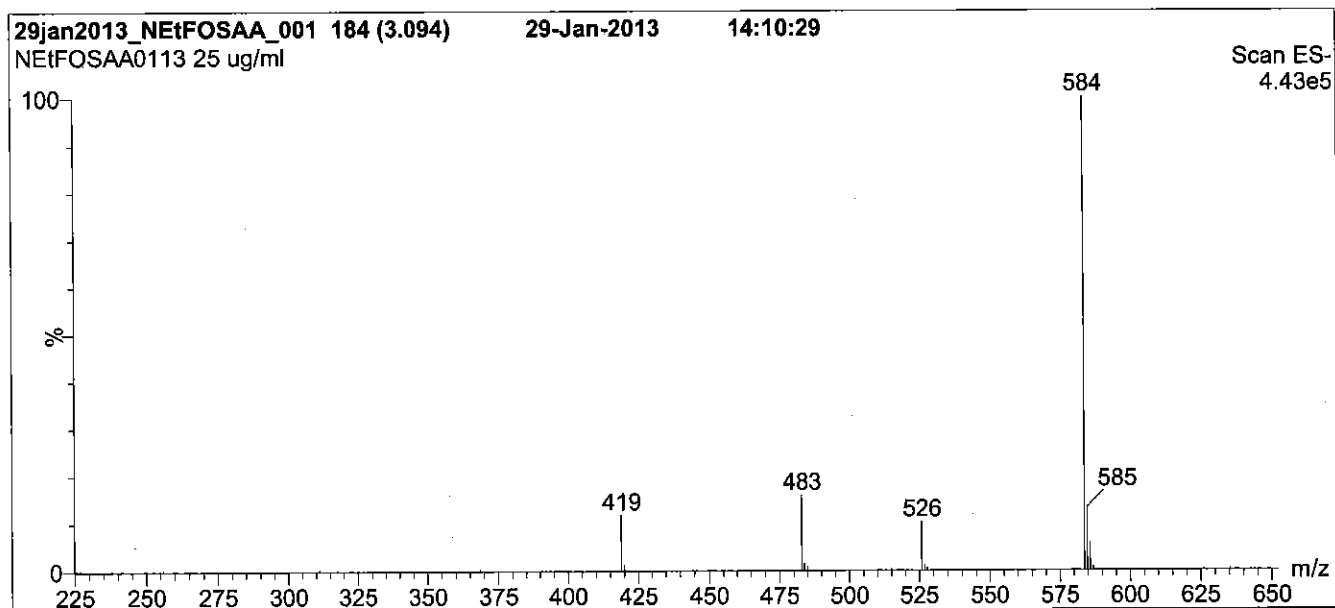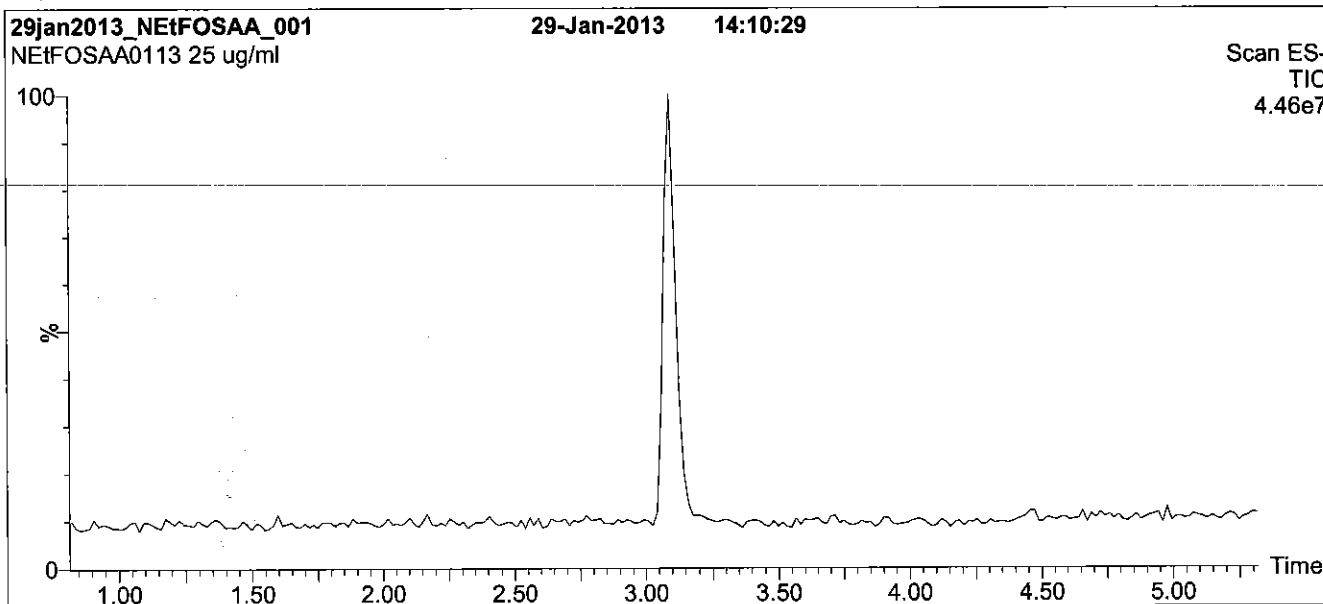

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 65% (80:20 MeOH:ACN) / 35% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 35.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: N-EtFOSAA; LC/MS/MS Data (Selected MRM Transitions)

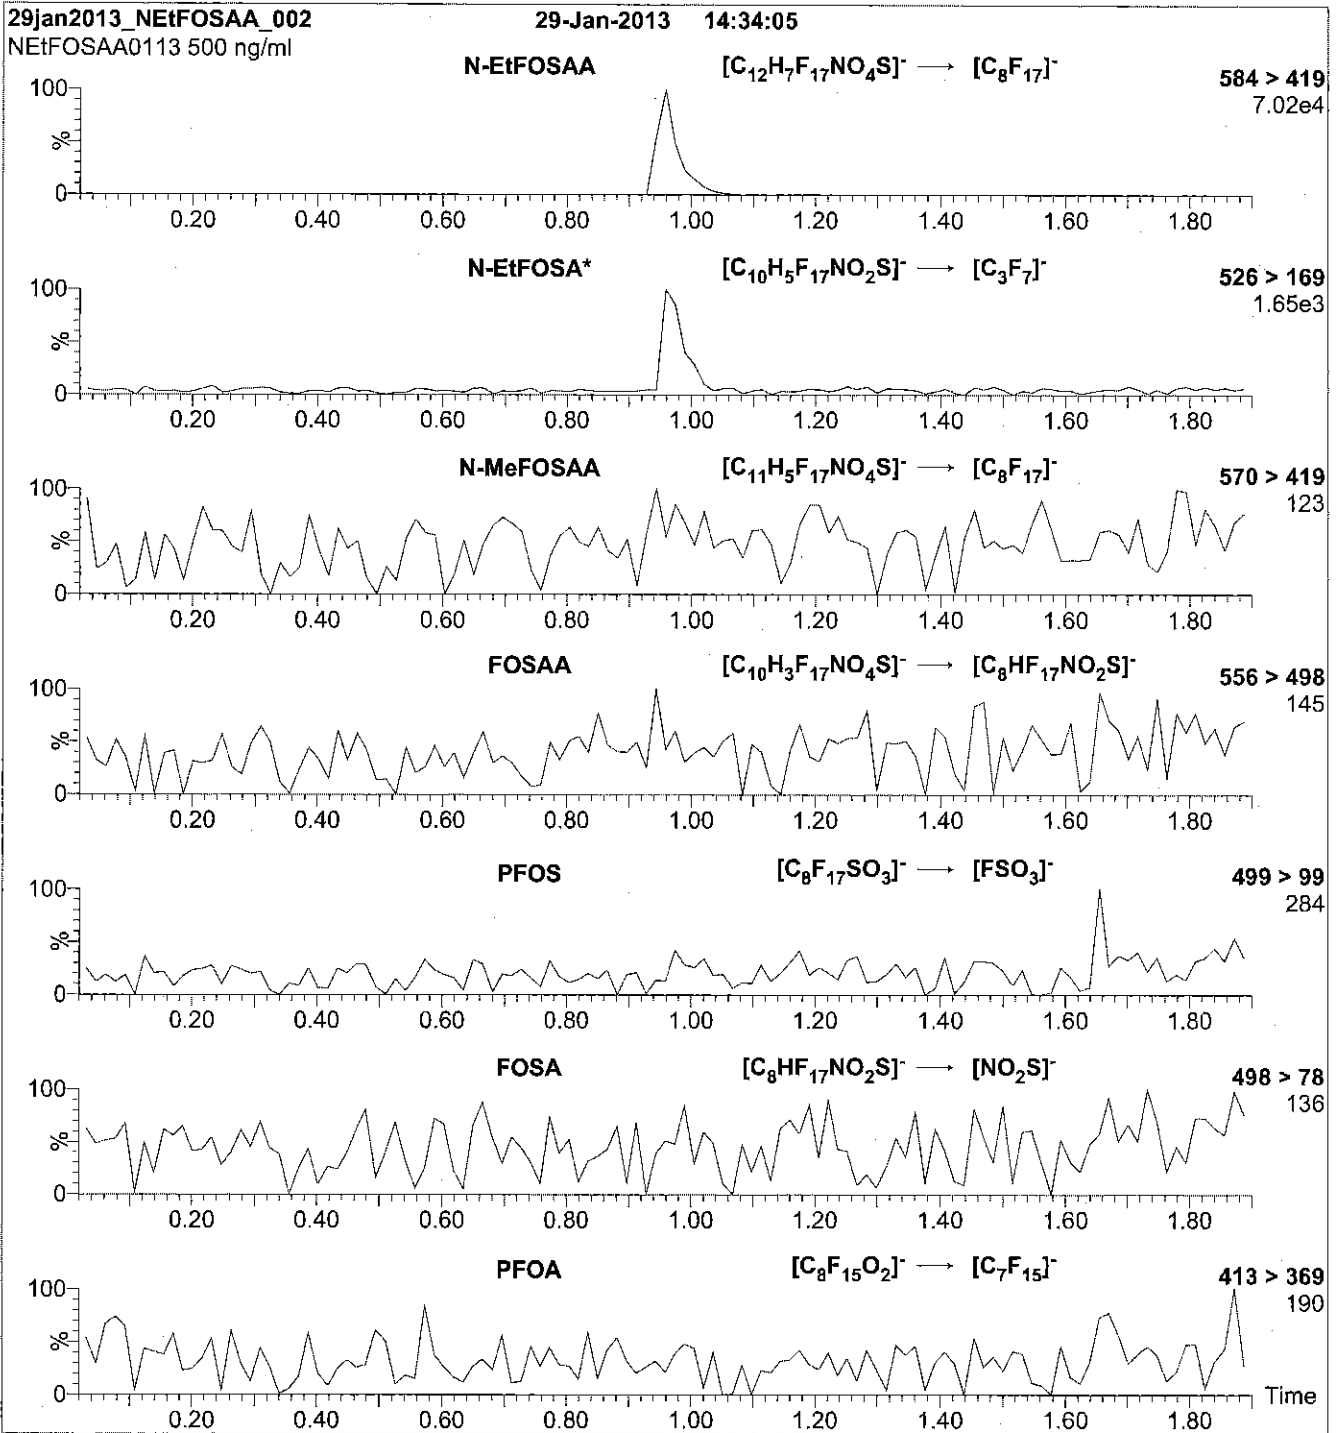

Note: N-EtFOSA is formed by fragmentation of N-EtFOSAA.

Conditions for Figure 2:

Injection: Direct loop injection
 10 μ l (500 ng/ml N-EtFOSAA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.43e-3
 Collision Energy (eV) = 25

Reagent

LCN-ETFOSAA_00002

R: 8/23/16 SBC



715561
ID: LCN-EiFOSAA_00002
Exp: 01/2021 Pp# 98C
N-EiFOSAA




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: N-EtFOSAA **LOT NUMBER:** NEiFOSAA0116
COMPOUND: N-ethylperfluoro-1-octanesulfonamidoacetic acid

STRUCTURE: **CAS #:** 2991-50-6



MOLECULAR FORMULA: C₁₂H₈F₁₇NO₄S **MOLECULAR WEIGHT:** 585.23
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Methanol
Water (<1%)
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 01/20/2016
EXPIRY DATE: (mm/dd/yyyy) 01/20/2021
RECOMMENDED STORAGE: Refrigerate ampoule


DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent the conversion of the acetic acid moiety to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 01/21/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • Info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: N-EtFOSAA; LC/MS Data (TIC and Mass Spectrum)

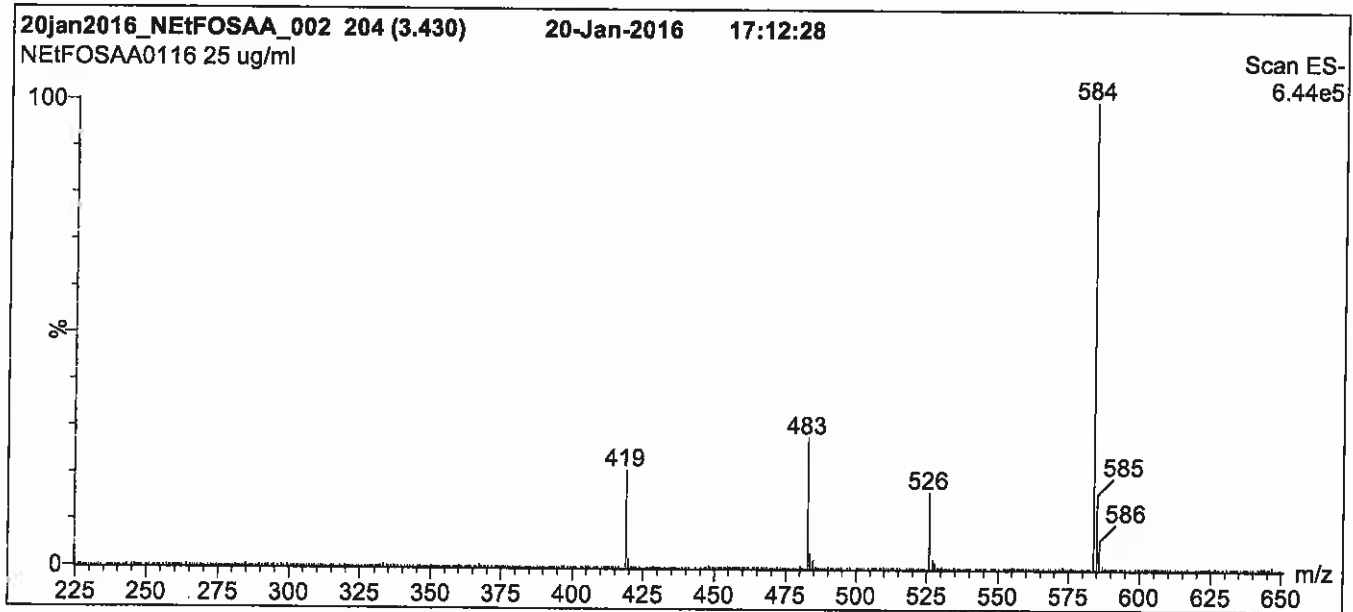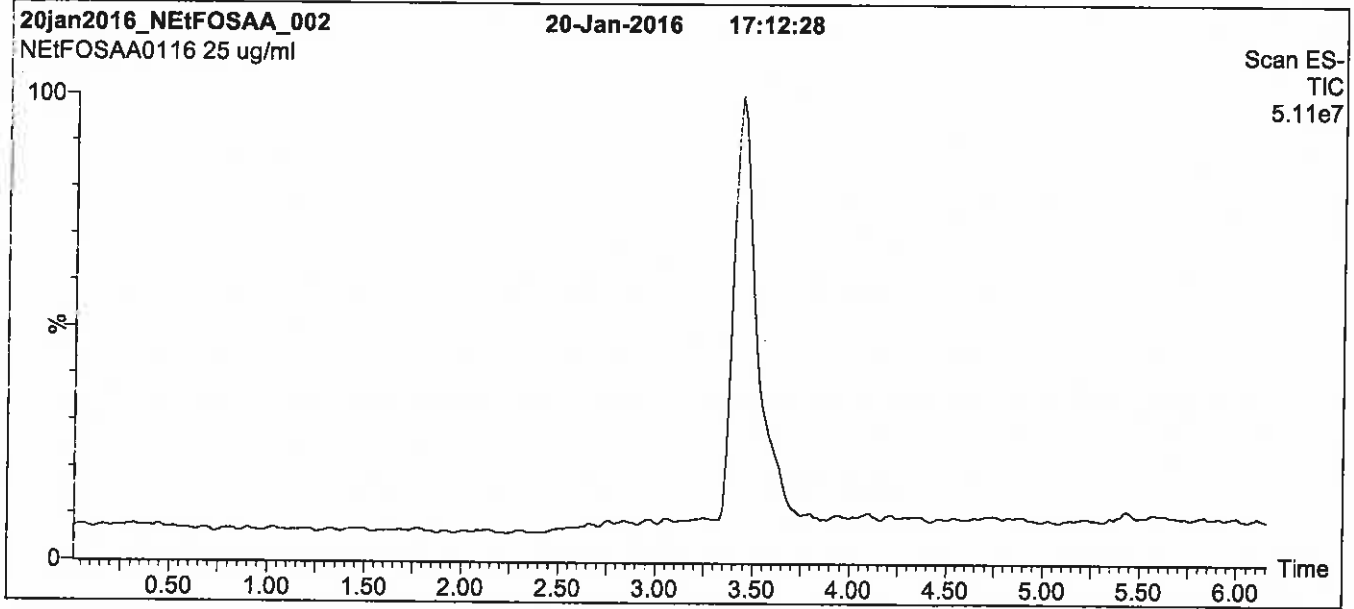

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 60% (80:20 MeOH:ACN) / 40% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 35.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: N-EtFOSAA; LC/MS/MS Data (Selected MRM Transitions)

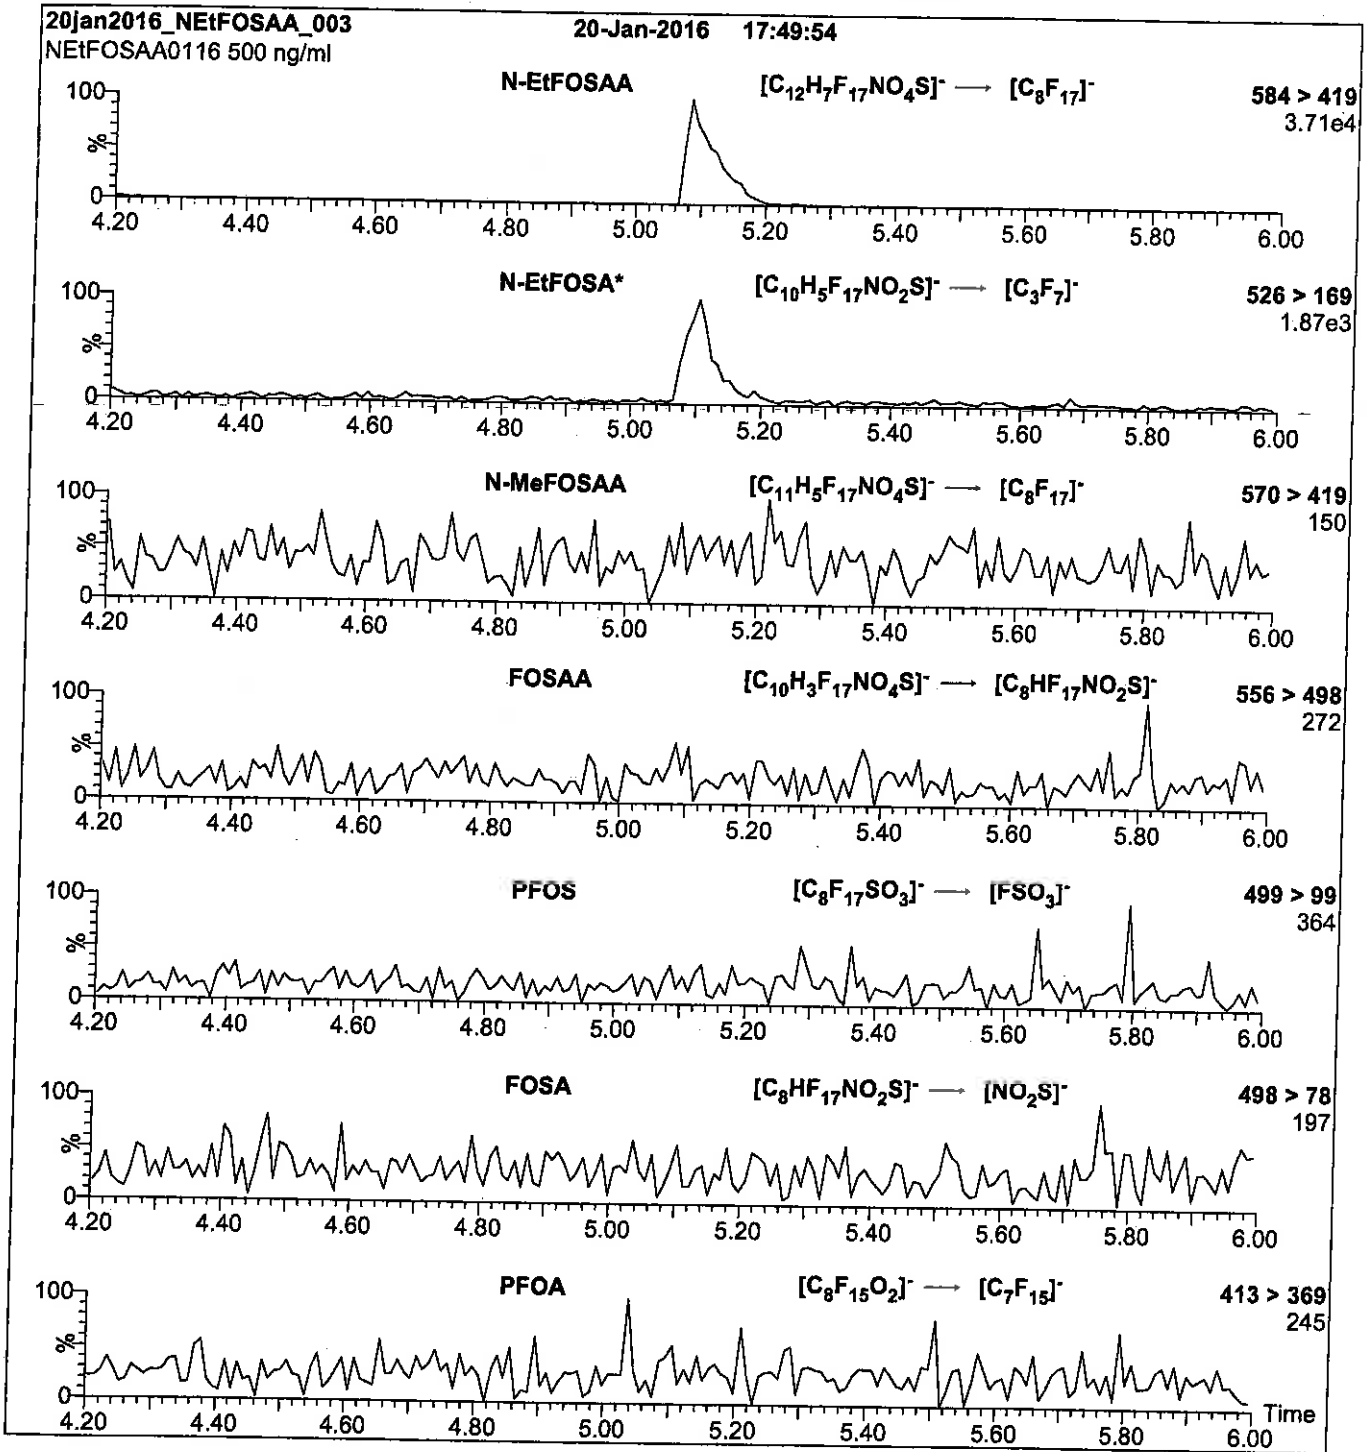

Note: N-EtFOSA is formed by fragmentation of N-EtFOSAA.

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml N-EtFOSAA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.66e-3
Collision Energy (eV) = 25

Reagent

LCN-MeFOSA-M_00001

V: 7/16/15 SPW




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: N-MeFOSA-M
COMPOUND: N-methylperfluoro-1-octanesulfonamide

LOT NUMBER: NMeFOSA0714M

STRUCTURE:  **CAS #:** 31506-32-8

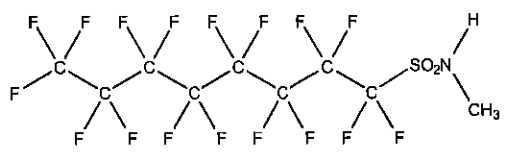

MOLECULAR FORMULA: C₉H₄F₁₇NO₂S
CONCENTRATION: 50 ± 2.5 µg/ml
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 07/15/2014
EXPIRY DATE: (mm/dd/yyyy) 07/15/2019
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

MOLECULAR WEIGHT: 513.17
SOLVENT(S): Methanol


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim

Date: 04/01/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: N-MeFOSA-M; LC/MS Data (TIC and Mass Spectrum)

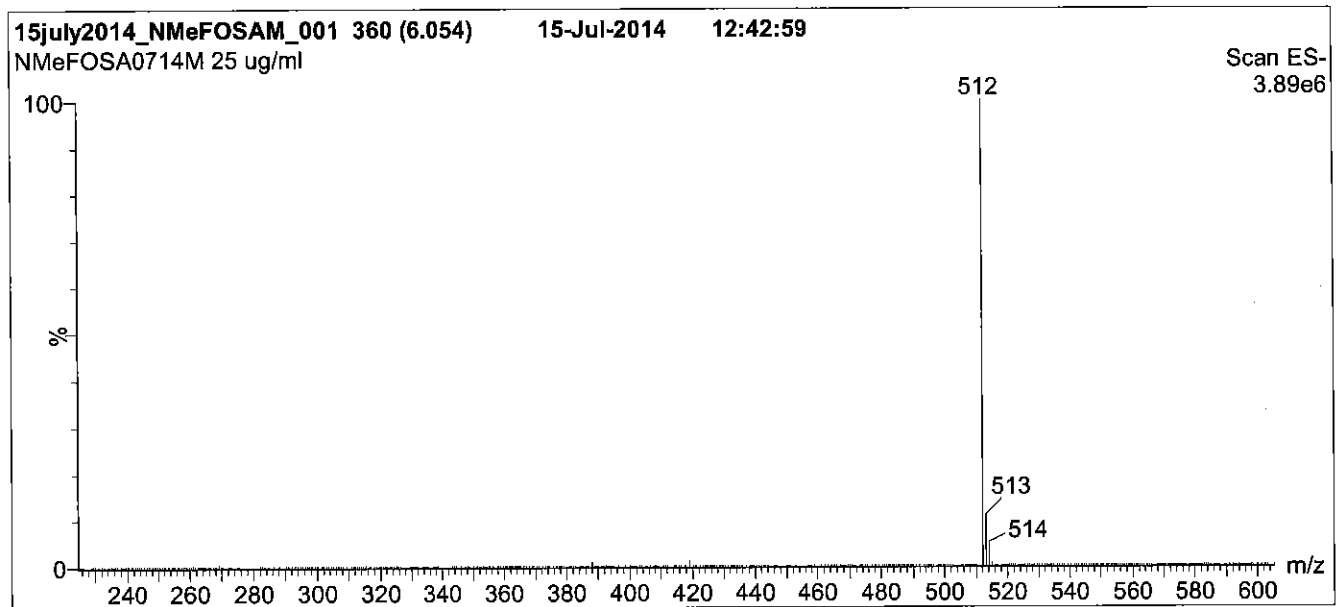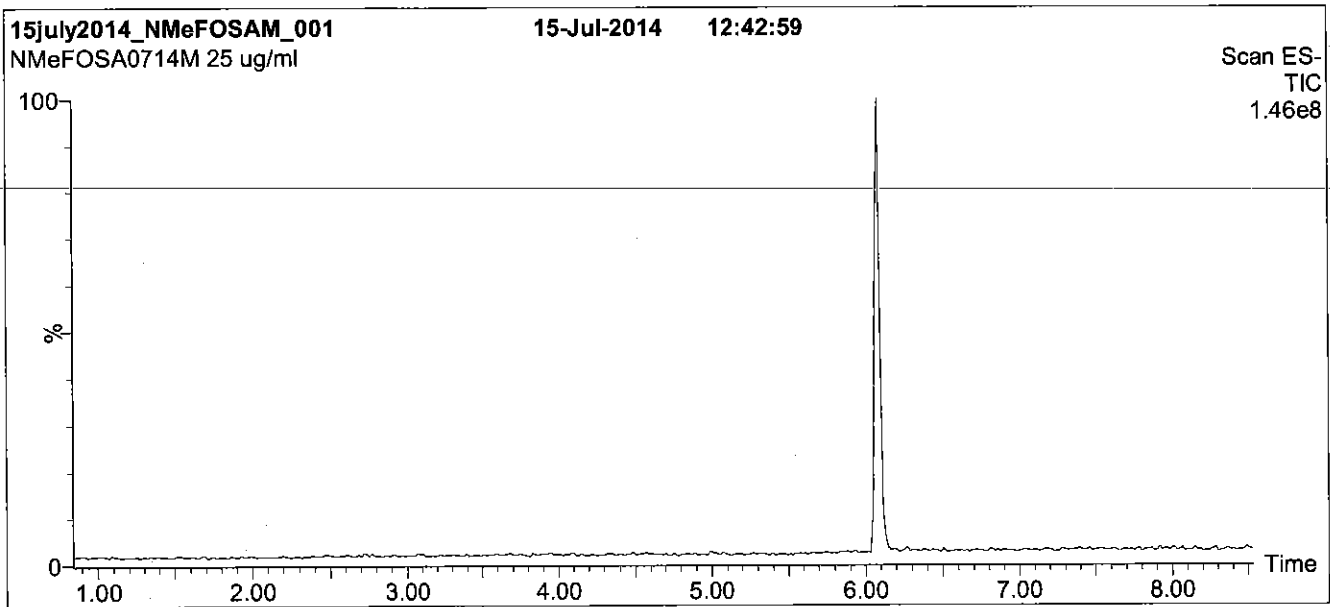

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 45% H₂O / 55% (80:20 MeOH:ACN)
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for
 2 min before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 950 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.50
 Cone Voltage (V) = 40.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: N-MeFOSA-M; LC/MS/MS Data (Selected MRM Transitions)

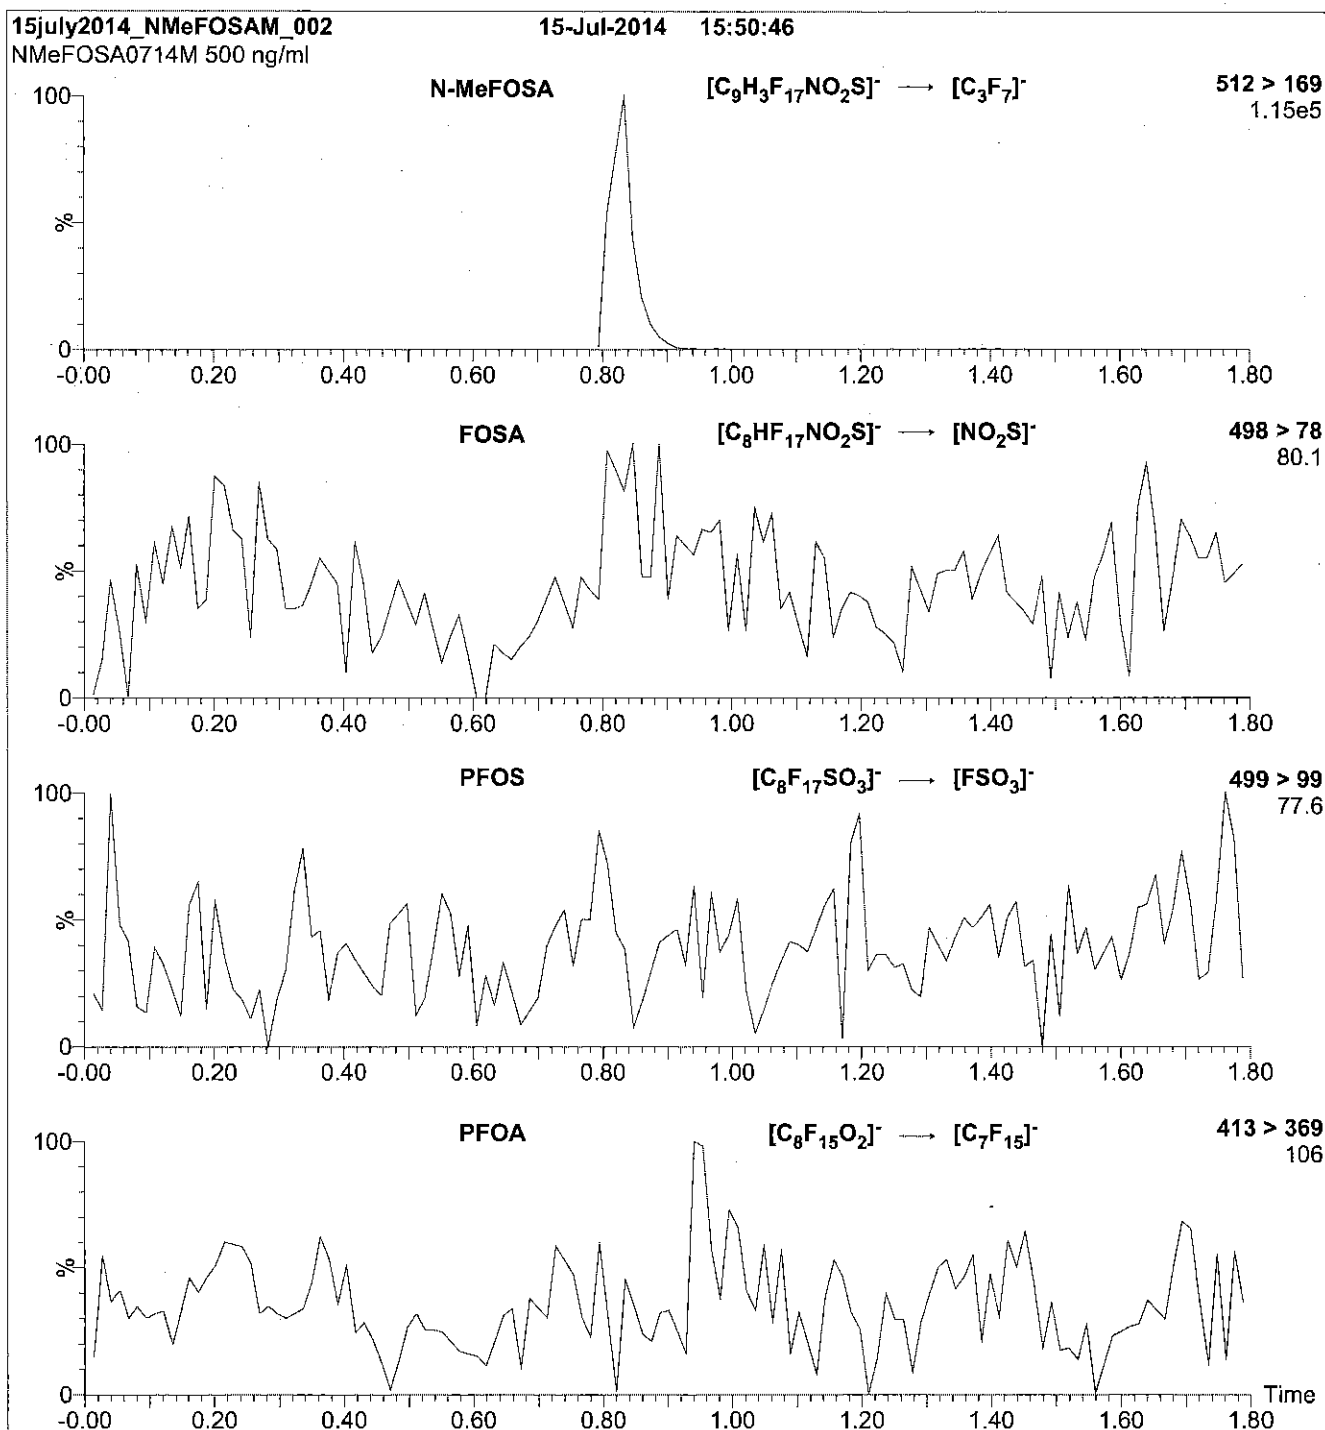

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml N-MeFOSA-M)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.54e-3
Collision Energy (eV) = 30

Reagent

LCN-MeFOSA-M_00002

R: 8/23/16 SBC




715564
ID: LCN-MeFOSA-M_00002
Exp: 05/24/21 Pppl: SBC
N-MeFOSA-M



WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: N-MeFOSA-M **LOT NUMBER:** NMeFOSA0516M
COMPOUND: N-methylperfluoro-1-octanesulfonamide
STRUCTURE: **CAS #:** 31506-32-8



MOLECULAR FORMULA: C₈H₄F₁₇NO₂S **MOLECULAR WEIGHT:** 513.17
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Methanol
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 05/24/2016
EXPIRY DATE: (mm/dd/yyyy) 05/24/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place


DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 05/26/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: N-MeFOSA-M; LC/MS Data (TIC and Mass Spectrum)

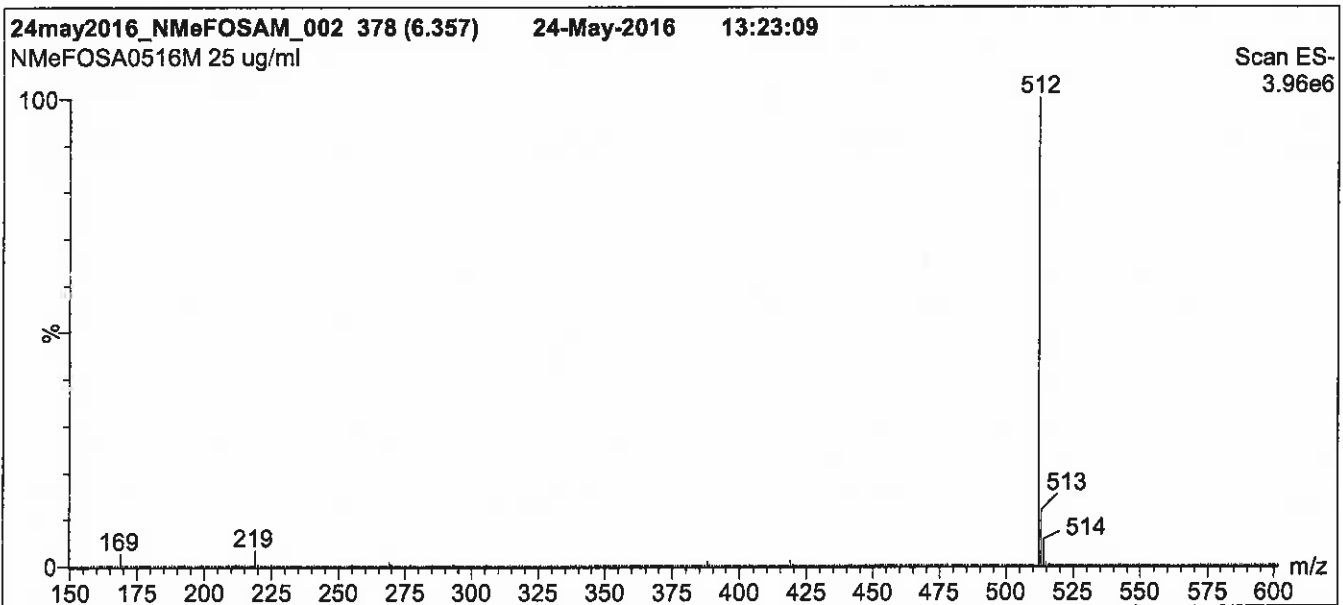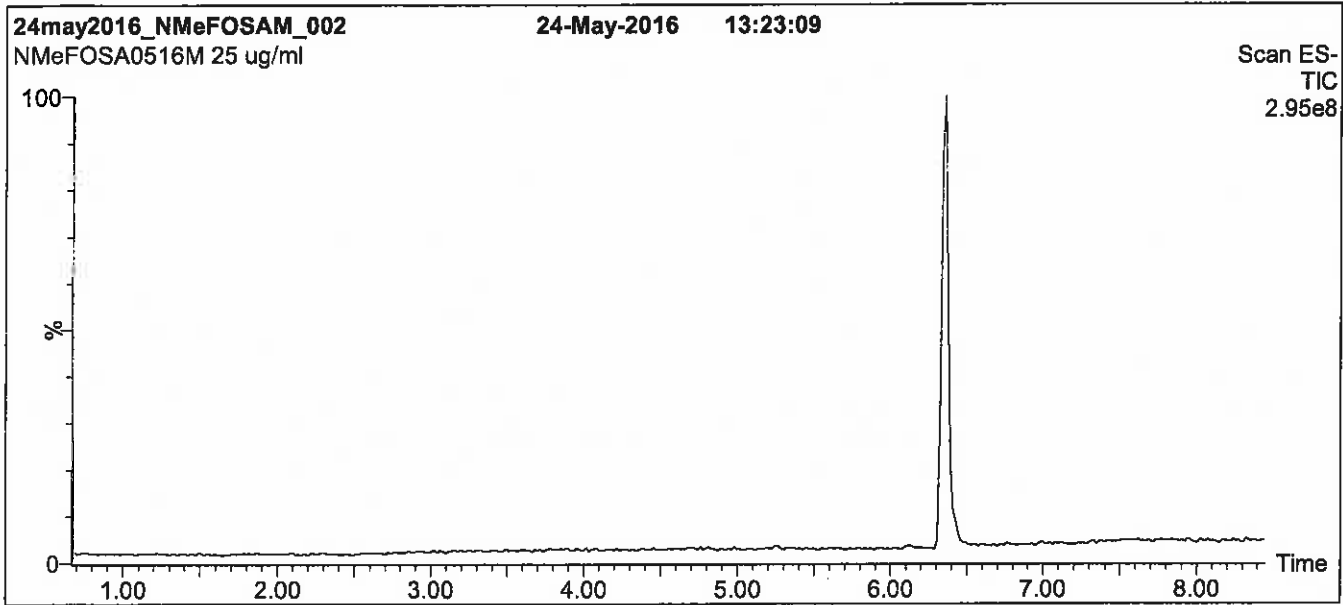

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 45% H₂O / 55% (80:20 MeOH:ACN)
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7.5 min and hold for
 1.5 min before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.50
 Cone Voltage (V) = 40.00
 Core Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: N-MeFOSA-M; LC/MS/MS Data (Selected MRM Transitions)

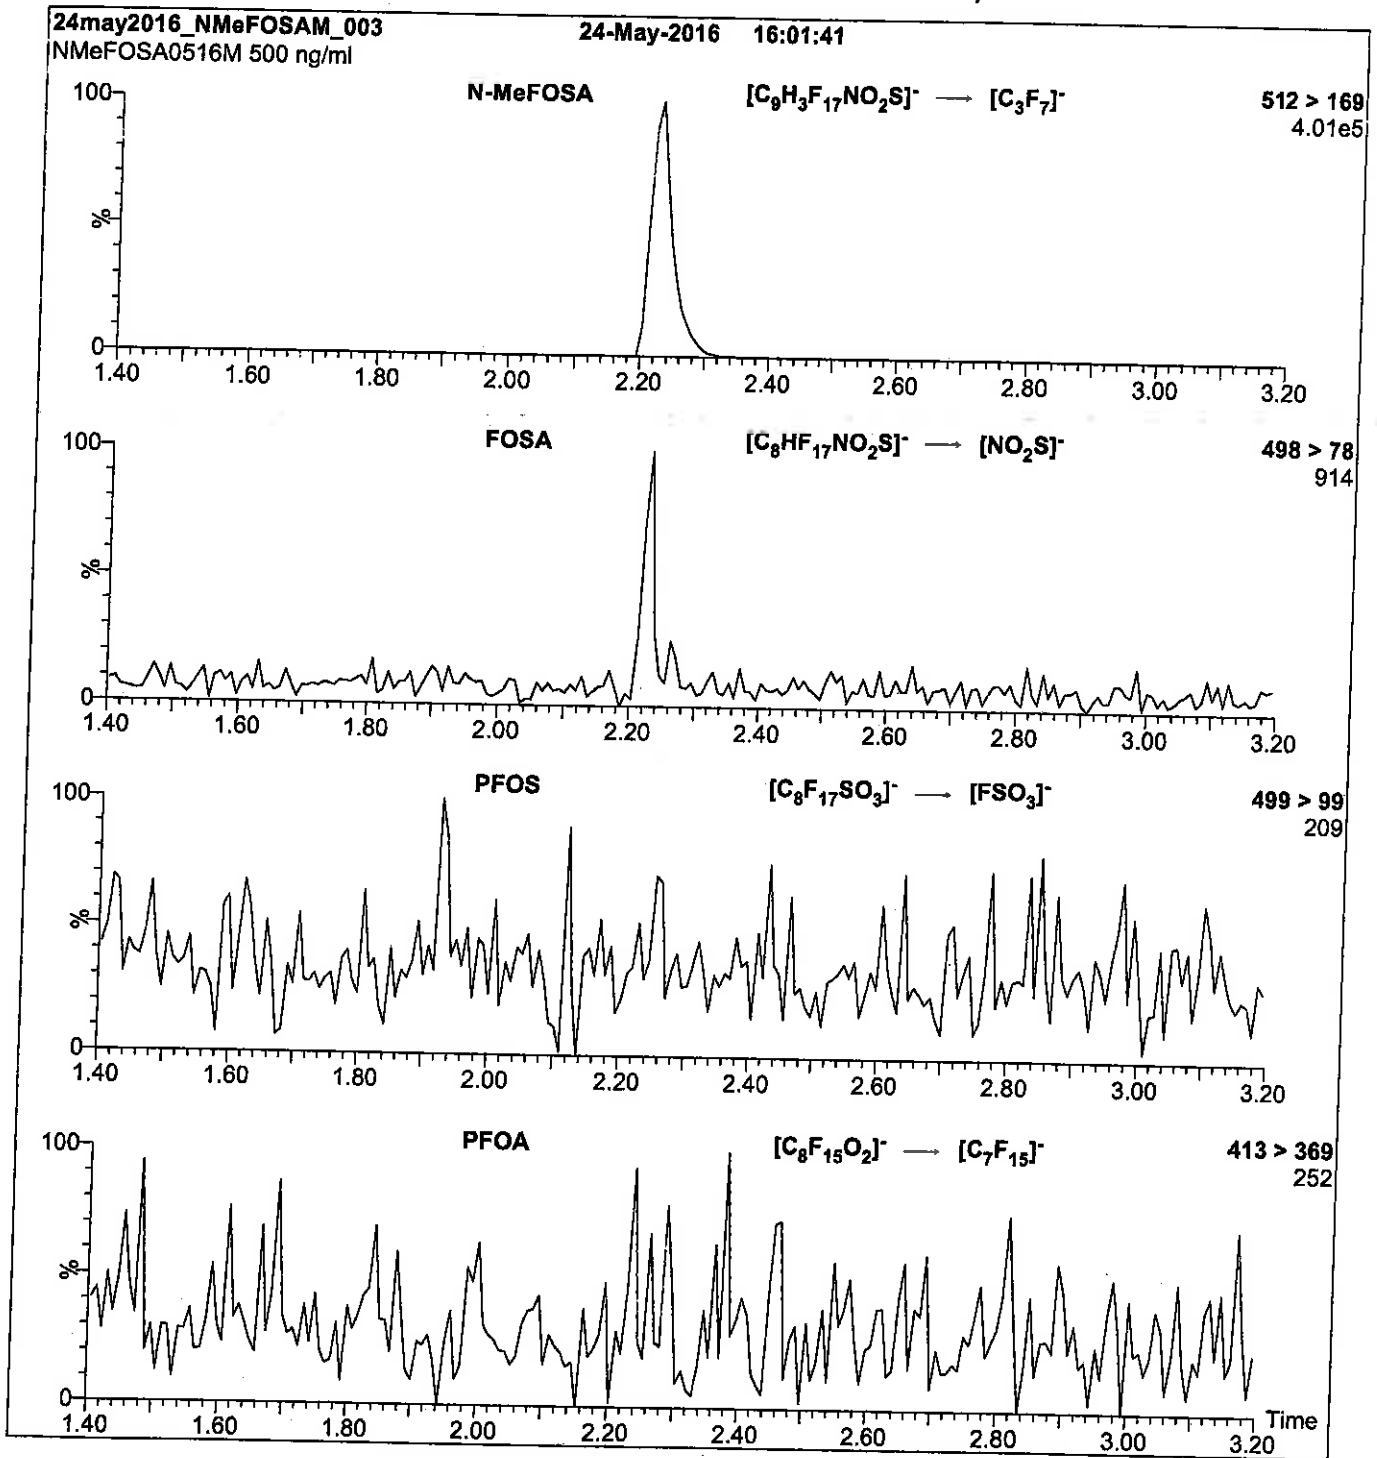

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml N-MeFOSA-M)

MS Parameters

Collision Gas (mbar) = 3.54e-3
Collision Energy (eV) = 30

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

Reagent

LCN-MeFOSAA_00001




WELLINGTON
LABORATORIES

CERTIFICATE OF ANALYSIS
DOCUMENTATION

PRODUCT CODE: N-MeFOSAA **LOT NUMBER:** NMeFOSAA1214
COMPOUND: N-methylperfluoro-1-octanesulfonamidoacetic acid

STRUCTURE: **CAS #:** 2355-31-9



MOLECULAR FORMULA: C₁₁H₆F₁₇NO₄S **MOLECULAR WEIGHT:** 571.21
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Methanol
 Water (<1%)
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 12/09/2014
EXPIRY DATE: (mm/dd/yyyy) 12/09/2019
RECOMMENDED STORAGE: Refrigerate ampoule


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent the conversion of the acetic acid moiety to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
 B.G. Chittim **Date:** 04/06/2015
 (mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
 519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: N-MeFOSAA; LC/MS Data (TIC and Mass Spectrum)

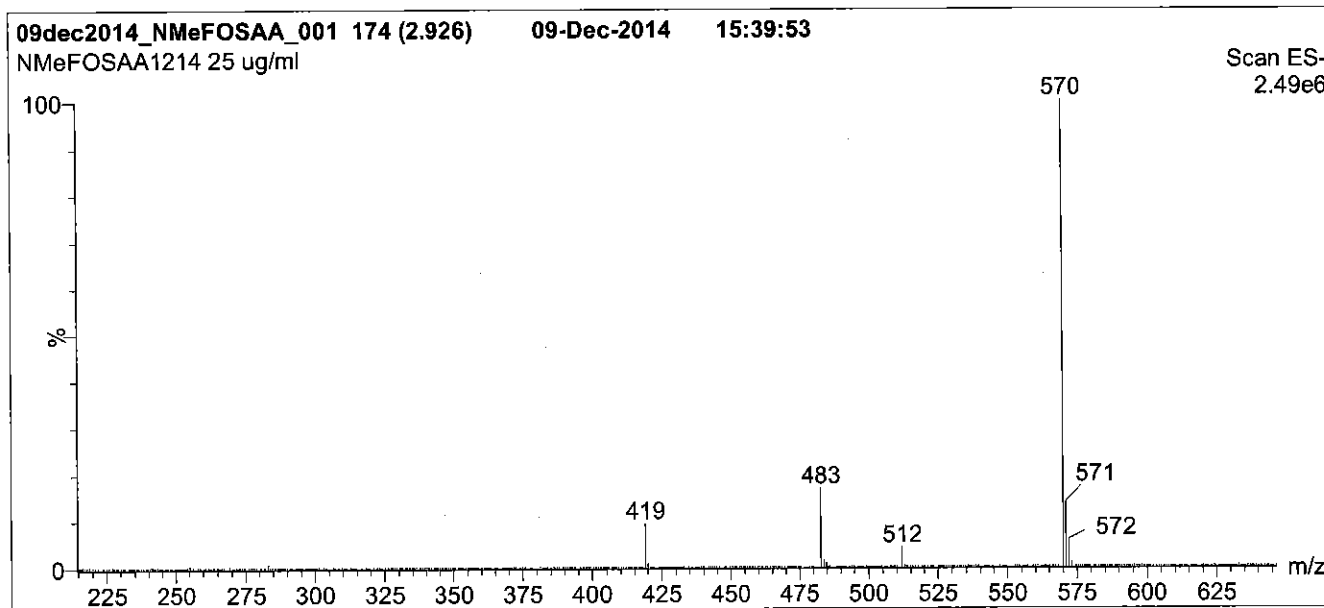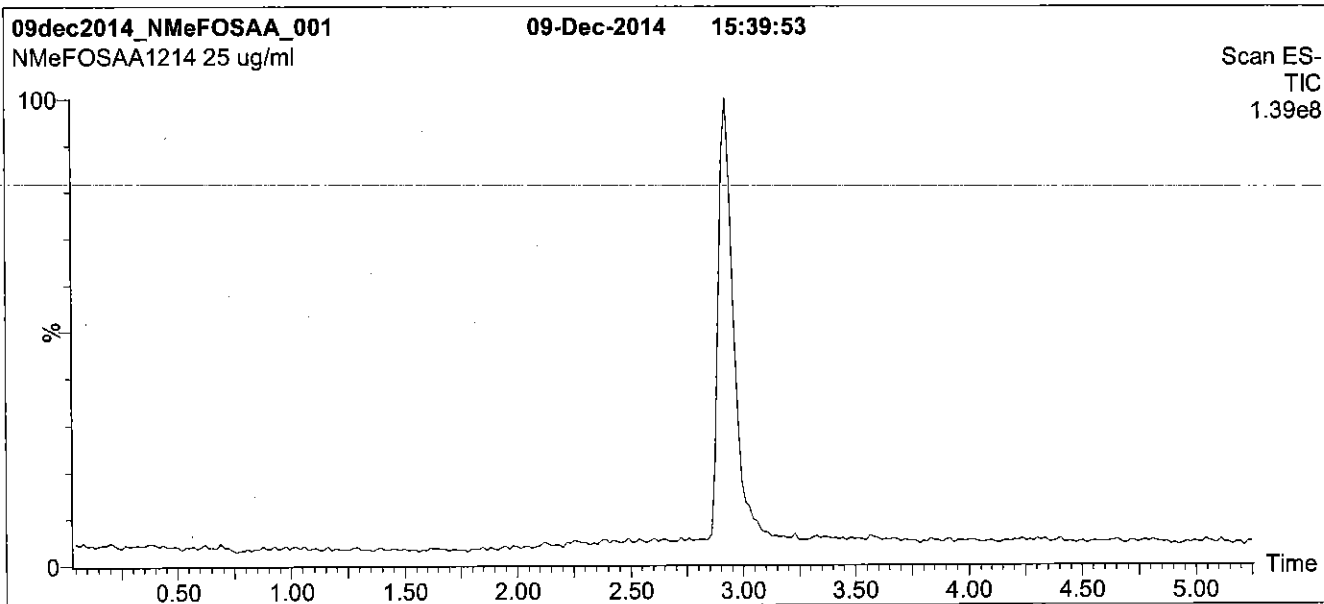

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 65% (80:20 MeOH:ACN) / 35% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (215 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 35.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: N-MeFOSAA; LC/MS/MS Data (Selected MRM Transitions)

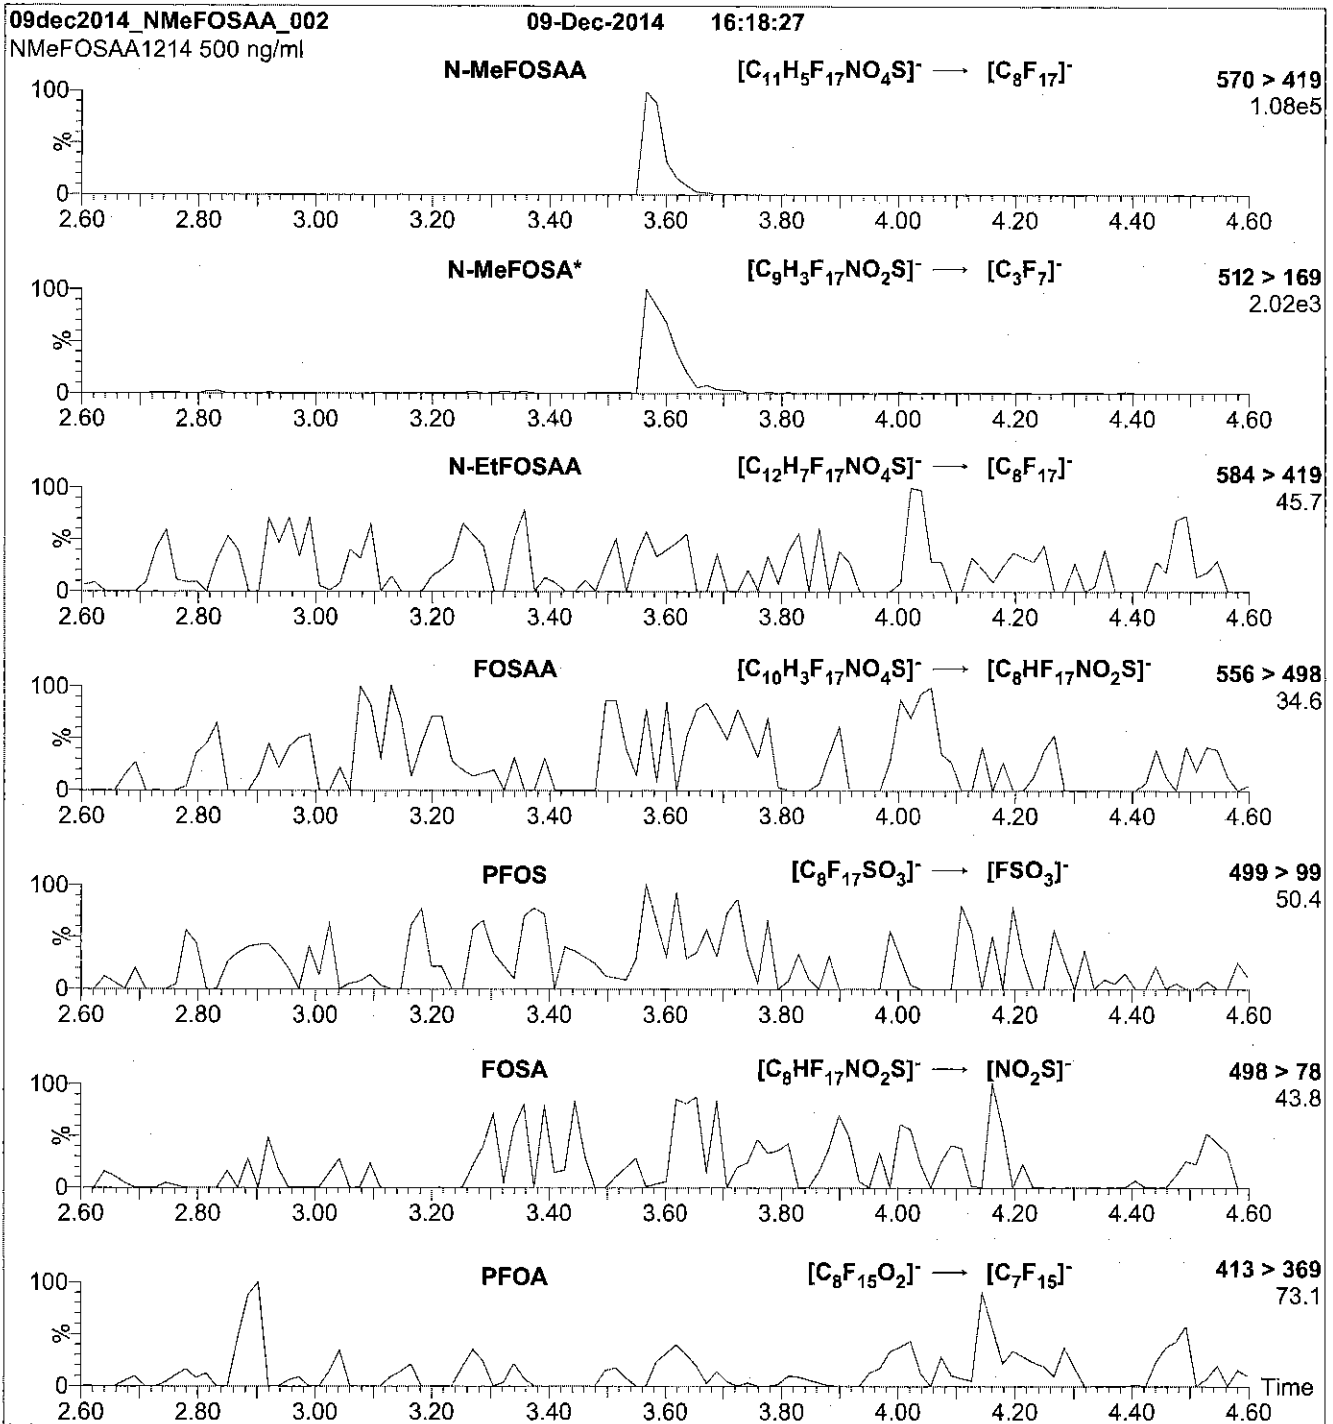

*Note: N-MeFOSA is formed by fragmentation of N-MeFOSAA.

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml N-MeFOSAA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.31e-3
Collision Energy (eV) = 25

Reagent

LCN-MeFOSAA_00003

R: 8/23/16 JAE

715562
ID: LCN-MeFOSAA_00003
Exp: 01/20/21 Prpd: SEC
N-MeFOSAA




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: N-MeFOSAA **LOT NUMBER:** NMeFOSAA0116
COMPOUND: N-methylperfluoro-1-octanesulfonamidoacetic acid

STRUCTURE: **CAS #:** 2355-31-9



MOLECULAR FORMULA: C₁₁H₈F₁₇NO₄S **MOLECULAR WEIGHT:** 571.21
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Methanol
Water (<1%)
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 01/20/2016
EXPIRY DATE: (mm/dd/yyyy) 01/20/2021
RECOMMENDED STORAGE: Refrigerate ampoule


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent the conversion of the acetic acid moiety to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:  **Date:** 01/21/2016
B.G. Chittim (mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: N-MeFOSAA; LC/MS Data (TIC and Mass Spectrum)

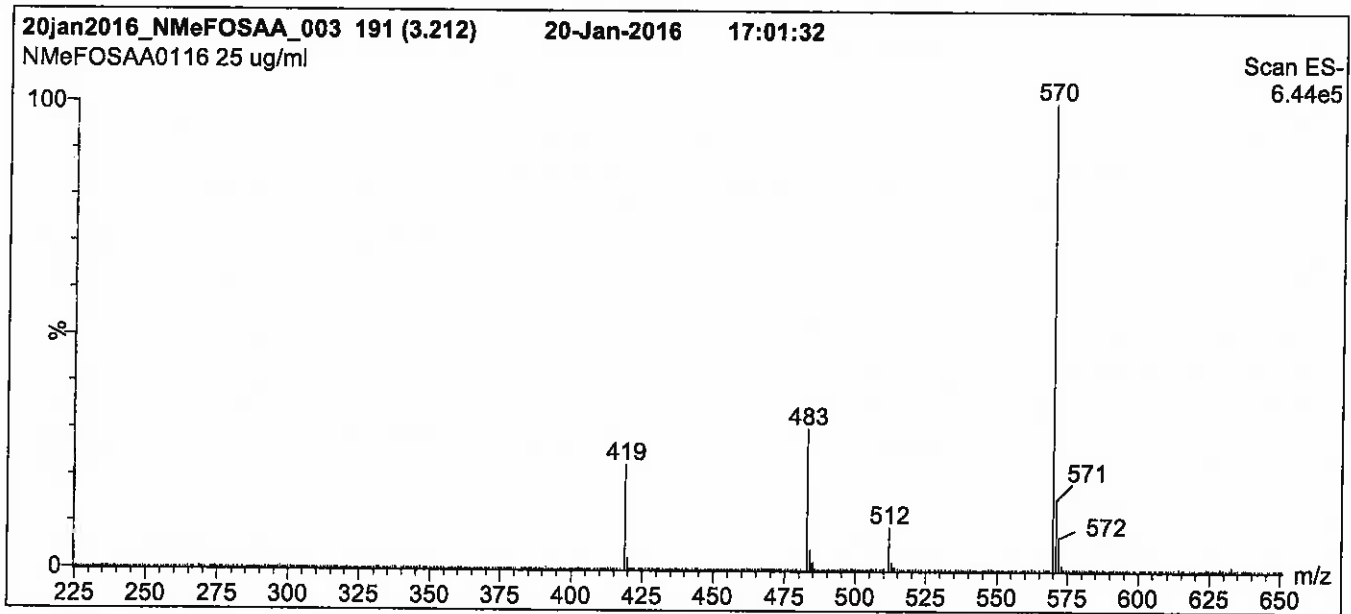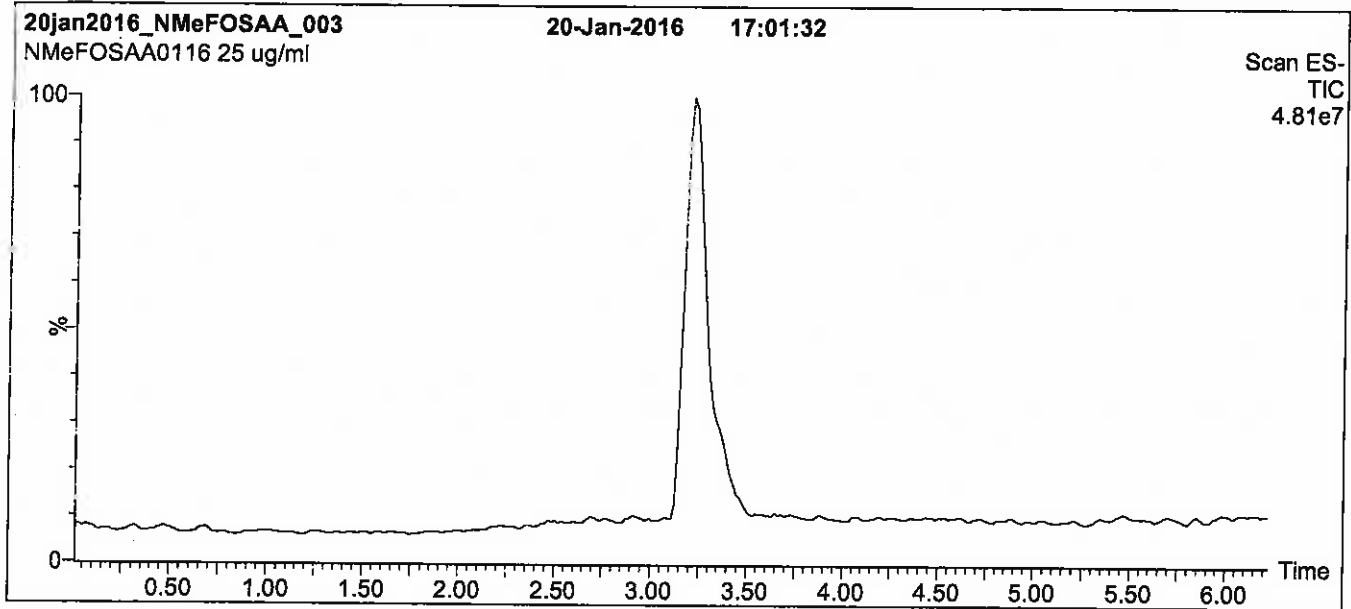

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 60% (80:20 MeOH:ACN) / 40% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 35.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: N-MeFOSAA; LC/MS/MS Data (Selected MRM Transitions)

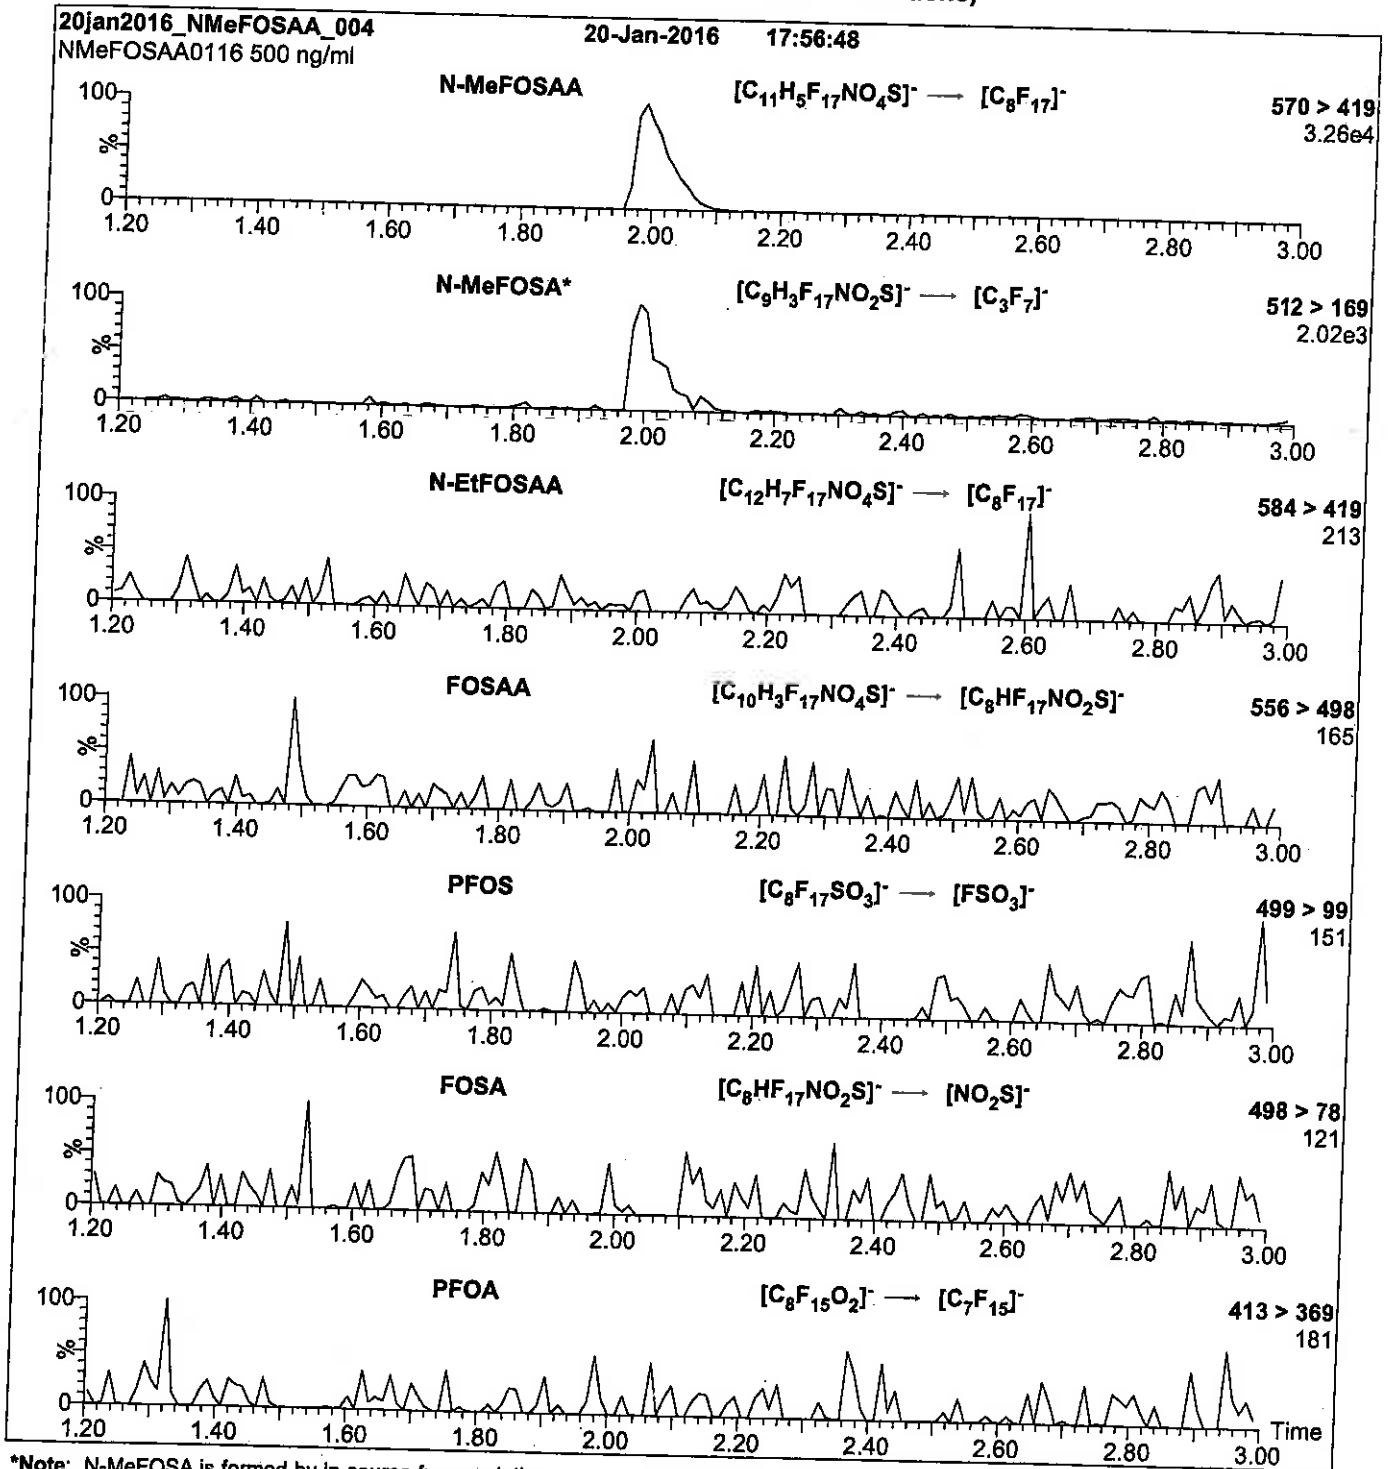

*Note: N-MeFOSA is formed by in-source fragmentation.

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml N-MeFOSAA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.66e-3
Collision Energy (eV) = 25

Reagent

LCPFACMXB_00007



WELLINGTON
LABORATORIES

CERTIFICATE OF ANALYSIS
DOCUMENTATION

PFAC-MXB

**Solution/Mixture of Native
Perfluoroalkylcarboxylic Acids and
Native Perfluoroalkylsulfonates**

PRODUCT CODE: PFAC-MXB
LOT NUMBER: PFACMXB1115
SOLVENT(S): Methanol / Water (<1%)
DATE PREPARED: (mm/dd/yyyy) 11/04/2015
LAST TESTED: (mm/dd/yyyy) 11/06/2015
EXPIRY DATE: (mm/dd/yyyy) 11/06/2020
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DESCRIPTION:

PFAC-MXB is a solution/mixture of thirteen native perfluoroalkylcarboxylic acids (C₄-C₁₄, C₁₆, and C₁₈) and four native perfluoroalkylsulfonates (C₄, C₆, C₈ and C₁₀). The full name, abbreviation and concentration for each of the components are given in Table A.

The individual perfluoroalkylcarboxylic acids and perfluoroalkylsulfonates all have chemical purities of >98%.

DOCUMENTATION/ DATA ATTACHED:

Table A: Components and Concentrations of the Solution/Mixture
 Figure 1: LC/MS Data (SiR)
 Figure 2: LC/MS/MS Data (Selected MRM Transitions)
 Figure 3: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acids to their respective methyl esters.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compounds it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.

QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com


Table A: PFAC-MXB; Components and Concentrations (ng/ml, ± 5% in Methanol / Water (<1%))

Name	Abbreviation	Concentration (ng/ml)		Peak Assignment in Figure 1
		as the salt	as the anion	
Perfluoro-n-butanoic acid	PFBA	2000		A
Perfluoro-n-pentanoic acid	PFPeA	2000		B
Perfluoro-n-hexanoic acid	PFHxA	2000		D
Perfluoro-n-heptanoic acid	PFHpA	2000		E
Perfluoro-n-octanoic acid	PFOA	2000		G
Perfluoro-n-nonanoic acid	PFNA	2000		H
Perfluoro-n-decanoic acid	PFDA	2000		J
Perfluoro-n-undecanoic acid	PFUdA	2000		K
Perfluoro-n-dodecanoic acid	PFDoA	2000		M
Perfluoro-n-tridecanoic acid	PFTrDA	2000		N
Perfluoro-n-tetradecanoic acid	PFTeDA	2000		O
Perfluoro-n-hexadecanoic acid	PFHxDA	2000		P
Perfluoro-n-octadecanoic acid	PFODA	2000		Q
Name	Abbreviation	Concentration (ng/ml)		Peak Assignment in Figure 1
		as the salt	as the anion	
Potassium perfluoro-1-butanesulfonate	L-PFBS	2000	1770	C
Sodium perfluoro-1-hexanesulfonate	L-PFHxS	2000	1890	F
Sodium perfluoro-1-octanesulfonate	L-PFOS	2000	1910	I
Sodium perfluoro-1-decanesulfonate	L-PFDS	2000	1930	L

Certified By: 
B.G. Chittim

Date: 11/11/2015
(mm/dd/yyyy)

Figure 1: PFAC-MXB; LC/MS Data (Total Ion Current Chromatogram; SIR)

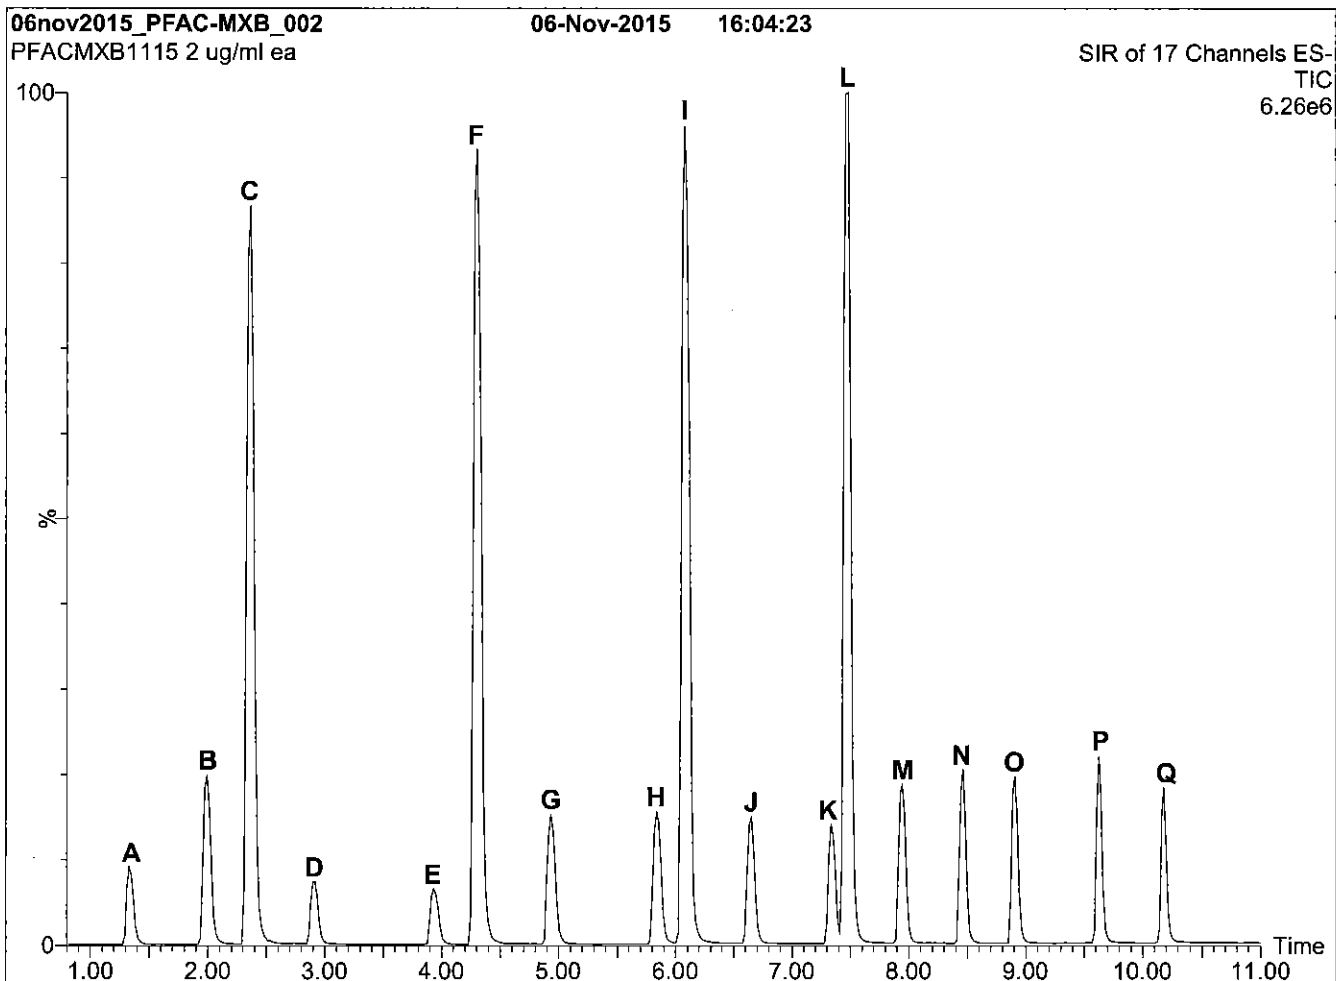

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 55% H₂O / 45% (80:20 MeOH:ACN)
(both with 10 mM NH₄OAc buffer)
Ramp to 95% organic over 10 min and hold for 1 min
before returning to initial conditions in 0.5 min.

Time: 12 min

Flow: 300 μ l/min

MS Parameters

Experiment: SIR of 17 Channels

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = variable (10-70)
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: PFAC-MXB; LC/MS/MS Data (Selected MRM Transitions)


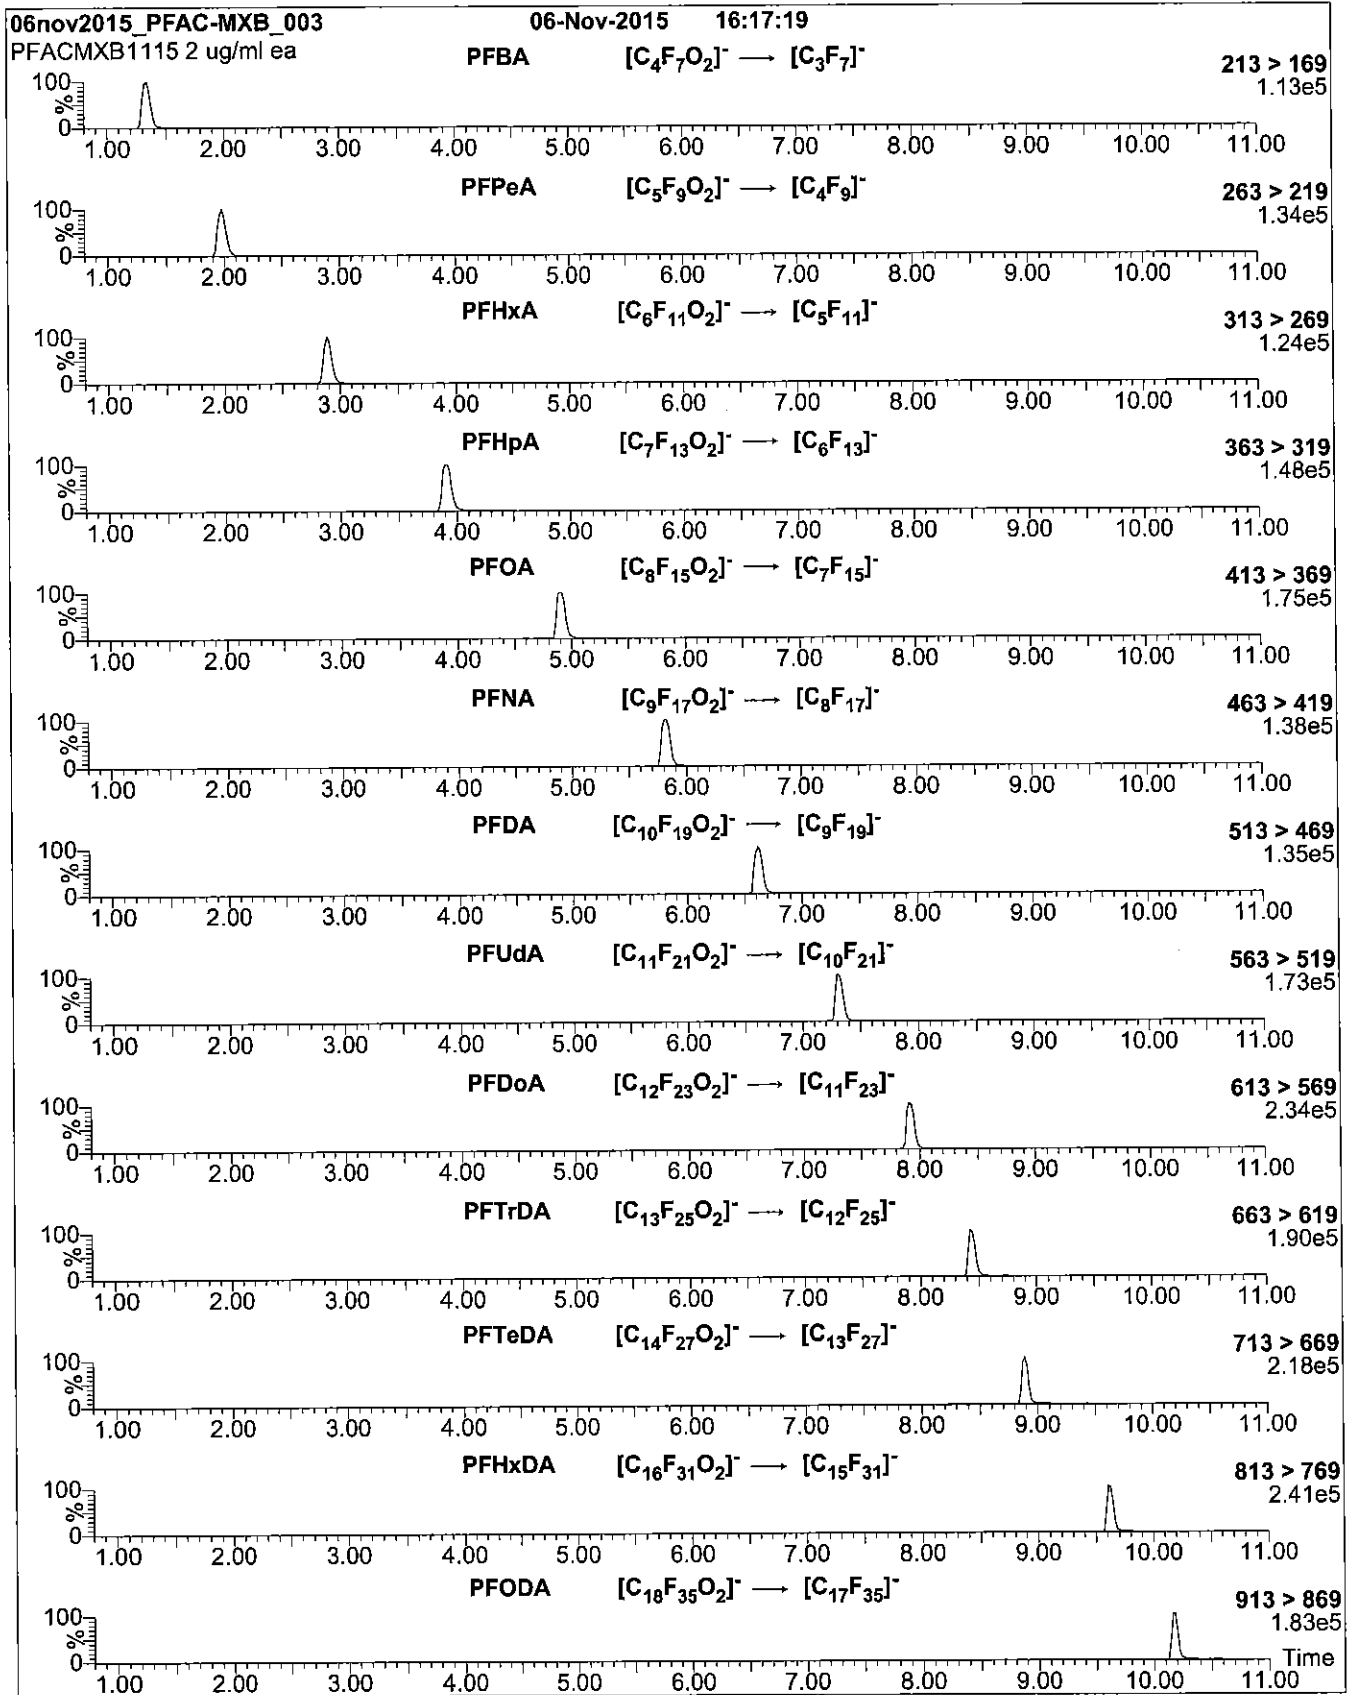


Figure 3: PFAC-MXB; LC/MS/MS Data (Selected MRM Transitions)

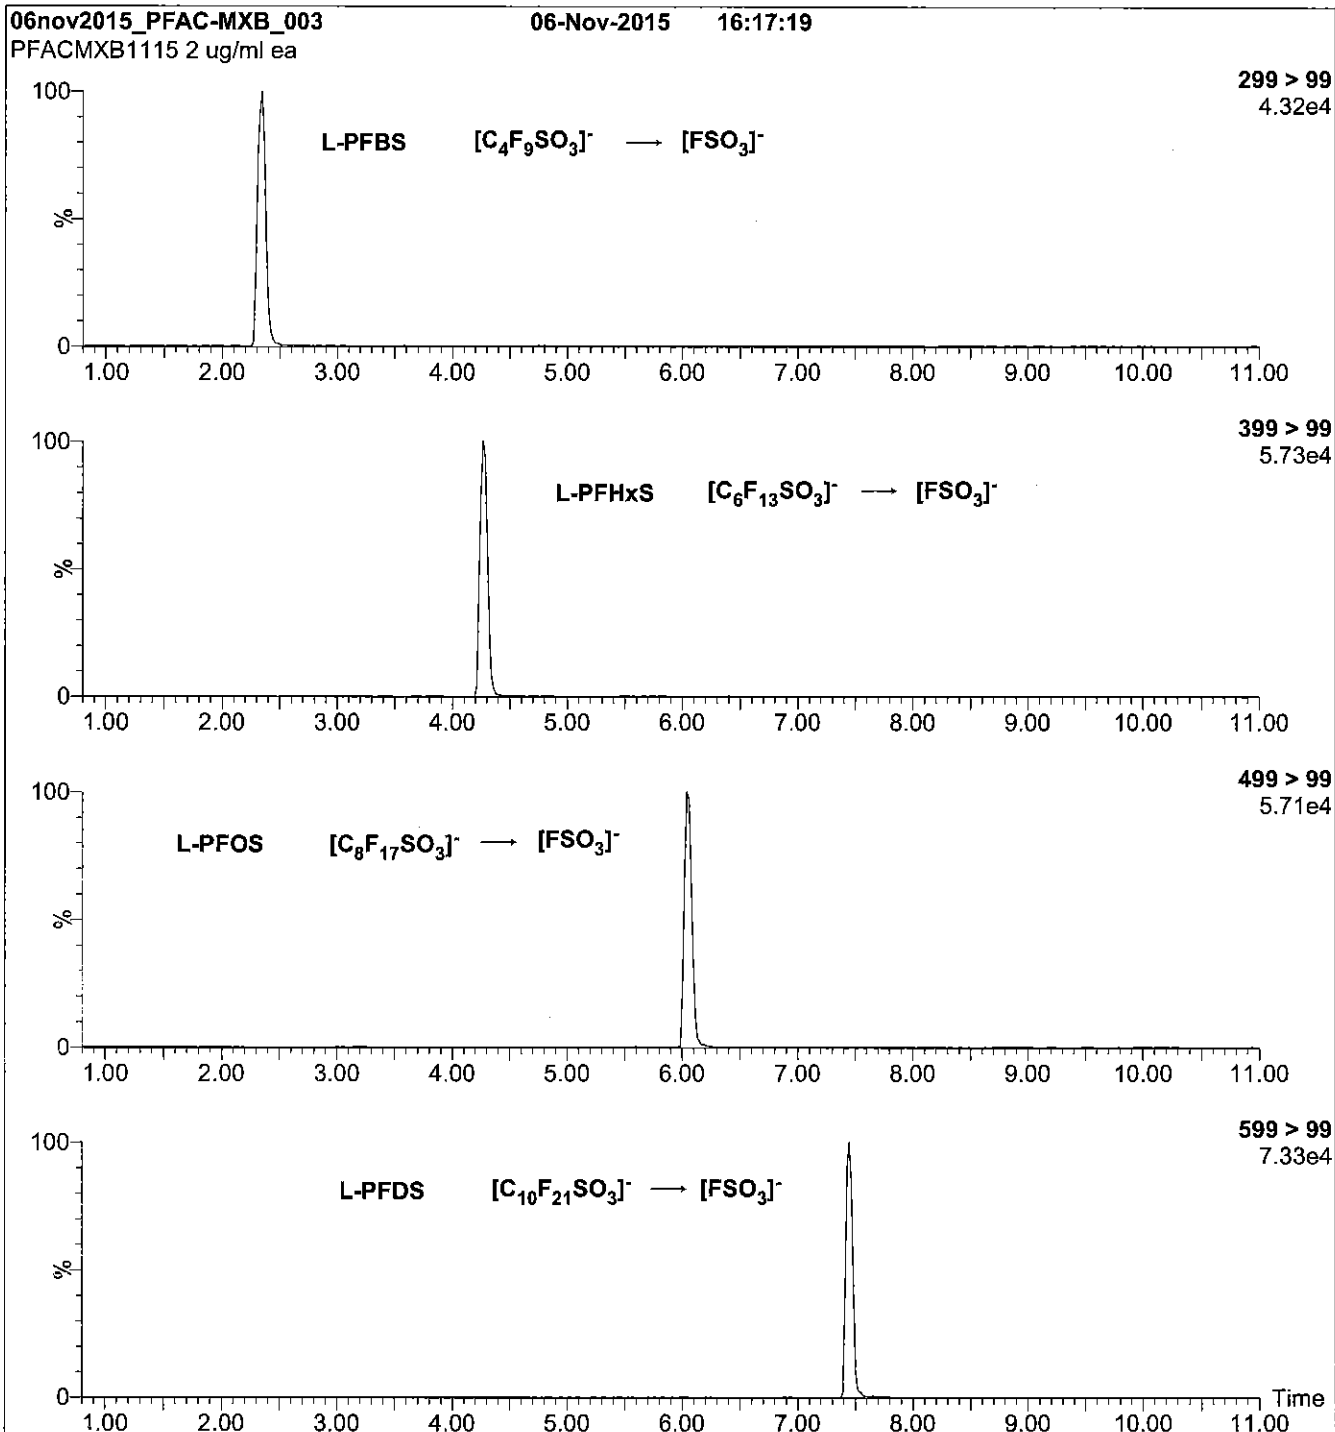

Conditions for Figures 2 and 3:

Injection: on-column (PFAC-MXB)
 Mobile phase: Same as Figure 1
 Flow: 300 μ /min

MS Parameters
 Collision Gas (mbar) = 3.24e-3
 Collision Energy (eV) = 8-50 (variable)

Reagent

LCPFBA_00005

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFBA; LC/MS Data (TIC and Mass Spectrum)

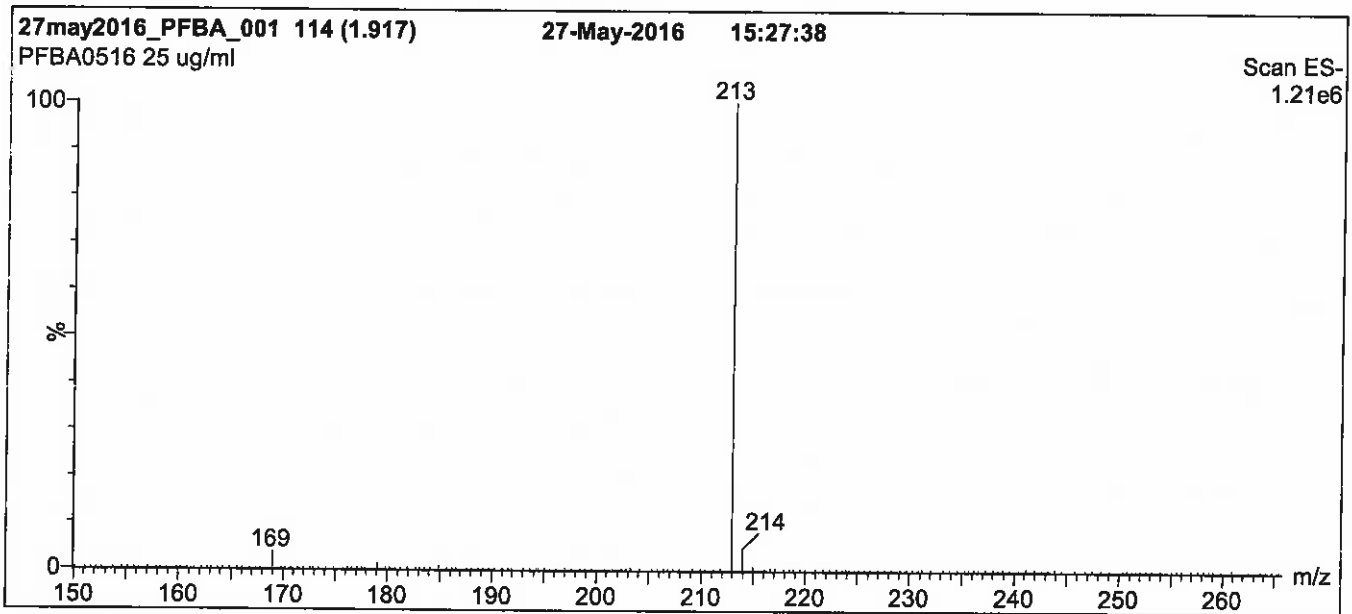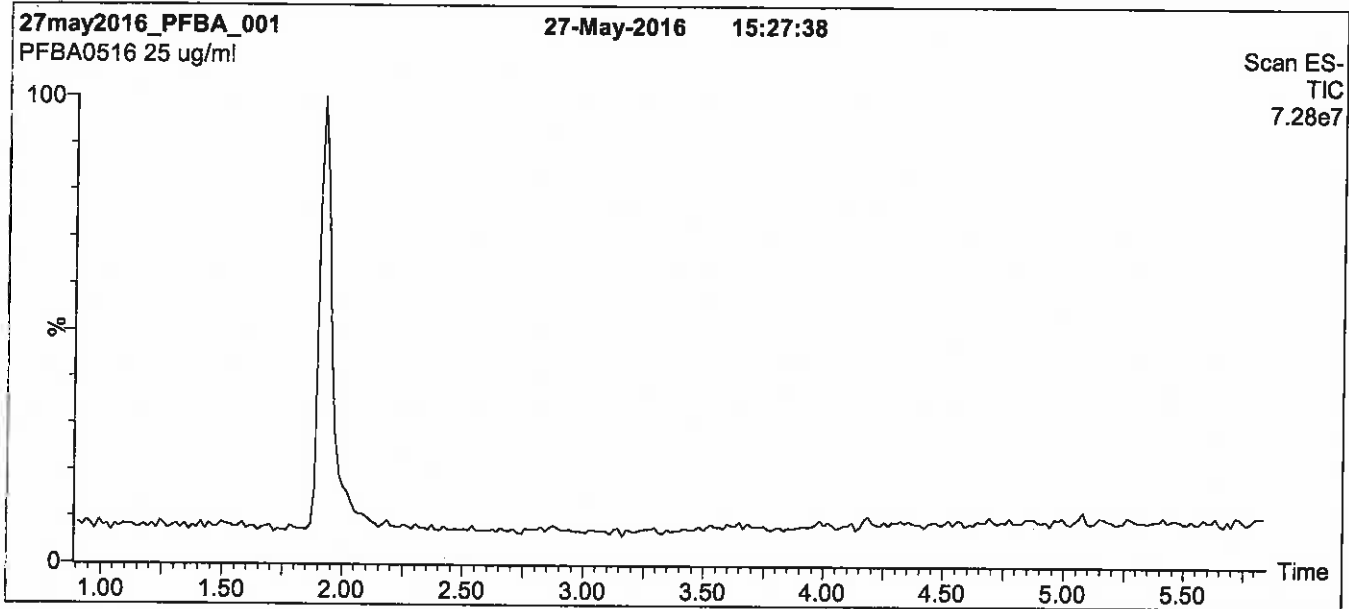

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 30% (80:20 MeOH:ACN) / 70% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 1.5 min before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 10.00
Cone Gas Flow (l/hr) = 100
Desolvation Gas Flow (l/hr) = 750

Figure 2: PFBA; LC/MS/MS Data (Selected MRM Transitions)

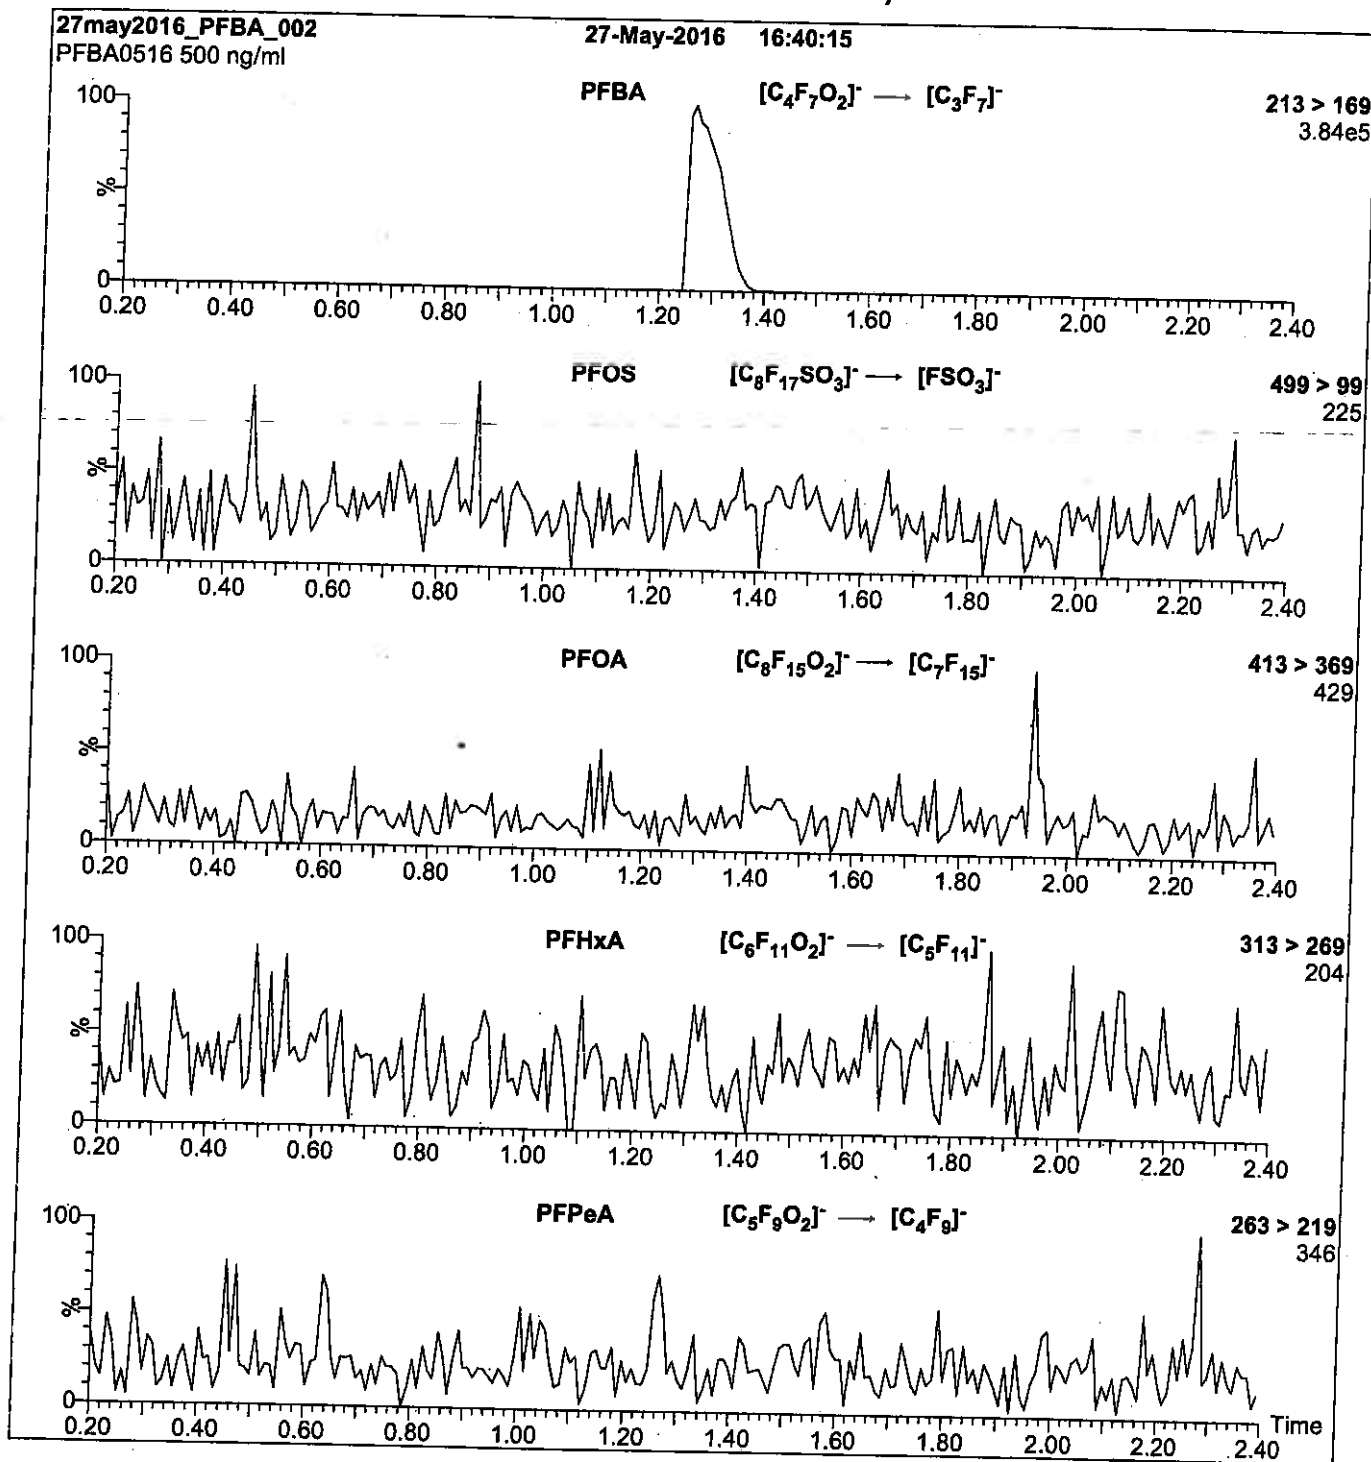

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml PFBA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.62e-3
Collision Energy (eV) = 10

Reagent

LCPFBS_00005

R: 9/9/16 gbe



728306
ID: LCM2-8:2FTS_00003
Exp: 01/08/21 Prpd: SBC
M2-8:2FTS




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: M2-8:2FTS **LOT NUMBER:** M282FTS0116
COMPOUND: Sodium 1H,1H,2H,2H-perfluoro-[1,2-¹³C₂]decane sulfonate

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA:	¹³ C ₂ ¹² C ₈ H ₄ F ₁₇ SO ₃ Na	MOLECULAR WEIGHT:	552.15
CONCENTRATION:	50.0 ± 2.5 µg/ml (Na salt)	SOLVENT(S):	Methanol
	47.9 ± 2.4 µg/ml (M2-8:2FTS anion)	ISOTOPIC PURITY:	≥99% ¹³ C
CHEMICAL PURITY:	>98%		(1,2- ¹³ C ₂)
LAST TESTED: (mm/dd/yyyy)	01/08/2016		
EXPIRY DATE: (mm/dd/yyyy)	01/08/2021		
RECOMMENDED STORAGE:	Refrigerate ampoule		

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- The native 8:2FTS contains 4.22% of ³⁴S (due to natural isotopic abundance) therefore both native 8:2FTS and M2-8:2FTS will produce signals in the m/z 529 to m/z 509 channel during SRM analysis. We recommend using the m/z 529 to m/z 81 transition to monitor for M2-8:2FTS during quantitative analysis as it will be free of any native contribution (see Figure 2).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 01/18/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: M2-8:2FTS; LC/MS Data (TIC and Mass Spectrum)

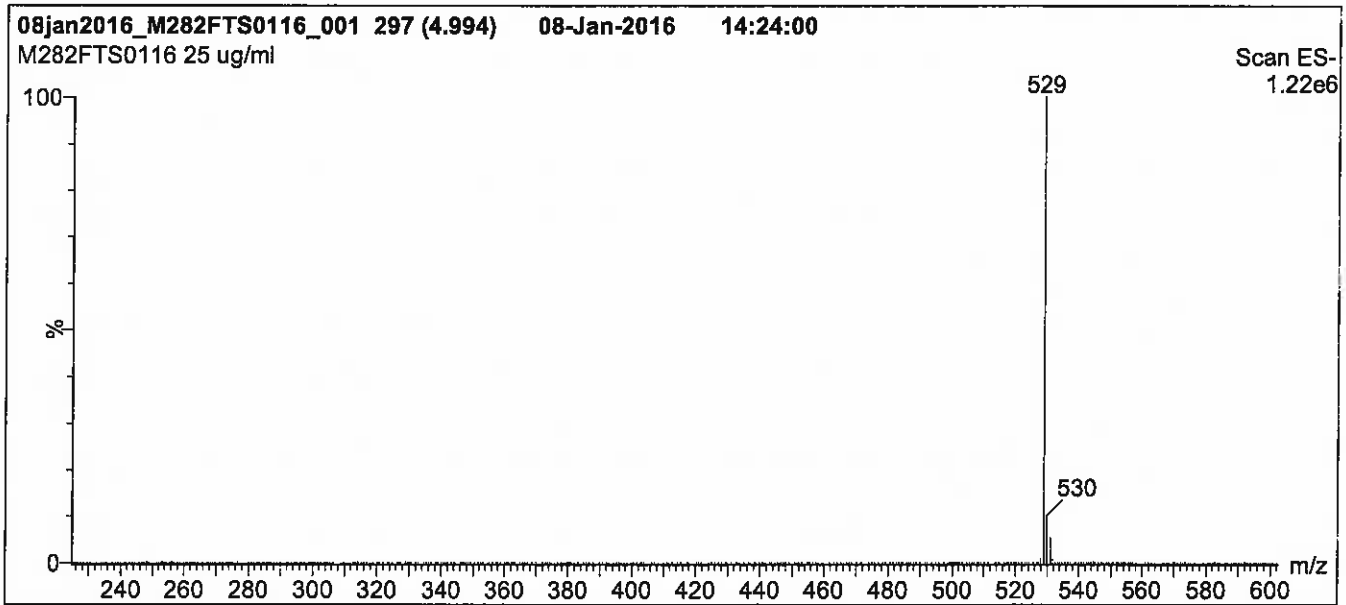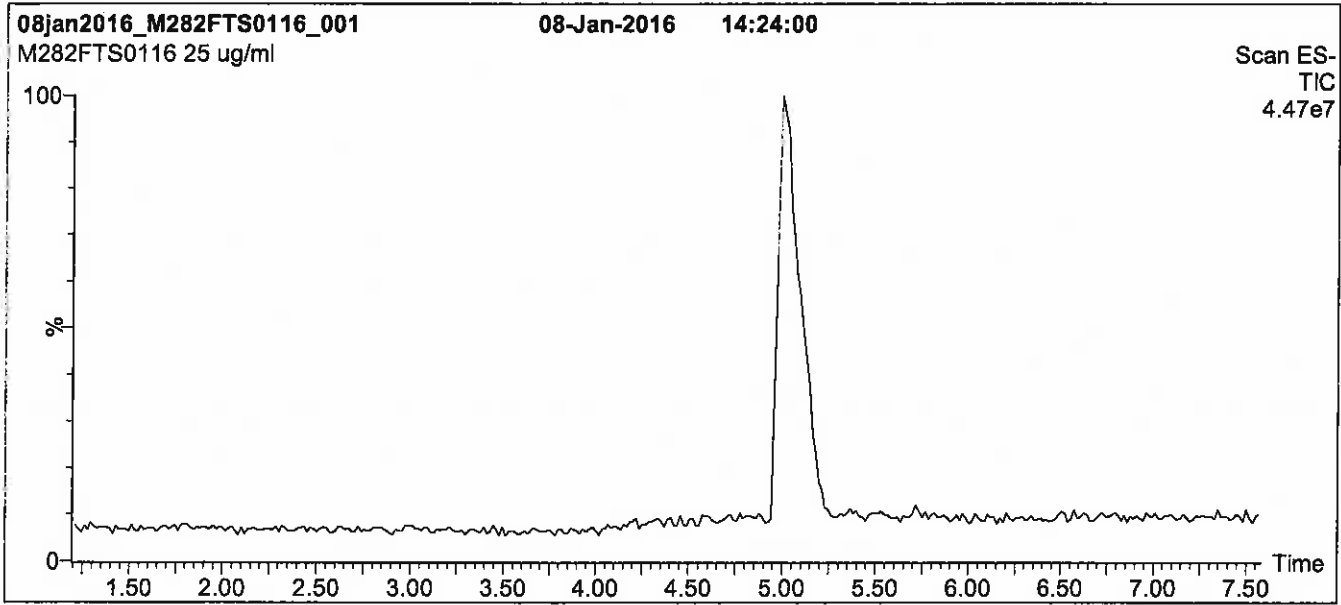

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min
and hold for 2 min before returning
to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 30.00
Cone Gas Flow (l/hr) = 100
Desolvation Gas Flow (l/hr) = 750

Figure 2: M2-8:2FTS; LC/MS/MS Data (Selected MRM Transitions)

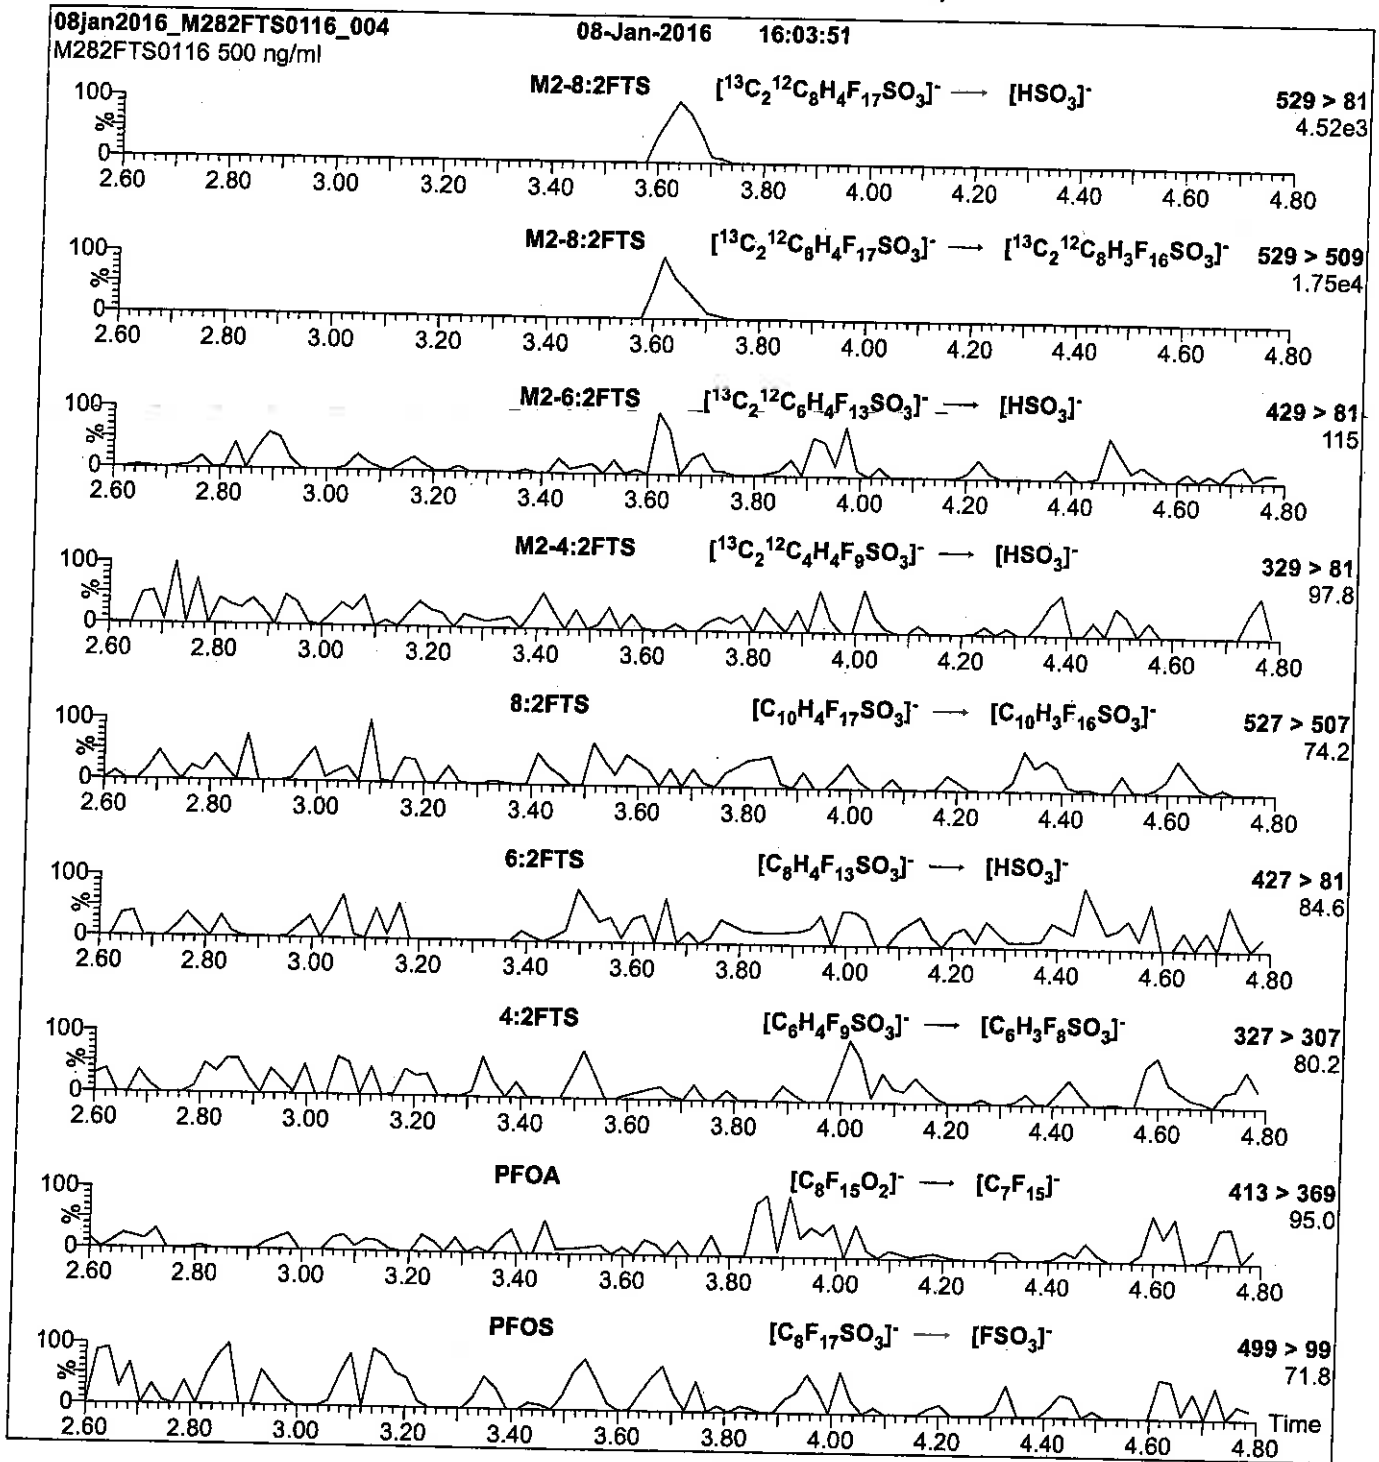

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml M2-8:2FTS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.20e-3
Collision Energy (eV) = 30

R: SBC 9/13/16



730511
ID: LCPFBS_00005
Exp: 03/15/21 Pripd: SBC
PF-1-butanesulfonate K sa




730512
ID: LCPFBS_00006
Exp: 03/15/21 Pripd: SBC
PF-1-butanesulfonate K sa



WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: L-PFBS **LOT NUMBER:** LPFBS0316
COMPOUND: Potassium perfluoro-1-butanesulfonate
STRUCTURE: **CAS #:** 29420-49-3



MOLECULAR FORMULA: C₄F₉SO₃K **MOLECULAR WEIGHT:** 338.19
CONCENTRATION: 50.0 ± 2.5 µg/ml (K salt) **SOLVENT(S):** Methanol
44.2 ± 2.2 µg/ml (PFBS anion)
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 03/15/2016
EXPIRY DATE: (mm/dd/yyyy) 03/15/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place


DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim Date: 03/21/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



****For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com****

Figure 1: L-PFBS; LC/MS Data (TIC and Mass Spectrum)

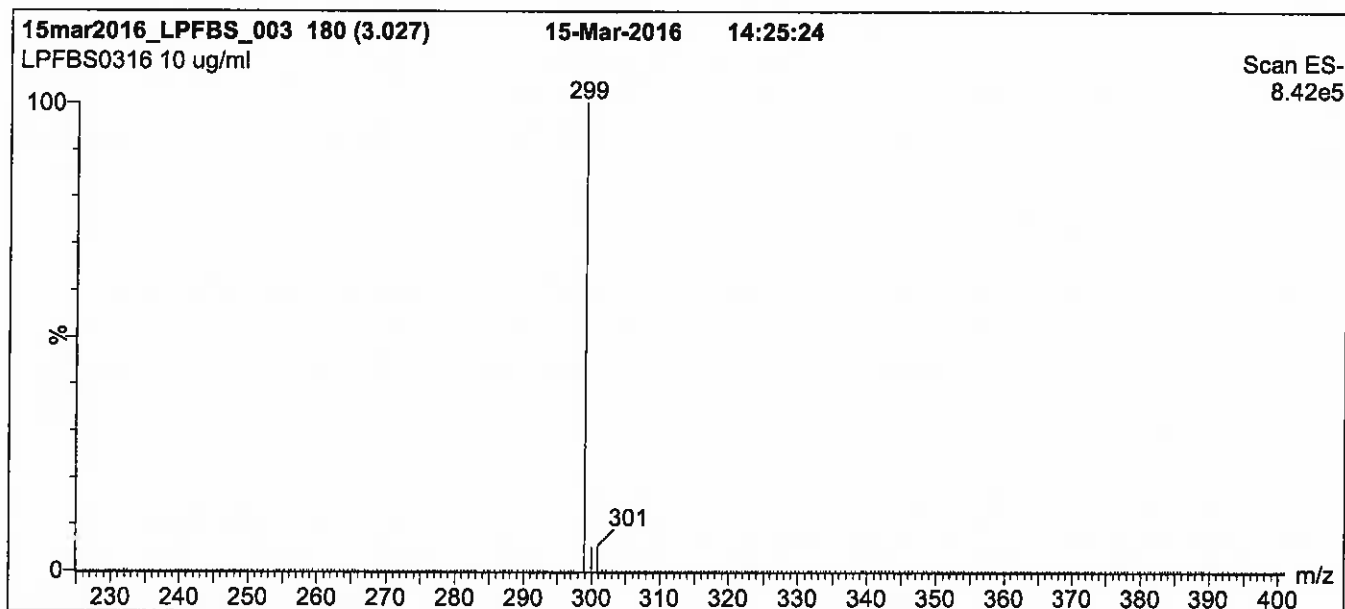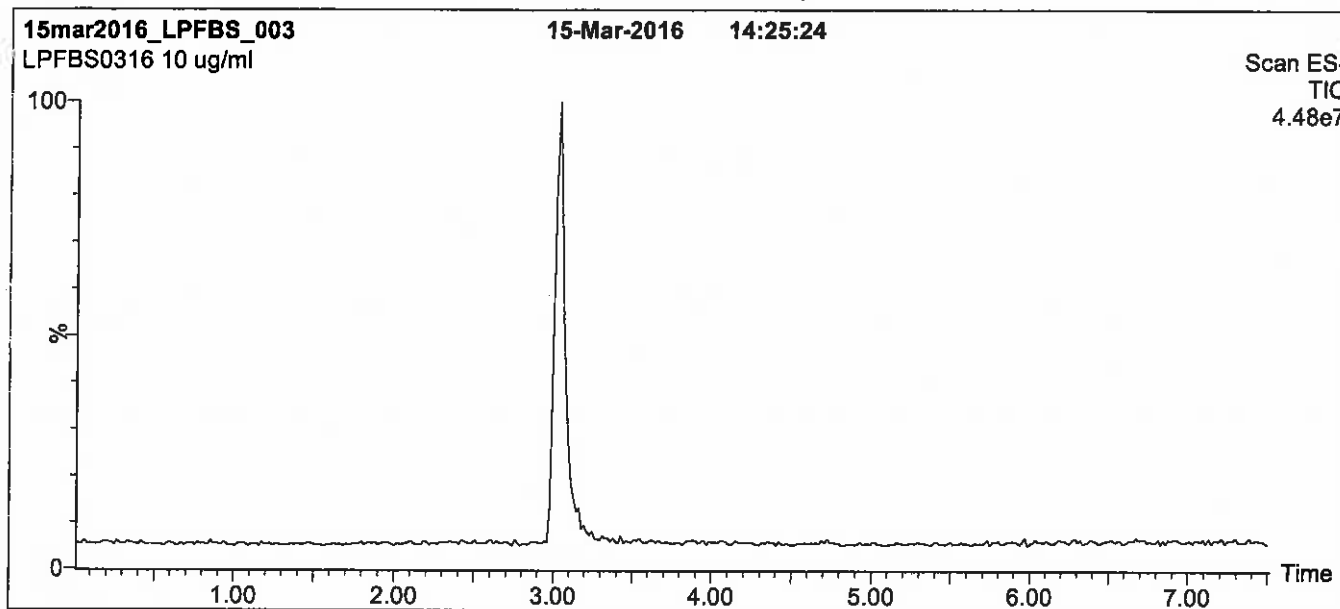

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 40% (80:20 MeOH:ACN) / 60% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 40.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: L-PFBS; LC/MS/MS Data (Selected MRM Transitions)

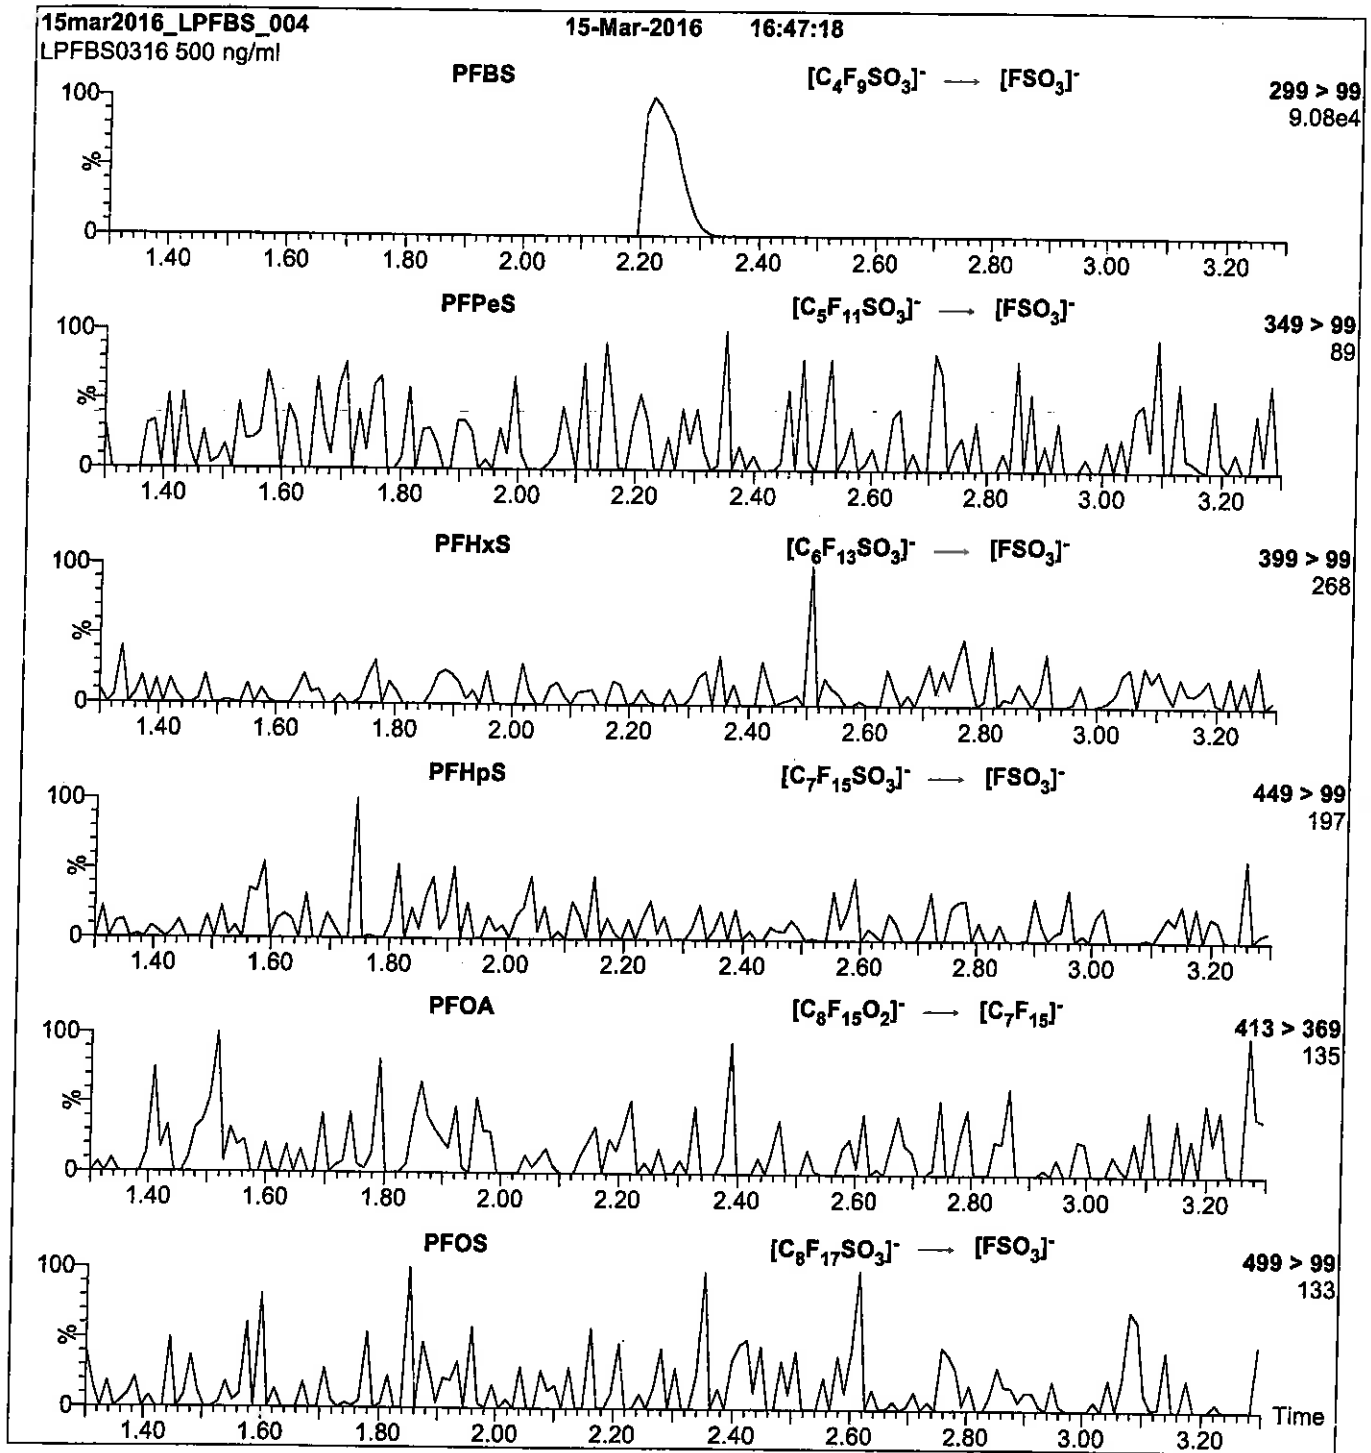

Conditions for Figure 2:

Injection: Direct loop injection
 10 μ l (500 ng/ml L-PFBS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.20e-3
 Collision Energy (eV) = 25

Reagent

LCPFDA_00005

R: 7/16/16 CBW



671576
ID: LCPFDA_00305
Exp: 07/02/20 Pipd: CBW
PF-n-decanoic acid




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: PFDA **LOT NUMBER:** PFDA0615
COMPOUND: Perfluoro-n-decanoic acid

STRUCTURE: **CAS #:** 335-76-2



MOLECULAR FORMULA: C₁₀H₁₉F₁₉O₂ **MOLECULAR WEIGHT:** 514.08
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Methanol
Water (<1%)
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 07/02/2015
EXPIRY DATE: (mm/dd/yyyy) 07/02/2020
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains ~ 0.6% PFNA and ~ 0.3% PFOA.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 07/24/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFDA; LC/MS Data (TIC and Mass Spectrum)

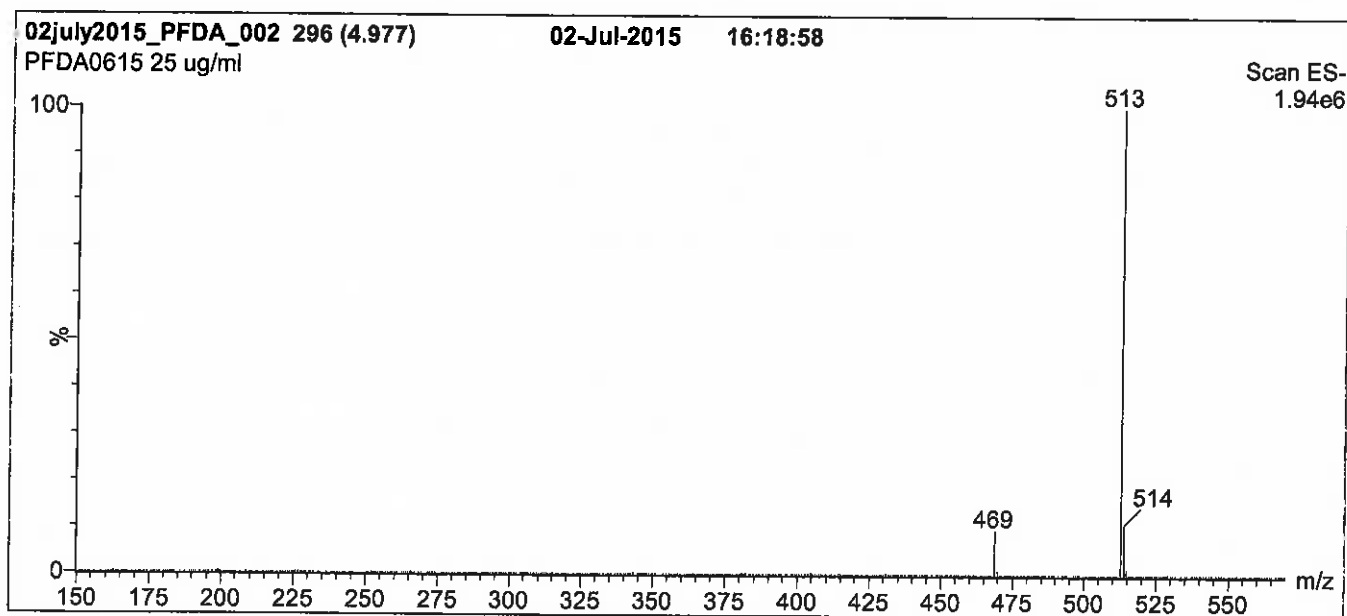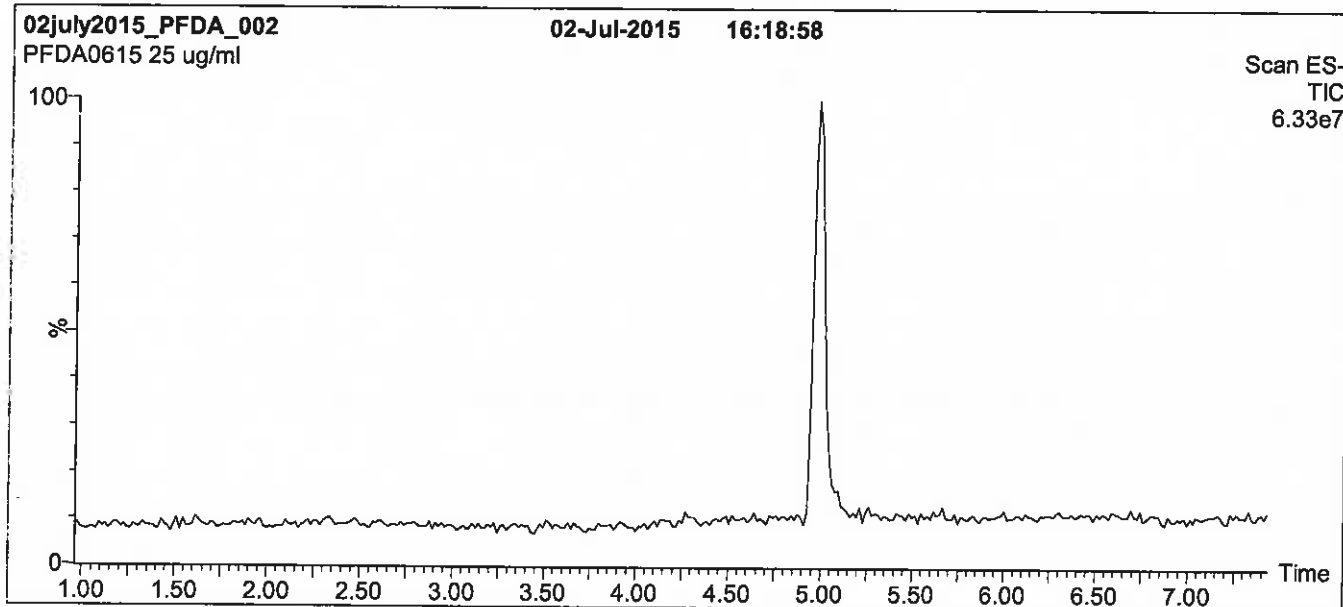

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for
2 min before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: PFDA; LC/MS/MS Data (Selected MRM Transitions)

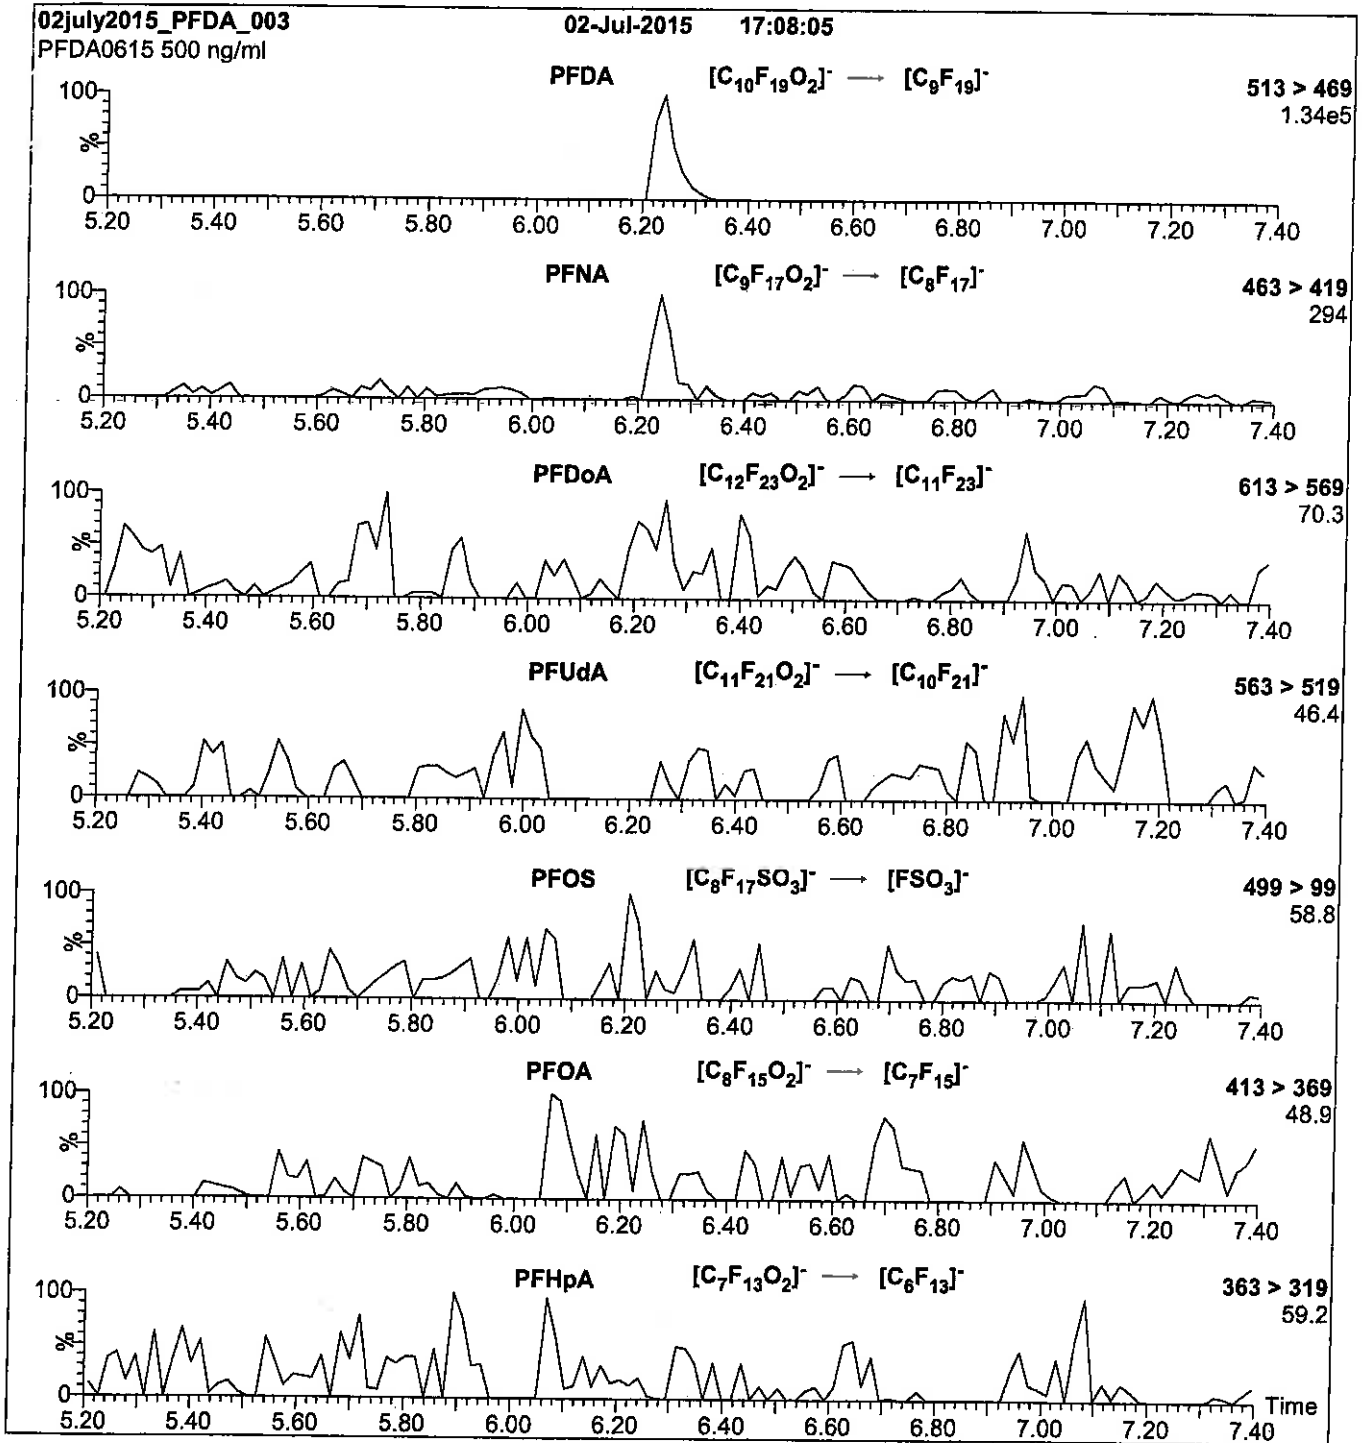

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml PFDA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.62e-3
Collision Energy (eV) = 13

Reagent

LCPFDoA_00005

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFD_oA; LC/MS Data (TIC and Mass Spectrum)

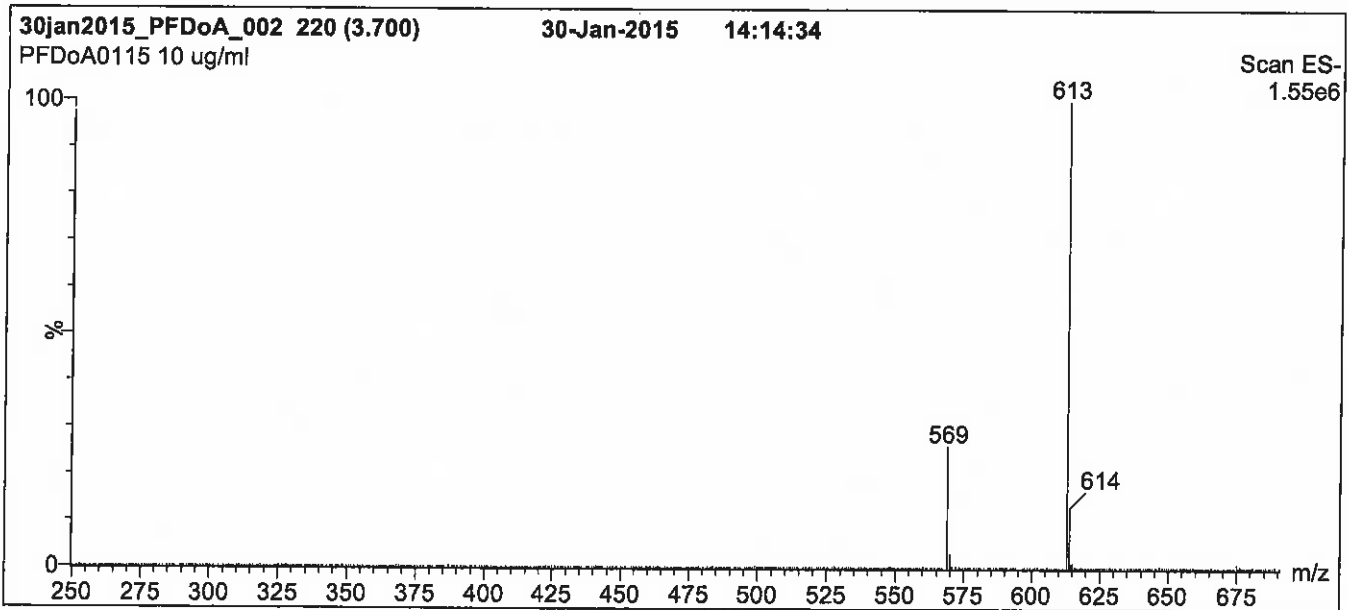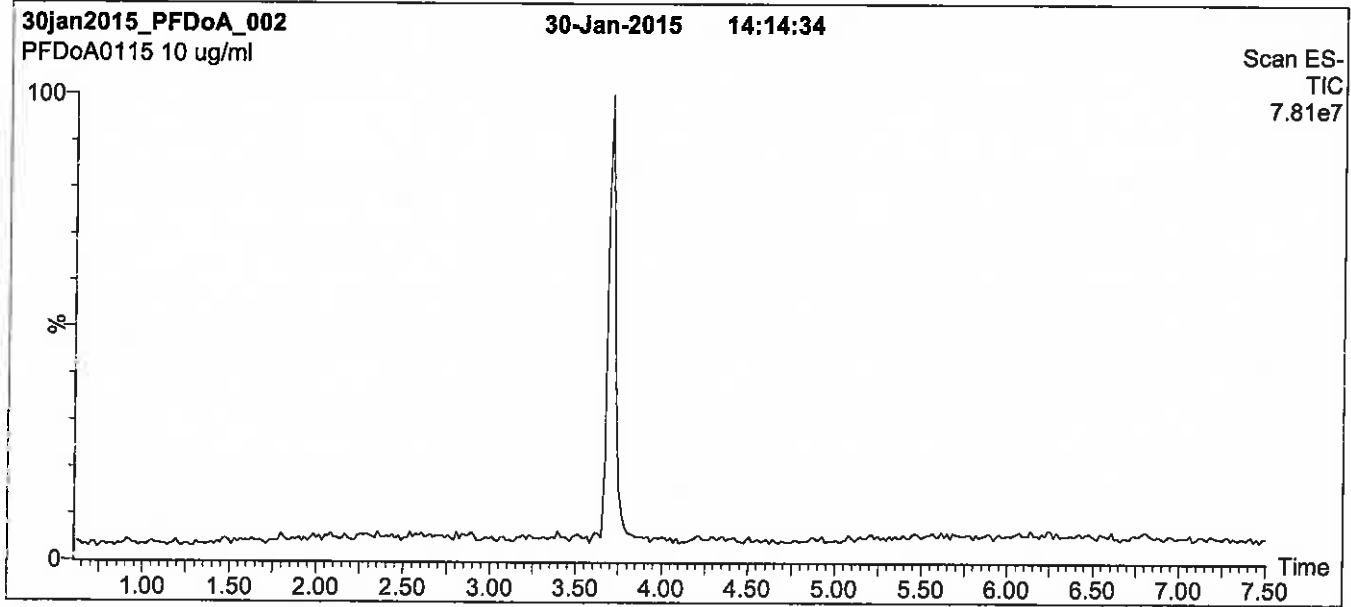

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 60% (80:20 MeOH:ACN) / 40% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (250 - 1000 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.00
 Cone Voltage (V) = 20.00
 Cone Gas Flow (l/hr) = 100
 Desolvation Gas Flow (l/hr) = 750

Figure 2: PFDoA; LC/MS/MS Data (Selected MRM Transitions)

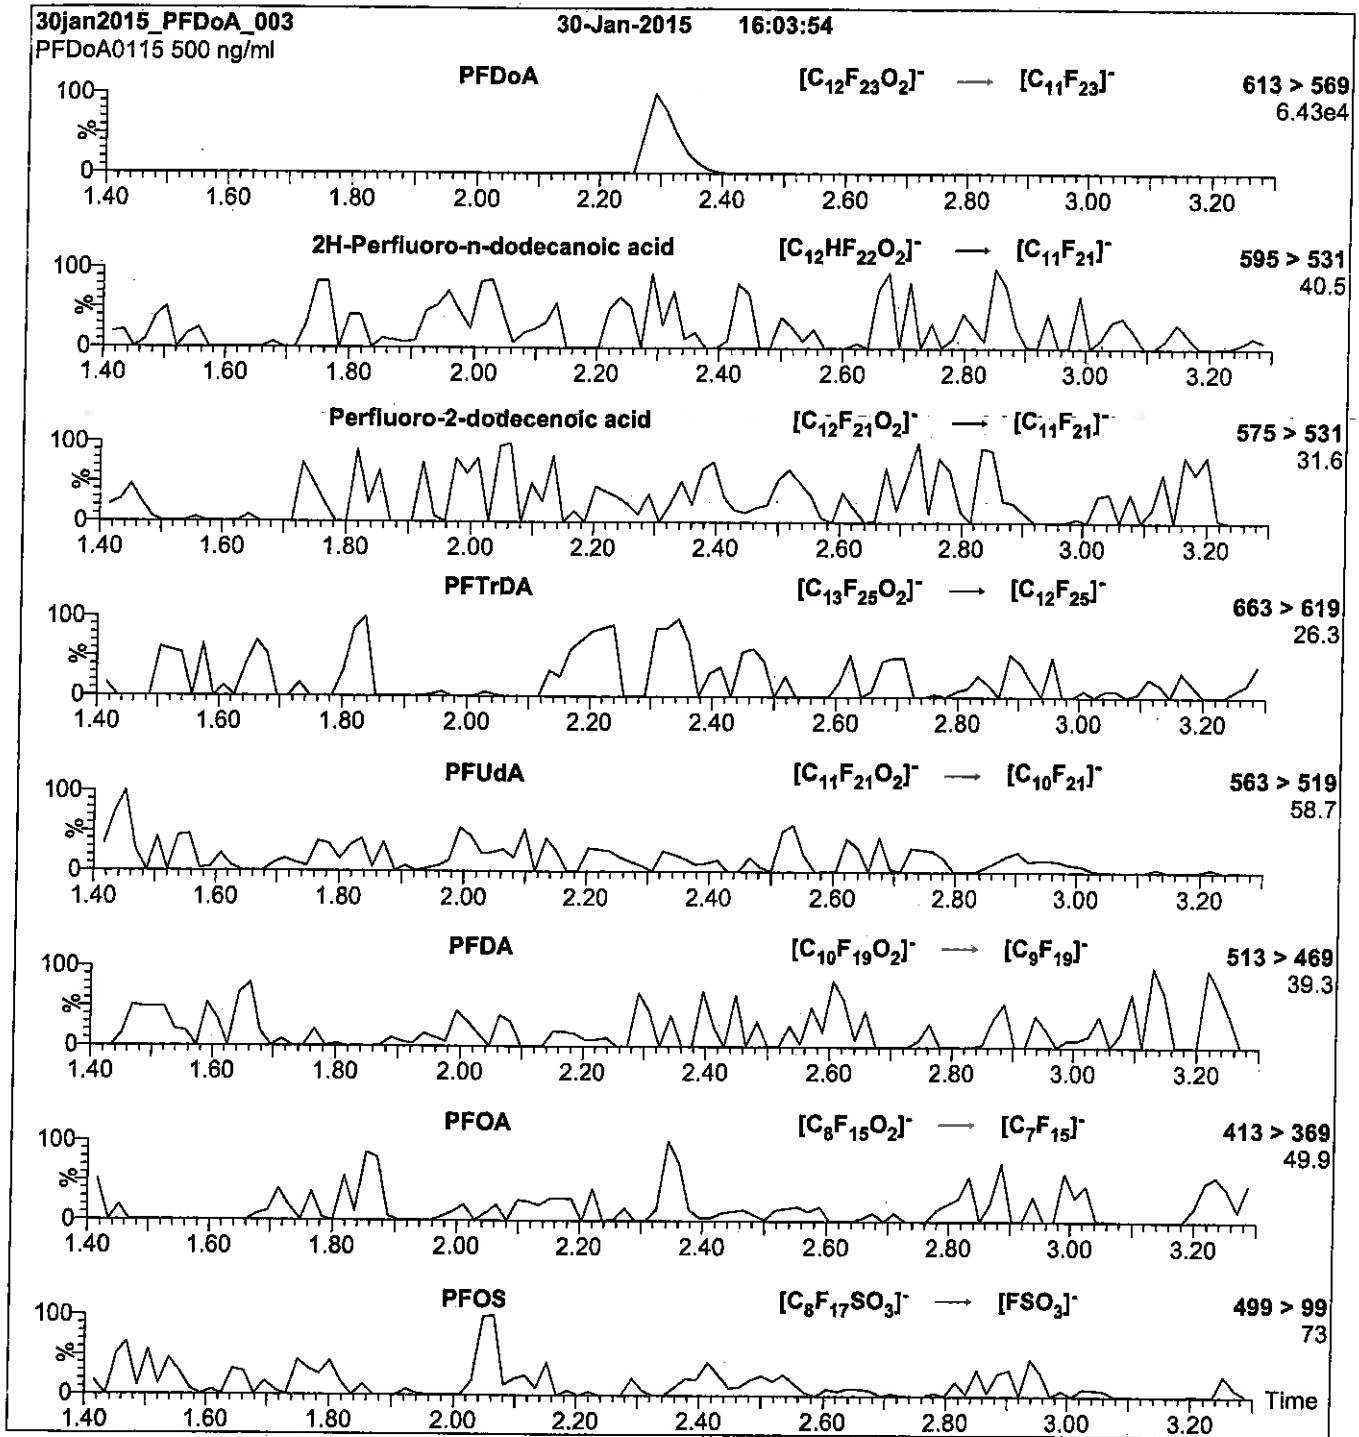

Conditions for Figure 2:

Injection: Direct loop injection
 10 μ l (500 ng/ml PFDoA)

MS Parameters

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)

Collision Gas (mbar) = 3.28e-3
 Collision Energy (eV) = 13

Flow: 300 μ l/min

Reagent

LCPFHpA_00005



609639

ID: LCPFHpA_00005

Exp: 01/22/21 Prpd: CBW

PF-n-heptanoic acid

R: 4/7/16 CBW



WELLINGTON LABORATORIES


CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: PFHpA
COMPOUND: Perfluoro-n-heptanoic acid

LOT NUMBER: PFHpA0116

STRUCTURE:

CAS #: 375-85-9

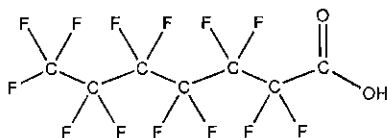

MOLECULAR FORMULA: C₇HF₁₃O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 364.06
SOLVENT(S): Methanol
Water (<1%)

CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 01/22/2016
EXPIRY DATE: (mm/dd/yyyy) 01/22/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:

B.G. Chittim

Date: 02/02/2016

(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON 'N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFHpA; LC/MS Data (TIC and Mass Spectrum)

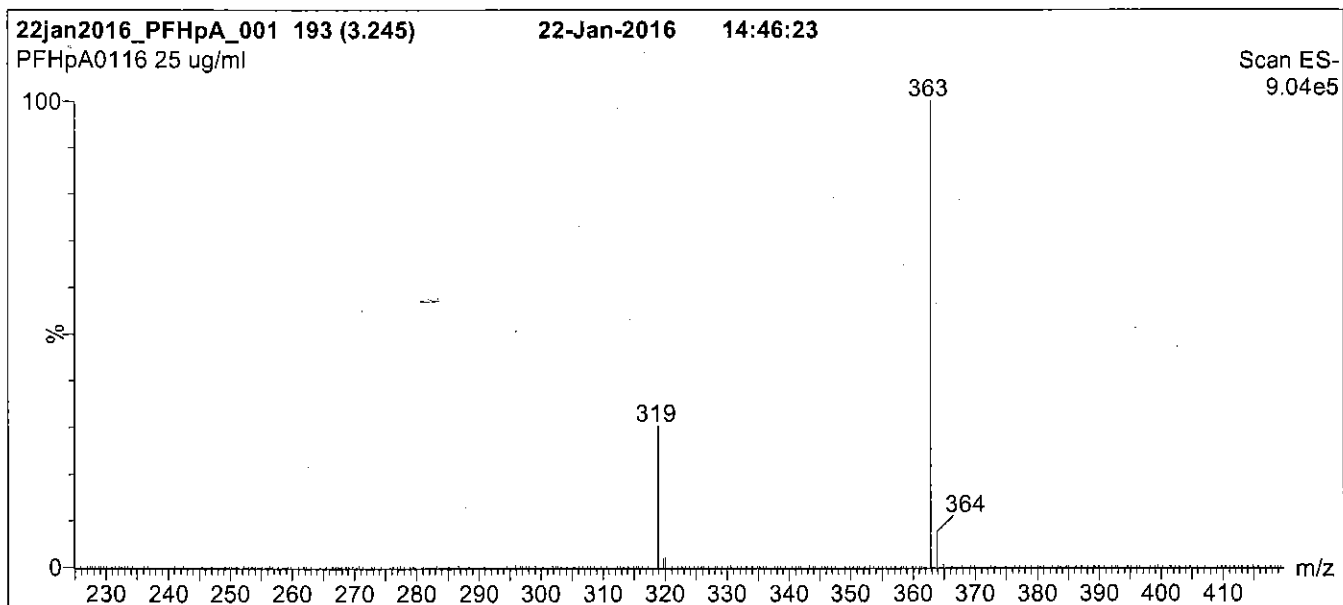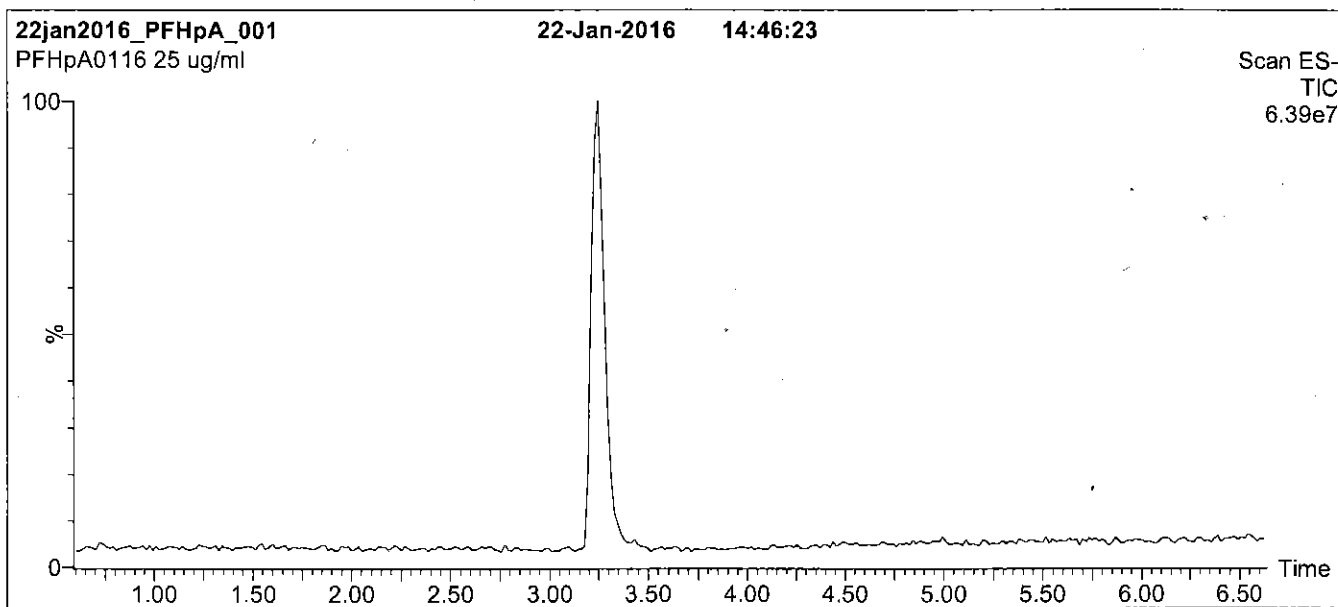

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 55% (80:20 MeOH:ACN) / 45% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for
 2 min before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.00
 Cone Voltage (V) = 15.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: PFHpA; LC/MS/MS Data (Selected MRM Transitions)

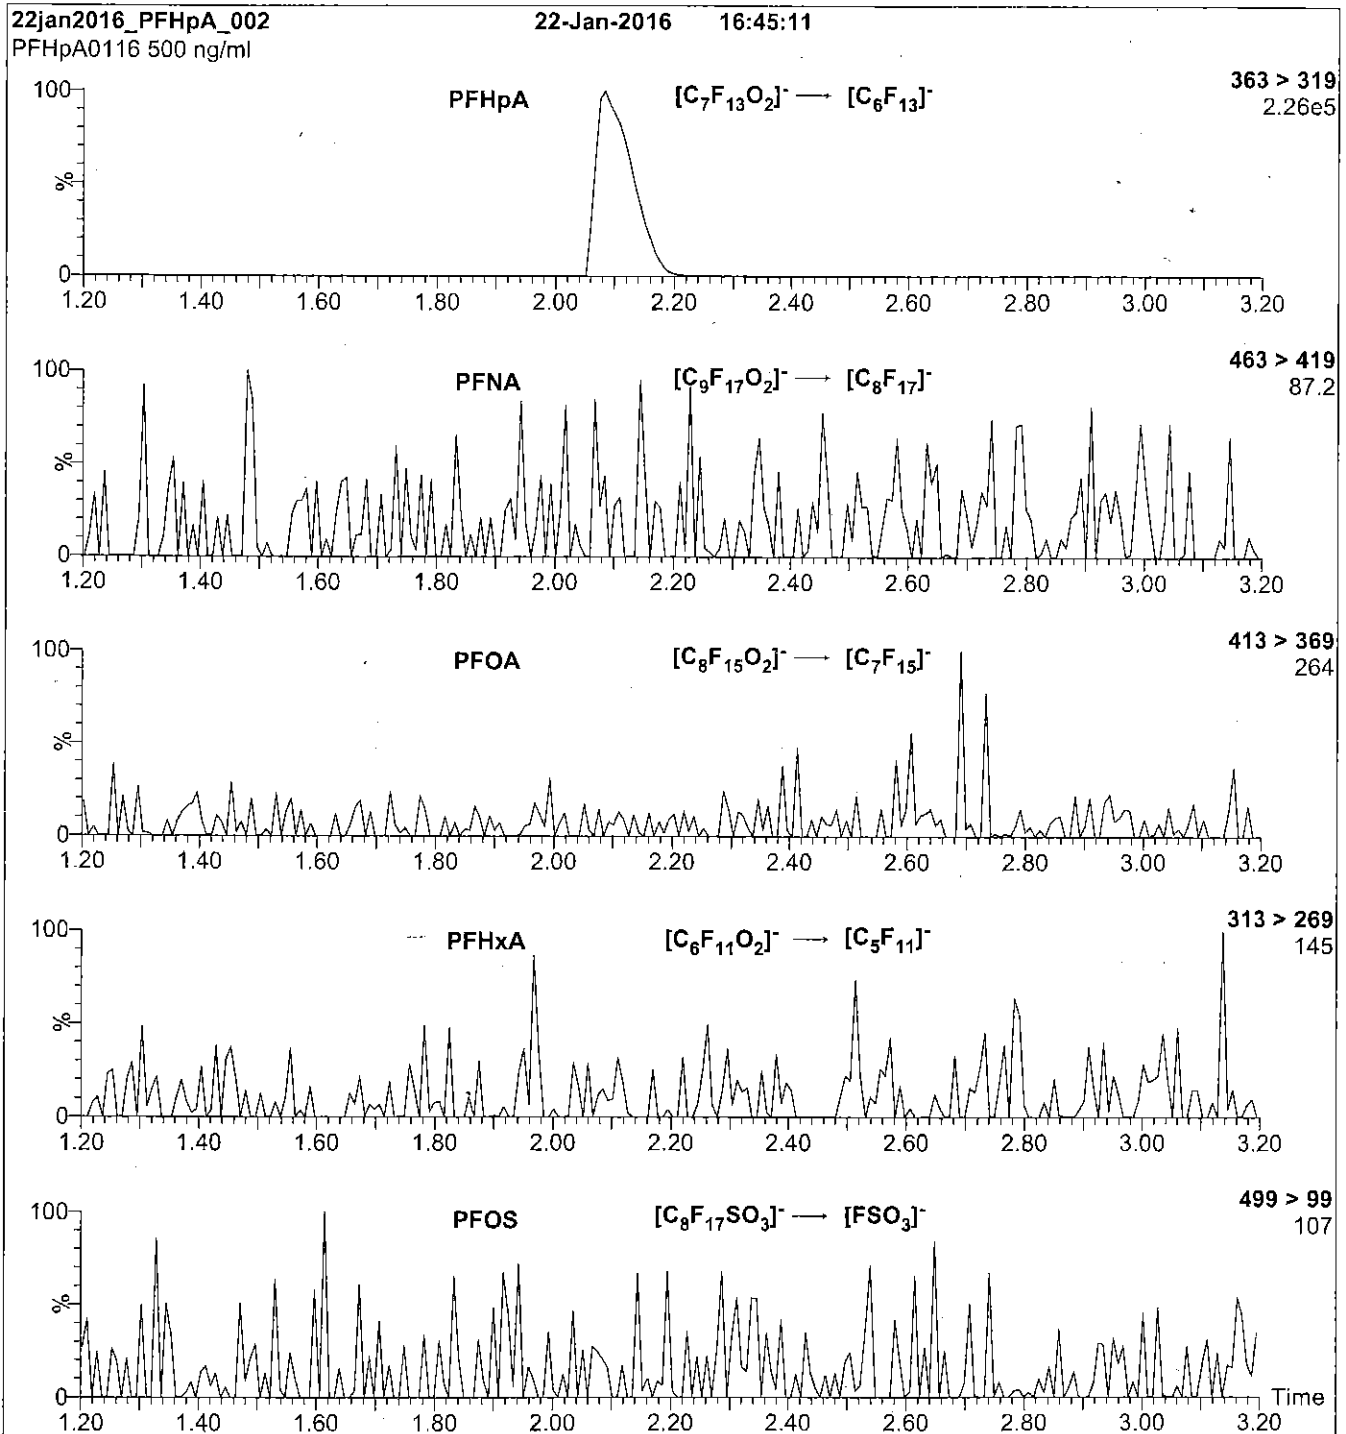

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml PFHpA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.50e-3
Collision Energy (eV) = 11

Reagent

LCPFHpA_00006

Scanned R: SBC 9/13/16
10/14/16 JK



730517
ID: LCPFHpa_00006
Exp: 01/22/21 Prpd: SBC
PF-n-heptanoic acid



730518
ID: LCPFHpa_00007
Exp: 01/22/21 Prpd: SBC
PF-n-heptanoic acid



WELLINGTON LABORATORIES


CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: PFHpA
COMPOUND: Perfluoro-n-heptanoic acid

LOT NUMBER: PFHpA0116

STRUCTURE:

CAS #: 375-85-9



MOLECULAR FORMULA: C₇HF₁₃O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 364.06
SOLVENT(S): Methanol
Water (<1%)

CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 01/22/2016
EXPIRY DATE: (mm/dd/yyyy) 01/22/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim

Date: 02/02/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFHpA; LC/MS Data (TIC and Mass Spectrum)

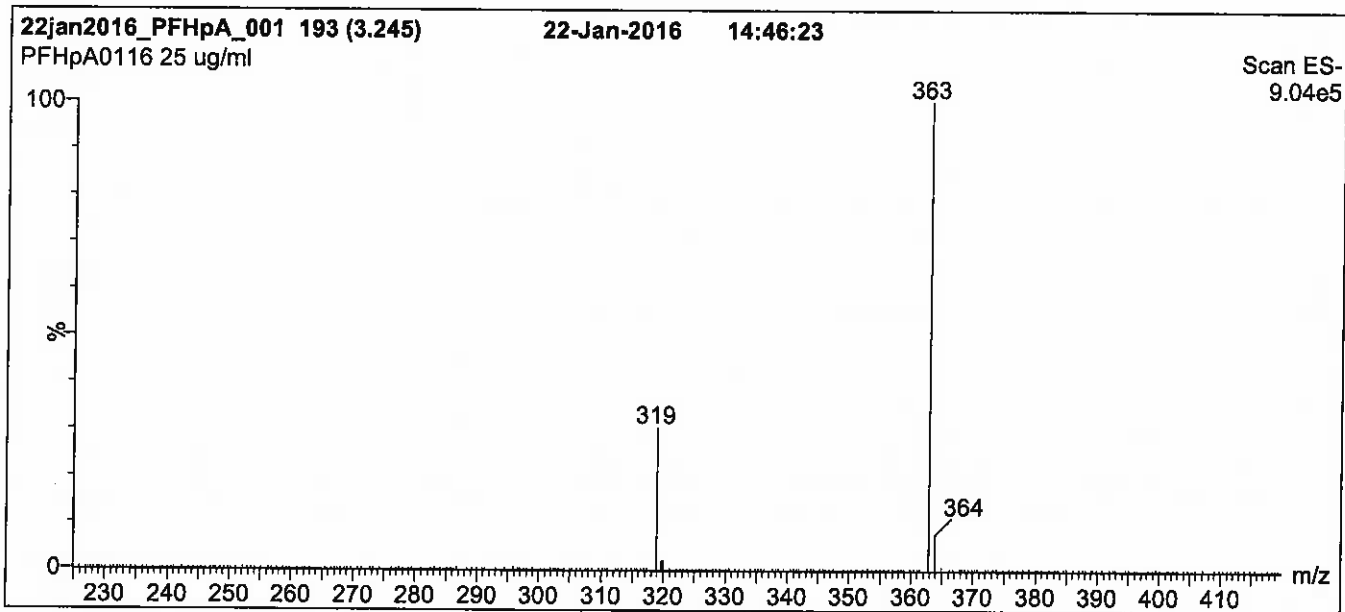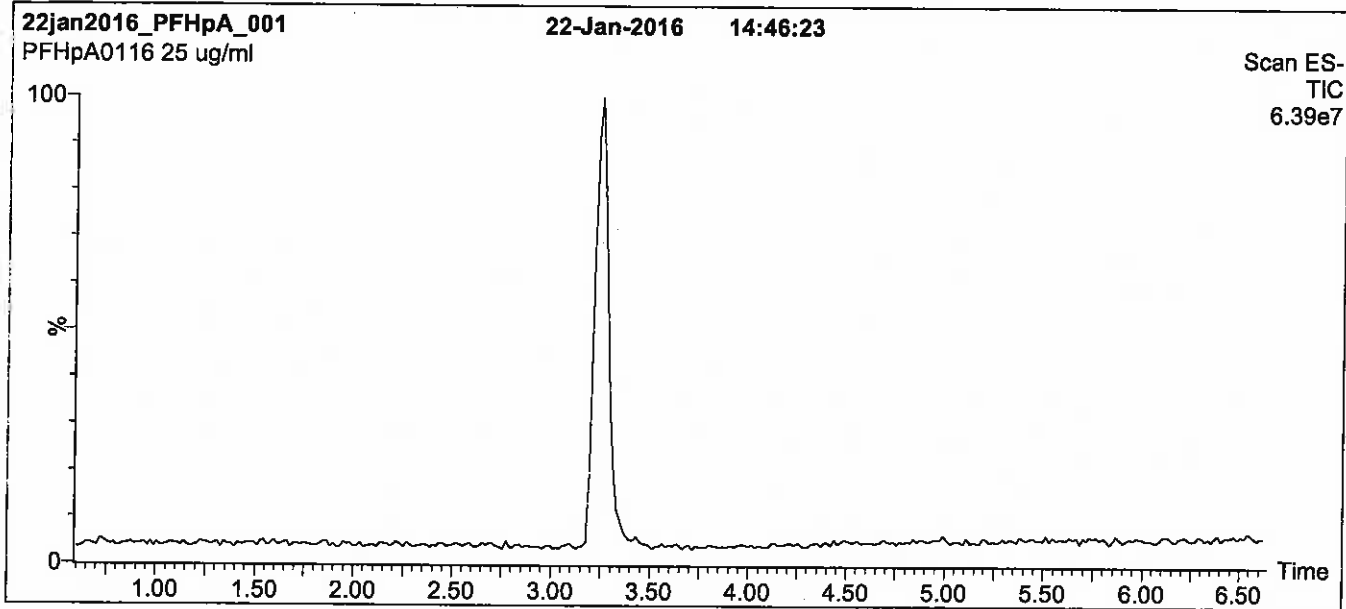

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 55% (80:20 MeOH:ACN) / 45% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for
2 min before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: PFHpA; LC/MS/MS Data (Selected MRM Transitions)

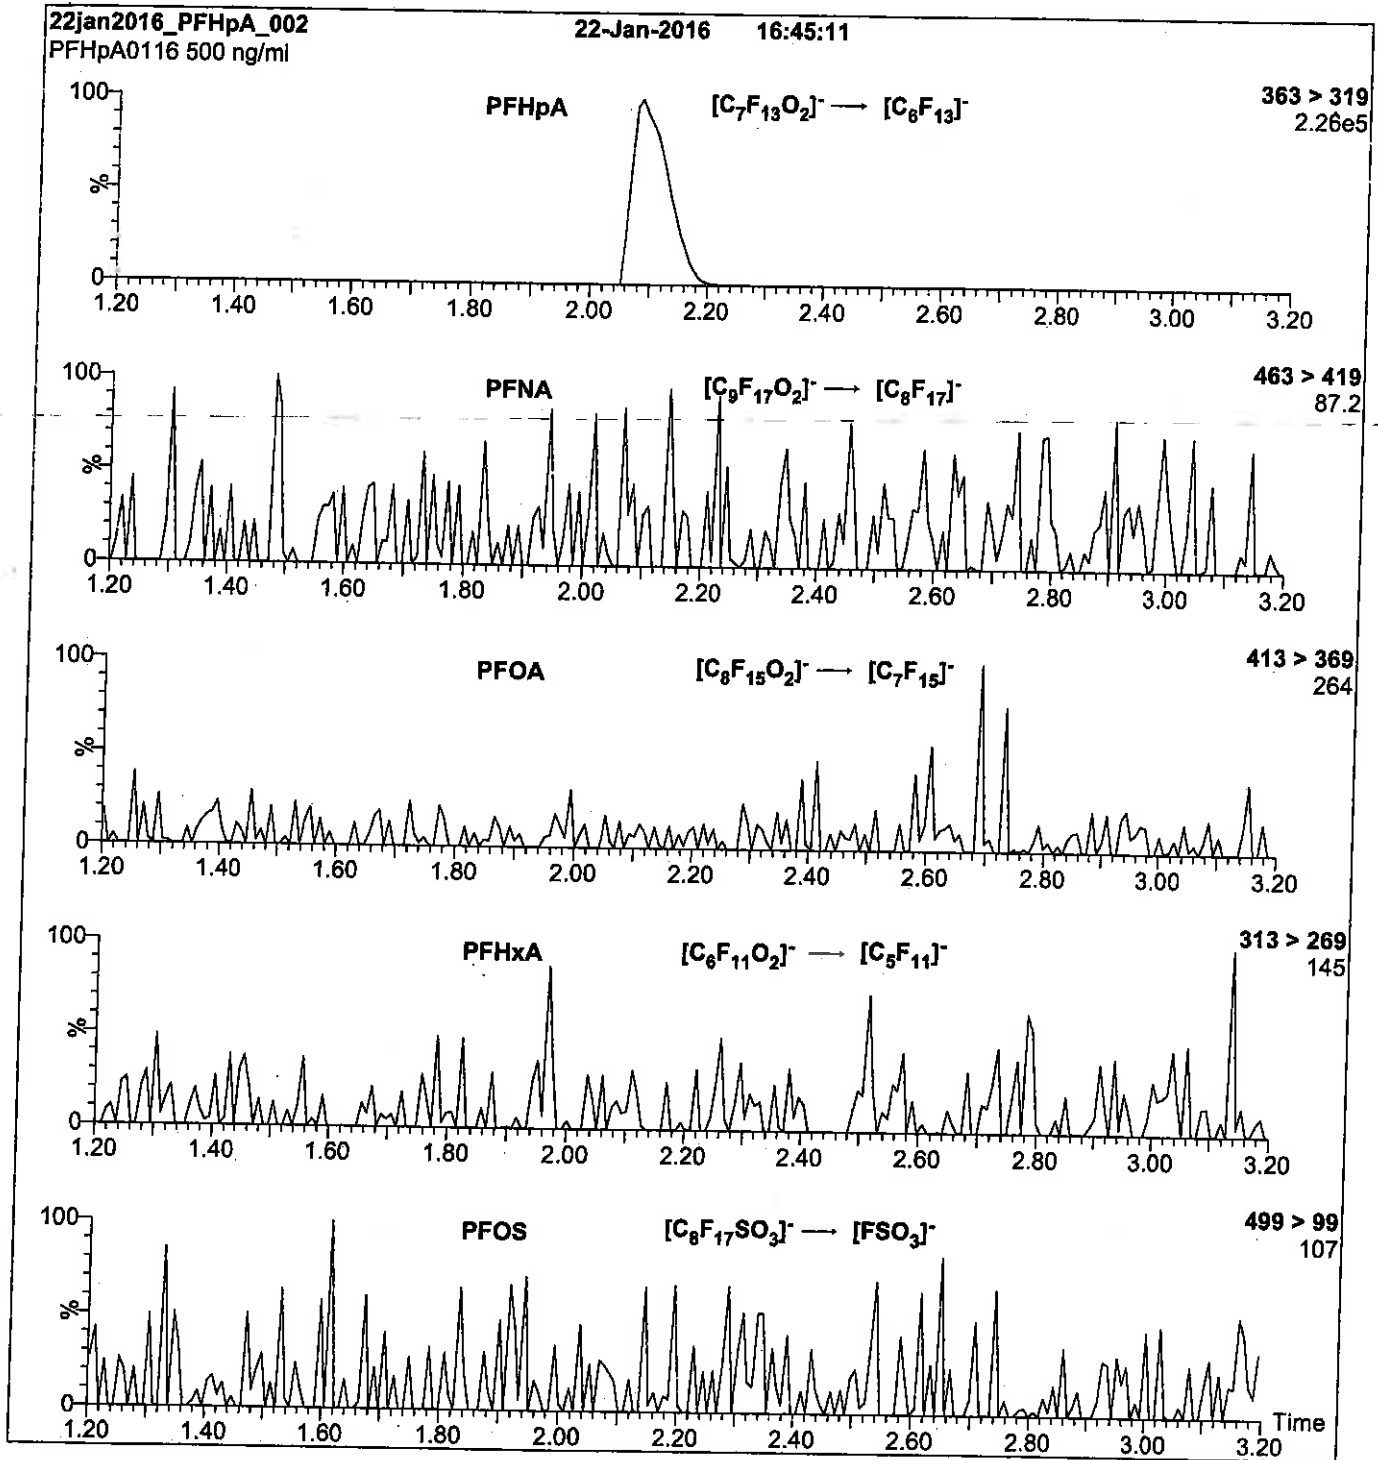

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml PFHpA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.50e-3
Collision Energy (eV) = 11

Reagent

LCPFHpS_00009

Scanned
10/14/16 SP
R: 8BC 9/13/16



730635
ID: LCPFHpS_00009
Exp: 11/06/20 Prpd: SBC
PFHpS at 47.6ug/mL



730639
ID: LCPFHpS_00010
Exp: 11/06/20 Prpd: SBC
PFHpS at 47.6ug/mL




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: L-PFHpS **LOT NUMBER:** LPFHpS1115
COMPOUND: Sodium perfluoro-1-heptanesulfonate

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: C₇F₁₅SO₃Na **MOLECULAR WEIGHT:** 472.10
CONCENTRATION: 50.0 ± 2.5 µg/ml (Na salt) **SOLVENT(S):** Methanol
47.6 ± 2.4 µg/ml (PFHpS anion)
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 11/06/2015
EXPIRY DATE: (mm/dd/yyyy) 11/06/2020
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains ~ 0.1% of L-PFHxS (C₆F₁₃SO₃Na) and ~ 0.2% of L-PFOS (C₈F₁₇SO₃Na).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:

B.G. Chittim

Date: 11/09/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to International Interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: L-PFHpS; LC/MS Data (TIC and Mass Spectrum)

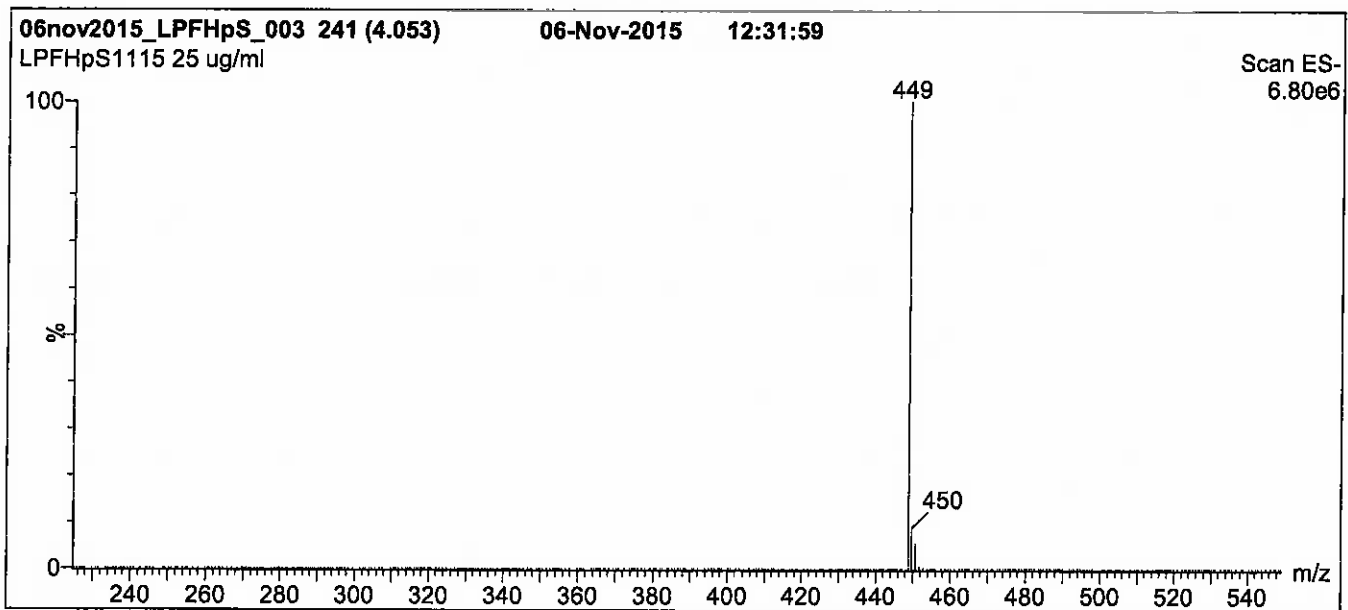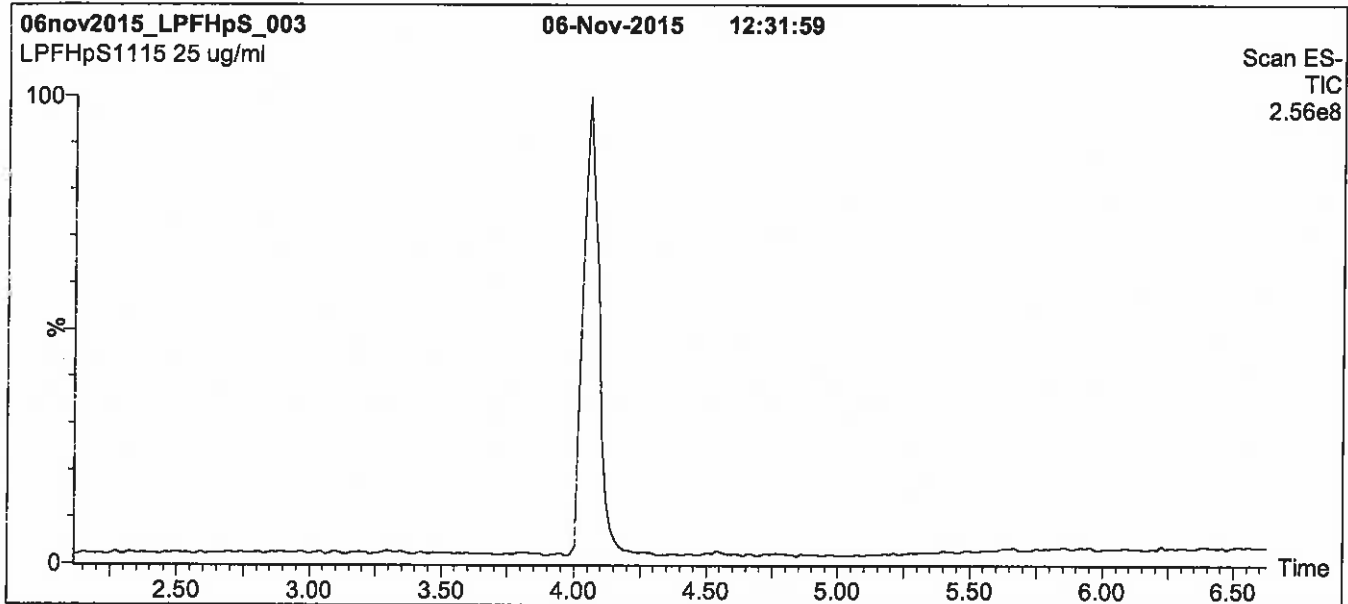

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈,
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 50% (80:20 MeOH:ACN) / 50% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold
 for 2 min before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.00
 Cone Voltage (V) = 60.00
 Cone Gas Flow (l/hr) = 60
 Desolvation Gas Flow (l/hr) = 750

Figure 2: L-PFHpS; LC/MS/MS Data (Selected MRM Transitions)

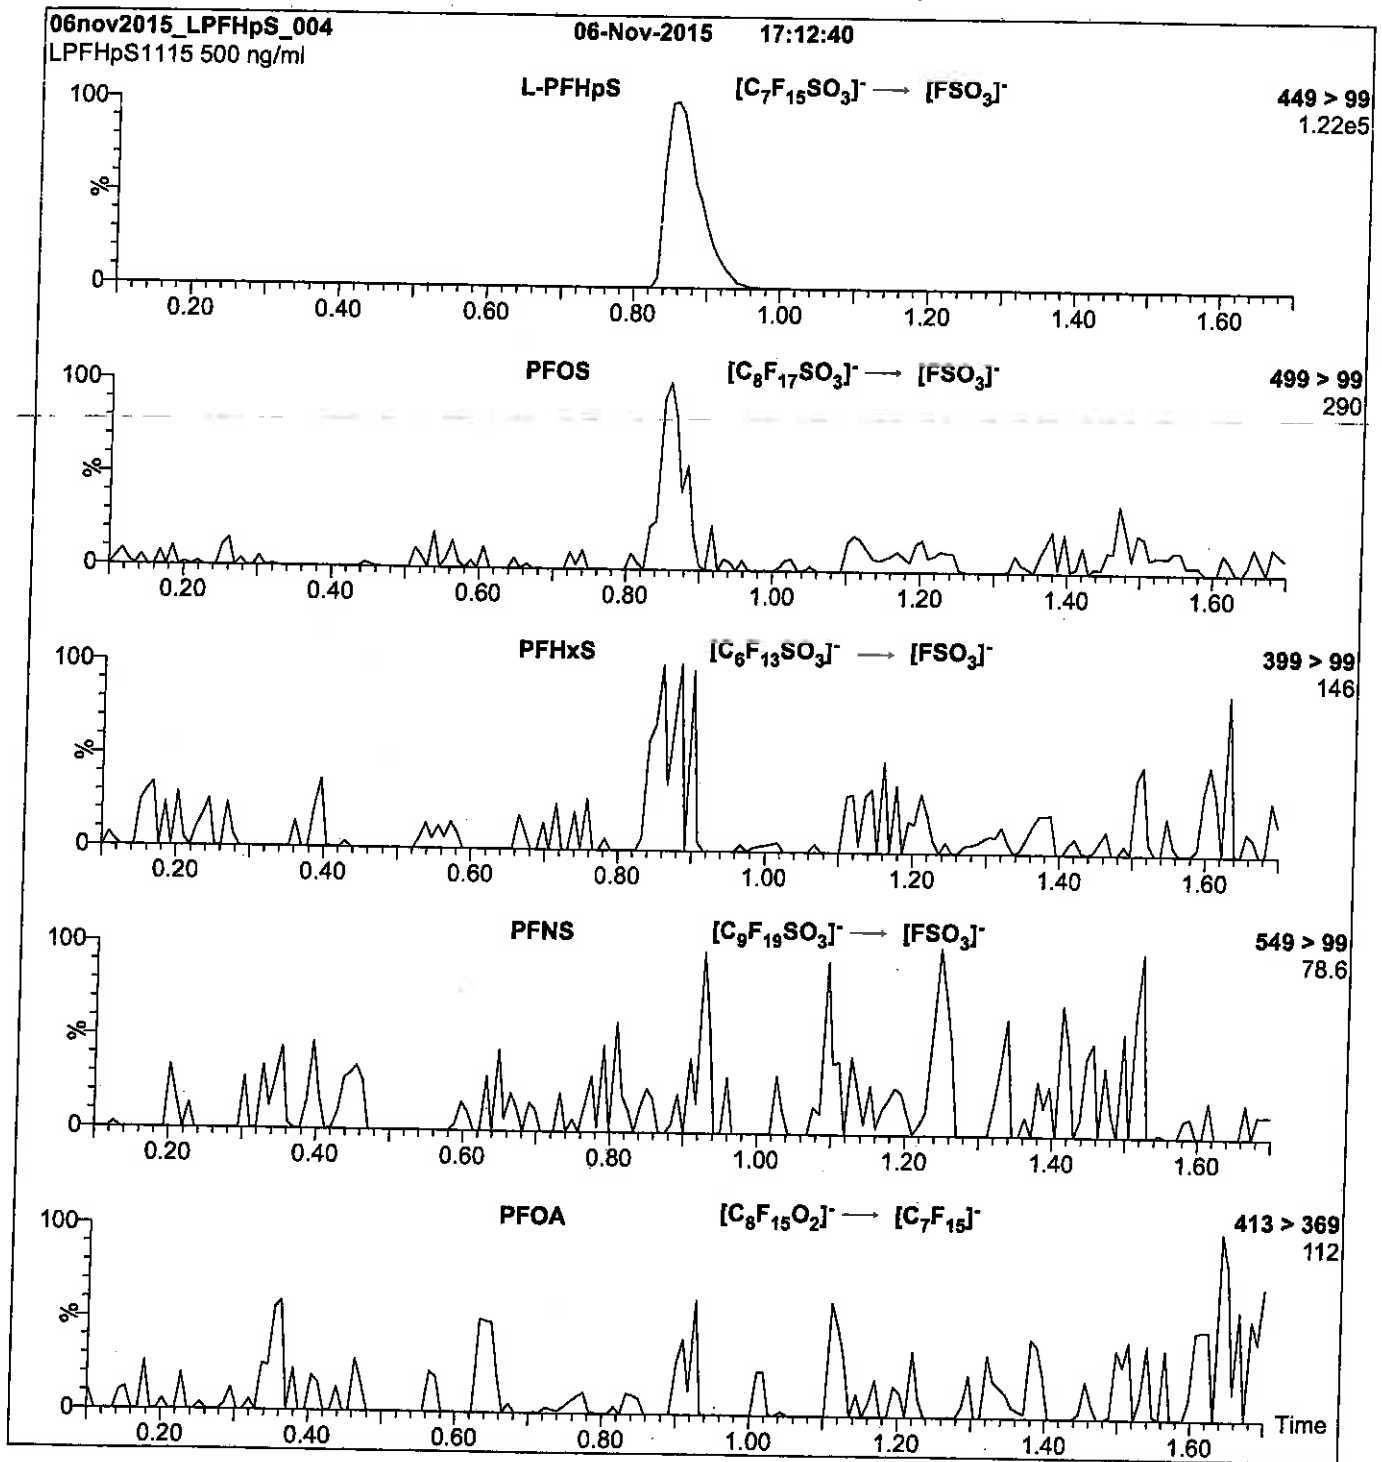

Conditions for Figure 2:

Injection: Direct loop injection
 10 μ l (500 ng/ml L-PFHpS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.31e-3
 Collision Energy (eV) = 35

Reagent

LCPFHxA_00004

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFHxA; LC/MS Data (TIC and Mass Spectrum)

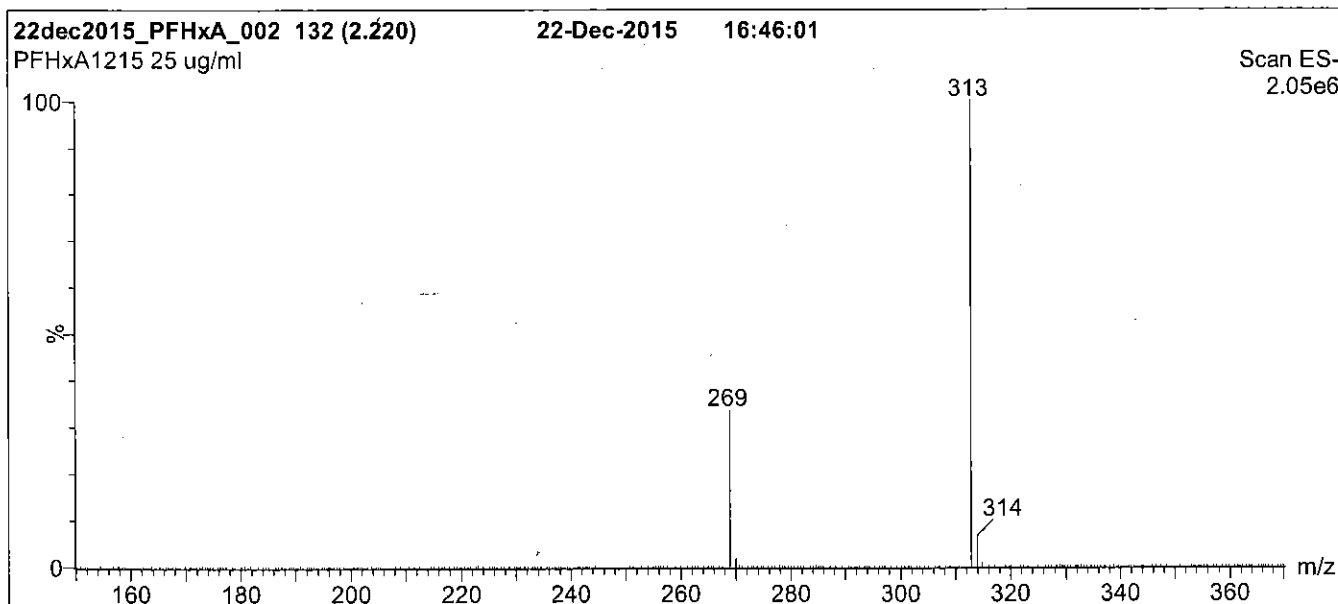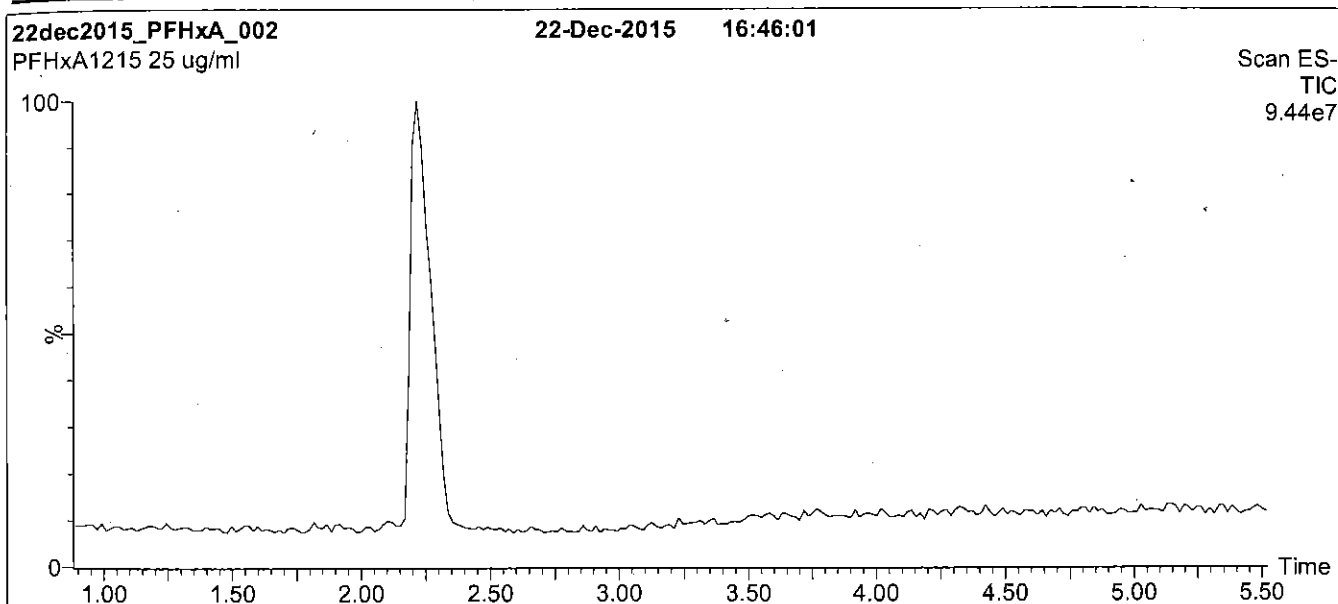

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 2 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 100
Desolvation Gas Flow (l/hr) = 750

Figure 2: PFHxA; LC/MS/MS Data (Selected MRM Transitions)

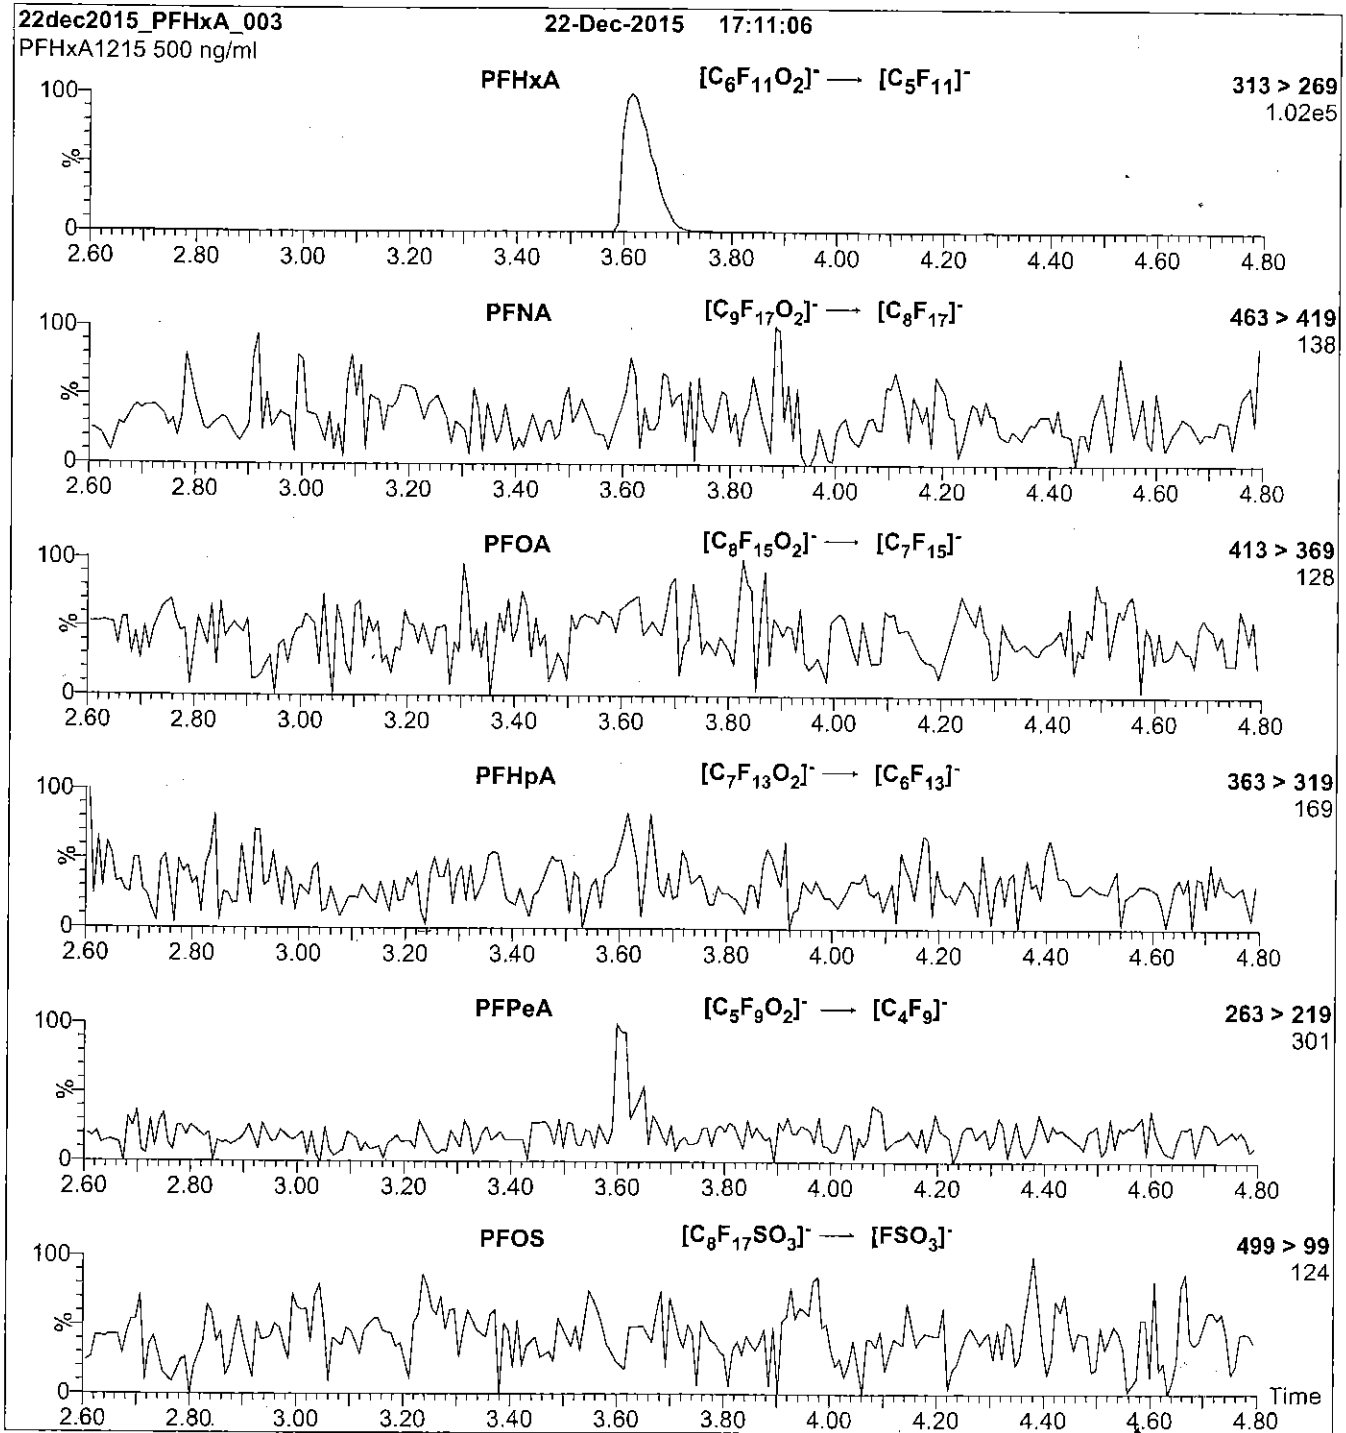

Conditions for Figure 2:

Injection: Direct loop injection
 10 μ l (500 ng/ml PFHxA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.43e-3
 Collision Energy (eV) = 10

Reagent

LCPFHxA_00005

R: 832 9/13/16



730551
ID: LCPFHxA_00005
Exp: 12/22/20 Prod: SBC
PF-n-hexanoic acid



730552
ID: LCPFHxA_00006
Exp: 12/22/20 Prod: SBC
PF-n-hexanoic acid




WELLINGTON
LABORATORIES

CERTIFICATE OF ANALYSIS
DOCUMENTATION

PRODUCT CODE: PFHxA **LOT NUMBER:** PFHxA1215
COMPOUND: Perfluoro-n-hexanoic acid

STRUCTURE: **CAS #:** 307-24-4



MOLECULAR FORMULA: $C_6HF_{11}O_2$ **MOLECULAR WEIGHT:** 314.05
CONCENTRATION: $50 \pm 2.5 \mu\text{g/ml}$ **SOLVENT(S):** Methanol
Water (<1%)
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 12/22/2015
EXPIRY DATE: (mm/dd/yyyy) 12/22/2020
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains ~ 0.2% of Perfluoro-n-pentanoic acid (PFPeA).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:

B.G. Chittim

Date: 12/23/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFHxA; LC/MS Data (TIC and Mass Spectrum)

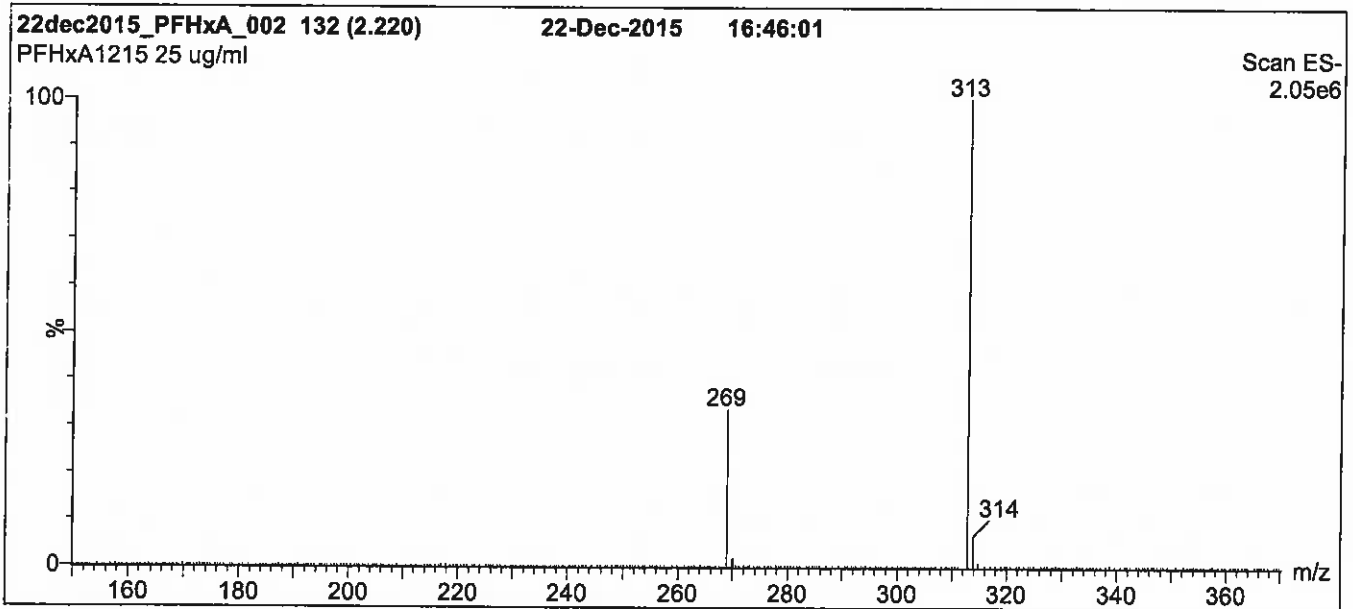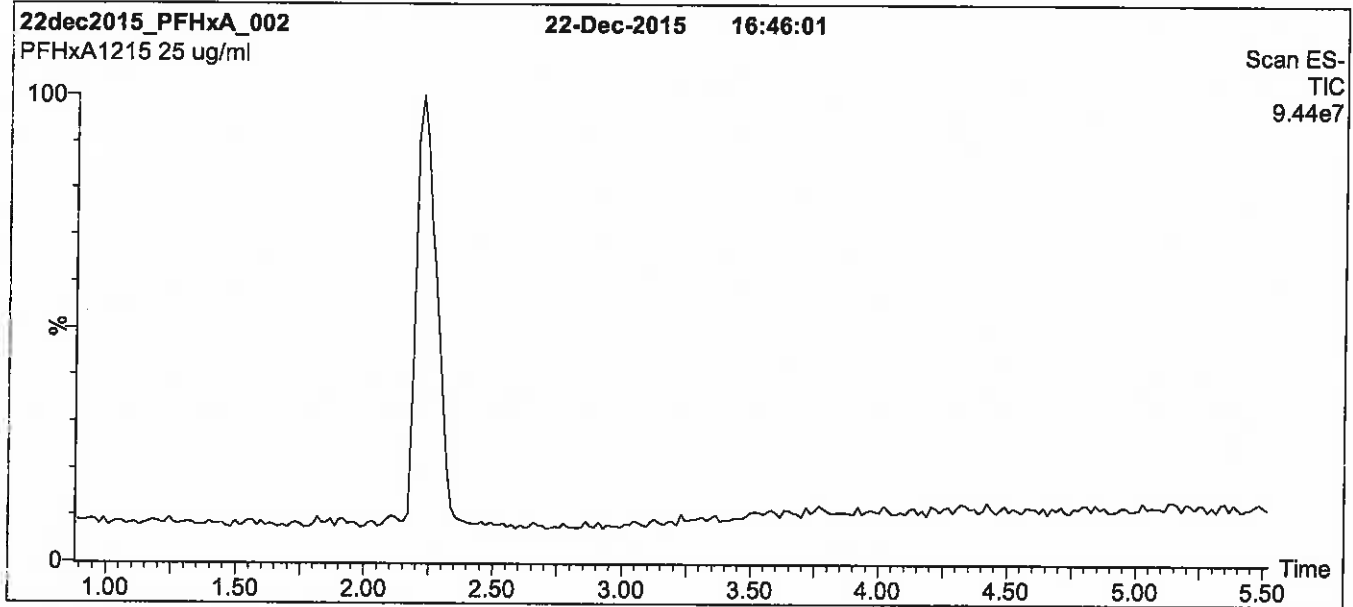

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 2 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 100
Desolvation Gas Flow (l/hr) = 750

Figure 2: PFHxA; LC/MS/MS Data (Selected MRM Transitions)

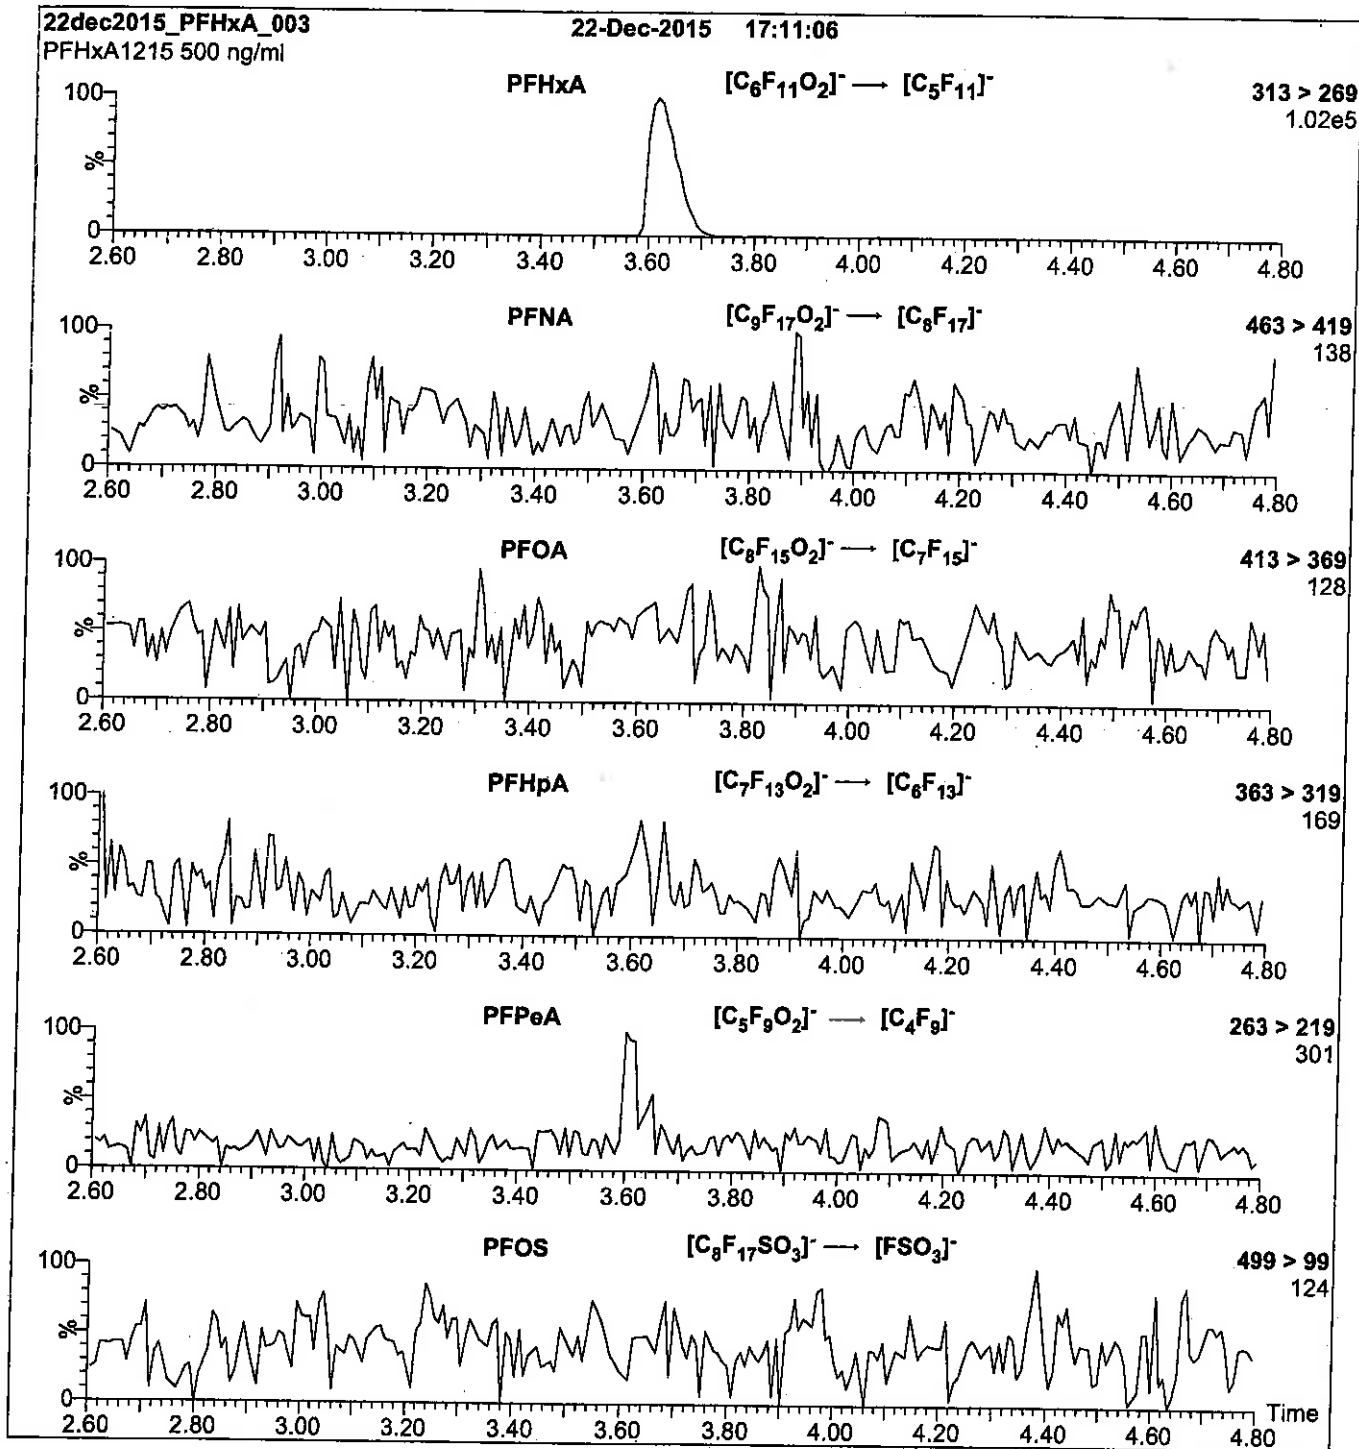

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml PFHxA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.43e-3
Collision Energy (eV) = 10

Reagent

LCPFHxDA_00006

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFHxDA; LC/MS Data (TIC and Mass Spectrum)

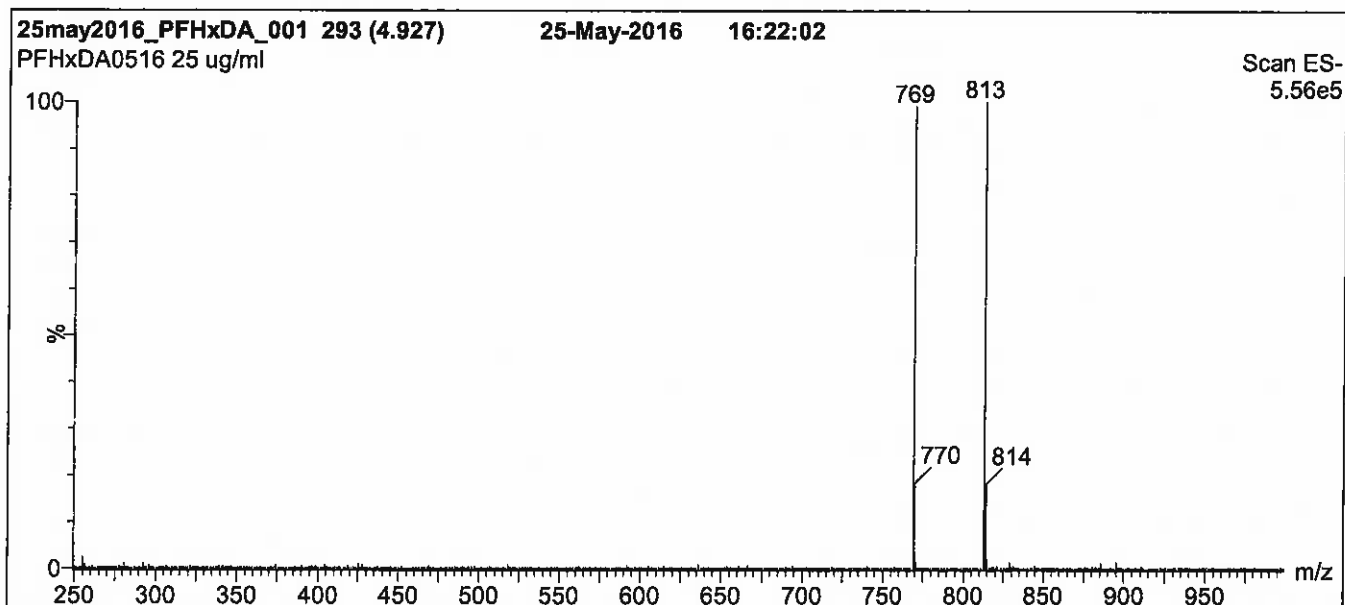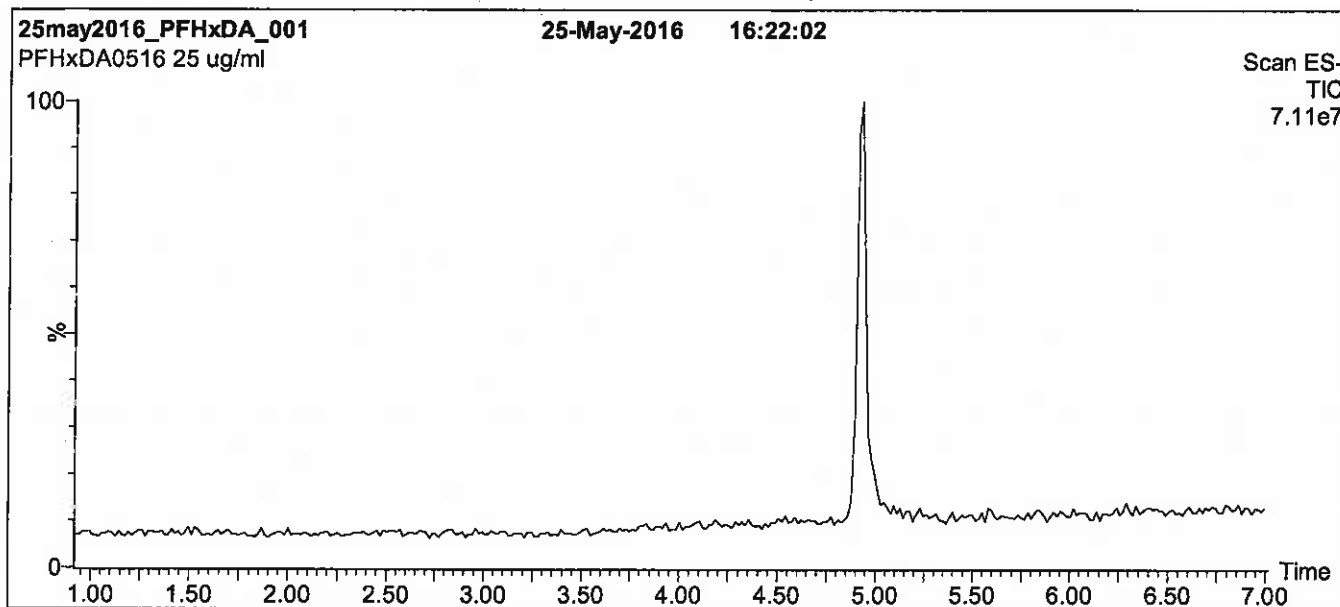

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 70% (80:20 MeOH:ACN) / 30% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 95% organic over 6 min and hold for 2.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (250 - 1250 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 25.00
Cone Gas Flow (l/hr) = 60
Desolvation Gas Flow (l/hr) = 750

Figure 2: PFHxDA; LC/MS/MS Data (Selected MRM Transitions)

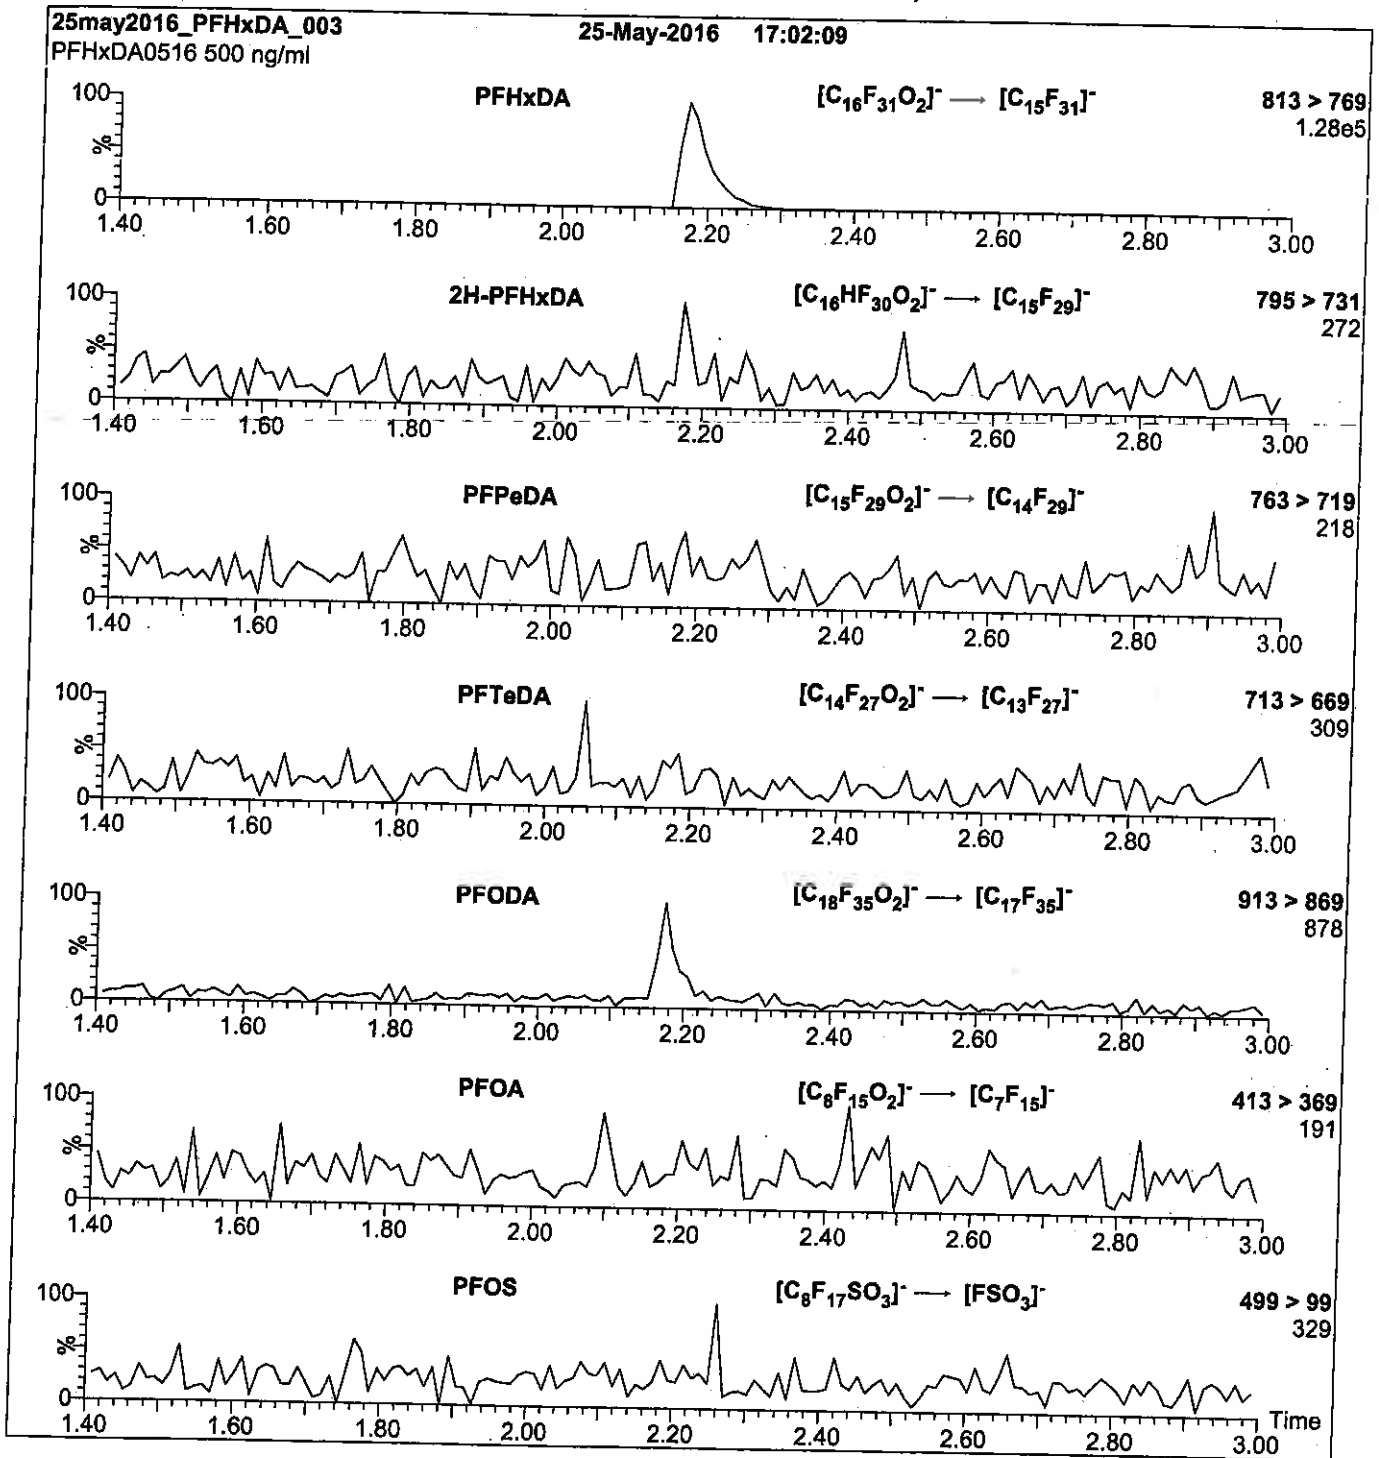

Conditions for Figure 2:

Injection: Direct loop injection
 10 μ l (500 ng/ml PFHxDA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.66e-3
 Collision Energy (eV) = 15

Reagent

LCPFHxS-br_00002

SBC
R: 9/13/16



730513
ID: LCPFHxS-br_00002
Exp: 07/03/20 Ppfd: SBC
Potassium Perfluorohexane



730514
ID: LCPFHxS-br_00003
Exp: 07/03/20 Ppfd: SBC
Potassium Perfluorohexane



WELLINGTON
LABORATORIES

CERTIFICATE OF ANALYSIS
DOCUMENTATION

br-PFHxSK

**Potassium Perfluorohexanesulfonate
Solution/Mixture of Linear and
Branched Isomers**

PRODUCT CODE: br-PFHxSK
LOT NUMBER: brPFHxSK0615
CONCENTRATION: 50.0 ± 2.5 µg/ml (total potassium salt)
45.5 ± 2.3 µg/ml (total PFHxS anion)
SOLVENT(S): Methanol
DATE PREPARED: (mm/dd/yyyy) 06/29/2015
LAST TESTED: (mm/dd/yyyy) 07/03/2015
EXPIRY DATE: (mm/dd/yyyy) 07/03/2020
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DESCRIPTION:

The chemical purity has been determined to be ≥98% perfluorohexanesulfonate linear and branched isomers. The full name, structure and percent composition for each of the identified isomeric components are given in Table A.

DOCUMENTATION/ DATA ATTACHED:

Table A: Isomeric Components and Percent Composition by ¹⁹F-NMR
Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS Data
Figure 3: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains ~ 0.5% of perfluoro-1-pentanesulfonate and ~ 0.2% of perfluoro-1-octanesulfonate.
- CAS#: 3871-99-6 (for linear isomer; potassium salt).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compounds it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.

QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Table A: br-PFHxSK; Isomeric Components and Percent Composition (by ¹⁹F-NMR)*



Isomer	Name	Structure	Percent Composition by ¹⁹ F-NMR
1	Potassium perfluoro-1-hexanesulfonate	CF ₃ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ SO ₃ ⁻ K ⁺	81.1
2	Potassium 1-trifluoromethylperfluoropentanesulfonate**	$\begin{array}{c} \text{CF}_3\text{CF}_2\text{CF}_2\text{CF}_2\text{CF}_2\text{SO}_3^-\text{K}^+ \\ \\ \text{CF}_3 \end{array}$	2.9
3	Potassium 2-trifluoromethylperfluoropentanesulfonate	$\begin{array}{c} \text{CF}_3\text{CF}_2\text{CF}_2\text{CF}_2\text{CF}_2\text{SO}_3^-\text{K}^+ \\ \\ \text{CF}_3 \end{array}$	1.4
4	Potassium 3-trifluoromethylperfluoropentanesulfonate	$\begin{array}{c} \text{CF}_3\text{CF}_2\text{CF}_2\text{CF}_2\text{CF}_2\text{SO}_3^-\text{K}^+ \\ \\ \text{CF}_3 \end{array}$	5.0
5	Potassium 4-trifluoromethylperfluoropentanesulfonate	$\begin{array}{c} \text{CF}_3\text{CF}_2\text{CF}_2\text{CF}_2\text{CF}_2\text{SO}_3^-\text{K}^+ \\ \\ \text{CF}_3 \end{array}$	8.9
6	Potassium 3,3-di(trifluoromethyl)perfluorobutanesulfonate	$\begin{array}{c} \text{CF}_3 \\ \\ \text{CF}_3\text{CCF}_2\text{CF}_2\text{SO}_3^-\text{K}^+ \\ \\ \text{CF}_3 \end{array}$	0.2
7	Other Unidentified Isomers		0.5

* Percent of total perfluorohexanesulfonate isomers only.
 ** Systematic Name: Potassium perfluorohexane-2-sulfonate.

Certified By: 
 B.G. Chittim

Date: 07/15/2015
(mm/dd/yyyy)

Figure 1: br-PFHxSK; LC/MS Data (TIC and Mass Spectrum)

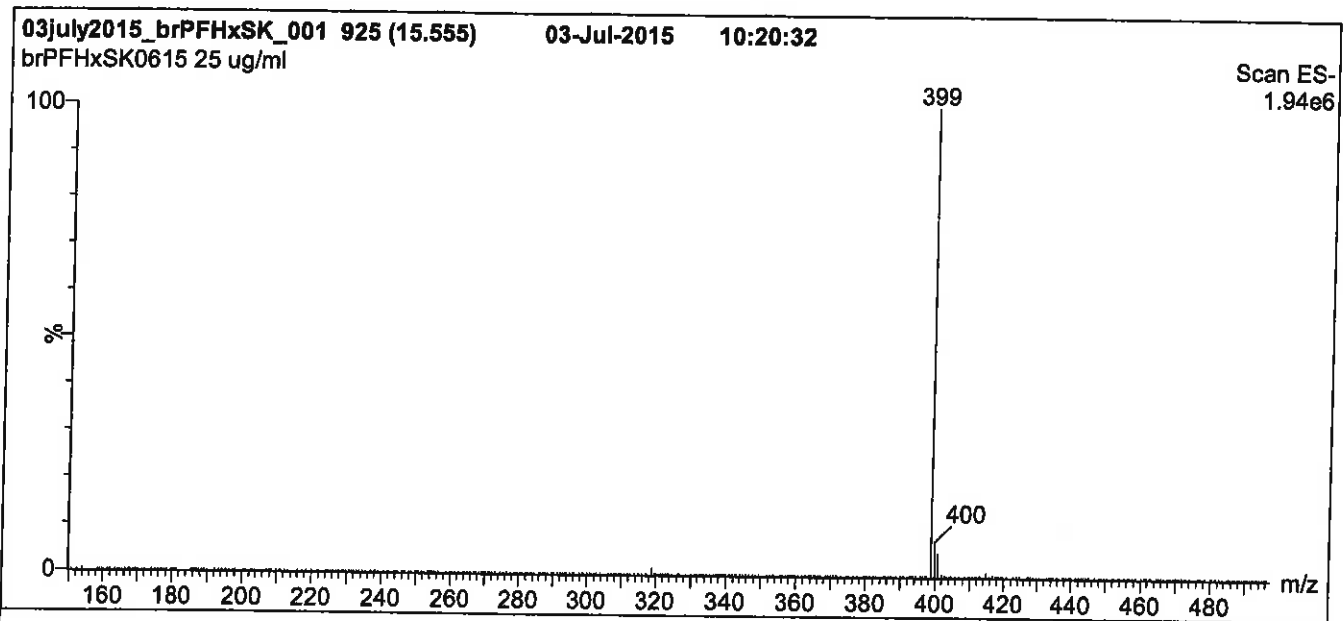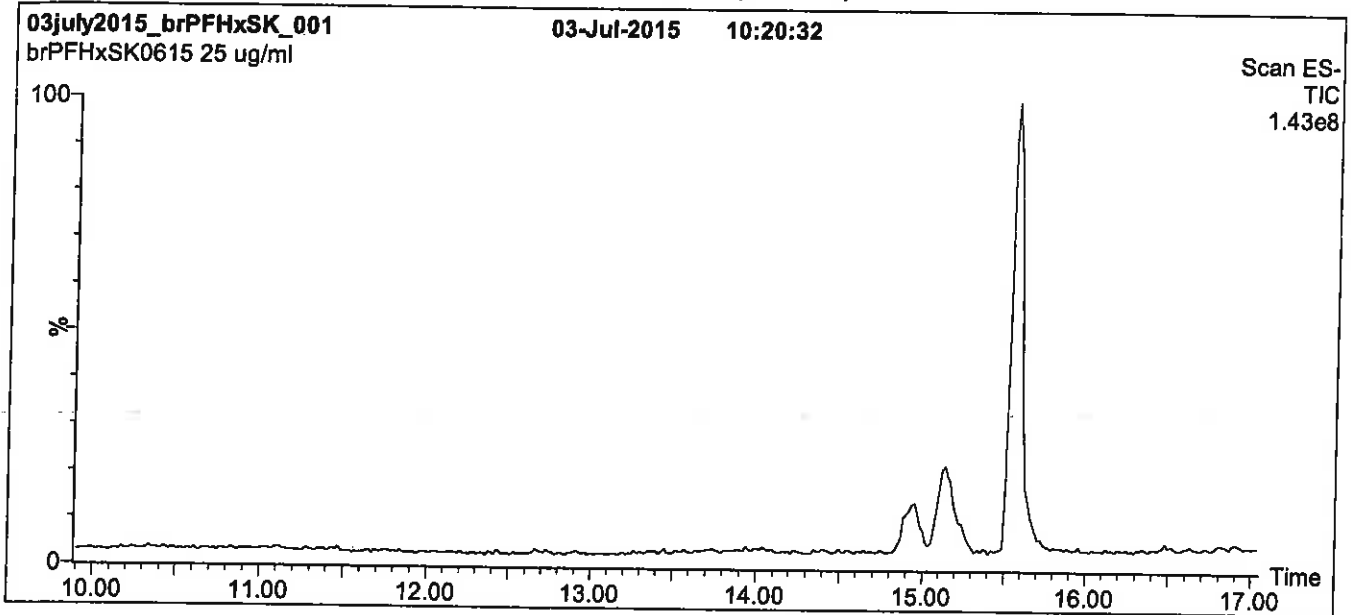

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 20% (80:20 MeOH:ACN) / 80% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 50% organic over 14 min. Ramp to
90% organic over 3 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 20 min


MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 50.00
Cone Gas Flow (l/hr) = 60
Desolvation Gas Flow (l/hr) = 750

Flow: 300 μ l/min

Figure 2: br-PFHxSK; LC/MS Data

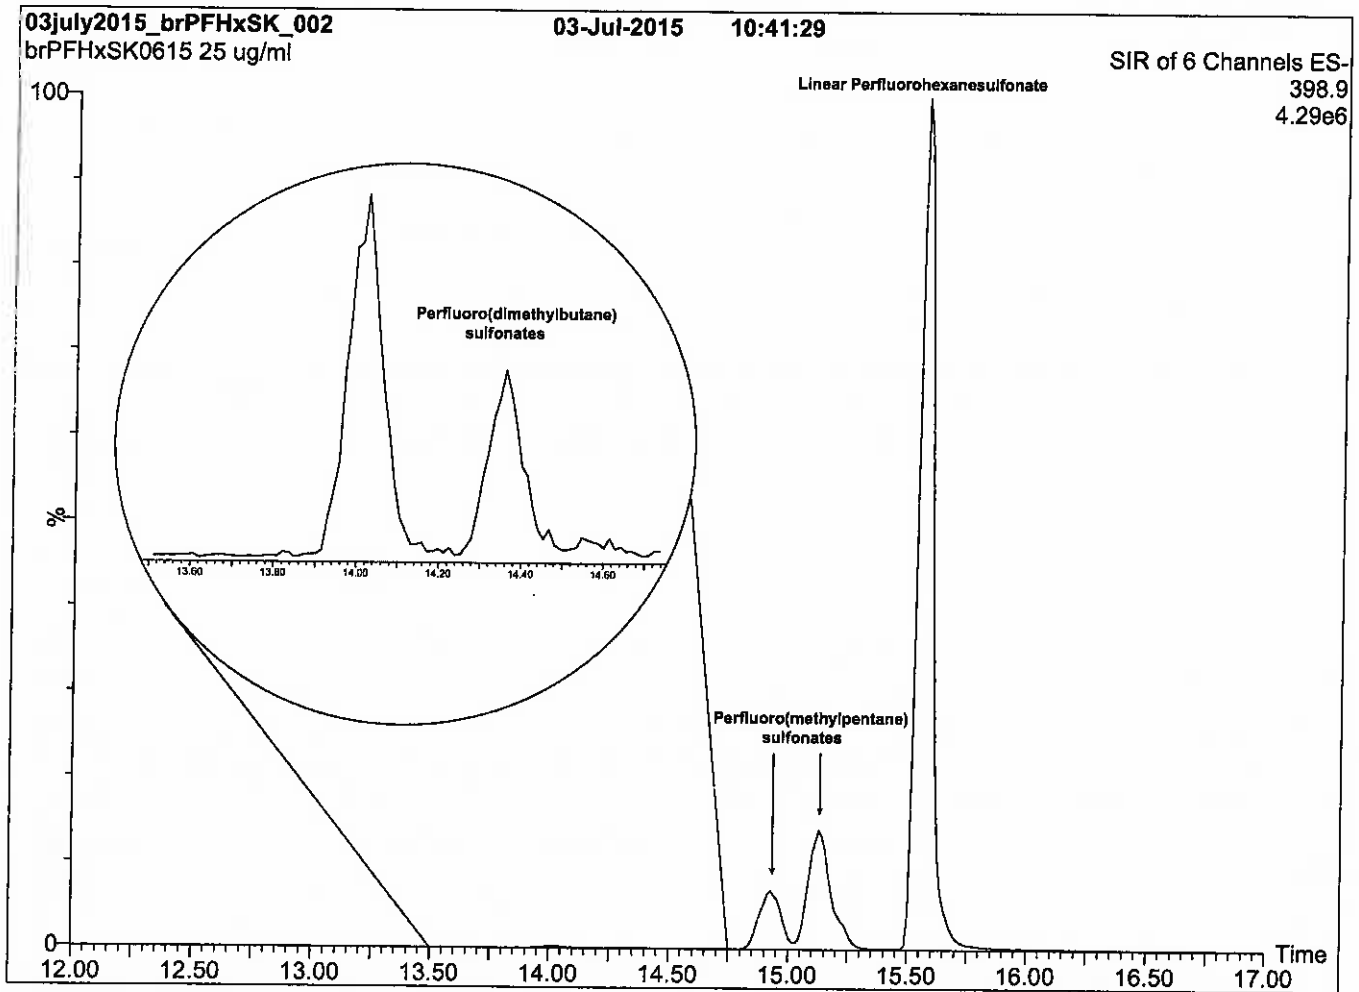

Conditions for Figure 2:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 20% (80:20 MeOH:ACN) / 80% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 50% organic over 14 min. Ramp to
 90% organic over 3 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 20 min


Flow: 300 μ l/min

MS Parameters

Experiment: SIR (6 channels)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 50.00
 Cone Gas Flow (l/hr) = 60
 Desolvation Gas Flow (l/hr) = 750

Figure 3: br-PFHxSK; LC/MS/MS Data (Selected MRM Transitions)

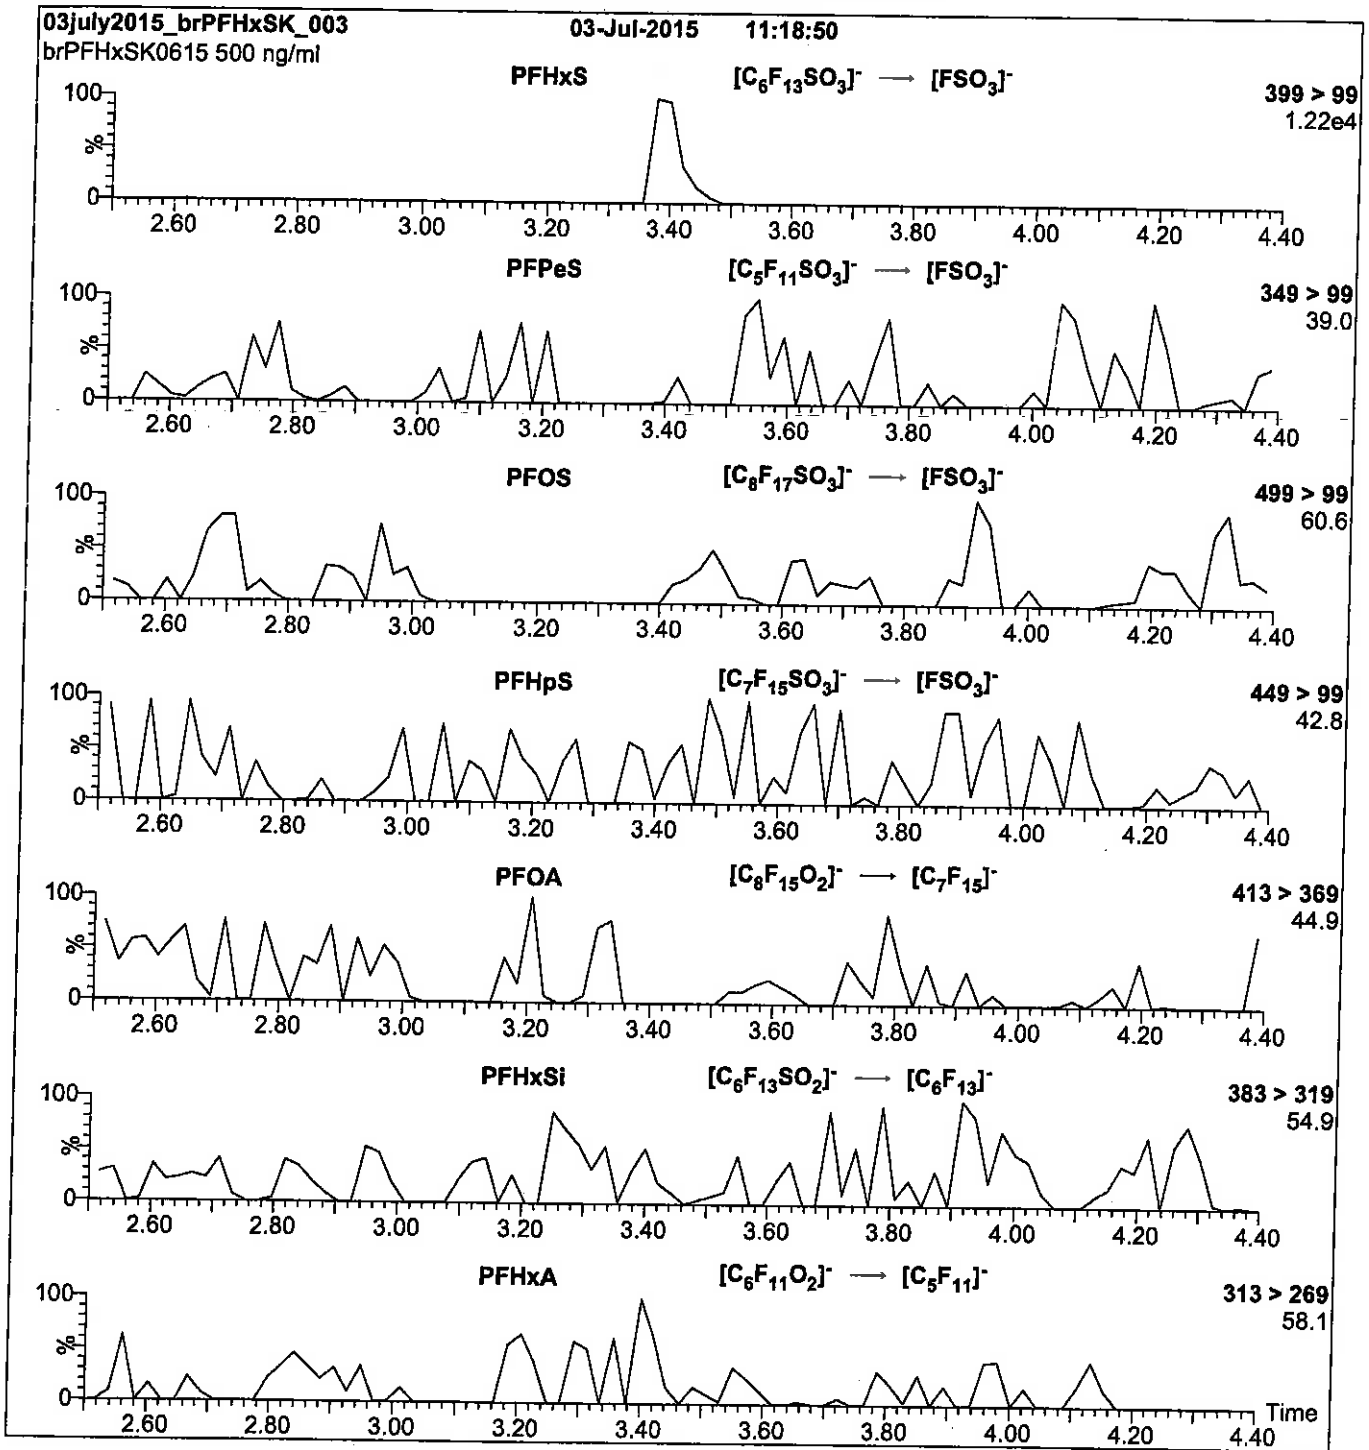

Conditions for Figure 3:

Injection: Direct loop injection
10 μ l (500 ng/ml br-PFHxSK)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.54e-3
Collision Energy (eV) = 30

Reagent

LCPFNA_00005




R: 4/7/16 CBW

609703

ID: LCPFNA_00005

Exp: 10/23/20 Prod: CBW

PF-n-nonanoic acid

**WELLINGTON**
LABORATORIES**CERTIFICATE OF ANALYSIS**
DOCUMENTATION**PRODUCT CODE:** PFNA
COMPOUND: Perfluoro-n-nonanoic acid**LOT NUMBER:** PFNA1015**STRUCTURE:****CAS #:** 375-95-1**MOLECULAR FORMULA:** C₉H_{F₁₇}O₂
CONCENTRATION: 50 ± 2.5 µg/ml**MOLECULAR WEIGHT:** 464.08
SOLVENT(S): Methanol
Water (<1%)**CHEMICAL PURITY:** >98%
LAST TESTED: (mm/dd/yyyy) 10/23/2015
EXPIRY DATE: (mm/dd/yyyy) 10/23/2020
RECOMMENDED STORAGE: Store ampoule in a cool, dark place**DOCUMENTATION/ DATA ATTACHED:**Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)**ADDITIONAL INFORMATION:**

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains ~ 0.1% of perfluoro-n-octanoic acid (PFOA) and < 0.1% of perfluoro-n-heptanoic acid (PFHpA).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:

B.G. Chittim

Date: 10/30/2015

(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON 'N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com


Figure 1: PFNA; LC/MS Data (TIC and Mass Spectrum)

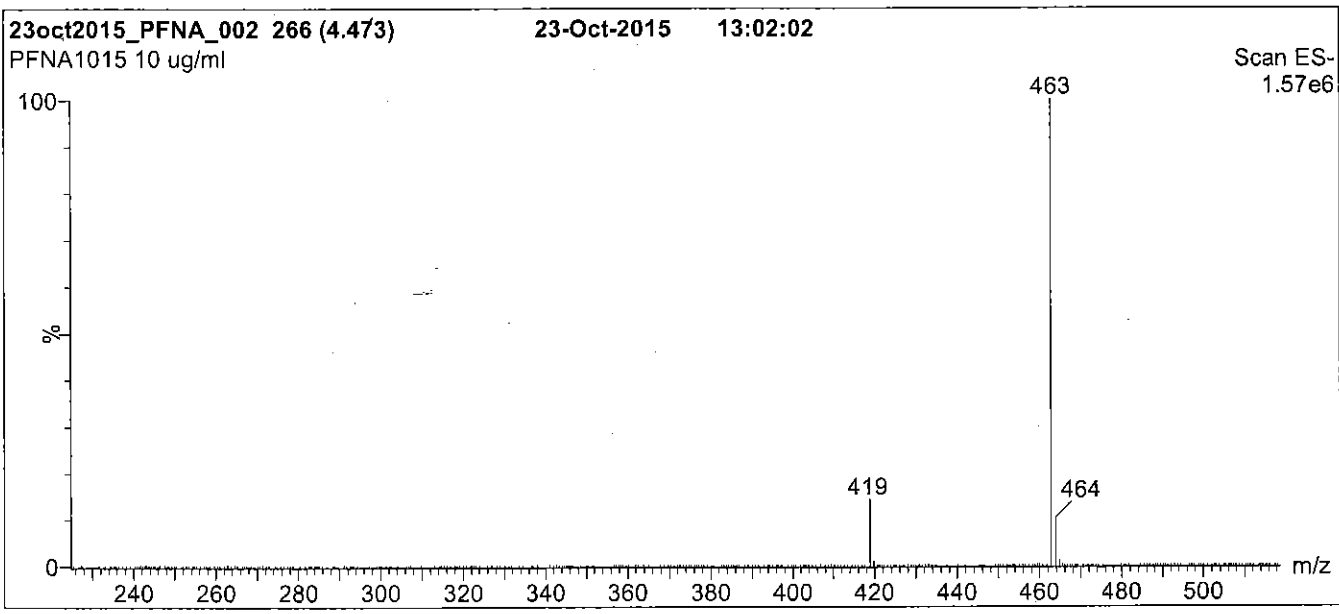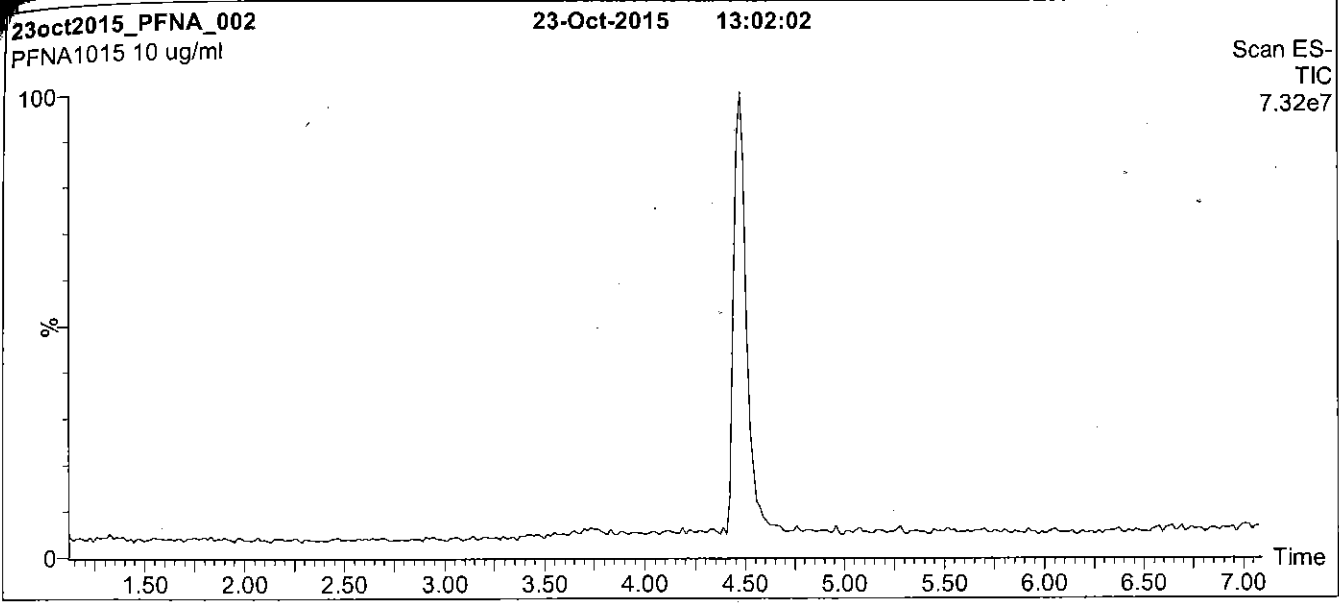

Conditions for Figure 1:

LC:	Waters Acquity Ultra Performance LC
MS:	Micromass Quattro <i>micro</i> API MS
Chromatographic Conditions	
Column:	Acquity UPLC BEH Shield RP ₁₈ 1.7 μ m, 2.1 x 100 mm
Mobile phase:	Gradient Start: 50% (80:20 MeOH:ACN) / 50% H ₂ O (both with 10 mM NH ₄ OAc buffer) Ramp to 90% organic over 7 min and hold for 2 min before returning to initial conditions in 0.5 min. Time: 10 min
Flow:	300 μ l/min
MS Parameters	
Experiment:	Full Scan (225 - 850 amu)
Source:	Electrospray (negative)
Capillary Voltage (kV):	2.00
Cone Voltage (V):	15.00
Cone Gas Flow (l/hr):	50
Desolvation Gas Flow (l/hr):	750

Figure 2: PFNA; LC/MS/MS Data (Selected MRM Transitions)

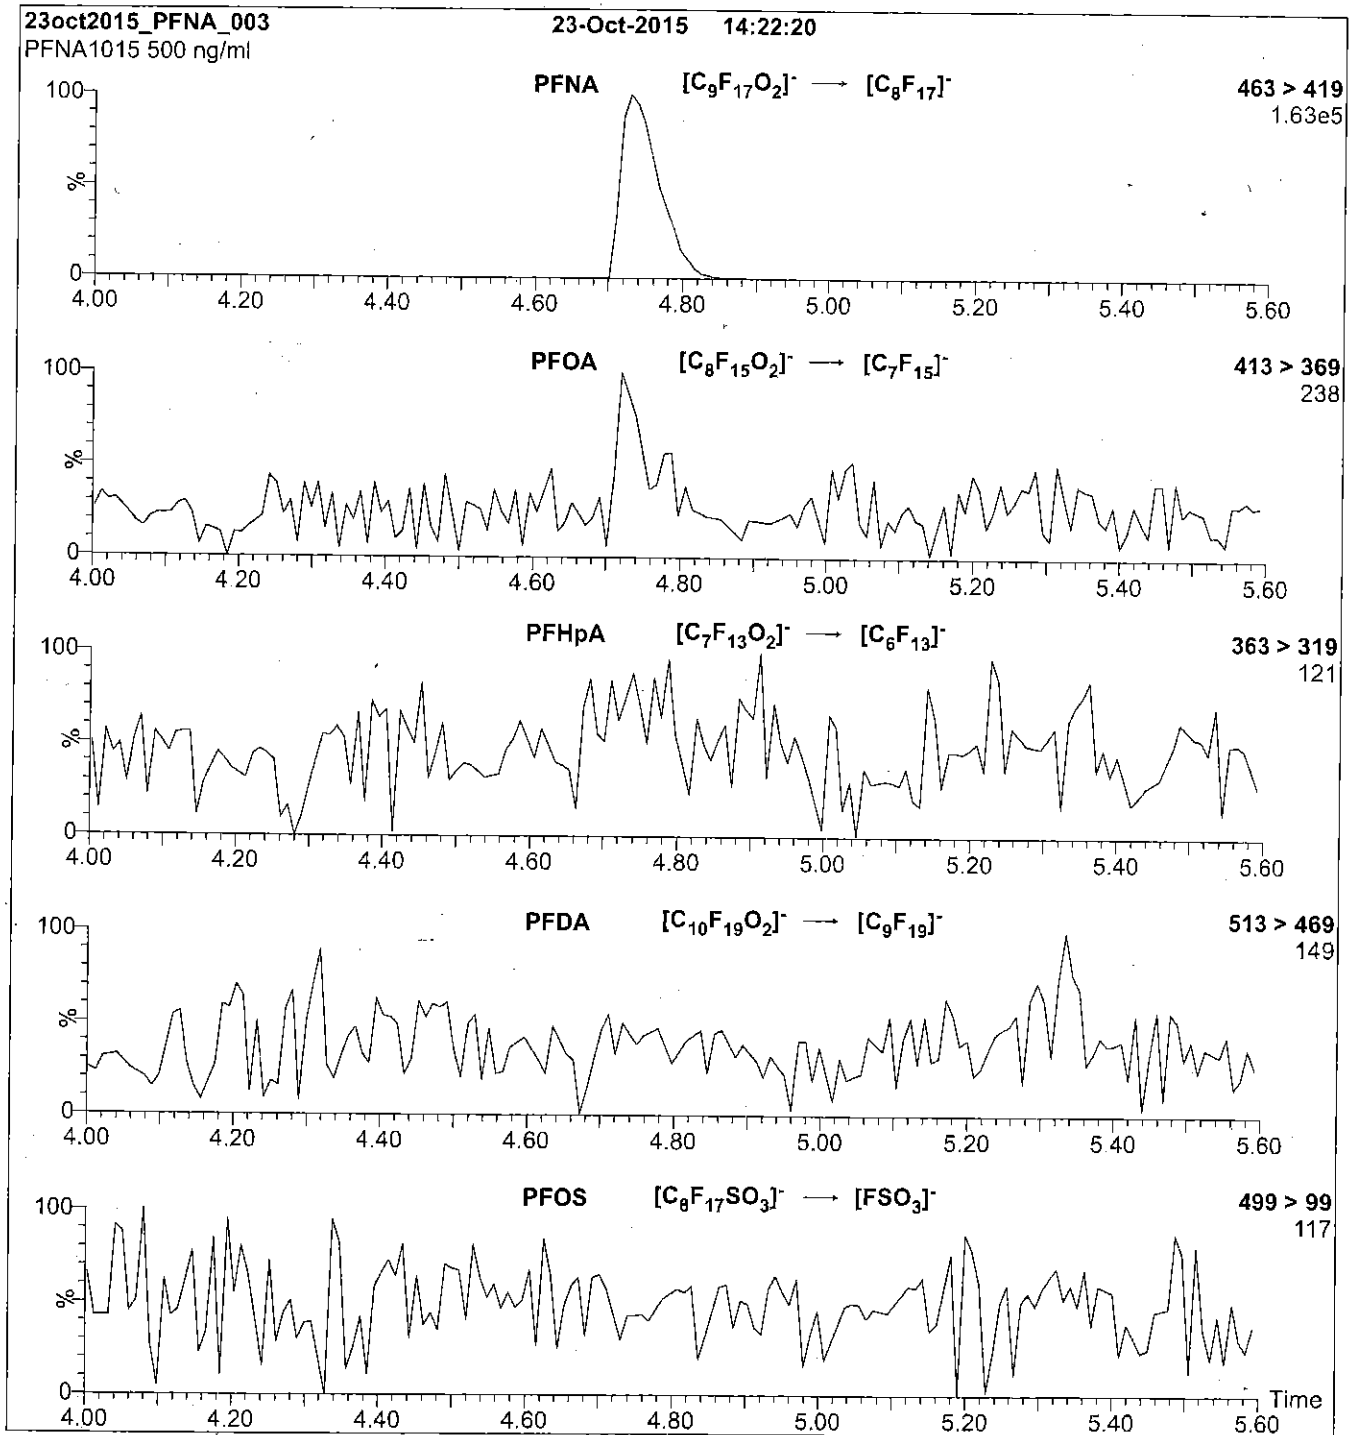

Conditions for Figure 2:

Injection: Direct loop injection
 10 μ l (500 ng/ml PFNA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.28e-3
 Collision Energy (eV) = 11

Reagent

LCPFNA_00006

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFNA; LC/MS Data (TIC and Mass Spectrum)

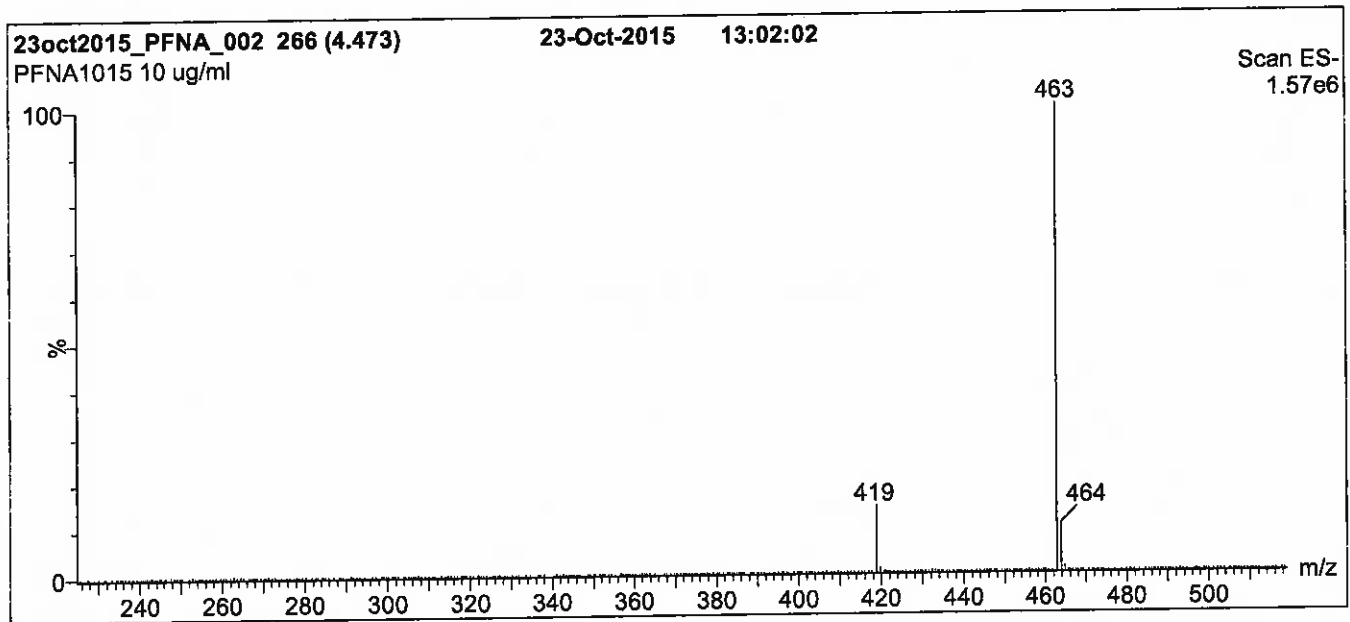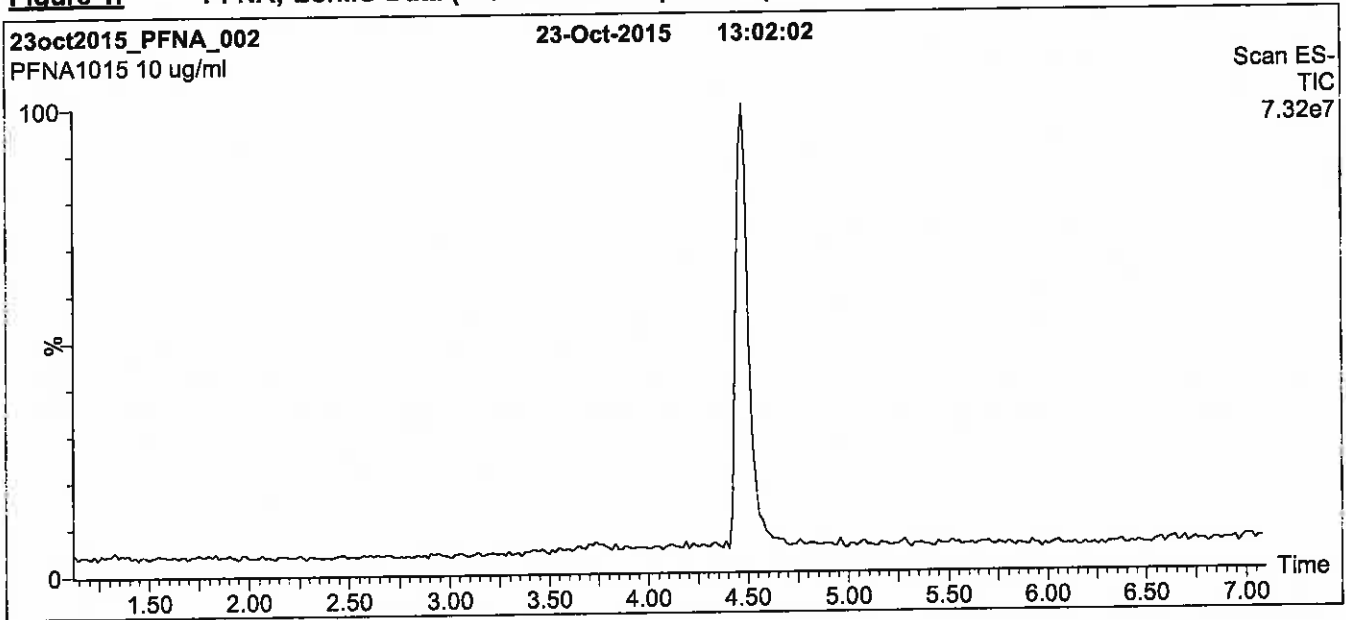

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 2 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: PFNA; LC/MS/MS Data (Selected MRM Transitions)

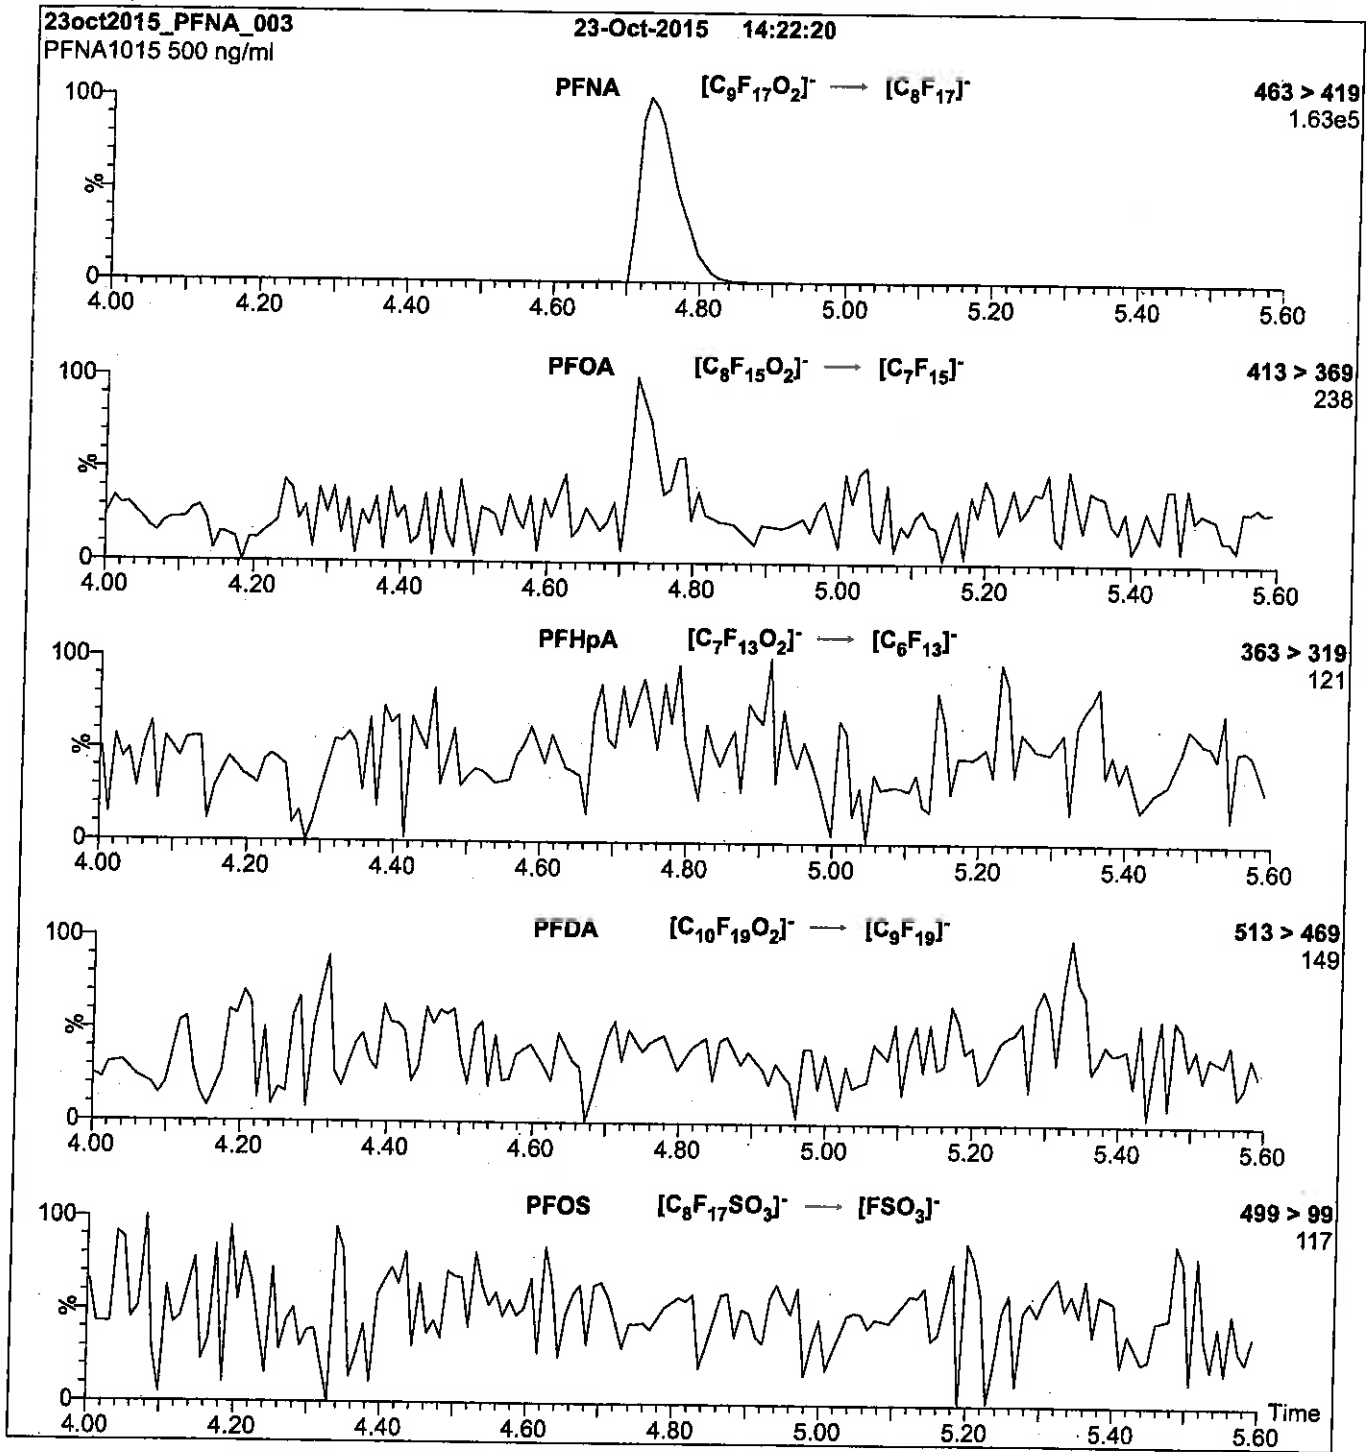

Conditions for Figure 2:

Injection: Direct loop injection
 10 μ l (500 ng/ml PFNA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.28e-3
 Collision Energy (eV) = 11

Reagent

LCPFOA_00006

R-7/6/16 CBW

671577
ID: LCPFOA_00006
Exp: 11/06/20 Prod: CBW
PF-n-octanoic acid




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: PFOA **LOT NUMBER:** PFOA1115
COMPOUND: Perfluoro-n-octanoic acid

STRUCTURE: **CAS #:** 335-67-1



MOLECULAR FORMULA: C₈HF₁₅O₂ **MOLECULAR WEIGHT:** 414.07
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Methanol
Water (<1%)
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 11/06/2015
EXPIRY DATE: (mm/dd/yyyy) 11/06/2020
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: B.G. Chittim **Date:** 11/11/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFOA; LC/MS Data (TIC and Mass Spectrum)

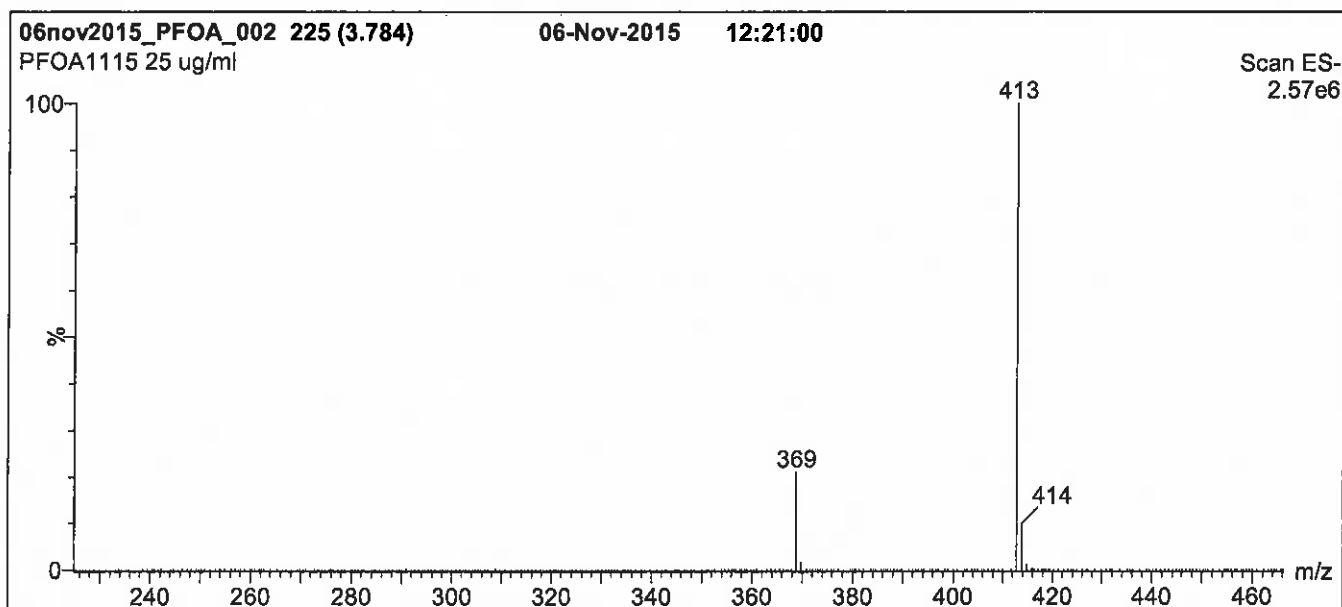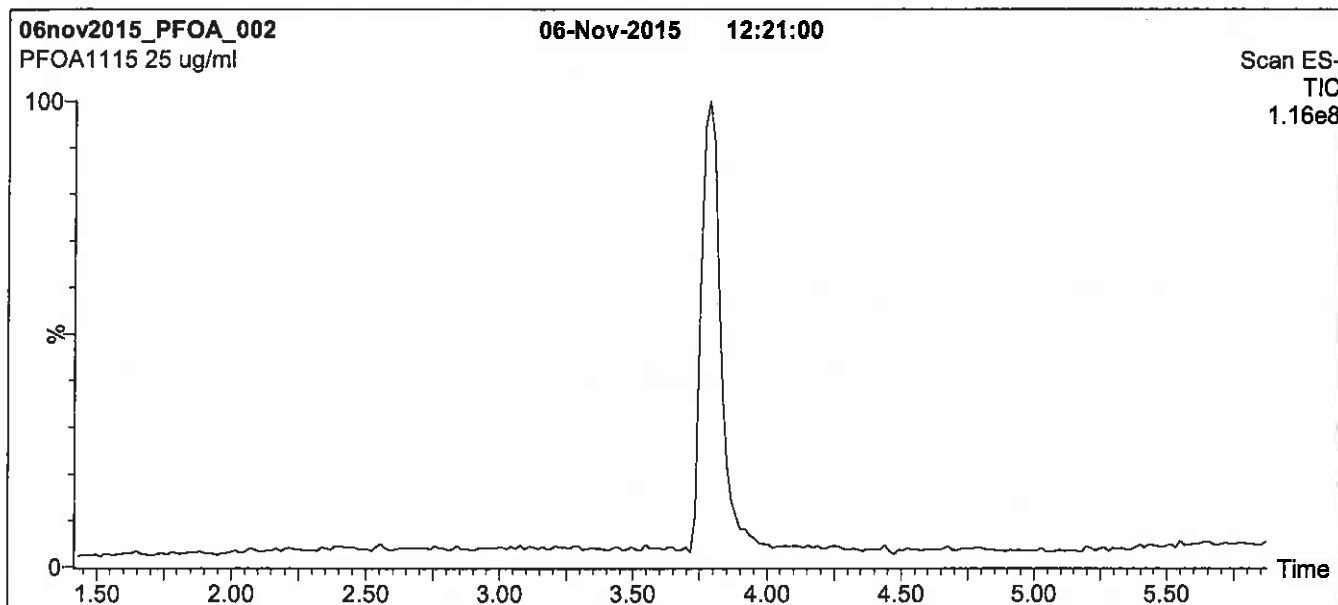

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈,
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 50% (80:20 MeOH:ACN) / 50% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for
 2 min before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 15.00
 Cone Gas Flow (l/hr) = 100
 Desolvation Gas Flow (l/hr) = 750

Figure 2: PFOA; LC/MS/MS Data (Selected MRM Transitions)

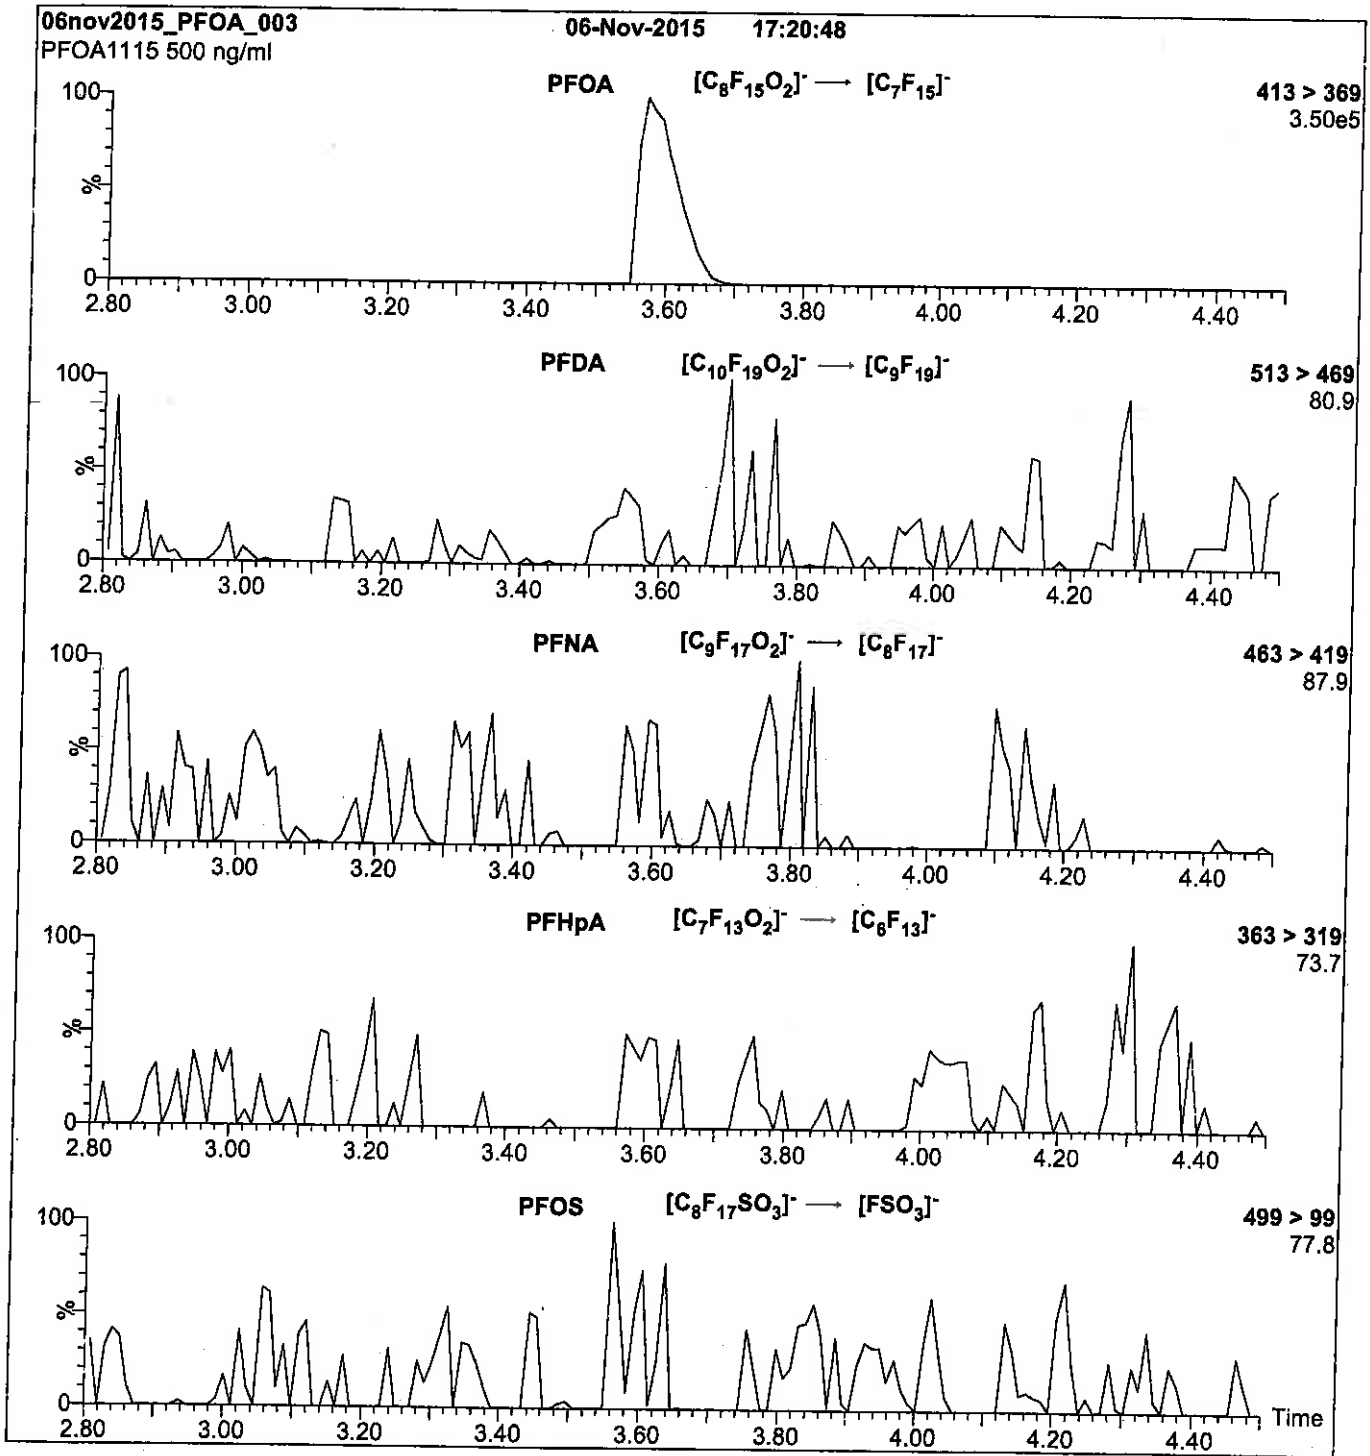

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml PFOA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.17e-3
Collision Energy (eV) = 10

Reagent

LCPFODA_00005




605234

ID: LCPFODA_00005

Exp: 01/30/20 Prod: CBW
PFODA stock 50ug/ml

Rec. 3/20/16 JRB

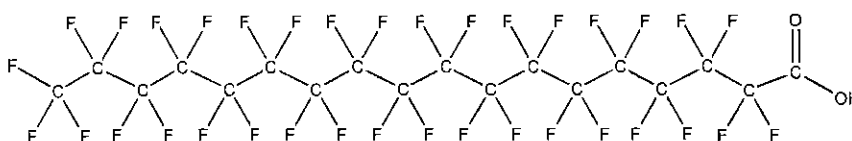**WELLINGTON**
LABORATORIES**CERTIFICATE OF ANALYSIS**
DOCUMENTATION**PRODUCT CODE:** PFODA **LOT NUMBER:** PFODA0115
COMPOUND: Perfluoro-n-octadecanoic acid**STRUCTURE:** **CAS #:** 16517-11-6

MOLECULAR FORMULA:	$C_{18}H_{35}O_2$	MOLECULAR WEIGHT:	914.14
CONCENTRATION:	$50 \pm 2.5 \mu\text{g/ml}$	SOLVENT(S):	Methanol Water (<1%)
CHEMICAL PURITY:	>98%		
LAST TESTED: (mm/dd/yyyy)	01/30/2015		
EXPIRY DATE: (mm/dd/yyyy)	01/30/2020		
RECOMMENDED STORAGE:	Store ampoule in a cool, dark place		

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
 Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:

B.G. Chittim

Date: 03/25/2015

(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
 519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFODA; LC/MS Data (TIC and Mass Spectrum)

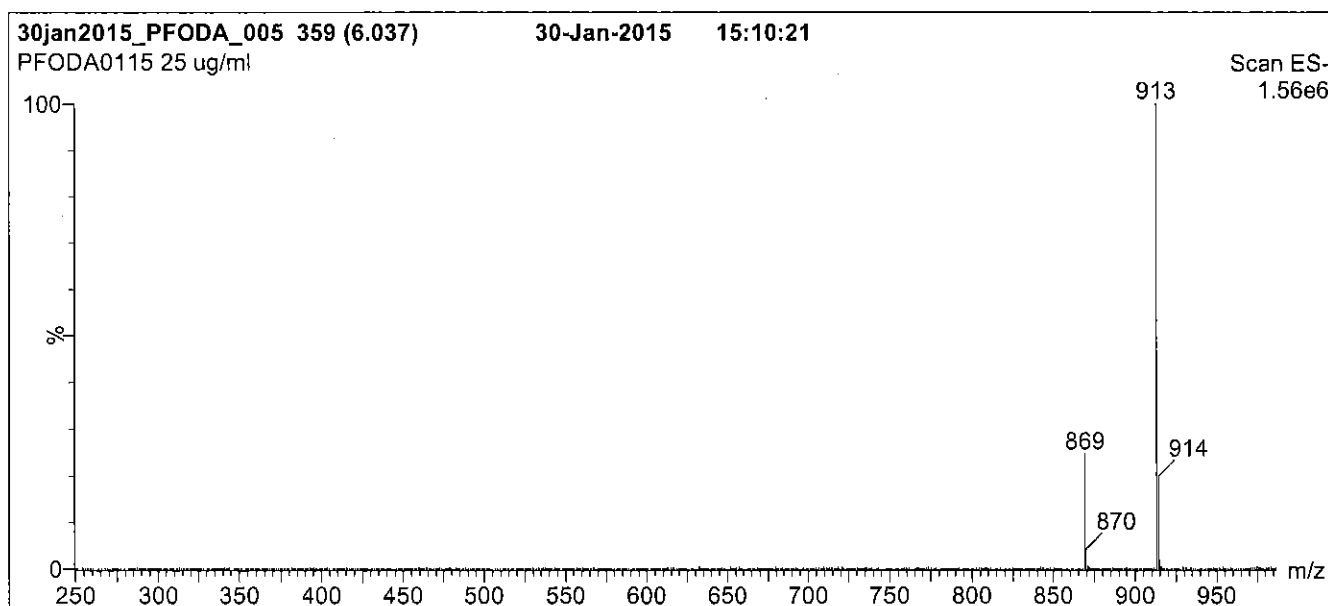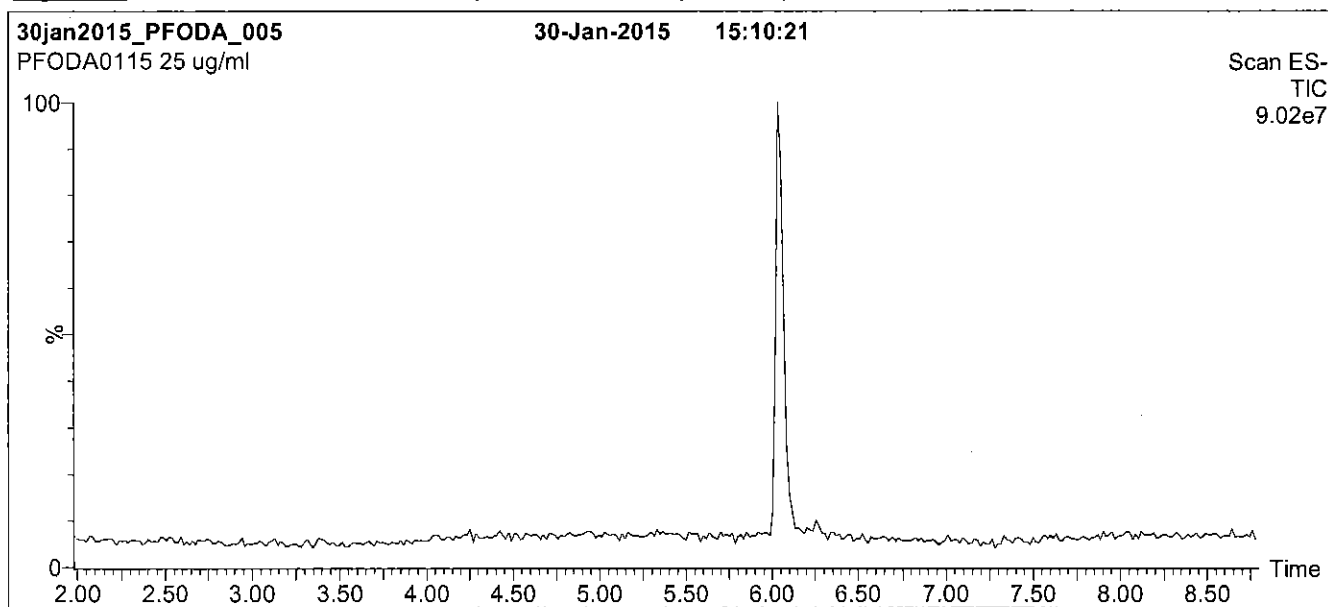

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 60% (80:20 MeOH:ACN) / 40% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for
1.5 min before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (250 - 1000 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 25.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: PFODA; LC/MS/MS Data (Selected MRM Transitions)

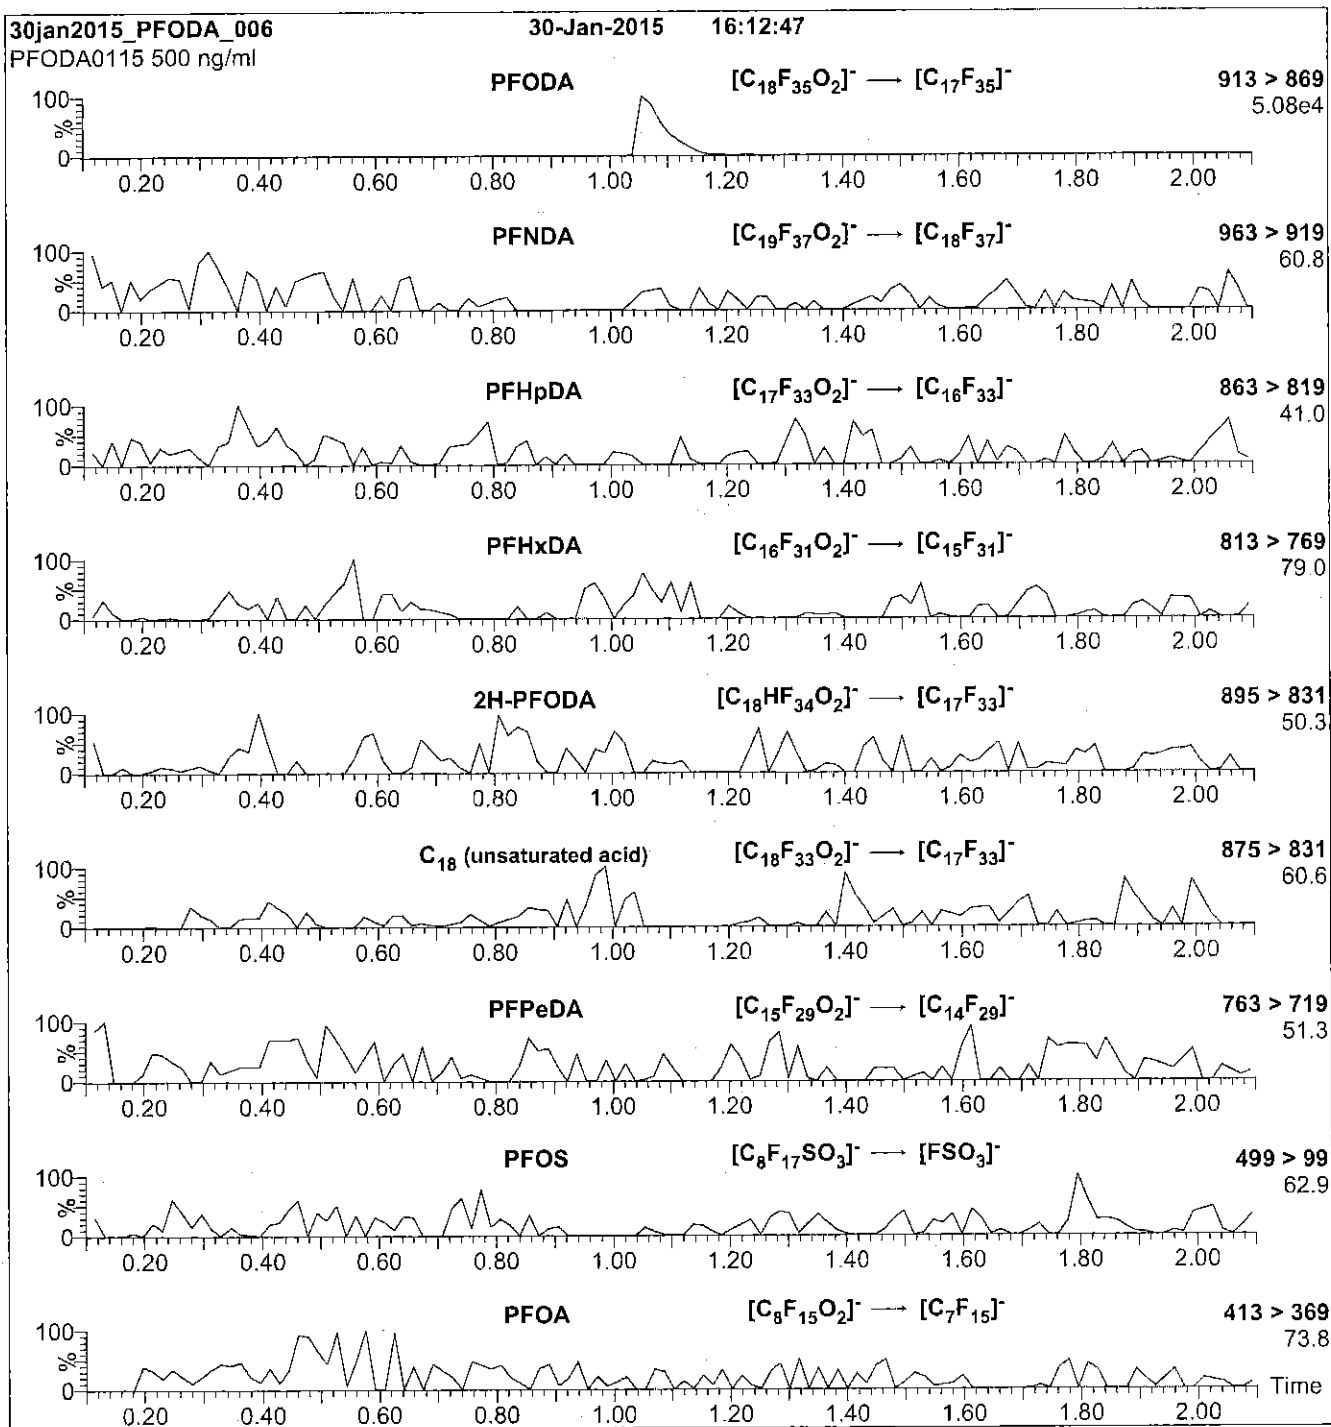

Conditions for Figure 2:

Injection: Direct loop injection
 10 µl (500 ng/ml PFODA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)

Flow: 300 µl/min

MS Parameters

Collision Gas (mbar) = 3.31e-3
 Collision Energy (eV) = 15

Reagent

LCPFODA_00006

Scanned
07/14/16

R: SBC
9/13/16

730632
ID: LCPFODA_00006
Exp: 04/29/21 Prod: SBC
PFODA stock 50ug/mL

730633
ID: LCPFODA_00007
Exp: 04/29/21 Prod: SBC
PFODA stock 50ug/mL




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: PFODA **LOT NUMBER:** PFODA0416
COMPOUND: Perfluoro-n-octadecanoic acid

STRUCTURE: **CAS #:** 16517-11-6



MOLECULAR FORMULA: $C_{18}HF_{36}O_2$ **MOLECULAR WEIGHT:** 914.14
CONCENTRATION: $50 \pm 2.5 \mu\text{g/ml}$ **SOLVENT(S):** Methanol
Water (<1%)
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 04/29/2016
EXPIRY DATE: (mm/dd/yyyy) 04/29/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:

B.G. Chittim

Date: 05/20/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFODA; LC/MS Data (TIC and Mass Spectrum)

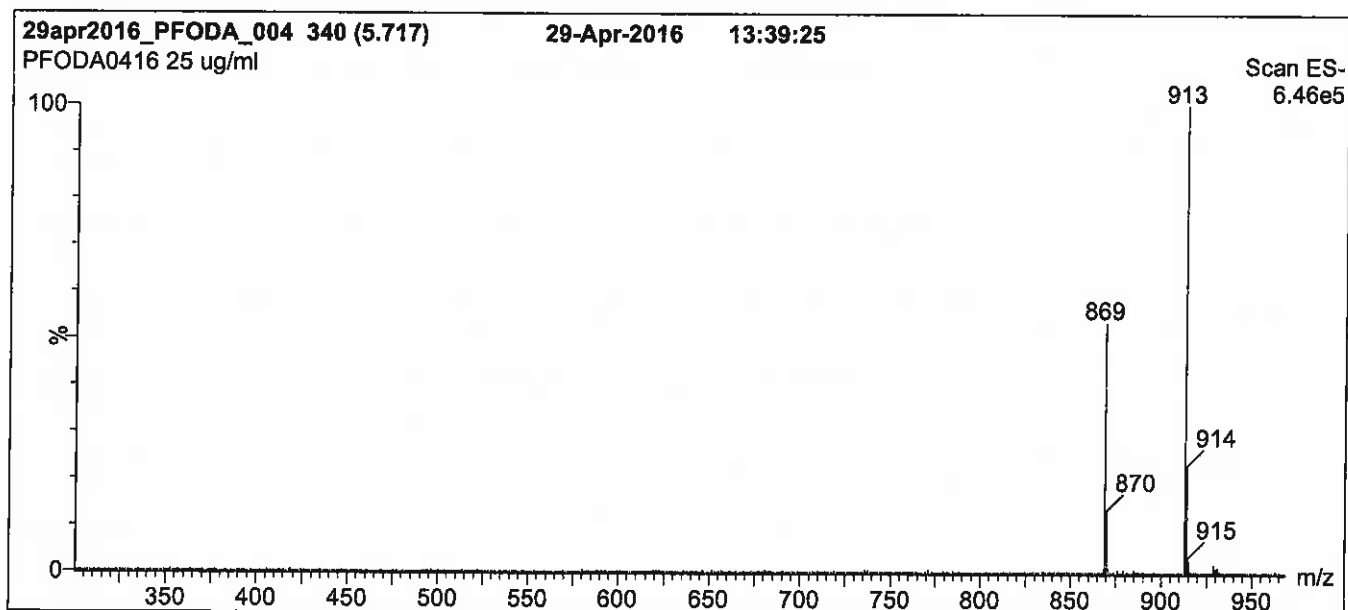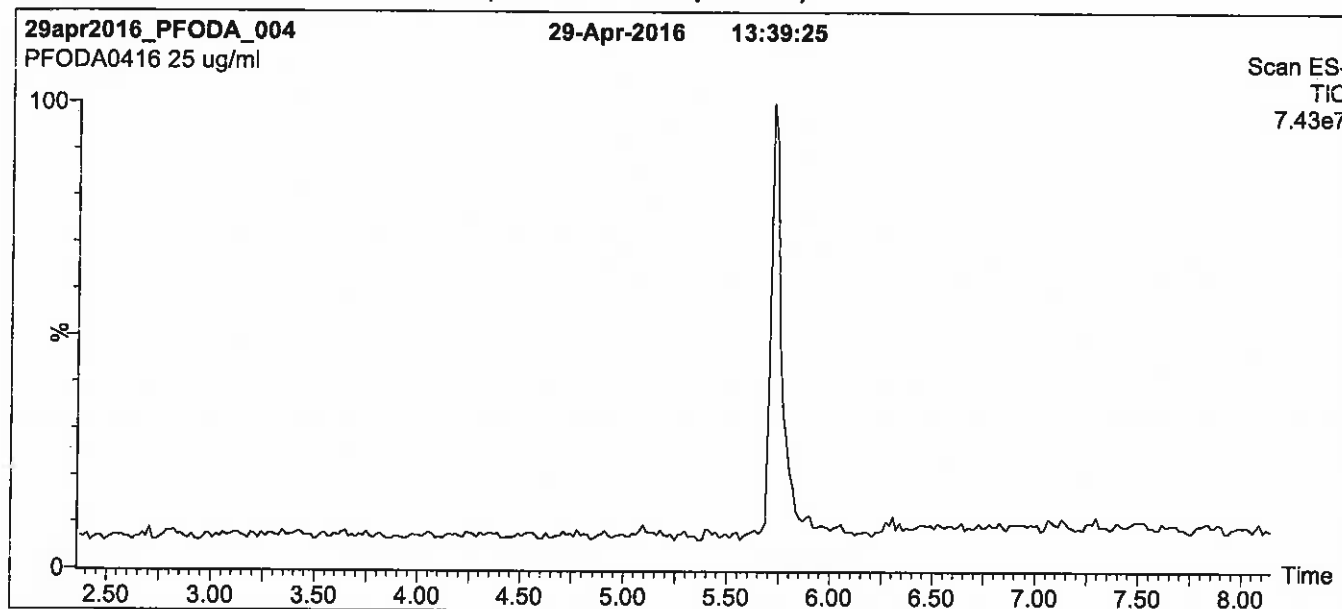

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 70% (80:20 MeOH:ACN) / 30% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 95% organic over 6 min and hold for
2.5 min before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (250 - 1000 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 25.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: PFODA; LC/MS/MS Data (Selected MRM Transitions)

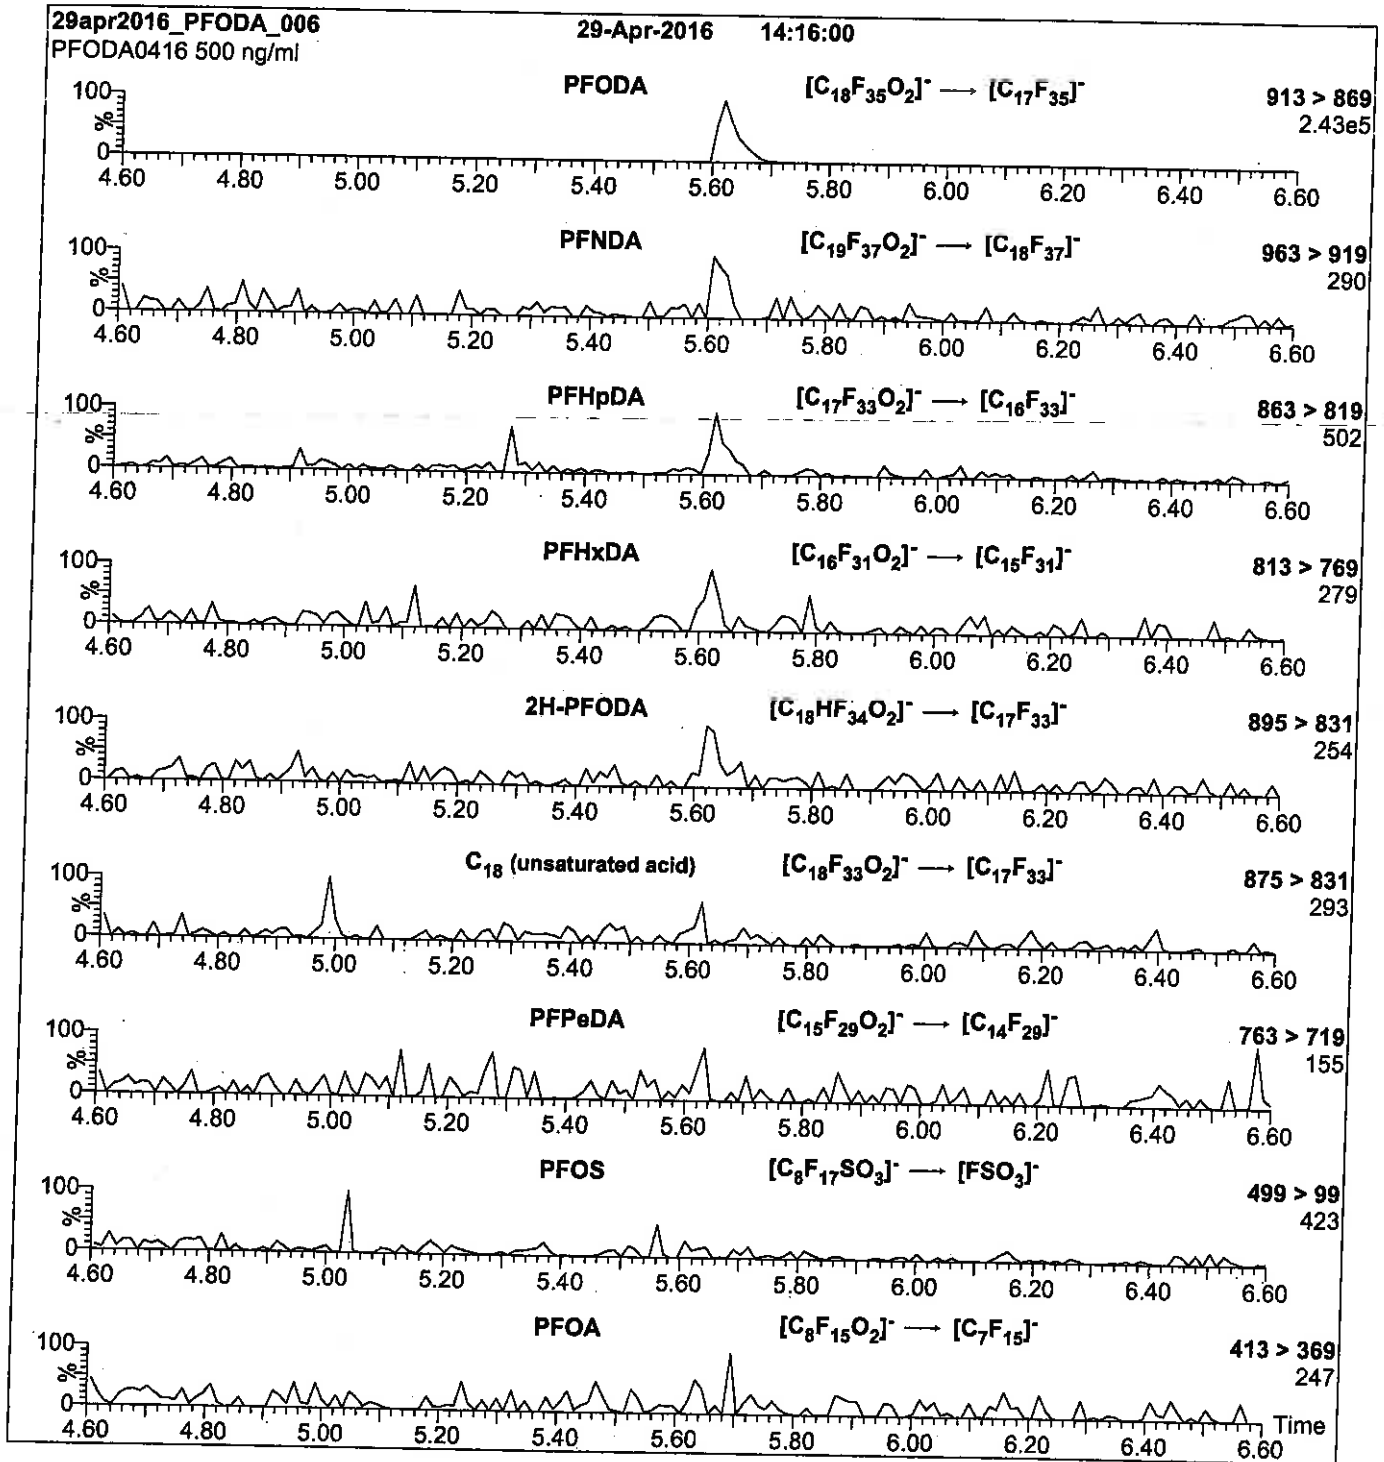

Conditions for Figure 2:

Injection: Direct loop injection
10 µl (500 ng/ml PFODA)

Mobile phase: Isocratic 90% (80:20 MeOH:ACN) / 10% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 µl/min

MS Parameters

Collision Gas (mbar) = 3.39e-3
Collision Energy (eV) = 15

Reagent

LCPFOS-br_00002

Scanned
10/14/16 SR

R: SBC 9/13/16



730515
ID: LCPFOS-br_00002
Exp: 10/14/20 Prpt: SBC
Potassium Perfluorooctane



730516
ID: LCPFOS-br_00003
Exp: 10/14/20 Prpt: SBC
Potassium Perfluorooctane



**WELLINGTON
LABORATORIES**

**CERTIFICATE OF ANALYSIS
DOCUMENTATION**

br-PFOSK

**Potassium Perfluorooctanesulfonate
Solution/Mixture of Linear and
Branched Isomers**

PRODUCT CODE: br-PFOSK
LOT NUMBER: brPFOSK1015
CONCENTRATION: 50 ± 2.5 µg/ml (total potassium salt)
46.4 ± 2.3 µg/ml (total PFOS anion)
SOLVENT(S): Methanol
DATE PREPARED: (mm/dd/yyyy) 10/13/2015
LAST TESTED: (mm/dd/yyyy) 10/14/2015
EXPIRY DATE: (mm/dd/yyyy) 10/14/2020
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DESCRIPTION:

The chemical purity has been determined to be ≥98% perfluorooctanesulfonate linear and branched isomers. The full name, structure and percent composition for each of the isomeric components are given in Table A.

DOCUMENTATION/ DATA ATTACHED:

Table A: Isomeric Components and Percent Composition by ¹⁹F-NMR
Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS Data (SIR)
Figure 3: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- A 5-point calibration curve was generated using linear PFOS (potassium salt) and mass-labelled PFOS as an internal standard to enable quantitation of br-PFOSK using isotopic dilution.
- CAS#: 2795-39-3 (for linear isomer; potassium salt).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

**Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com**

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compounds it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: br-PFOSK; LC/MS Data (TIC and Mass Spectrum)

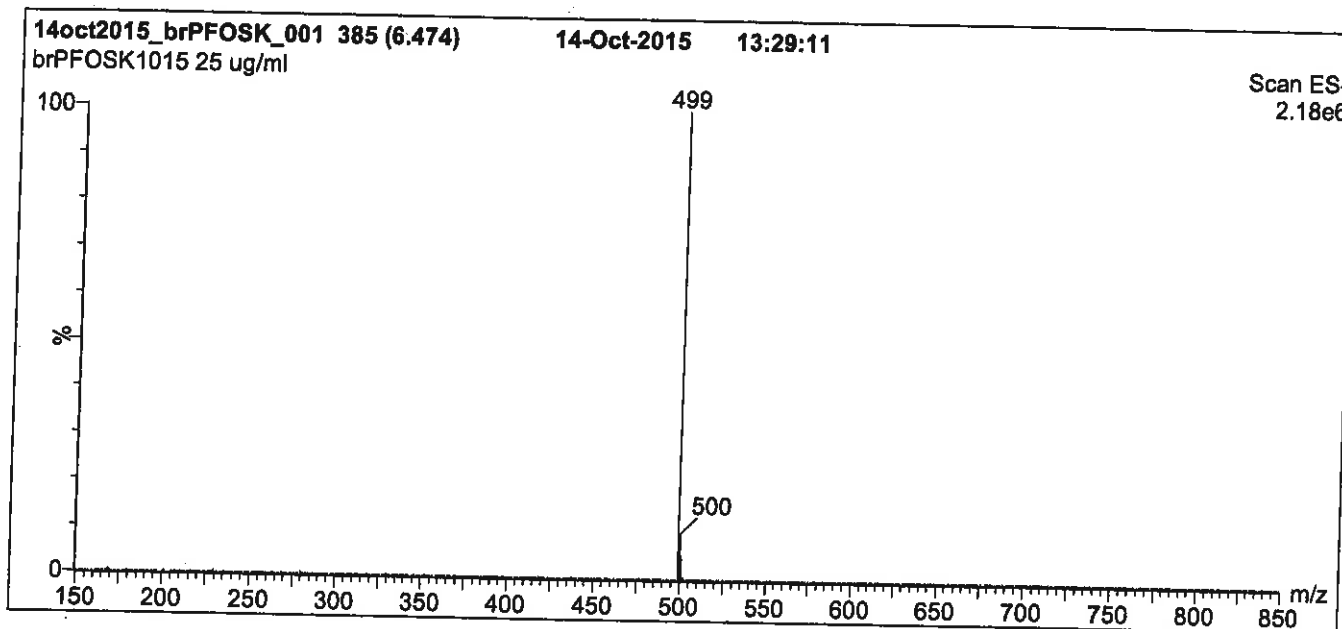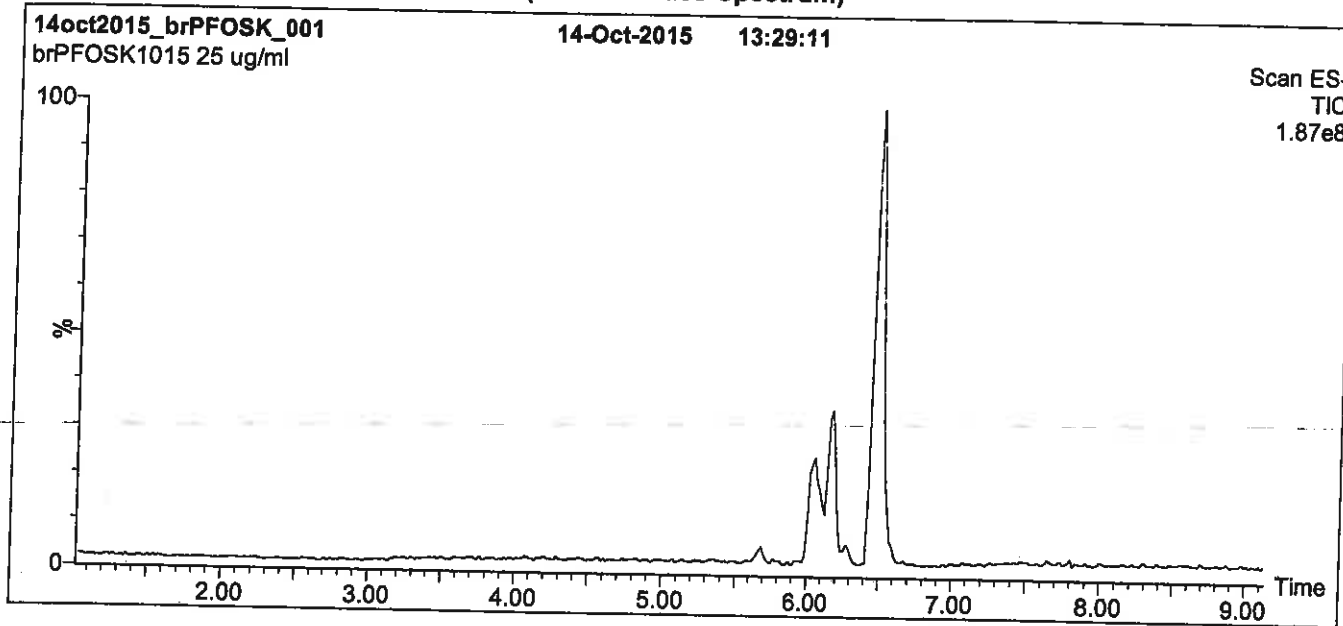

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈,
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 45% (80:20 MeOH:ACN) / 55% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 12 min and hold for 2 min.
Return to initial conditions over 0.5 min.
Time: 16 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 60.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: br-PFOSK; LC/MS Data (SIR)

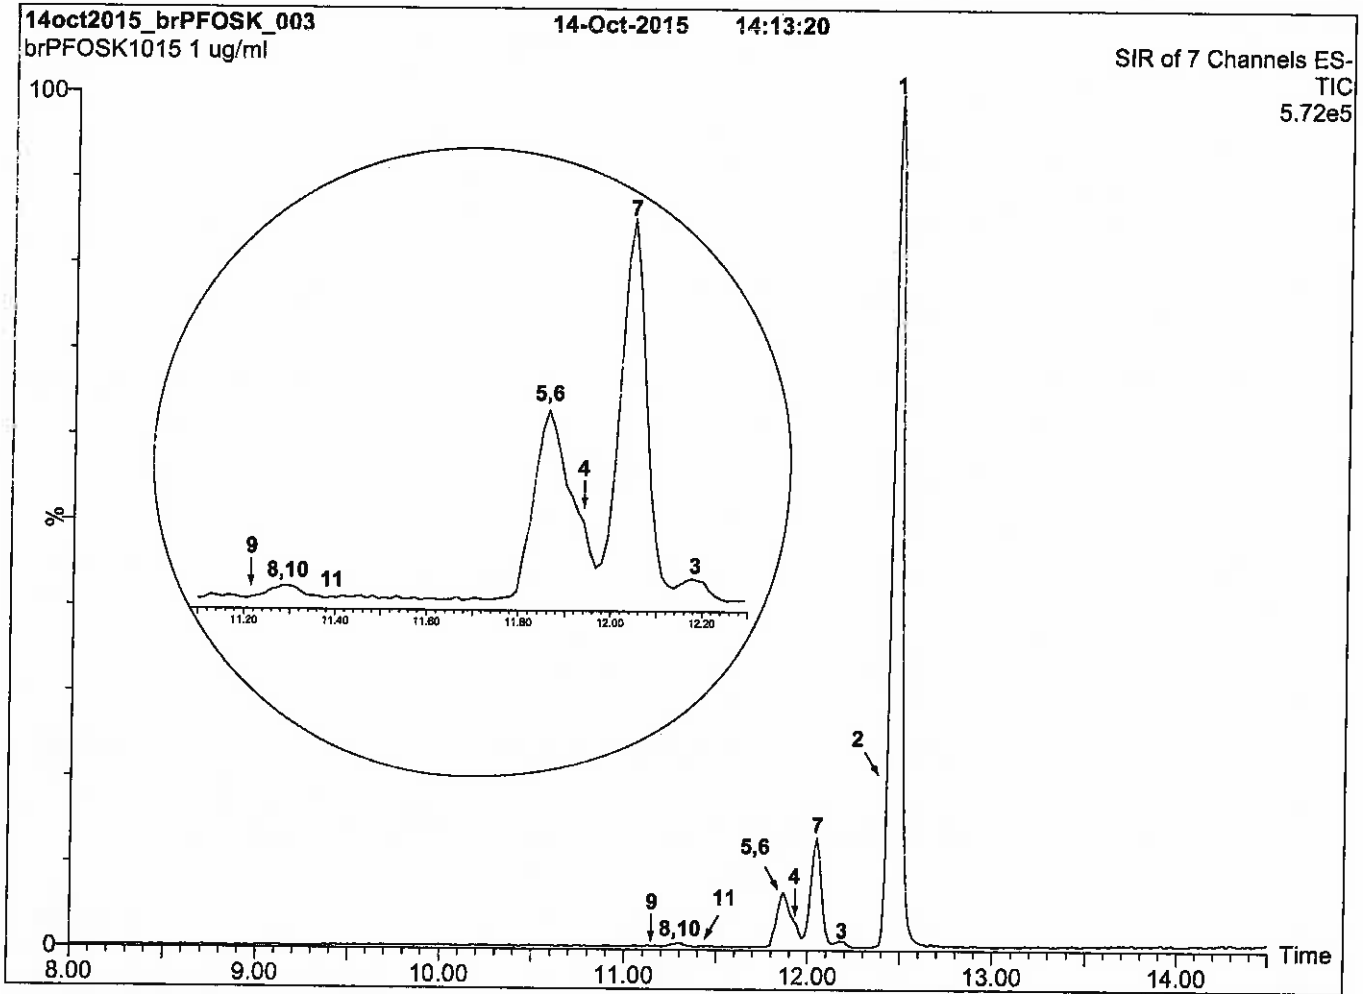

Conditions for Figure 2:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS


Chromatographic Conditions:

Column: Acquity UPLC BEH Shield RP₁₈ (1.7 μ m, 2.1 x 100 mm)
Injection: 1.0 μ g/ml of br-PFOSK
Mobile Phase: Gradient
45% (80:20 MeOH:ACN) / 55% H₂O (both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 15 min and hold for 3 min.
Return to initial conditions over 1 min.
Time: 20 min
Flow: 300 μ l/min

MS Conditions:

SIR (ES)
Source = 110 °C
Desolvation = 325 °C
Cone Voltage = 60V

Figure 3: br-PFOSK; LC/MS/MS Data (Selected MRM Transitions)

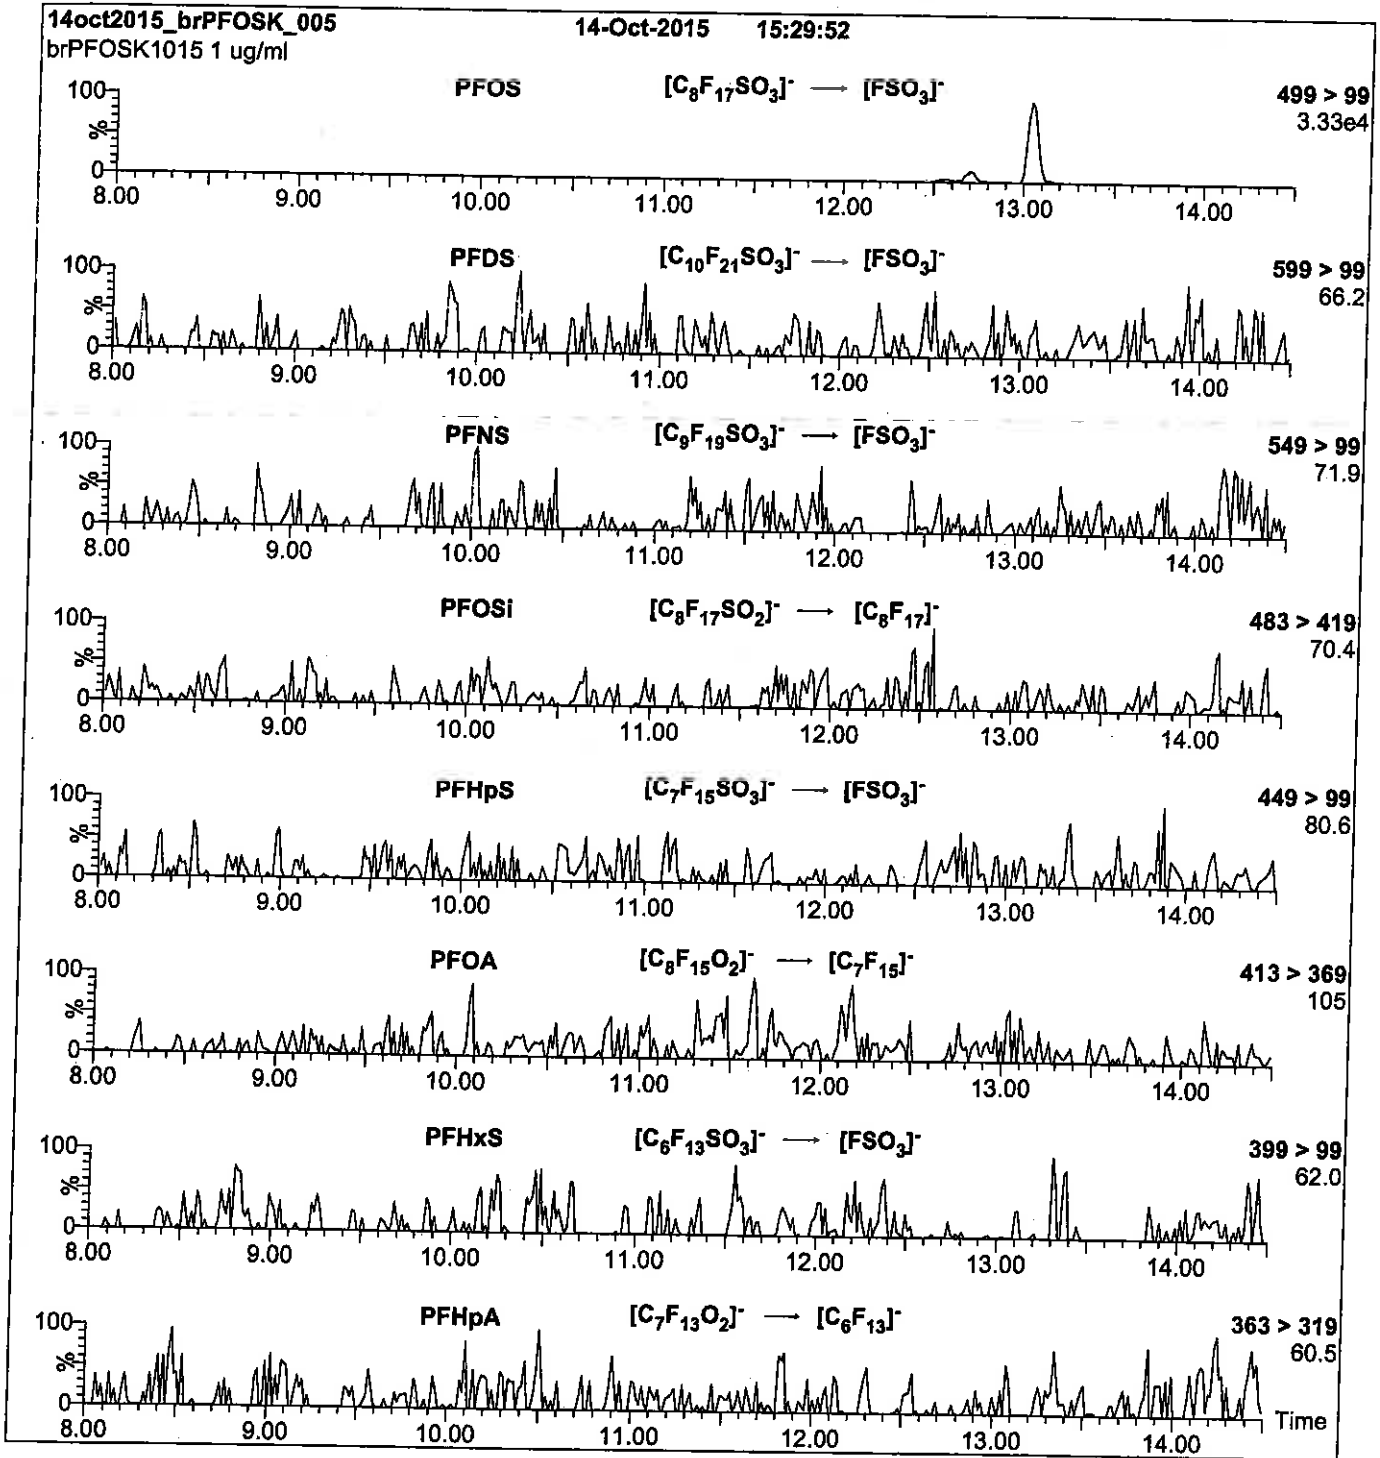

Conditions for Figure 3:

Injection: On-column

Mobile phase: Same as Figure 2

Flow: 300 μ /min

MS Parameters

Collision Gas (mbar) = 3.06e-3

Collision Energy (eV) = 11-50 (variable)

Reagent

LCPFOSA_00006




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: FOSA-I **LOT NUMBER:** FOSA0815I
COMPOUND: Perfluoro-1-octanesulfonamide

STRUCTURE: **CAS #:** 754-91-6



MOLECULAR FORMULA: $C_8H_2F_{17}NO_2S$ **MOLECULAR WEIGHT:** 499.14
CONCENTRATION: $50 \pm 2.5 \mu\text{g/ml}$ **SOLVENT(S):** Isopropanol
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 09/02/2015
EXPIRY DATE: (mm/dd/yyyy) 09/02/2017
RECOMMENDED STORAGE: Refrigerate ampoule

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
 Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: _____


 B.G. Chittim

Date: 09/11/2015
 (mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
 519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: FOSA-I; LC/MS Data (TIC and Mass Spectrum)

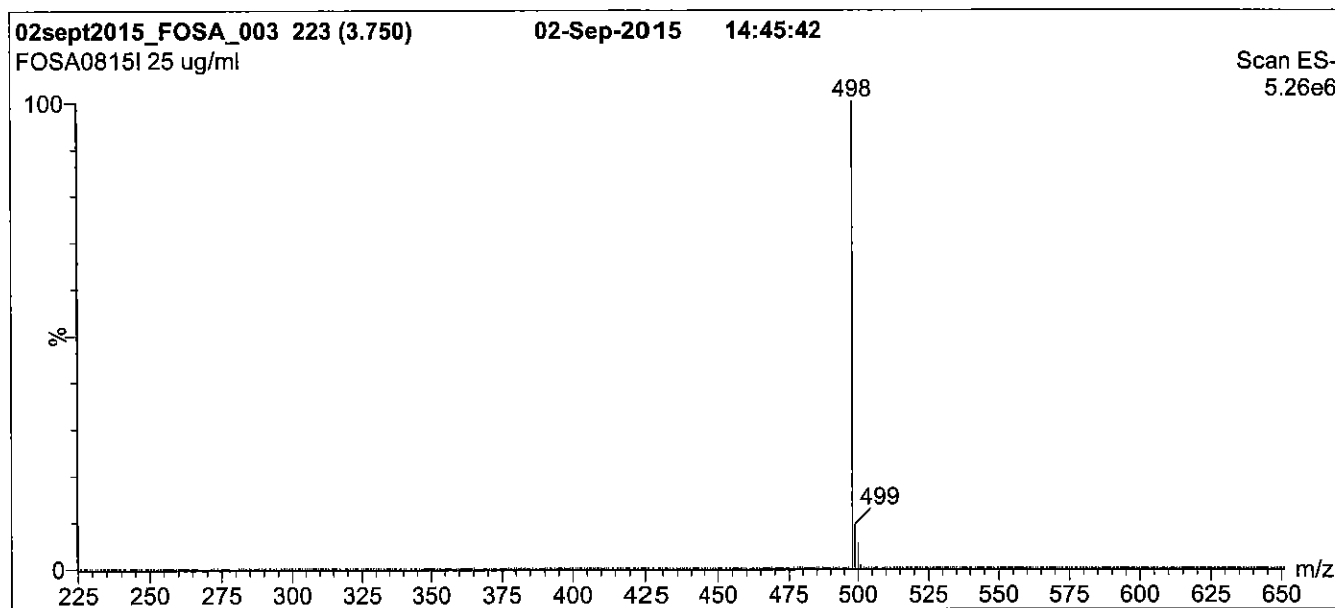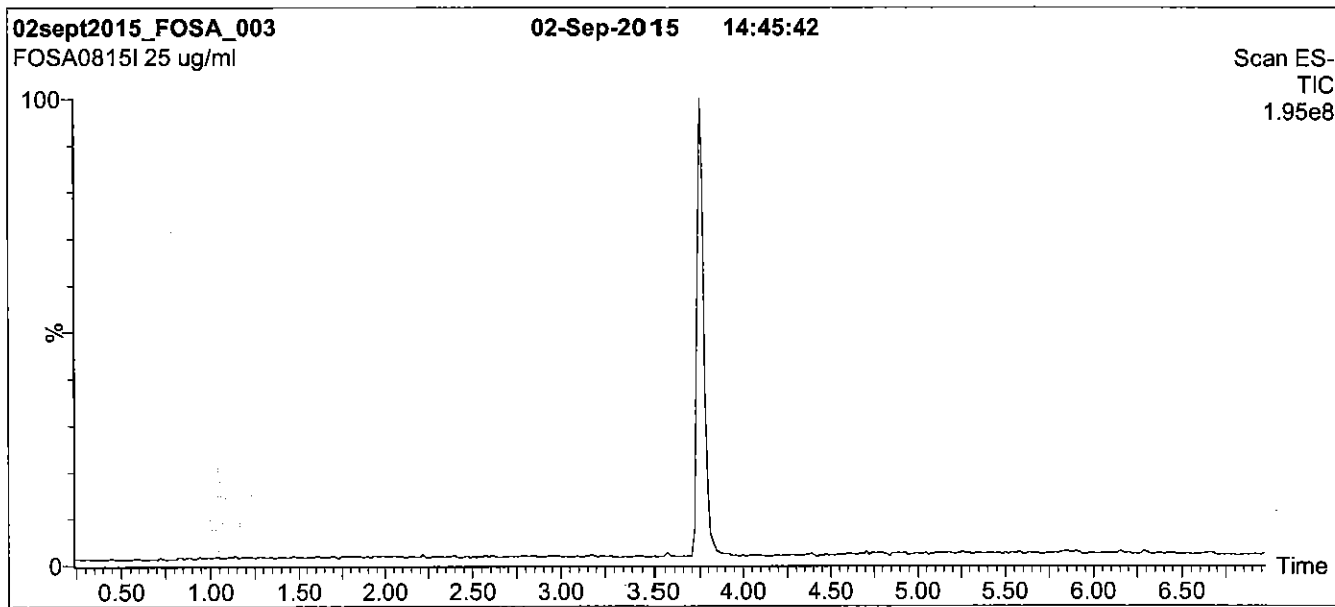

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP_{1a}
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 60% (80:20 MeOH:ACN) / 40% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.50
 Cone Voltage (V) = 40.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: FOSA-I; LC/MS/MS Data (Selected MRM Transitions)

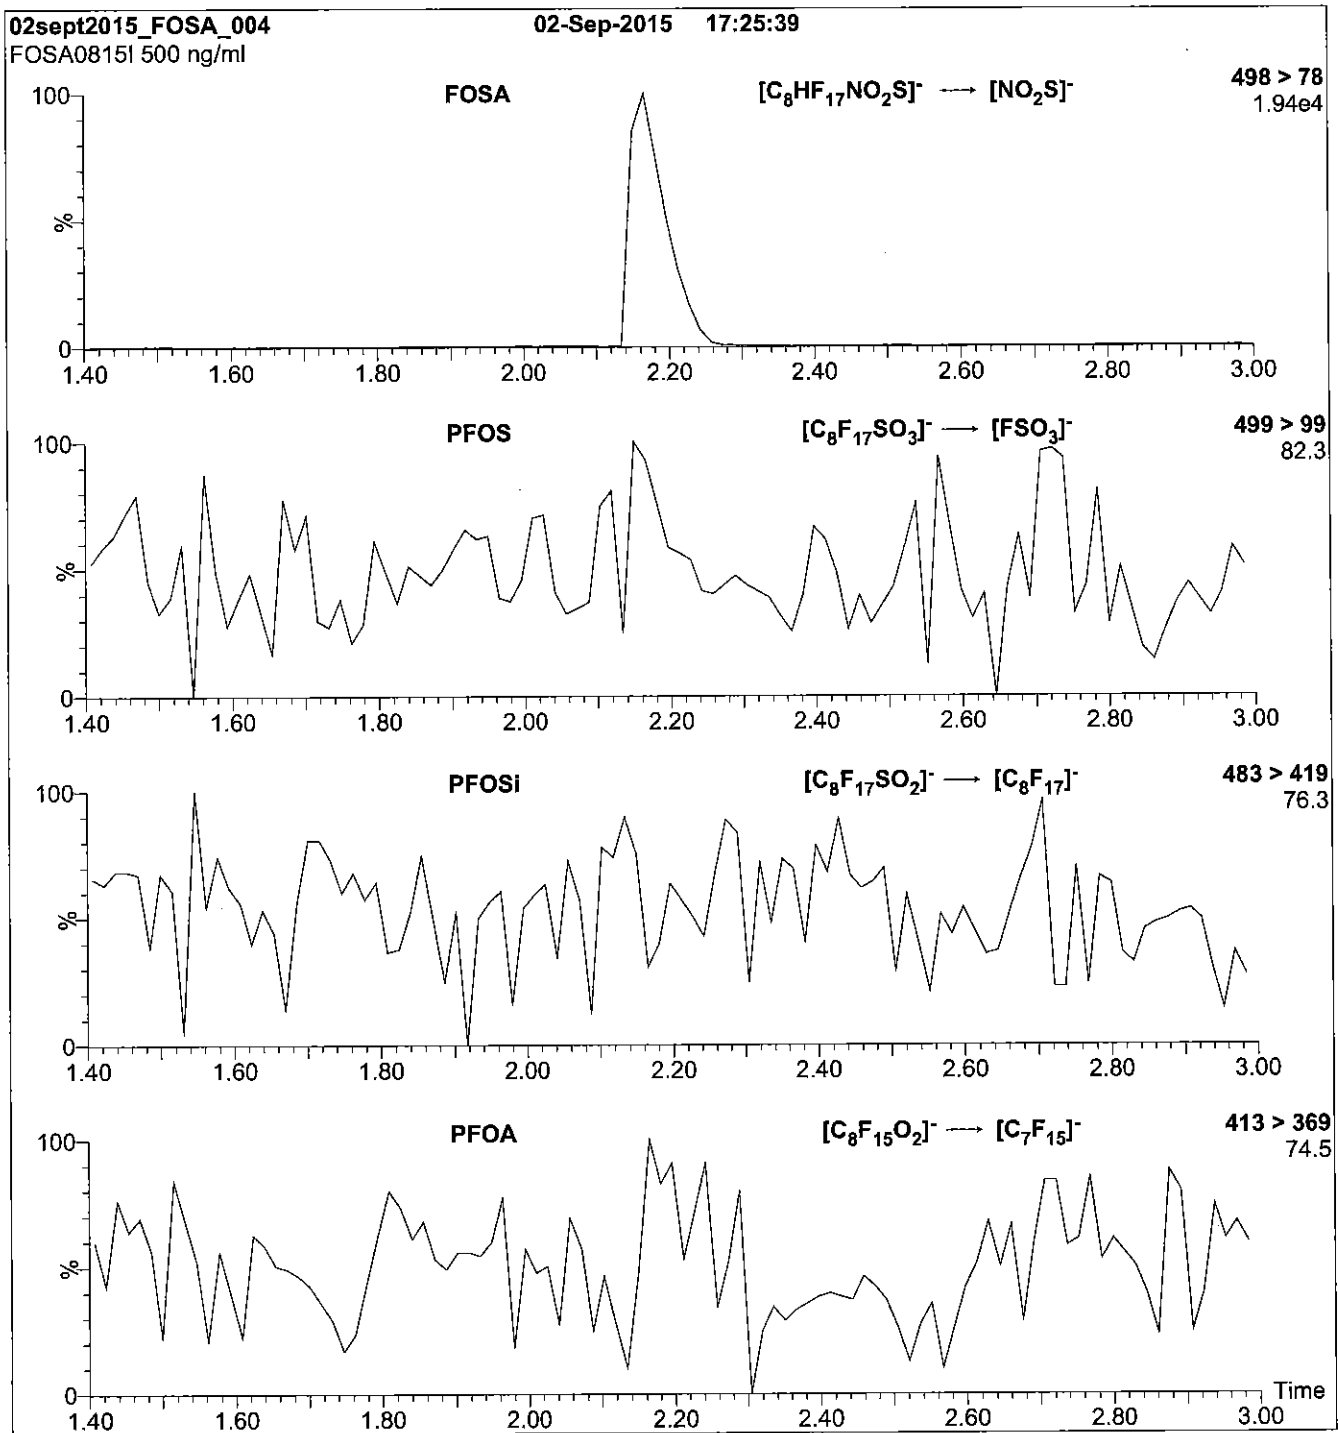

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml FOSA-I)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.54e-3
Collision Energy (eV) = 30

Reagent

LCPFOSA_00008

Scanned
10/14/16

R: SBC 9/13/16



730534
ID: LCPFOA_00009
Exp: 09/02/17 Prod: SBC
PF-1-octanesulfonamide



730533
ID: LCPFOA_00008
Exp: 09/02/17 Prod: SBC
PF-1-octanesulfonamide



WELLINGTON
LABORATORIES


CERTIFICATE OF ANALYSIS
DOCUMENTATION

PRODUCT CODE: FOSA-I
COMPOUND: Perfluoro-1-octanesulfonamide

LOT NUMBER: FOSA0815I

STRUCTURE:

CAS #: 754-91-6



MOLECULAR FORMULA: C₈H₂F₁₇NO₂S
CONCENTRATION: 50 ± 2.5 µg/ml
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 09/02/2015
EXPIRY DATE: (mm/dd/yyyy) 09/02/2017
RECOMMENDED STORAGE: Refrigerate ampoule

MOLECULAR WEIGHT: 499.14
SOLVENT(S): Isopropanol

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim

Date: 09/11/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: FOSA-I; LC/MS Data (TIC and Mass Spectrum)

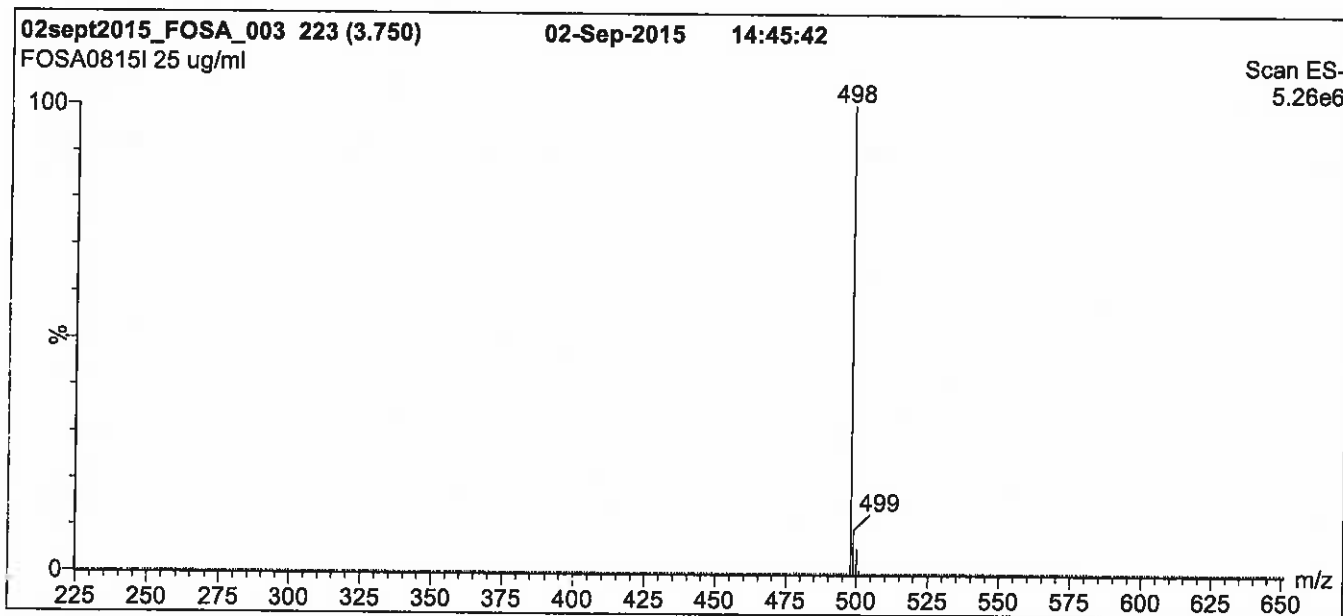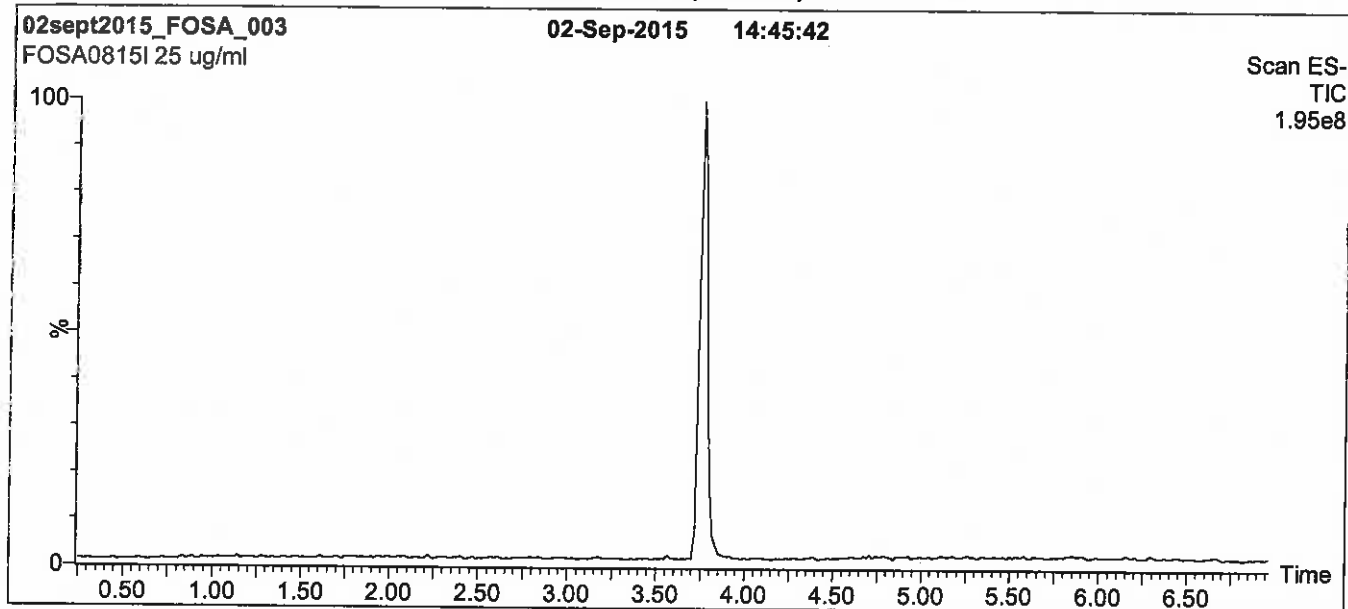

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro micro API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 60% (80:20 MeOH:ACN) / 40% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 2.50
Cone Voltage (V) = 40.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: FOSA-I; LC/MS/MS Data (Selected MRM Transitions)

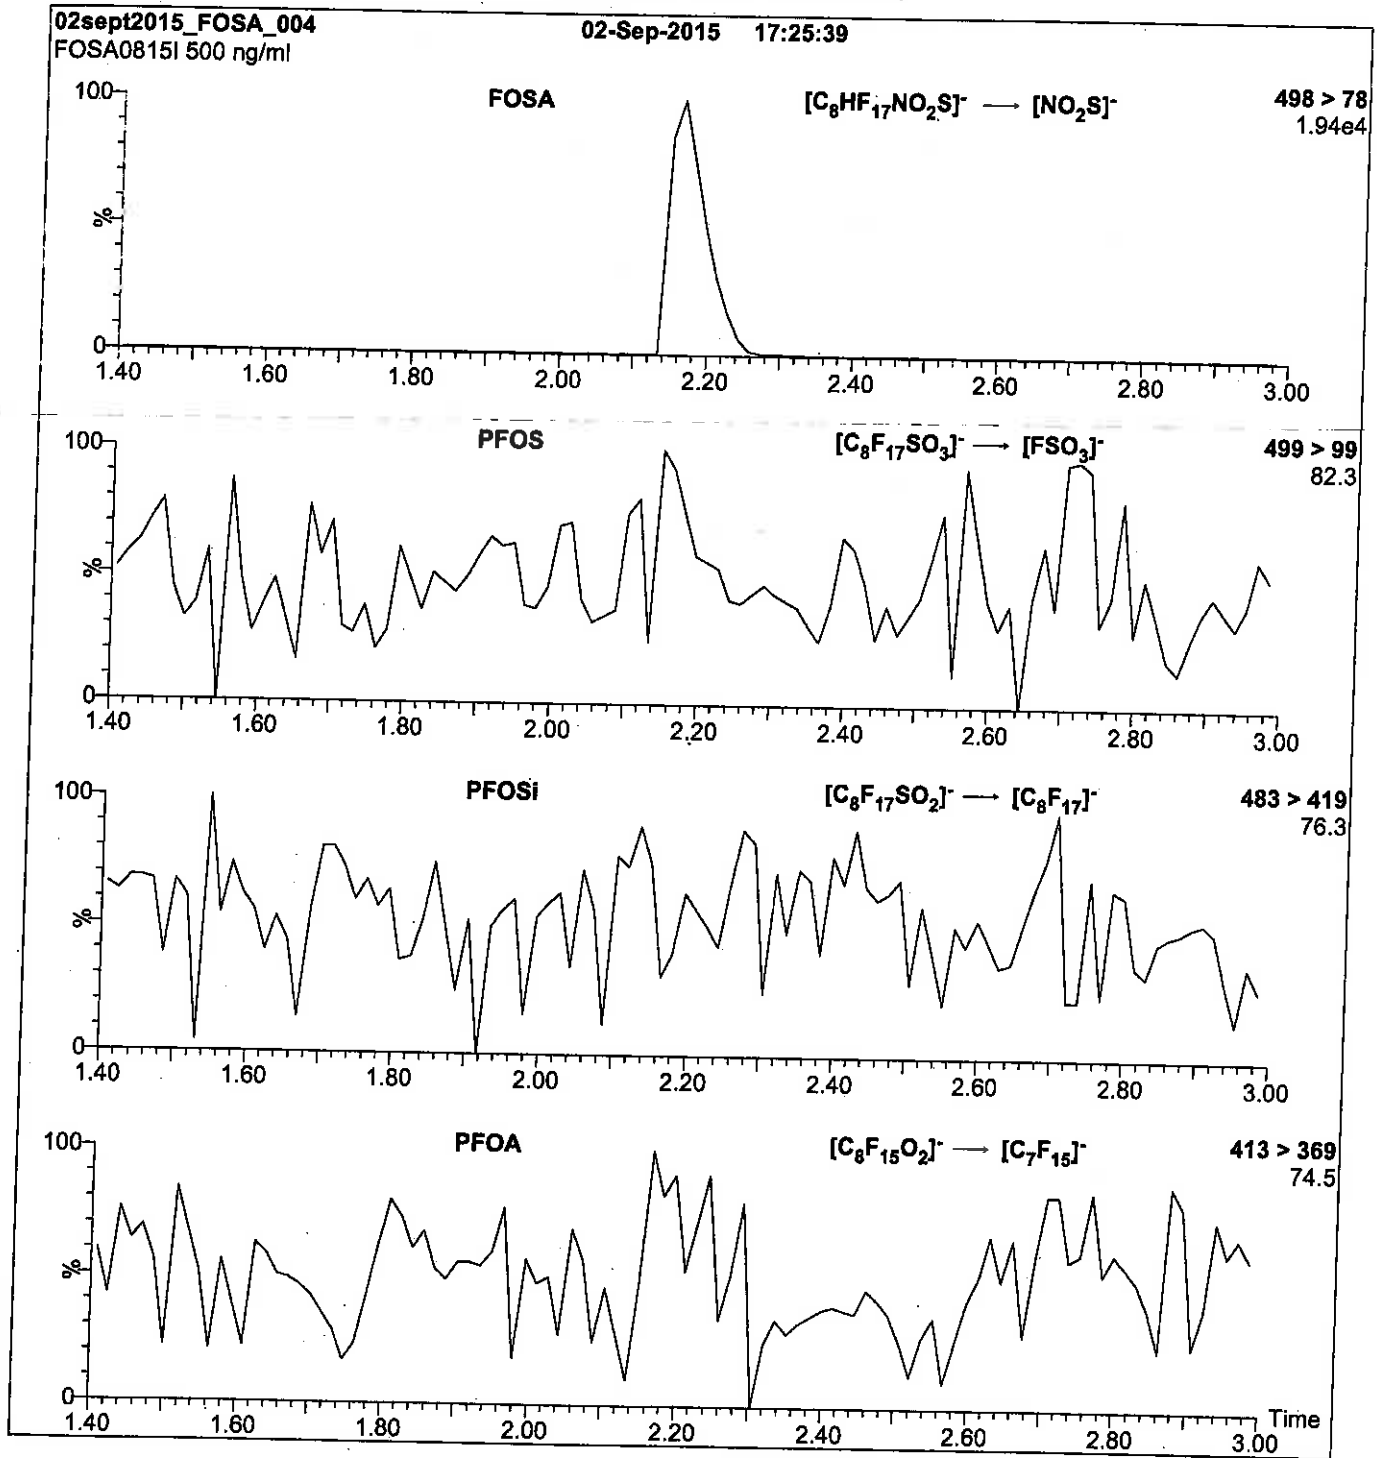

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml FOSA-I)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.54e-3
Collision Energy (eV) = 30

Reagent

LCFPeA_00005

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFPeA; LC/MS Data (TIC and Mass Spectrum)

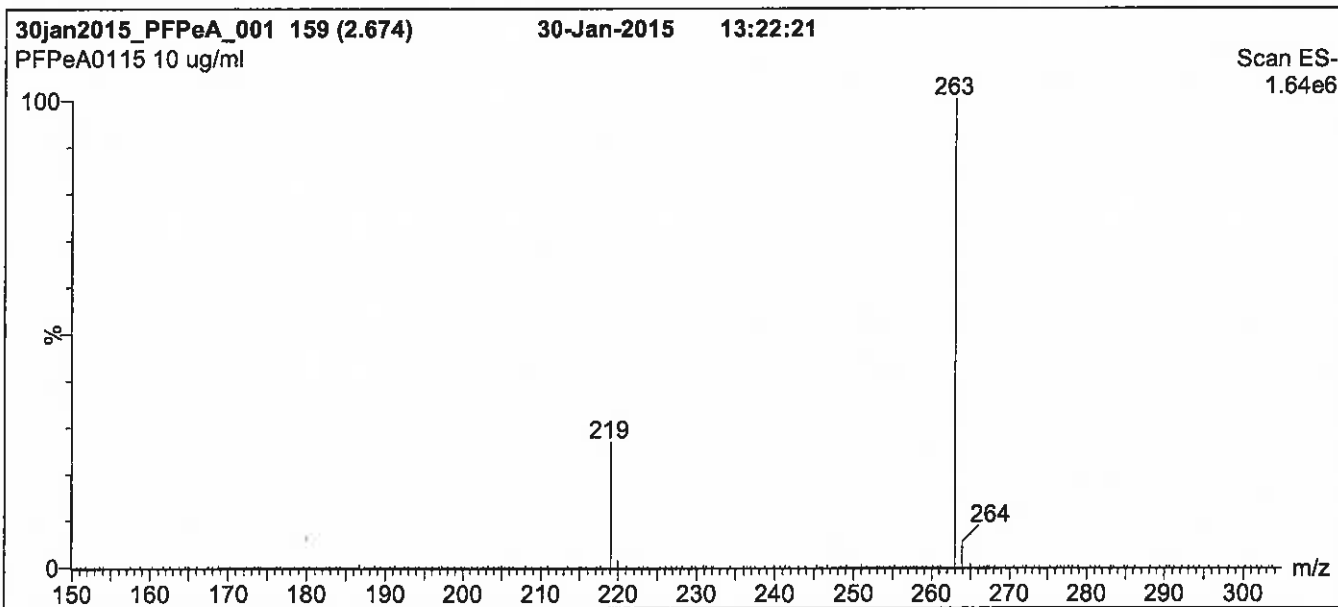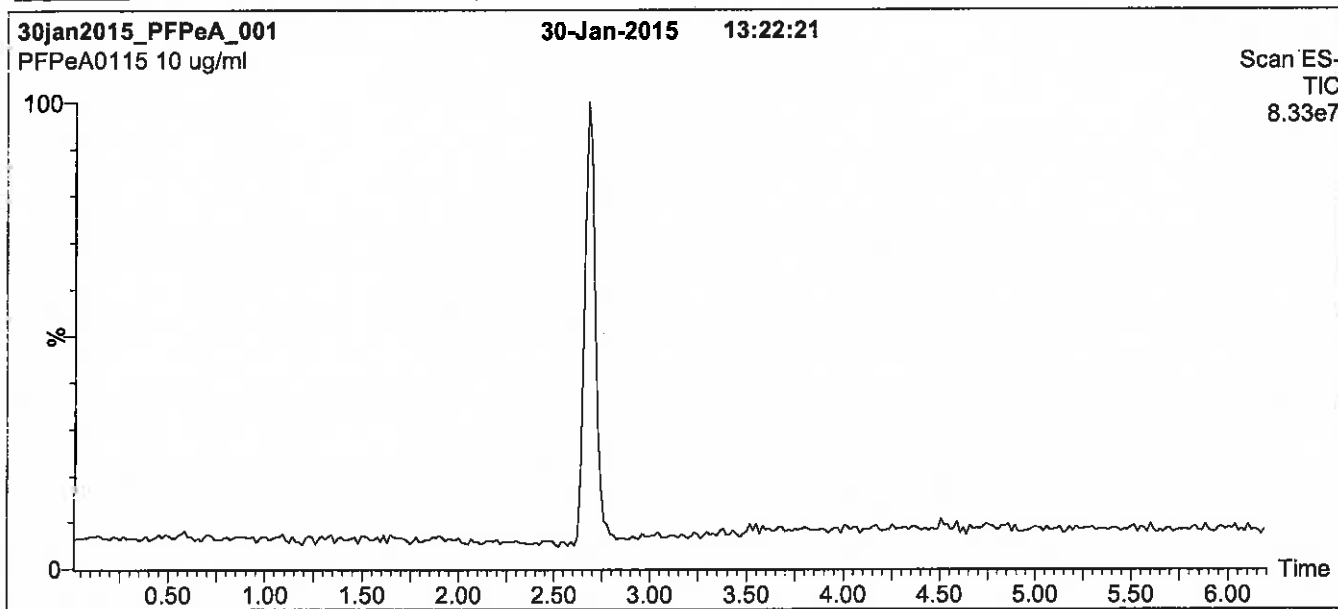

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 30% (80:20 MeOH:ACN) / 70% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7.5 min and hold for 1 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.00
 Cone Voltage (V) = 15.00
 Cone Gas Flow (l/hr) = 60
 Desolvation Gas Flow (l/hr) = 750

Figure 2: PFPeA; LC/MS/MS Data (Selected MRM Transitions)

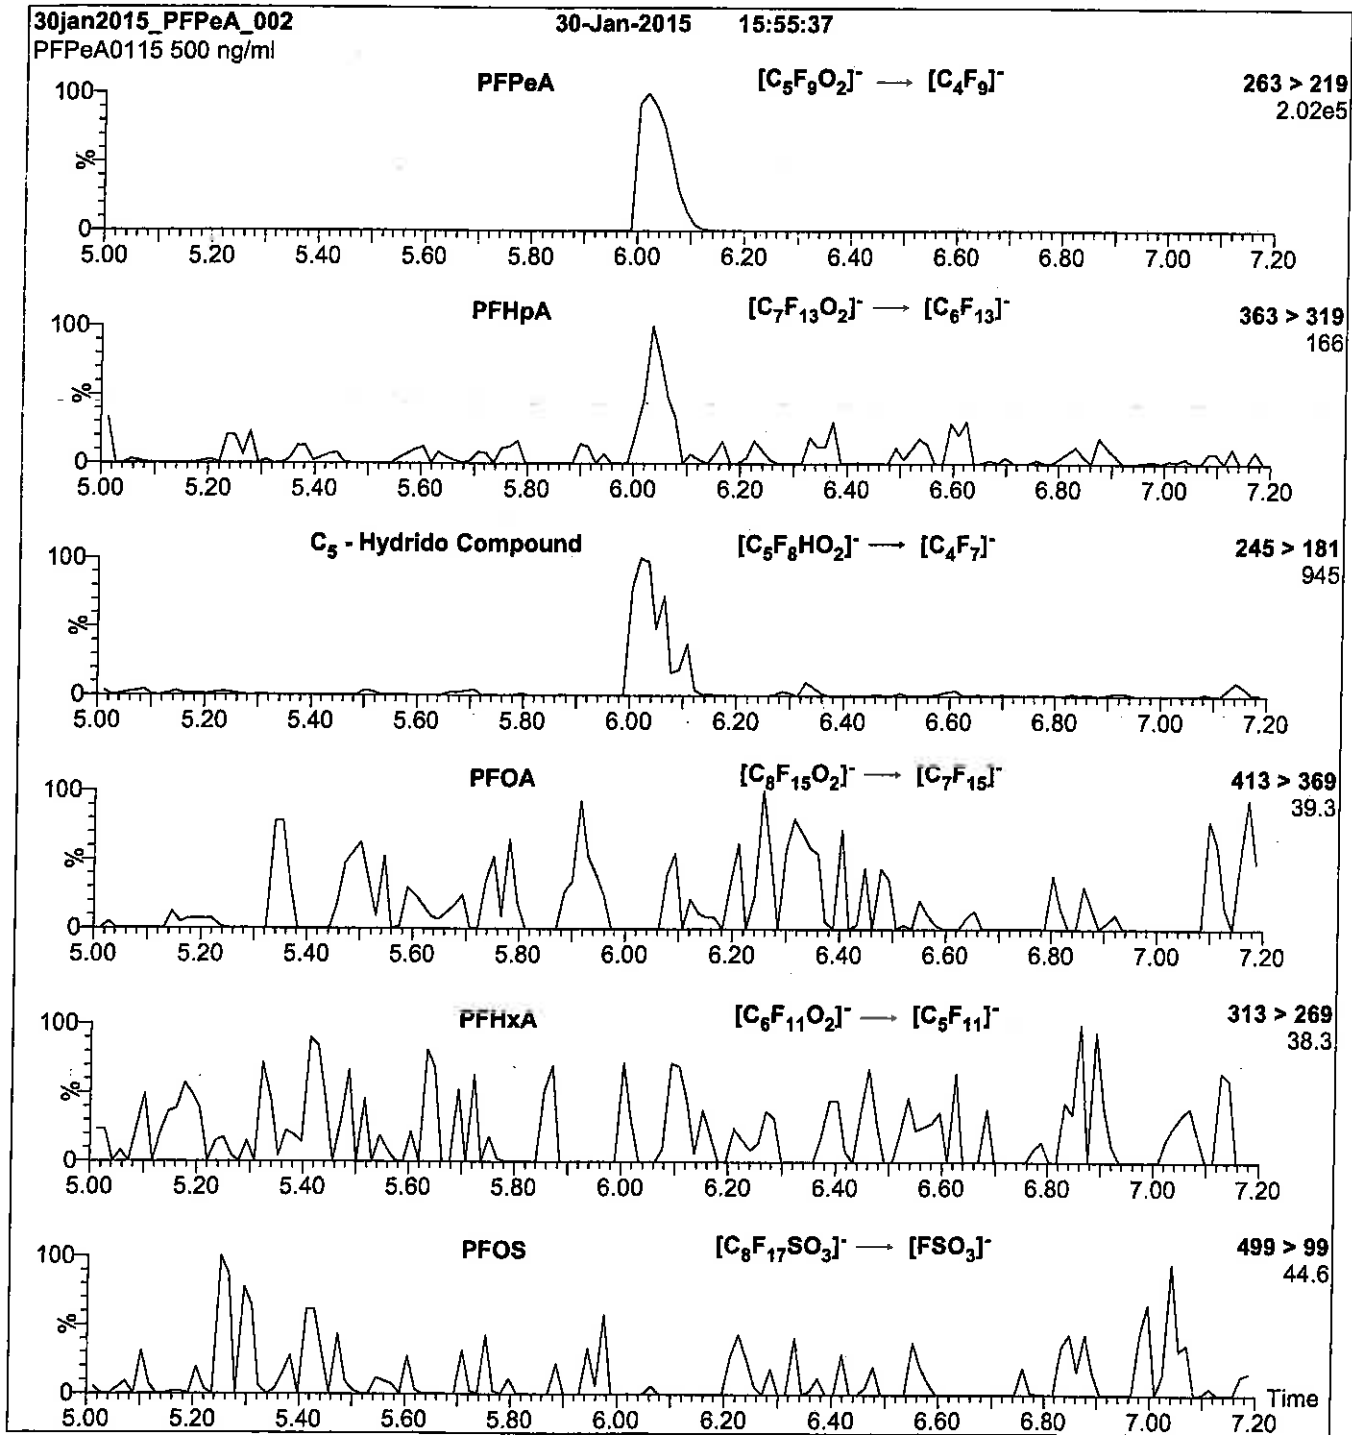

Conditions for Figure 2:

Injection: Direct loop injection
 10 μ l (500 ng/ml PFPeA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.35e-3
 Collision Energy (eV) = 9

Reagent

LCPFTeDA_00004




R: 4/7/16 CBW

609636

ID: LCPFTeDA_00004

Exp: 12/09/20 Prod: CBW

PF-n-tetradecanoic acid

**WELLINGTON**
LABORATORIES**CERTIFICATE OF ANALYSIS**
DOCUMENTATION**PRODUCT CODE:** PFTeDA **LOT NUMBER:** PFTeDA1215
COMPOUND: Perfluoro-n-tetradecanoic acid**STRUCTURE:** **CAS #:** 376-06-7

MOLECULAR FORMULA:	$C_{14}H_{27}O_2$	MOLECULAR WEIGHT:	714.11
CONCENTRATION:	$50 \pm 2.5 \mu\text{g/ml}$	SOLVENT(S):	Methanol Water (<1%)
CHEMICAL PURITY:	>98%		
LAST TESTED: (mm/dd/yyyy)	12/09/2015		
EXPIRY DATE: (mm/dd/yyyy)	12/09/2020		
RECOMMENDED STORAGE:	Store ampoule in a cool, dark place		

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains ~ 0.2% of PFDoA ($C_{12}H_{23}O_2$) and ~ 0.2% of PFPeDA ($C_{15}H_{29}O_2$).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:

B.G. Chittim

Date: 12/09/2015

(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFTeDA; LC/MS Data (TIC and Mass Spectrum)

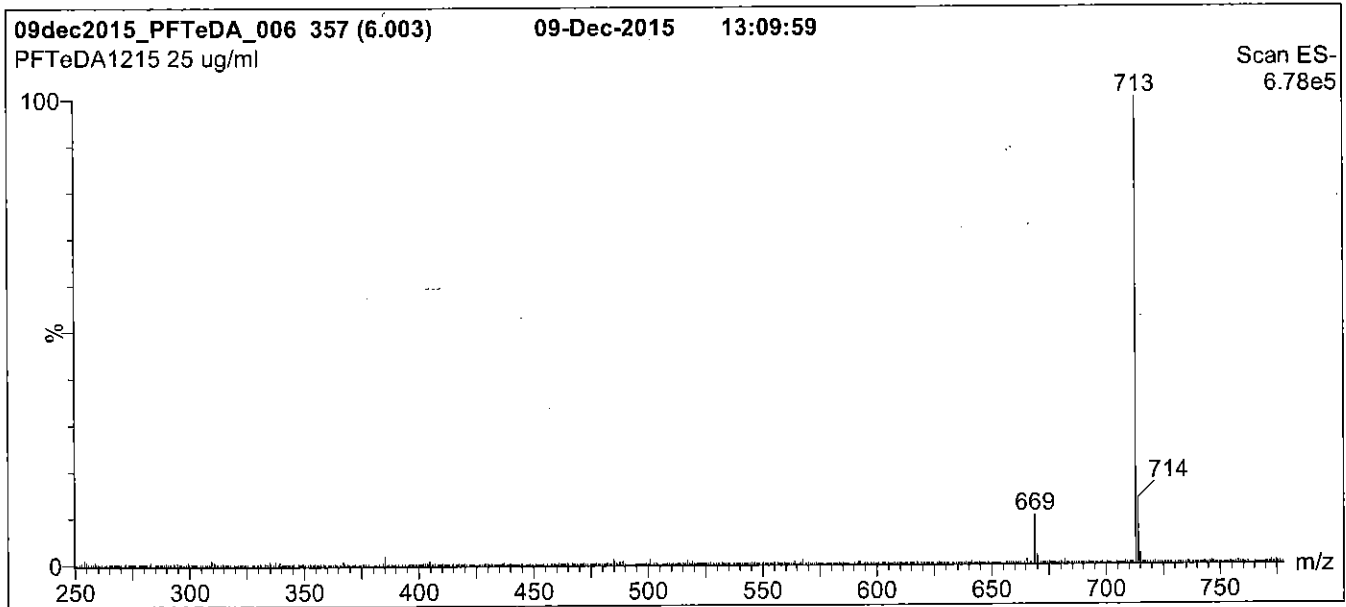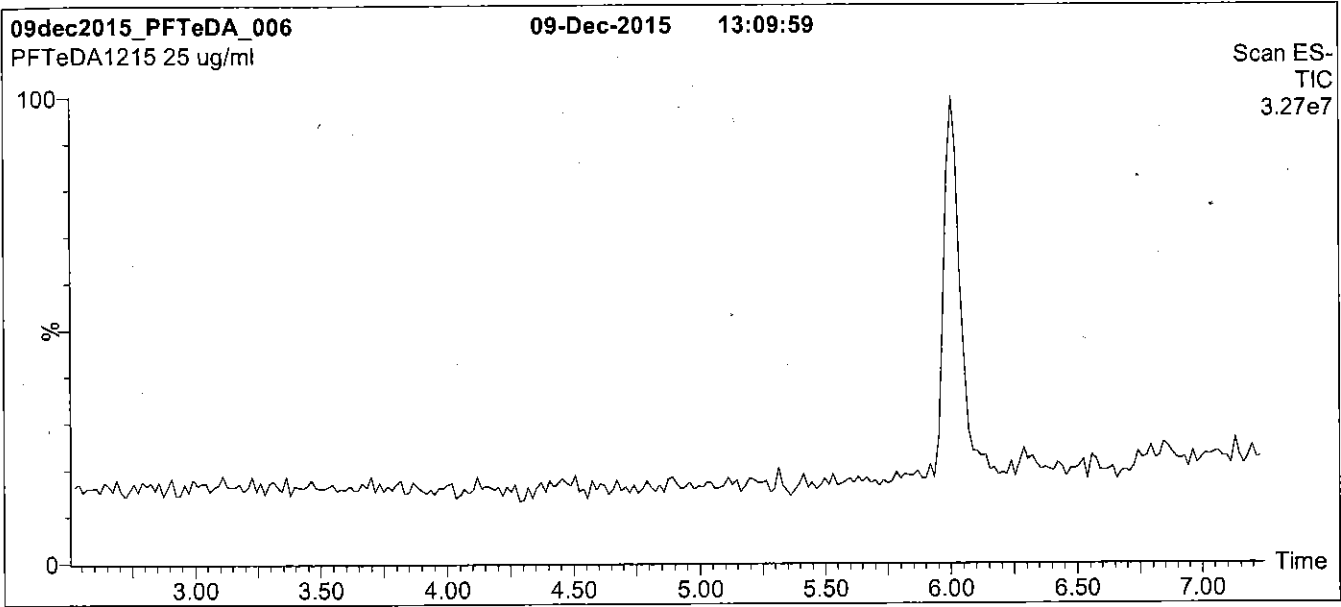

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro micro API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 65% (80:20 MeOH:ACN) / 35% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7.5 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (250 - 1250 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 15.00
 Cone Gas Flow (l/hr) = 60
 Desolvation Gas Flow (l/hr) = 750

Figure 2: PFTeDA; LC/MS/MS Data (Selected MRM Transitions)

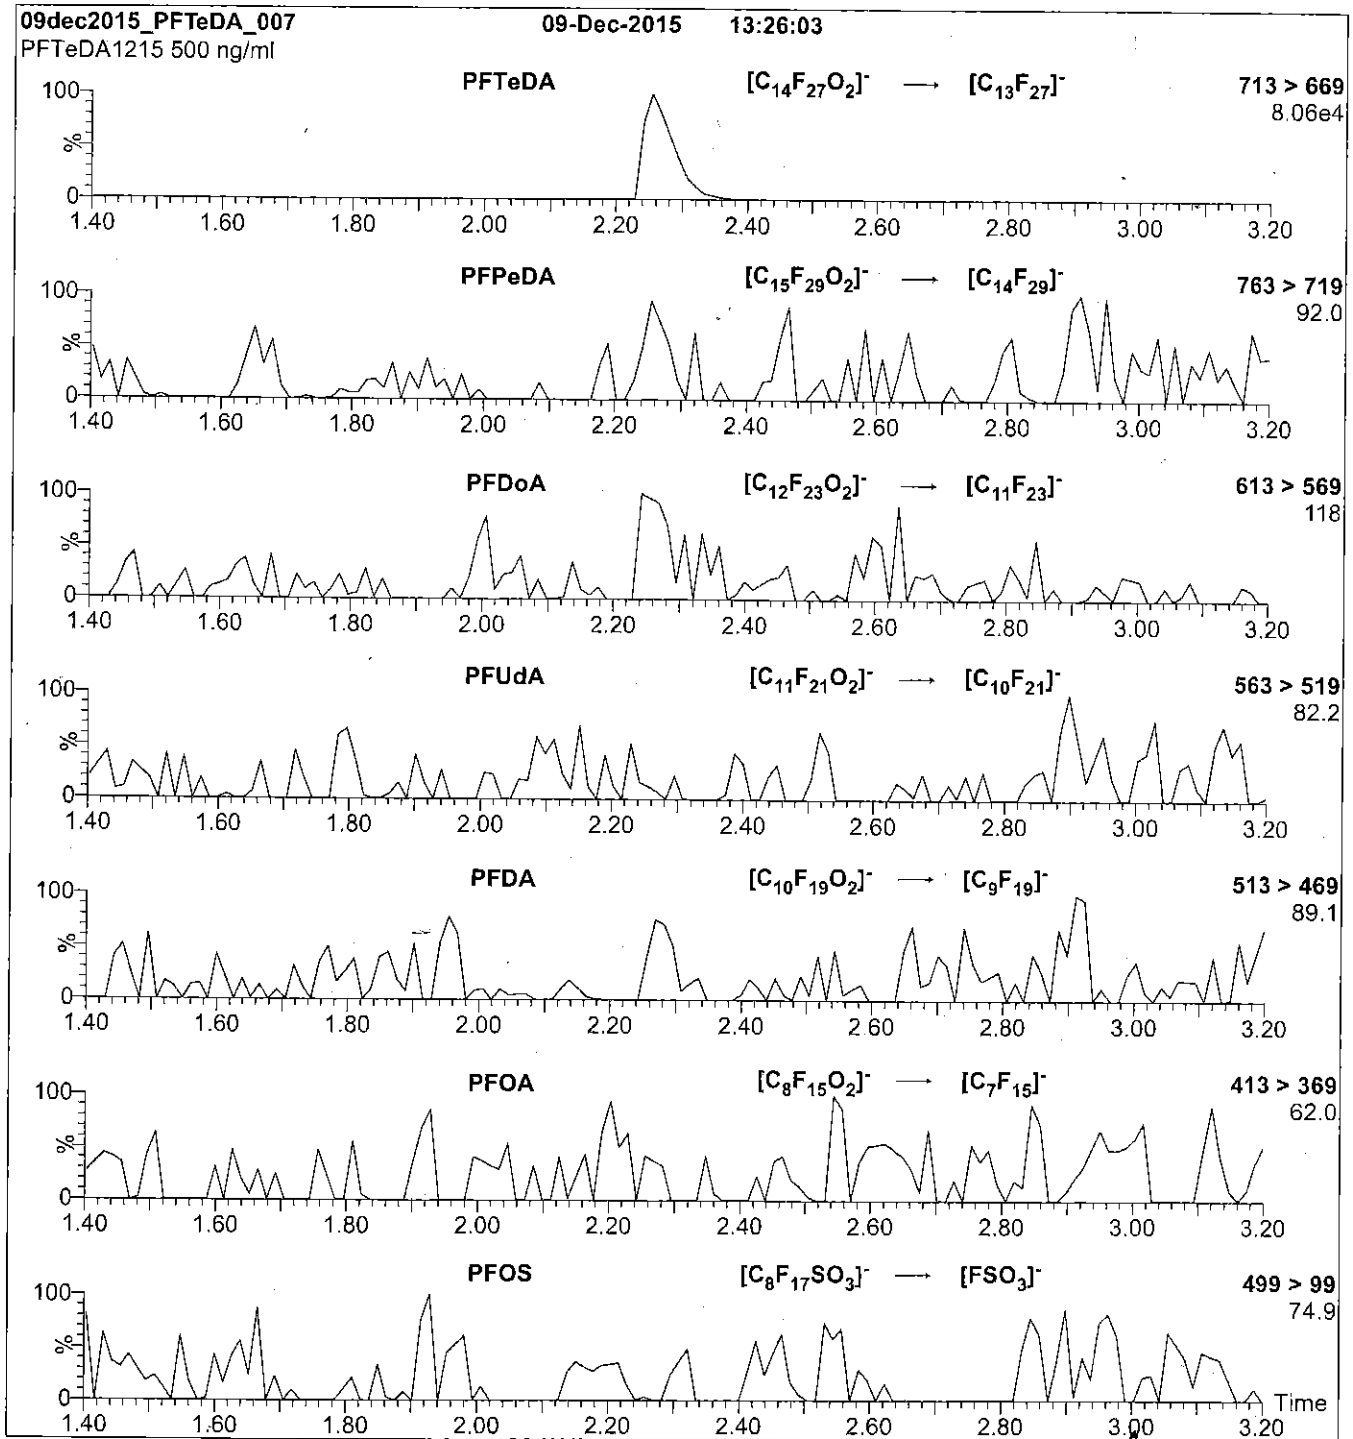

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml PFTeDA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.43e-3
Collision Energy (eV) = 14

Reagent

LCPFTeDA_00005

R: SBG 9/13/16



730645
ID: LCPFTeDA_00005
Exp: 12/09/20 Prpd: SEC
PF-n-tetradecanoic acid



730659
ID: LCPFTeDA_00006
Exp: 12/09/20 Prpd: SEC
PF-n-tetradecanoic acid




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: PFTeDA **LOT NUMBER:** PFTeDA1215
COMPOUND: Perfluoro-n-tetradecanoic acid

STRUCTURE: **CAS #:** 376-06-7

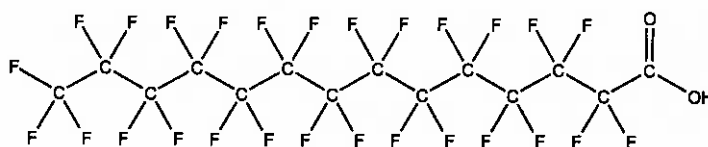

MOLECULAR FORMULA: C₁₄H₂₇F₂₇O₂ **MOLECULAR WEIGHT:** 714.11
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Methanol
Water (<1%)
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 12/09/2015
EXPIRY DATE: (mm/dd/yyyy) 12/09/2020
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains ~ 0.2% of PFDoA (C₁₂H₂₃F₂₃O₂) and ~ 0.2% of PFPeDA (C₁₆H₂₉F₂₉O₂).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:

B.G. Chittim

Date: 12/09/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFTeDA; LC/MS Data (TIC and Mass Spectrum)

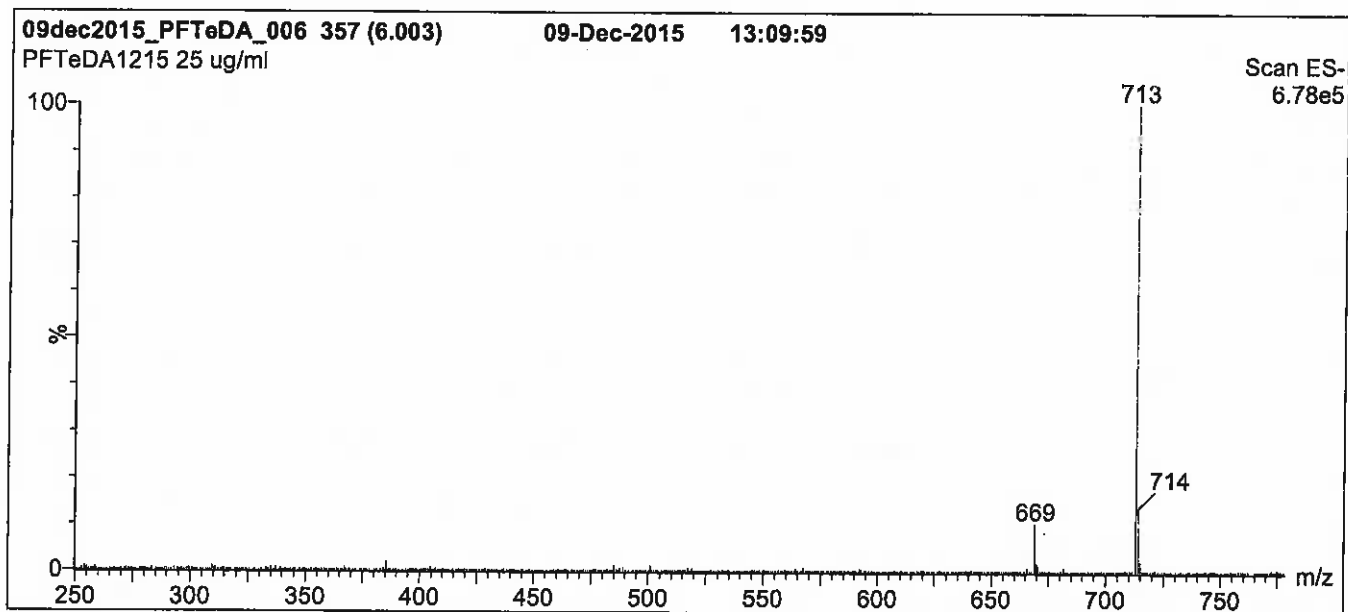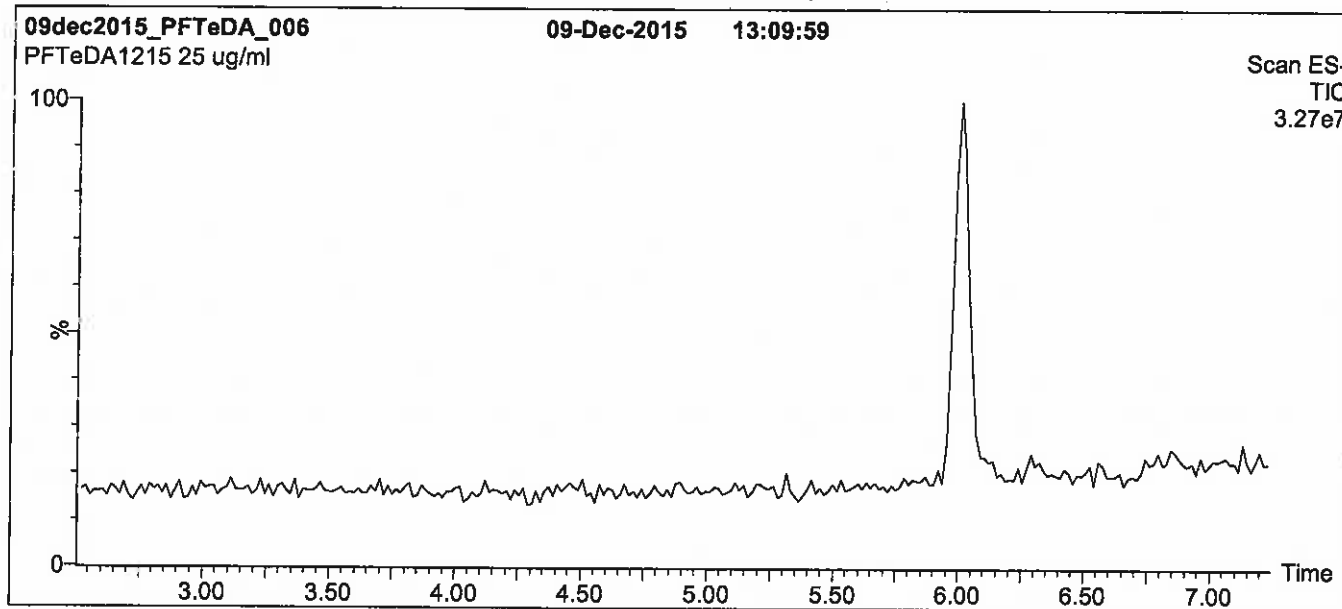

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 65% (80:20 MeOH:ACN) / 35% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7.5 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (250 - 1250 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 60
Desolvation Gas Flow (l/hr) = 750

Figure 2: PFTeDA; LC/MS/MS Data (Selected MRM Transitions)

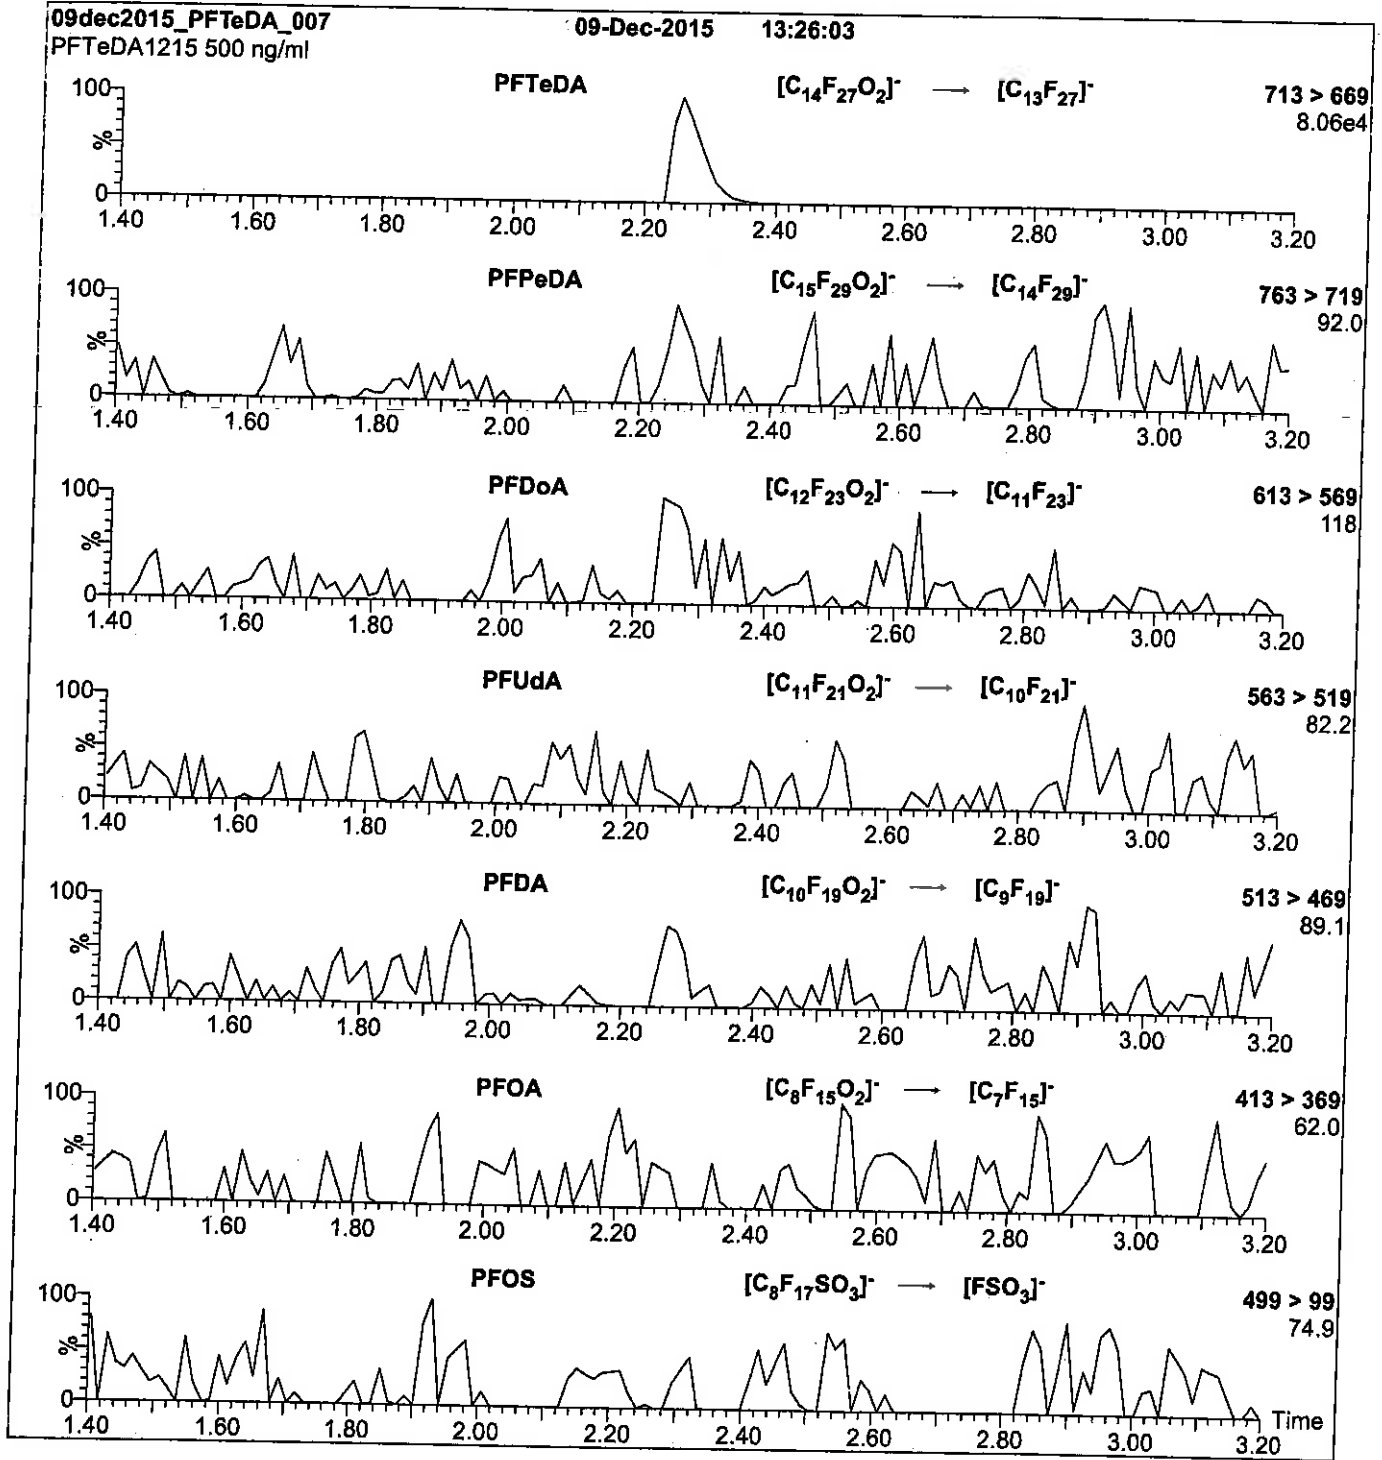

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml PFTeDA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.43e-3
Collision Energy (eV) = 14

Reagent

LCPFT_rDA_00004





R: 4/7/16 CBW

609697

ID: LCPFTrDA_00004

Exp: 12/10/18 Ppdt: CBW

PF-n-tridecanoic acid

**WELLINGTON**
LABORATORIES**CERTIFICATE OF ANALYSIS**
DOCUMENTATION**PRODUCT CODE:** PFTTrDA **LOT NUMBER:** PFTTrDA1213
COMPOUND: Perfluoro-n-tridecanoic acid**STRUCTURE:** **CAS #:** 72629-94-8

MOLECULAR FORMULA:	$C_{13}H_2F_{25}O_2$	MOLECULAR WEIGHT:	664.11
CONCENTRATION:	$50 \pm 2.5 \mu\text{g/ml}$	SOLVENT(S):	Methanol Water (<1%)
CHEMICAL PURITY:	>98%		
LAST TESTED: (mm/dd/yyyy)	12/10/2013		
EXPIRY DATE: (mm/dd/yyyy)	12/10/2018		
RECOMMENDED STORAGE:	Store ampoule in a cool, dark place		

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains ~ 0.1% of PFUdA ($C_{11}H_2F_{21}O_2$); ~ 0.4% of PFDaA ($C_{12}H_2F_{23}O_2$), and ~ 0.1% of PFTeDA ($C_{14}H_2F_{27}O_2$).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:

B.G. Chittim
Date: 03/25/2015
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON 'N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFTrDA; LC/MS Data (TIC and Mass Spectrum)

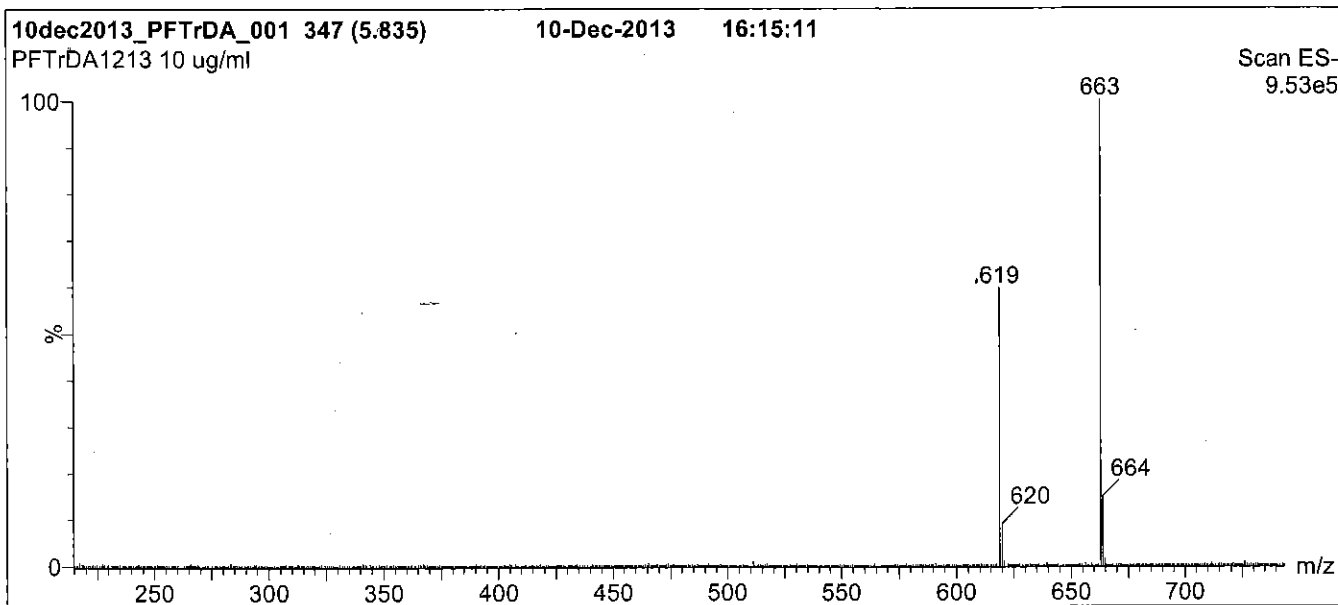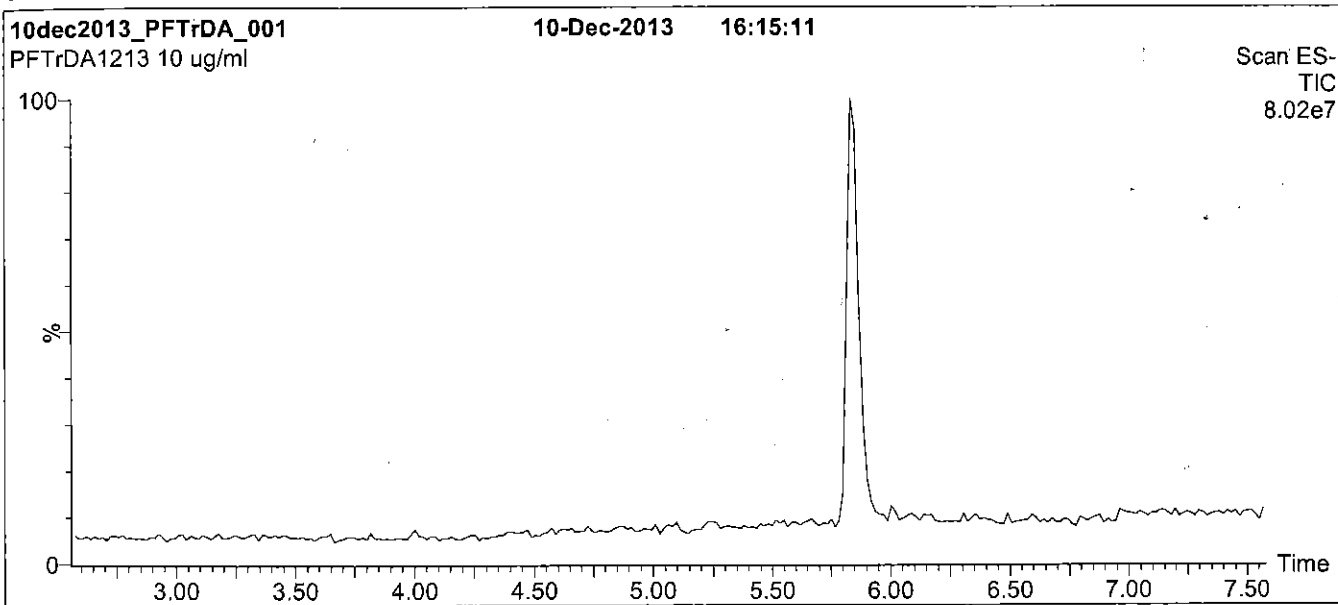

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 60% (80:20 MeOH:ACN) / 40% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (215 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.00
 Cone Voltage (V) = 22.00
 Cone Gas Flow (l/hr) = 60
 Desolvation Gas Flow (l/hr) = 650

Figure 2: PFTrDA; LC/MS/MS Data (Selected MRM Transitions)

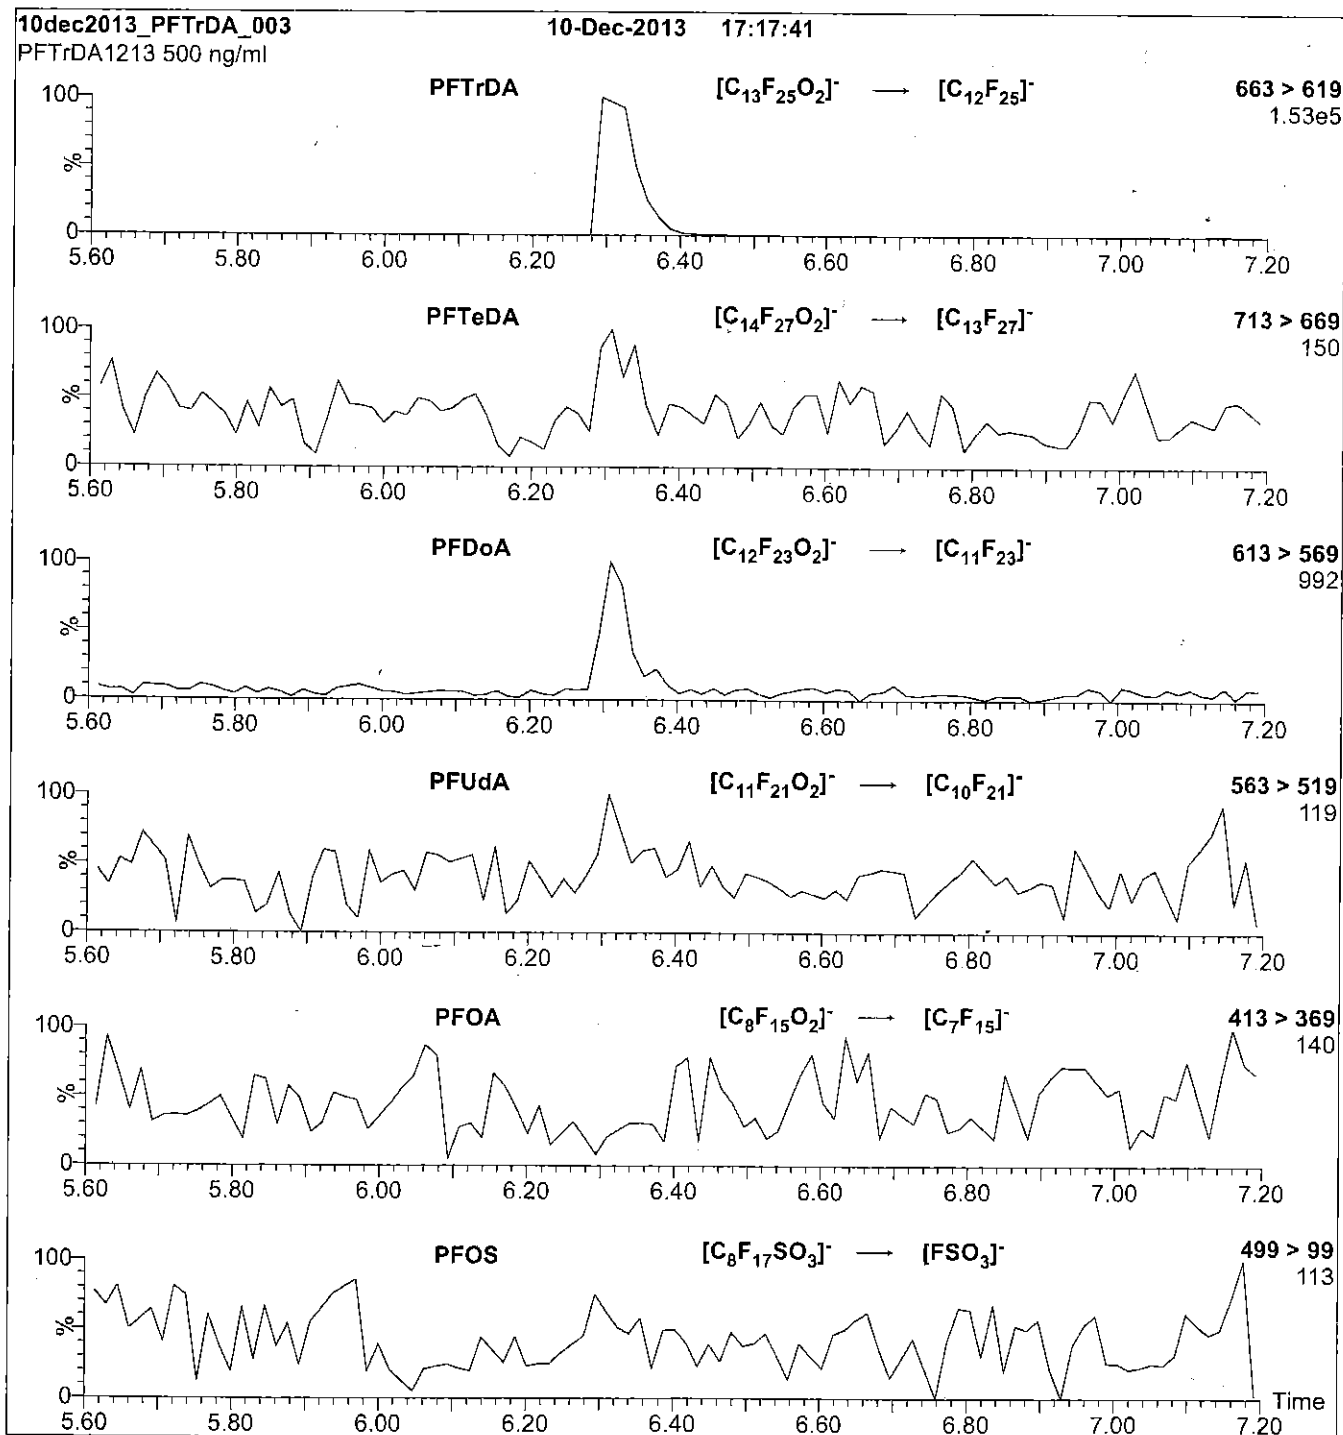

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml PFTrDA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.28e-3
Collision Energy (eV) = 15

Reagent

LCPFT_rDA_00005

R: SBC 9/13/16



730665
ID: LCPFTrDA_00005
Exp: 02/12/21 Prod: SBC
PF-n-tridecanoic acid



730666
ID: LCPFTrDA_00006
Exp: 02/12/21 Prod: SBC
PF-n-tridecanoic acid




WELLINGTON
LABORATORIES

CERTIFICATE OF ANALYSIS
DOCUMENTATION

PRODUCT CODE: PFTrDA **LOT NUMBER:** PFTrDA0216
COMPOUND: Perfluoro-n-tridecanoic acid

STRUCTURE: **CAS #:** 72629-94-8



MOLECULAR FORMULA: $C_{13}HF_{25}O_2$ **MOLECULAR WEIGHT:** 664.11
CONCENTRATION: $50 \pm 2.5 \mu\text{g/ml}$ **SOLVENT(S):** Methanol
Water (<1%)
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 02/12/2016
EXPIRY DATE: (mm/dd/yyyy) 02/12/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains ~ 0.1% of PFUdA ($C_{11}HF_{21}O_2$), ~ 0.4% of PFDdA ($C_{12}HF_{23}O_2$), and ~ 0.1% of PFTeDA ($C_{14}HF_{27}O_2$).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:

B.G. Chittim

Date: 02/16/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFTTrDA; LC/MS Data (TIC and Mass Spectrum)

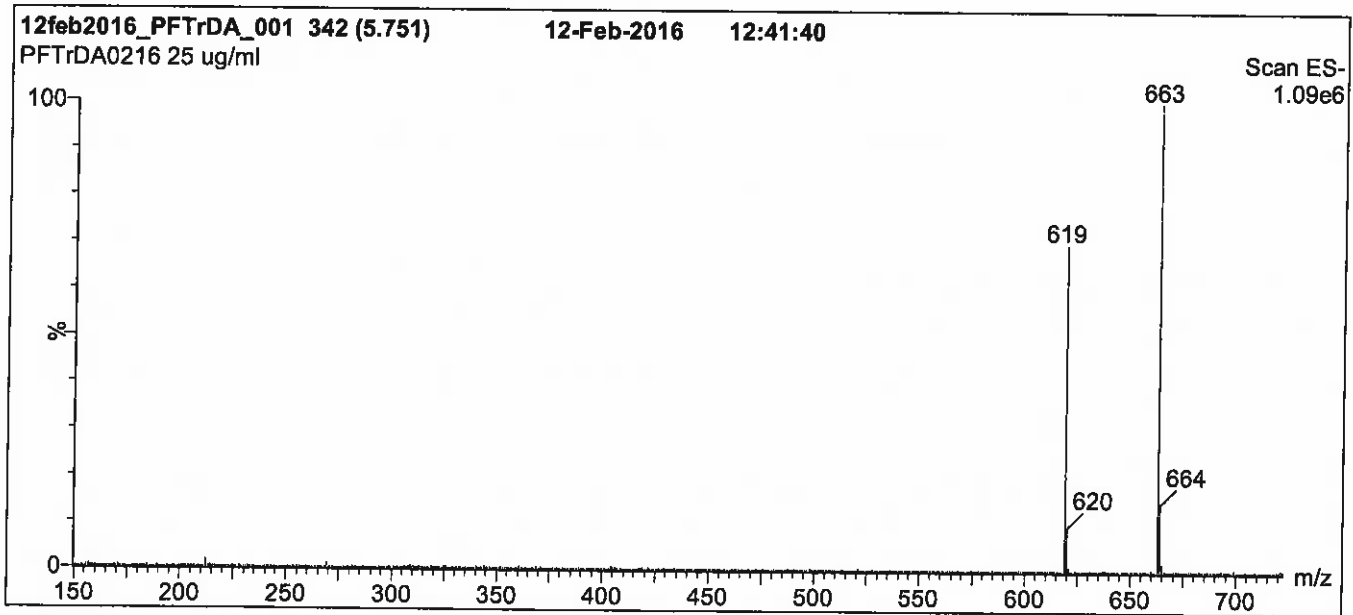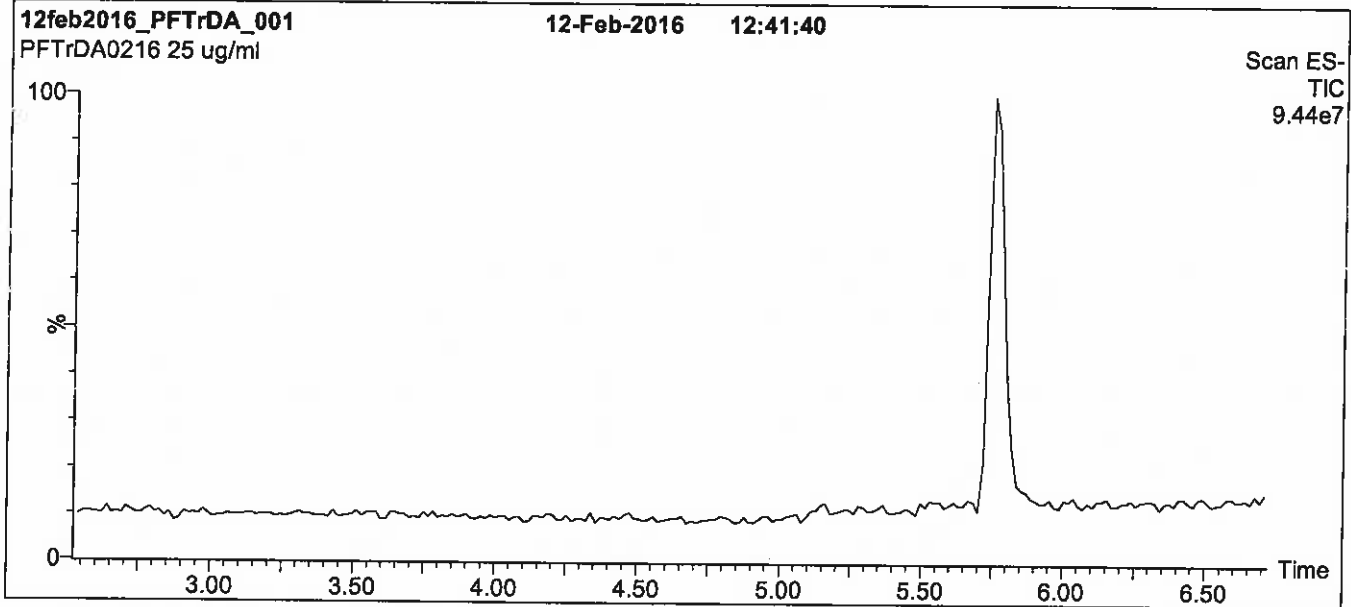

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 60% (80:20 MeOH:ACN) / 40% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 22.00
Cone Gas Flow (l/hr) = 60
Desolvation Gas Flow (l/hr) = 650

Figure 2: PFTrDA; LC/MS/MS Data (Selected MRM Transitions)

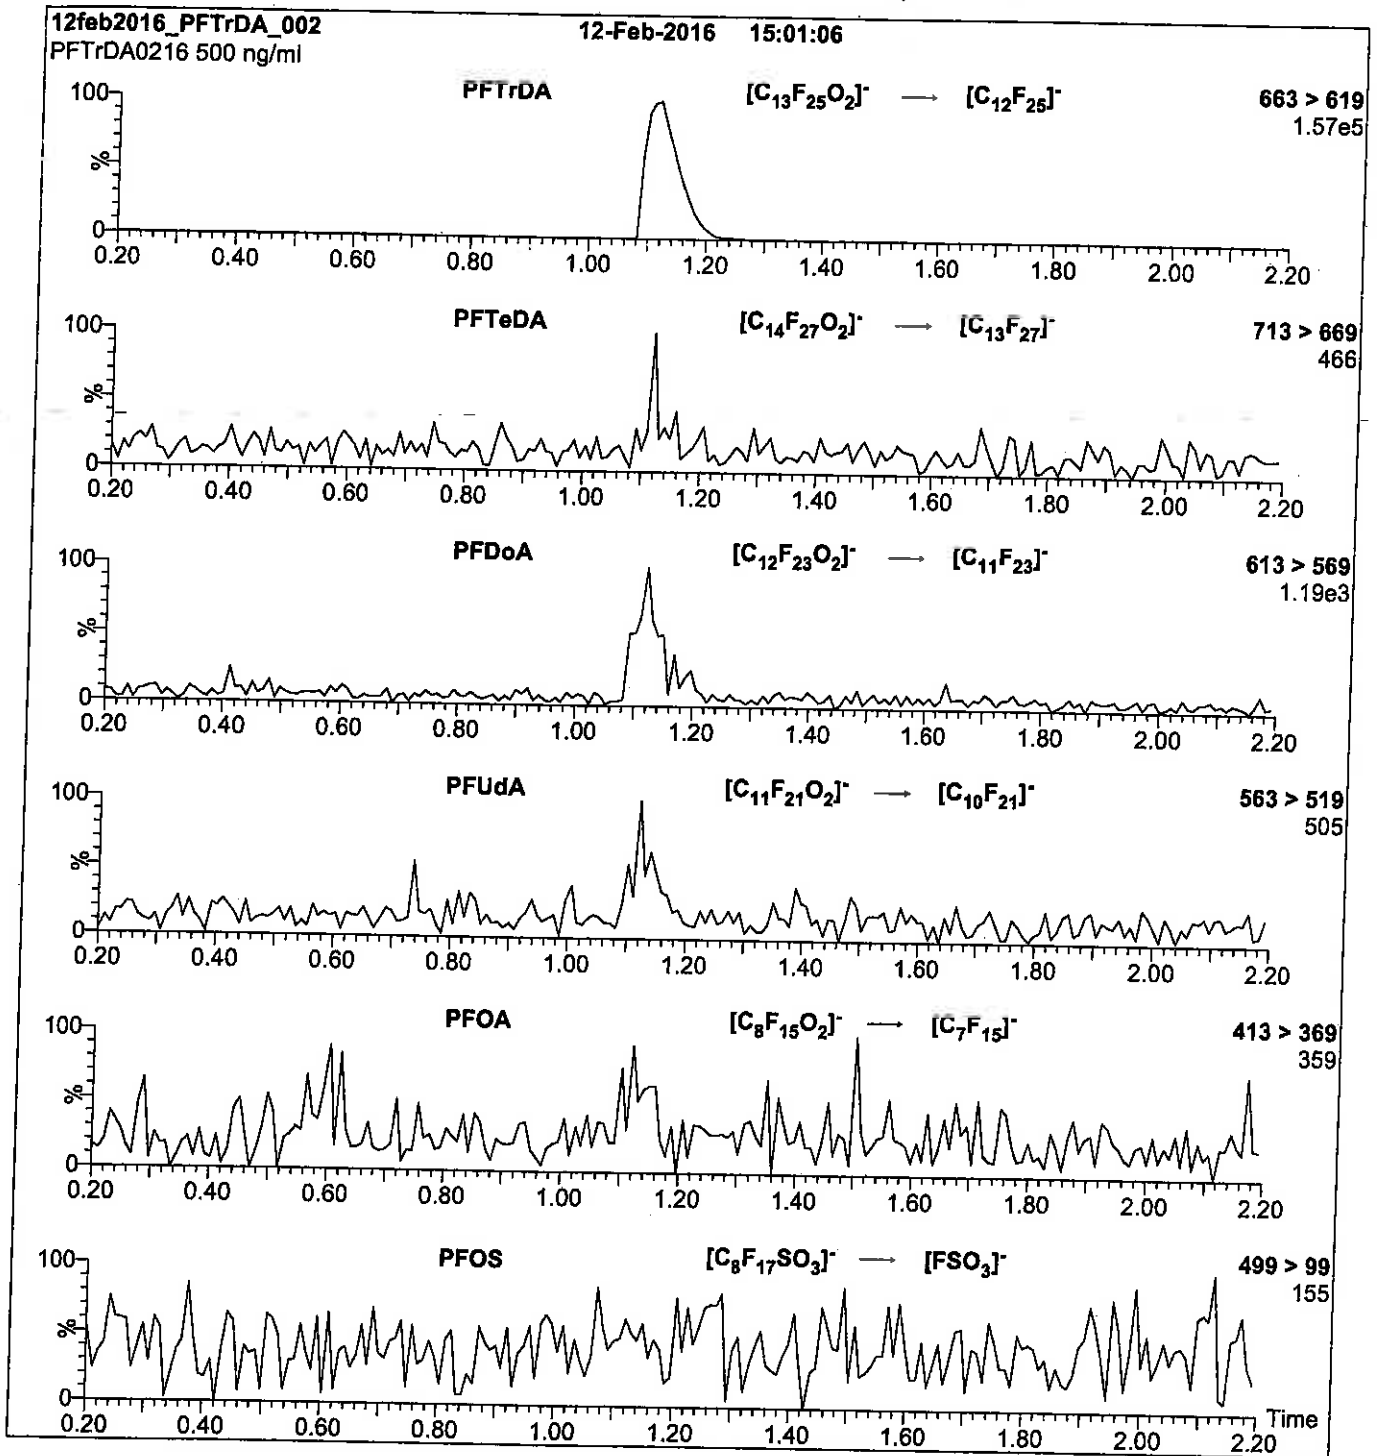

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml PFTrDA)

Mobile phase: Isocratic 80% MeOH / 20% H₂O

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.35e-3
Collision Energy (eV) = 15

Reagent

LCPFUdA_00005

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFUdA; LC/MS Data (TIC and Mass Spectrum)

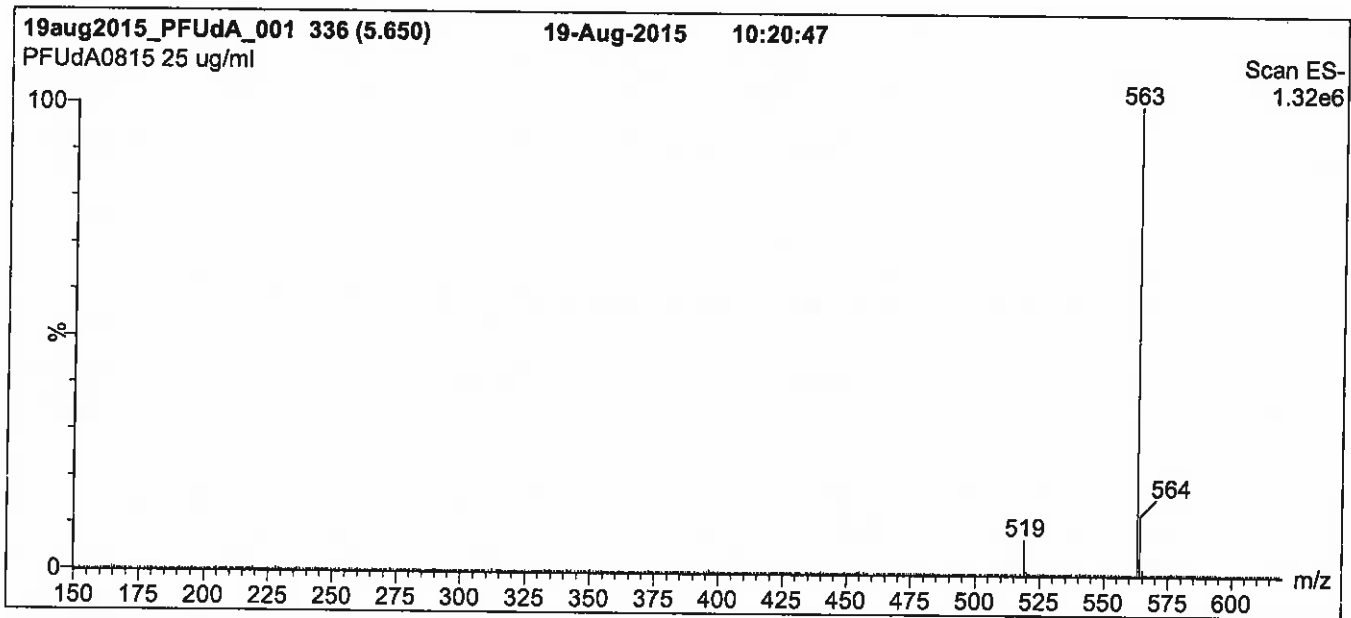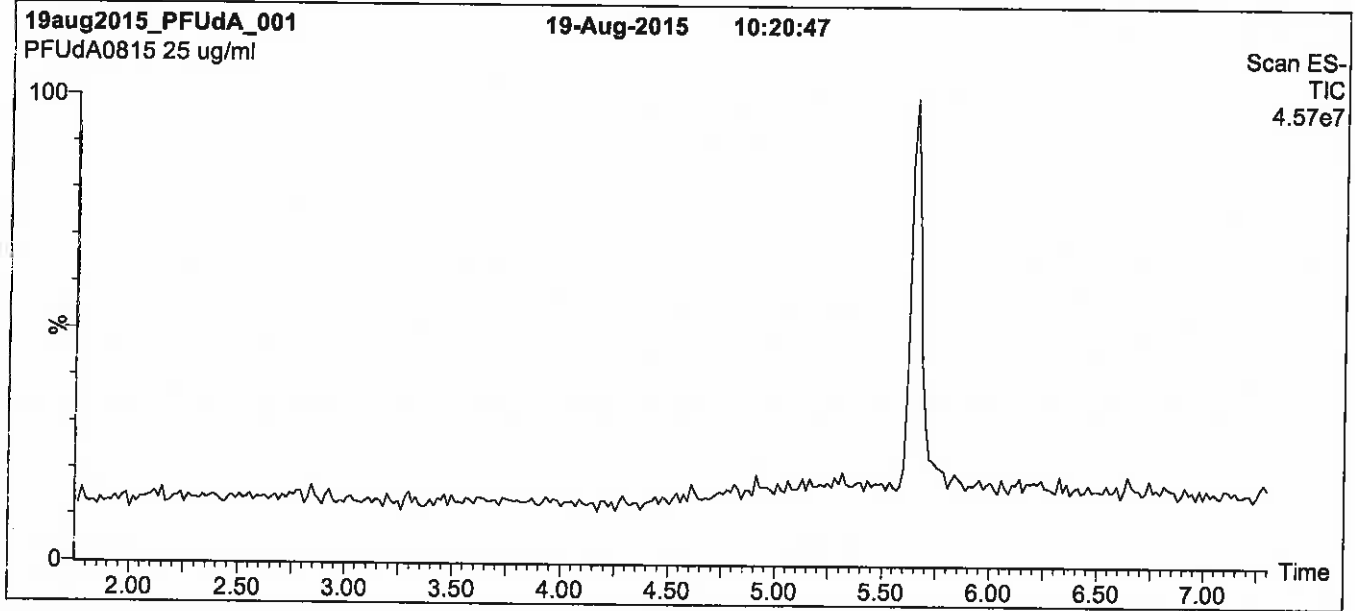

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro micro API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 2 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 65
Desolvation Gas Flow (l/hr) = 750

Figure 2: PFUdA; LC/MS/MS Data (Selected MRM Transitions)

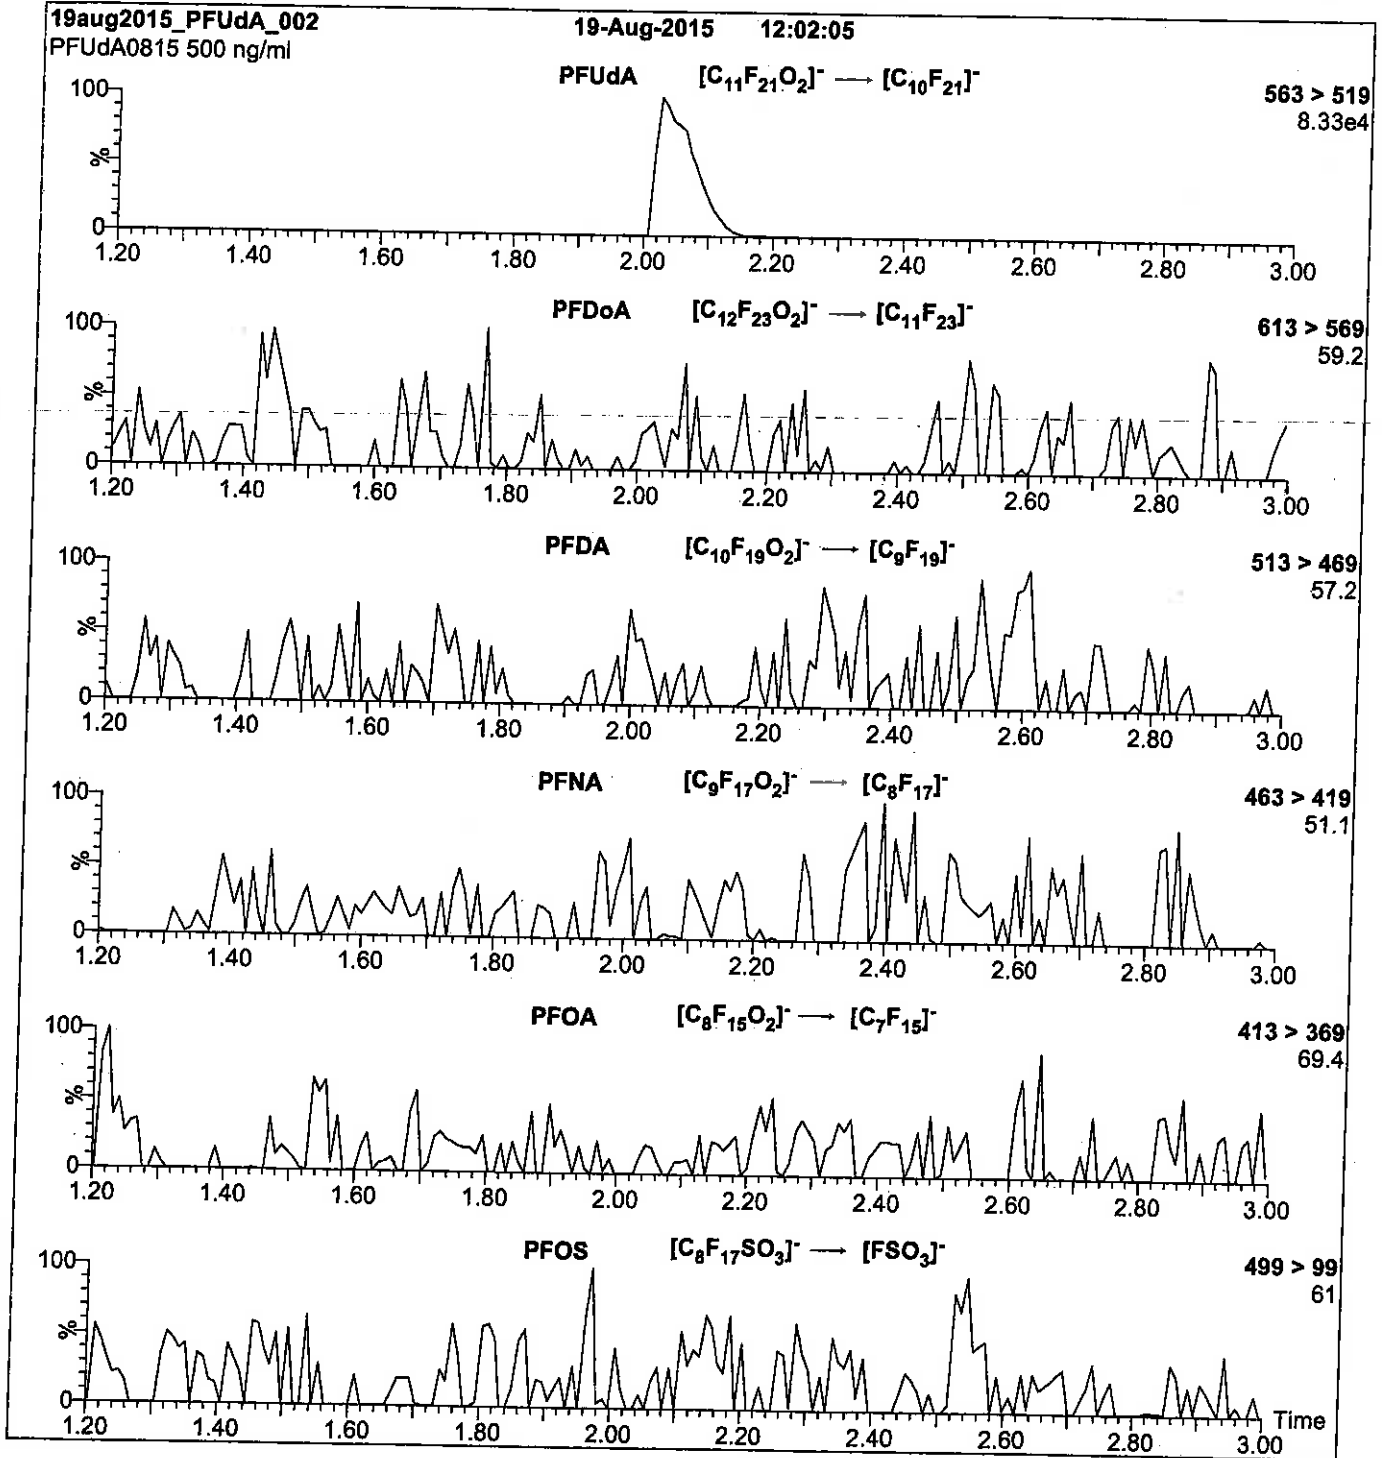

Conditions for Figure 2:

Injection: Direct loop injection
 10 μ l (500 ng/ml PFUdA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.31e-3
 Collision Energy (eV) = 11

Method PFC DOD

Perfluronated Hydrocarbons (LC/MS)
by Method PFC_DOD

FORM II
LCMS SURROGATE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1

SDG No.: _____

Matrix: Water Level: Low

GC Column (1): Acquity ID: 2.1 (mm)

Client Sample ID	Lab Sample ID	PFBA #	13CPeA #	PFHxA #	13CHpA #	PFHxS #	PFOA #	PFOS #	PFNA #
TB-1	320-24118-1	131	141	133	142	125	145	131	142
FB-1	320-24118-2	131	140	130	139	123	144	128	140
CS-10	320-24118-3	103	123	105	106	123	100	131	79
CS-41	320-24118-4	86	101	87	90	101	82	104	63
CS-12	320-24118-5	84	93	83	85	101	79	104	62
CS-1	320-24118-6	94	117	95	94	122	81	129	54
	MB 320-142235/1-A	118	126	118	127	111	128	115	125
	LCS 320-142235/2-A	105	107	103	110	100	110	101	111
CS-1 MS	320-24118-6 MS	93	117	102	107	123	101	125	82
CS-1 MSD	320-24118-6 MSD	95	115	101	105	118	97	125	76

QC LIMITS

PFBA = 13C4 PFBA	25-150
13CPeA = 13C5 PFPeA	25-150
PFHxA = 13C2 PFHxA	25-150
13CHpA = 13C4-PFHpA	25-150
PFHxS = 1802 PFHxS	25-150
PFOA = 13C4 PFOA	25-150
PFOS = 13C4 PFOS	25-150
PFNA = 13C5 PFNA	25-150

Column to be used to flag recovery values

FORM II 537 (Modified)

FORM II
LCMS SURROGATE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1

SDG No.: _____

Matrix: Water Level: Low

GC Column (1): Acquity ID: 2.1 (mm)

Client Sample ID	Lab Sample ID	13C8FOS #	PFDA #	PFUnA #	PFDoA #
TB-1	320-24118-1	14 Q	151 Q	153 Q	148
FB-1	320-24118-2	50	150	145	148
CS-10	320-24118-3	4 Q	73	77	99
CS-41	320-24118-4	3 Q	55	62	80
CS-12	320-24118-5	4 Q	59	64	80
CS-1	320-24118-6	5 Q	48	63	84
	MB 320-142235/1-A	39	136	135	129
	LCS 320-142235/2-A	13 Q	122	116	112
CS-1 MS	320-24118-6 MS	6 Q	82	92	110
CS-1 MSD	320-24118-6 MSD	4 Q	83	87	99

13C8FOS = 13C8 FOSA
PFDA = 13C2 PFDA
PFUnA = 13C2 PFUnA
PFDoA = 13C2 PFDoA

QC LIMITS
25-150
25-150
25-150
25-150

Column to be used to flag recovery values

FORM II 537 (Modified)

FORM III
LCMS LAB CONTROL SAMPLE RECOVERY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Matrix: Water Level: Low

Lab File ID: 15DEC2016B_030.d

Lab ID: LCS 320-142235/2-A

Client ID: _____

COMPOUND	SPIKE ADDED (ng/L)	LCS CONCENTRATION (ng/L)	LCS % REC	QC LIMITS REC	#
Perfluorobutanoic acid (PFBA)	40.0	41.3	103	60-140	
Perfluoropentanoic acid (PFPeA)	40.0	40.6	101	60-140	
Perfluorohexanoic acid (PFHxA)	40.0	38.6	97	60-140	
Perfluoroheptanoic acid (PFHpA)	40.0	37.8	95	60-140	
Perfluorooctanoic acid (PFOA)	40.0	39.8	99	60-140	
Perfluorononanoic acid (PFNA)	40.0	38.5	96	60-140	M
Perfluorodecanoic acid (PFDA)	40.0	37.7	94	60-140	
Perfluoroundecanoic acid (PFUnA)	40.0	38.1	95	60-140	
Perfluorododecanoic acid (PFDoA)	40.0	38.5	96	60-140	
Perfluorotridecanoic Acid (PFTriA)	40.0	41.4	103	50-150	
Perfluorotetradecanoic acid (PFTeA)	40.0	43.7	109	50-150	
Perfluorobutanesulfonic acid (PFBS)	35.4	39.8	113	50-150	
Perfluorohexanesulfonic acid (PFHxS)	36.4	34.7	95	60-140	
Perfluorooctanesulfonic acid (PFOS)	37.1	37.5	101	60-140	
Perfluorodecanesulfonic acid (PFDS)	38.6	38.2	99	50-150	
Perfluorooctane Sulfonamide (FOSA)	40.0	38.3	96	60-140	
13C8 FOSA	100	13.0	13	25-150	Q
13C4 PFBA	100	105	105	25-150	
13C2 PFHxA	100	103	103	25-150	
13C4 PFOA	100	110	110	25-150	
13C5 PFNA	100	111	111	25-150	
13C2 PFDA	100	122	122	25-150	
13C2 PFUnA	100	116	116	25-150	
13C2 PFDoA	100	112	112	25-150	
18O2 PFHxS	94.6	94.5	100	25-150	
13C4 PFOS	95.6	96.9	101	25-150	
13C4-PFHpA	100	110	110	25-150	
13C5 PFPeA	100	107	107	25-150	

Column to be used to flag recovery and RPD values

FORM III 537 (Modified)

FORM III
LCMS MATRIX SPIKE RECOVERY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Matrix: Water Level: Low

Lab File ID: 15DEC2016B_037.d

Lab ID: 320-24118-6 MS

Client ID: CS-1 MS

COMPOUND	SPIKE ADDED (ng/L)	SAMPLE CONCENTRATION (ng/L)	MS CONCENTRATION (ng/L)	MS % REC	QC LIMITS REC	#
Perfluorobutanoic acid (PFBA)	38.3	1.0 U	40.3	105	60-140	
Perfluoropentanoic acid (PFPeA)	38.3	2.0 U	38.5	100	60-140	
Perfluorohexanoic acid (PFHxA)	38.3	2.0 U	37.3	97	60-140	
Perfluoroheptanoic acid (PFHpA)	38.3	2.0 U	37.4	98	60-140	
Perfluorooctanoic acid (PFOA)	38.3	2.0 U	38.1	99	60-140	
Perfluorononanoic acid (PFNA)	38.3	2.0 U	37.4	98	60-140	
Perfluorodecanoic acid (PFDA)	38.3	1.0 U	36.8	96	60-140	
Perfluoroundecanoic acid (PFUnA)	38.3	2.0 U	37.7	98	60-140	
Perfluorododecanoic acid (PFDoA)	38.3	2.0 U	37.6	98	60-140	
Perfluorotridecanoic Acid (PFTriA)	38.3	2.0 U	52.7	138	50-150	
Perfluorotetradecanoic acid (PFTeA)	38.3	0.75 J	58.5	151	50-150	J
Perfluorobutanesulfonic acid (PFBS)	33.9	2.0 U	39.2	116	50-150	
Perfluorohexanesulfonic acid (PFHxS)	34.9	2.0 U	34.1	98	60-140	
Perfluorooctanesulfonic acid (PFOS)	35.6	3.0 U	37.8	106	60-140	
Perfluorodecanesulfonic acid (PFDS)	37.0	3.0 U	37.7	102	50-150	
Perfluorooctane Sulfonamide (FOSA)	38.3	2.0 U	37.6	98	60-140	
13C8 FOSA	95.9	5.3	5.40	6	25-150	Q
13C4 PFBA	95.9	93	89.2	93	25-150	
13C2 PFHxA	95.9	95	97.6	102	25-150	
13C4 PFOA	95.9	81	97.2	101	25-150	
13C5 PFNA	95.9	54	78.3	82	25-150	
13C2 PFDA	95.9	48	78.9	82	25-150	
13C2 PFUnA	95.9	63	88.1	92	25-150	
13C2 PFDoA	95.9	84	105	110	25-150	
18O2 PFHxS	90.7	120	111	123	25-150	
13C4 PFOS	91.6	120	115	125	25-150	
13C4-PFHpA	95.9	94	103	107	25-150	
13C5 PFPeA	95.9	120	113	117	25-150	

Column to be used to flag recovery and RPD values

FORM III 537 (Modified)

FORM III
LCMS MATRIX SPIKE DUPLICATE RECOVERY

Lab Name: TestAmerica Sacramento

Job No.: 320-24118-1

SDG No.: _____

Matrix: Water Level: Low

Lab File ID: 16DEC2016BB_003.d

Lab ID: 320-24118-6 MSD

Client ID: CS-1 MSD

COMPOUND	SPIKE ADDED (ng/L)	MSD CONCENTRATION (ng/L)	MSD % REC	% RPD	QC LIMITS		#
					RPD	REC	
Perfluorobutanoic acid (PFBA)	39.1	41.1	105	2	30	60-140	
Perfluoropentanoic acid (PFPeA)	39.1	39.3	101	2	30	60-140	
Perfluorohexanoic acid (PFHxA)	39.1	38.1	97	2	30	60-140	
Perfluoroheptanoic acid (PFHpA)	39.1	38.2	98	2	30	60-140	
Perfluorooctanoic acid (PFOA)	39.1	39.0	100	2	30	60-140	
Perfluorononanoic acid (PFNA)	39.1	37.6	96	1	30	60-140	
Perfluorodecanoic acid (PFDA)	39.1	36.4	93	1	30	60-140	
Perfluoroundecanoic acid (PFUnA)	39.1	38.3	98	2	30	60-140	
Perfluorododecanoic acid (PFDoA)	39.1	38.8	99	3	30	60-140	
Perfluorotridecanoic Acid (PFTriA)	39.1	51.3	131	3	30	50-150	
Perfluorotetradecanoic acid (PFTeA)	39.1	68.0	172	15	30	50-150	J
Perfluorobutanesulfonic acid (PFBS)	34.6	42.3	122	8	30	50-150	
Perfluorohexanesulfonic acid (PFHxS)	35.6	35.7	100	5	30	60-140	
Perfluorooctanesulfonic acid (PFOS)	36.3	37.1	102	2	30	60-140	
Perfluorodecanesulfonic acid (PFDS)	37.7	37.2	99	1	30	50-150	
Perfluorooctane Sulfonamide (FOSA)	39.1	36.9	94	2	30	60-140	
13C8 FOSA	97.8	4.21	4			25-150	Q
13C4 PFBA	97.8	92.8	95			25-150	
13C2 PFHxA	97.8	99.1	101			25-150	
13C4 PFOA	97.8	94.4	97			25-150	
13C5 PFNA	97.8	74.0	76			25-150	
13C2 PFDA	97.8	81.1	83			25-150	
13C2 PFUnA	97.8	85.2	87			25-150	
13C2 PFDoA	97.8	96.8	99			25-150	
18O2 PFHxS	92.5	109	118			25-150	
13C4 PFOS	93.5	117	125			25-150	
13C4-PFHpA	97.8	102	105			25-150	
13C5 PFPeA	97.8	113	115			25-150	

Column to be used to flag recovery and RPD values

FORM III 537 (Modified)

FORM IV
LCMS METHOD BLANK SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Lab File ID: 15DEC2016B_029.d Lab Sample ID: MB 320-142235/1-A
 Matrix: Water Date Extracted: 12/14/2016 18:18
 Instrument ID: A8_N Date Analyzed: 12/15/2016 16:24
 Level: (Low/Med) Low

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES:

CLIENT SAMPLE ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
	LCS 320-142235/2-A	15DEC2016B_030.d	12/15/2016 16:31
TB-1	320-24118-1	15DEC2016B_031.d	12/15/2016 16:39
FB-1	320-24118-2	15DEC2016B_032.d	12/15/2016 16:46
CS-10	320-24118-3	15DEC2016B_033.d	12/15/2016 16:54
CS-41	320-24118-4	15DEC2016B_034.d	12/15/2016 17:01
CS-12	320-24118-5	15DEC2016B_035.d	12/15/2016 17:09
CS-1	320-24118-6	15DEC2016B_036.d	12/15/2016 17:16
CS-1 MS	320-24118-6 MS	15DEC2016B_037.d	12/15/2016 17:24
CS-1 MSD	320-24118-6 MSD	16DEC2016BB_003.d	12/16/2016 15:37

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: TB-1 Lab Sample ID: 320-24118-1
 Matrix: Water Lab File ID: 15DEC2016B_031.d
 Analysis Method: 537 (Modified) Date Collected: 12/06/2016 08:00
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 243.6(mL) Date Analyzed: 12/15/2016 16:39
 Con. Extract Vol.: 0.5(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: Acquity ID: 2.1(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142379 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
375-22-4	Perfluorobutanoic acid (PFBA)	1.0	U	2.6	1.0	0.47
2706-90-3	Perfluoropentanoic acid (PFPeA)	2.1	U	2.6	2.1	1.0
307-24-4	Perfluorohexanoic acid (PFHxA)	2.1	U M	2.6	2.1	0.81
375-85-9	Perfluoroheptanoic acid (PFHpA)	2.1	U	2.6	2.1	0.82
335-67-1	Perfluorooctanoic acid (PFOA)	2.1	U	2.6	2.1	0.77
375-95-1	Perfluorononanoic acid (PFNA)	2.1	U	2.6	2.1	0.67
335-76-2	Perfluorodecanoic acid (PFDA)	1.0	U	2.6	1.0	0.45
2058-94-8	Perfluoroundecanoic acid (PFUnA)	2.1	U	2.6	2.1	0.77
307-55-1	Perfluorododecanoic acid (PFDoA)	2.1	U	2.6	2.1	0.60
72629-94-8	Perfluorotridecanoic Acid (PFTriA)	2.1	U	2.6	2.1	0.57
376-06-7	Perfluorotetradecanoic acid (PFTeA)	0.54	J	2.6	1.0	0.41
375-73-5	Perfluorobutanesulfonic acid (PFBS)	2.1	U	2.6	2.1	0.94
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	2.1	U	2.6	2.1	0.89
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	3.1	U	4.1	3.1	1.3
335-77-3	Perfluorodecanesulfonic acid (PFDS)	3.1	U	4.1	3.1	1.2
754-91-6	Perfluorooctane Sulfonamide (FOSA)	2.1	U	2.6	2.1	0.65

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: TB-1 Lab Sample ID: 320-24118-1
 Matrix: Water Lab File ID: 15DEC2016B_031.d
 Analysis Method: 537 (Modified) Date Collected: 12/06/2016 08:00
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 243.6(mL) Date Analyzed: 12/15/2016 16:39
 Con. Extract Vol.: 0.5(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: Acquity ID: 2.1(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142379 Units: ng/L

CAS NO.	ISOTOPE DILUTION	%REC	Q	LIMITS
STL01056	13C8 FOSA	14	Q	25-150
STL00992	13C4 PFBA	131		25-150
STL00993	13C2 PFHxA	133		25-150
STL00990	13C4 PFOA	145		25-150
STL00995	13C5 PFNA	142		25-150
STL00996	13C2 PFDA	151	Q	25-150
STL00997	13C2 PFUnA	153	Q	25-150
STL00998	13C2 PFDoA	148		25-150
STL00994	18O2 PFHxS	125		25-150
STL00991	13C4 PFOS	131		25-150
STL01892	13C4-PFHpA	142		25-150
STL01893	13C5 PFPeA	141		25-150

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_031.d
 Lims ID: 320-24118-B-1-A
 Client ID: TB-1
 Sample Type: Client
 Inject. Date: 15-Dec-2016 16:39:19 ALS Bottle#: 39 Worklist Smp#: 31
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-24118-b-1-a
 Misc. Info.: Plate: 1 Rack: 5
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 15:30:05 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 16-Dec-2016 09:39:10

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.633	1.534	0.099	22760704	65.5		131	1010785	
1 Perfluorobutyric acid	212.90 > 169.00	1.657	1.535	0.122	18956	0.0488			70.7	
D 4 13C5-PFPeA	267.90 > 223.00	1.929	1.810	0.119	18754315	70.5		141	1099281	
3 Perfluoropentanoic acid	262.90 > 219.00	1.929	1.810	0.119	32303	0.0873			198	
7 Perfluorohexanoic acid	313.00 > 269.00	2.231	2.096	0.135	14456	0.0477			334	M
D 6 13C2 PFHxA	315.00 > 270.00	2.231	2.097	0.134	16305127	66.5		133	963632	
D 11 13C4-PFHpA	367.00 > 322.00	2.581	2.426	0.155	16034252	70.8		142	989004	
D 10 18O2 PFHxS	403.00 > 84.00	2.597	2.446	0.151	19316139	59.1		125	1497884	
D 14 13C4 PFOA	417.00 > 372.00	2.944	2.783	0.161	16722003	72.6		145	698271	
D 17 13C4 PFOS	503.00 > 80.00	3.322	3.151	0.171	15592987	62.7		131	621558	
D 19 13C5 PFNA	468.00 > 423.00	3.322	3.153	0.169	12635403	71.1		142	472049	
D 21 13C8 FOSA	506.00 > 78.00	3.654	3.488	0.166	2734226	7.12		14.2	173902	
24 Perfluorodecanoic acid	513.00 > 469.00	3.683	3.510	0.173	7056	0.0314			199	
D 23 13C2 PFDA	515.00 > 470.00	3.683	3.513	0.170	11896586	75.6		151	249194	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
26 Perfluorodecane Sulfonic acid	599.00 > 80.00	3.983	3.822	0.161	1.000	4055	0.0213			
28 Perfluoroundecanoic acid	563.00 > 519.00	3.992	3.839	0.153	1.000	25427	0.1480		618	
D 27 13C2 PFUnA	565.00 > 520.00	4.002	3.842	0.160		8985559	76.6	153	573758	
D 30 13C2 PFDaA	615.00 > 570.00	4.295	4.132	0.163		8183606	73.8	148	268083	
29 Perfluorododecanoic acid	613.00 > 569.00	4.295	4.136	0.159	1.000	9837	0.0655		21.9	
31 Perfluorotridecanoic acid	663.00 > 619.00	4.562	4.400	0.162	1.000	13465	0.0907		14.2	
33 Perfluorotetradecanoic acid	712.50 > 668.90	4.796	4.642	0.154	1.000	68663	0.2647		29.7	
	713.00 > 169.00	4.796	4.642	0.154	1.000	10936	6.28(0.00-0.00)		1201	

QC Flag Legend

Review Flags

M - Manually Integrated




TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_031.d
Injection Date: 15-Dec-2016 16:39:19 Instrument ID: A8_N
Lims ID: 320-24118-B-1-A Lab Sample ID: 320-24118-1
Client ID: TB-1
Operator ID: A8-PC\A8 ALS Bottle#: 39 Worklist Smp#: 31
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL

D 2 13C4 PFBA

1 Perfluorobutyric acid




D 4 13C5-PFPeA



3 Perfluoropentanoic acid

5 Perfluorobutanesulfonic acid (ND)




5 Perfluorobutanesulfonic acid (ND)



7 Perfluorohexanoic acid (M)

D 6 13C2 PFHxA




D 11 13C4-PFHpA

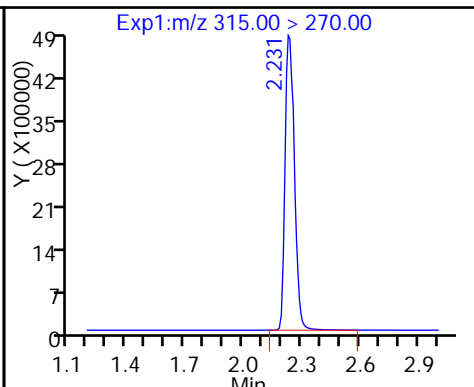


12 Perfluoroheptanoic acid (ND)

9 Perfluorohexanesulfonic acid (ND)


D 10 18O2 PFHxS

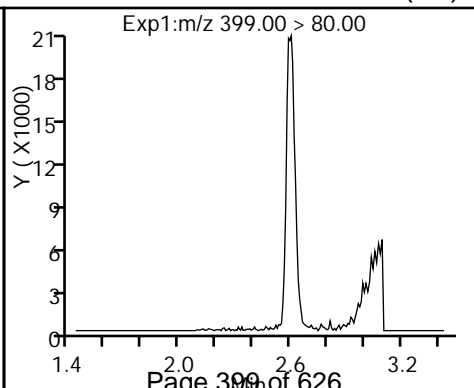


D 14 13C4 PFOA




15 Perfluorooctanoic acid (ND)

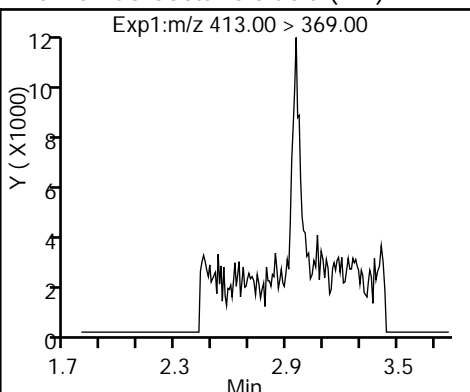


15 Perfluorooctanoic acid (ND)




18 Perfluorooctane sulfonic acid (ND)




18 Perfluorooctane sulfonic acid (ND)




D 17 13C4 PFOS




D 19 13C5 PFNA




20 Perfluorononanoic acid (ND)




D 21 13C8 FOSA




22 Perfluorooctane Sulfonamide (ND)




24 Perfluorodecanoic acid




D 23 13C2 PFDA




26 Perfluorodecane Sulfonic acid




28 Perfluoroundecanoic acid

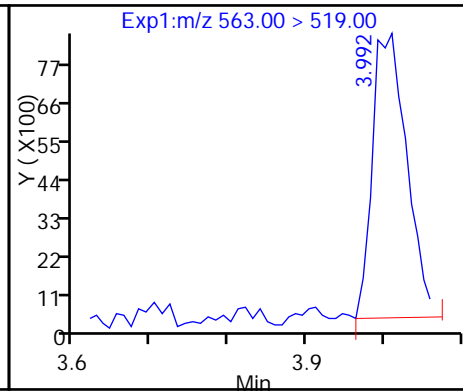


D 27 13C2 PFUnA

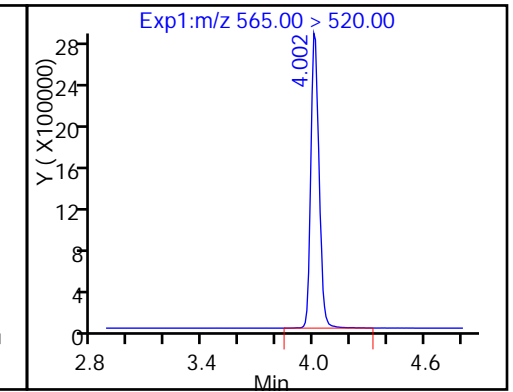


D 30 13C2 PFDaA




29 Perfluorododecanoic acid




31 Perfluorotridecanoic acid

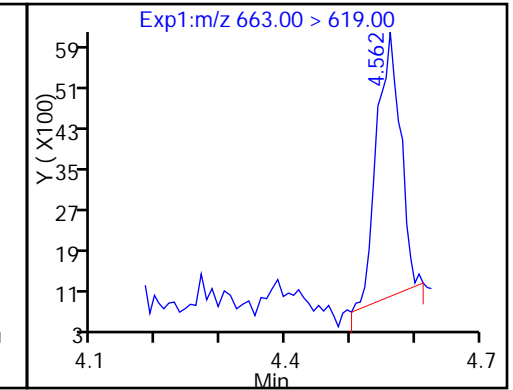

33 Perfluorotetradecanoic acid



33 Perfluorotetradecanoic acid



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_031.d
Injection Date: 15-Dec-2016 16:39:19 Instrument ID: A8_N
Lims ID: 320-24118-B-1-A Lab Sample ID: 320-24118-1
Client ID: TB-1
Operator ID: A8-PC\A8 ALS Bottle#: 39 Worklist Smp#: 31
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL
Column: Detector EXP1

7 Perfluorohexanoic acid, CAS: 307-24-4

Signal: 1


RT: 2.23
Area: 1848
Amount: 0.006101
Amount Units: ng/ml

Processing Integration Results

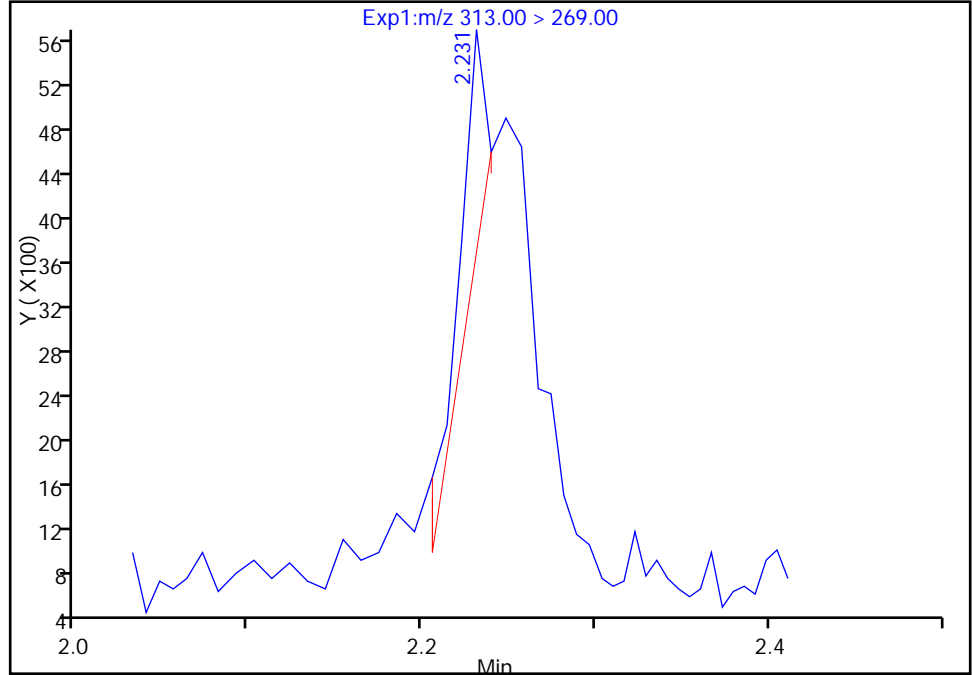

RT: 2.23
Area: 14456
Amount: 0.047729
Amount Units: ng/ml

Manual Integration Results

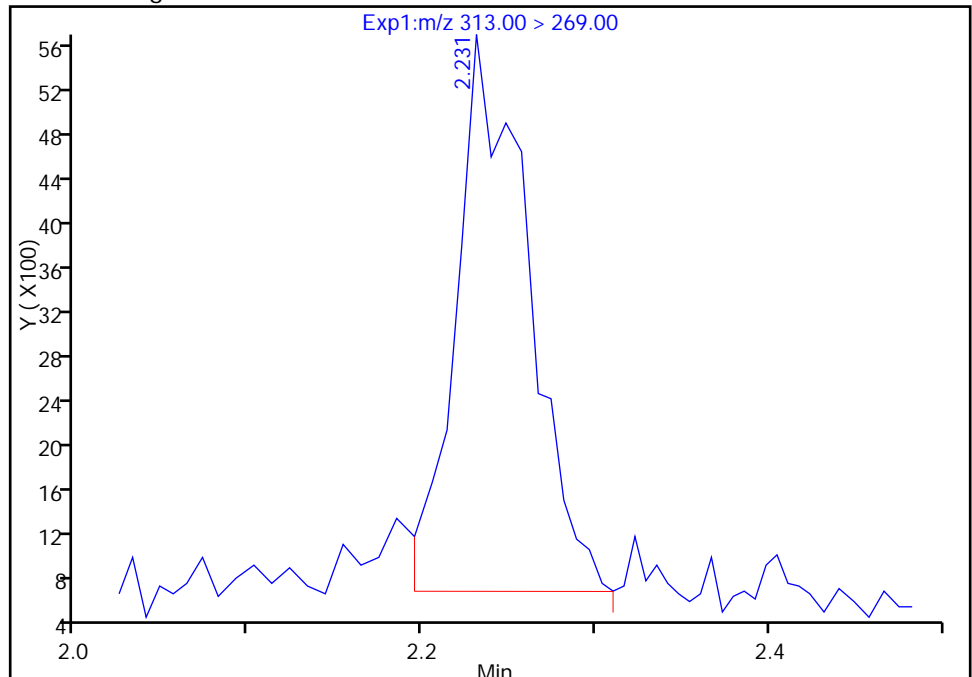

Reviewer: chandrasenas, 16-Dec-2016 09:39:10

Audit Action: Manually Integrated

Audit Reason: Incomplete Integration

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: FB-1 Lab Sample ID: 320-24118-2
 Matrix: Water Lab File ID: 15DEC2016B_032.d
 Analysis Method: 537 (Modified) Date Collected: 12/06/2016 09:22
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 261.5 (mL) Date Analyzed: 12/15/2016 16:46
 Con. Extract Vol.: 0.5 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: Acquity ID: 2.1 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142379 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
375-22-4	Perfluorobutanoic acid (PFBA)	0.96	U	2.4	0.96	0.44
2706-90-3	Perfluoropentanoic acid (PFPeA)	1.9	U	2.4	1.9	0.95
307-24-4	Perfluorohexanoic acid (PFHxA)	1.9	U	2.4	1.9	0.75
375-85-9	Perfluoroheptanoic acid (PFHpA)	1.9	U	2.4	1.9	0.77
335-67-1	Perfluorooctanoic acid (PFOA)	1.9	U	2.4	1.9	0.72
375-95-1	Perfluorononanoic acid (PFNA)	1.9	U	2.4	1.9	0.63
335-76-2	Perfluorodecanoic acid (PFDA)	0.96	U	2.4	0.96	0.42
2058-94-8	Perfluoroundecanoic acid (PFUnA)	1.9	U	2.4	1.9	0.72
307-55-1	Perfluorododecanoic acid (PFDoA)	1.9	U	2.4	1.9	0.56
72629-94-8	Perfluorotridecanoic Acid (PFTriA)	1.9	U	2.4	1.9	0.53
376-06-7	Perfluorotetradecanoic acid (PFTeA)	0.96	U	2.4	0.96	0.38
375-73-5	Perfluorobutanesulfonic acid (PFBS)	1.9	U	2.4	1.9	0.88
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	1.9	U M	2.4	1.9	0.83
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	2.9	U	3.8	2.9	1.2
335-77-3	Perfluorodecanesulfonic acid (PFDS)	2.9	U	3.8	2.9	1.2
754-91-6	Perfluorooctane Sulfonamide (FOSA)	1.9	U	2.4	1.9	0.61

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: FB-1 Lab Sample ID: 320-24118-2
 Matrix: Water Lab File ID: 15DEC2016B_032.d
 Analysis Method: 537 (Modified) Date Collected: 12/06/2016 09:22
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 261.5 (mL) Date Analyzed: 12/15/2016 16:46
 Con. Extract Vol.: 0.5 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: Acquity ID: 2.1 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142379 Units: ng/L

CAS NO.	ISOTOPE DILUTION	%REC	Q	LIMITS
STL01056	13C8 FOSA	50		25-150
STL00992	13C4 PFBA	131		25-150
STL00993	13C2 PFHxA	130		25-150
STL00990	13C4 PFOA	144		25-150
STL00995	13C5 PFNA	140		25-150
STL00996	13C2 PFDA	150		25-150
STL00997	13C2 PFUnA	145		25-150
STL00998	13C2 PFDoA	148		25-150
STL00994	18O2 PFHxS	123		25-150
STL00991	13C4 PFOS	128		25-150
STL01892	13C4-PFHpA	139		25-150
STL01893	13C5 PFPeA	140		25-150

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_032.d
 Lims ID: 320-24118-B-2-A
 Client ID: FB-1
 Sample Type: Client
 Inject. Date: 15-Dec-2016 16:46:49 ALS Bottle#: 40 Worklist Smp#: 32
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-24118-b-2-a
 Misc. Info.: Plate: 1 Rack: 5
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 15:30:05 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 16-Dec-2016 09:39:22

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.633	1.534	0.099	22693956	65.3		131	2003910	
1 Perfluorobutyric acid	212.90 > 169.00	1.649	1.535	0.114	23758	0.0613			83.6	
D 4 13C5-PFPeA	267.90 > 223.00	1.929	1.810	0.119	18595104	69.9		140	917941	
3 Perfluoropentanoic acid	262.90 > 219.00	1.919	1.810	0.109	35926	0.0979			264	
7 Perfluorohexanoic acid	313.00 > 269.00	2.232	2.096	0.136	14442	0.0487			283	
D 6 13C2 PFHxA	315.00 > 270.00	2.232	2.097	0.135	15953461	65.1		130	1189700	
D 11 13C4-PFHpA	367.00 > 322.00	2.574	2.426	0.148	15693666	69.3		139	1573462	
9 Perfluorohexanesulfonic acid	399.00 > 80.00	2.605	2.431	0.174	65260	0.1580				M M
D 10 18O2 PFHxS	403.00 > 84.00	2.605	2.446	0.159	18967046	58.0		123	1449159	
D 14 13C4 PFOA	417.00 > 372.00	2.953	2.783	0.170	16552299	71.9		144	723708	
D 17 13C4 PFOS	503.00 > 80.00	3.315	3.151	0.164	15248636	61.3		128	921921	
D 19 13C5 PFNA	468.00 > 423.00	3.330	3.153	0.177	12457387	70.1		140	503189	
D 21 13C8 FOSA	506.00 > 78.00	3.655	3.488	0.167	9600883	25.0		50.0	432660	
22 Perfluorooctane Sulfonamide	498.00 > 78.00	3.655	3.491	0.164	10054	0.0561			1034	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
24 Perfluorodecanoic acid	513.00 > 469.00	3.511	3.510	0.001	1.000	710	0.003199		22.1	
D 23 13C2 PFDA	515.00 > 470.00	3.674	3.513	0.161		11758668	74.8	150	248374	
26 Perfluorodecane Sulfonic acid	599.00 > 80.00	3.878	3.822	0.056	1.000	411	0.002206			
28 Perfluoroundecanoic acid	563.00 > 519.00	4.012	3.839	0.173	1.000	19799	0.1216		470	
D 27 13C2 PFDUnA	565.00 > 520.00	4.002	3.842	0.160		8516673	72.6	145	444368	
D 30 13C2 PFDaA	615.00 > 570.00	4.287	4.132	0.155		8204145	73.9	148	194643	
33 Perfluorotetradecanoic acid	712.50 > 668.90	4.799	4.642	0.157	1.000	47769	0.1837		26.4	
	713.00 > 169.00	4.783	4.642	0.141	0.997	5679		8.41(0.00-0.00)	578	

QC Flag Legend

Review Flags

M - Manually Integrated

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_032.d

Injection Date: 15-Dec-2016 16:46:49

Instrument ID: A8_N

Lims ID: 320-24118-B-2-A

Lab Sample ID: 320-24118-2

Client ID: FB-1

Operator ID: A8-PC\A8

ALS Bottle#: 40

Worklist Smp#: 32

Injection Vol: 2.0 ul

Dil. Factor: 1.0000













Method: A8_N

Limit Group: LC PFC_DOD ICAL


D 2 13C4 PFBA

1 Perfluorobutyric acid


D 4 13C5-PFPeA

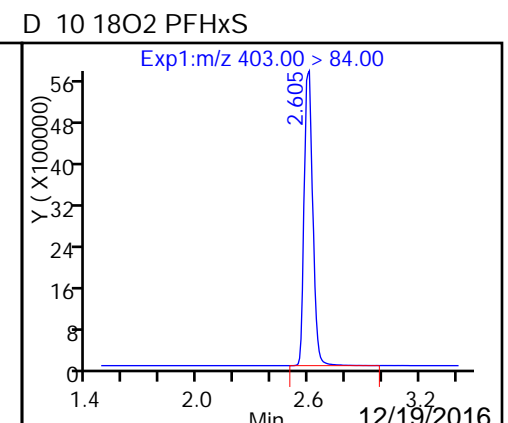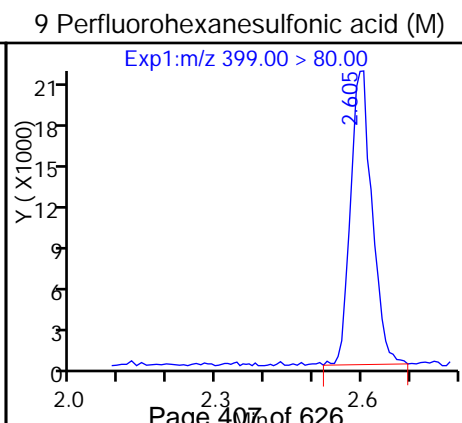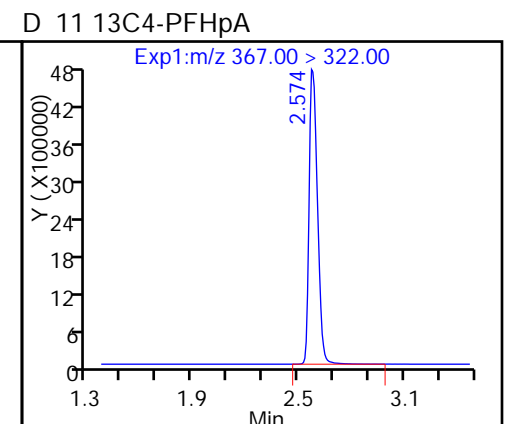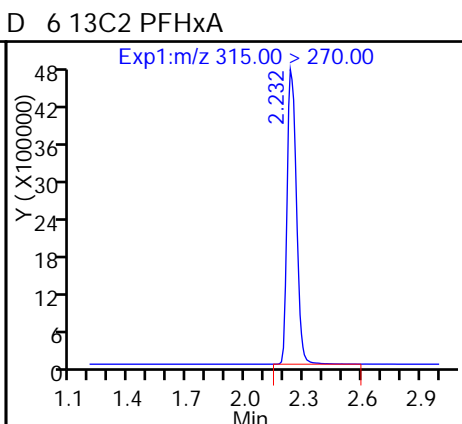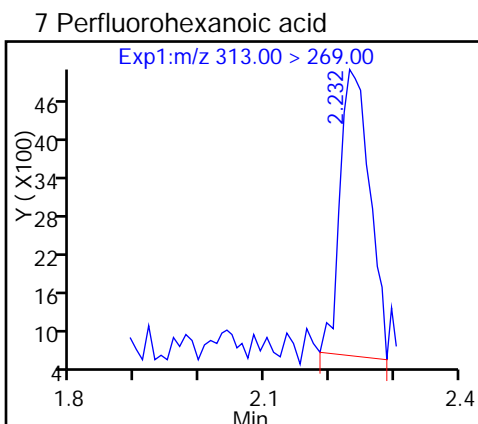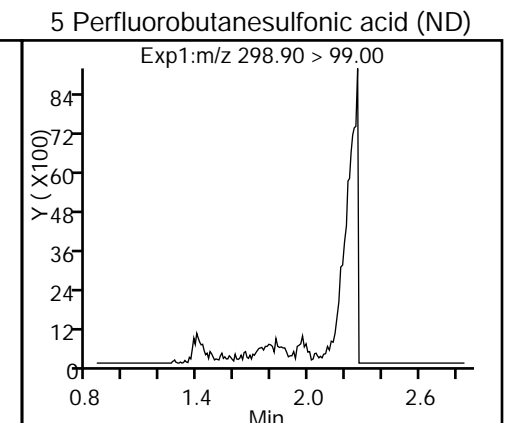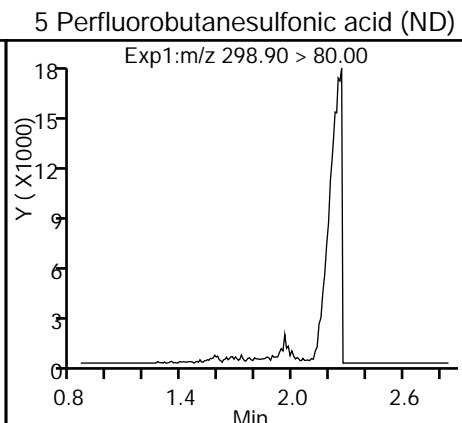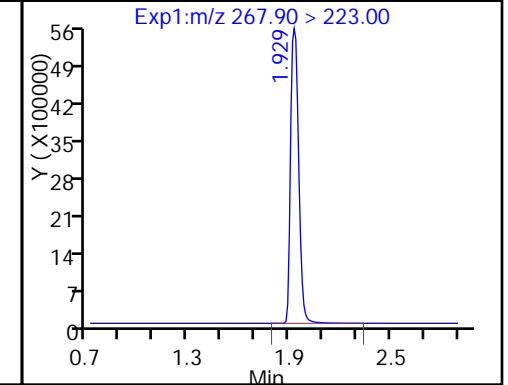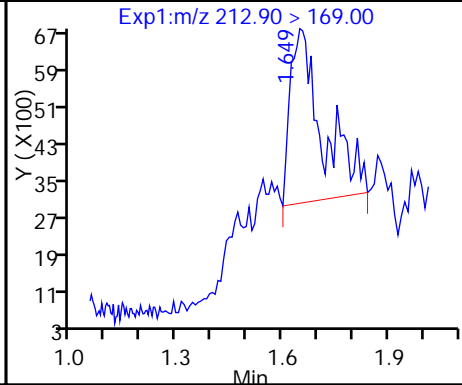


D 14 13C4 PFOA




15 Perfluorooctanoic acid (ND)




15 Perfluorooctanoic acid (ND)

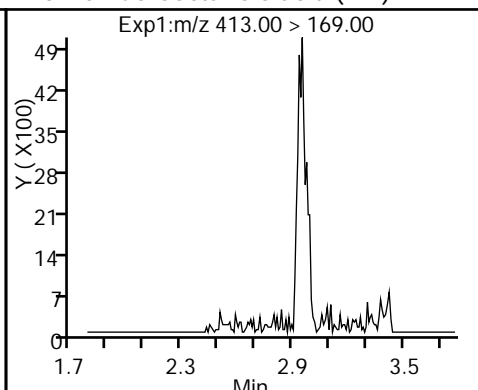


18 Perfluorooctane sulfonic acid (ND)




18 Perfluorooctane sulfonic acid (ND)




D 17 13C4 PFOS

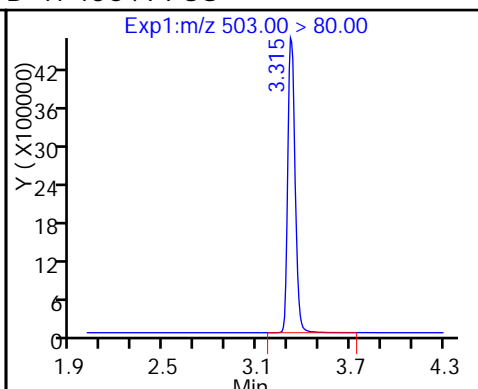


D 19 13C5 PFNA




20 Perfluorononanoic acid (ND)




D 21 13C8 FOSA

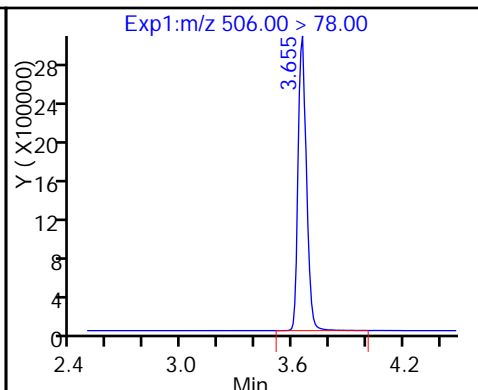


22 Perfluorooctane Sulfonamide




24 Perfluorodecanoic acid




D 23 13C2 PFDA

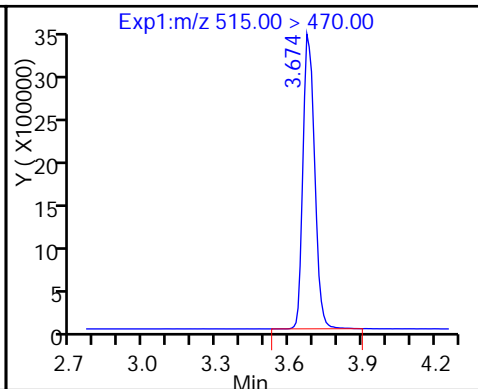


26 Perfluorodecane Sulfonic acid




28 Perfluoroundecanoic acid




D 27 13C2 PFUnA

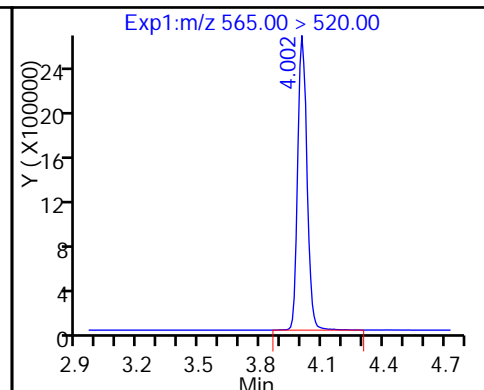


D 30 13C2 PFDaA




29 Perfluorododecanoic acid (ND)

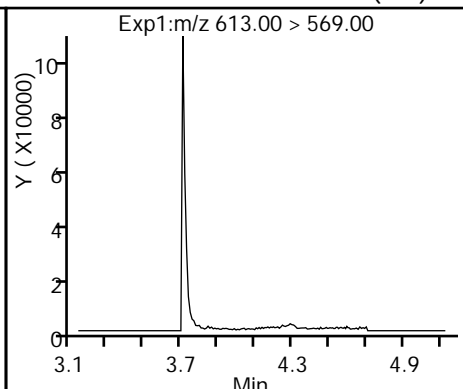


31 Perfluorotridecanoic acid (ND)

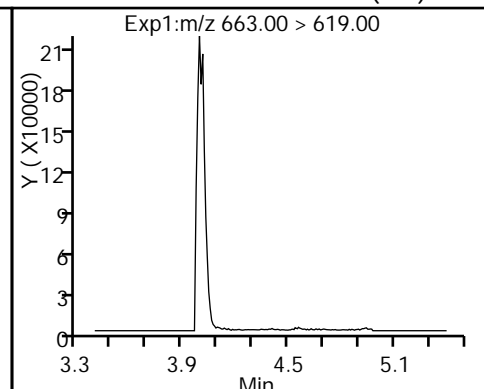

33 Perfluorotetradecanoic acid



33 Perfluorotetradecanoic acid



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_032.d
Injection Date: 15-Dec-2016 16:46:49 Instrument ID: A8_N
Lims ID: 320-24118-B-2-A Lab Sample ID: 320-24118-2
Client ID: FB-1
Operator ID: A8-PC\A8 ALS Bottle#: 40 Worklist Smp#: 32
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL
Column: Detector EXP1

9 Perfluorohexanesulfonic acid, CAS: 355-46-4

Signal: 1


Not Detected
Expected RT: 2.43

Processing Integration Results

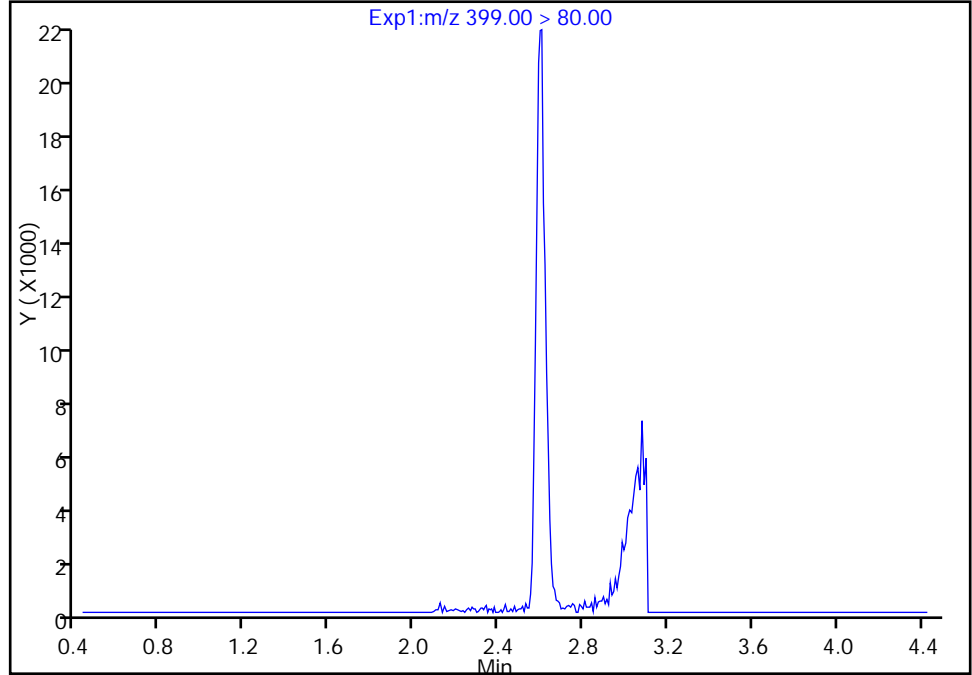

Manual Integration Results

RT: 2.60
Area: 65260
Amount: 0.158010
Amount Units: ng/ml

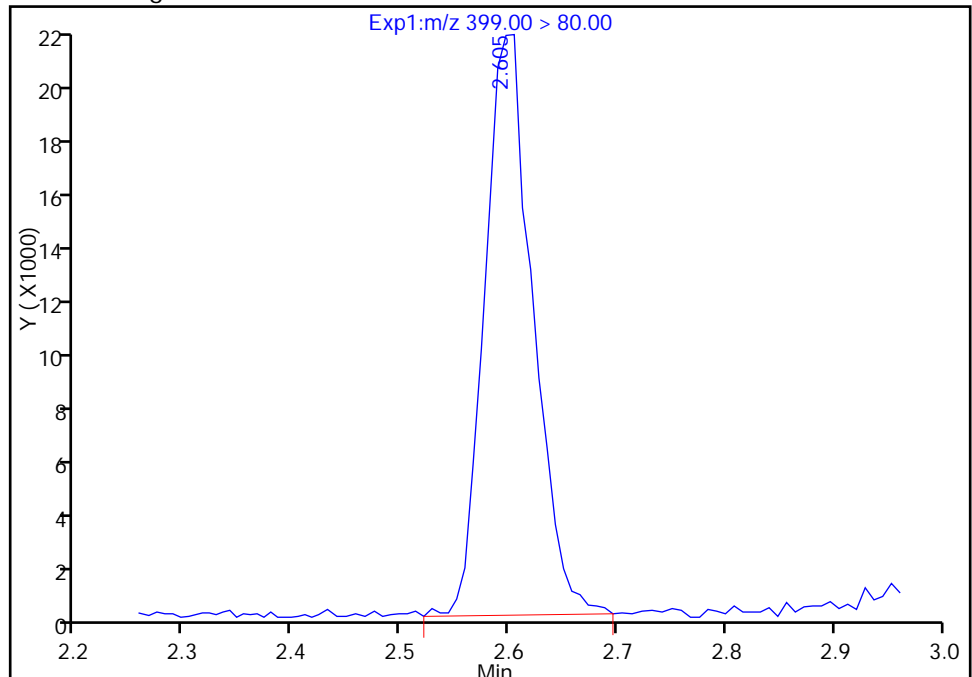

Reviewer: chandrasenas, 16-Dec-2016 09:39:22

Audit Action: Assigned Compound ID

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_032.d
Injection Date: 15-Dec-2016 16:46:49 Instrument ID: A8_N
Lims ID: 320-24118-B-2-A Lab Sample ID: 320-24118-2
Client ID: FB-1
Operator ID: A8-PC\A8 ALS Bottle#: 40 Worklist Smp#: 32
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL
Column: Detector EXP1

9 Perfluorohexanesulfonic acid, CAS: 355-46-4

Signal: 1


Not Detected
Expected RT: 2.43

Processing Integration Results

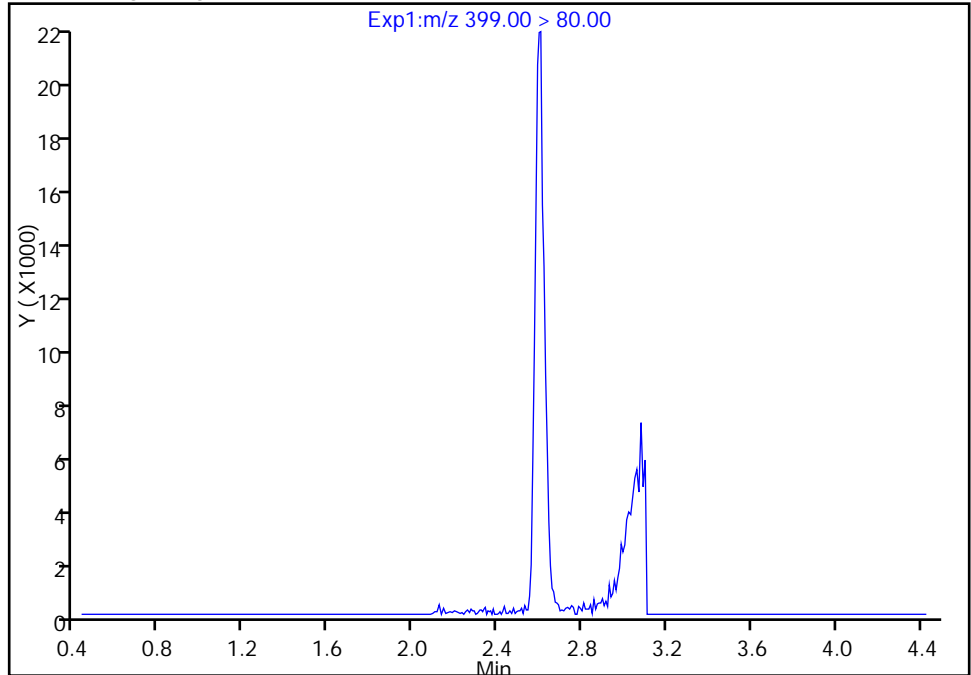

Manual Integration Results

RT: 2.60
Area: 65260
Amount: 0.158010
Amount Units: ng/ml

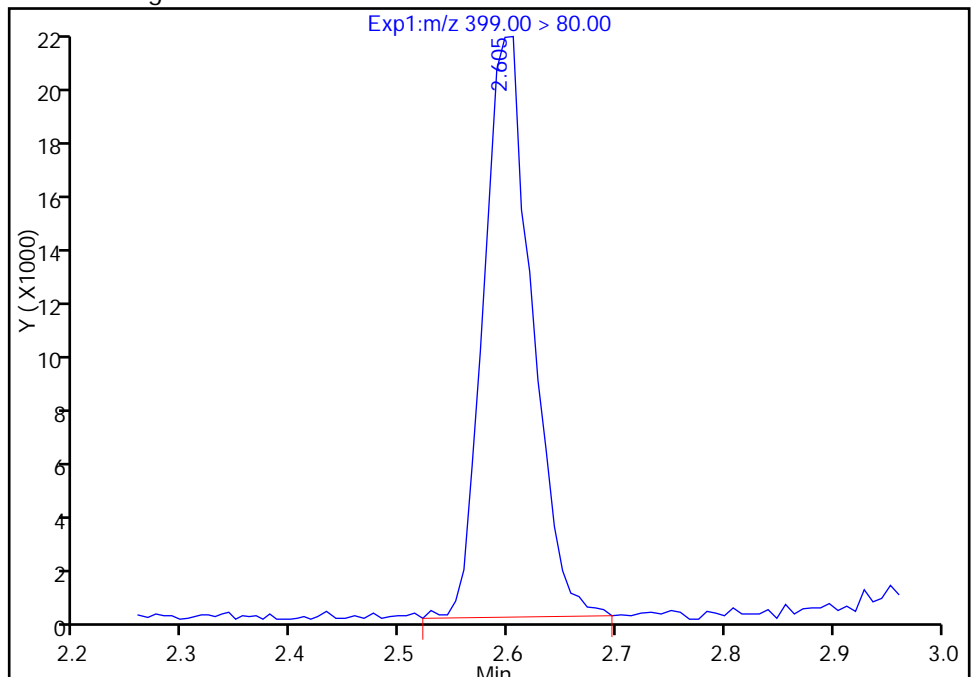

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: CS-10 Lab Sample ID: 320-24118-3
 Matrix: Water Lab File ID: 15DEC2016B_033.d
 Analysis Method: 537 (Modified) Date Collected: 12/06/2016 10:40
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 259.7 (mL) Date Analyzed: 12/15/2016 16:54
 Con. Extract Vol.: 0.5 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: Acquity ID: 2.1 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142379 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
375-22-4	Perfluorobutanoic acid (PFBA)	0.51	J	2.4	0.96	0.44
2706-90-3	Perfluoropentanoic acid (PFPeA)	1.9	U	2.4	1.9	0.95
307-24-4	Perfluorohexanoic acid (PFHxA)	1.1	J	2.4	1.9	0.76
375-85-9	Perfluoroheptanoic acid (PFHpA)	1.9	U M	2.4	1.9	0.77
335-67-1	Perfluorooctanoic acid (PFOA)	0.72	J	2.4	1.9	0.72
375-95-1	Perfluorononanoic acid (PFNA)	1.9	U	2.4	1.9	0.63
335-76-2	Perfluorodecanoic acid (PFDA)	0.96	U	2.4	0.96	0.42
2058-94-8	Perfluoroundecanoic acid (PFUnA)	1.9	U	2.4	1.9	0.72
307-55-1	Perfluorododecanoic acid (PFDoA)	1.9	U	2.4	1.9	0.56
72629-94-8	Perfluorotridecanoic Acid (PFTriA)	1.9	U	2.4	1.9	0.53
376-06-7	Perfluorotetradecanoic acid (PFTeA)	0.53	J	2.4	0.96	0.39
375-73-5	Perfluorobutanesulfonic acid (PFBS)	1.3	J M	2.4	1.9	0.88
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	10		2.4	1.9	0.84
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	17		3.9	2.9	1.2
335-77-3	Perfluorodecanesulfonic acid (PFDS)	2.9	U	3.9	2.9	1.2
754-91-6	Perfluorooctane Sulfonamide (FOSA)	1.9	U	2.4	1.9	0.61

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: CS-10 Lab Sample ID: 320-24118-3
 Matrix: Water Lab File ID: 15DEC2016B_033.d
 Analysis Method: 537 (Modified) Date Collected: 12/06/2016 10:40
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 259.7 (mL) Date Analyzed: 12/15/2016 16:54
 Con. Extract Vol.: 0.5 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: Acquity ID: 2.1 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142379 Units: ng/L

CAS NO.	ISOTOPE DILUTION	%REC	Q	LIMITS
STL01056	13C8 FOSA	4	Q	25-150
STL00992	13C4 PFBA	103		25-150
STL00993	13C2 PFHxA	105		25-150
STL00990	13C4 PFOA	100		25-150
STL00995	13C5 PFNA	79		25-150
STL00996	13C2 PFDA	73		25-150
STL00997	13C2 PFUnA	77		25-150
STL00998	13C2 PFDoA	99		25-150
STL00994	18O2 PFHxS	123		25-150
STL00991	13C4 PFOS	131		25-150
STL01892	13C4-PFHpA	106		25-150
STL01893	13C5 PFPeA	123		25-150

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_033.d
 Lims ID: 320-24118-B-3-A
 Client ID: CS-10
 Sample Type: Client
 Inject. Date: 15-Dec-2016 16:54:18 ALS Bottle#: 41 Worklist Smp#: 33
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-24118-b-3-a
 Misc. Info.: Plate: 1 Rack: 5
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 15:30:05 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 16-Dec-2016 09:41:46

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.638	1.534	0.104	17864399	51.4		103	984049	
1 Perfluorobutyric acid	212.90 > 169.00	1.638	1.535	0.103	81219	0.2663			491	
D 4 13C5-PFPeA	267.90 > 223.00	1.926	1.810	0.116	16332410	61.4		123	1661444	
3 Perfluoropentanoic acid	262.90 > 219.00	1.935	1.810	0.125	144002	0.4467			1310	
5 Perfluorobutanesulfonic acid	298.90 > 80.00	1.974	1.848	0.126	396869	0.6949				M
	298.90 > 99.00	1.964	1.848	0.116	169649		2.34(0.00-0.00)			M
7 Perfluorohexanoic acid	313.00 > 269.00	2.244	2.096	0.148	139304	0.5808			2287	
D 6 13C2 PFHxA	315.00 > 270.00	2.244	2.097	0.147	12911228	52.7		105	994970	
D 11 13C4-PFHpA	367.00 > 322.00	2.582	2.426	0.156	12045564	53.2		106	738145	
12 Perfluoroheptanoic acid	363.00 > 319.00	2.582	2.428	0.154	43181	0.1831			452	M
9 Perfluorohexanesulfonic acid	399.00 > 80.00	2.521	2.431	0.090	2152825	5.19				
D 10 18O2 PFHxS	403.00 > 84.00	2.597	2.446	0.151	19065546	58.3		123	1888669	
D 14 13C4 PFOA	417.00 > 372.00	2.953	2.783	0.170	11568140	50.2		100	1825236	
15 Perfluorooctanoic acid	413.00 > 369.00	2.953	2.783	0.170	87062	0.3751			643	
	413.00 > 169.00	2.945	2.783	0.162	58649		1.48(0.90-1.10)		2850	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
18 Perfluorooctane sulfonic acid										
499.00 > 80.00	3.201	3.118	0.083	1.000	2808487	8.65			121270	
499.00 > 99.00	3.331	3.118	0.213	1.040	611858		4.59(0.90-1.10)		29432	
D 17 13C4 PFOS										
503.00 > 80.00	3.315	3.151	0.164		15608933	62.7		131	482124	
D 19 13C5 PFNA										
468.00 > 423.00	3.323	3.153	0.170		7014961	39.5		79.0	313661	
D 21 13C8 FOSA										
506.00 > 78.00	3.655	3.488	0.167		784225	2.04		4.1	47902	
24 Perfluorodecanoic acid										
513.00 > 469.00	3.519	3.510	0.009	1.000	649	0.005959			52.7	
D 23 13C2 PFDA										
515.00 > 470.00	3.683	3.513	0.170		5770284	36.7		73.4	132158	
26 Perfluorodecane Sulfonic acid										
599.00 > 80.00	3.783	3.822	-0.039	1.000	848	0.004447				
28 Perfluoroundecanoic acid										
563.00 > 519.00	3.993	3.839	0.154	1.000	10625	0.1234			228	
D 27 13C2 PFUnA										
565.00 > 520.00	4.011	3.842	0.169		4501296	38.4		76.8	486522	
D 30 13C2 PFDaA										
615.00 > 570.00	4.295	4.132	0.163		5498070	49.6		99.1	156627	
33 Perfluorotetradecanoic acid										
712.50 > 668.90	4.803	4.642	0.161	1.000	48241	0.2768			34.0	
713.00 > 169.00	4.795	4.642	0.153	0.998	6157		7.84(0.00-0.00)		656	

QC Flag Legend

Review Flags

M - Manually Integrated

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_033.d

Injection Date: 15-Dec-2016 16:54:18

Instrument ID: A8_N

Lims ID: 320-24118-B-3-A

Lab Sample ID: 320-24118-3

Client ID: CS-10

Operator ID: A8-PC\A8

ALS Bottle#: 41

Worklist Smp#: 33

Injection Vol: 2.0 ul

Dil. Factor: 1.0000













Method: A8_N

Limit Group: LC PFC_DOD ICAL


D 2 13C4 PFBA

1 Perfluorobutyric acid


D 4 13C5-PFPeA

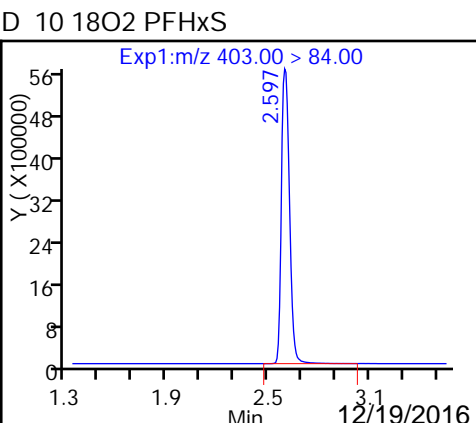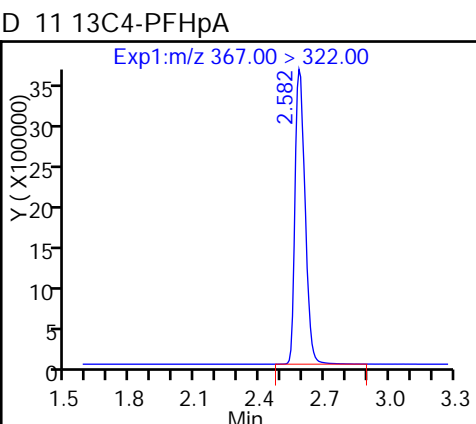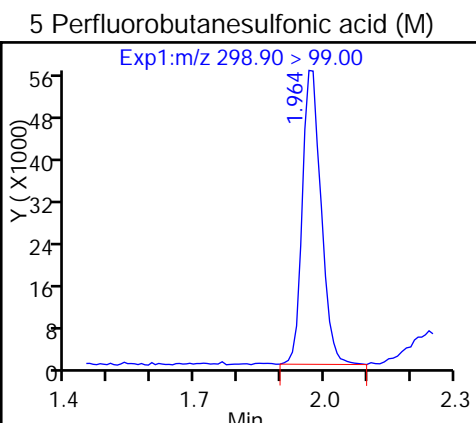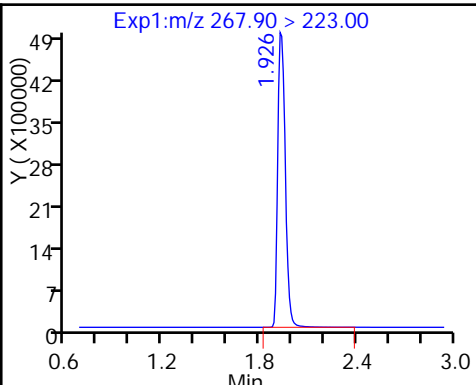


D 14 13C4 PFOA




15 Perfluorooctanoic acid




15 Perfluorooctanoic acid




18 Perfluorooctane sulfonic acid




18 Perfluorooctane sulfonic acid

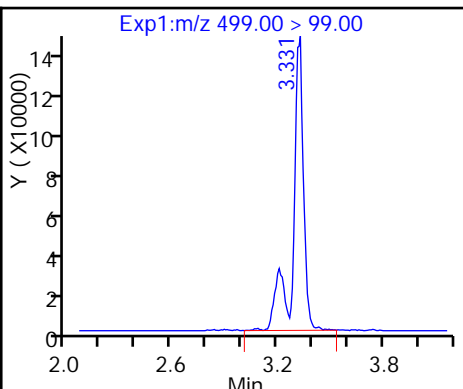


D 17 13C4 PFOS




D 19 13C5 PFNA




20 Perfluorononanoic acid (ND)




D 21 13C8 FOSA




22 Perfluorooctane Sulfonamide (ND)




24 Perfluorodecanoic acid

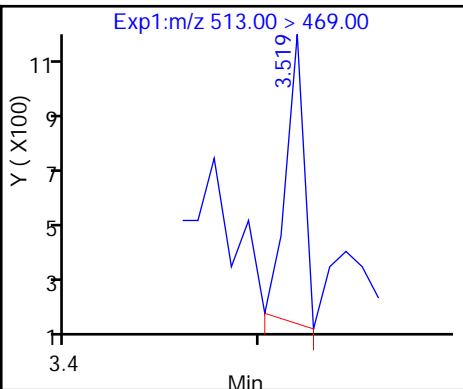


D 23 13C2 PFDA




26 Perfluorodecane Sulfonic acid




28 Perfluoroundecanoic acid

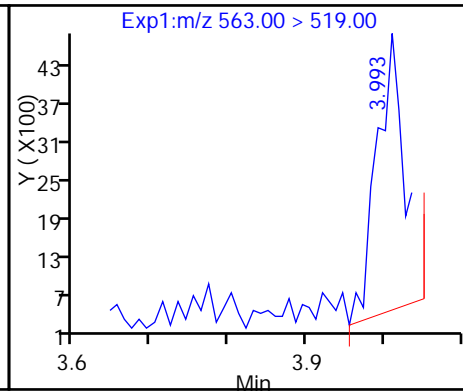


D 27 13C2 PFUnA

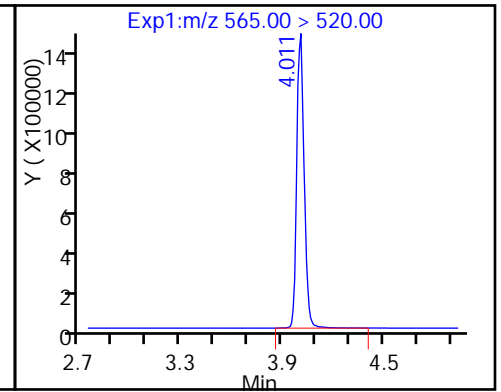


D 30 13C2 PFDaA




29 Perfluorododecanoic acid (ND)




31 Perfluorotridecanoic acid (ND)

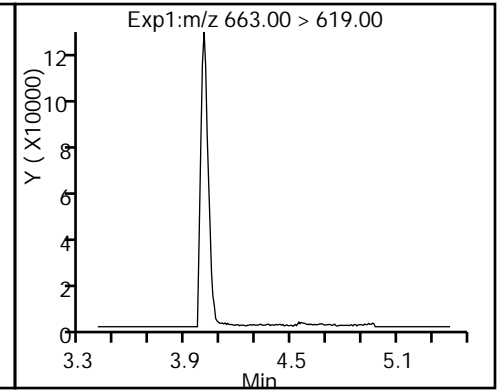

33 Perfluorotetradecanoic acid



33 Perfluorotetradecanoic acid



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_033.d
Injection Date: 15-Dec-2016 16:54:18 Instrument ID: A8_N
Lims ID: 320-24118-B-3-A Lab Sample ID: 320-24118-3
Client ID: CS-10
Operator ID: A8-PC\A8 ALS Bottle#: 41 Worklist Smp#: 33
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL
Column: Detector EXP1

12 Perfluoroheptanoic acid, CAS: 375-85-9

Signal: 1


Not Detected
Expected RT: 2.43

Processing Integration Results

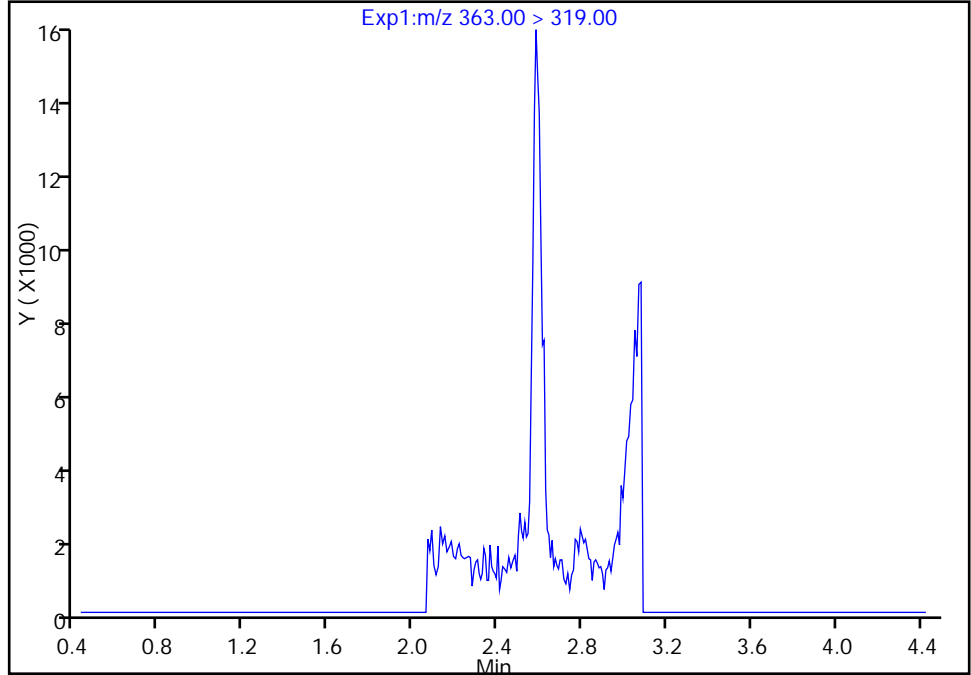

Manual Integration Results

RT: 2.58
Area: 43181
Amount: 0.183119
Amount Units: ng/ml

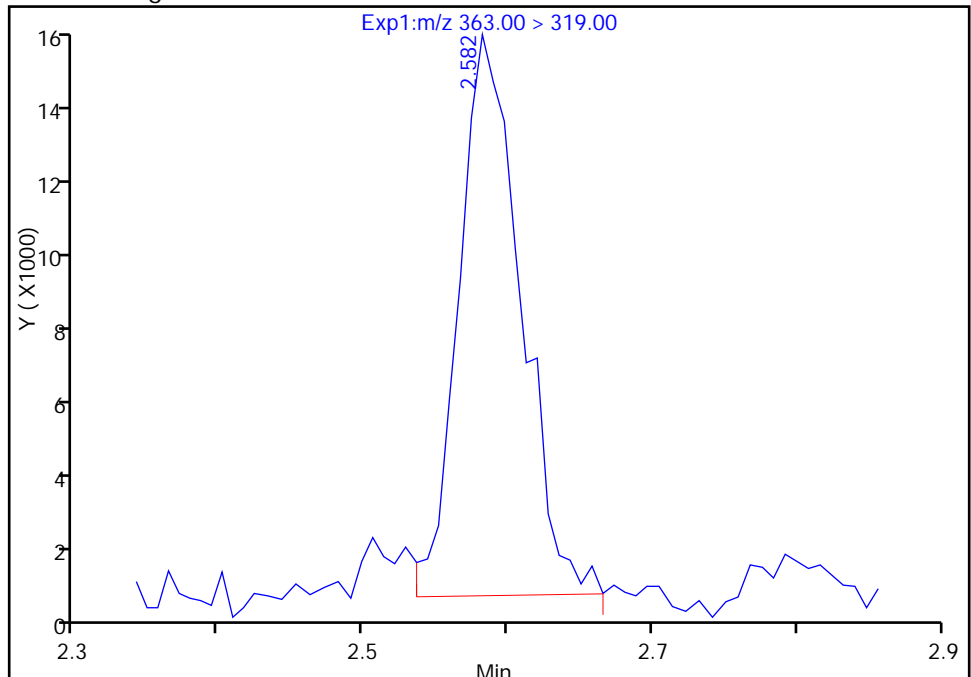

Reviewer: chandrasenas, 16-Dec-2016 09:41:46
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_033.d
Injection Date: 15-Dec-2016 16:54:18 Instrument ID: A8_N
Lims ID: 320-24118-B-3-A Lab Sample ID: 320-24118-3
Client ID: CS-10
Operator ID: A8-PC\A8 ALS Bottle#: 41 Worklist Smp#: 33
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL
Column: Detector EXP1

5 Perfluorobutanesulfonic acid, CAS: 375-73-5

Signal: 1


RT: 1.97
Area: 382939
Amount: 0.670480
Amount Units: ng/ml

Processing Integration Results

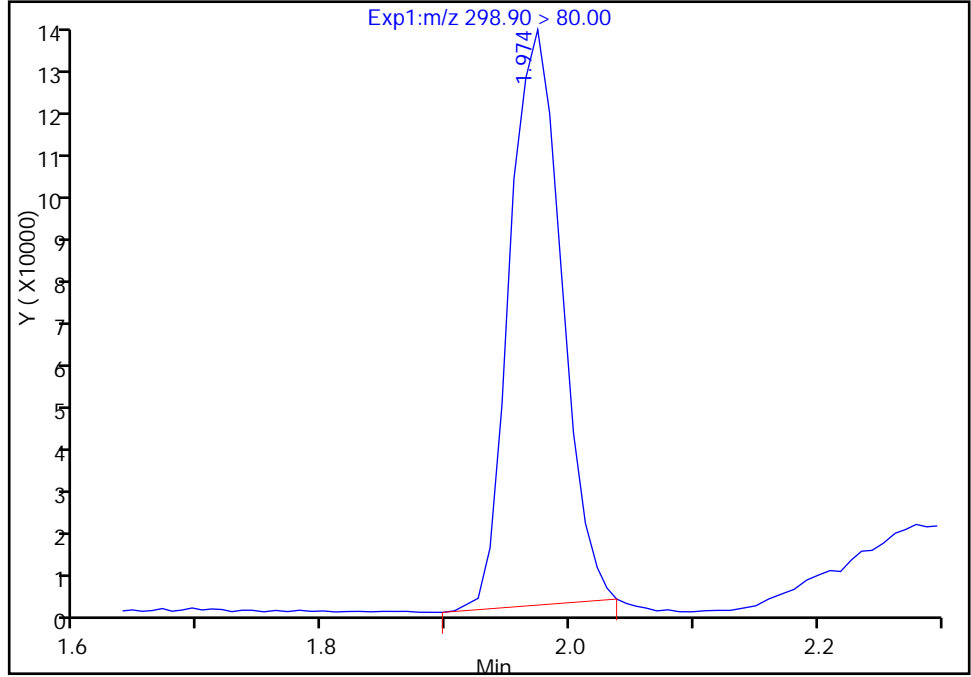

RT: 1.97
Area: 396869
Amount: 0.694869
Amount Units: ng/ml

Manual Integration Results

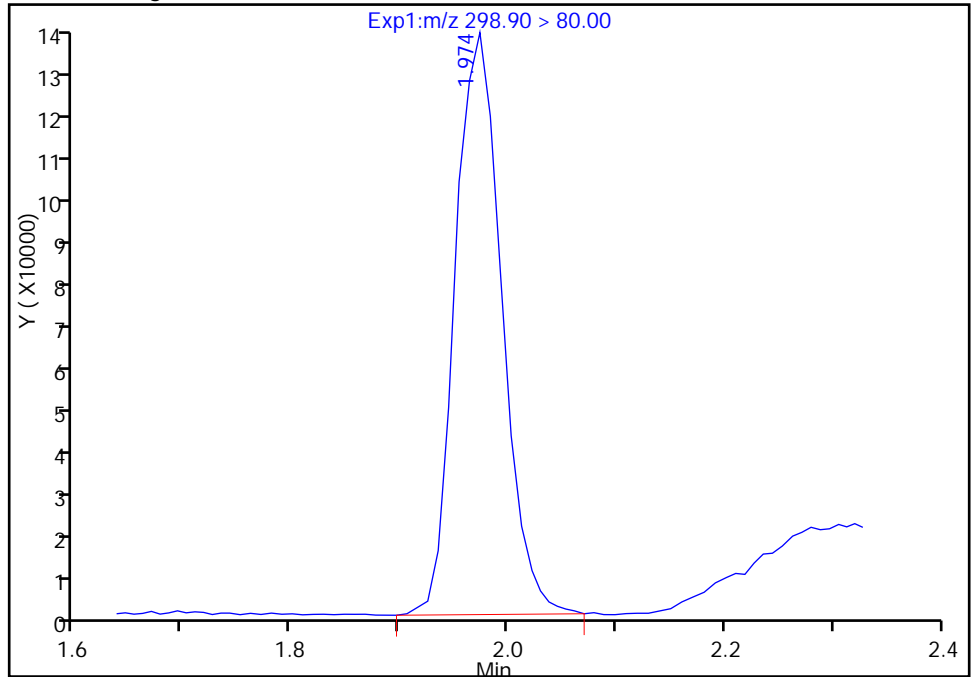

Reviewer: chandrasenas, 16-Dec-2016 09:41:46
Audit Action: Manually Integrated

Audit Reason: Incomplete Integration

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_033.d
Injection Date: 15-Dec-2016 16:54:18 Instrument ID: A8_N
Lims ID: 320-24118-B-3-A Lab Sample ID: 320-24118-3
Client ID: CS-10
Operator ID: A8-PC\A8 ALS Bottle#: 41 Worklist Smp#: 33
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL
Column: Detector EXP1

5 Perfluorobutanesulfonic acid, CAS: 375-73-5

Signal: 2


RT: 1.96
Area: 151724
Amount: 0.670480
Amount Units: ng/ml

Processing Integration Results

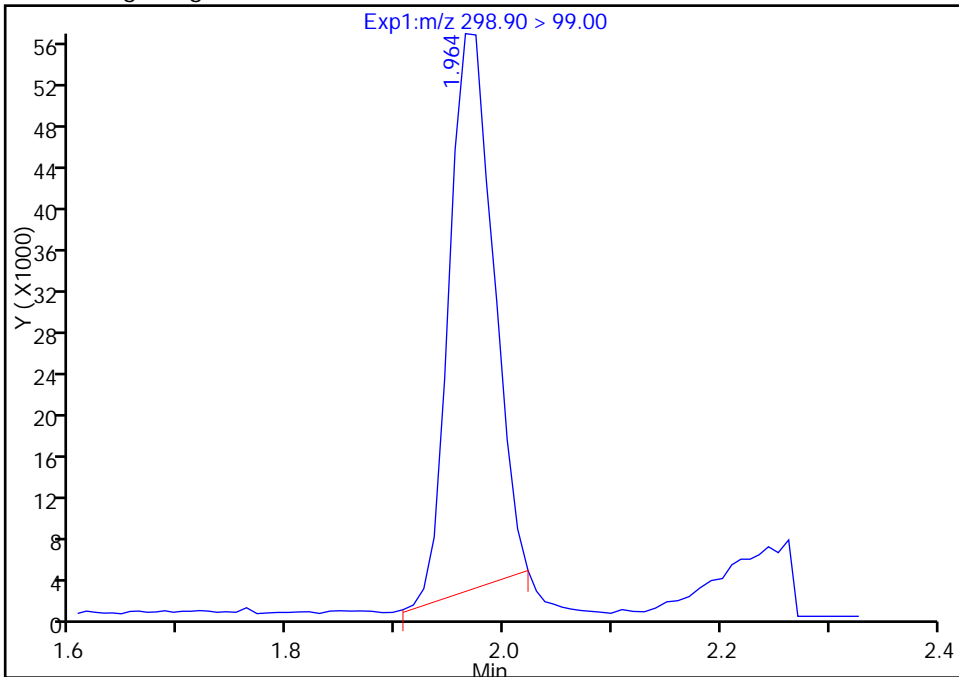

RT: 1.96
Area: 169649
Amount: 0.694869
Amount Units: ng/ml

Manual Integration Results

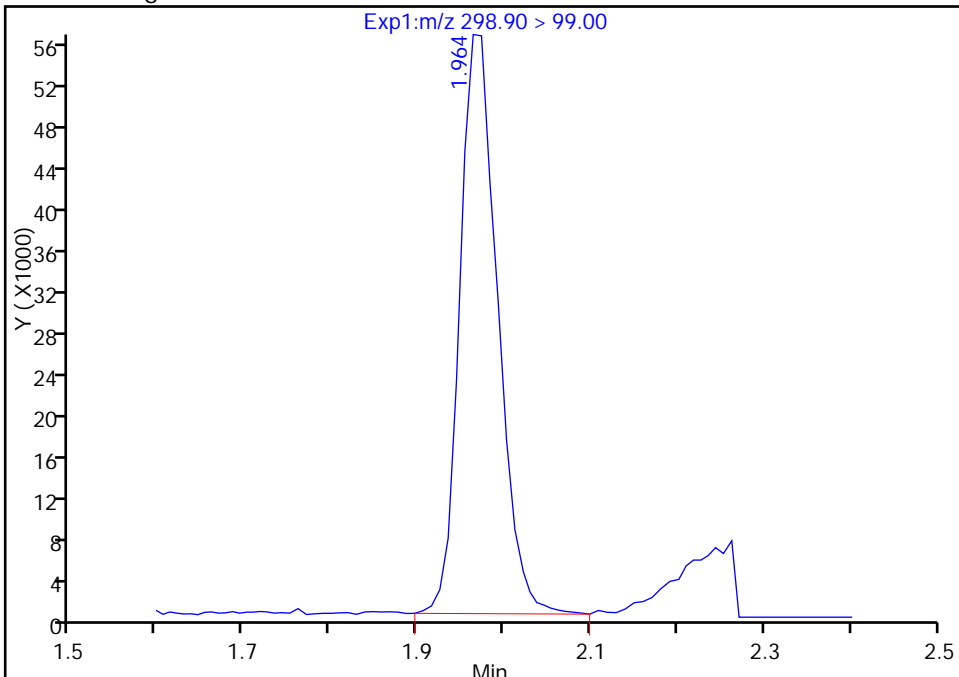

Reviewer: chandrasenas, 16-Dec-2016 09:41:46

Audit Action: Manually Integrated

Audit Reason: Incomplete Integration

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: CS-41 Lab Sample ID: 320-24118-4
 Matrix: Water Lab File ID: 15DEC2016B_034.d
 Analysis Method: 537 (Modified) Date Collected: 12/06/2016 08:30
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 246.6(mL) Date Analyzed: 12/15/2016 17:01
 Con. Extract Vol.: 0.5(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: Acquity ID: 2.1(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142379 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
375-22-4	Perfluorobutanoic acid (PFBA)	1.0	U	2.5	1.0	0.46
2706-90-3	Perfluoropentanoic acid (PFPeA)	2.0	U	2.5	2.0	1.0
307-24-4	Perfluorohexanoic acid (PFHxA)	2.0	U	2.5	2.0	0.80
375-85-9	Perfluoroheptanoic acid (PFHpA)	2.0	U	2.5	2.0	0.81
335-67-1	Perfluorooctanoic acid (PFOA)	2.0	U	2.5	2.0	0.76
375-95-1	Perfluorononanoic acid (PFNA)	2.0	U	2.5	2.0	0.66
335-76-2	Perfluorodecanoic acid (PFDA)	1.0	U	2.5	1.0	0.45
2058-94-8	Perfluoroundecanoic acid (PFUnA)	2.0	U	2.5	2.0	0.76
307-55-1	Perfluorododecanoic acid (PFDoA)	2.0	U	2.5	2.0	0.59
72629-94-8	Perfluorotridecanoic Acid (PFTriA)	2.0	U	2.5	2.0	0.56
376-06-7	Perfluorotetradecanoic acid (PFTeA)	0.51	J	2.5	1.0	0.41
375-73-5	Perfluorobutanesulfonic acid (PFBS)	2.0	U	2.5	2.0	0.93
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	2.0	U M	2.5	2.0	0.88
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	3.0	U	4.1	3.0	1.3
335-77-3	Perfluorodecanesulfonic acid (PFDS)	3.0	U	4.1	3.0	1.2
754-91-6	Perfluorooctane Sulfonamide (FOSA)	2.0	U	2.5	2.0	0.65

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: CS-41 Lab Sample ID: 320-24118-4
 Matrix: Water Lab File ID: 15DEC2016B_034.d
 Analysis Method: 537 (Modified) Date Collected: 12/06/2016 08:30
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 246.6(mL) Date Analyzed: 12/15/2016 17:01
 Con. Extract Vol.: 0.5(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: Acquity ID: 2.1(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142379 Units: ng/L

CAS NO.	ISOTOPE DILUTION	%REC	Q	LIMITS
STL01056	13C8 FOSA	3	Q	25-150
STL00992	13C4 PFBA	86		25-150
STL00993	13C2 PFHxA	87		25-150
STL00990	13C4 PFOA	82		25-150
STL00995	13C5 PFNA	63		25-150
STL00996	13C2 PFDA	55		25-150
STL00997	13C2 PFUnA	62		25-150
STL00998	13C2 PFDoA	80		25-150
STL00994	18O2 PFHxS	101		25-150
STL00991	13C4 PFOS	104		25-150
STL01892	13C4-PFHpA	90		25-150
STL01893	13C5 PFPeA	101		25-150

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_034.d
 Lims ID: 320-24118-B-4-A
 Client ID: CS-41
 Sample Type: Client
 Inject. Date: 15-Dec-2016 17:01:47 ALS Bottle#: 42 Worklist Smp#: 34
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-24118-b-4-a
 Misc. Info.: Plate: 1 Rack: 5
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 17:09:28 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 16-Dec-2016 17:09:28

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.641	1.534	0.107	15008001	43.2		86.3	1339667	
1 Perfluorobutyric acid	212.90 > 169.00	1.633	1.535	0.098	15636	0.0610			88.1	
D 4 13C5-PFPeA	267.90 > 223.00	1.938	1.810	0.128	13391721	50.3		101	832529	
3 Perfluoropentanoic acid	262.90 > 219.00	1.919	1.810	0.109	17128	0.0648			149	
7 Perfluorohexanoic acid	313.00 > 269.00	2.247	2.096	0.151	9571	0.0482			204	
D 6 13C2 PFHxA	315.00 > 270.00	2.238	2.097	0.141	10682361	43.6		87.2	416520	
D 11 13C4-PFHpA	367.00 > 322.00	2.579	2.426	0.153	10167615	44.9		89.8	544201	
9 Perfluorohexanesulfonic acid	399.00 > 80.00	2.595	2.431	0.164	102539	0.3012				M M
D 10 18O2 PFHxS	403.00 > 84.00	2.602	2.446	0.156	15636371	47.8		101	1620595	
D 14 13C4 PFOA	417.00 > 372.00	2.951	2.783	0.168	9416968	40.9		81.8	735241	
D 17 13C4 PFOS	503.00 > 80.00	3.321	3.151	0.170	12340788	49.6		104	425253	
D 19 13C5 PFNA	468.00 > 423.00	3.328	3.153	0.175	5605150	31.5		63.1	276062	
D 21 13C8 FOSA	506.00 > 78.00	3.652	3.488	0.164	584864	1.52		3.0	30294	
24 Perfluorodecanoic acid	513.00 > 469.00	3.474	3.510	-0.036	1408	0.0171			21.5	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 23 13C2 PFDA										
515.00 > 470.00	3.691	3.513	0.178		4350926	27.7		55.3	153241	
26 Perfluorodecane Sulfonic acid										
599.00 > 80.00	3.882	3.822	0.060	1.000	779	0.005167				
28 Perfluoroundecanoic acid										
563.00 > 519.00	4.016	3.839	0.177	1.000	14405	0.2075			368	
D 27 13C2 PUnA										
565.00 > 520.00	4.007	3.842	0.165		3630436	31.0		61.9	187551	
D 30 13C2 PFDaA										
615.00 > 570.00	4.299	4.132	0.167		4442811	40.0		80.1	284571	
33 Perfluorotetradecanoic acid										
712.50 > 668.90	4.808	4.642	0.166	1.000	35229	0.2502			34.1	
713.00 > 169.00	4.808	4.642	0.166	1.000	4343		8.11(0.00-0.00)		486	

QC Flag Legend

Review Flags

M - Manually Integrated

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_034.d

Injection Date: 15-Dec-2016 17:01:47

Instrument ID: A8_N

Lims ID: 320-24118-B-4-A

Lab Sample ID: 320-24118-4

Client ID: CS-41

Operator ID: A8-PC\A8

ALS Bottle#: 42

Worklist Smp#: 34

Injection Vol: 2.0 ul

Dil. Factor: 1.0000













Method: A8_N

Limit Group: LC PFC_DOD ICAL


D 2 13C4 PFBA

1 Perfluorobutyric acid


D 4 13C5-PFPeA

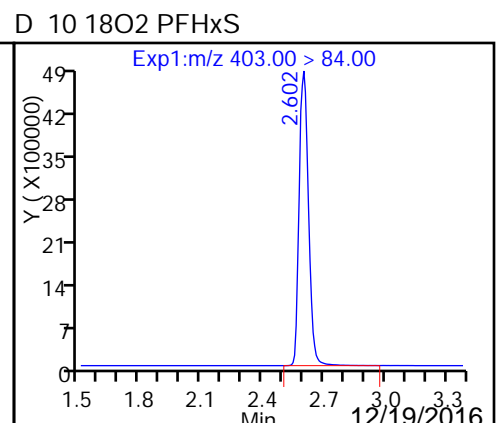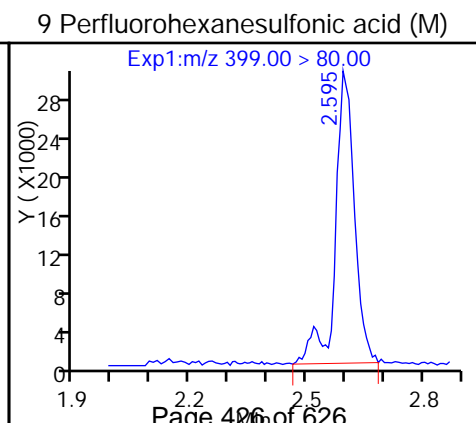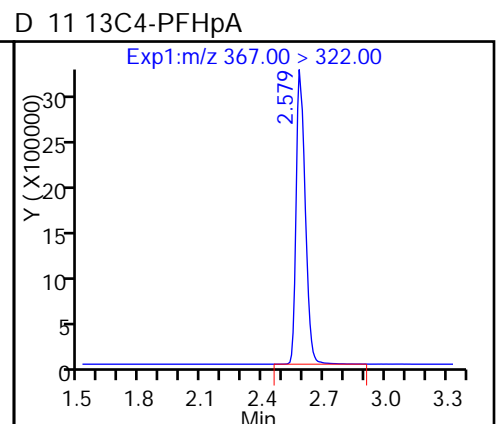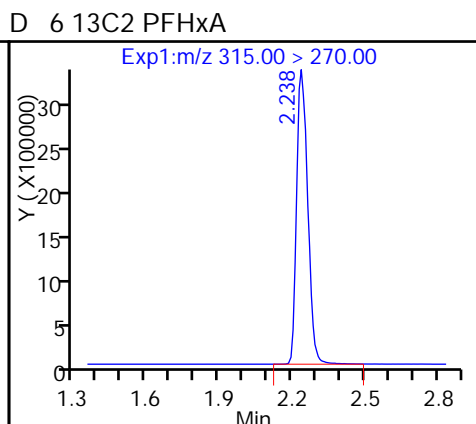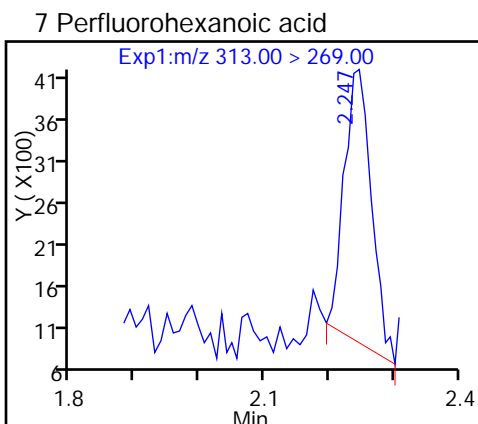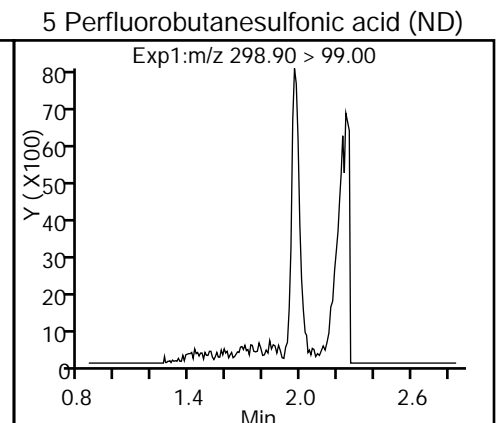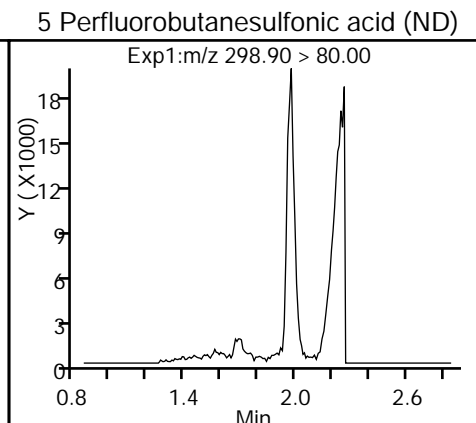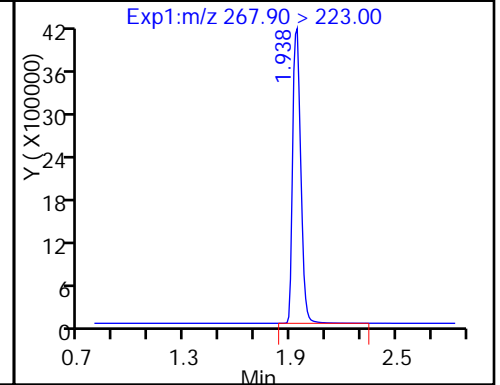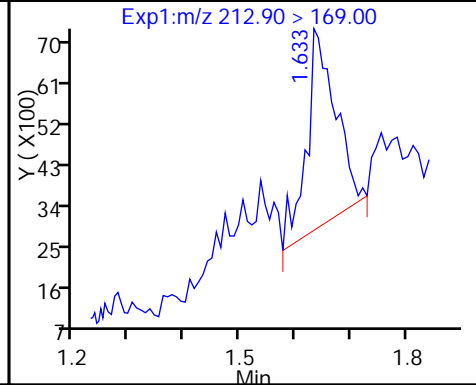


D 14 13C4 PFOA




15 Perfluorooctanoic acid (ND)




15 Perfluorooctanoic acid (ND)

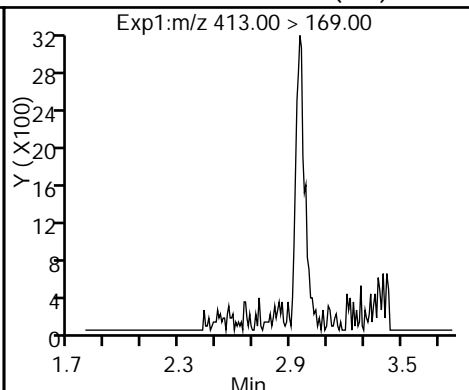


18 Perfluorooctane sulfonic acid (ND)




18 Perfluorooctane sulfonic acid (ND)




D 17 13C4 PFOS




D 19 13C5 PFNA




20 Perfluorononanoic acid (ND)




D 21 13C8 FOSA

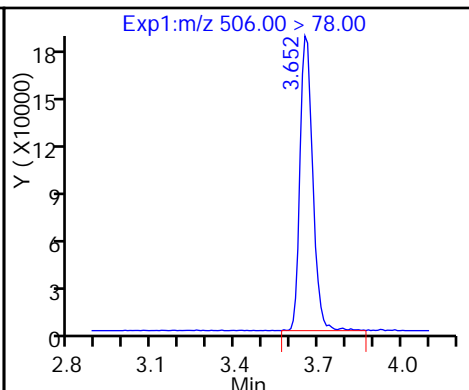


22 Perfluorooctane Sulfonamide (ND)




24 Perfluorodecanoic acid



D 23 13C2 PFDA



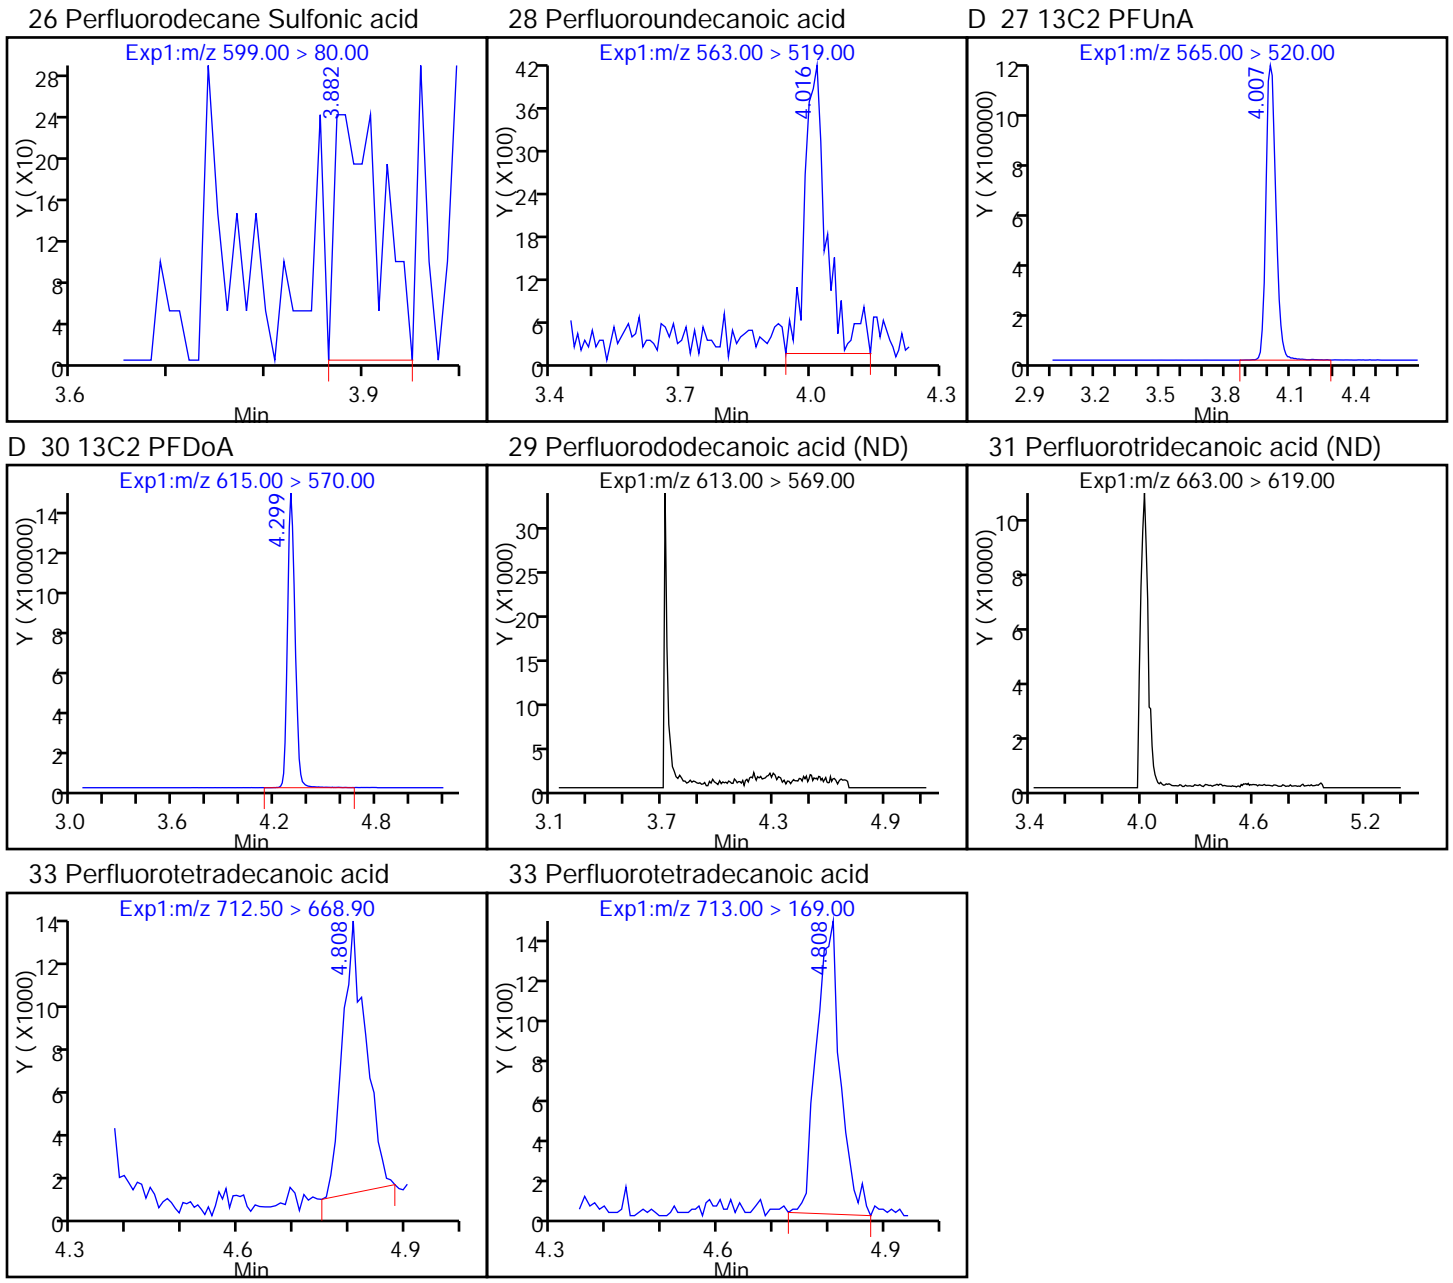

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_034.d
Injection Date: 15-Dec-2016 17:01:47 Instrument ID: A8_N
Lims ID: 320-24118-B-4-A Lab Sample ID: 320-24118-4
Client ID: CS-41
Operator ID: A8-PC\A8 ALS Bottle#: 42 Worklist Smp#: 34
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL
Column: Detector EXP1

9 Perfluorohexanesulfonic acid, CAS: 355-46-4

Signal: 1


Not Detected
Expected RT: 2.43

Processing Integration Results

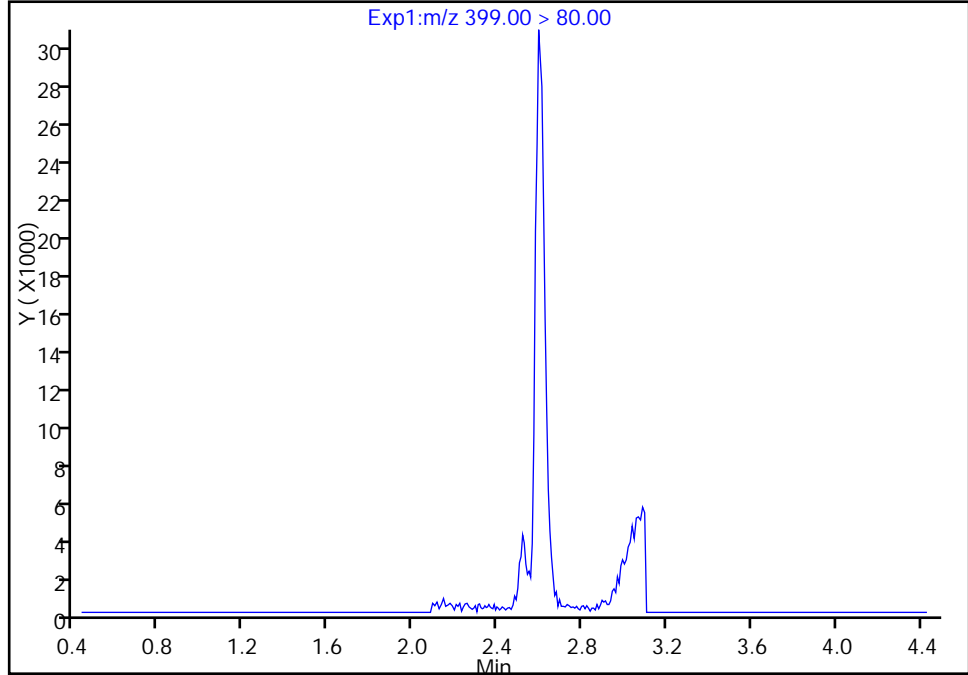

Manual Integration Results

RT: 2.59
Area: 102539
Amount: 0.301155
Amount Units: ng/ml

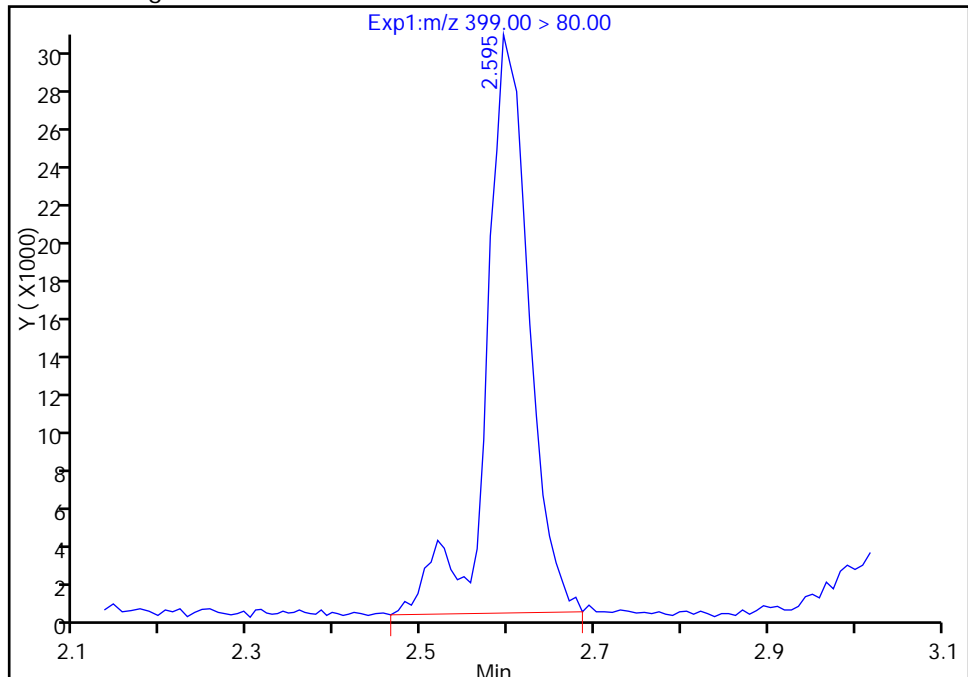

Reviewer: chandrasenas, 16-Dec-2016 09:42:33

Audit Action: Manually Integrated

Audit Reason: Assign Peak

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: CS-12 Lab Sample ID: 320-24118-5
 Matrix: Water Lab File ID: 15DEC2016B_035.d
 Analysis Method: 537 (Modified) Date Collected: 12/06/2016 10:00
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 261.6(mL) Date Analyzed: 12/15/2016 17:09
 Con. Extract Vol.: 0.5(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: Acquity ID: 2.1(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142379 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
375-22-4	Perfluorobutanoic acid (PFBA)	0.96	U	2.4	0.96	0.44
2706-90-3	Perfluoropentanoic acid (PFPeA)	1.9	U	2.4	1.9	0.95
307-24-4	Perfluorohexanoic acid (PFHxA)	1.9	U	2.4	1.9	0.75
375-85-9	Perfluoroheptanoic acid (PFHpA)	1.9	U	2.4	1.9	0.77
335-67-1	Perfluorooctanoic acid (PFOA)	1.9	U	2.4	1.9	0.71
375-95-1	Perfluorononanoic acid (PFNA)	1.9	U	2.4	1.9	0.63
335-76-2	Perfluorodecanoic acid (PFDA)	0.96	U	2.4	0.96	0.42
2058-94-8	Perfluoroundecanoic acid (PFUnA)	1.9	U	2.4	1.9	0.71
307-55-1	Perfluorododecanoic acid (PFDoA)	1.9	U	2.4	1.9	0.56
72629-94-8	Perfluorotridecanoic Acid (PFTriA)	1.9	U	2.4	1.9	0.53
376-06-7	Perfluorotetradecanoic acid (PFTeA)	0.72	J	2.4	0.96	0.38
375-73-5	Perfluorobutanesulfonic acid (PFBS)	1.9	U	2.4	1.9	0.88
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	1.9	U	2.4	1.9	0.83
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	2.9	U	3.8	2.9	1.2
335-77-3	Perfluorodecanesulfonic acid (PFDS)	2.9	U	3.8	2.9	1.2
754-91-6	Perfluorooctane Sulfonamide (FOSA)	1.9	U	2.4	1.9	0.61

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: CS-12 Lab Sample ID: 320-24118-5
 Matrix: Water Lab File ID: 15DEC2016B_035.d
 Analysis Method: 537 (Modified) Date Collected: 12/06/2016 10:00
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 261.6(mL) Date Analyzed: 12/15/2016 17:09
 Con. Extract Vol.: 0.5(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: Acquity ID: 2.1(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142379 Units: ng/L

CAS NO.	ISOTOPE DILUTION	%REC	Q	LIMITS
STL01056	13C8 FOSA	4	Q	25-150
STL00992	13C4 PFBA	84		25-150
STL00993	13C2 PFHxA	83		25-150
STL00990	13C4 PFOA	79		25-150
STL00995	13C5 PFNA	62		25-150
STL00996	13C2 PFDA	59		25-150
STL00997	13C2 PFUnA	64		25-150
STL00998	13C2 PFDoA	80		25-150
STL00994	18O2 PFHxS	101		25-150
STL00991	13C4 PFOS	104		25-150
STL01892	13C4-PFHpA	85		25-150
STL01893	13C5 PFPeA	93		25-150

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_035.d
 Lims ID: 320-24118-B-5-A
 Client ID: CS-12
 Sample Type: Client
 Inject. Date: 15-Dec-2016 17:09:18 ALS Bottle#: 43 Worklist Smp#: 35
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-24118-b-5-a
 Misc. Info.: Plate: 1 Rack: 5
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 15:30:05 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 16-Dec-2016 09:43:02

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.641	1.534	0.107	14643031	42.1		84.2	1310113	
1 Perfluorobutyric acid	212.90 > 169.00	1.650	1.535	0.115	14085	0.0563			77.6	
D 4 13C5-PFPeA	267.90 > 223.00	1.929	1.810	0.119	12331926	46.3		92.7	783758	
3 Perfluoropentanoic acid	262.90 > 219.00	1.929	1.810	0.119	22011	0.0904			177	
D 6 13C2 PFHxA	315.00 > 270.00	2.247	2.097	0.150	10115220	41.3		82.5	1064698	
D 11 13C4-PFHpA	367.00 > 322.00	2.587	2.426	0.161	9576761	42.3		84.6	505121	
D 10 18O2 PFHxS	403.00 > 84.00	2.602	2.446	0.156	15659451	47.9		101	1200630	
D 14 13C4 PFOA	417.00 > 372.00	2.960	2.783	0.177	9095647	39.5		79.0	979174	
D 17 13C4 PFOS	503.00 > 80.00	3.329	3.151	0.178	12314316	49.5		104	430244	
D 19 13C5 PFNA	468.00 > 423.00	3.337	3.153	0.184	5505423	31.0		62.0	323335	
D 21 13C8 FOSA	506.00 > 78.00	3.663	3.488	0.175	679386	1.77		3.5	71103	
24 Perfluorodecanoic acid	513.00 > 469.00	3.526	3.510	0.016	728	0.008373			24.3	
D 23 13C2 PFDA	515.00 > 470.00	3.702	3.513	0.189	4606381	29.3		58.6	119193	
26 Perfluorodecane Sulfonic acid	599.00 > 80.00	3.983	3.822	0.161	550	0.003656				

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
28 Perfluoroundecanoic acid	563.00 > 519.00	4.019	3.839	0.180	1.000	10747	0.1503		296	
D 27 13C2 PFUnA	565.00 > 520.00	4.010	3.842	0.168		3738367	31.9	63.8	288164	
D 30 13C2 PFDoA	615.00 > 570.00	4.314	4.132	0.182		4460036	40.2	80.4	120007	
33 Perfluorotetradecanoic acid	712.50 > 668.90	4.804	4.642	0.162	1.000	52909	0.3743		41.7	
	713.00 > 169.00	4.812	4.642	0.170	1.002	7100	7.45(0.00-0.00)		1279	




TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_035.d
Injection Date: 15-Dec-2016 17:09:18 Instrument ID: A8_N
Lims ID: 320-24118-B-5-A Lab Sample ID: 320-24118-5
Client ID: CS-12
Operator ID: A8-PC\A8 ALS Bottle#: 43 Worklist Smp#: 35
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL

D 2 13C4 PFBA

1 Perfluorobutyric acid




D 4 13C5-PFPeA

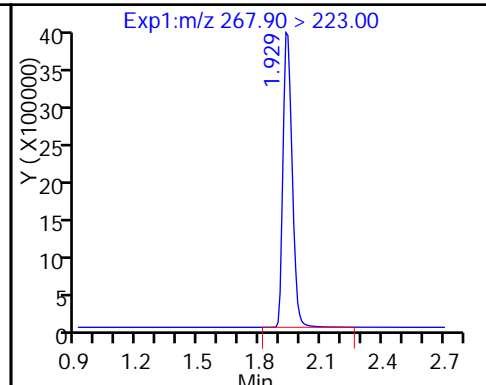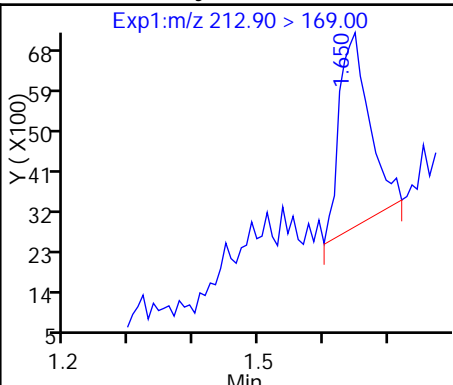

3 Perfluoropentanoic acid

5 Perfluorobutanesulfonic acid (ND)




5 Perfluorobutanesulfonic acid (ND)

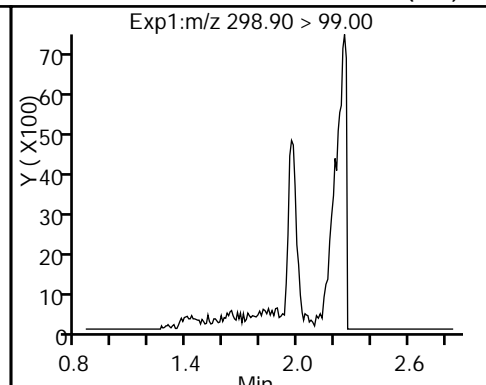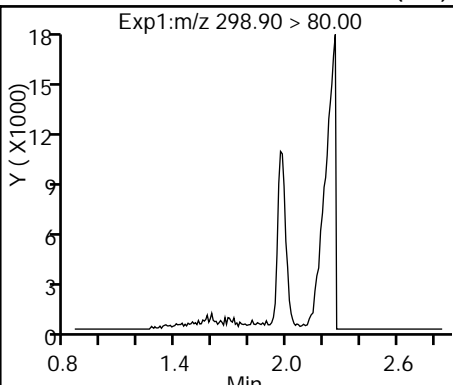

7 Perfluorohexanoic acid (ND)

D 6 13C2 PFHxA




D 11 13C4-PFHpA

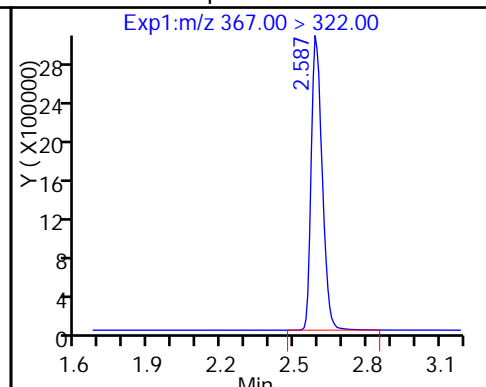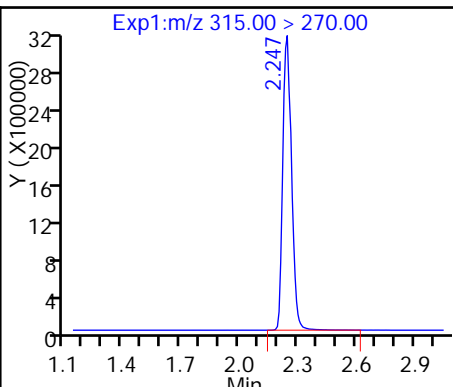


12 Perfluoroheptanoic acid (ND)

9 Perfluorohexanesulfonic acid (ND)


D 10 18O2 PFHxS

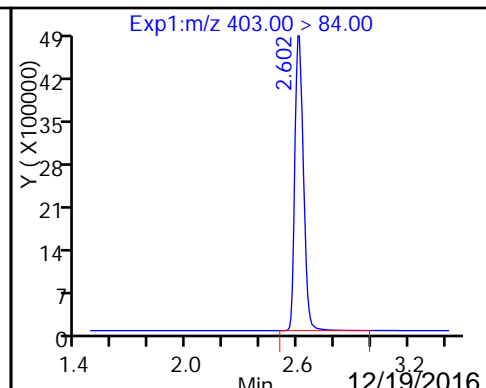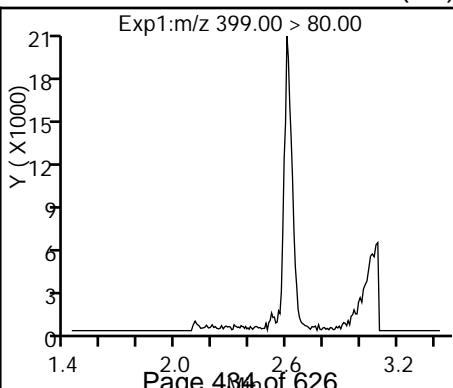


D 14 13C4 PFOA




15 Perfluorooctanoic acid (ND)

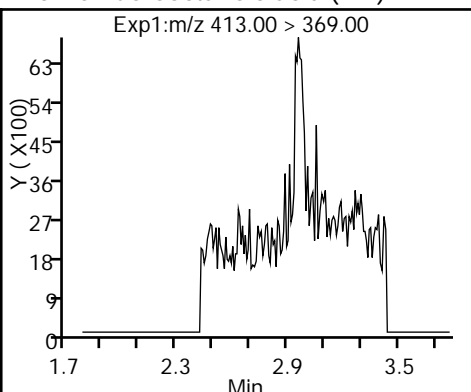


15 Perfluorooctanoic acid (ND)

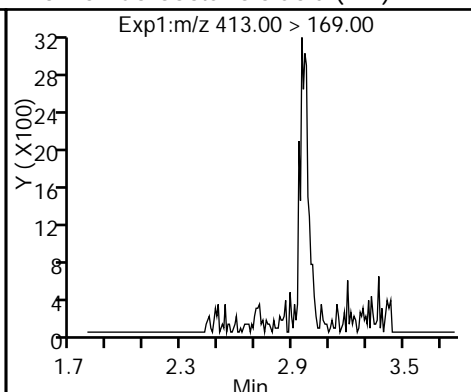


18 Perfluorooctane sulfonic acid (ND)




18 Perfluorooctane sulfonic acid (ND)




D 17 13C4 PFOS




D 19 13C5 PFNA




20 Perfluorononanoic acid (ND)




D 21 13C8 FOSA




22 Perfluorooctane Sulfonamide (ND)




24 Perfluorodecanoic acid



D 23 13C2 PFDA



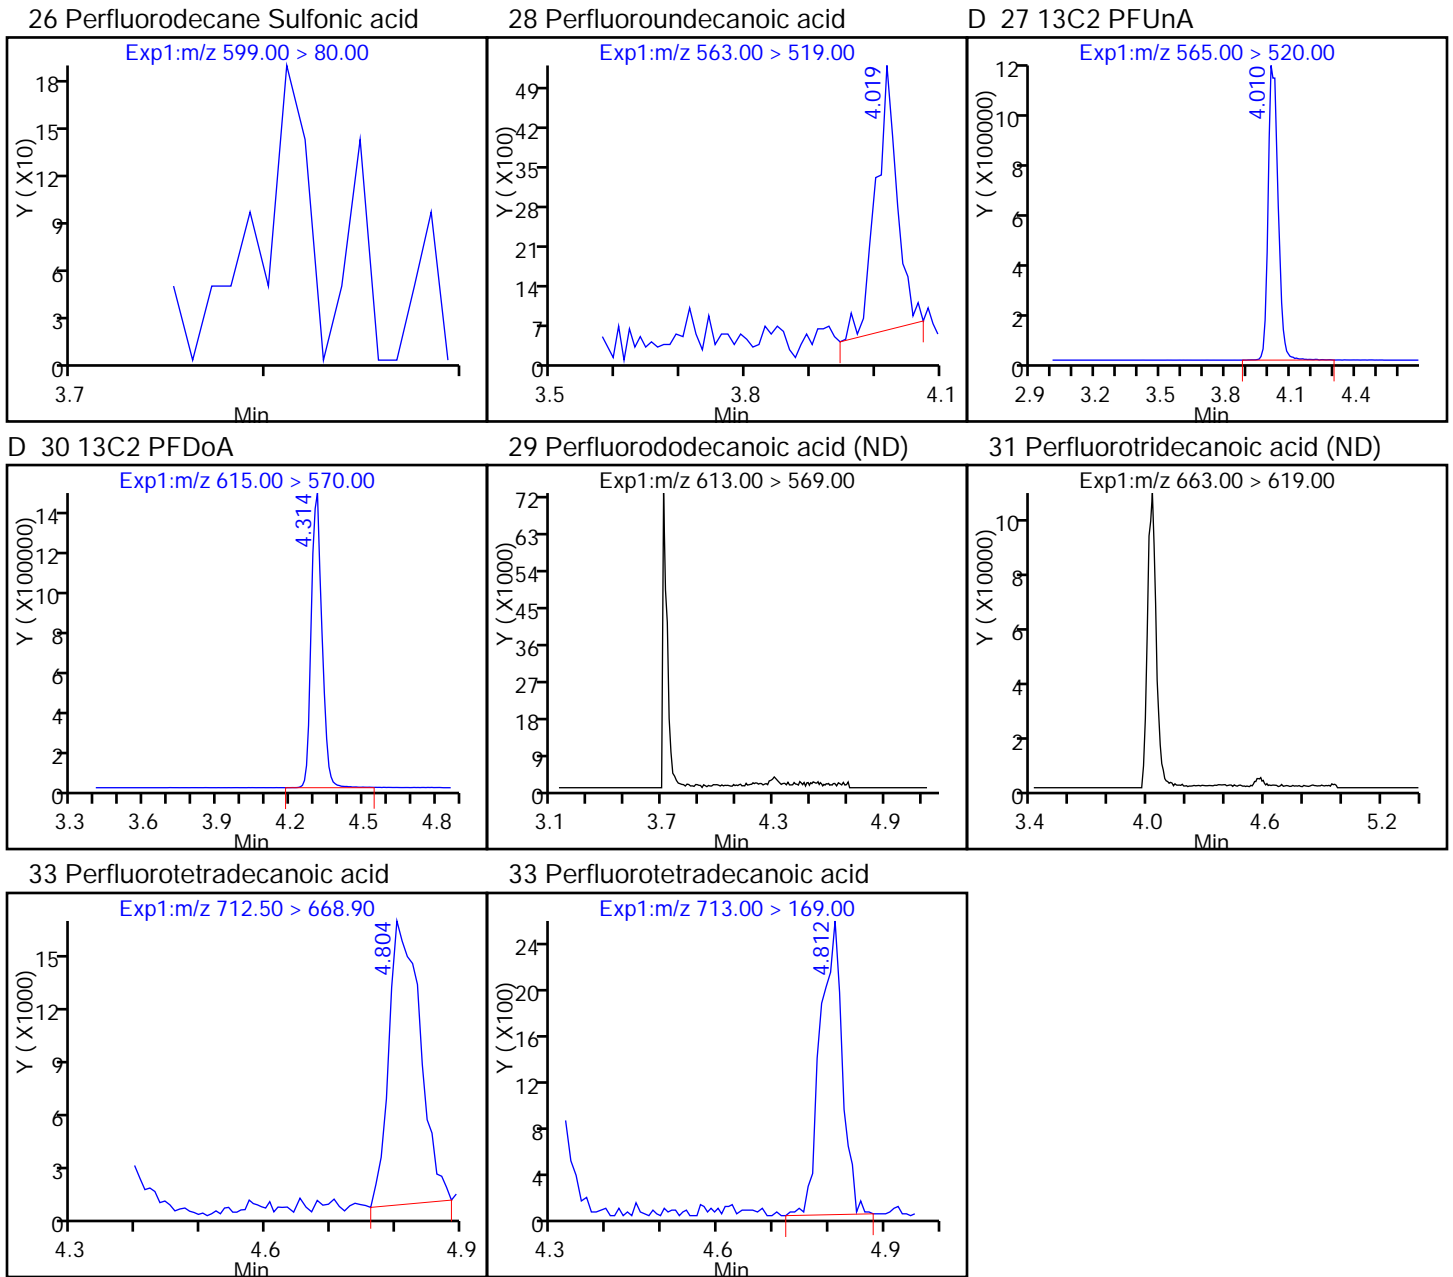

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: CS-1 Lab Sample ID: 320-24118-6
 Matrix: Water Lab File ID: 15DEC2016B_036.d
 Analysis Method: 537 (Modified) Date Collected: 12/06/2016 09:17
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 250.2 (mL) Date Analyzed: 12/15/2016 17:16
 Con. Extract Vol.: 0.5 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: Acquity ID: 2.1 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142379 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
375-22-4	Perfluorobutanoic acid (PFBA)	1.0	U	2.5	1.0	0.46
2706-90-3	Perfluoropentanoic acid (PFPeA)	2.0	U	2.5	2.0	0.99
307-24-4	Perfluorohexanoic acid (PFHxA)	2.0	U	2.5	2.0	0.79
375-85-9	Perfluoroheptanoic acid (PFHpA)	2.0	U	2.5	2.0	0.80
335-67-1	Perfluorooctanoic acid (PFOA)	2.0	U	2.5	2.0	0.75
375-95-1	Perfluorononanoic acid (PFNA)	2.0	U	2.5	2.0	0.65
335-76-2	Perfluorodecanoic acid (PFDA)	1.0	U	2.5	1.0	0.44
2058-94-8	Perfluoroundecanoic acid (PFUnA)	2.0	U	2.5	2.0	0.75
307-55-1	Perfluorododecanoic acid (PFDoA)	2.0	U	2.5	2.0	0.58
72629-94-8	Perfluorotridecanoic Acid (PFTriA)	2.0	U	2.5	2.0	0.55
376-06-7	Perfluorotetradecanoic acid (PFTeA)	0.75	J	2.5	1.0	0.40
375-73-5	Perfluorobutanesulfonic acid (PFBS)	2.0	U	2.5	2.0	0.92
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	2.0	U	2.5	2.0	0.87
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	3.0	U	4.0	3.0	1.3
335-77-3	Perfluorodecanesulfonic acid (PFDS)	3.0	U	4.0	3.0	1.2
754-91-6	Perfluorooctane Sulfonamide (FOSA)	2.0	U	2.5	2.0	0.64

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: CS-1 Lab Sample ID: 320-24118-6
 Matrix: Water Lab File ID: 15DEC2016B_036.d
 Analysis Method: 537 (Modified) Date Collected: 12/06/2016 09:17
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 250.2 (mL) Date Analyzed: 12/15/2016 17:16
 Con. Extract Vol.: 0.5 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: Acquity ID: 2.1 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142379 Units: ng/L

CAS NO.	ISOTOPE DILUTION	%REC	Q	LIMITS
STL01056	13C8 FOSA	5	Q	25-150
STL00992	13C4 PFBA	94		25-150
STL00993	13C2 PFHxA	95		25-150
STL00990	13C4 PFOA	81		25-150
STL00995	13C5 PFNA	54		25-150
STL00996	13C2 PFDA	48		25-150
STL00997	13C2 PFUnA	63		25-150
STL00998	13C2 PFDoA	84		25-150
STL00994	18O2 PFHxS	122		25-150
STL00991	13C4 PFOS	129		25-150
STL01892	13C4-PFHpA	94		25-150
STL01893	13C5 PFPeA	117		25-150

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_036.d
 Lims ID: 320-24118-B-6-A
 Client ID: CS-1
 Sample Type: Client
 Inject. Date: 15-Dec-2016 17:16:48 ALS Bottle#: 44 Worklist Smp#: 36
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-24118-b-6-a
 Misc. Info.: Plate: 1 Rack: 5
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 15:30:05 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 16-Dec-2016 09:44:09

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.666	1.534	0.132	16262756	46.8		93.5	1481096	
1 Perfluorobutyric acid	212.90 > 169.00	1.666	1.535	0.131	13993	0.0504			85.6	
D 4 13C5-PFPeA	267.90 > 223.00	1.958	1.810	0.148	15603089	58.6		117	1188779	
3 Perfluoropentanoic acid	262.90 > 219.00	1.958	1.810	0.148	22714	0.0738			205	
7 Perfluorohexanoic acid	313.00 > 269.00	2.275	2.096	0.179	8341	0.0384			162	
D 6 13C2 PFHxA	315.00 > 270.00	2.283	2.097	0.186	11685484	47.7		95.3	743043	
D 11 13C4-PFHpA	367.00 > 322.00	2.631	2.426	0.205	10618299	46.9		93.8	816214	
D 10 18O2 PFHxS	403.00 > 84.00	2.646	2.446	0.200	18819157	57.6		122	1129820	
D 14 13C4 PFOA	417.00 > 372.00	3.002	2.783	0.219	9333338	40.5		81.0	548927	
D 17 13C4 PFOS	503.00 > 80.00	3.375	3.151	0.224	15288164	61.4		129	644999	
D 19 13C5 PFNA	468.00 > 423.00	3.384	3.153	0.231	4809700	27.1		54.1	339416	
D 21 13C8 FOSA	506.00 > 78.00	3.702	3.488	0.214	1009980	2.63		5.3	77008	
24 Perfluorodecanoic acid	513.00 > 469.00	3.535	3.510	0.025	1242	0.0175			38.4	
43 Sodium 1H,1H,2H,2H-perfluorooctane	527.00 > 507.00	3.722	3.511	0.211	449	NR				

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 23 13C2 PFDA	515.00 > 470.00	3.742	3.513	0.229		3759423	23.9	47.8	96490	
D 42 M2-8:2FTS	529.00 > 509.00	3.722	3.513	0.209		291	0.002708	0.0		
D 45 d3-NMeFOSAA	573.00 > 419.00	3.887	3.676	0.211		1776	0.0236	0.0		
26 Perfluorodecane Sulfonic acid	599.00 > 80.00	4.022	3.822	0.200	1.000	1184	0.006339			
28 Perfluoroundecanoic acid	563.00 > 519.00	4.062	3.839	0.223	1.000	8920	0.1265		318	
D 27 13C2 PFUnA	565.00 > 520.00	4.054	3.842	0.212		3687706	31.5	62.9	303962	
D 46 d5-NEtFOSAA	589.00 > 419.00	3.858	3.842	0.016		2000	0.0255	0.0		
49 N-ethyl perfluorooctane sulfonamid	584.00 > 419.00	4.054	3.854	0.200	1.051	1623	NR			
D 52 d-N-MeFOSA-M	515.00 > 169.00	4.054	3.992	0.062		470	0.004944	0.0		
D 30 13C2 PFDaA	615.00 > 570.00	4.346	4.132	0.214		4661620	42.0	84.0	117105	
53 N-ethylperfluoro-1-octanesulfonami	526.00 > 169.00	4.247	4.187	0.060	1.000	267	NR			
D 32 13C2-PFTeDA	715.00 > 670.00	4.843	4.641	0.202		17686030	77.8	156	991403	
33 Perfluorotetradecanoic acid	712.50 > 668.90	4.843	4.642	0.201	1.000	55766	0.3774		48.4	
	713.00 > 169.00	4.843	4.642	0.201	1.000	7563	7.37(0.00-0.00)		946	
D 34 13C2-PFHxDA	815.00 > 770.00	5.253	5.057	0.196		7277931	58.4	117	196758	
35 Perfluorohexadecanoic acid	813.00 > 769.00	5.029	5.059	-0.030	1.000	1497	-0.5258		1.7	
36 Perfluorooctadecanoic acid	913.00 > 869.00	5.518	5.414	0.104	1.000	5311	0.0553		5.6	

QC Flag Legend

Processing Flags

NR - Missing Quant Standard




TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_036.d
Injection Date: 15-Dec-2016 17:16:48 Instrument ID: A8_N
Lims ID: 320-24118-B-6-A Lab Sample ID: 320-24118-6
Client ID: CS-1
Operator ID: A8-PC\A8 ALS Bottle#: 44 Worklist Smp#: 36
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL

D 2 13C4 PFBA

1 Perfluorobutyric acid




D 4 13C5-PFPeA

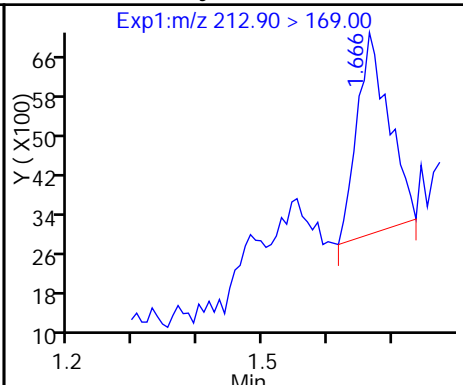

3 Perfluoropentanoic acid

5 Perfluorobutanesulfonic acid (ND)




5 Perfluorobutanesulfonic acid (ND)

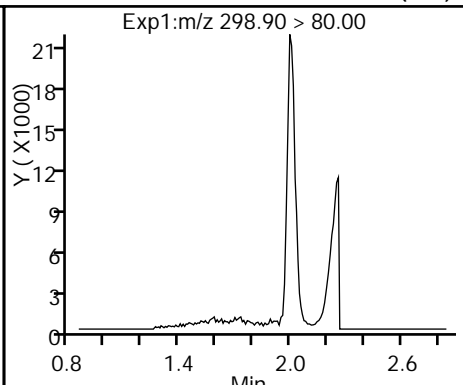

7 Perfluorohexanoic acid

D 6 13C2 PFHxA




D 11 13C4-PFHpA

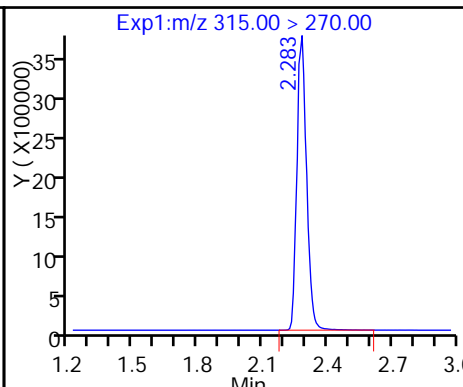

12 Perfluoroheptanoic acid (ND)


9 Perfluorohexanesulfonic acid (ND)

D 10 18O2 PFHxS

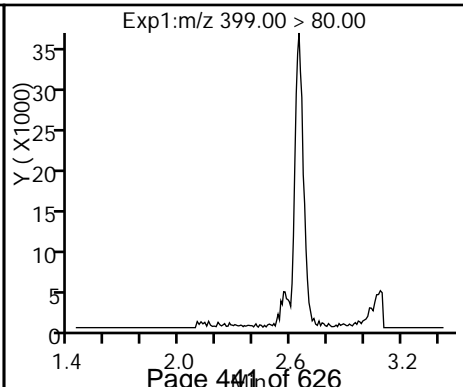

D 47 M2-6:2FTS (ND)


48 Sodium 1H,1H,2H,2H-perfluorooctadecanoate (ND) 13C4 PFOA

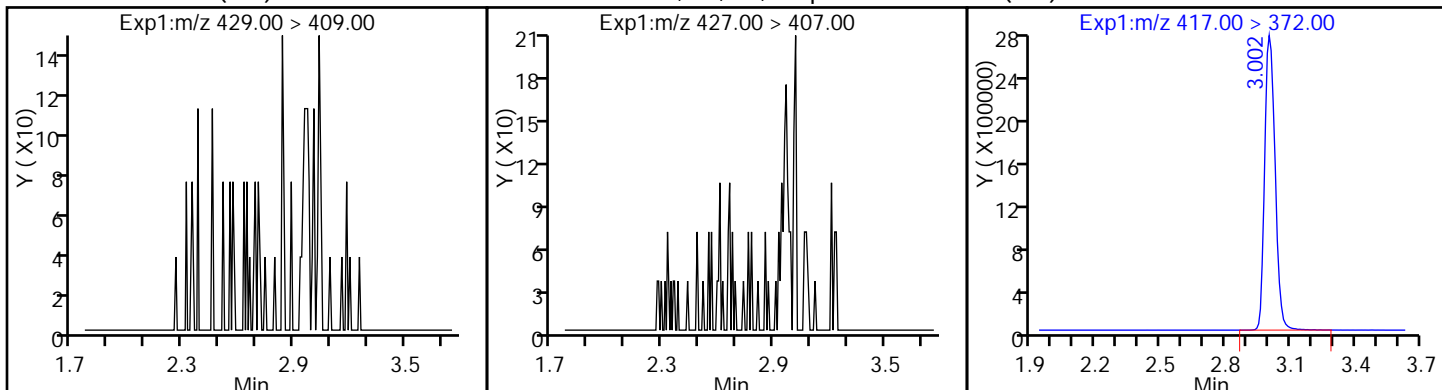

15 Perfluorooctanoic acid (ND)

15 Perfluorooctanoic acid (ND)


13 Perfluoroheptanesulfonic Acid (ND)

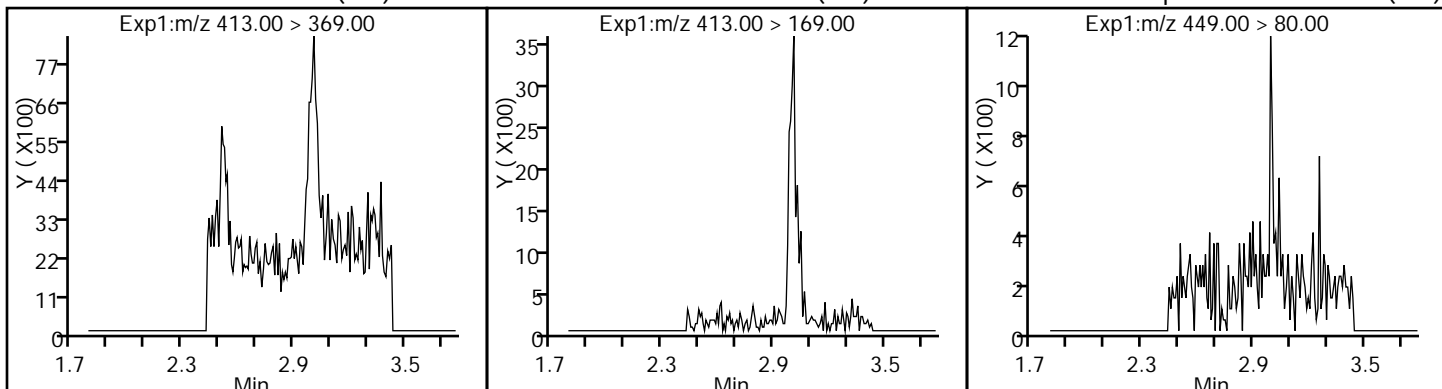

18 Perfluorooctane sulfonic acid (ND)

18 Perfluorooctane sulfonic acid (ND)


D 17 13C4 PFOS

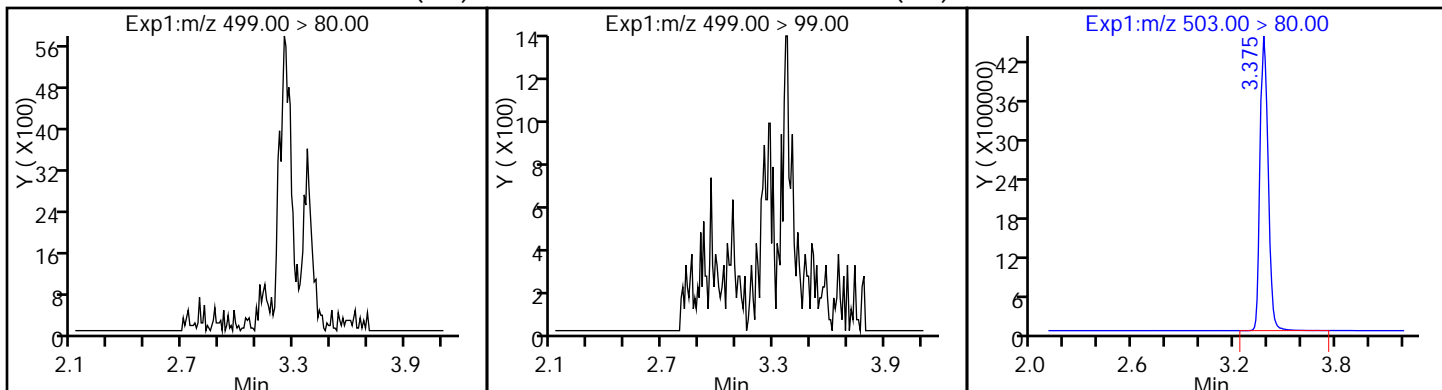

D 19 13C5 PFNA

20 Perfluorononanoic acid (ND)




D 21 13C8 FOSA

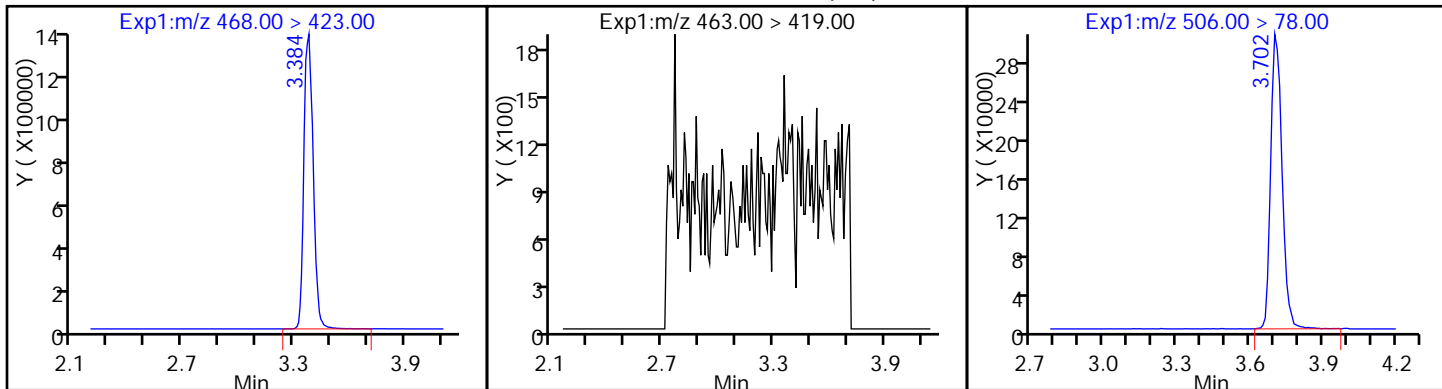

22 Perfluorooctane Sulfonamide (ND)

24 Perfluorodecanoic acid




43 Sodium 1H,1H,2H,2H-perfluorooctane

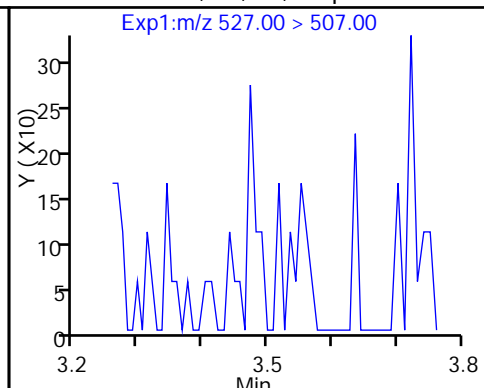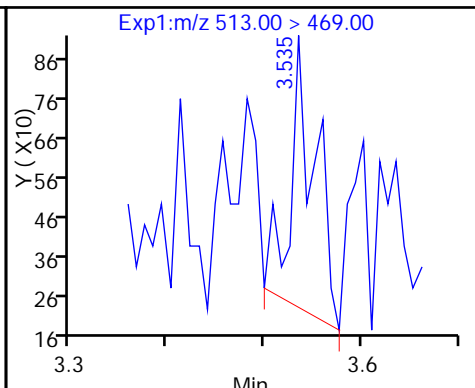

D 23 13C2 PFDA

D 42 M2-8:2FTS




D 45 d3-NMeFOSAA

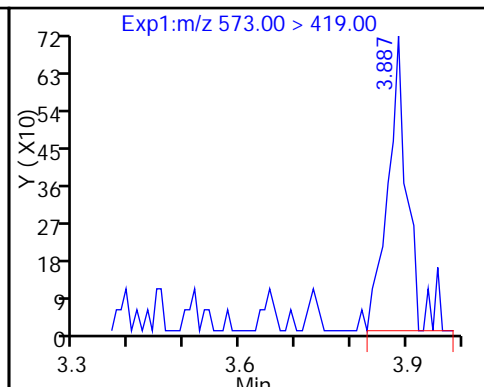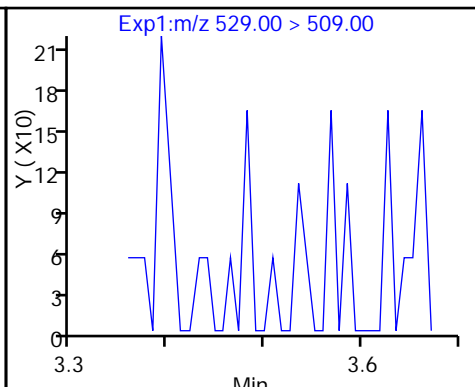

44 N-methyl perfluorooctane sulfonami

26 Perfluorodecanoic acid




28 Perfluoroundecanoic acid

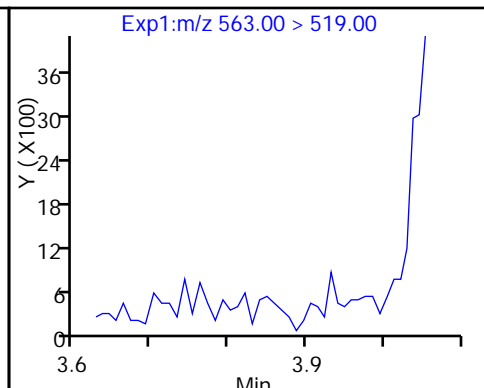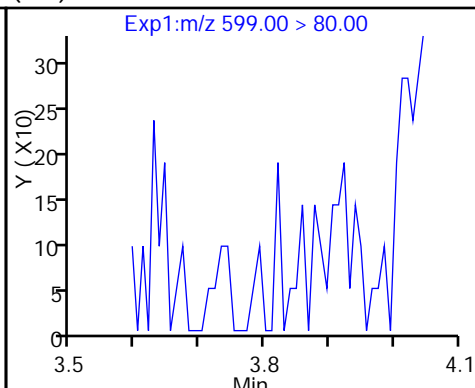


D 27 13C2 PUnA

D 46 d5-NEtFOSAA


49 N-ethyl perfluorooctane sulfonamid

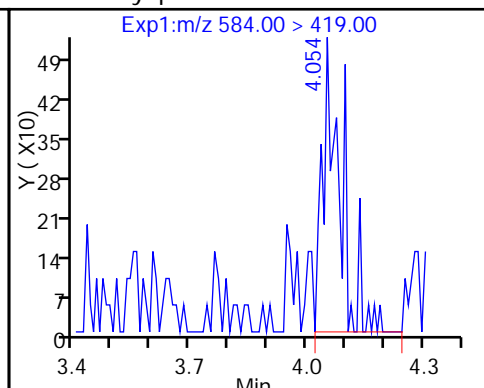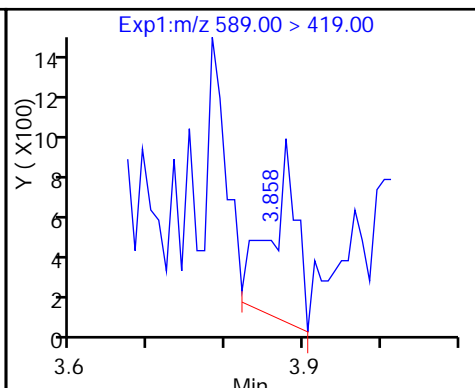


D 52 d-N-MeFOSA-M




54 MeFOSA (ND)




D 30 13C2 PFDaA

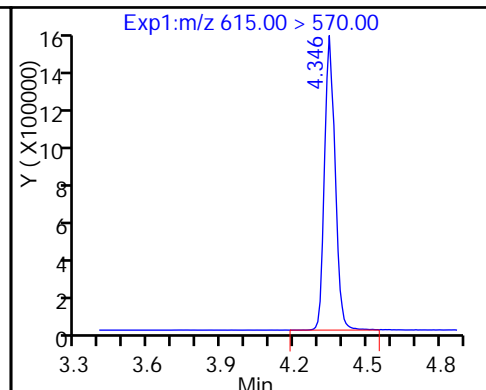


29 Perfluorododecanoic acid (ND)




D 51 d-N-EtFOSA-M (ND)

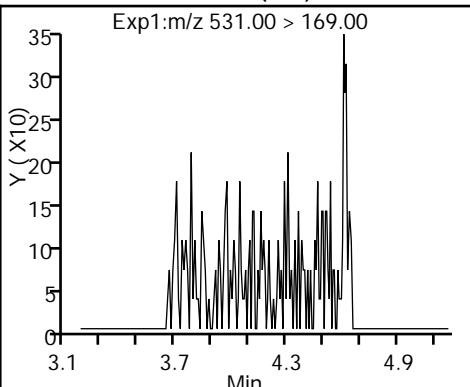


53 N-ethylperfluoro-1-octanesulfonami

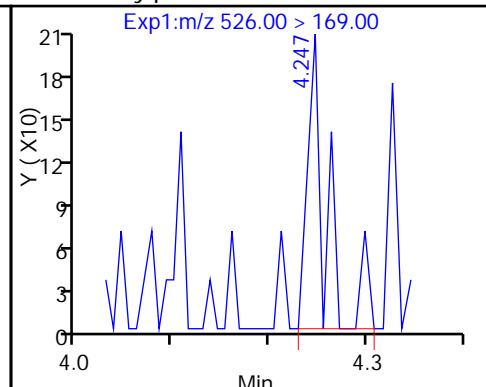


31 Perfluorotridecanoic acid (ND)




D 32 13C2-PFTeDA

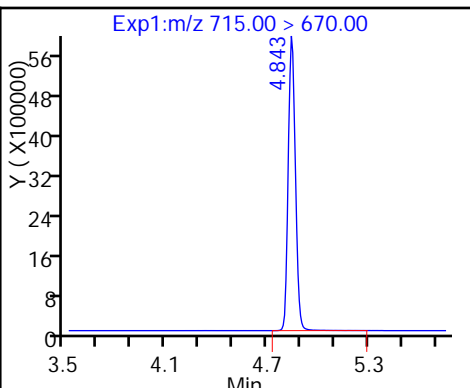


33 Perfluorotetradecanoic acid

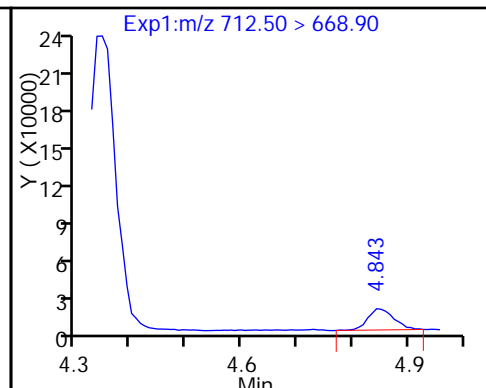


33 Perfluorotetradecanoic acid




D 34 13C2-PFHxDA

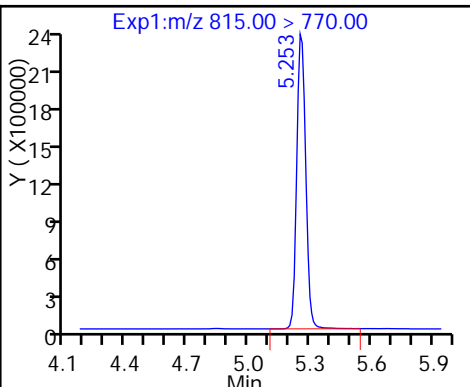

35 Perfluorohexadecanoic acid

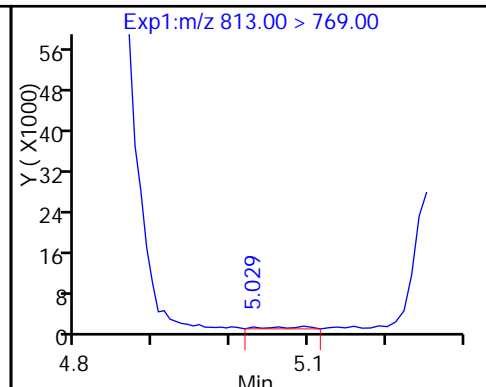

36 Perfluorooctadecanoic acid

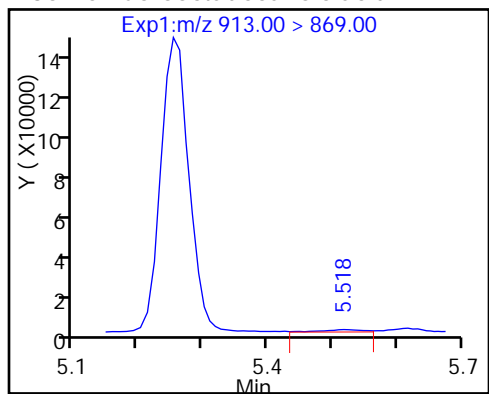

FORM VI
LCMS BY EXTERNAL STANDARD - INITIAL CALIBRATION DATA
RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1 Analy Batch No.: 142379

SDG No.: _____

Instrument ID: A8_N GC Column: Acquity ID: 2.1(mm) Heated Purge: (Y/N) N

Calibration Start Date: 12/15/2016 12:29 Calibration End Date: 12/15/2016 14:18 Calibration ID: 27089

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-142379/4	15DEC2016B_004.d
Level 2	IC 320-142379/13	15DEC2016BE_013.d
Level 3	IC 320-142379/5	15DEC2016B_005.d
Level 4	IC 320-142379/14	15DEC2016B_014.d
Level 5	IC 320-142379/6	15DEC2016B_006.d
Level 6	IC 320-142379/15	15DEC2016B_015.d
Level 7	IC 320-142379/7	15DEC2016B_007.d
Level 8	IC 320-142379/16	15DEC2016B_016.d
Level 9	IC 320-142379/8	15DEC2016B_008.d
Level 10	IC 320-142379/17	15DEC2016B_017.d
Level 11	IC 320-142379/9	15DEC2016B_009.d
Level 12	IC 320-142379/18	15DEC2016B_018.d

ANALYTE	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5	LVL 6	LVL 7	LVL 8	LVL 9	LVL 10	RT WINDOW	AVG RT
	LVL 11	LVL 12										
Perfluorobutanoic acid (PFBA)	1.542 1.537		1.530		1.534		1.534		1.533		1.285 - 1.785	1.535
Perfluoropentanoic acid (PFPeA)	1.810 1.813		1.805		1.810		1.810		1.810		1.560 - 2.060	1.810
Perfluorobutanesulfonic acid (PFBS)	1.849 1.852		1.844		1.849		1.849		1.848		1.668 - 2.028	1.849
Perfluorohexanoic acid (PFHxA)	2.097 2.096		2.092		2.097		2.093		2.098		1.846 - 2.346	2.096
Perfluorohexanesulfonic acid (PFHxS)	++++ 2.444		2.445		2.364		2.440		2.446		2.181 - 2.681	2.428
Perfluoroheptanoic acid (PFHpA)	2.430 2.426		2.430		2.432		2.426		2.424		2.178 - 2.678	2.428
6:2FTS		++++ 2.769		2.761		2.768		2.767		2.767	2.518 - 3.018	2.766
Perfluorooctanoic acid (PFOA)	++++ 2.783		2.781		2.783		2.785		2.782		2.533 - 3.033	2.783
Perfluoroheptanesulfonic Acid (PFHpS)	2.790 2.791		2.789		2.792		2.785		2.791		2.540 - 3.040	2.790
Perfluorooctanesulfonic acid (PFOS)	++++ 2.977		3.149		3.153		3.129		3.151		2.868 - 3.368	3.112
Perfluorononanoic acid (PFNA)	3.159 3.160		3.157		3.153		3.153		3.151		2.905 - 3.405	3.156
Perfluorooctane Sulfonamide (FOSA)	3.490 3.491		3.489		3.492		3.492		3.490		3.241 - 3.741	3.491
Perfluorodecanoic acid (PFDA)	3.515 3.516		3.506		3.509		3.509		3.507		3.260 - 3.760	3.510
8:2FTS		3.511 3.516		3.502		3.511		3.511		3.512	3.261 - 3.761	3.511

FORM VI
LCMS BY EXTERNAL STANDARD - INITIAL CALIBRATION DATA
RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1 Analy Batch No.: 142379

SDG No.: _____

Instrument ID: A8_N GC Column: Acquity ID: 2.1(mm) Heated Purge: (Y/N) N

Calibration Start Date: 12/15/2016 12:29 Calibration End Date: 12/15/2016 14:18 Calibration ID: 27089

ANALYTE	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5	LVL 6	LVL 7	LVL 8	LVL 9	LVL 10	RT WINDOW	AVG RT
	LVL 11	LVL 12										
N-methyl perfluorooctane sulfonamidoacetic acid (NMeFOSAA)		3.684 3.680		3.673		3.683		3.683		3.684	3.431 - 3.931	3.681
Perfluorodecanesulfonic acid (PFDS)	3.826 3.819		3.824		3.819		3.827		3.818		3.572 - 4.072	3.822
Perfluoroundecanoic acid (PFUnA)	3.834 3.845		3.833		3.837		3.844		3.844		3.589 - 4.089	3.840
N-ethyl perfluorooctane sulfonamidoacetic acid (NEtFOSAA)		3.865 3.853		3.855		3.847		3.847		3.857	3.604 - 4.104	3.854
MeFOSA		3.998 4.004		3.997		3.997		3.997		3.999	3.749 - 4.249	3.999
Perfluorododecanoic acid (PFDoA)	4.141 4.136		4.133		4.136		4.135		4.135		3.886 - 4.386	4.136
N-EtFOSA-M		4.187 4.193		4.179		4.186		4.186		4.189	3.937 - 4.437	4.187
Perfluorotridecanoic Acid (PFTriA)	4.404 4.407		4.396		4.398		4.398		4.398		4.150 - 4.650	4.400
Perfluorotetradecanoic acid (PFTeA)	4.643 4.635		4.643		4.645		4.644		4.645		4.392 - 4.892	4.643
Perfluoro-n-hexadecanoic acid (PFHxDA)	++++ 5.060		5.058		5.059		5.059		5.059		4.809 - 5.309	5.059
Perfluoro-n-octadecanoic acid (PFODA)	5.413 5.414		5.413		5.414		5.413		5.413		5.164 - 5.664	5.413
13C4 PFBA	1.534 1.537		1.530		1.534		1.534		1.533		1.284 - 1.784	1.534
13C5 PFPeA	1.810 1.813		1.805		1.810		1.810		1.810		1.560 - 2.060	1.810
13C2 PFHxA	2.097 2.096		2.092		2.097		2.102		2.098		1.847 - 2.347	2.097
13C4-PFHpA	2.430 2.426		2.423		2.425		2.426		2.424		2.176 - 2.676	2.426
18O2 PFHxS	2.452 2.444		2.445		2.447		2.440		2.446		2.196 - 2.696	2.446
M2-6:2FTS		2.760 2.776		2.761		2.768		2.767		2.767	2.517 - 3.017	2.767
13C4 PFOA	2.782 2.783		2.781		2.783		2.785		2.782		2.533 - 3.033	2.783
13C4 PFOS	3.151 3.152		3.149		3.153		3.153		3.151		2.901 - 3.401	3.152
13C5 PFNA	3.159 3.152		3.149		3.153		3.153		3.151		2.903 - 3.403	3.153
13C8 FOSA	3.490 3.491		3.489		3.484		3.484		3.490		3.238 - 3.738	3.488
13C2 PFDA	3.515 3.508		3.514		3.509		3.517		3.516		3.263 - 3.763	3.513

FORM VI
 LCMS BY EXTERNAL STANDARD - INITIAL CALIBRATION DATA
 RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1 Analy Batch No.: 142379

SDG No.: _____

Instrument ID: A8_N GC Column: Acquity ID: 2.1(mm) Heated Purge: (Y/N) N

Calibration Start Date: 12/15/2016 12:29 Calibration End Date: 12/15/2016 14:18 Calibration ID: 27089

ANALYTE	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5	LVL 6	LVL 7	LVL 8	LVL 9	LVL 10	RT WINDOW	AVG RT
	LVL 11	LVL 12										
M2-8:2FTS		3.511 3.516		3.511		3.511		3.511		3.520	3.263 - 3.763	3.513
d3-NMeFOSAA		3.684 3.680		3.673		3.673		3.673		3.675	3.426 - 3.926	3.676
13C2 PFUnA	3.843 3.845		3.842		3.845		3.835		3.844		3.592 - 4.092	3.842
d5-NEtFOSAA		3.848 3.845		3.838		3.838		3.838		3.848	3.592 - 4.092	3.843
d-N-MeFOSA-M		3.988 3.995		3.987		3.987		3.997		3.999	3.742 - 4.242	3.992
13C2 PFDoA	4.134 4.129		4.133		4.129		4.135		4.135		3.882 - 4.382	4.133
d-N-EtFOSA-M		4.180 4.186		4.172		4.179		4.179		4.182	3.930 - 4.430	4.180
13C2-PFTeDA	4.643 4.635		4.633		4.645		4.644		4.645		4.391 - 4.891	4.641
13C2-PFHxDA	5.058 5.060		5.047		5.059		5.059		5.059		4.807 - 5.307	5.057

FORM VI
LCMS BY EXTERNAL STANDARD - INITIAL CALIBRATION DATA
CURVE EVALUATION

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1 Analy Batch No.: 142379

SDG No.: _____

Instrument ID: A8_N GC Column: Acquity ID: 2.1(mm) Heated Purge: (Y/N) N

Calibration Start Date: 12/15/2016 12:29 Calibration End Date: 12/15/2016 14:18 Calibration ID: 27089

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-142379/4	15DEC2016B_004.d
Level 2	IC 320-142379/13	15DEC2016BE_013.d
Level 3	IC 320-142379/5	15DEC2016B_005.d
Level 4	IC 320-142379/14	15DEC2016B_014.d
Level 5	IC 320-142379/6	15DEC2016B_006.d
Level 6	IC 320-142379/15	15DEC2016B_015.d
Level 7	IC 320-142379/7	15DEC2016B_007.d
Level 8	IC 320-142379/16	15DEC2016B_016.d
Level 9	IC 320-142379/8	15DEC2016B_008.d
Level 10	IC 320-142379/17	15DEC2016B_017.d
Level 11	IC 320-142379/9	15DEC2016B_009.d
Level 12	IC 320-142379/18	15DEC2016B_018.d

ANALYTE	CF				CURVE TYPE	COEFFICIENT			#	MIN CF	%RSD	#	MAX %RSD	R^2 OR COD	#	MIN R^2 OR COD
	LVL 1	LVL 2	LVL 3	LVL 4		B	M1	M2								
	LVL 5	LVL 6	LVL 7	LVL 8												
13C4 PFBA	365277 360742 345484		364028 351708 299221		Ave		347743.167			7.2		50.0				
13C5 PFPeA	282426 281261 261073		281354 272343 217976		Ave		266072.353			9.4		50.0				
13C2 PFHxA	253106 254198 247986		256296 252164 206910		Ave		245109.910			7.7		50.0				
13C4-PFHpA	244814 245211 216032		244964 235764 171281		Ave		226344.393			12.9		50.0				
18O2 PFHxS	341723 342975 323020		340234 339593 274309		Ave		326975.747			8.2		50.0				
M2-6:2FTS		112694 117279 110718		107543 136249 117410	Ave		116982.140			8.7		50.0				
13C4 PFOA	250090 252701 222856		252554 236364 167605		Ave		230361.637			14.3		50.0				

Note: The m1 coefficient is the same as Ave CF for an Ave curve type.

FORM VI
LCMS BY EXTERNAL STANDARD - INITIAL CALIBRATION DATA
CURVE EVALUATION

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1 Analy Batch No.: 142379

SDG No.: _____

Instrument ID: A8_N GC Column: Acquity ID: 2.1(mm) Heated Purge: (Y/N) N

Calibration Start Date: 12/15/2016 12:29 Calibration End Date: 12/15/2016 14:18 Calibration ID: 27089

ANALYTE	CF				CURVE TYPE	COEFFICIENT			#	MIN CF	%RSD	#	MAX %RSD	R^2 OR COD	#	MIN R^2 OR COD
	LVL 1 LVL 5 LVL 9	LVL 2 LVL 6 LVL 10	LVL 3 LVL 7 LVL 11	LVL 4 LVL 8 LVL 12		B	M1	M2								
13C4 PFOS	256822 261188 249930		260657 254876 209612		Ave		248847.249			7.9		50.0				
13C5 PFNA	189110 195552 171630		190741 184721 134367		Ave		177686.923			12.8		50.0				
13C8 FOSA	407109 400699 376084		404776 394065 322114		Ave		384141.077			8.4		50.0				
13C2 PFDA	168454 164694 153437		169609 162695 124922		Ave		157301.833			10.7		50.0				
M2-8:2FTS		100584 111541 99917		96024 124933 111666	Ave		107444.339			10.0		50.0				
d3-NMeFOSAA		72700 80292 68450		71182 87583 71744	Ave		75324.9433			9.6		50.0				
13C2 PFUnA	127043 125252 113156		124385 124531 89132		Ave		117249.927			12.5		50.0				
d5-NEtFOSAA		77796 84707 69727		75140 88209 74518	Ave		78349.4833			8.8		50.0				
d-N-MeFOSA-M		86501 102439 90246		92791 105280 93163	Ave		95069.8233			7.6		50.0				
13C2 PFDoA	116302 115598 108083		116442 116336 92982		Ave		110957.213			8.5		50.0				
d-N-EtFOSA-M		75857 91238 82985		82198 93456 88971	Ave		85784.0067			7.7		50.0				
13C2-PFTEdA	239125 244965 219010		237709 233101 190415		Ave		227387.480			8.8		50.0				
13C2-PFHxDA	131492 130859 120547		133987 126716 103803		Ave		124567.543			9.0		50.0				

Note: The m1 coefficient is the same as Ave CF for an Ave curve type.

FORM VI

CURVE EVALUATION

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1 Analy Batch No.: 142379
 SDG No.: _____
 Instrument ID: A8_N GC Column: Acquity ID: 2.1 (mm) Heated Purge: (Y/N) N
 Calibration Start Date: 12/15/2016 12:29 Calibration End Date: 12/15/2016 14:18 Calibration ID: 27089

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD	#	MAX %RSD	R^2 OR COD	#	MIN R^2 OR COD
	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
	LVL 6 LVL 11	LVL 7 LVL 12	LVL 8	LVL 9	LVL 10												
Perfluorobutanoic acid (PFBA)	310962 213818	334546	310647	308231	310088	AveID	0.8537				9.1		35.0				
Perfluoropentanoic acid (PFPeA)	304642 171455	288512	287573	263221	271648	AveID	0.9868				10.7		35.0				
Perfluorobutanesulfonic acid (PFBS)	490041 286903	557732	479895	487779	500362	AveID	1.4170				14.1		50.0				
Perfluorohexanoic acid (PFHxA)	252858 166120	246488	239458	230141	236657	AveID	0.9288				7.3		35.0				
Perfluorohexanesulfonic acid (PFHxS)	++++ 253974	363991	382940	335246	339121	AveID	1.0300				7.4		35.0				
Perfluoroheptanoic acid (PFHpA)	258208 151171	237386	237734	215989	235022	AveID	0.9788				5.9		35.0				
6:2FTS	85456	++++ 89174	127446	112813	109001	AveID	0.8914				15.8		35.0				
Perfluorooctanoic acid (PFOA)	++++ 153922	255488	254861	228712	247908	AveID	1.0031				6.0		35.0				
Perfluoroheptanesulfonic Acid (PFHpS)	283576 201995	315862	279184	286553	283857	AveID	1.1019				8.2		50.0				
Perfluorooctanesulfonic acid (PFOS)	++++ 215911	272566	237468	253058	247933	AveID	0.9945				6.4		35.0				
Perfluorononanoic acid (PFNA)	180132 123966	178149	188341	164925	180502	AveID	0.9518				2.7		35.0				
Perfluorooctane Sulfonamide (FOSA)	391498 239019	399542	381363	354739	397863	AveID	0.9327				10.5		35.0				

Note: The m1 coefficient is the same as Ave RRF for an Ave curve type.

CURVE EVALUATION

Lab Name: TestAmerica SacramentoJob No.: 320-24118-1Analy Batch No.: 142379

SDG No.: _____

Instrument ID: A8_NGC Column: Acquity ID: 2.1(mm)Heated Purge: (Y/N) NCalibration Start Date: 12/15/2016 12:29Calibration End Date: 12/15/2016 14:18Calibration ID: 27089

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD	#	MAX %RSD	R^2 OR COD	#	MIN R^2 OR COD
	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
	LVL 6	LVL 7	LVL 8	LVL 9	LVL 10												
Perfluorodecanoic acid (PFDA)	164274 113084	158337	155537	146490	154381	AveID	0.9438				3.1		35.0				
8:2FTS	83185	83106 84092	116095	79051	100536	AveID	0.8473				12.1		35.0				
N-methyl perfluorooctane sulfonamidoacetic acid (NMeFOSAA)	57133	59646 64621	85412	57389	74839	AveID	0.8846				15.4		35.0				
Perfluorodecanesulfonic acid (PFDS)	143714 124235	159960	145051	150246	147895	AveID	0.5840				4.8		50.0				
Perfluoroundecanoic acid (PFUnA)	130000 84265	121036	119189	108755	109942	AveID	0.9563				4.9		35.0				
N-ethyl perfluorooctane sulfonamidoacetic acid (NEtFOSAA)	53544	59930 59690	75946	53623	68286	AveID	0.7929				15.1		35.0				
MeFOSA	68699	72138 80570	97349	70049	88147	AveID	0.8376				13.3		35.0				
Perfluorododecanoic acid (PFDoA)	105614 87129	111590	103481	101460	101274	AveID	0.9180				3.5		35.0				
N-EtFOSA-M	65375	61986 78901	90659	62962	85286	AveID	0.8640				13.9		35.0				
Perfluorotridecanoic Acid (PFTriA)	106640 80194	104393	109461	99013	105018	AveID	0.9069				2.9		50.0				
Perfluorotetradecanoic acid (PFTeA)	197042 136554	183949	187123	172910	180115	AveID	1.5848				4.6		50.0				
Perfluoro-n-hexadecanoic acid (PFHxDA)	++++ 88775	113395	173261	106364	119906	L1ID	0.5185	0.9555						1.0000		0.9900	
Perfluoro-n-octadecanoic acid (PFODA)	123098 91965	122262	114997	117393	116752	AveID	1.0304				3.9		50.0				

Note: The m1 coefficient is the same as Ave RRF for an Ave curve type.

FORM VI
LCMS BY EXTERNAL STANDARD - INITIAL CALIBRATION DATA
RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1 Analy Batch No.: 142379

SDG No.: _____

Instrument ID: A8_N GC Column: Acquity ID: 2.1(mm) Heated Purge: (Y/N) N

Calibration Start Date: 12/15/2016 12:29 Calibration End Date: 12/15/2016 14:18 Calibration ID: 27089

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-142379/4	15DEC2016B_004.d
Level 2	IC 320-142379/13	15DEC2016BE_013.d
Level 3	IC 320-142379/5	15DEC2016B_005.d
Level 4	IC 320-142379/14	15DEC2016B_014.d
Level 5	IC 320-142379/6	15DEC2016B_006.d
Level 6	IC 320-142379/15	15DEC2016B_015.d
Level 7	IC 320-142379/7	15DEC2016B_007.d
Level 8	IC 320-142379/16	15DEC2016B_016.d
Level 9	IC 320-142379/8	15DEC2016B_008.d
Level 10	IC 320-142379/17	15DEC2016B_017.d
Level 11	IC 320-142379/9	15DEC2016B_009.d
Level 12	IC 320-142379/18	15DEC2016B_018.d

ANALYTE	CURVE TYPE	RESPONSE					CONCENTRATION (NG/ML)				
		LVL 1	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5
		LVL 6	LVL 7	LVL 8	LVL 9	LVL 10	LVL 6	LVL 7	LVL 8	LVL 9	LVL 10
13C4 PFBA	Ave	18263829	17585378	18201393	17274187	18037108	50.0	50.0	50.0	50.0	50.0
		14961055					50.0				
13C5 PFPeA	Ave	14121285	13617158	14067714	13053659	14063070	50.0	50.0	50.0	50.0	50.0
		10898820					50.0				
13C2 PFHxA	Ave	12655304	12608210	12814780	12399280	12709919	50.0	50.0	50.0	50.0	50.0
		10345480					50.0				
13C4-PFHpA	Ave	12240718	11788221	12248222	10801604	12260528	50.0	50.0	50.0	50.0	50.0
		8564025					50.0				
1802 PFHxS	Ave	16163510	16062766	16093048	15278828	16222736	47.3	47.3	47.3	47.3	47.3
		12974829					47.3				
M2-6:2FTS	Ave	5570739	5352965	6471813	5108306	5259120	47.5	47.5	47.5	47.5	47.5
			5576967					47.5			
13C4 PFOA	Ave	12504504	11818203	12627691	11142777	12635065	50.0	50.0	50.0	50.0	50.0
		8380251					50.0				
13C4 PFOS	Ave	12276070	12183062	12459383	11946650	12484772	47.8	47.8	47.8	47.8	47.8
		10019454					47.8				

FORM VI
LCMS BY EXTERNAL STANDARD - INITIAL CALIBRATION DATA
RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1 Analy Batch No.: 142379

SDG No.: _____

Instrument ID: A8_N GC Column: Acquity ID: 2.1(mm) Heated Purge: (Y/N) N

Calibration Start Date: 12/15/2016 12:29 Calibration End Date: 12/15/2016 14:18 Calibration ID: 27089

ANALYTE	CURVE TYPE	RESPONSE					CONCENTRATION (NG/ML)				
		LVL 1 LVL 6 LVL 11	LVL 2 LVL 7 LVL 12	LVL 3 LVL 8	LVL 4 LVL 9	LVL 5 LVL 10	LVL 1 LVL 6 LVL 11	LVL 2 LVL 7 LVL 12	LVL 3 LVL 8	LVL 4 LVL 9	LVL 5 LVL 10
13C5 PFNA	Ave	9455492 6718354	9236073	9537045	8581504	9777609	50.0 50.0	50.0	50.0	50.0	50.0
13C8 FOSA	Ave	20355431 16105707	19703272	20238792	18804188	20034933	50.0 50.0	50.0	50.0	50.0	50.0
13C2 PFDA	Ave	8422718 6246112	8134734	8480447	7671861	8234678	50.0 50.0	50.0	50.0	50.0	50.0
M2-8:2FTS	Ave	5342826	4817997 5348797	5984276	4599569	4786038	47.9	47.9 47.9	47.9	47.9	47.9
d3-NMeFOSAA	Ave	4014623	3634985 3587176	4379131	3559083	3422485	50.0	50.0 50.0	50.0	50.0	50.0
13C2 PFUnA	Ave	6352135 4456593	6226562	6219248	5657823	6262617	50.0 50.0	50.0	50.0	50.0	50.0
d5-NEtFOSAA	Ave	4235352	3889792 3725902	4410456	3757014	3486329	50.0	50.0 50.0	50.0	50.0	50.0
d-N-MeFOSA-M	Ave	5121953	4325034 4658153	5263980	4639527	4512300	50.0	50.0 50.0	50.0	50.0	50.0
13C2 PFDoA	Ave	5815120 4649092	5816809	5822114	5404154	5779875	50.0 50.0	50.0	50.0	50.0	50.0
d-N-EtFOSA-M	Ave	4561882	3792851 4448546	4672820	4109875	4149228	50.0	50.0 50.0	50.0	50.0	50.0
13C2-PFTeDA	Ave	11956257 9520749	11655048	11885446	10950502	12248242	50.0 50.0	50.0	50.0	50.0	50.0
13C2-PFHxDA	Ave	6574607 5190172	6335821	6699329	6027362	6542972	50.0 50.0	50.0	50.0	50.0	50.0

Curve Type Legend:

Ave = Average

RESPONSE AND CONCENTRATION

Lab Name: TestAmerica SacramentoJob No.: 320-24118-1Analy Batch No.: 142379

SDG No.: _____

Instrument ID: A8_NGC Column: Acquity ID: 2.1(mm)Heated Purge: (Y/N) NCalibration Start Date: 12/15/2016 12:29Calibration End Date: 12/15/2016 14:18Calibration ID: 27089

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-142379/4	15DEC2016B_004.d
Level 2	IC 320-142379/13	15DEC2016BE_013.d
Level 3	IC 320-142379/5	15DEC2016B_005.d
Level 4	IC 320-142379/14	15DEC2016B_014.d
Level 5	IC 320-142379/6	15DEC2016B_006.d
Level 6	IC 320-142379/15	15DEC2016B_015.d
Level 7	IC 320-142379/7	15DEC2016B_007.d
Level 8	IC 320-142379/16	15DEC2016B_016.d
Level 9	IC 320-142379/8	15DEC2016B_008.d
Level 10	IC 320-142379/17	15DEC2016B_017.d
Level 11	IC 320-142379/9	15DEC2016B_009.d
Level 12	IC 320-142379/18	15DEC2016B_018.d

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (NG/ML)				
			LVL 1	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5
			LVL 6	LVL 7	LVL 8	LVL 9	LVL 10	LVL 6	LVL 7	LVL 8	LVL 9	LVL 10
Perfluorobutanoic acid (PFBA)		AveID	155481	6690917	310647	15411527	1550440	0.500	20.0	1.00	50.0	5.00
			42763611					200				
Perfluoropentanoic acid (PFPeA)		AveID	152321	5770240	287573	13161065	1358239	0.500	20.0	1.00	50.0	5.00
			34291076					200				
Perfluorobutanesulfonic acid (PFBS)		AveID	216598	9860707	424227	21559838	2211602	0.442	17.7	0.884	44.2	4.42
			50724469					177				
Perfluorohexanoic acid (PFHxA)		AveID	126429	4929766	239458	11507044	1183286	0.500	20.0	1.00	50.0	5.00
			33223923					200				
Perfluorohexanesulfonic acid (PFHxS)		AveID	+++++	6624638	348475	15253691	1543002	+++++	18.2	0.910	45.5	4.55
			46223186					182				
Perfluoroheptanoic acid (PFHpA)		AveID	129104	4747711	237734	10799449	1175112	0.500	20.0	1.00	50.0	5.00
			30234194					200				
6:2FTS		AveID	405060	+++++	2416384	106947	5166665	4.74	+++++	19.0	0.948	47.4
			16907459	190								
Perfluorooctanoic acid (PFOA)		AveID	+++++	5109766	254861	11435583	1239541	+++++	20.0	1.00	50.0	5.00
			30784387					200				

RESPONSE AND CONCENTRATION

Lab Name: TestAmerica SacramentoJob No.: 320-24118-1Analy Batch No.: 142379

SDG No.: _____

Instrument ID: A8_NGC Column: AcquityID: 2.1(mm)Heated Purge: (Y/N) NCalibration Start Date: 12/15/2016 12:29Calibration End Date: 12/15/2016 14:18Calibration ID: 27089

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (NG/ML)				
			LVL 1	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5
			LVL 6	LVL 7	LVL 8	LVL 9	LVL 10	LVL 6	LVL 7	LVL 8	LVL 9	LVL 10
Perfluoroheptanesulfonic Acid (PFHpS)		AveID	134982 38459925	6014021	265783	13639927	1351160	0.476 190	19.0	0.952	47.6	4.76
Perfluorooctanesulfonic acid (PFOS)		AveID	++++ 40073141	5058824	220370	11741891	1150410	++++ 186	18.6	0.928	46.4	4.64
Perfluorononanoic acid (PFNA)		AveID	90066 24793148	3562981	188341	8246252	902512	0.500 200	20.0	1.00	50.0	5.00
Perfluorooctane Sulfonamide (FOSA)		AveID	195749 47803717	7990835	381363	17736944	1989314	0.500 200	20.0	1.00	50.0	5.00
Perfluorodecanoic acid (PFDA)		AveID	82137 22616781	3166735	155537	7324495	771905	0.500 200	20.0	1.00	50.0	5.00
8:2FTS		AveID	398457	39808 16111959	2224381	75731	4815680	4.79 192	0.479	19.2	0.958	47.9
N-methyl perfluorooctane sulfonamidoacetic acid (NMeFOSAA)		AveID	285665	29823 12924122	1708231	57389	3741936	5.00 200	0.500	20.0	1.00	50.0
Perfluorodecanesulfonic acid (PFDS)		AveID	69270 23952412	3084031	139829	7241868	712852	0.482 193	19.3	0.964	48.2	4.82
Perfluoroundecanoic acid (PFUnA)		AveID	65000 16852945	2420719	119189	5437764	549708	0.500 200	20.0	1.00	50.0	5.00
N-ethyl perfluorooctane sulfonamidoacetic acid (NEtFOSAA)		AveID	267721	29965 11938061	1518918	53623	3414301	5.00 200	0.500	20.0	1.00	50.0
MeFOSA		AveID	343493	36069 16114020	1946985	70049	4407328	5.00 200	0.500	20.0	1.00	50.0
Perfluorododecanoic acid (PFDoA)		AveID	52807 17425873	2231794	103481	5072994	506369	0.500 200	20.0	1.00	50.0	5.00
N-EtFOSA-M		AveID	326877	30993 15780196	1813178	62962	4264314	5.00 200	0.500	20.0	1.00	50.0

RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1 Analy Batch No.: 142379

SDG No.: _____

Instrument ID: A8_N GC Column: Acquity ID: 2.1(mm) Heated Purge: (Y/N) N

Calibration Start Date: 12/15/2016 12:29 Calibration End Date: 12/15/2016 14:18 Calibration ID: 27089

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (NG/ML)				
			LVL 1	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5
			LVL 6	LVL 7	LVL 8	LVL 9	LVL 10	LVL 6	LVL 7	LVL 8	LVL 9	LVL 10
Perfluorotridecanoic Acid (PFTriA)		AveID	53320	2087859	109461	4950651	525090	0.500	20.0	1.00	50.0	5.00
			16038809					200				
Perfluorotetradecanoic acid (PFTeA)		AveID	98521	3678976	187123	8645519	900575	0.500	20.0	1.00	50.0	5.00
			27310864					200				
Perfluoro-n-hexadecanoic acid (PFHxDA)		L1ID	++++	2267892	173261	5318207	599529	++++	20.0	1.00	50.0	5.00
			17754908					200				
Perfluoro-n-octadecanoic acid (PFODA)		AveID	61549	2445236	114997	5869666	583761	0.500	20.0	1.00	50.0	5.00
			18392980					200				

Curve Type Legend:

AveID = Average isotope dilution
L1ID = Linear 1/conc IsoDil

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_004.d
 Lims ID: IC L1
 Client ID:
 Sample Type: IC Calib Level: 1
 Inject. Date: 15-Dec-2016 12:29:18 ALS Bottle#: 37 Worklist Smp#: 4
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L1_b
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Sublist: chrom-A8_N*sub6
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 14:34:11 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d

Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 15-Dec-2016 13:48:59

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.534	1.534	0.0	18263829	52.5		105	1469089	
1 Perfluorobutyric acid	212.90 > 169.00	1.542	1.535	0.007	155481	0.4986		99.7	1121	
D 4 13C5-PFPeA	267.90 > 223.00	1.810	1.810	0.0	14121285	53.1		106	1079323	
3 Perfluoropentanoic acid	262.90 > 219.00	1.810	1.810	0.0	152321	0.5465		109	1332	
5 Perfluorobutanesulfonic acid	298.90 > 80.00	1.849	1.848	0.001	216598	0.4473		101		
	298.90 > 99.00	1.849	1.848	0.001	87630		2.47(0.00-0.00)	101		
7 Perfluorohexanoic acid	313.00 > 269.00	2.097	2.096	0.001	126429	0.5378		108	4416	
D 6 13C2 PFHxA	315.00 > 270.00	2.097	2.097	0.0	12655304	51.6		103	589404	
D 11 13C4-PFHpA	367.00 > 322.00	2.430	2.426	0.004	12240718	54.1		108	647338	
12 Perfluoroheptanoic acid	363.00 > 319.00	2.430	2.428	0.002	129104	0.5388		108	1246	M
9 Perfluorohexanesulfonic acid	399.00 > 80.00	2.444	2.431	0.013	204063	0.5798		127		M
D 10 18O2 PFHxS	403.00 > 84.00	2.452	2.446	0.006	16163510	49.4		105	1405328	
D 14 13C4 PFOA	417.00 > 372.00	2.782	2.783	-0.001	12504504	54.3		109	532215	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
15 Perfluorooctanoic acid										
413.00 > 369.00	2.782	2.783	-0.001	1.000	145696	0.5807		116	1257	
413.00 > 169.00	2.790	2.783	0.007	1.003	87089		1.67(0.90-1.10)	116	4416	
13 Perfluoroheptanesulfonic Acid										
449.00 > 80.00	2.790	2.790	0.0	1.000	134982	0.4770		100		
18 Perfluorooctane sulfonic acid										
499.00 > 80.00	3.151	3.118	0.033	1.000	116569	0.4564		98.4	7996	M
499.00 > 99.00	3.159	3.118	0.041	1.003	24244		4.81(0.90-1.10)	98.4	1329	M
D 17 13C4 PFOS										
503.00 > 80.00	3.151	3.151	0.0		12276070	49.3		103	1128009	
D 19 13C5 PFNA										
468.00 > 423.00	3.159	3.153	0.006		9455492	53.2		106	520740	
20 Perfluorononanoic acid										
463.00 > 419.00	3.159	3.155	0.004	1.000	90066	0.5004		100	1349	
D 21 13C8 FOSA										
506.00 > 78.00	3.490	3.488	0.002		20355431	53.0		106	727464	
22 Perfluorooctane Sulfonamide										
498.00 > 78.00	3.490	3.491	-0.001	1.000	195749	0.5155		103	25454	
24 Perfluorodecanoic acid										
513.00 > 469.00	3.515	3.510	0.005	1.000	82137	0.5166		103	2772	
D 23 13C2 PFDA										
515.00 > 470.00	3.515	3.513	0.002		8422718	53.5		107	284895	
26 Perfluorodecane Sulfonic acid										
599.00 > 80.00	3.826	3.822	0.004	1.000	69270	0.4619		95.8		
28 Perfluoroundecanoic acid										
563.00 > 519.00	3.834	3.839	-0.005	1.000	65000	0.5350		107	1918	
D 27 13C2 PFUnA										
565.00 > 520.00	3.843	3.842	0.001		6352135	54.2		108	398643	
D 30 13C2 PFDoA										
615.00 > 570.00	4.134	4.132	0.002		5815120	52.4		105	205155	
29 Perfluorododecanoic acid										
613.00 > 569.00	4.141	4.136	0.005	1.000	52807	0.4946		98.9	1204	M
31 Perfluorotridecanoic acid										
663.00 > 619.00	4.404	4.400	0.004	1.000	53320	0.5055		101	1256	
D 32 13C2-PFTeDA										
715.00 > 670.00	4.643	4.641	0.002		11956257	52.6		105	663687	
33 Perfluorotetradecanoic acid										
712.50 > 668.90	4.643	4.642	0.001	1.000	98521	0.5345		107	1284	
713.00 > 169.00	4.633	4.642	-0.009	0.998	17902		5.50(0.00-0.00)	107	7022	
D 34 13C2-PFHxDA										
815.00 > 770.00	5.058	5.057	0.001		6574607	52.8		106	132486	
35 Perfluorohexadecanoic acid										
813.00 > 769.00	5.058	5.059	-0.001	1.000	125860	0.5899		118	92.5	
36 Perfluorooctadecanoic acid										
913.00 > 869.00	5.413	5.414	-0.001	1.000	61549	0.5136		103	54.0	

QC Flag Legend

Review Flags

M - Manually Integrated

Reagents:

LCPFC-L1_00022

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_004.d

Injection Date: 15-Dec-2016 12:29:18

Instrument ID: A8_N

Lims ID: IC L1

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 37

Worklist Smp#: 4

Injection Vol: 2.0 ul

Dil. Factor: 1.0000













Method: A8_N

Limit Group: LC PFC_DOD ICAL


D 2 13C4 PFBA

1 Perfluorobutyric acid


D 4 13C5-PFPeA

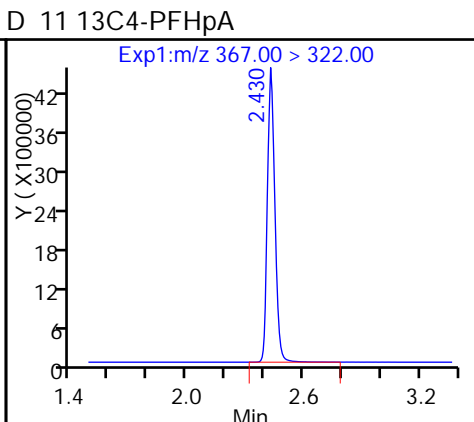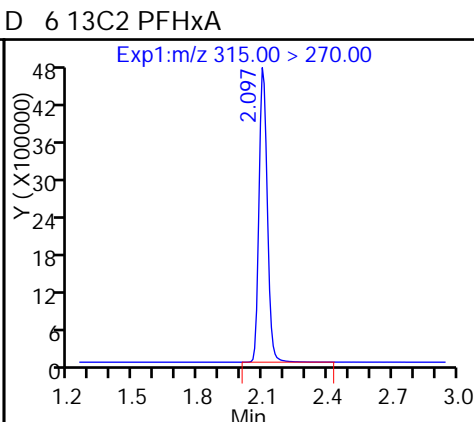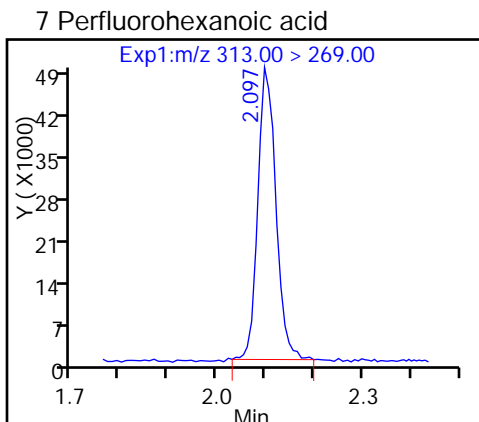


D 14 13C4 PFOA




15 Perfluorooctanoic acid




15 Perfluorooctanoic acid

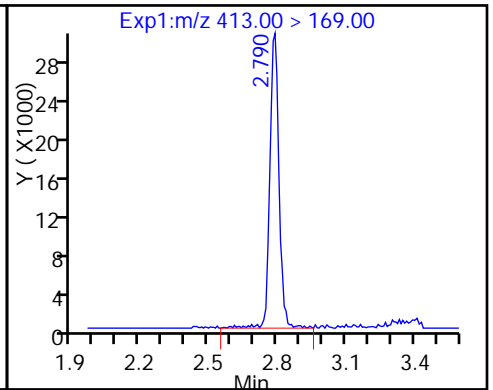


13 Perfluoroheptanesulfonic Acid

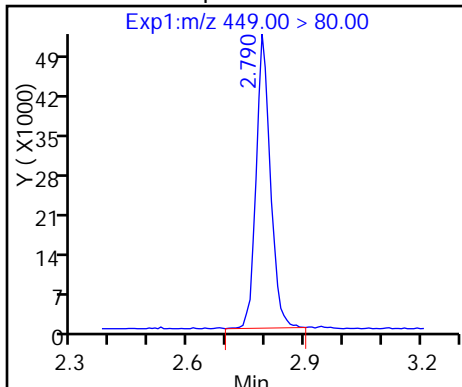


18 Perfluorooctane sulfonic acid (M)

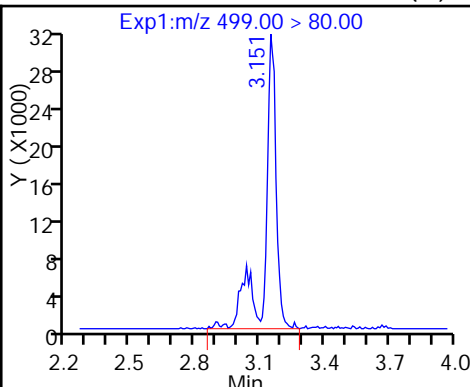


18 Perfluorooctane sulfonic acid (M)

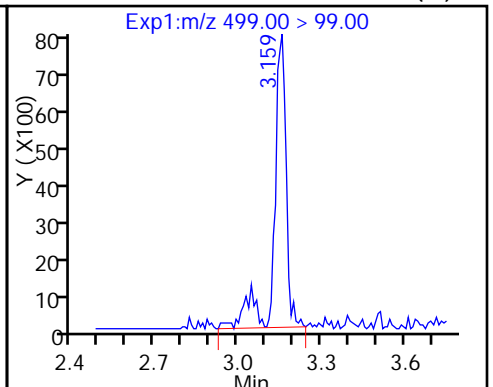


D 17 13C4 PFOS




D 19 13C5 PFNA

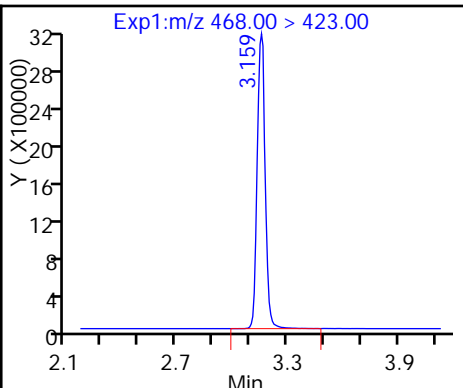


20 Perfluorononanoic acid

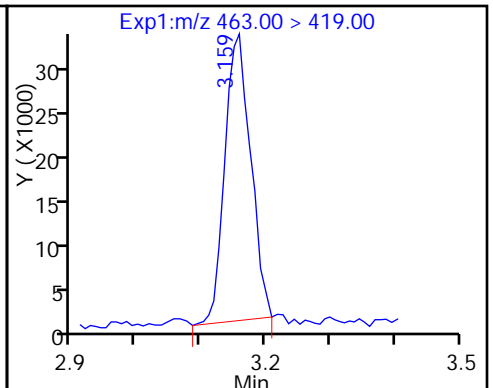


D 21 13C8 FOSA




22 Perfluorooctane Sulfonamide

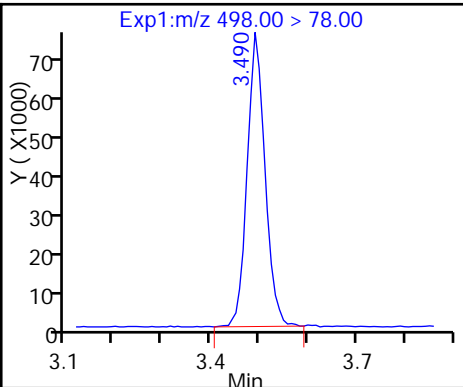


24 Perfluorodecanoic acid

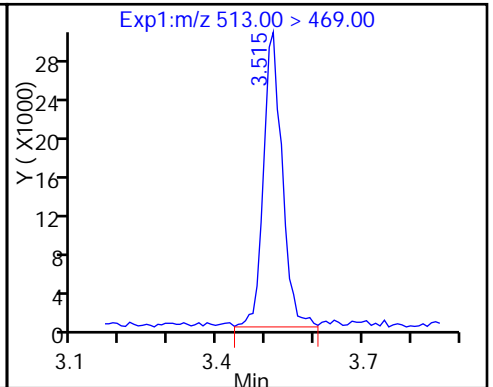


D 23 13C2 PFDA




26 Perfluorodecane Sulfonic acid

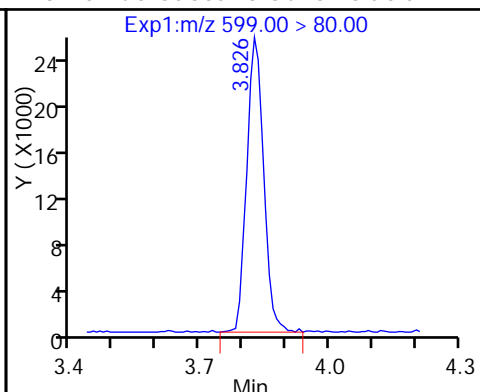


28 Perfluoroundecanoic acid




D 27 13C2 PFUa




D 30 13C2 PFDa




29 Perfluorododecanoic acid (M)




31 Perfluorotridecanoic acid




D 32 13C2-PFTeDA




33 Perfluorotetradecanoic acid




33 Perfluorotetradecanoic acid




D 34 13C2-PFHxDA



35 Perfluorohexadecanoic acid



36 Perfluorooctadecanoic acid

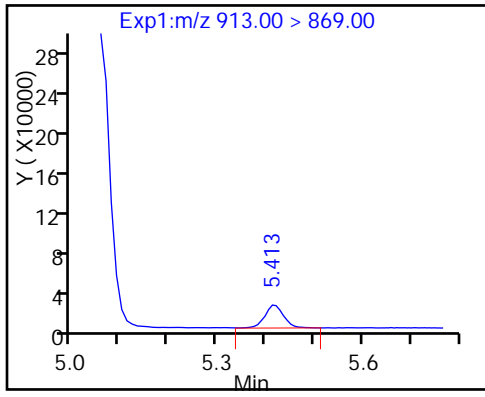

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_004.d
Injection Date: 15-Dec-2016 12:29:18 Instrument ID: A8_N
Lims ID: IC L1
Client ID:
Operator ID: A8-PC\A8 ALS Bottle#: 37 Worklist Smp#: 4
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL
Column: Detector EXP1

12 Perfluoroheptanoic acid, CAS: 375-85-9

Signal: 1


Not Detected
Expected RT: 2.43

Processing Integration Results

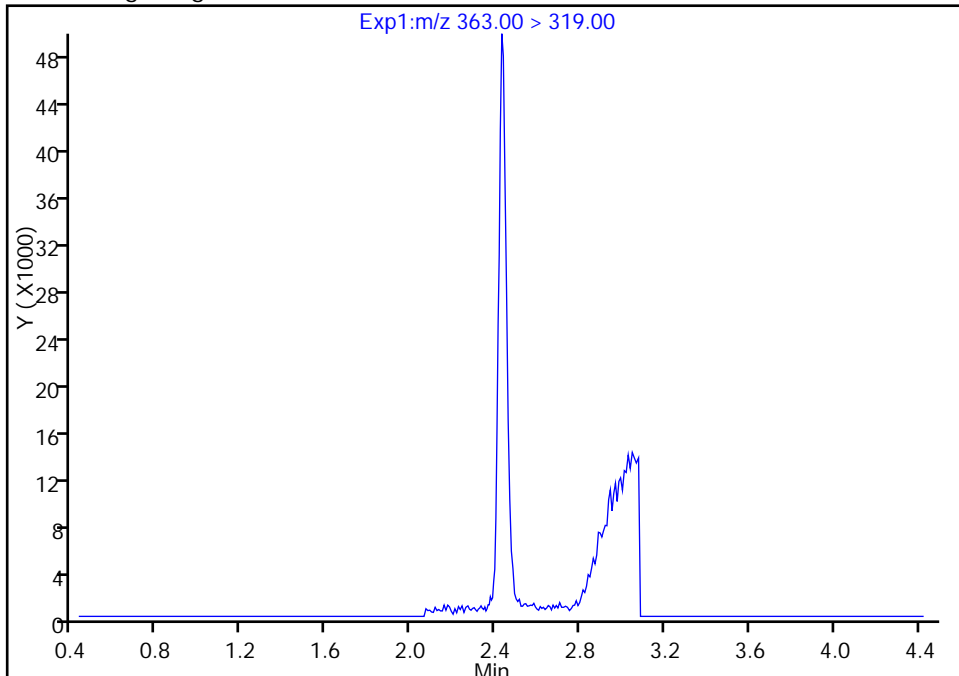

RT: 2.43
Area: 129104
Amount: 0.538766
Amount Units: ng/ml

Manual Integration Results

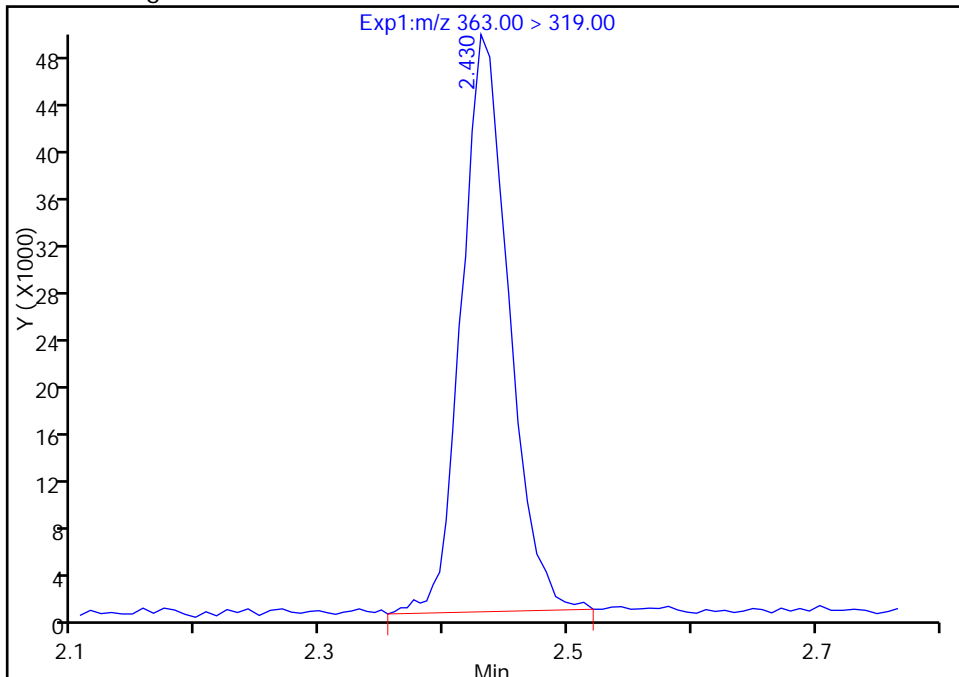

Reviewer: chandrasenas, 15-Dec-2016 13:48:59
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_004.d
Injection Date: 15-Dec-2016 12:29:18 Instrument ID: A8_N
Lims ID: IC L1
Client ID:
Operator ID: A8-PC\A8 ALS Bottle#: 37 Worklist Smp#: 4
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL
Column: Detector EXP1

9 Perfluorohexanesulfonic acid, CAS: 355-46-4


Signal: 1

Not Detected
Expected RT: 2.43

Processing Integration Results

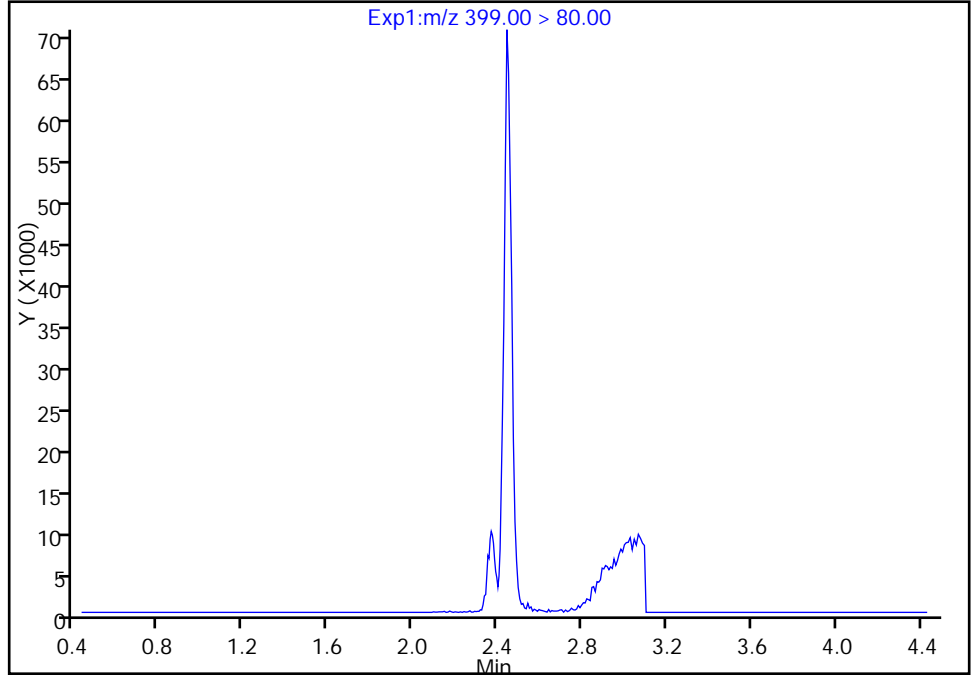

Manual Integration Results

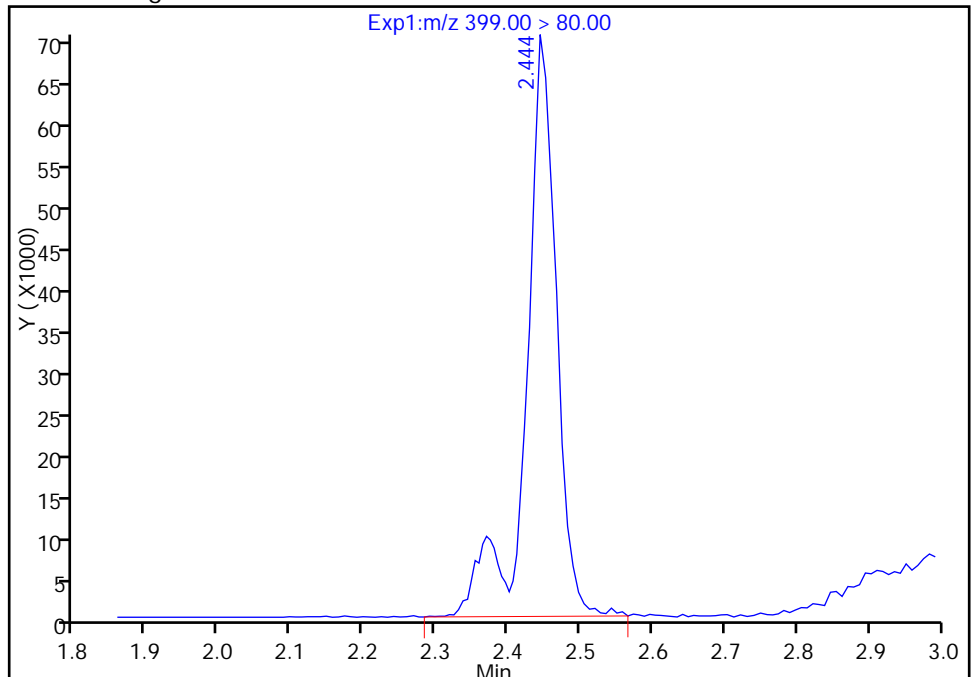

RT: 2.44
Area: 204063
Amount: 0.579783
Amount Units: ng/ml

Reviewer: chandrasenas, 15-Dec-2016 13:48:59
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_004.d
Injection Date: 15-Dec-2016 12:29:18 Instrument ID: A8_N
Lims ID: IC L1
Client ID:
Operator ID: A8-PC\A8 ALS Bottle#: 37 Worklist Smp#: 4
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL
Column: Detector EXP1

18 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 3.12

Processing Integration Results

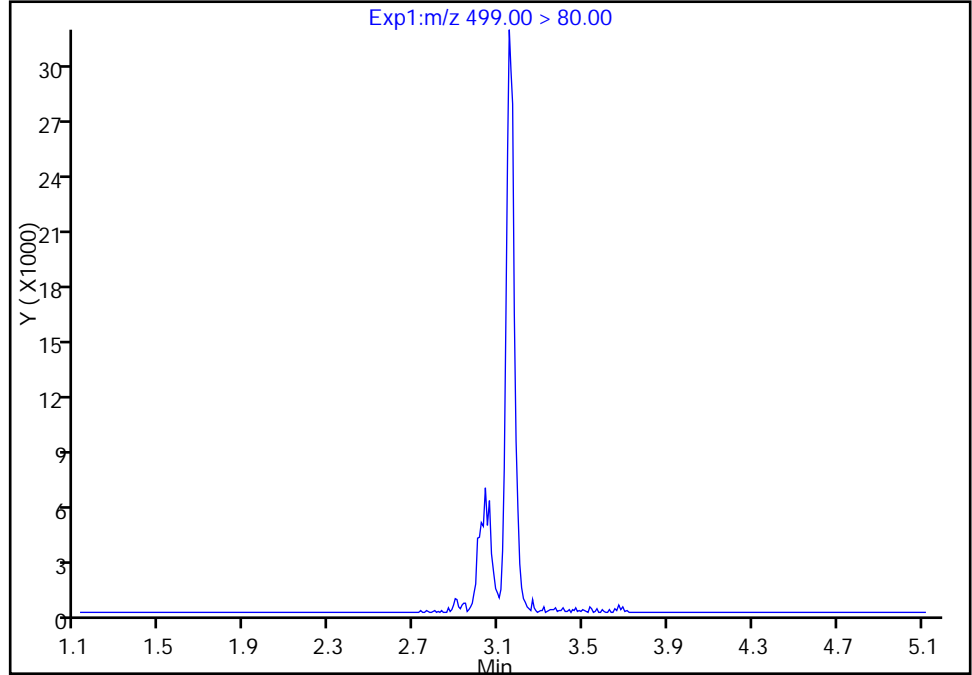

RT: 3.15
Area: 116569
Amount: 0.456423
Amount Units: ng/ml

Manual Integration Results

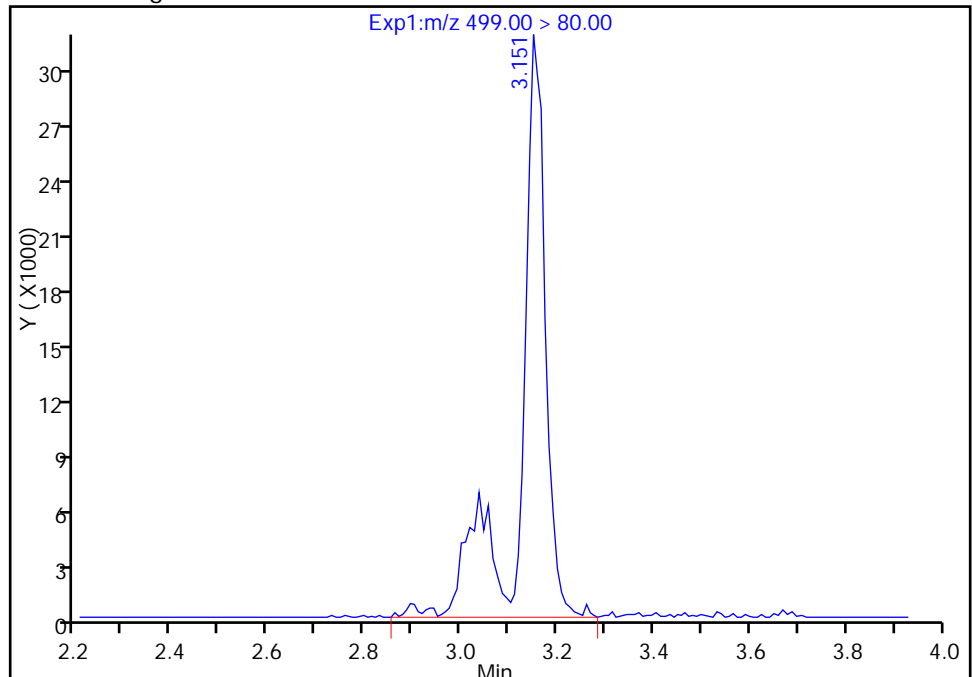

Reviewer: chandrasenas, 15-Dec-2016 13:48:59
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_004.d
Injection Date: 15-Dec-2016 12:29:18 Instrument ID: A8_N
Lims ID: IC L1
Client ID:
Operator ID: A8-PC\A8 ALS Bottle#: 37 Worklist Smp#: 4
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL
Column: Detector EXP1

18 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 3.12

Processing Integration Results

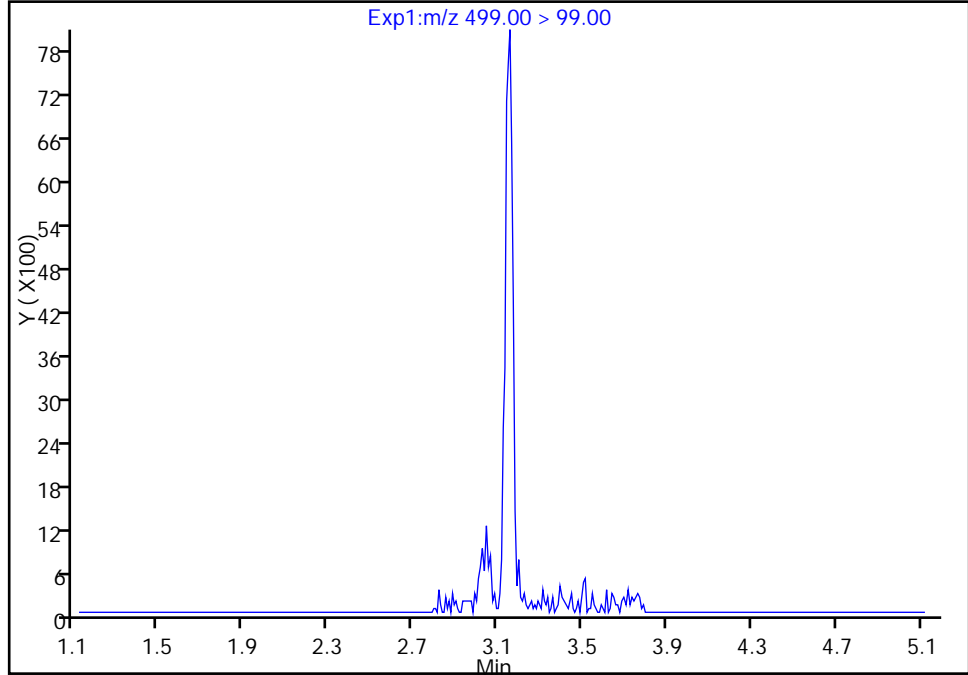

RT: 3.16
Area: 24244
Amount: 0.456423
Amount Units: ng/ml

Manual Integration Results

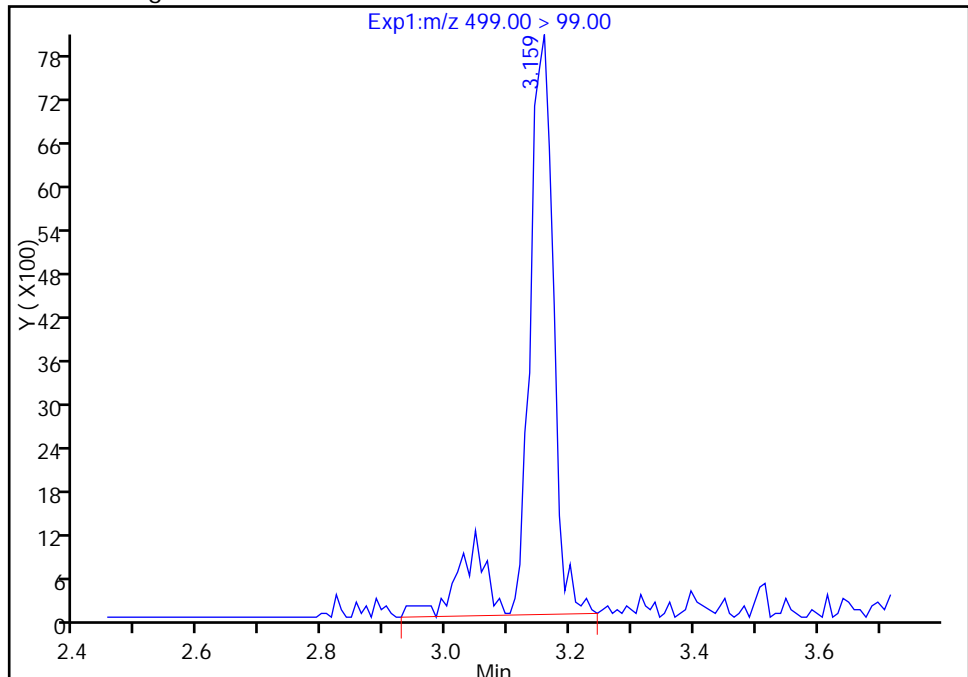

Reviewer: chandrasenas, 15-Dec-2016 13:48:59

Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_004.d
Injection Date: 15-Dec-2016 12:29:18 Instrument ID: A8_N
Lims ID: IC L1
Client ID:
Operator ID: A8-PC\A8 ALS Bottle#: 37 Worklist Smp#: 4
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL
Column: Detector EXP1

29 Perfluorododecanoic acid, CAS: 307-55-1

Signal: 1


RT: 4.13
Area: 43489
Amount: 0.419548
Amount Units: ng/ml

Processing Integration Results

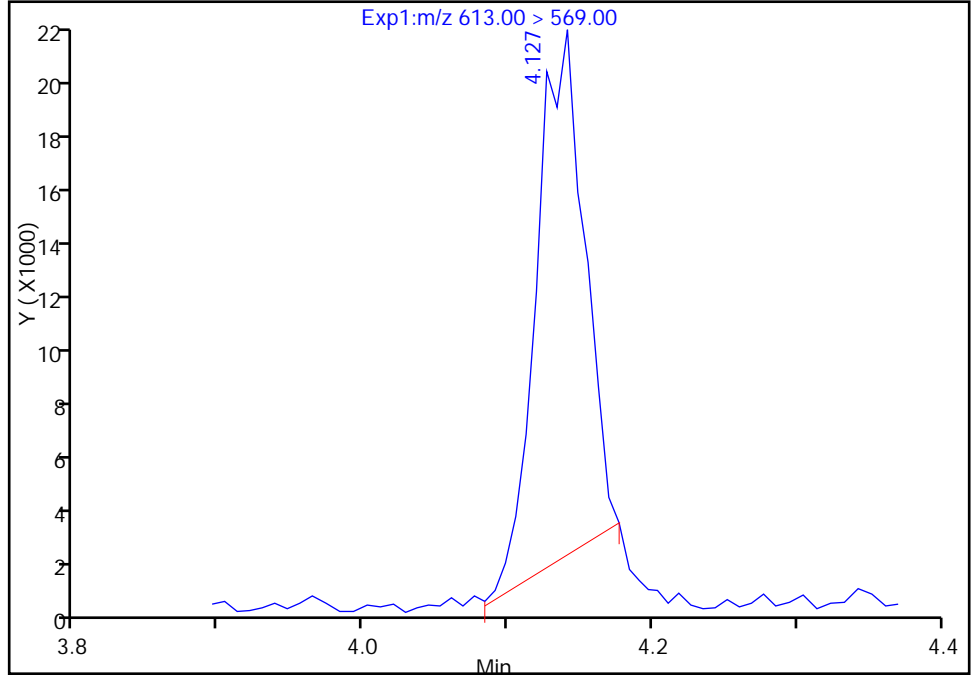

RT: 4.14
Area: 52807
Amount: 0.494620
Amount Units: ng/ml

Manual Integration Results

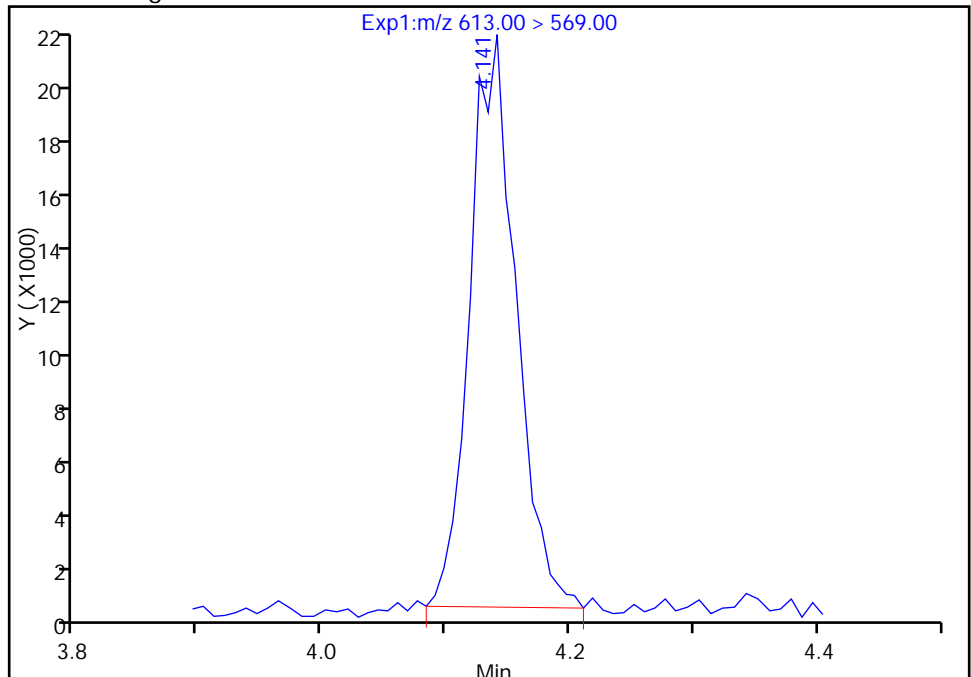

Reviewer: chandrasenas, 15-Dec-2016 13:48:59
Audit Action: Manually Integrated

Audit Reason: Incomplete Integration

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_005.d
 Lims ID: IC L2
 Client ID:
 Sample Type: IC Calib Level: 2
 Inject. Date: 15-Dec-2016 12:36:48 ALS Bottle#: 38 Worklist Smp#: 5
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L2_b
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Sublist: chrom-A8_N*sub6
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 14:34:15 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d

Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 15-Dec-2016 13:50:02

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.530	1.534	-0.004	18201393	52.3		105	1000291	
1 Perfluorobutyric acid	212.90 > 169.00	1.530	1.535	-0.005	310647	1.00		100.0	2583	
D 4 13C5-PFPeA	267.90 > 223.00	1.805	1.810	-0.005	14067714	52.9		106	1093447	
3 Perfluoropentanoic acid	262.90 > 219.00	1.805	1.810	-0.005	287573	1.04		104	2935	
5 Perfluorobutanesulfonic acid	298.90 > 80.00	1.844	1.848	-0.004	424227	0.8800		99.5		
	298.90 > 99.00	1.844	1.848	-0.004	171864		2.47(0.00-0.00)	99.5		
7 Perfluorohexanoic acid	313.00 > 269.00	2.092	2.096	-0.004	239458	1.01		101	6854	
D 6 13C2 PFHxA	315.00 > 270.00	2.092	2.097	-0.005	12814780	52.3		105	582538	
D 11 13C4-PFHpA	367.00 > 322.00	2.423	2.426	-0.003	12248222	54.1		108	431068	
12 Perfluoroheptanoic acid	363.00 > 319.00	2.430	2.428	0.002	237734	0.99		99.1	1884	
9 Perfluorohexanesulfonic acid	399.00 > 80.00	2.445	2.431	0.014	348475	0.99		109		
D 10 18O2 PFHxS	403.00 > 84.00	2.445	2.446	-0.001	16093048	49.2		104	960828	
D 14 13C4 PFOA	417.00 > 372.00	2.781	2.783	-0.002	12627691	54.8		110	657205	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
15 Perfluorooctanoic acid										
413.00 > 369.00	2.781	2.783	-0.002	1.000	254861	1.01		101	2003	
413.00 > 169.00	2.781	2.783	-0.002	1.000	159259		1.60(0.90-1.10)	101	7007	
13 Perfluoroheptanesulfonic Acid										
449.00 > 80.00	2.789	2.790	-0.001	1.000	265783	0.9254		97.2		
18 Perfluorooctane sulfonic acid										
499.00 > 80.00	3.149	3.118	0.031	1.000	220370	0.8502		91.6	15877	M
499.00 > 99.00	3.157	3.118	0.039	1.003	52990		4.16(0.90-1.10)	91.6	5530	M
D 17 13C4 PFOS										
503.00 > 80.00	3.149	3.151	-0.002		12459383	50.1		105	1105467	
D 19 13C5 PFNA										
468.00 > 423.00	3.149	3.153	-0.004		9537045	53.7		107	472742	
20 Perfluorononanoic acid										
463.00 > 419.00	3.157	3.155	0.002	1.000	188341	1.04		104	2906	
D 21 13C8 FOSA										
506.00 > 78.00	3.489	3.488	0.001		20238792	52.7		105	766772	
22 Perfluorooctane Sulfonamide										
498.00 > 78.00	3.489	3.491	-0.002	1.000	381363	1.01		101	46576	
24 Perfluorodecanoic acid										
513.00 > 469.00	3.506	3.510	-0.004	1.000	155537	0.9716		97.2	5243	
D 23 13C2 PFDA										
515.00 > 470.00	3.514	3.513	0.001		8480447	53.9		108	439565	
26 Perfluorodecane Sulfonic acid										
599.00 > 80.00	3.824	3.822	0.002	1.000	139829	0.9186		95.3		
28 Perfluoroundecanoic acid										
563.00 > 519.00	3.833	3.839	-0.006	1.000	119189	1.00		100	2937	
D 27 13C2 PFUnA										
565.00 > 520.00	3.842	3.842	0.0		6219248	53.0		106	280274	
D 30 13C2 PFDoA										
615.00 > 570.00	4.133	4.132	0.001		5822114	52.5		105	270055	
29 Perfluorododecanoic acid										
613.00 > 569.00	4.133	4.136	-0.003	1.000	103481	0.9681		96.8	2745	
31 Perfluorotridecanoic acid										
663.00 > 619.00	4.396	4.400	-0.004	1.000	109461	1.04		104	2155	
D 32 13C2-PFTeDA										
715.00 > 670.00	4.633	4.641	-0.008		11885446	52.3		105	710542	
33 Perfluorotetradecanoic acid										
712.50 > 668.90	4.643	4.642	0.001	1.000	187123	1.01		101	2896	
713.00 > 169.00	4.633	4.642	-0.009	0.998	31916		5.86(0.00-0.00)	101	12057	
D 34 13C2-PFHxDA										
815.00 > 770.00	5.047	5.057	-0.010		6699329	53.8		108	126940	
35 Perfluorohexadecanoic acid										
813.00 > 769.00	5.058	5.059	-0.001	1.000	173261	1.01		101	135	
36 Perfluorooctadecanoic acid										
913.00 > 869.00	5.413	5.414	-0.001	1.000	114997	0.9585		95.8	91.0	

QC Flag Legend

Review Flags

M - Manually Integrated

Reagents:

LCPFC-L2_00023

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_005.d

Injection Date: 15-Dec-2016 12:36:48

Instrument ID: A8_N

Lims ID: IC L2

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 38

Worklist Smp#: 5

Injection Vol: 2.0 ul

Dil. Factor: 1.0000













Method: A8_N

Limit Group: LC PFC_DOD ICAL


D 2 13C4 PFBA

1 Perfluorobutyric acid


D 4 13C5-PFPeA

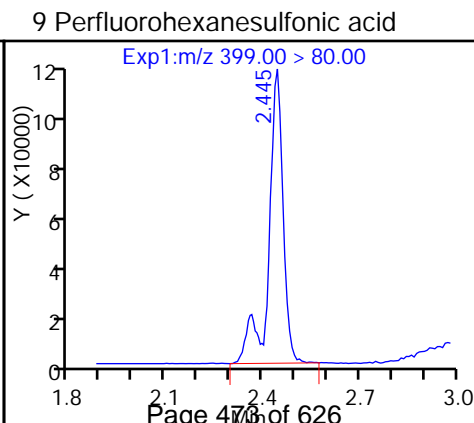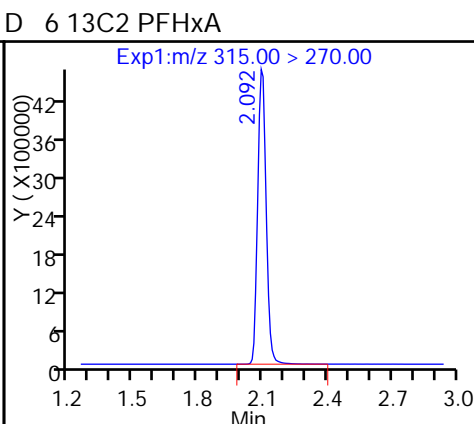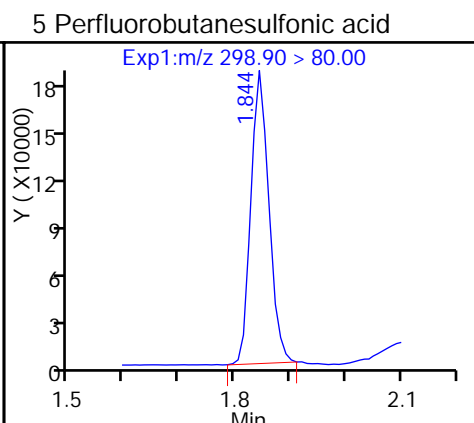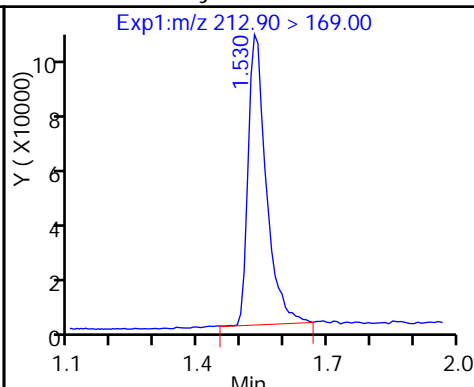


D 14 13C4 PFOA

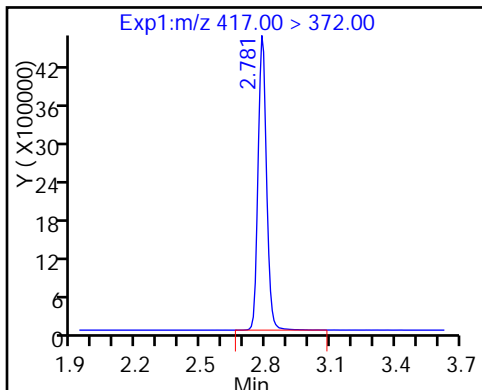


15 Perfluorooctanoic acid

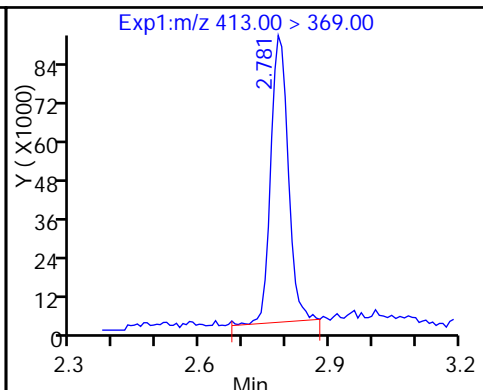


15 Perfluorooctanoic acid




13 Perfluoroheptanesulfonic Acid

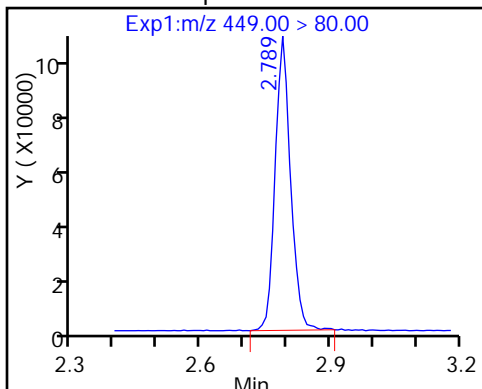


18 Perfluorooctane sulfonic acid (M)

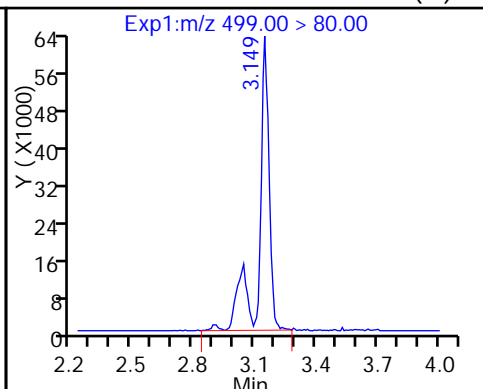


18 Perfluorooctane sulfonic acid (M)




D 17 13C4 PFOS

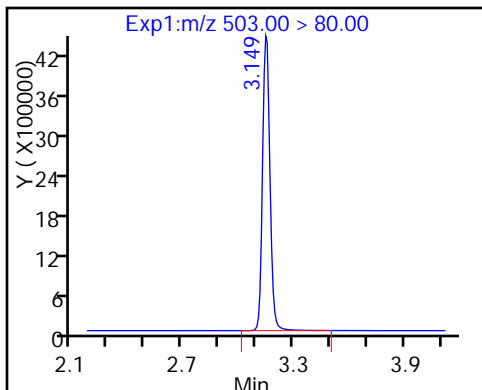


D 19 13C5 PFNA

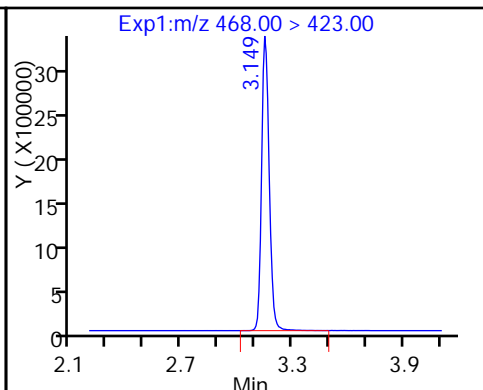


20 Perfluorononanoic acid




D 21 13C8 FOSA

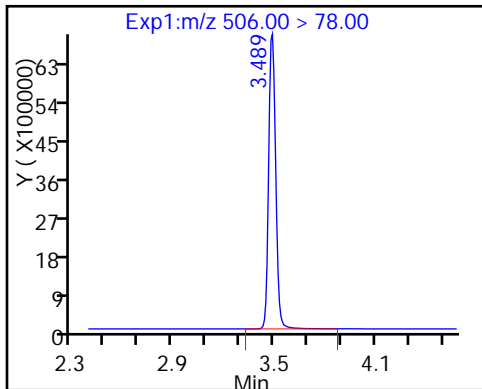

22 Perfluorooctane Sulfonamide

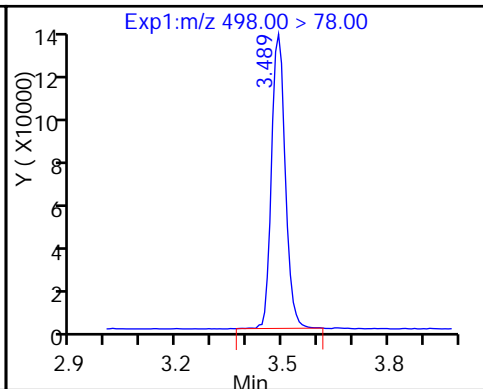




24 Perfluorodecanoic acid



D 23 13C2 PFDA

26 Perfluorodecane Sulfonic acid




28 Perfluoroundecanoic acid



D 27 13C2 PFUa

D 30 13C2 PFDa




29 Perfluorododecanoic acid



31 Perfluorotridecanoic acid

D 32 13C2-PFTeDA




33 Perfluorotetradecanoic acid




33 Perfluorotetradecanoic acid

D 34 13C2-PFHxDa

35 Perfluorohexadecanoic acid



36 Perfluorooctadecanoic acid

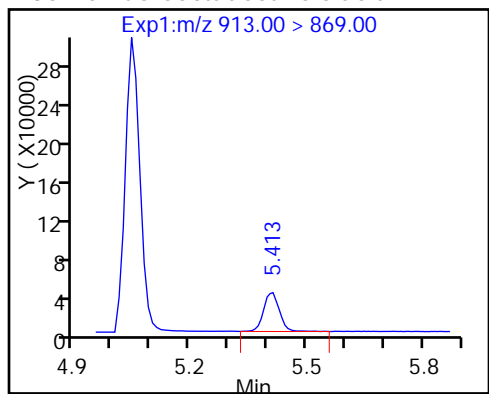

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_005.d
Injection Date: 15-Dec-2016 12:36:48 Instrument ID: A8_N
Lims ID: IC L2
Client ID:
Operator ID: A8-PC\A8 ALS Bottle#: 38 Worklist Smp#: 5
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL
Column: Detector EXP1

18 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 3.12

Processing Integration Results

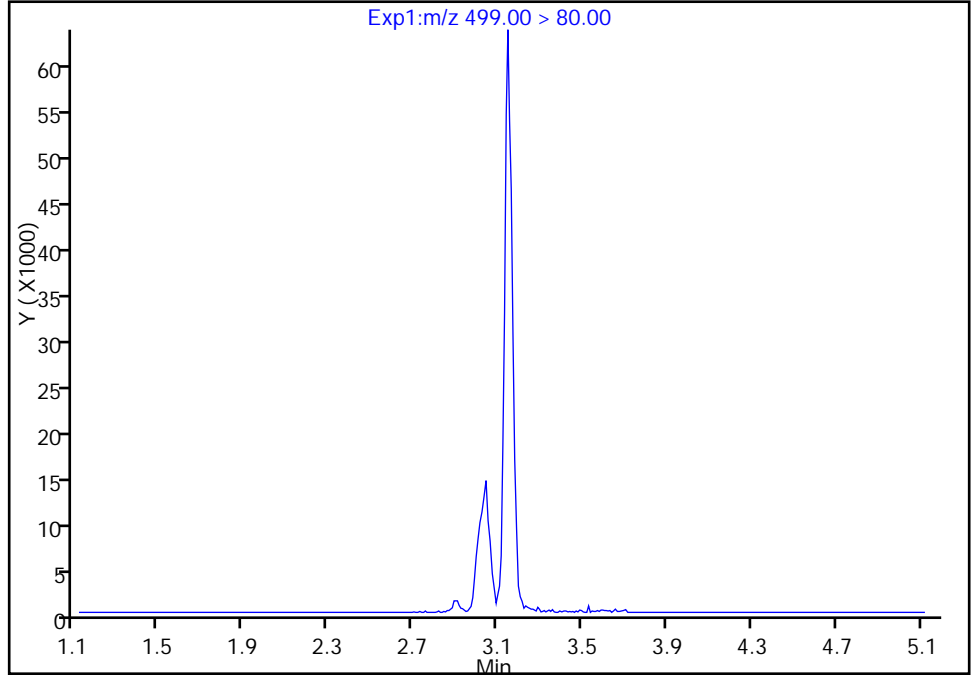

RT: 3.15
Area: 220370
Amount: 0.850158
Amount Units: ng/ml

Manual Integration Results

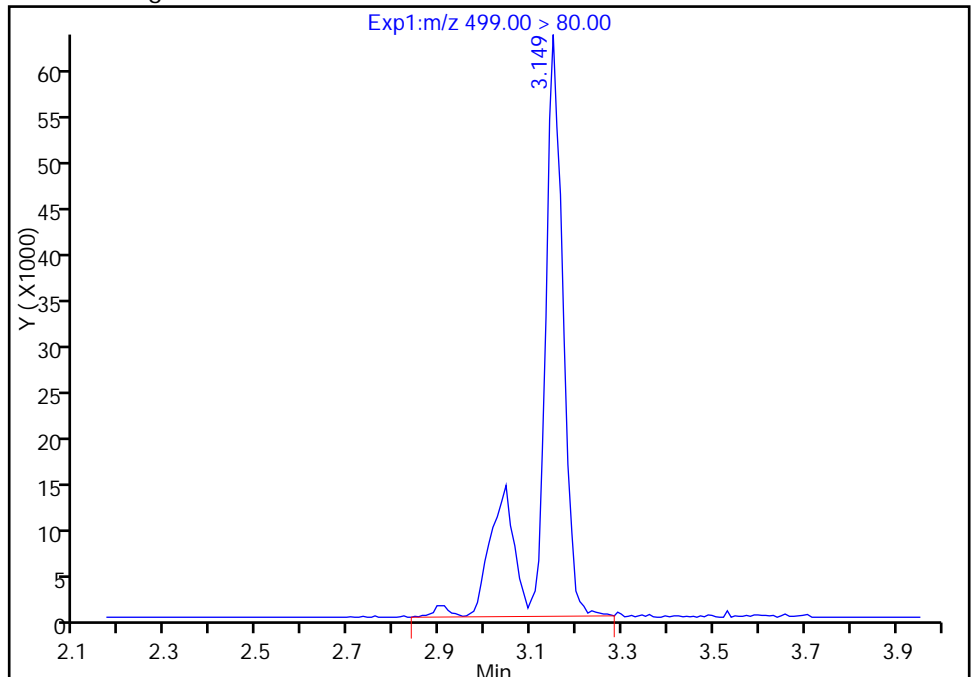

Reviewer: chandrasenas, 15-Dec-2016 13:50:02
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_005.d
Injection Date: 15-Dec-2016 12:36:48 Instrument ID: A8_N
Lims ID: IC L2
Client ID:
Operator ID: A8-PC\A8 ALS Bottle#: 38 Worklist Smp#: 5
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL
Column: Detector EXP1

18 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 3.12

Processing Integration Results

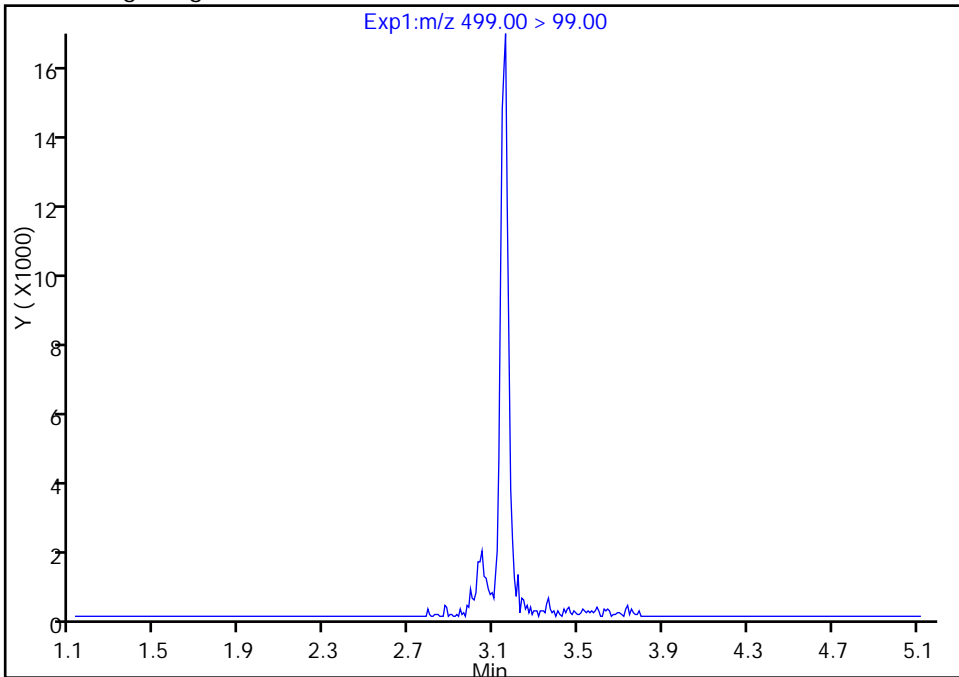

Manual Integration Results

RT: 3.16
Area: 52990
Amount: 0.850158
Amount Units: ng/ml

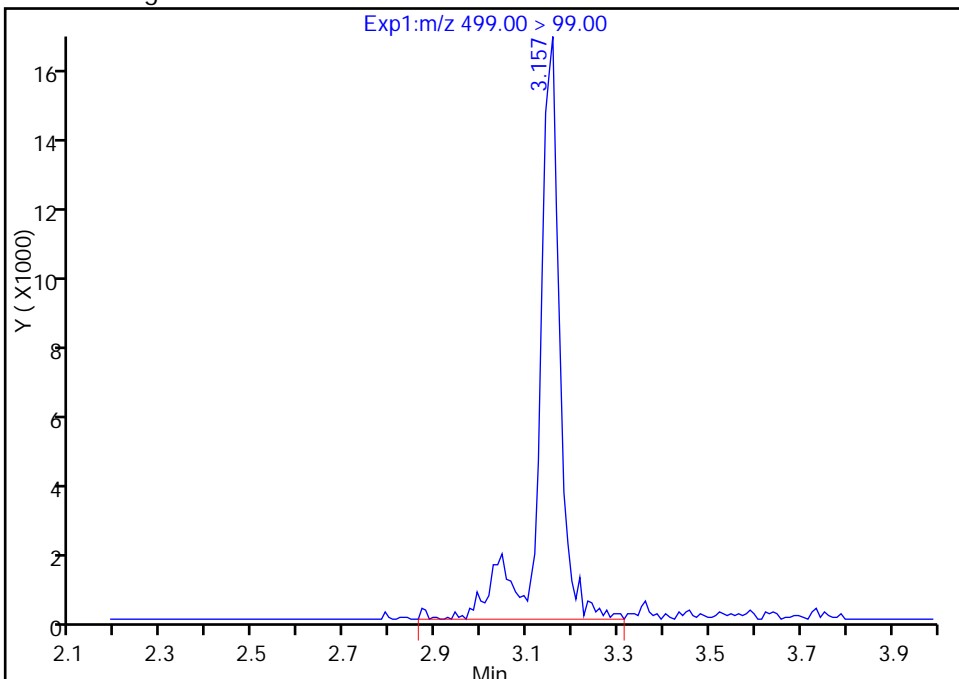

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_006.d
 Lims ID: IC L3
 Client ID:
 Sample Type: IC Calib Level: 3
 Inject. Date: 15-Dec-2016 12:44:16 ALS Bottle#: 39 Worklist Smp#: 6
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L3_b
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Sublist: chrom-A8_N*sub6
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 14:34:18 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 15-Dec-2016 13:50:22

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.534	1.534	0.0	18037108	51.9		104	828248	
1 Perfluorobutyric acid	212.90 > 169.00	1.534	1.535	-0.001	1550440	5.03		101	13427	
D 4 13C5-PFPeA	267.90 > 223.00	1.810	1.810	0.0	14063070	52.9		106	1078697	
3 Perfluoropentanoic acid	262.90 > 219.00	1.810	1.810	0.0	1358239	4.89		97.9	15178	
5 Perfluorobutanesulfonic acid	298.90 > 80.00	1.849	1.848	0.001	2211602	4.55		103		
	298.90 > 99.00	1.849	1.848	0.001	918055		2.41(0.00-0.00)	103		
7 Perfluorohexanoic acid	313.00 > 269.00	2.097	2.096	0.001	1183286	5.01		100	39266	
D 6 13C2 PFHxA	315.00 > 270.00	2.097	2.097	0.0	12709919	51.9		104	753338	
D 11 13C4-PFHpA	367.00 > 322.00	2.425	2.426	-0.001	12260528	54.2		108	1467079	
12 Perfluoroheptanoic acid	363.00 > 319.00	2.432	2.428	0.004	1175112	4.90		97.9	8914	
9 Perfluorohexanesulfonic acid	399.00 > 80.00	2.364	2.431	-0.067	1543002	4.37		96.0		
D 10 18O2 PFHxS	403.00 > 84.00	2.447	2.446	0.001	16222736	49.6		105	651458	
D 14 13C4 PFOA	417.00 > 372.00	2.783	2.783	0.0	12635065	54.8		110	746410	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
15 Perfluorooctanoic acid										
413.00 > 369.00	2.783	2.783	0.0	1.000	1239541	4.89		97.8	9812	
413.00 > 169.00	2.783	2.783	0.0	1.000	731249		1.70(0.90-1.10)	97.8	28264	
13 Perfluoroheptanesulfonic Acid										
449.00 > 80.00	2.792	2.790	0.002	1.000	1351160	4.69		98.6		
18 Perfluorooctane sulfonic acid										
499.00 > 80.00	3.153	3.118	0.035	1.000	1150410	4.43		95.5	65030	
499.00 > 99.00	3.153	3.118	0.035	1.000	246751		4.66(0.90-1.10)	95.5	15530	
D 17 13C4 PFOS										
503.00 > 80.00	3.153	3.151	0.002		12484772	50.2		105	473035	
D 19 13C5 PFNA										
468.00 > 423.00	3.153	3.153	0.0		9777609	55.0		110	653324	
20 Perfluorononanoic acid										
463.00 > 419.00	3.153	3.155	-0.002	1.000	902512	4.85		97.0	13825	
D 21 13C8 FOSA										
506.00 > 78.00	3.484	3.488	-0.004		20034933	52.2		104	309657	
22 Perfluorooctane Sulfonamide										
498.00 > 78.00	3.492	3.491	0.001	1.000	1989314	5.32		106	140153	
24 Perfluorodecanoic acid										
513.00 > 469.00	3.509	3.510	-0.001	1.000	771905	4.97		99.3	27905	
D 23 13C2 PFDA										
515.00 > 470.00	3.509	3.513	-0.004		8234678	52.3		105	259288	
26 Perfluorodecane Sulfonic acid										
599.00 > 80.00	3.819	3.822	-0.003	1.000	712852	4.67		97.0		
28 Perfluoroundecanoic acid										
563.00 > 519.00	3.837	3.839	-0.002	1.000	549708	4.59		91.8	14816	
D 27 13C2 PFUnA										
565.00 > 520.00	3.845	3.842	0.003		6262617	53.4		107	379922	
D 30 13C2 PFDoA										
615.00 > 570.00	4.129	4.132	-0.003		5779875	52.1		104	227122	
29 Perfluorododecanoic acid										
613.00 > 569.00	4.136	4.136	0.0	1.000	506369	4.77		95.4	11299	
31 Perfluorotridecanoic acid										
663.00 > 619.00	4.398	4.400	-0.002	1.000	525090	5.01		100	10475	
D 32 13C2-PFTeDA										
715.00 > 670.00	4.645	4.641	0.004		12248242	53.9		108	1049274	
33 Perfluorotetradecanoic acid										
712.50 > 668.90	4.645	4.642	0.003	1.000	900575	4.92		98.3	12522	
713.00 > 169.00	4.635	4.642	-0.007	0.998	149199		6.04(0.00-0.00)	98.3	58819	
D 34 13C2-PFHxDA										
815.00 > 770.00	5.059	5.057	0.002		6542972	52.5		105	140605	
35 Perfluorohexadecanoic acid										
813.00 > 769.00	5.059	5.059	0.0	1.000	599529	4.89		97.7	502	
36 Perfluorooctadecanoic acid										
913.00 > 869.00	5.414	5.414	0.0	1.000	583761	4.90		98.0	536	

Reagents:

LCPFC-L3_00020

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_006.d

Injection Date: 15-Dec-2016 12:44:16

Instrument ID: A8_N

Lims ID: IC L3

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 39

Worklist Smp#: 6

Injection Vol: 2.0 ul

Dil. Factor: 1.0000













Method: A8_N

Limit Group: LC PFC_DOD ICAL


D 2 13C4 PFBA

1 Perfluorobutyric acid


D 4 13C5-PFPeA

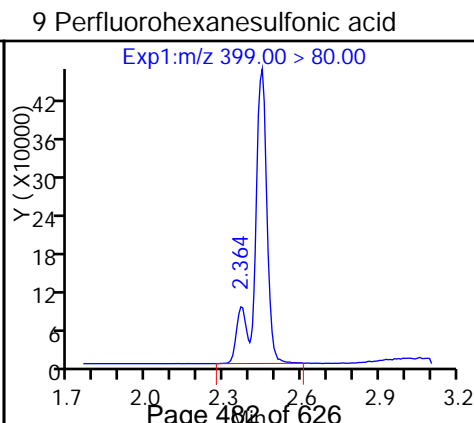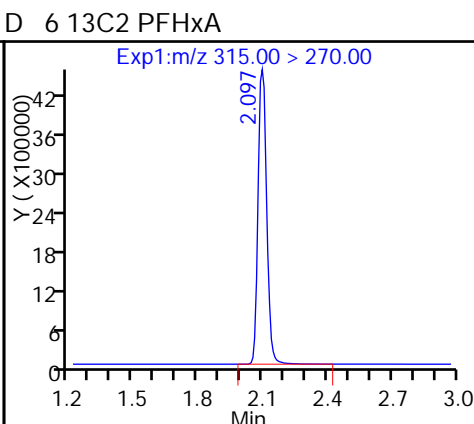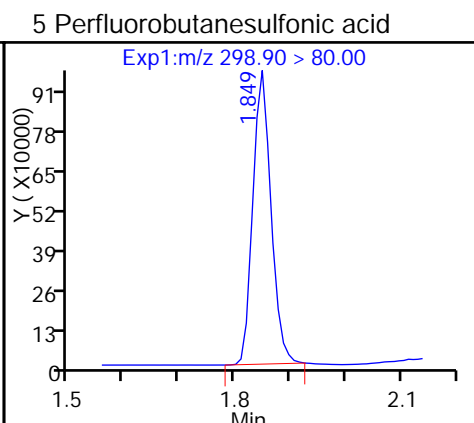


D 14 13C4 PFOA




15 Perfluorooctanoic acid




15 Perfluorooctanoic acid




13 Perfluoroheptanesulfonic Acid




18 Perfluorooctane sulfonic acid




18 Perfluorooctane sulfonic acid




D 17 13C4 PFOS




D 19 13C5 PFNA




20 Perfluorononanoic acid




D 21 13C8 FOSA




22 Perfluorooctane Sulfonamide




24 Perfluorodecanoic acid




D 23 13C2 PFDA




26 Perfluorodecane Sulfonic acid




28 Perfluoroundecanoic acid

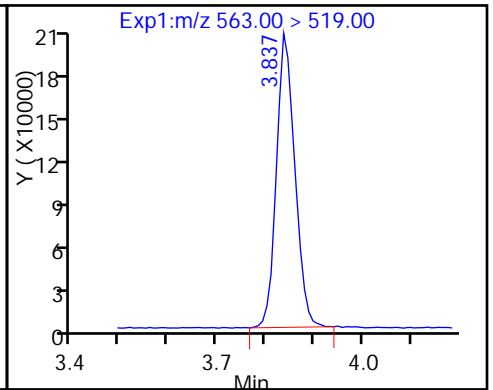


D 27 13C2 PFUa




D 30 13C2 PFDa

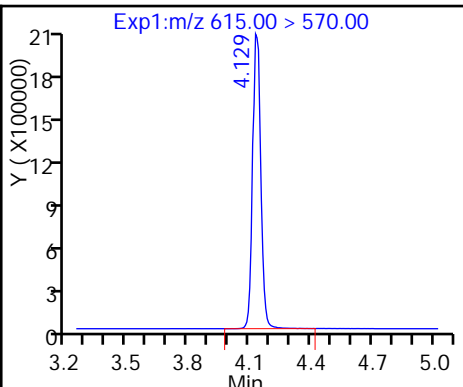


29 Perfluorododecanoic acid

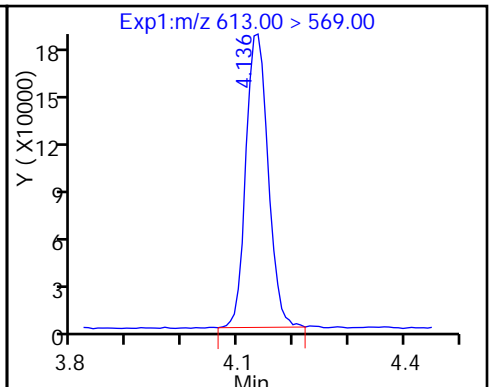


31 Perfluorotridecanoic acid




D 32 13C2-PFTeDA




33 Perfluorotetradecanoic acid

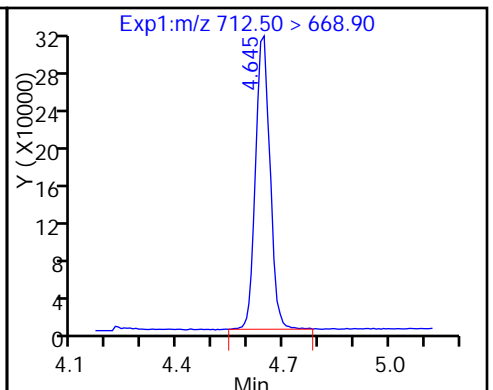


33 Perfluorotetradecanoic acid




D 34 13C2-PFHxDA

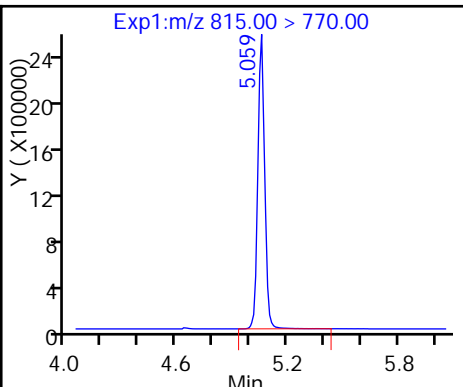

35 Perfluorohexadecanoic acid

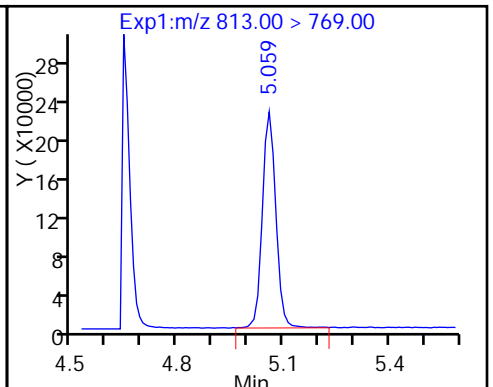

36 Perfluorooctadecanoic acid

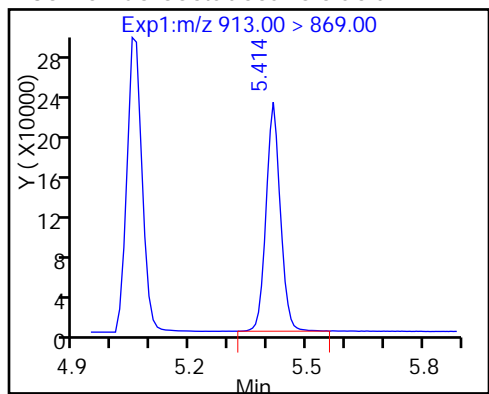

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_007.d
 Lims ID: IC L4
 Client ID:
 Sample Type: IC Calib Level: 4
 Inject. Date: 15-Dec-2016 12:51:47 ALS Bottle#: 40 Worklist Smp#: 7
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L4_b
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Sublist: chrom-A8_N*sub6
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 14:34:21 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 15-Dec-2016 13:46:14

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.534	1.534	0.0	17585378	50.6		101	1140977	
1 Perfluorobutyric acid	212.90 > 169.00	1.534	1.535	-0.001	1.000	6690917	22.3	111	52374	
D 4 13C5-PFPeA	267.90 > 223.00	1.810	1.810	0.0	13617158	51.2		102	860552	
3 Perfluoropentanoic acid	262.90 > 219.00	1.810	1.810	0.0	1.000	5770240	21.5	107	61088	
5 Perfluorobutanesulfonic acid	298.90 > 80.00	1.849	1.848	0.001	1.000	9860707	20.5	116		
	298.90 > 99.00	1.849	1.848	0.001	1.000	4111615	2.40(0.00-0.00)	116		
7 Perfluorohexanoic acid	313.00 > 269.00	2.093	2.096	-0.003	1.000	4929766	21.0	105	144495	
D 6 13C2 PFHxA	315.00 > 270.00	2.102	2.097	0.005		12608210	51.4	103	627430	
D 11 13C4-PFHpA	367.00 > 322.00	2.426	2.426	0.0		11788221	52.1	104	459454	
12 Perfluoroheptanoic acid	363.00 > 319.00	2.426	2.428	-0.002	1.000	4747711	20.6	103	44179	
9 Perfluorohexanesulfonic acid	399.00 > 80.00	2.440	2.431	0.009	1.000	6624638	18.9	104		
D 10 18O2 PFHxS	403.00 > 84.00	2.440	2.446	-0.006		16062766	49.1	104	697379	
D 14 13C4 PFOA	417.00 > 372.00	2.785	2.783	0.002		11818203	51.3	103	403727	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
15 Perfluorooctanoic acid										
413.00 > 369.00	2.785	2.783	0.002	1.000	5109766	21.6		108	40900	
413.00 > 169.00	2.785	2.783	0.002	1.000	3083663		1.66(0.90-1.10)	108	124075	
13 Perfluoroheptanesulfonic Acid										
449.00 > 80.00	2.785	2.790	-0.005	1.000	6014021	21.4		112		
18 Perfluorooctane sulfonic acid										
499.00 > 80.00	3.129	3.118	0.011	1.000	5058824	20.0		108	109804	
499.00 > 99.00	3.153	3.118	0.035	1.008	1125313		4.50(0.90-1.10)	108	92390	
D 17 13C4 PFOS										
503.00 > 80.00	3.153	3.151	0.002		12183062	49.0		102	250792	
D 19 13C5 PFNA										
468.00 > 423.00	3.153	3.153	0.0		9236073	52.0		104	341338	
20 Perfluorononanoic acid										
463.00 > 419.00	3.153	3.155	-0.002	1.000	3562981	20.3		101	53054	
D 21 13C8 FOSA										
506.00 > 78.00	3.484	3.488	-0.004		19703272	51.3		103	612200	
22 Perfluorooctane Sulfonamide										
498.00 > 78.00	3.492	3.491	0.001	1.000	7990835	21.7		109	298669	
24 Perfluorodecanoic acid										
513.00 > 469.00	3.509	3.510	-0.001	1.000	3166735	20.6		103	81817	
D 23 13C2 PFDA										
515.00 > 470.00	3.517	3.513	0.004		8134734	51.7		103	195073	
26 Perfluorodecane Sulfonic acid										
599.00 > 80.00	3.827	3.822	0.005	1.000	3084031	20.7		107		
28 Perfluoroundecanoic acid										
563.00 > 519.00	3.844	3.839	0.005	1.000	2420719	20.3		102	65024	
D 27 13C2 PFUnA										
565.00 > 520.00	3.835	3.842	-0.007		6226562	53.1		106	471162	
D 30 13C2 PFDoA										
615.00 > 570.00	4.135	4.132	0.003		5816809	52.4		105	222845	
29 Perfluorododecanoic acid										
613.00 > 569.00	4.135	4.136	-0.001	1.000	2231794	20.9		104	47124	
31 Perfluorotridecanoic acid										
663.00 > 619.00	4.398	4.400	-0.002	1.000	2087859	19.8		98.9	37986	
D 32 13C2-PFTeDA										
715.00 > 670.00	4.644	4.641	0.003		11655048	51.3		103	471362	
33 Perfluorotetradecanoic acid										
712.50 > 668.90	4.644	4.642	0.002	1.000	3678976	20.0		99.8	48461	
713.00 > 169.00	4.635	4.642	-0.007	0.998	596997		6.16(0.00-0.00)	99.8	56132	
D 34 13C2-PFHxDA										
815.00 > 770.00	5.059	5.057	0.002		6335821	50.9		102	120381	
35 Perfluorohexadecanoic acid										
813.00 > 769.00	5.059	5.059	0.0	1.000	2267892	19.9		99.3	1990	
36 Perfluorooctadecanoic acid										
913.00 > 869.00	5.413	5.414	-0.001	1.000	2445236	20.4		102	2369	

Reagents:

LCPFC-L4_00024

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_007.d

Injection Date: 15-Dec-2016 12:51:47

Instrument ID: A8_N

Lims ID: IC L4

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 40

Worklist Smp#: 7

Injection Vol: 2.0 ul

Dil. Factor: 1.0000













Method: A8_N

Limit Group: LC PFC_DOD ICAL


D 2 13C4 PFBA

1 Perfluorobutyric acid


D 4 13C5-PFPeA

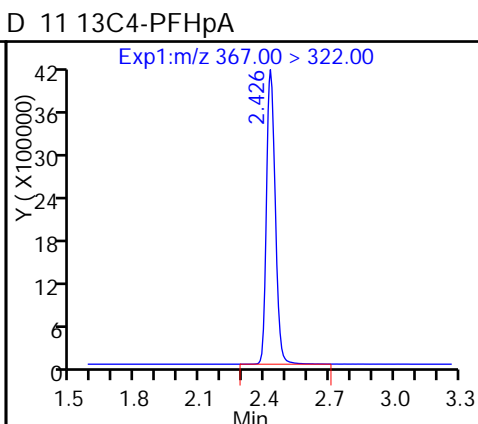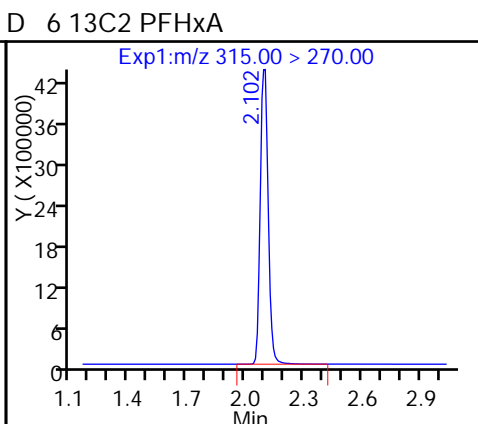


D 14 13C4 PFOA

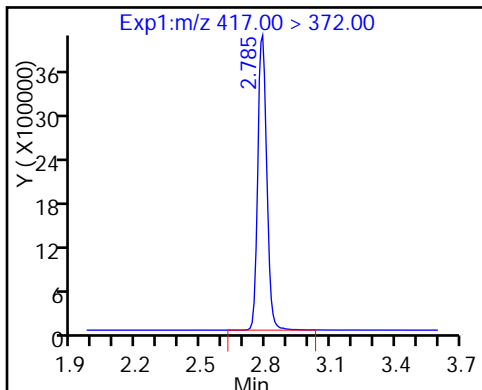


15 Perfluorooctanoic acid

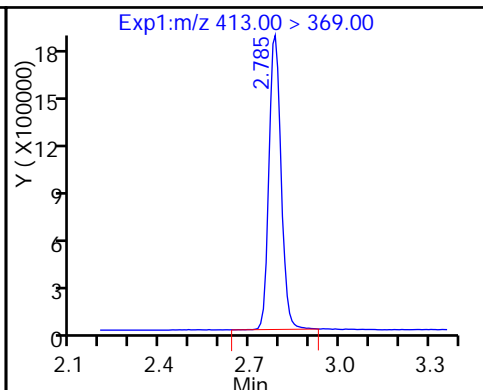


15 Perfluorooctanoic acid




13 Perfluoroheptanesulfonic Acid

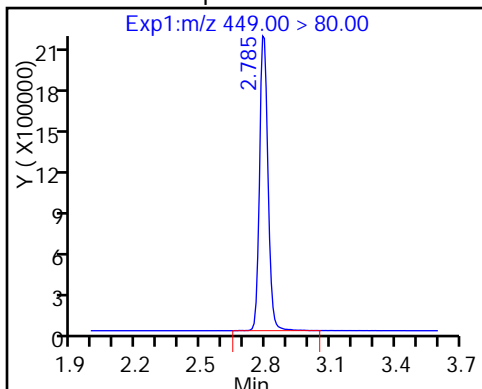


18 Perfluorooctane sulfonic acid

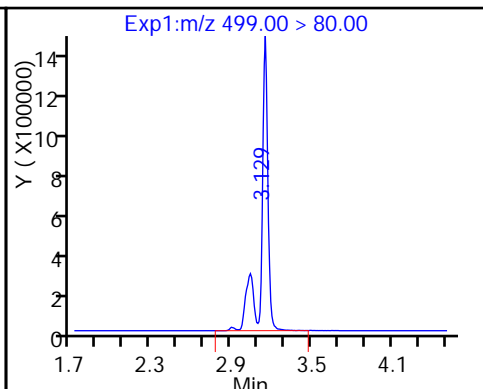


18 Perfluorooctane sulfonic acid




D 17 13C4 PFOS

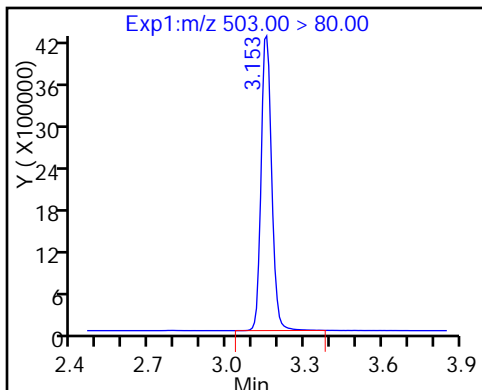


D 19 13C5 PFNA

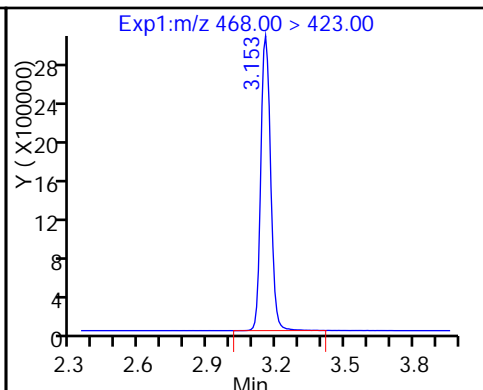


20 Perfluorononanoic acid




D 21 13C8 FOSA

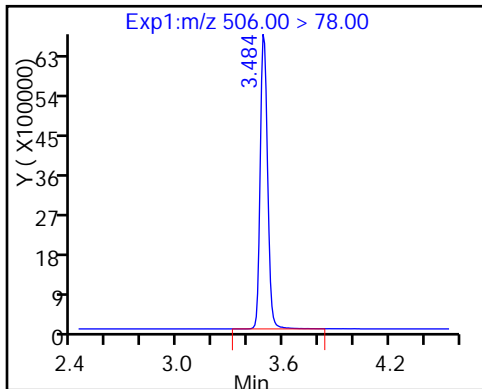


22 Perfluorooctane Sulfonamide

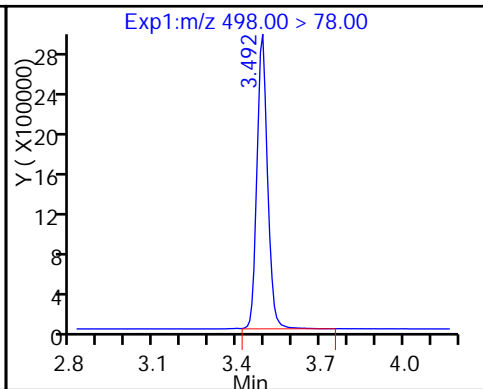


24 Perfluorodecanoic acid




D 23 13C2 PFDA




26 Perfluorodecane Sulfonic acid




28 Perfluoroundecanoic acid




D 27 13C2 PFUa




D 30 13C2 PFDa




29 Perfluorododecanoic acid




31 Perfluorotridecanoic acid




D 32 13C2-PFTeDA




33 Perfluorotetradecanoic acid




33 Perfluorotetradecanoic acid




D 34 13C2-PFHxDA



35 Perfluorohexadecanoic acid



36 Perfluorooctadecanoic acid

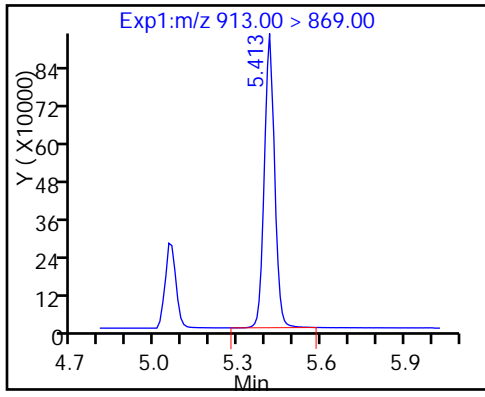

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_008.d
 Lims ID: IC L5
 Client ID:
 Sample Type: IC Calib Level: 5
 Inject. Date: 15-Dec-2016 12:59:16 ALS Bottle#: 41 Worklist Smp#: 8
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L5_b
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Sublist: chrom-A8_N*sub6
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 14:34:24 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d

Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 15-Dec-2016 13:51:06

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.533	1.534	-0.001	17274187	49.7		99.4	927175	
1 Perfluorobutyric acid	212.90 > 169.00	1.533	1.535	-0.002	15411527	52.3		105	124871	
D 4 13C5-PFPeA	267.90 > 223.00	1.810	1.810	0.0	13053659	49.1		98.1	1261104	
3 Perfluoropentanoic acid	262.90 > 219.00	1.810	1.810	0.0	13161065	51.1		102	158308	
5 Perfluorobutanesulfonic acid	298.90 > 80.00	1.848	1.848	0.0	21559838	47.1		107		
	298.90 > 99.00	1.848	1.848	0.0	10128422		2.13(0.00-0.00)	107		
7 Perfluorohexanoic acid	313.00 > 269.00	2.098	2.096	0.002	11507044	50.0		99.9	330809	
D 6 13C2 PFHxA	315.00 > 270.00	2.098	2.097	0.001	12399280	50.6		101	688050	
D 11 13C4-PFHpA	367.00 > 322.00	2.424	2.426	-0.002	10801604	47.7		95.4	530896	
12 Perfluoroheptanoic acid	363.00 > 319.00	2.424	2.428	-0.004	10799449	51.1		102	85838	
9 Perfluorohexanesulfonic acid	399.00 > 80.00	2.446	2.431	0.015	15253691	45.8		101		
D 10 18O2 PFHxS	403.00 > 84.00	2.446	2.446	0.0	15278828	46.7		98.8	1046737	
D 14 13C4 PFOA	417.00 > 372.00	2.782	2.783	-0.001	11142777	48.4		96.7	755641	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
15 Perfluorooctanoic acid										
413.00 > 369.00	2.782	2.783	-0.001	1.000	11435583	51.2		102	92940	
413.00 > 169.00	2.782	2.783	-0.001	1.000	6849991		1.67(0.90-1.10)	102	293728	
13 Perfluoroheptanesulfonic Acid										
449.00 > 80.00	2.791	2.790	0.001	1.000	13639927	49.5		104		
18 Perfluorooctane sulfonic acid										
499.00 > 80.00	3.151	3.118	0.033	1.000	11741891	47.2		102	399791	
499.00 > 99.00	3.151	3.118	0.033	1.000	2632984		4.46(0.90-1.10)	102	139087	
D 17 13C4 PFOS										
503.00 > 80.00	3.151	3.151	0.0		11946650	48.0		100	237614	
D 19 13C5 PFNA										
468.00 > 423.00	3.151	3.153	-0.002		8581504	48.3		96.6	574194	
20 Perfluorononanoic acid										
463.00 > 419.00	3.151	3.155	-0.004	1.000	8246252	50.5		101	123521	
D 21 13C8 FOSA										
506.00 > 78.00	3.490	3.488	0.002		18804188	49.0		97.9	642404	
22 Perfluorooctane Sulfonamide										
498.00 > 78.00	3.490	3.491	-0.001	1.000	17736944	50.6		101	676782	
24 Perfluorodecanoic acid										
513.00 > 469.00	3.507	3.510	-0.003	1.000	7324495	50.6		101	172410	
D 23 13C2 PFDA										
515.00 > 470.00	3.516	3.513	0.003		7671861	48.8		97.5	212001	
26 Perfluorodecane Sulfonic acid										
599.00 > 80.00	3.818	3.822	-0.004	1.000	7241868	49.6		103		
28 Perfluoroundecanoic acid										
563.00 > 519.00	3.844	3.839	0.005	1.000	5437764	50.3		101	105822	
D 27 13C2 PFUnA										
565.00 > 520.00	3.844	3.842	0.002		5657823	48.3		96.5	259964	
D 30 13C2 PFDoA										
615.00 > 570.00	4.135	4.132	0.003		5404154	48.7		97.4	211794	
29 Perfluorododecanoic acid										
613.00 > 569.00	4.135	4.136	-0.001	1.000	5072994	51.1		102	98593	
31 Perfluorotridecanoic acid										
663.00 > 619.00	4.398	4.400	-0.002	1.000	4950651	50.5		101	84213	
D 32 13C2-PFTeDA										
715.00 > 670.00	4.645	4.641	0.004		10950502	48.2		96.3	504805	
33 Perfluorotetradecanoic acid										
712.50 > 668.90	4.645	4.642	0.003	1.000	8645519	50.5		101	145963	
713.00 > 169.00	4.635	4.642	-0.007	0.998	1380699		6.26(0.00-0.00)	101	249413	
D 34 13C2-PFHxDA										
815.00 > 770.00	5.059	5.057	0.002		6027362	48.4		96.8	112750	
35 Perfluorohexadecanoic acid										
813.00 > 769.00	5.059	5.059	0.0	1.000	5318207	51.0		102	4484	
36 Perfluorooctadecanoic acid										
913.00 > 869.00	5.413	5.414	-0.001	1.000	5869666	52.7		105	5549	

Reagents:

LCPFC-L5_00022

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_008.d

Injection Date: 15-Dec-2016 12:59:16

Instrument ID: A8_N

Lims ID: IC L5

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 41

Worklist Smp#: 8

Injection Vol: 2.0 ul

Dil. Factor: 1.0000













Method: A8_N

Limit Group: LC PFC_DOD ICAL


D 2 13C4 PFBA

1 Perfluorobutyric acid


D 4 13C5-PFPeA

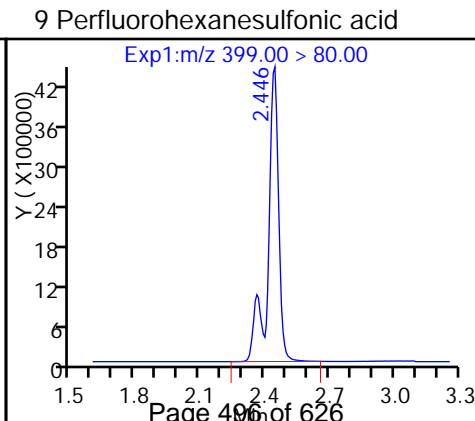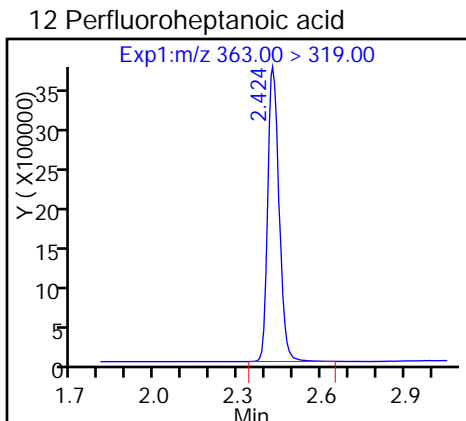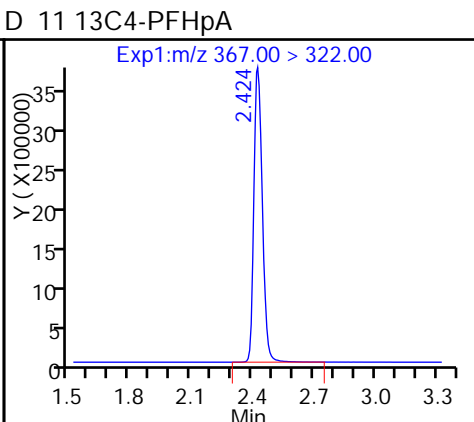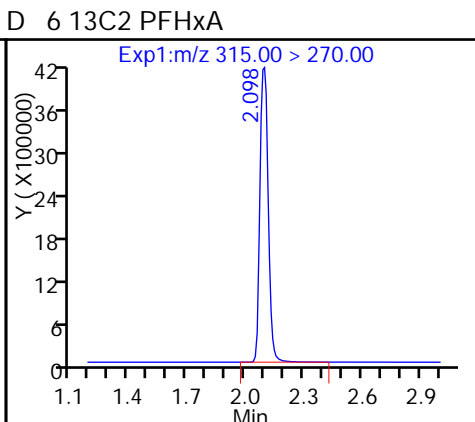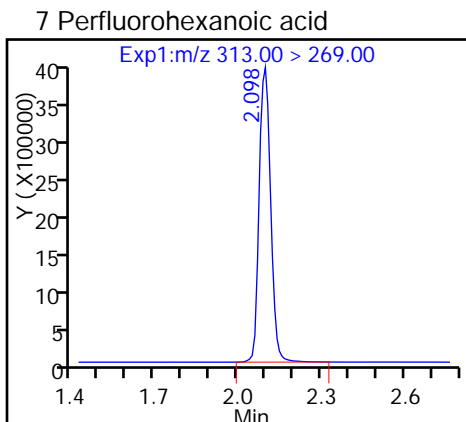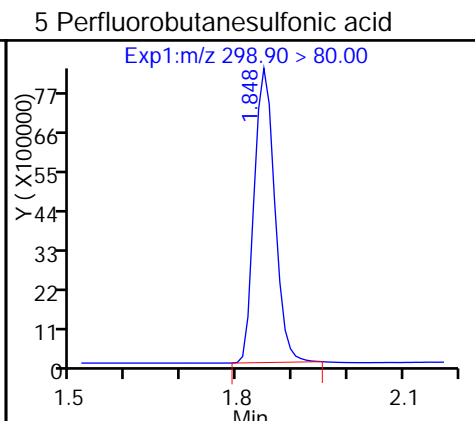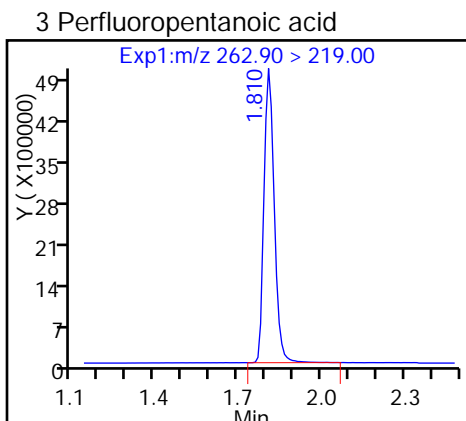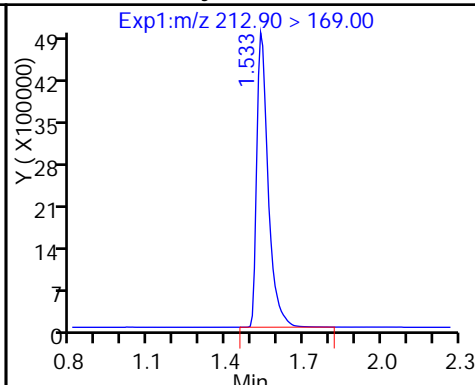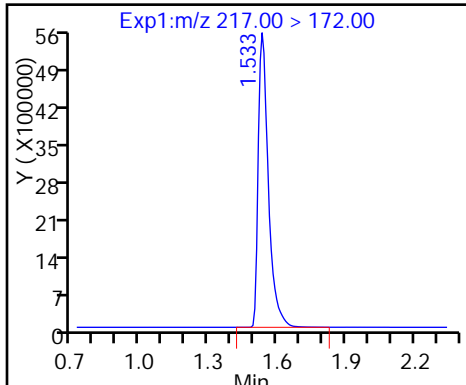


D 14 13C4 PFOA




15 Perfluorooctanoic acid




15 Perfluorooctanoic acid




13 Perfluoroheptanesulfonic Acid




18 Perfluorooctane sulfonic acid




18 Perfluorooctane sulfonic acid




D 17 13C4 PFOS




D 19 13C5 PFNA




20 Perfluorononanoic acid




D 21 13C8 FOSA




22 Perfluorooctane Sulfonamide




24 Perfluorodecanoic acid




D 23 13C2 PFDA




26 Perfluorodecane Sulfonic acid

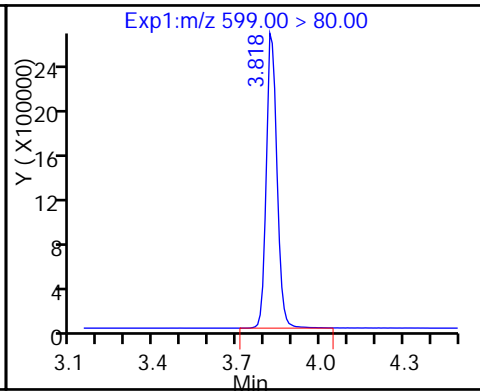


28 Perfluoroundecanoic acid

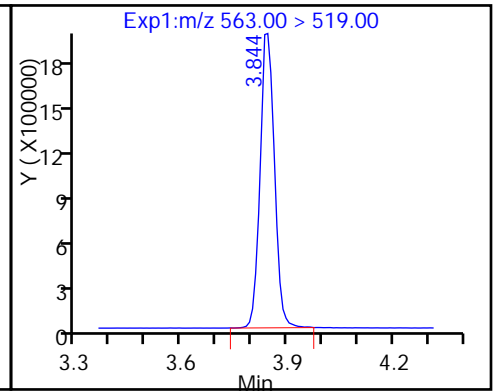


D 27 13C2 PFUa




D 30 13C2 PFDa




29 Perfluorododecanoic acid

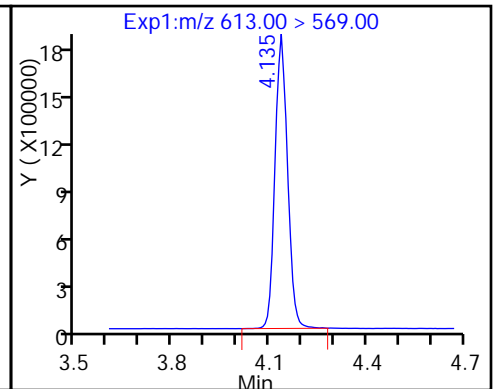


31 Perfluorotridecanoic acid




D 32 13C2-PFTeDA




33 Perfluorotetradecanoic acid

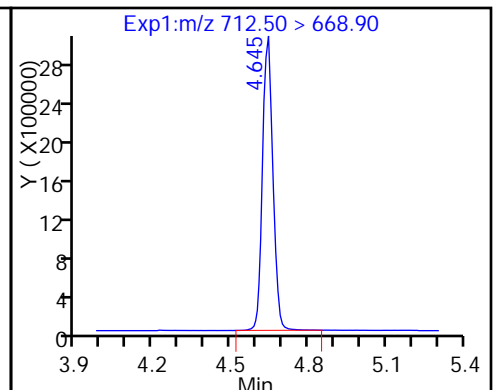


33 Perfluorotetradecanoic acid




D 34 13C2-PFHxDA



35 Perfluorohexadecanoic acid

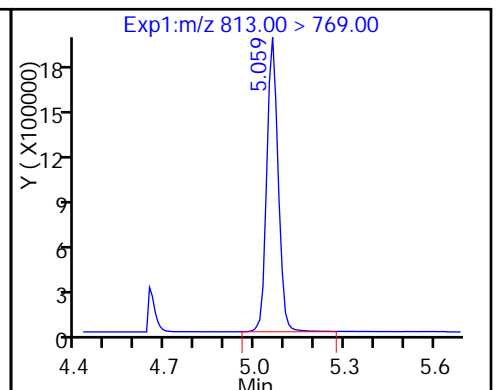

36 Perfluorooctadecanoic acid

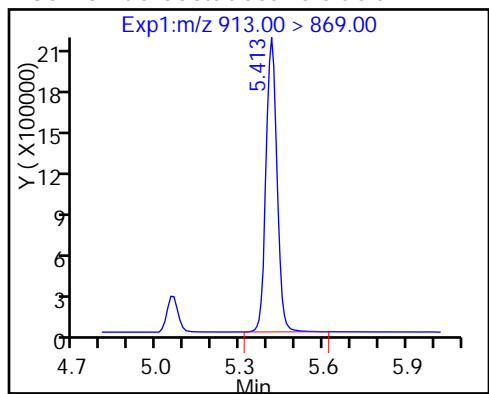

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_009.d
 Lims ID: IC L6
 Client ID:
 Sample Type: IC Calib Level: 6
 Inject. Date: 15-Dec-2016 13:06:46 ALS Bottle#: 42 Worklist Smp#: 9
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L6_b
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Sublist: chrom-A8_N*sub6
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 14:34:27 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 15-Dec-2016 13:51:28

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.537	1.534	0.003	14961055	43.0		86.0	920014	
1 Perfluorobutyric acid	212.90 > 169.00	1.537	1.535	0.002	1.000	42763611	167.4	83.7	246189	
D 4 13C5-PFPeA	267.90 > 223.00	1.813	1.810	0.003	10898820	41.0		81.9	1007026	
3 Perfluoropentanoic acid	262.90 > 219.00	1.813	1.810	0.003	1.000	34291076	159.4	79.7	297823	
5 Perfluorobutanesulfonic acid	298.90 > 80.00	1.852	1.848	0.004	1.000	50724469	130.5	73.8		
	298.90 > 99.00	1.842	1.848	-0.006	0.995	28243355	1.80(0.00-0.00)	73.8		
7 Perfluorohexanoic acid	313.00 > 269.00	2.096	2.096	0.0	1.000	33223923	172.9	86.4	549724	
D 6 13C2 PFHxA	315.00 > 270.00	2.096	2.097	-0.001	10345480	42.2		84.4	508201	
D 11 13C4-PFHpA	367.00 > 322.00	2.426	2.426	0.0	8564025	37.8		75.7	487796	
12 Perfluoroheptanoic acid	363.00 > 319.00	2.426	2.428	-0.002	1.000	30234194	180.3	90.2	213534	
9 Perfluorohexanesulfonic acid	399.00 > 80.00	2.444	2.431	0.013	1.000	46223186	163.6	89.9		
D 10 18O2 PFHxS	403.00 > 84.00	2.444	2.446	-0.002	12974829	39.7		83.9	628886	
D 14 13C4 PFOA	417.00 > 372.00	2.783	2.783	0.0	8380251	36.4		72.8	402245	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
15 Perfluorooctanoic acid										
413.00 > 369.00	2.783	2.783	0.0	1.000	30784387	183.1		91.5	229181	
413.00 > 169.00	2.783	2.783	0.0	1.000	20338648		1.51(0.90-1.10)	91.5	70063	
13 Perfluoroheptanesulfonic Acid										
449.00 > 80.00	2.791	2.790	0.001	1.000	38459925	166.5		87.5		
18 Perfluorooctane sulfonic acid										
499.00 > 80.00	2.977	3.118	-0.141	1.000	40073141	192.2		104	5896	
499.00 > 99.00	3.152	3.118	0.034	1.059	9632026		4.16(0.90-1.10)	104	407968	
D 17 13C4 PFOS										
503.00 > 80.00	3.152	3.151	0.001		10019454	40.3		84.2	105595	
D 19 13C5 PFNA										
468.00 > 423.00	3.152	3.153	-0.001		6718354	37.8		75.6	515582	
20 Perfluorononanoic acid										
463.00 > 419.00	3.160	3.155	0.005	1.000	24793148	193.9		96.9	307568	
D 21 13C8 FOSA										
506.00 > 78.00	3.491	3.488	0.003		16105707	41.9		83.9	486146	
22 Perfluorooctane Sulfonamide										
498.00 > 78.00	3.491	3.491	0.0	1.000	47803717	159.1		79.6	542400	
24 Perfluorodecanoic acid										
513.00 > 469.00	3.516	3.510	0.006	1.000	22616781	191.8		95.9	376094	
D 23 13C2 PFDA										
515.00 > 470.00	3.508	3.513	-0.005		6246112	39.7		79.4	243806	
26 Perfluorodecane Sulfonic acid										
599.00 > 80.00	3.819	3.822	-0.004	1.000	23952412	195.7		101		
28 Perfluoroundecanoic acid										
563.00 > 519.00	3.845	3.839	0.006	1.000	16852945	197.7		98.9	570796	
D 27 13C2 PFUnA										
565.00 > 520.00	3.845	3.842	0.003		4456593	38.0		76.0	208308	
D 30 13C2 PFDoA										
615.00 > 570.00	4.129	4.132	-0.003		4649092	41.9		83.8	168499	
29 Perfluorododecanoic acid										
613.00 > 569.00	4.136	4.136	0.0	1.000	17425873	204.2		102	228085	
31 Perfluorotridecanoic acid										
663.00 > 619.00	4.407	4.400	0.007	1.000	16038809	190.2		95.1	237459	
D 32 13C2-PFTeDA										
715.00 > 670.00	4.635	4.641	-0.006		9520749	41.9		83.7	374846	
33 Perfluorotetradecanoic acid										
712.50 > 668.90	4.635	4.642	-0.007	1.000	27310864	185.3		92.7	329988	
713.00 > 169.00	4.635	4.642	-0.007	1.000	4963804		5.50(0.00-0.00)	92.7	195544	
D 34 13C2-PFHxDA										
815.00 > 770.00	5.060	5.057	0.003		5190172	41.7		83.3	150380	
35 Perfluorohexadecanoic acid										
813.00 > 769.00	5.060	5.059	0.001	1.000	17754908	199.3		99.6	19037	
36 Perfluorooctadecanoic acid										
913.00 > 869.00	5.414	5.414	0.0	1.000	18392980	192.0		96.0	19845	

Reagents:

LCPFC-L6_00020

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_009.d

Injection Date: 15-Dec-2016 13:06:46

Instrument ID: A8_N

Lims ID: IC L6

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 42

Worklist Smp#: 9

Injection Vol: 2.0 ul

Dil. Factor: 1.0000













Method: A8_N

Limit Group: LC PFC_DOD ICAL


D 2 13C4 PFBA

1 Perfluorobutyric acid


D 4 13C5-PFPeA

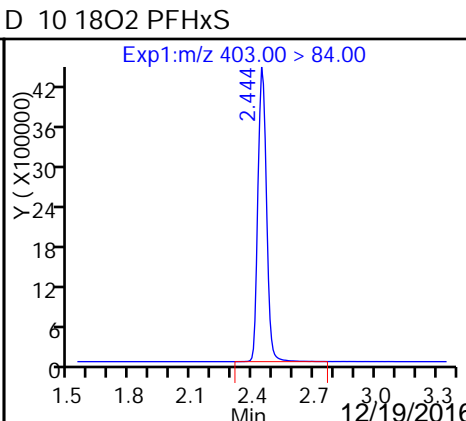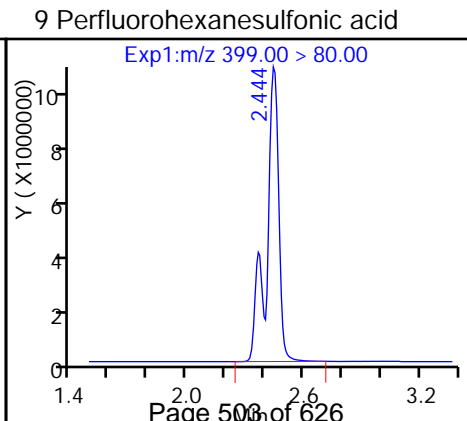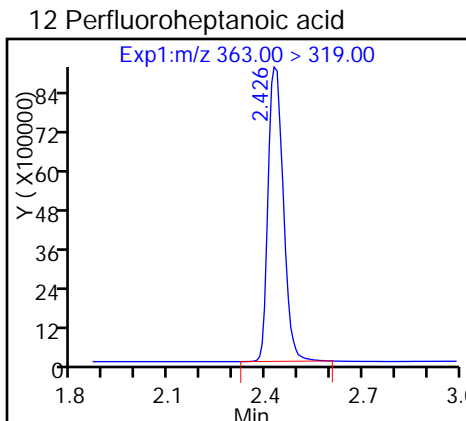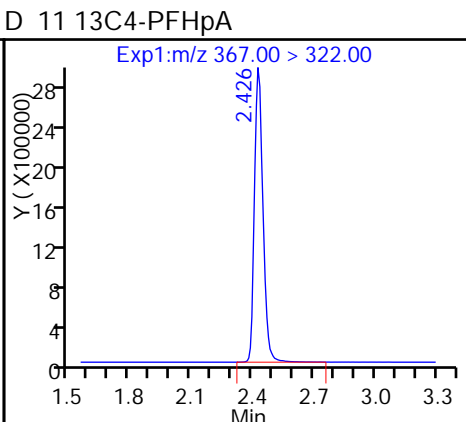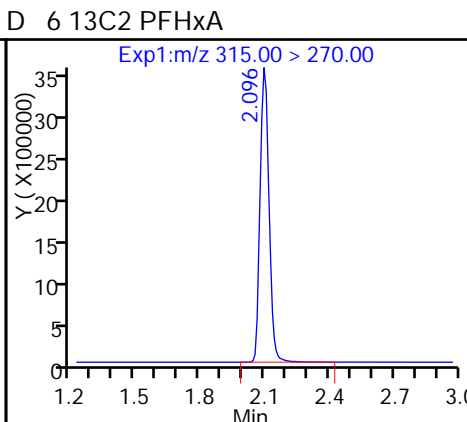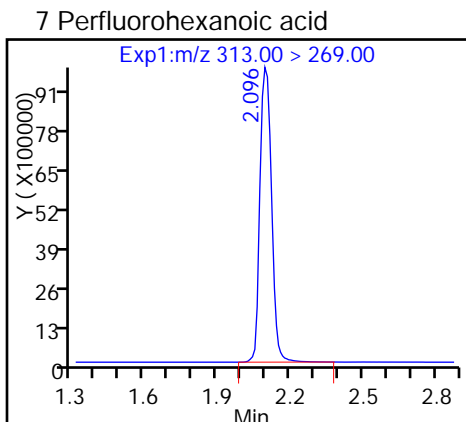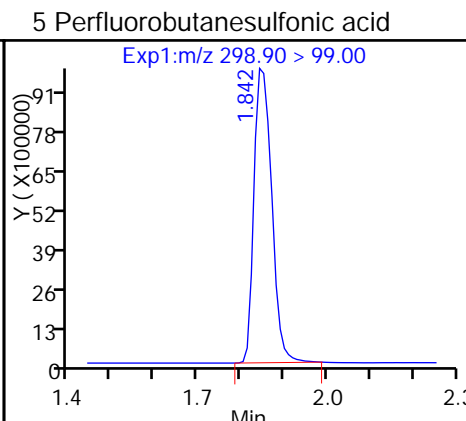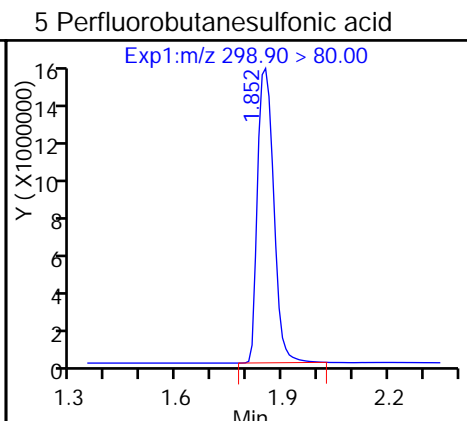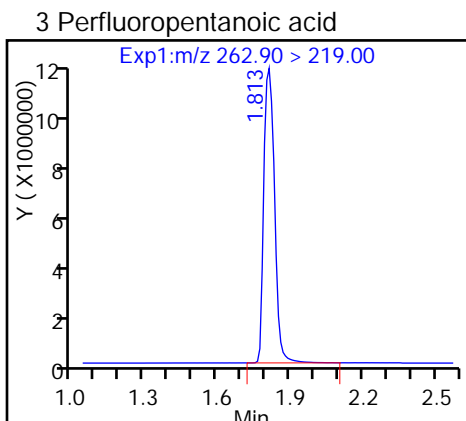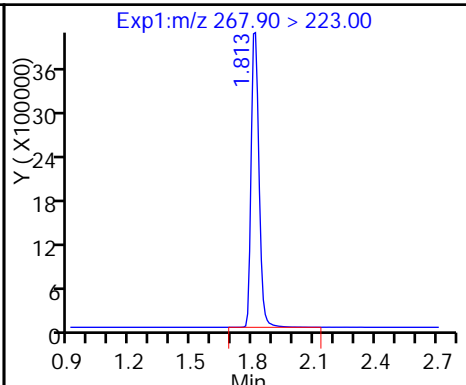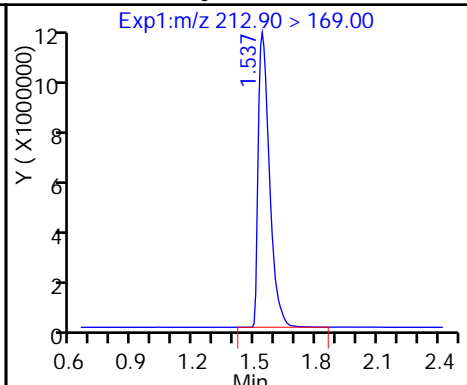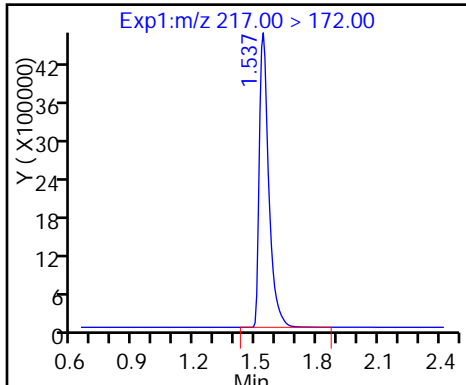


D 14 13C4 PFOA




15 Perfluorooctanoic acid




15 Perfluorooctanoic acid

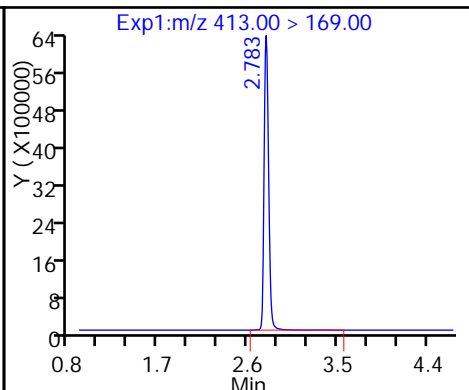


13 Perfluoroheptanesulfonic Acid




18 Perfluorooctane sulfonic acid




18 Perfluorooctane sulfonic acid




D 17 13C4 PFOS




D 19 13C5 PFNA




20 Perfluorononanoic acid

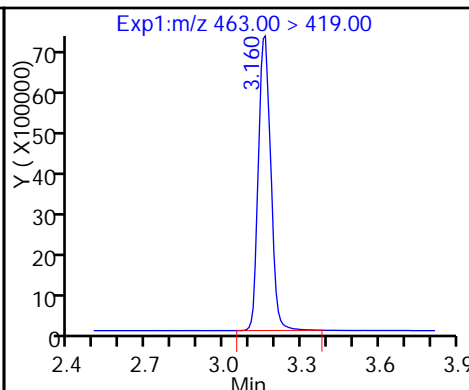


D 21 13C8 FOSA




22 Perfluorooctane Sulfonamide




24 Perfluorodecanoic acid




D 23 13C2 PFDA




26 Perfluorodecane Sulfonic acid




28 Perfluoroundecanoic acid

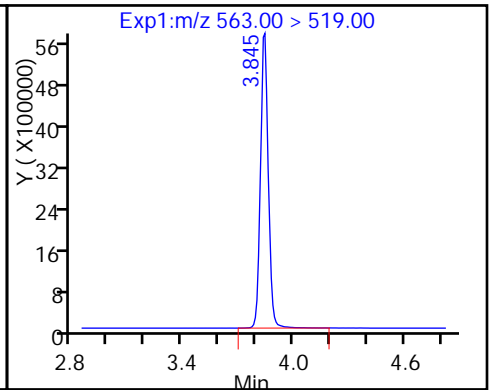


D 27 13C2 PFUa




D 30 13C2 PFDa

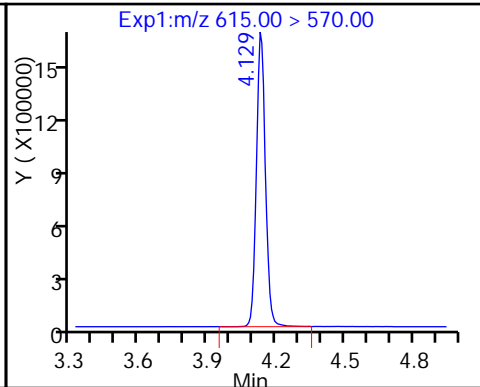


29 Perfluorododecanoic acid

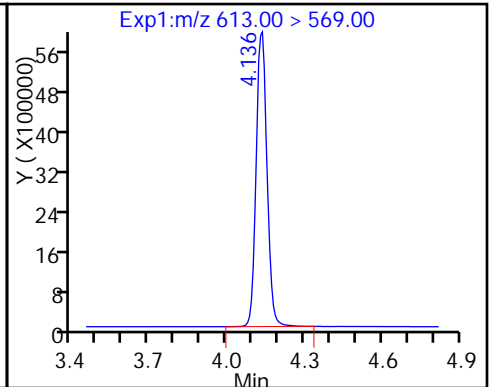


31 Perfluorotridecanoic acid




D 32 13C2-PFTeDA

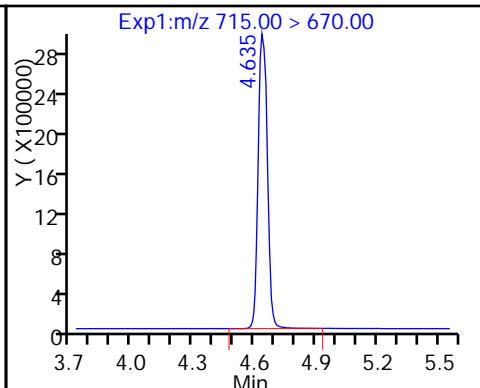


33 Perfluorotetradecanoic acid

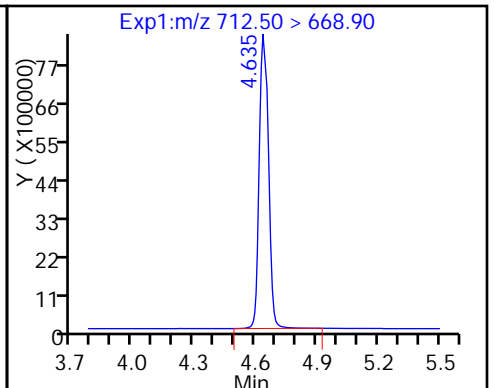


33 Perfluorotetradecanoic acid




D 34 13C2-PFHxDA

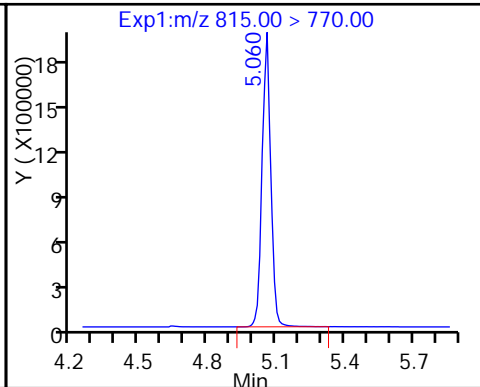

35 Perfluorohexadecanoic acid

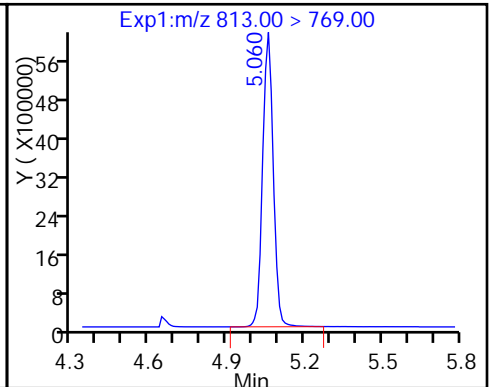

36 Perfluorooctadecanoic acid

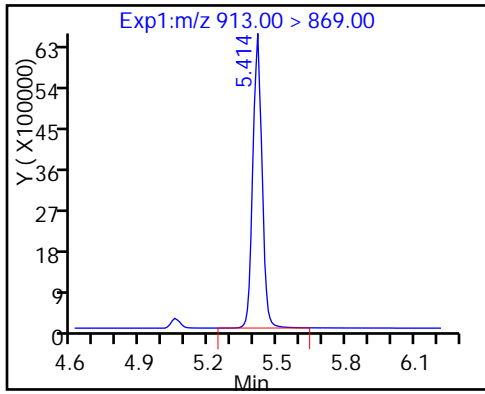

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016BB_013.d
 Lims ID: IC L1 Add-on
 Client ID:
 Sample Type: IC Calib Level: 1
 Inject. Date: 15-Dec-2016 13:41:05 ALS Bottle#: 46 Worklist Smp#: 13
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L1 ADD ON
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Sublist: chrom-A8_N*sub6
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 14:34:44 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 15-Dec-2016 16:37:58

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 47 M2-6:2FTS	429.00 > 409.00	2.760	2.767	-0.007	5352965	45.8		96.3		
48 Sodium 1H,1H,2H,2H-perfluorooctane	427.00 > 407.00	2.776	2.768	0.008	1.000	48011	0.4779	101		
43 Sodium 1H,1H,2H,2H-perfluorooctane	527.00 > 507.00	3.511	3.511	0.0	1.000	39808	0.4671	97.5		
D 42 M2-8:2FTS	529.00 > 509.00	3.511	3.513	-0.002	4817997	44.8		93.6		
D 45 d3-NMeFOSAA	573.00 > 419.00	3.684	3.676	0.008	3634985	48.3		96.5		
44 N-methyl perfluorooctane sulfonami	570.00 > 419.00	3.684	3.681	0.003	1.000	29823	0.4637	92.7		
D 46 d5-NEtFOSAA	589.00 > 419.00	3.848	3.842	0.006	3889792	49.6		99.3		
49 N-ethyl perfluorooctane sulfonamid	584.00 > 419.00	3.865	3.854	0.011	1.005	29965	0.4858	97.2		
D 52 d-N-MeFOSA-M	515.00 > 169.00	3.988	3.992	-0.004	4325034	45.5		91.0		
54 MeFOSA	512.00 > 169.00	3.998	3.999	-0.001	1.000	36069	0.4978	99.6		
D 51 d-N-EtFOSA-M	531.00 > 169.00	4.180	4.180	0.0	3792851	44.2		88.4		
53 N-ethylperfluoro-1-octanesulfonami	526.00 > 169.00	4.187	4.187	0.0	1.000	30993	0.4729	94.6		

Reagents:

LCPFC2-L1_00002

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016BB_013.d

Injection Date: 15-Dec-2016 13:41:05

Instrument ID: A8_N

Lims ID: IC L1 Add-on

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 46

Worklist Smp#: 13

Injection Vol: 2.0 ul




Dil. Factor: 1.0000

Method: A8_N

Limit Group: LC PFC_DOD ICAL

D 47 M2-6:2FTS




48 Sodium 1H,1H,2H,2H-perfluorooctane-43 Sodium 1H,1H,2H,2H-perfluorooctane

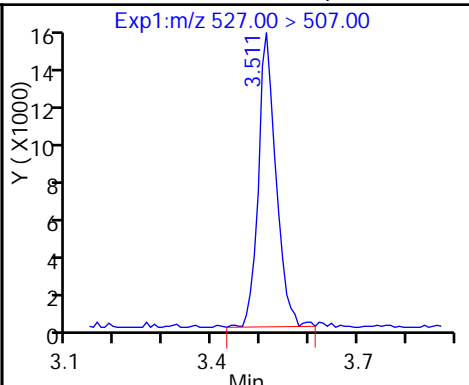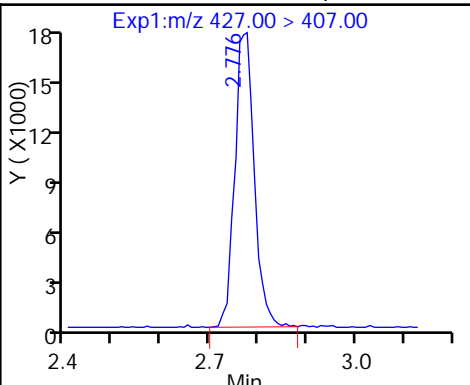

D 42 M2-8:2FTS




D 45 d3-NMeFOSAA

44 N-methyl perfluorooctane sulfonami

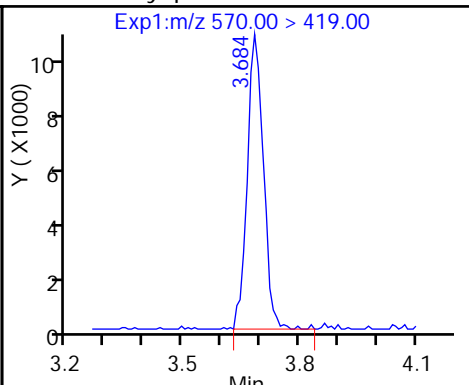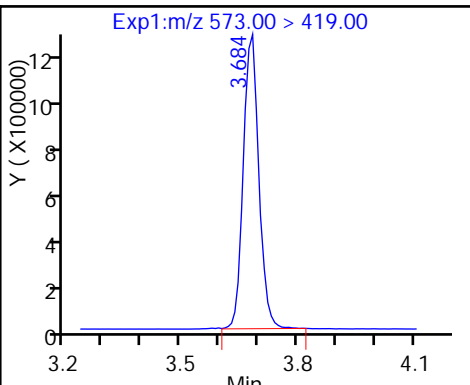

D 46 d5-NEtFOSAA




49 N-ethyl perfluorooctane sulfonamid D 52 d-N-MeFOSA-M

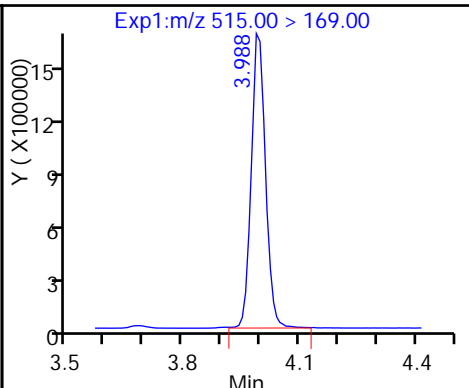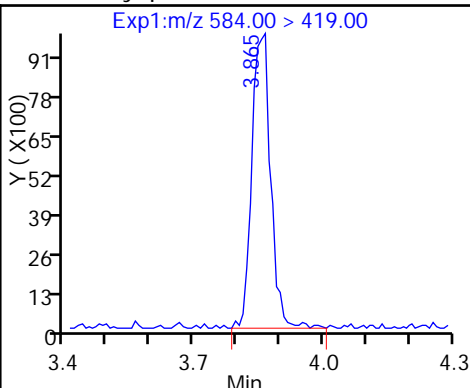

54 MeFOSA

D 51 d-N-EtFOSA-M

53 N-ethylperfluoro-1-octanesulfonami

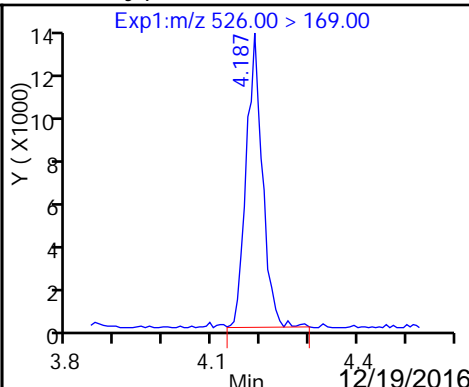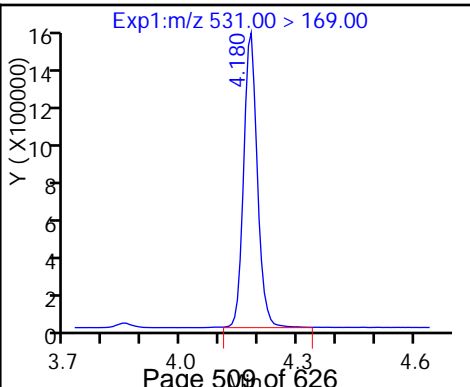

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_014.d
 Lims ID: IC L2 Add-on
 Client ID:
 Sample Type: IC Calib Level: 2
 Inject. Date: 15-Dec-2016 13:48:34 ALS Bottle#: 47 Worklist Smp#: 14
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L2 ADD ON
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Sublist: chrom-A8_N*sub6
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 14:34:46 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 15-Dec-2016 16:38:07

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 47 M2-6:2FTS	429.00 > 409.00	2.761	2.767	-0.006	5108306	43.7		91.9		
48 Sodium 1H,1H,2H,2H-perfluorooctane	427.00 > 407.00	2.761	2.768	-0.007	106947	1.12	1.000	118		
43 Sodium 1H,1H,2H,2H-perfluorooctane	527.00 > 507.00	3.502	3.511	-0.009	75731	0.9308	0.998	97.2		
D 42 M2-8:2FTS	529.00 > 509.00	3.511	3.513	-0.002	4599569	42.8		89.4		
D 45 d3-NMeFOSAA	573.00 > 419.00	3.673	3.676	-0.003	3559083	47.2		94.5		
44 N-methyl perfluorooctane sulfonami	570.00 > 419.00	3.673	3.681	-0.008	57389	0.9114	1.000	91.1		
D 46 d5-NEtFOSAA	589.00 > 419.00	3.838	3.842	-0.004	3757014	48.0		95.9		
49 N-ethyl perfluorooctane sulfonamid	584.00 > 419.00	3.855	3.854	0.001	53623	0.9000	1.005	90.0		
D 52 d-N-MeFOSA-M	515.00 > 169.00	3.987	3.992	-0.005	4639527	48.8		97.6		
54 MeFOSA	512.00 > 169.00	3.997	3.999	-0.002	70049	0.9013	1.000	90.1		
D 51 d-N-EtFOSA-M	531.00 > 169.00	4.172	4.180	-0.008	4109875	47.9		95.8		
53 N-ethylperfluoro-1-octanesulfonami	526.00 > 169.00	4.179	4.187	-0.008	62962	0.8865	1.000	88.7		

Reagents:

LCPFC2-L2_00002

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_014.d

Injection Date: 15-Dec-2016 13:48:34

Instrument ID: A8_N

Lims ID: IC L2 Add-on

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 47

Worklist Smp#: 14

Injection Vol: 2.0 ul




Dil. Factor: 1.0000

Method: A8_N

Limit Group: LC PFC_DOD ICAL

D 47 M2-6:2FTS




48 Sodium 1H,1H,2H,2H-perfluorooctane-4,3 Sodium 1H,1H,2H,2H-perfluorooctane

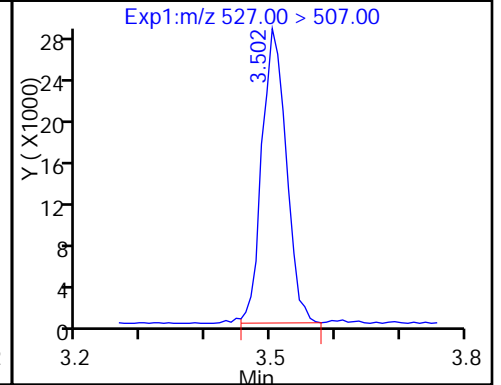

D 42 M2-8:2FTS




D 45 d3-NMeFOSAA

44 N-methyl perfluorooctane sulfonami

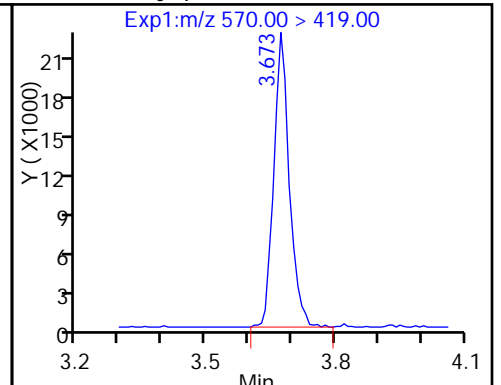

D 46 d5-NEtFOSAA




49 N-ethyl perfluorooctane sulfonamid D 52 d-N-MeFOSA-M

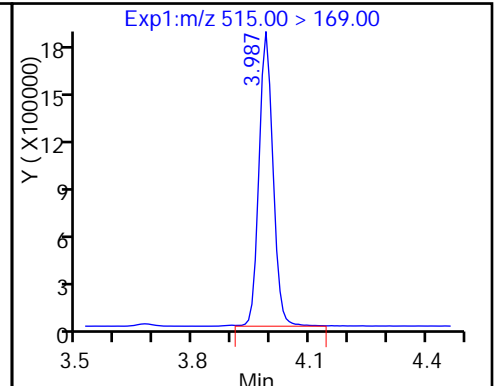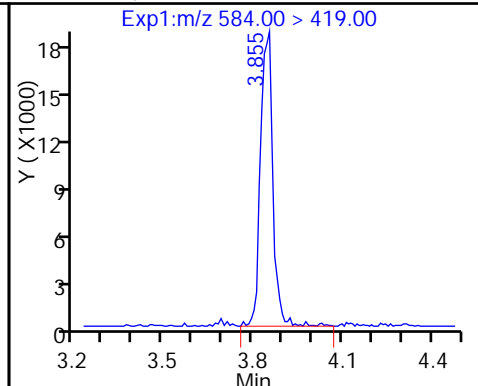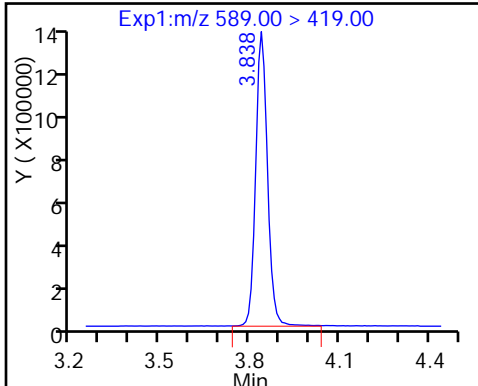

54 MeFOSA

D 51 d-N-EtFOSA-M

53 N-ethylperfluoro-1-octanesulfonami

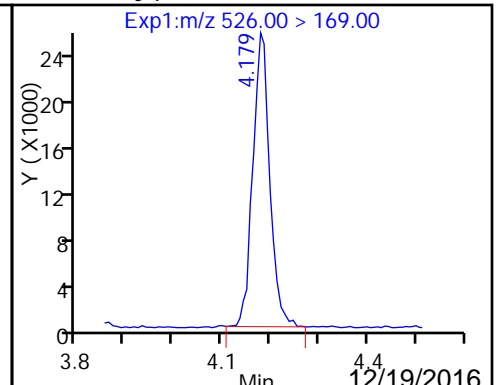

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_015.d
 Lims ID: IC L3 Add-on
 Client ID:
 Sample Type: IC Calib Level: 3
 Inject. Date: 15-Dec-2016 13:56:03 ALS Bottle#: 48 Worklist Smp#: 15
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L3 ADD ON
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Sublist: chrom-A8_N*sub6
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 14:34:48 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 15-Dec-2016 16:38:17

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 47 M2-6:2FTS	429.00 > 409.00	2.768	2.767	0.001	5570739	47.6		100		
48 Sodium 1H,1H,2H,2H-perfluorooctane	427.00 > 407.00	2.768	2.768	0.0	405060	3.87		81.7		
43 Sodium 1H,1H,2H,2H-perfluorooctane	527.00 > 507.00	3.511	3.511	0.0	398457	4.22		88.0		
D 42 M2-8:2FTS	529.00 > 509.00	3.511	3.513	-0.002	5342826	49.7		104		
D 45 d3-NMeFOSAA	573.00 > 419.00	3.673	3.676	-0.003	4014623	53.3		107		
44 N-methyl perfluorooctane sulfonami	570.00 > 419.00	3.683	3.681	0.002	285665	4.02		80.4		
D 46 d5-NEtFOSAA	589.00 > 419.00	3.838	3.842	-0.004	4235352	54.1		108		
49 N-ethyl perfluorooctane sulfonamid	584.00 > 419.00	3.847	3.854	-0.007	267721	3.99		79.7		
D 52 d-N-MeFOSA-M	515.00 > 169.00	3.987	3.992	-0.005	5121953	53.9		108		
54 MeFOSA	512.00 > 169.00	3.997	3.999	-0.002	343493	4.00		80.1		
D 51 d-N-EtFOSA-M	531.00 > 169.00	4.179	4.180	-0.001	4561882	53.2		106		
53 N-ethylperfluoro-1-octanesulfonami	526.00 > 169.00	4.186	4.187	-0.001	326877	4.15		82.9		

Reagents:

LCPFC2-L3_00002

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_015.d

Injection Date: 15-Dec-2016 13:56:03

Instrument ID: A8_N

Lims ID: IC L3 Add-on

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 48

Worklist Smp#: 15

Injection Vol: 2.0 ul




Dil. Factor: 1.0000

Method: A8_N

Limit Group: LC PFC_DOD ICAL

D 47 M2-6:2FTS




48 Sodium 1H,1H,2H,2H-perfluorooctane-4,3 Sodium 1H,1H,2H,2H-perfluorooctane

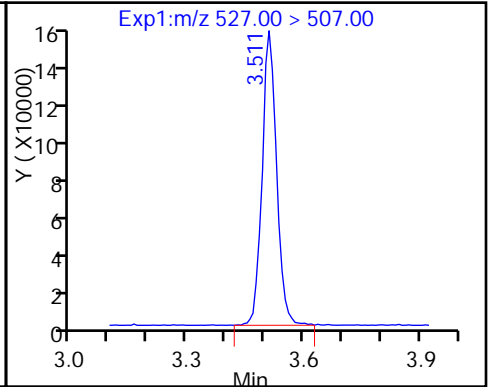

D 42 M2-8:2FTS




D 45 d3-NMeFOSAA

44 N-methyl perfluorooctane sulfonami

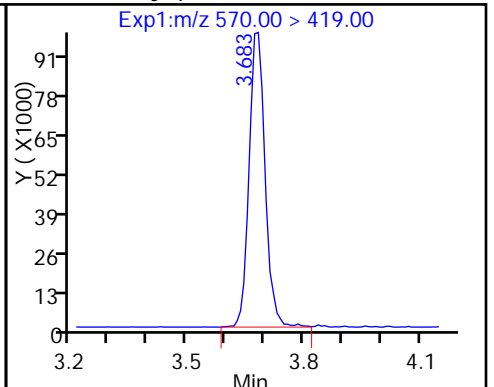

D 46 d5-NEtFOSAA




49 N-ethyl perfluorooctane sulfonamid D 52 d-N-MeFOSA-M

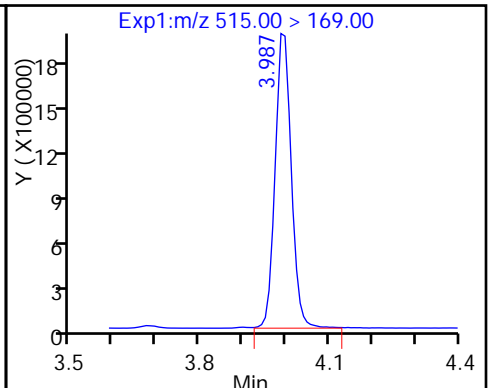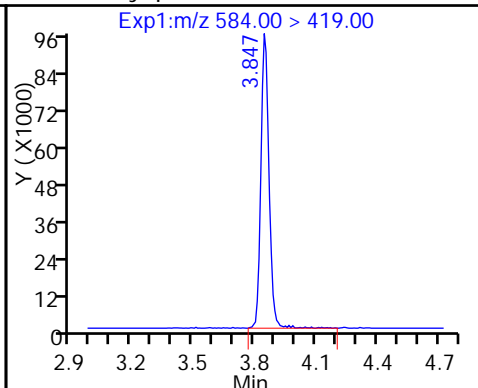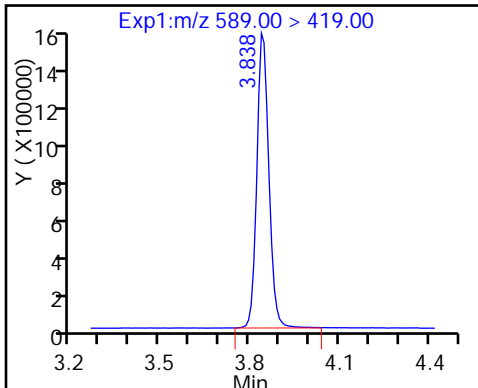

54 MeFOSA

D 51 d-N-EtFOSA-M

53 N-ethylperfluoro-1-octanesulfonami

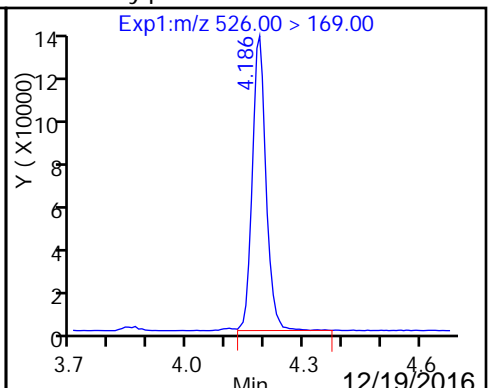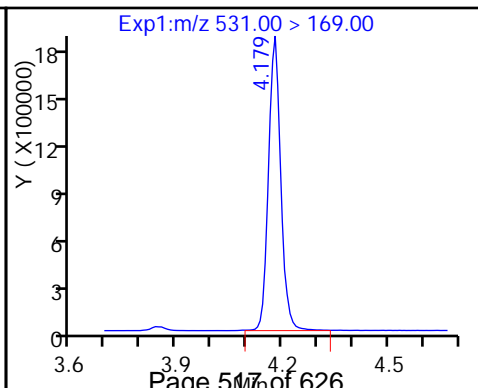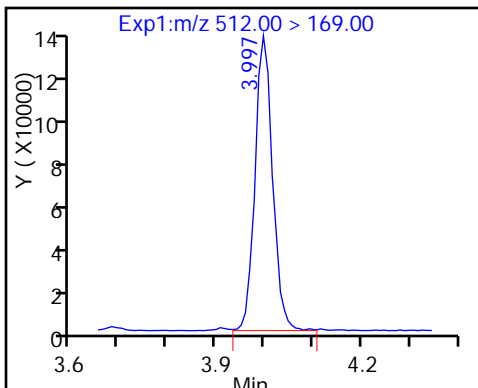

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_016.d
 Lims ID: IC L4 Add-on
 Client ID:
 Sample Type: IC Calib Level: 4
 Inject. Date: 15-Dec-2016 14:03:33 ALS Bottle#: 49 Worklist Smp#: 16
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L4 ADD ON
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Sublist: chrom-A8_N*sub6
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 14:34:49 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d

Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 15-Dec-2016 16:37:50

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
--------	----	--------	--------	--------	----------	--------------	---------------	------	-----	-------

D 47 M2-6:2FTS	429.00 > 409.00	2.767	2.767	0.0	6471813	55.3		116		
48 Sodium 1H,1H,2H,2H-perfluorooctane	427.00 > 407.00	2.767	2.768	-0.001	2416384	19.9		105		
43 Sodium 1H,1H,2H,2H-perfluorooctane	527.00 > 507.00	3.511	3.511	0.0	2224381	21.0		110		
D 42 M2-8:2FTS	529.00 > 509.00	3.511	3.513	-0.002	5984276	55.7		116		
D 45 d3-NMeFOSAA	573.00 > 419.00	3.673	3.676	-0.003	4379131	58.1		116		
44 N-methyl perfluorooctane sulfonami	570.00 > 419.00	3.683	3.681	0.002	1708231	22.0		110		
D 46 d5-NEtFOSAA	589.00 > 419.00	3.838	3.842	-0.004	4410456	56.3		113		
49 N-ethyl perfluorooctane sulfonamid	584.00 > 419.00	3.847	3.854	-0.007	1518918	21.7		109		
D 52 d-N-MeFOSA-M	515.00 > 169.00	3.997	3.992	0.005	5263980	55.4		111		
54 MeFOSA	512.00 > 169.00	3.997	3.999	-0.002	1946985	22.1		110		
D 51 d-N-EtFOSA-M	531.00 > 169.00	4.179	4.180	-0.001	4672820	54.5		109		
53 N-ethylperfluoro-1-octanesulfonami	526.00 > 169.00	4.186	4.187	-0.001	1813178	22.5		112		

Reagents:

LCPFC2-L4_00003

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_016.d

Injection Date: 15-Dec-2016 14:03:33

Instrument ID: A8_N

Lims ID: IC L4 Add-on

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 49

Worklist Smp#: 16

Injection Vol: 2.0 ul




Dil. Factor: 1.0000

Method: A8_N

Limit Group: LC PFC_DOD ICAL

D 47 M2-6:2FTS




48 Sodium 1H,1H,2H,2H-perfluorooctane-43 Sodium 1H,1H,2H,2H-perfluorooctane

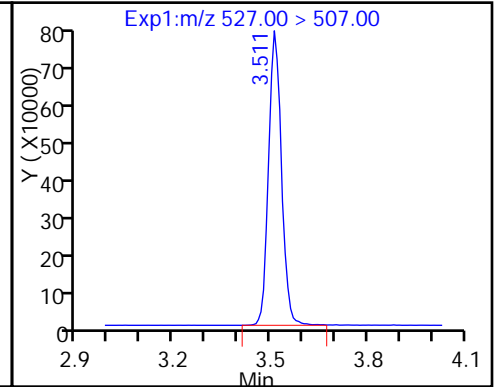

D 42 M2-8:2FTS




D 45 d3-NMeFOSAA

44 N-methyl perfluorooctane sulfonami

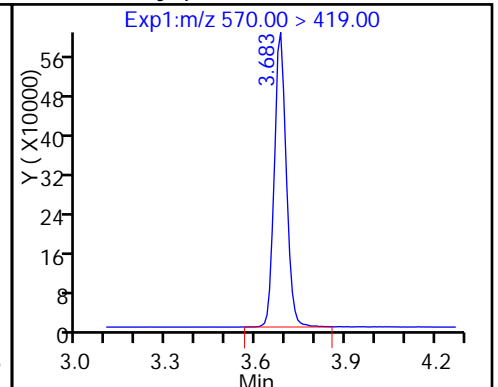

D 46 d5-NEtFOSAA




49 N-ethyl perfluorooctane sulfonamid D 52 d-N-MeFOSA-M

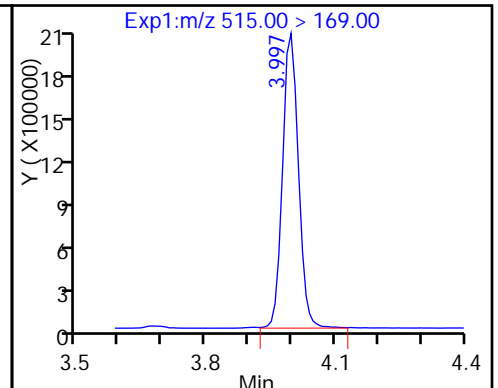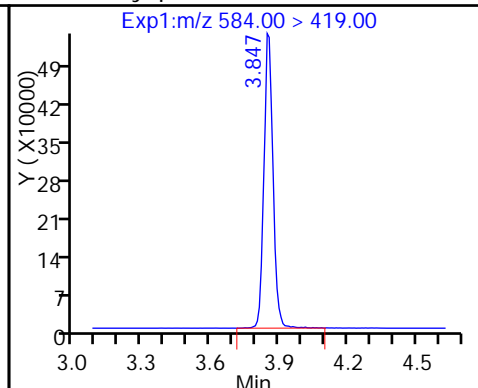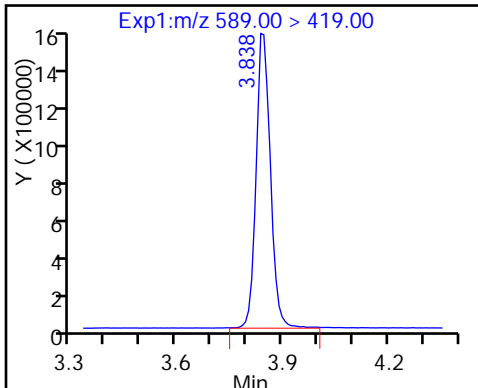

54 MeFOSA

D 51 d-N-EtFOSA-M

53 N-ethylperfluoro-1-octanesulfonami

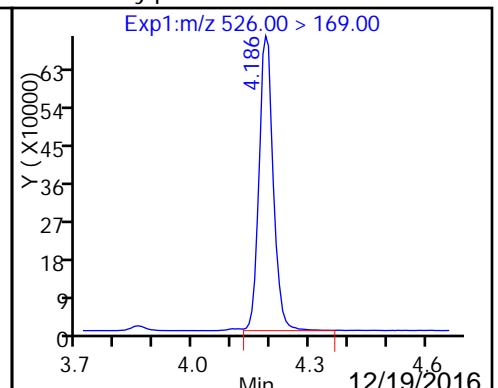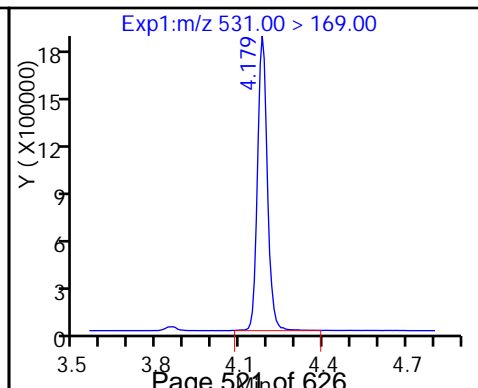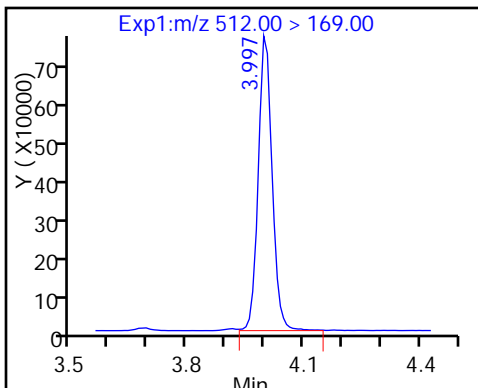

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_017.d
 Lims ID: IC L5 Add-on
 Client ID:
 Sample Type: IC Calib Level: 5
 Inject. Date: 15-Dec-2016 14:11:03 ALS Bottle#: 50 Worklist Smp#: 17
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L5 ADD ON
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Sublist: chrom-A8_N*sub6
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 14:34:51 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 15-Dec-2016 16:38:32

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 47 M2-6:2FTS	429.00 > 409.00	2.767	2.767	0.0	5259120	45.0		94.6		
48 Sodium 1H,1H,2H,2H-perfluorooctane	427.00 > 407.00	2.767	2.768	-0.001 1.000	5166665	52.3		110		
43 Sodium 1H,1H,2H,2H-perfluorooctane	527.00 > 507.00	3.512	3.511	0.001 0.998	4815680	56.9		119		
D 42 M2-8:2FTS	529.00 > 509.00	3.520	3.513	0.007	4786038	44.5		93.0		
D 45 d3-NMeFOSAA	573.00 > 419.00	3.675	3.676	-0.001	3422485	45.4		90.9		
44 N-methyl perfluorooctane sulfonami	570.00 > 419.00	3.684	3.681	0.003 1.003	3741936	61.8		124		
D 46 d5-NEtFOSAA	589.00 > 419.00	3.848	3.842	0.006	3486329	44.5		89.0		
49 N-ethyl perfluorooctane sulfonamid	584.00 > 419.00	3.857	3.854	0.003 1.002	3414301	61.8		124		
D 52 d-N-MeFOSA-M	515.00 > 169.00	3.999	3.992	0.007	4512300	47.5		94.9		
54 MeFOSA	512.00 > 169.00	3.999	3.999	0.0 1.000	4407328	58.3		117		
D 51 d-N-EtFOSA-M	531.00 > 169.00	4.182	4.180	0.002	4149228	48.4		96.7		
53 N-ethylperfluoro-1-octanesulfonami	526.00 > 169.00	4.189	4.187	0.002 1.000	4264314	59.5		119		

Reagents:

LCPFC2-L5_00002

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_017.d

Injection Date: 15-Dec-2016 14:11:03

Instrument ID: A8_N

Lims ID: IC L5 Add-on

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 50

Worklist Smp#: 17

Injection Vol: 2.0 ul




Dil. Factor: 1.0000

Method: A8_N

Limit Group: LC PFC_DOD ICAL

D 47 M2-6:2FTS




48 Sodium 1H,1H,2H,2H-perfluorooctane sulfonamide

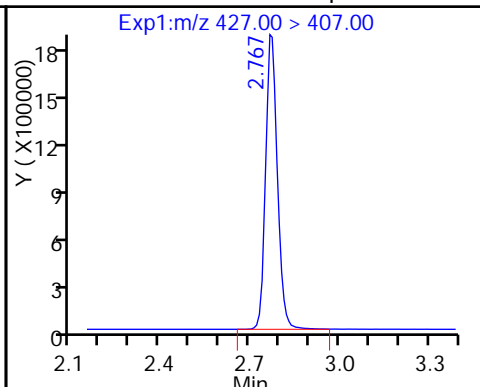

D 42 M2-8:2FTS

D 45 d3-NMeFOSAA




44 N-methyl perfluorooctane sulfonamide

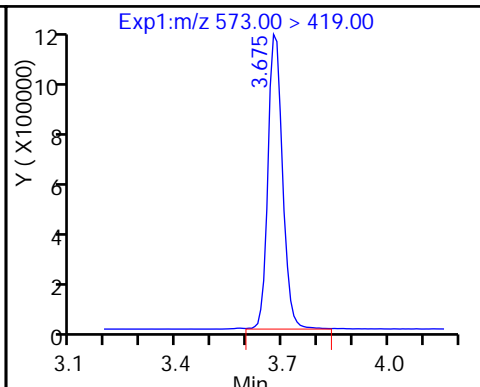

D 46 d5-NEtFOSAA

49 N-ethyl perfluorooctane sulfonamide




D 52 d-N-MeFOSA-M

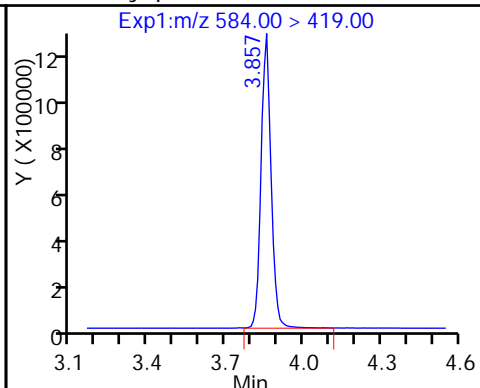

54 MeFOSA

D 51 d-N-EtFOSA-M

53 N-ethylperfluoro-1-octanesulfonamide

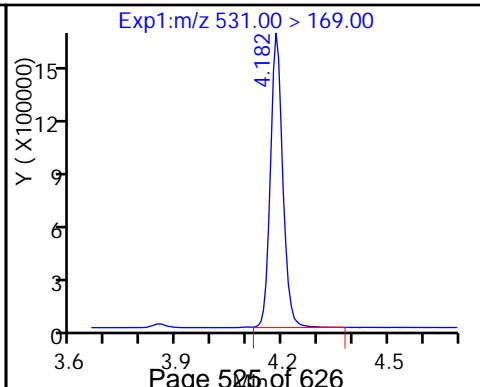

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Lims ID: IC L6 Add-on
 Client ID:
 Sample Type: IC Calib Level: 6
 Inject. Date: 15-Dec-2016 14:18:33 ALS Bottle#: 51 Worklist Smp#: 18
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L6 ADD ON
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Sublist: chrom-A8_N*sub6
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 14:34:52 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 15-Dec-2016 16:38:39

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 47 M2-6:2FTS	429.00 > 409.00	2.776	2.767	0.009	5576967	47.7		100		
48 Sodium 1H,1H,2H,2H-perfluorooctane	427.00 > 407.00	2.769	2.768	0.001	16907459	161.5		85.2		
43 Sodium 1H,1H,2H,2H-perfluorooctane	527.00 > 507.00	3.516	3.511	0.005	16111959	170.3		88.9		
D 42 M2-8:2FTS	529.00 > 509.00	3.516	3.513	0.003	5348797	49.8		104		
D 45 d3-NMeFOSAA	573.00 > 419.00	3.680	3.676	0.004	3587176	47.6		95.2		
44 N-methyl perfluorooctane sulfonami	570.00 > 419.00	3.680	3.681	-0.001	12924122	203.6		102		
D 46 d5-NEtFOSAA	589.00 > 419.00	3.845	3.842	0.003	3725902	47.6		95.1		
49 N-ethyl perfluorooctane sulfonamid	584.00 > 419.00	3.853	3.854	-0.001	11938061	202.0		101		
D 52 d-N-MeFOSA-M	515.00 > 169.00	3.995	3.992	0.003	4658153	49.0		98.0		
54 MeFOSA	512.00 > 169.00	4.004	3.999	0.005	16114020	206.5		103		
D 51 d-N-EtFOSA-M	531.00 > 169.00	4.186	4.180	0.006	4448546	51.9		104		
53 N-ethylperfluoro-1-octanesulfonami	526.00 > 169.00	4.193	4.187	0.006	15780196	205.3		103		

Reagents:

LCPFC2-L6_00002

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d

Injection Date: 15-Dec-2016 14:18:33

Instrument ID: A8_N

Lims ID: IC L6 Add-on

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 51

Worklist Smp#: 18

Injection Vol: 2.0 ul




Dil. Factor: 1.0000

Method: A8_N

Limit Group: LC PFC_DOD ICAL

D 47 M2-6:2FTS




48 Sodium 1H,1H,2H,2H-perfluorooctane-43 Sodium 1H,1H,2H,2H-perfluorooctane



D 42 M2-8:2FTS




D 45 d3-NMeFOSAA

44 N-methyl perfluorooctane sulfonami



D 46 d5-NEtFOSAA




49 N-ethyl perfluorooctane sulfonamid D 52 d-N-MeFOSA-M

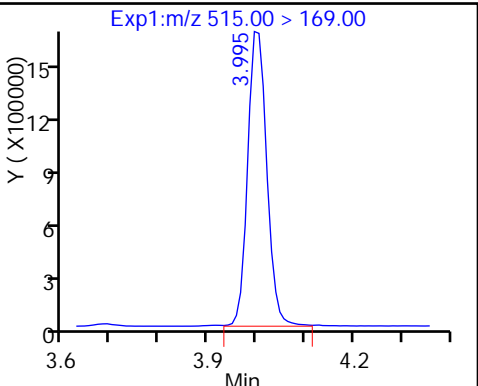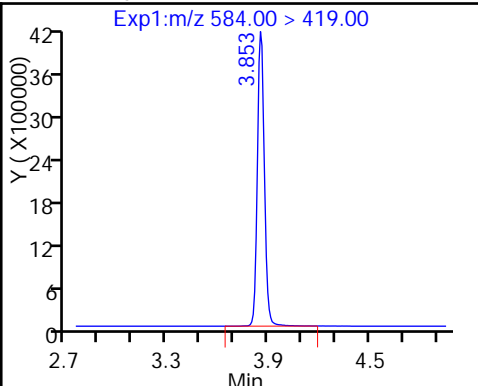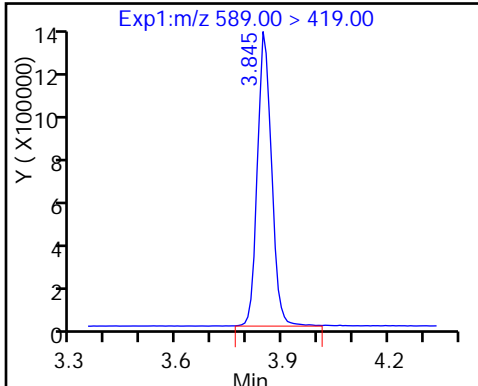

54 MeFOSA

D 51 d-N-EtFOSA-M

53 N-ethylperfluoro-1-octanesulfonami



FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Lab Sample ID: ICV 320-142379/11 Calibration Date: 12/15/2016 13:21
 Instrument ID: A8_N Calib Start Date: 12/15/2016 12:29
 GC Column: Acquity ID: 2.10 (mm) Calib End Date: 12/15/2016 14:18
 Lab File ID: 15DEC2016B_011.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanoic acid (PFBA)	AveID	0.8537	0.8479		49.7	50.0	-0.7	25.0
Perfluoropentanoic acid (PFPeA)	AveID	0.9868	0.9654		48.9	50.0	-2.2	25.0
Perfluorobutanesulfonic acid (PFBS)	AveID	1.417	1.478		46.2	44.3	4.3	25.0
Perfluorohexanoic acid (PFHxA)	AveID	0.9288	0.9123		49.1	50.0	-1.8	25.0
Perfluoroheptanoic acid (PFHpA)	AveID	0.9788	0.9679		49.4	50.0	-1.1	25.0
Perfluorohexanesulfonic acid (PFHxS)	AveID	1.030	0.9556		43.8	47.3	-7.2	25.0
Perfluorooctanoic acid (PFOA)	AveID	1.003	1.000		49.9	50.0	-0.3	25.0
Perfluoroheptanesulfonic Acid (PFHpS)	AveID	1.102	1.160		50.1	47.6	5.2	25.0
Perfluorononanoic acid (PFNA)	AveID	0.9518	0.9360		49.2	50.0	-1.7	25.0
Perfluorooctanesulfonic acid (PFOS)	AveID	0.9945	0.9040		43.4	47.8	-9.1	25.0
Perfluorooctane Sulfonamide (FOSA)	AveID	0.9327	0.9182		49.2	50.0	-1.5	25.0
Perfluorodecanoic acid (PFDA)	AveID	0.9438	0.9109		48.3	50.0	-3.5	25.0
Perfluorodecanesulfonic acid (PFDS)	AveID	0.5840	0.5921		48.9	48.3	1.4	25.0
Perfluoroundecanoic acid (PFUnA)	AveID	0.9563	0.9285		48.5	50.0	-2.9	25.0
Perfluorododecanoic acid (PFDoA)	AveID	0.9180	0.8958		48.8	50.0	-2.4	25.0
Perfluorotridecanoic Acid (PFTriA)	AveID	0.9069	0.9189		50.7	50.0	1.3	25.0
Perfluorotetradecanoic acid (PFTeA)	AveID	1.585	1.555		49.1	50.0	-1.9	25.0
Perfluoro-n-hexadecanoic acid (PFHxDA)	L1ID		0.9309		48.2	50.0	-3.7	25.0
Perfluoro-n-octadecanoic acid (PFODA)	AveID	1.030	0.8547		41.5	50.0	-17.0	25.0
13C4 PFBA	Ave	347743	335296		48.2	50.0	-3.6	50.0
13C5 PFPeA	Ave	266072	251719		47.3	50.0	-5.4	50.0
13C2 PFHxA	Ave	245110	240514		49.1	50.0	-1.9	50.0
13C4-PFHpA	Ave	226344	215455		47.6	50.0	-4.8	50.0
18O2 PFHxS	Ave	326976	320282		46.3	47.3	-2.0	50.0
13C4 PFOA	Ave	230362	219488		47.6	50.0	-4.7	50.0
13C4 PFOS	Ave	248847	244549		47.0	47.8	-1.7	50.0
13C5 PFNA	Ave	177687	171464		48.2	50.0	-3.5	50.0
13C8 FOSA	Ave	384141	381142		49.6	50.0	-0.8	50.0
13C2 PFDA	Ave	157302	151370		48.1	50.0	-3.8	50.0
13C2 PFUnA	Ave	117250	116265		49.6	50.0	-0.8	50.0
13C2 PFDoA	Ave	110957	105818		47.7	50.0	-4.6	50.0
13C2-PFTeA	Ave	227387	214066		47.1	50.0	-5.9	50.0
13C2-PFHxDA	Ave	124568	118207		47.4	50.0	-5.1	50.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_011.d
 Lims ID: ICV
 Client ID:
 Sample Type: ICV
 Inject. Date: 15-Dec-2016 13:21:44 ALS Bottle#: 44 Worklist Smp#: 11
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: ICV_b
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Sublist:

Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 14:41:15 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d

Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 15-Dec-2016 13:56:27

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.533	1.534	-0.001	16764776	48.2		96.4	1068457	
1 Perfluorobutyric acid	212.90 > 169.00	1.541	1.535	0.006	14214515	49.7			107570	
D 4 13C5-PFPeA	267.90 > 223.00	1.810	1.810	0.0	12585925	47.3		94.6	1186150	
3 Perfluoropentanoic acid	262.90 > 219.00	1.810	1.810	0.0	12149802	48.9			115067	
5 Perfluorobutanesulfonic acid	298.90 > 80.00	1.848	1.848	0.0	20951066	46.2				
	298.90 > 99.00	1.848	1.848	0.0	9653760		2.17(0.00-0.00)			
7 Perfluorohexanoic acid	313.00 > 269.00	2.100	2.096	0.004	10971106	49.1			243419	
D 6 13C2 PFHxA	315.00 > 270.00	2.100	2.097	0.003	12025693	49.1		98.1	480449	
D 11 13C4-PFHpA	367.00 > 322.00	2.425	2.426	-0.001	10772772	47.6		95.2	728689	
12 Perfluoroheptanoic acid	363.00 > 319.00	2.433	2.428	0.005	10426957	49.4			97176	
9 Perfluorohexanesulfonic acid	399.00 > 80.00	2.449	2.431	0.018	14462013	43.8				
D 10 18O2 PFHxS	403.00 > 84.00	2.449	2.446	0.003	15149334	46.3		98.0	878432	
D 14 13C4 PFOA	417.00 > 372.00	2.785	2.783	0.002	10974392	47.6		95.3	756643	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
15 Perfluorooctanoic acid										
413.00 > 369.00	2.785	2.783	0.002	1.000	10976634	49.9			90975	
413.00 > 169.00	2.793	2.783	0.010	1.003	6473539		1.70(0.90-1.10)		241007	
13 Perfluoroheptanesulfonic Acid										
449.00 > 80.00	2.793	2.790	0.003	1.000	13497259	50.1				
18 Perfluorooctane sulfonic acid										
499.00 > 80.00	3.162	3.118	0.044	1.000	10556247	43.4			368282	
499.00 > 99.00	3.154	3.118	0.036	0.997	2582918		4.09(0.90-1.10)		118191	
D 17 13C4 PFOS										
503.00 > 80.00	3.162	3.151	0.011		11689450	47.0		98.3	325285	
D 19 13C5 PFNA										
468.00 > 423.00	3.162	3.153	0.009		8573219	48.2		96.5	485749	
20 Perfluorononanoic acid										
463.00 > 419.00	3.162	3.155	0.007	1.000	8024621	49.2			123355	
D 21 13C8 FOSA										
506.00 > 78.00	3.495	3.488	0.007		19057117	49.6		99.2	610709	
22 Perfluorooctane Sulfonamide										
498.00 > 78.00	3.495	3.491	0.004	1.000	17498900	49.2			383568	
24 Perfluorodecanoic acid										
513.00 > 469.00	3.520	3.510	0.010	1.000	6894043	48.3			189508	
D 23 13C2 PFDA										
515.00 > 470.00	3.520	3.513	0.007		7568491	48.1		96.2	377092	
26 Perfluorodecane Sulfonic acid										
599.00 > 80.00	3.830	3.822	0.008	1.000	6986242	48.9				
28 Perfluoroundecanoic acid										
563.00 > 519.00	3.848	3.839	0.009	1.000	5397748	48.5			115044	
D 27 13C2 PFUnA										
565.00 > 520.00	3.848	3.842	0.006		5813248	49.6		99.2	413801	
D 30 13C2 PFDoA										
615.00 > 570.00	4.139	4.132	0.007		5290885	47.7		95.4	272661	
29 Perfluorododecanoic acid										
613.00 > 569.00	4.139	4.136	0.003	1.000	4739775	48.8			99907	
31 Perfluorotridecanoic acid										
663.00 > 619.00	4.411	4.400	0.011	1.000	4861713	50.7			113110	
D 32 13C2-PFTeDA										
715.00 > 670.00	4.642	4.641	0.001		10703301	47.1		94.1	614243	
33 Perfluorotetradecanoic acid										
712.50 > 668.90	4.652	4.642	0.010	1.000	8229099	49.1			142471	
713.00 > 169.00	4.642	4.642	0.0	0.998	1339943		6.14(0.00-0.00)		99778	
D 34 13C2-PFHxDA										
815.00 > 770.00	5.058	5.057	0.001		5910325	47.4		94.9	128290	
35 Perfluorohexadecanoic acid										
813.00 > 769.00	5.058	5.059	-0.001	1.000	4925242	48.2			4012	
36 Perfluorooctadecanoic acid										
913.00 > 869.00	5.421	5.414	0.007	1.000	4522136	41.5			4448	

Reagents:

LCPFCIC_00020

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_011.d

Injection Date: 15-Dec-2016 13:21:44

Instrument ID: A8_N

Lims ID: ICV

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 44

Worklist Smp#: 11

Injection Vol: 2.0 ul

Dil. Factor: 1.0000













Method: A8_N

Limit Group: LC PFC_DOD ICAL


D 2 13C4 PFBA

1 Perfluorobutyric acid


D 4 13C5-PFPeA

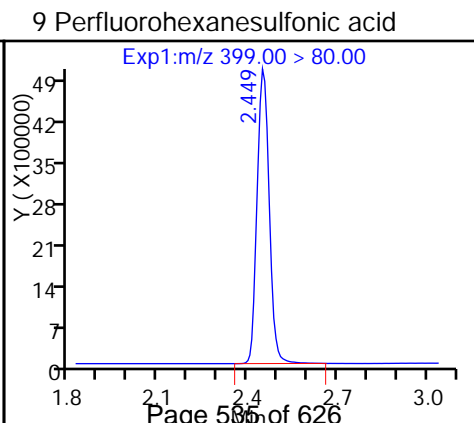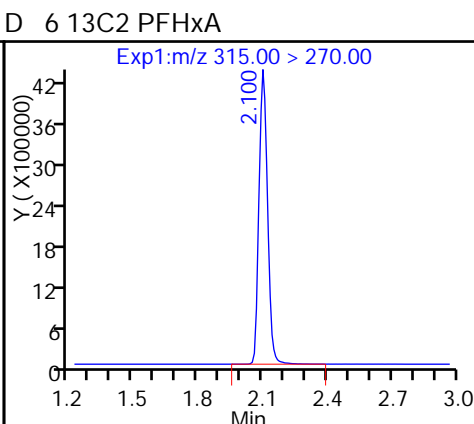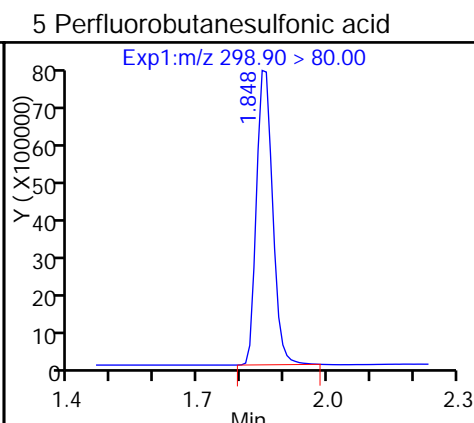


D 14 13C4 PFOA




15 Perfluorooctanoic acid




15 Perfluorooctanoic acid




13 Perfluoroheptanesulfonic Acid




18 Perfluorooctane sulfonic acid




18 Perfluorooctane sulfonic acid




D 17 13C4 PFOS




D 19 13C5 PFNA




20 Perfluorononanoic acid




D 21 13C8 FOSA




22 Perfluorooctane Sulfonamide




24 Perfluorodecanoic acid




D 23 13C2 PFDA




26 Perfluorodecane Sulfonic acid

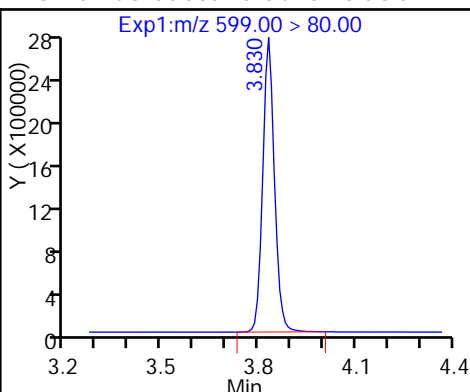


28 Perfluoroundecanoic acid

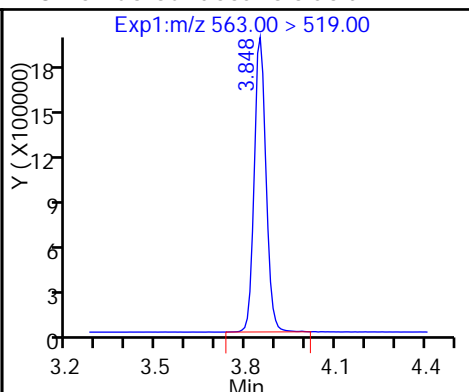


D 27 13C2 PFUa




D 30 13C2 PFDa




29 Perfluorododecanoic acid




31 Perfluorotridecanoic acid




D 32 13C2-PFTeDA




33 Perfluorotetradecanoic acid

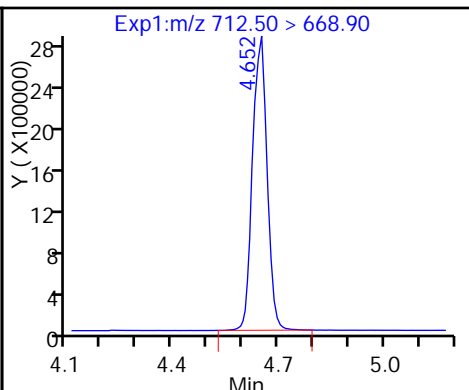


33 Perfluorotetradecanoic acid




D 34 13C2-PFHxDA



35 Perfluorohexadecanoic acid



36 Perfluorooctadecanoic acid

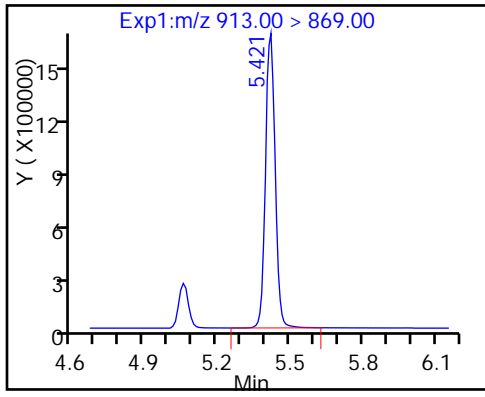

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Lab Sample ID: CCV 320-142379/27 Calibration Date: 12/15/2016 16:09
 Instrument ID: A8_N Calib Start Date: 12/15/2016 12:29
 GC Column: Acquity ID: 2.10 (mm) Calib End Date: 12/15/2016 14:18
 Lab File ID: 15DEC2016B_027.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanoic acid (PFBA)	AveID	0.8537	0.9551		22.4	20.0	11.9	25.0
Perfluoropentanoic acid (PFPeA)	AveID	0.9868	1.058		21.4	20.0	7.2	25.0
Perfluorobutanesulfonic acid (PFBS)	AveID	1.417	1.688		21.1	17.7	19.1	25.0
Perfluorohexanoic acid (PFHxA)	AveID	0.9288	0.9622		20.7	20.0	3.6	25.0
Perfluoroheptanoic acid (PFHpA)	AveID	0.9788	1.022		20.9	20.0	4.5	25.0
Perfluorohexanesulfonic acid (PFHxS)	AveID	1.030	1.052		18.6	18.2	2.1	25.0
Perfluoroheptanesulfonic Acid (PFHpS)	AveID	1.102	1.185		20.5	19.0	7.6	25.0
Perfluorooctanoic acid (PFOA)	AveID	1.003	1.072		21.4	20.0	6.8	25.0
Perfluorooctanesulfonic acid (PFOS)	AveID	0.9945	1.038		19.4	18.6	4.3	25.0
Perfluorononanoic acid (PFNA)	AveID	0.9518	0.9773		20.5	20.0	2.7	25.0
Perfluorooctane Sulfonamide (FOSA)	AveID	0.9327	1.022		21.9	20.0	9.6	25.0
Perfluorodecanoic acid (PFDA)	AveID	0.9438	0.9932		21.0	20.0	5.2	25.0
Perfluorodecanesulfonic acid (PFDS)	AveID	0.5840	0.6273		20.7	19.3	7.4	25.0
Perfluoroundecanoic acid (PFUnA)	AveID	0.9563	1.012		21.2	20.0	5.8	25.0
Perfluorododecanoic acid (PFDoA)	AveID	0.9180	0.9630		21.0	20.0	4.9	25.0
Perfluorotridecanoic Acid (PFTriA)	AveID	0.9069	0.9217		20.3	20.0	1.6	25.0
Perfluorotetradecanoic acid (PFTeA)	AveID	1.585	1.400		17.7	20.0	-11.7	25.0
Perfluoro-n-hexadecanoic acid (PFHxDA)	L1ID		0.9851		20.1	20.0	0.4	25.0
Perfluoro-n-octadecanoic acid (PFODA)	AveID	1.030	1.113		21.6	20.0	8.1	25.0
13C4 PFBA	Ave	347743	340235		48.9	50.0	-2.2	50.0
13C5 PFPeA	Ave	266072	271011		50.9	50.0	1.9	50.0
13C2 PFHxA	Ave	245110	248174		50.6	50.0	1.2	50.0
13C4-PFHpA	Ave	226344	223885		49.5	50.0	-1.1	50.0
18O2 PFHxS	Ave	326976	321187		46.5	47.3	-1.8	50.0
13C4 PFOA	Ave	230362	246807		53.6	50.0	7.1	50.0
13C4 PFOS	Ave	248847	255548		49.1	47.8	2.7	50.0
13C5 PFNA	Ave	177687	196267		55.2	50.0	10.5	50.0
13C8 FOSA	Ave	384141	409697		53.3	50.0	6.7	50.0
13C2 PFDA	Ave	157302	174974		55.6	50.0	11.2	50.0
13C2 PFUnA	Ave	117250	128656		54.9	50.0	9.7	50.0
13C2 PFDoA	Ave	110957	125941		56.8	50.0	13.5	50.0
13C2-PFTeA	Ave	227387	223825		49.2	50.0	-1.6	50.0
13C2-PFHxDA	Ave	124568	135255		54.3	50.0	8.6	50.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_027.d
 Lims ID: CCV L4
 Client ID:
 Sample Type: CCV
 Inject. Date: 15-Dec-2016 16:09:19 ALS Bottle#: 40 Worklist Smp#: 27
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L4
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Sublist: chrom-A8_N*sub5
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 14:59:00 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 15-Dec-2016 16:45:48

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.641	1.534	0.107	17011740	48.9		97.8	891137	
1 Perfluorobutyric acid	212.90 > 169.00	1.649	1.535	0.114	6499185	22.4		112	45202	
D 4 13C5-PFPeA	267.90 > 223.00	1.938	1.810	0.128	13550531	50.9		102	1015103	
3 Perfluoropentanoic acid	262.90 > 219.00	1.938	1.810	0.128	5736117	21.4		107	43772	
5 Perfluorobutanesulfonic acid	298.90 > 80.00	1.977	1.848	0.129	9586793	21.1		119		
7 Perfluorohexanoic acid	298.90 > 99.00	1.977	1.848	0.129	3967789		2.42(0.00-0.00)			
6 13C2 PFHxA	313.00 > 269.00	2.253	2.096	0.157	4775586	20.7		104	163994	
D 6 13C2 PFHxA	315.00 > 270.00	2.244	2.097	0.147	12408683	50.6		101	931825	
D 11 13C4-PFHpA	367.00 > 322.00	2.594	2.426	0.168	11194257	49.5		98.9	1739917	
12 Perfluoroheptanoic acid	363.00 > 319.00	2.594	2.428	0.166	4578340	20.9		104	54389	
9 Perfluorohexanesulfonic acid	399.00 > 80.00	2.609	2.431	0.178	6149484	18.6		102		
D 10 18O2 PFHxS	403.00 > 84.00	2.609	2.446	0.163	15192143	46.5		98.2	1562400	
D 14 13C4 PFOA	417.00 > 372.00	2.960	2.783	0.177	12340370	53.6		107	933470	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
15 Perfluorooctanoic acid										
413.00 > 369.00	2.960	2.783	0.177	1.000	5289479	21.4		107	42874	
413.00 > 169.00	2.960	2.783	0.177	1.000	3066933		1.72(0.90-1.10)		153850	
13 Perfluoroheptanesulfonic Acid										
449.00 > 80.00	2.960	2.790	0.170	1.000	5766903	20.5		108		
18 Perfluorooctane sulfonic acid										
499.00 > 80.00	3.304	3.118	0.186	1.000	4921082	19.4		104	94146	
499.00 > 99.00	3.335	3.118	0.217	1.009	1042321		4.72(0.90-1.10)		58590	
D 17 13C4 PFOS										
503.00 > 80.00	3.335	3.151	0.184		12215209	49.1		103	378836	
D 19 13C5 PFNA										
468.00 > 423.00	3.342	3.153	0.189		9813365	55.2		110	462272	
20 Perfluorononanoic acid										
463.00 > 419.00	3.335	3.155	0.180	1.000	3836248	20.5		103	49175	
D 21 13C8 FOSA										
506.00 > 78.00	3.665	3.488	0.177		20484858	53.3		107	770097	
22 Perfluorooctane Sulfonamide										
498.00 > 78.00	3.665	3.491	0.174	1.000	8376603	21.9		110	288421	
24 Perfluorodecanoic acid										
513.00 > 469.00	3.694	3.510	0.184	1.000	3475784	21.0		105	89973	
D 23 13C2 PFDA										
515.00 > 470.00	3.694	3.513	0.181		8748696	55.6		111	196676	
26 Perfluorodecane Sulfonic acid										
599.00 > 80.00	4.005	3.822	0.183	1.000	3090740	20.7		107		
28 Perfluoroundecanoic acid										
563.00 > 519.00	4.015	3.839	0.176	1.000	2604005	21.2		106	69907	
D 27 13C2 PFUnA										
565.00 > 520.00	4.015	3.842	0.173		6432780	54.9		110	269911	
D 30 13C2 PFDoA										
615.00 > 570.00	4.310	4.132	0.178		6297025	56.8		114	212210	
29 Perfluorododecanoic acid										
613.00 > 569.00	4.310	4.136	0.174	1.000	2425632	21.0		105	3655	
31 Perfluorotridecanoic acid										
663.00 > 619.00	4.573	4.400	0.173	1.000	2321490	20.3		102	2476	
D 32 13C2-PFTeDA										
715.00 > 670.00	4.810	4.641	0.169		11191243	49.2		98.4	709486	
33 Perfluorotetradecanoic acid										
712.50 > 668.90	4.810	4.642	0.168	1.000	3526417	17.7		88.3	1638	
713.00 > 169.00	4.802	4.642	0.160	0.998	606214		5.82(0.00-0.00)		39010	
D 34 13C2-PFHxDA										
815.00 > 770.00	5.221	5.057	0.164		6762751	54.3		109	146557	
35 Perfluorohexadecanoic acid										
813.00 > 769.00	5.232	5.059	0.173	1.000	2481363	20.1		100	2243	
36 Perfluorooctadecanoic acid										
913.00 > 869.00	5.588	5.414	0.174	1.000	2804218	21.6		108	2979	

Reagents:

LCPFC-L4_00024

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_027.d

Injection Date: 15-Dec-2016 16:09:19

Instrument ID: A8_N

Lims ID: CCV L4

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 40

Worklist Smp#: 27

Injection Vol: 2.0 ul

Dil. Factor: 1.0000













Method: A8_N

Limit Group: LC PFC_DOD ICAL


D 2 13C4 PFBA

1 Perfluorobutyric acid


D 4 13C5-PFPeA

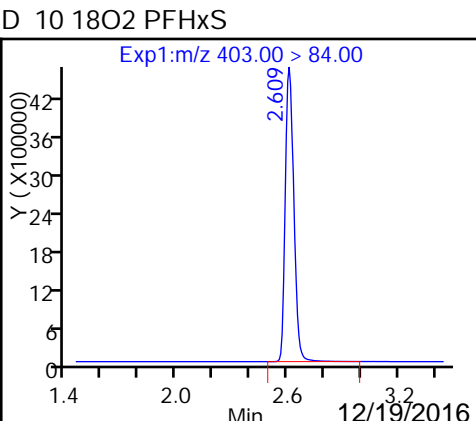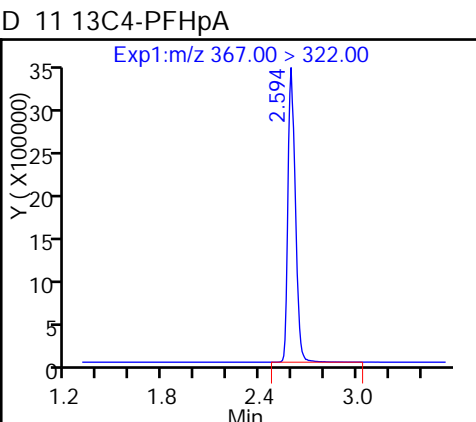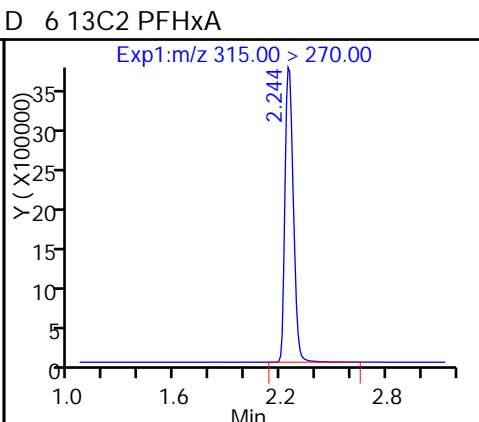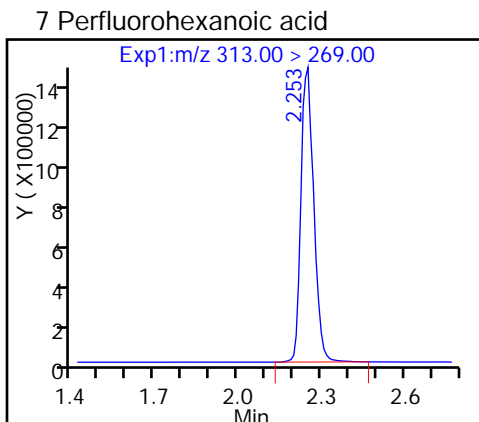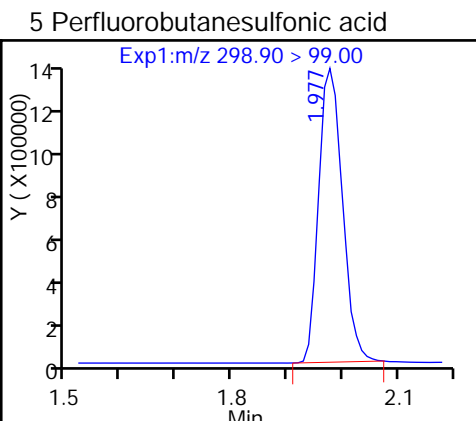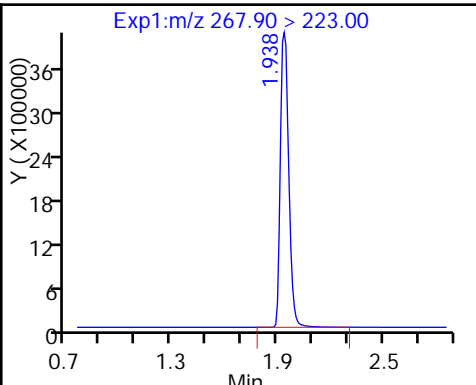


D 14 13C4 PFOA

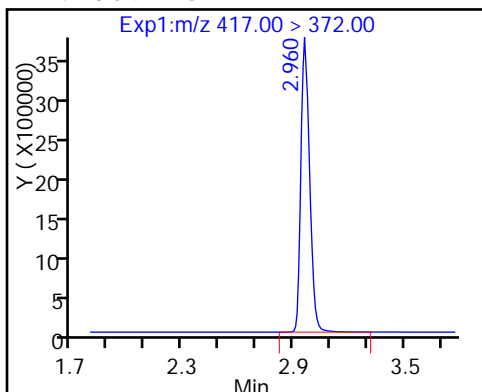


15 Perfluorooctanoic acid

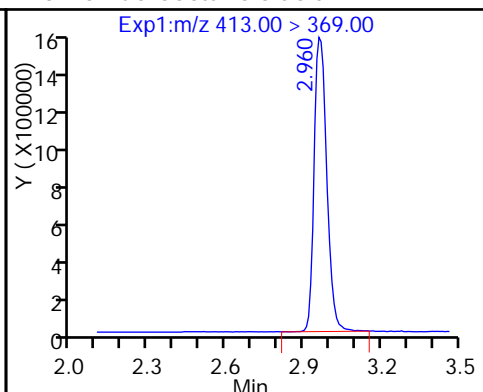


15 Perfluorooctanoic acid




13 Perfluoroheptanesulfonic Acid

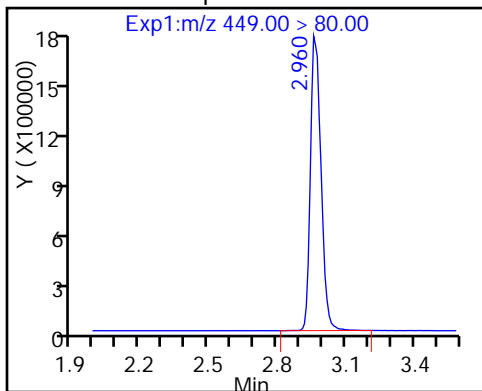


18 Perfluorooctane sulfonic acid

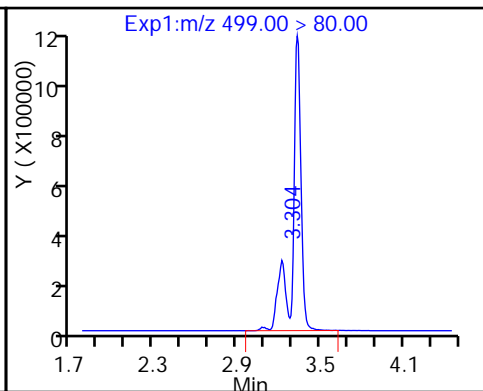


18 Perfluorooctane sulfonic acid

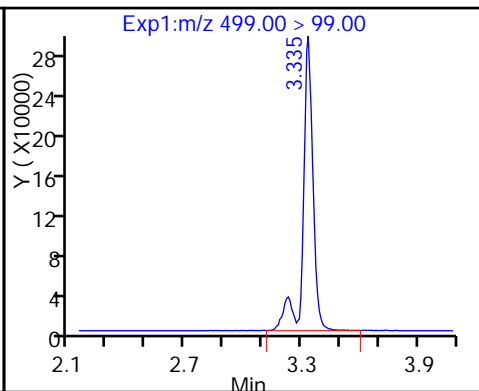


D 17 13C4 PFOS

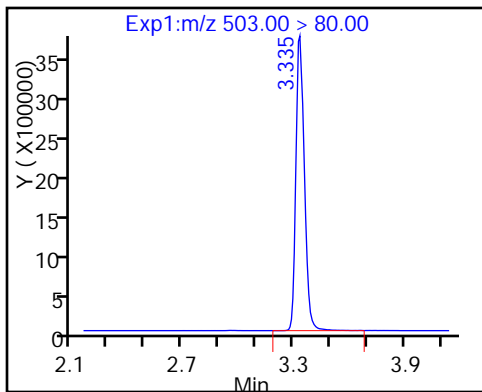


D 19 13C5 PFNA

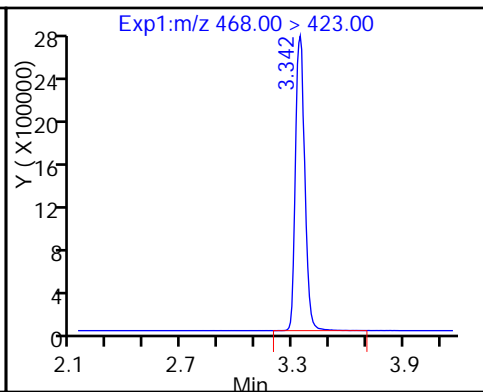


20 Perfluorononanoic acid




D 21 13C8 FOSA

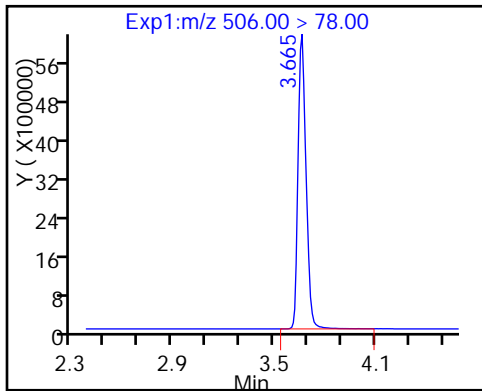


22 Perfluorooctane Sulfonamide

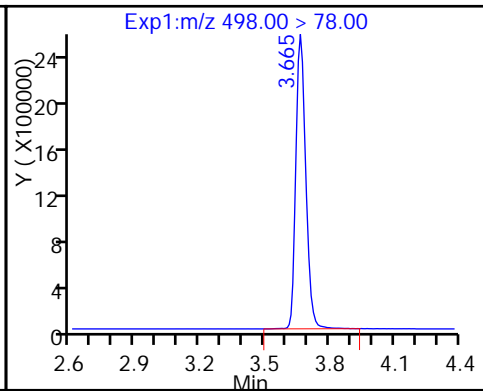


24 Perfluorodecanoic acid

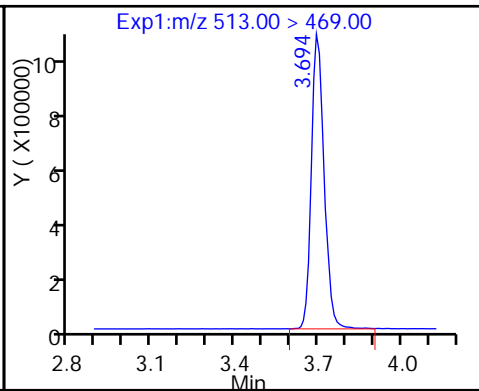


D 23 13C2 PFDA

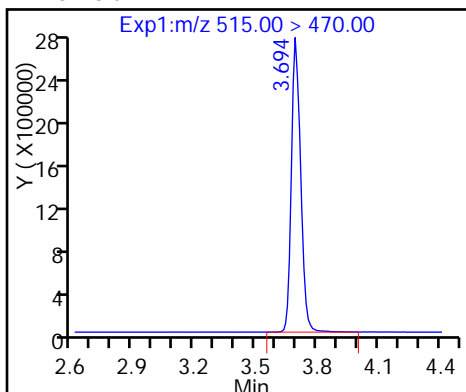


26 Perfluorodecane Sulfonic acid

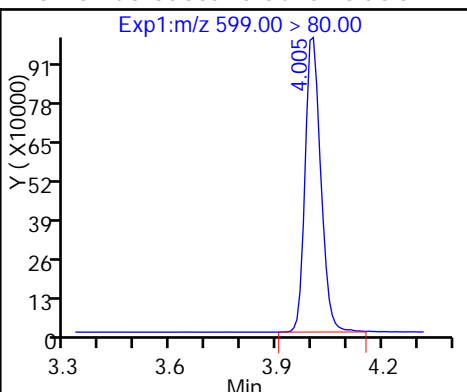


28 Perfluoroundecanoic acid

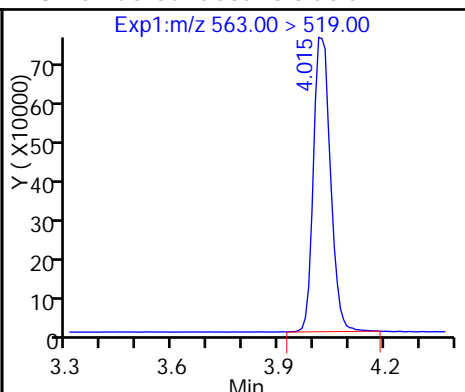


D 27 13C2 PFUnA

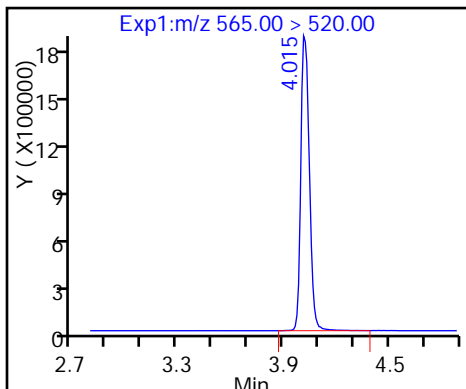


D 30 13C2 PFDaA

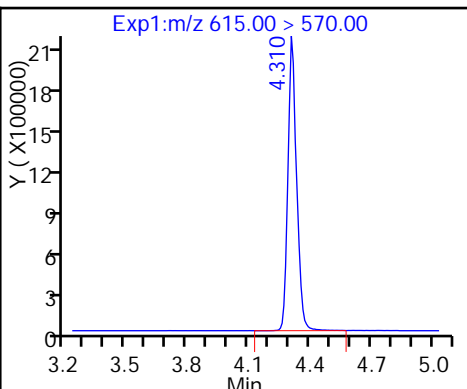


29 Perfluorododecanoic acid

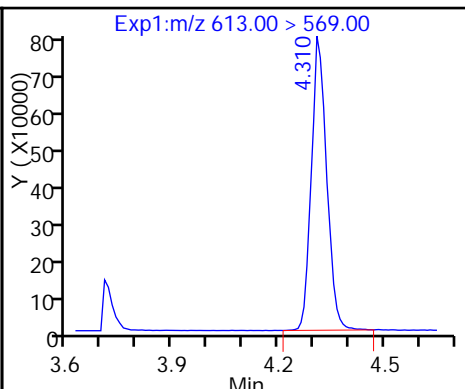


31 Perfluorotridecanoic acid

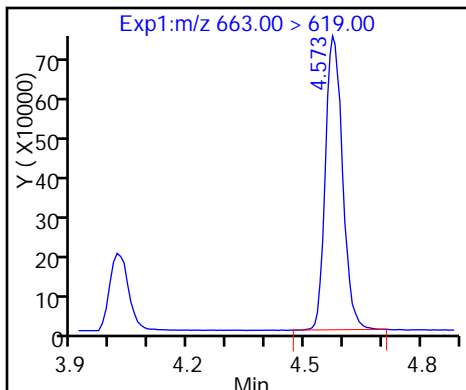


D 32 13C2-PFTeDA

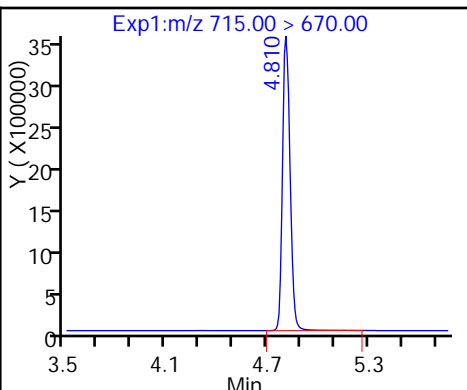


33 Perfluorotetradecanoic acid

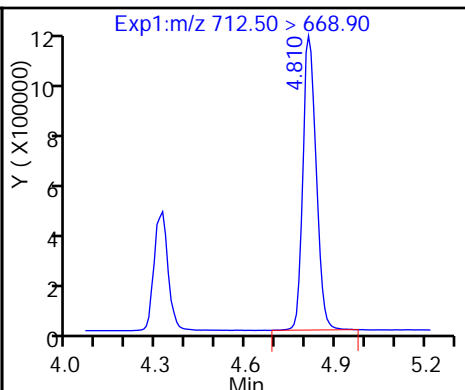


33 Perfluorotetradecanoic acid

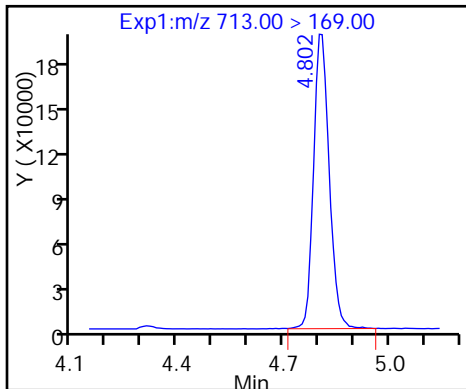


D 34 13C2-PFHxDA

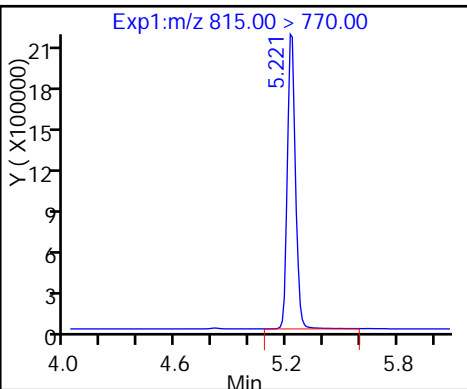

35 Perfluorohexadecanoic acid

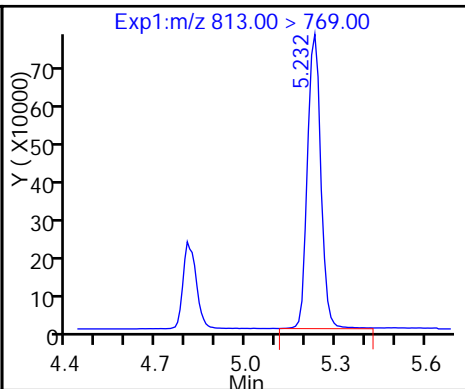

36 Perfluorooctadecanoic acid

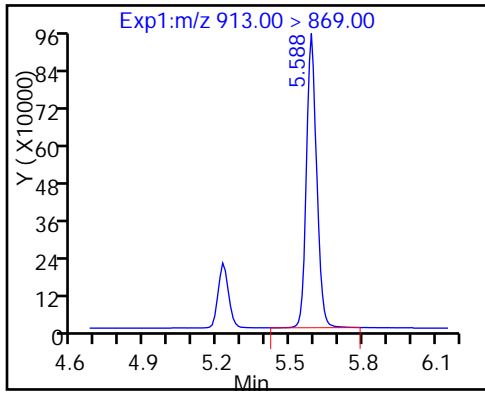

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Lab Sample ID: CCV 320-142379/42 Calibration Date: 12/15/2016 19:54
 Instrument ID: A8_N Calib Start Date: 12/15/2016 12:29
 GC Column: Acquity ID: 2.10 (mm) Calib End Date: 12/15/2016 14:18
 Lab File ID: 15DEC2016BB_039.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanoic acid (PFBA)	AveID	0.8537	0.8988		52.6	50.0	5.3	25.0
Perfluoropentanoic acid (PFPeA)	AveID	0.9868	0.9883		50.1	50.0	0.1	25.0
Perfluorobutanesulfonic acid (PFBS)	AveID	1.417	1.612		50.3	44.2	13.8	25.0
Perfluorohexanoic acid (PFHxA)	AveID	0.9288	0.9355		50.4	50.0	0.7	25.0
Perfluoroheptanoic acid (PFHpA)	AveID	0.9788	0.9735		49.7	50.0	-0.5	25.0
Perfluorohexanesulfonic acid (PFHxS)	AveID	1.030	1.039		45.9	45.5	0.9	25.0
Perfluoroheptanesulfonic Acid (PFHpS)	AveID	1.102	1.168		50.4	47.6	6.0	25.0
Perfluorooctanoic acid (PFOA)	AveID	1.003	1.034		51.5	50.0	3.0	25.0
Perfluorooctanesulfonic acid (PFOS)	AveID	0.9945	1.035		48.3	46.4	4.1	25.0
Perfluorononanoic acid (PFNA)	AveID	0.9518	0.9667		50.8	50.0	1.6	25.0
Perfluorooctane Sulfonamide (FOSA)	AveID	0.9327	0.9484		50.8	50.0	1.7	25.0
Perfluorodecanoic acid (PFDA)	AveID	0.9438	0.9304		49.3	50.0	-1.4	25.0
Perfluorodecanesulfonic acid (PFDS)	AveID	0.5840	0.6267		51.7	48.2	7.3	25.0
Perfluoroundecanoic acid (PFUnA)	AveID	0.9563	0.9697		50.7	50.0	1.4	25.0
Perfluorododecanoic acid (PFDoA)	AveID	0.9180	0.8999		49.0	50.0	-2.0	25.0
Perfluorotridecanoic Acid (PFTriA)	AveID	0.9069	0.9089		50.1	50.0	0.2	25.0
Perfluorotetradecanoic acid (PFTeA)	AveID	1.585	1.459		46.0	50.0	-7.9	25.0
Perfluoro-n-hexadecanoic acid (PFHxDA)	L1ID		1.005		52.1	50.0	4.1	25.0
Perfluoro-n-octadecanoic acid (PFODA)	AveID	1.030	1.028		49.9	50.0	-0.3	25.0
13C4 PFBA	Ave	347743	326570		47.0	50.0	-6.1	50.0
13C5 PFPeA	Ave	266072	254305		47.8	50.0	-4.4	50.0
13C2 PFHxA	Ave	245110	234405		47.8	50.0	-4.4	50.0
13C4-PFHpA	Ave	226344	206393		45.6	50.0	-8.8	50.0
18O2 PFHxS	Ave	326976	301572		43.6	47.3	-7.8	50.0
13C4 PFOA	Ave	230362	219396		47.6	50.0	-4.8	50.0
13C4 PFOS	Ave	248847	247305		47.5	47.8	-0.6	50.0
13C5 PFNA	Ave	177687	176719		49.7	50.0	-0.5	50.0
13C8 FOSA	Ave	384141	399901		52.1	50.0	4.1	50.0
13C2 PFDA	Ave	157302	175394		55.8	50.0	11.5	50.0
13C2 PFUnA	Ave	117250	125622		53.6	50.0	7.1	50.0
13C2 PFDoA	Ave	110957	125609		56.6	50.0	13.2	50.0
13C2-PFTeA	Ave	227387	238018		52.3	50.0	4.7	50.0
13C2-PFHxDA	Ave	124568	145465		58.4	50.0	16.8	50.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016BB_039.d
 Lims ID: CCV L5
 Client ID:
 Sample Type: CCV
 Inject. Date: 15-Dec-2016 19:54:43 ALS Bottle#: 41 Worklist Smp#: 42
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L5
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Sublist: chrom-A8_N*sub5
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 15:32:21 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 16-Dec-2016 09:44:30

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.633	1.534	0.099	16328502	47.0		93.9	779195	
1 Perfluorobutyric acid	212.90 > 169.00	1.641	1.535	0.106	14675557	52.6		105	114766	
D 4 13C5-PFPeA	267.90 > 223.00	1.928	1.810	0.118	12715232	47.8		95.6	1429796	
3 Perfluoropentanoic acid	262.90 > 219.00	1.928	1.810	0.118	12565782	50.1		100	97201	
5 Perfluorobutanesulfonic acid	298.90 > 80.00	1.967	1.848	0.119	21490090	50.3		114		
	298.90 > 99.00	1.967	1.848	0.119	9899915		2.17(0.00-0.00)			
7 Perfluorohexanoic acid	313.00 > 269.00	2.241	2.096	0.145	10964091	50.4		101	364017	
D 6 13C2 PFHxA	315.00 > 270.00	2.241	2.097	0.144	11720257	47.8		95.6	1322107	
D 11 13C4-PFHpA	367.00 > 322.00	2.582	2.426	0.156	10319656	45.6		91.2	842630	
12 Perfluoroheptanoic acid	363.00 > 319.00	2.590	2.428	0.162	10046131	49.7		99.5	128559	
9 Perfluorohexanesulfonic acid	399.00 > 80.00	2.605	2.431	0.174	14262834	45.9		101		
D 10 18O2 PFHxS	403.00 > 84.00	2.605	2.446	0.159	14264364	43.6		92.2	1206486	
D 14 13C4 PFOA	417.00 > 372.00	2.962	2.783	0.179	10969797	47.6		95.2	949562	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
15 Perfluorooctanoic acid										
413.00 > 369.00	2.962	2.783	0.179	1.000	11339061	51.5		103	94403	
413.00 > 169.00	2.954	2.783	0.171	0.997	6883159		1.65(0.90-1.10)		383975	
13 Perfluoroheptanesulfonic Acid										
449.00 > 80.00	2.962	2.790	0.172	1.000	13746812	50.4		106		
18 Perfluorooctane sulfonic acid										
499.00 > 80.00	3.224	3.118	0.106	1.000	11878391	48.3		104	99220	
499.00 > 99.00	3.297	3.118	0.179	1.023	2632899		4.51(0.90-1.10)		24955	
D 17 13C4 PFOS										
503.00 > 80.00	3.335	3.151	0.184		11821169	47.5		99.4	245495	
D 19 13C5 PFNA										
468.00 > 423.00	3.335	3.153	0.182		8835928	49.7		99.5	695059	
20 Perfluorononanoic acid										
463.00 > 419.00	3.335	3.155	0.180	1.000	8542057	50.8		102	86538	
D 21 13C8 FOSA										
506.00 > 78.00	3.641	3.488	0.153		19995036	52.1		104	551328	
22 Perfluorooctane Sulfonamide										
498.00 > 78.00	3.650	3.491	0.159	1.000	18963374	50.8		102	485393	
24 Perfluorodecanoic acid										
513.00 > 469.00	3.698	3.510	0.188	1.000	8159682	49.3		98.6	162976	
D 23 13C2 PFDA										
515.00 > 470.00	3.698	3.513	0.185		8769718	55.8		112	272902	
26 Perfluorodecane Sulfonic acid										
599.00 > 80.00	4.001	3.822	0.179	1.000	7470349	51.7		107		
28 Perfluoroundecanoic acid										
563.00 > 519.00	4.020	3.839	0.181	1.000	6090971	50.7		101	91815	
D 27 13C2 PFUnA										
565.00 > 520.00	4.020	3.842	0.178		6281115	53.6		107	372101	
D 30 13C2 PFDoA										
615.00 > 570.00	4.313	4.132	0.181		6280430	56.6		113	175657	
29 Perfluorododecanoic acid										
613.00 > 569.00	4.313	4.136	0.177	1.000	5651648	49.0		98.0	7833	
31 Perfluorotridecanoic acid										
663.00 > 619.00	4.581	4.400	0.181	1.000	5707999	50.1		100	6879	
D 32 13C2-PFTeDA										
715.00 > 670.00	4.812	4.641	0.171		11900875	52.3		105	983834	
33 Perfluorotetradecanoic acid										
712.50 > 668.90	4.821	4.642	0.179	1.000	9162310	46.0		92.1	5129	
713.00 > 169.00	4.812	4.642	0.170	0.998	1648921		5.56(0.00-0.00)		118077	
D 34 13C2-PFHxDA										
815.00 > 770.00	5.239	5.057	0.182		7273226	58.4		117	133729	
35 Perfluorohexadecanoic acid										
813.00 > 769.00	5.239	5.059	0.180	1.000	6314036	52.1		104	6794	
36 Perfluorooctadecanoic acid										
913.00 > 869.00	5.604	5.414	0.190	1.000	6454544	49.9		99.7	12134	

Reagents:

LCPFC-L5_00022

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016BB_039.d

Injection Date: 15-Dec-2016 19:54:43

Instrument ID: A8_N

Lims ID: CCV L5

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 41

Worklist Smp#: 42

Injection Vol: 2.0 ul

Dil. Factor: 1.0000













Method: A8_N

Limit Group: LC PFC_DOD ICAL


D 2 13C4 PFBA

1 Perfluorobutyric acid


D 4 13C5-PFPeA

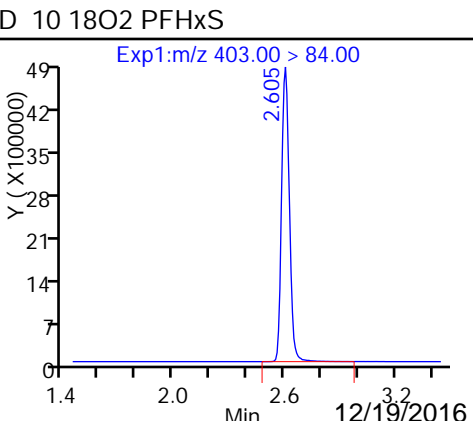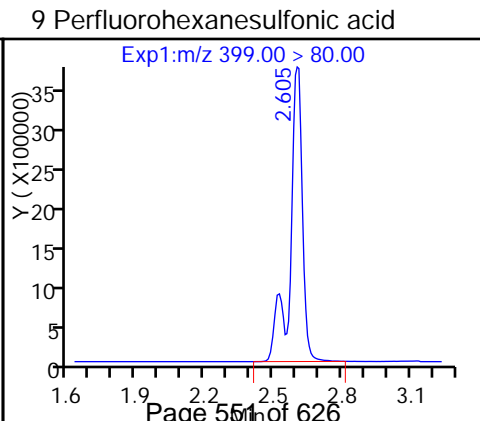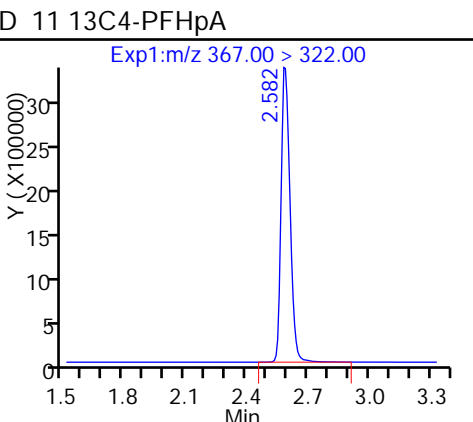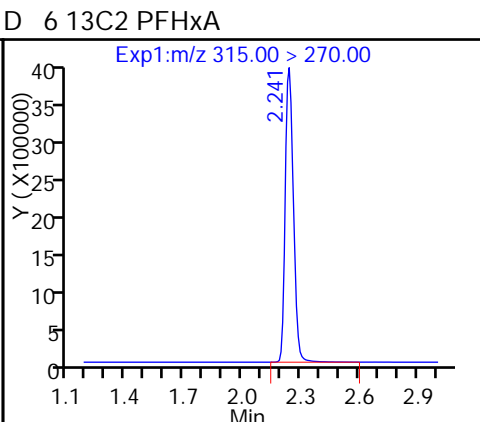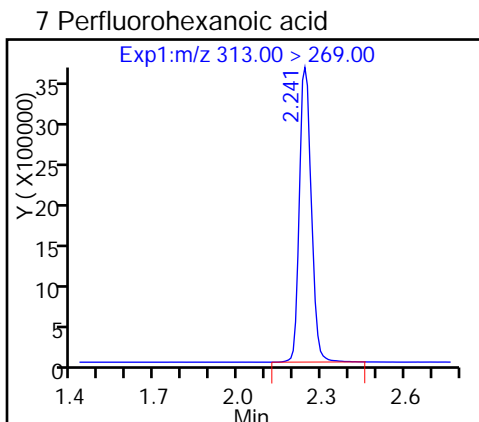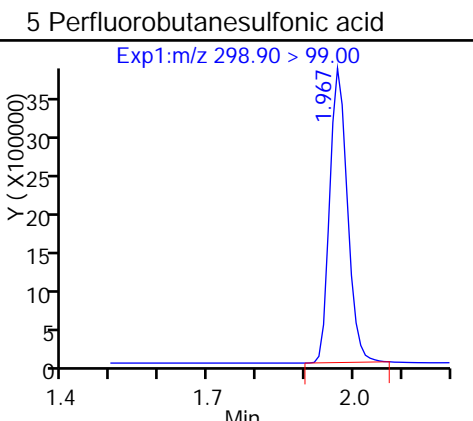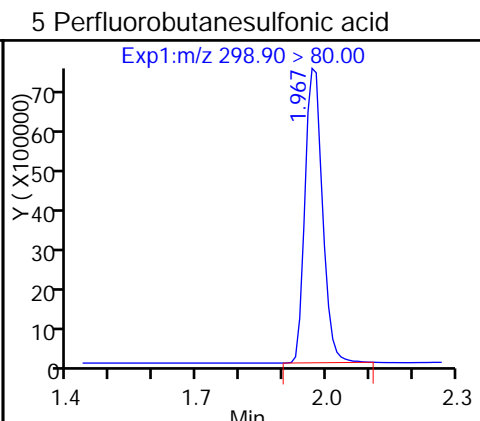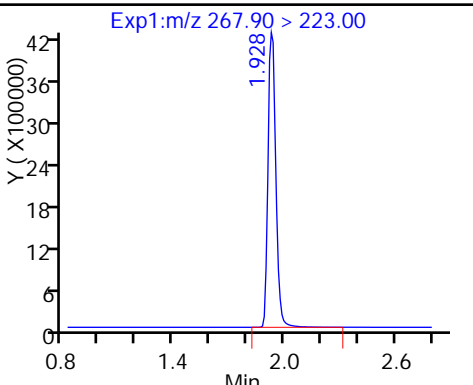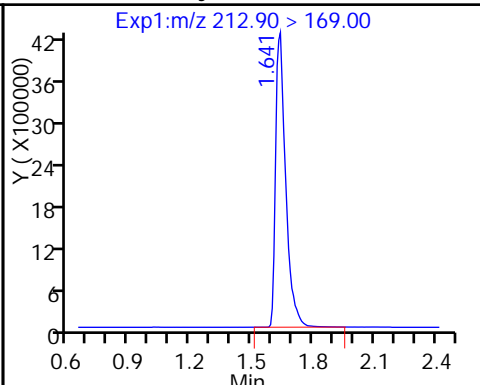


D 14 13C4 PFOA




15 Perfluorooctanoic acid

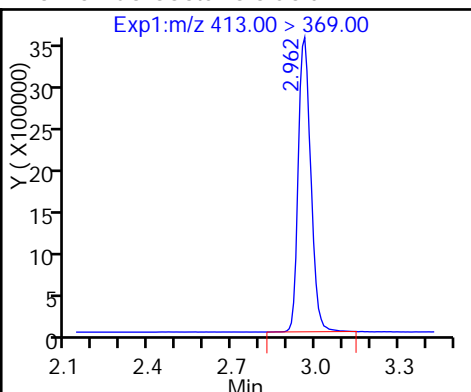


15 Perfluorooctanoic acid

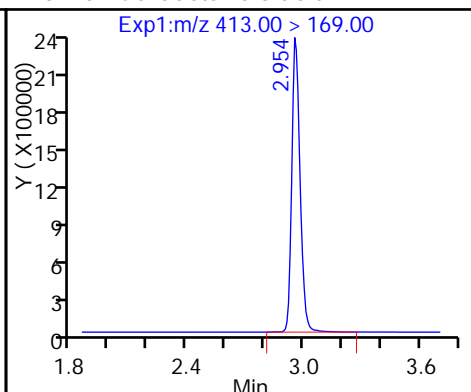


13 Perfluoroheptanesulfonic Acid




18 Perfluorooctane sulfonic acid




18 Perfluorooctane sulfonic acid




D 17 13C4 PFOS




D 19 13C5 PFNA




20 Perfluorononanoic acid




D 21 13C8 FOSA



22 Perfluorooctane Sulfonamide






24 Perfluorodecanoic acid



D 23 13C2 PFDA

26 Perfluorodecane Sulfonic acid




28 Perfluoroundecanoic acid

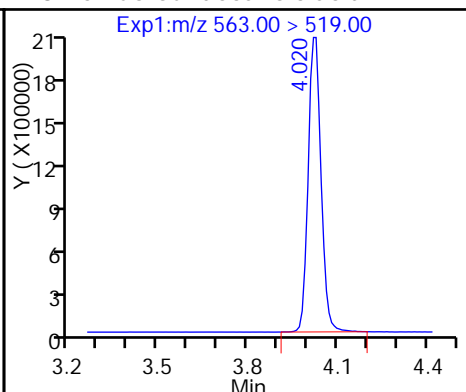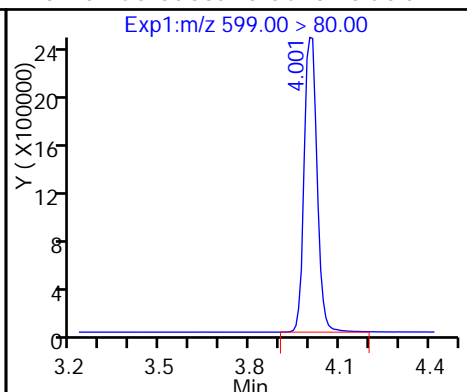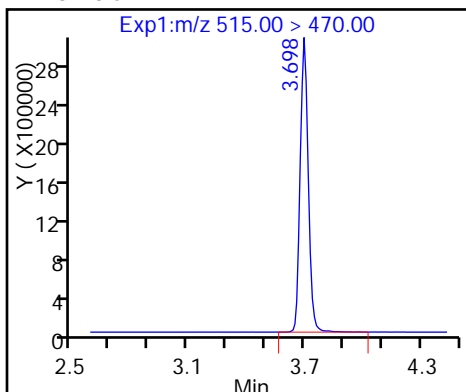

D 27 13C2 PFUnA

D 30 13C2 PFDaA




29 Perfluorododecanoic acid

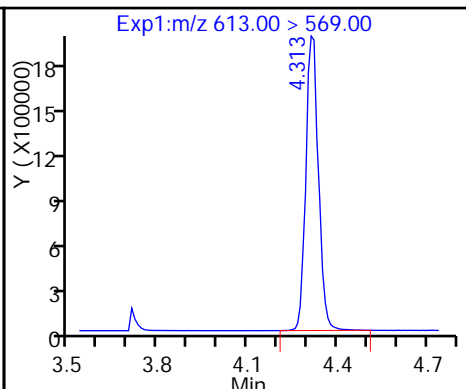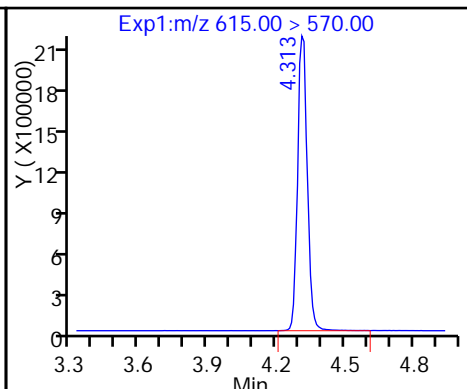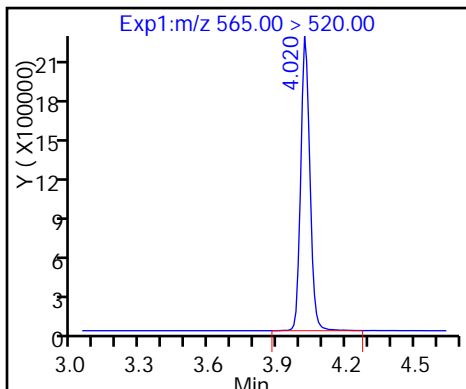

31 Perfluorotridecanoic acid

D 32 13C2-PFTeDA




33 Perfluorotetradecanoic acid

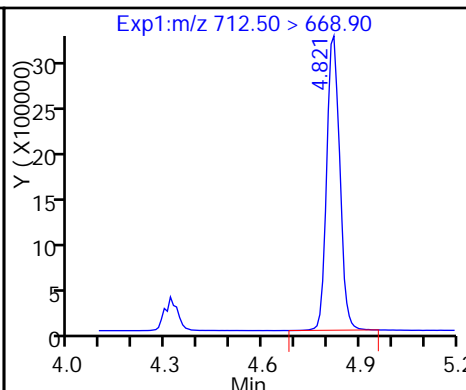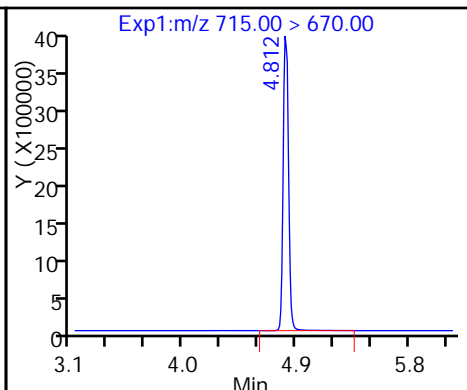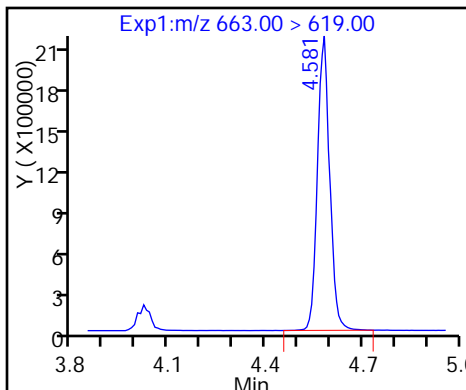


33 Perfluorotetradecanoic acid

D 34 13C2-PFHxDA

35 Perfluorohexadecanoic acid

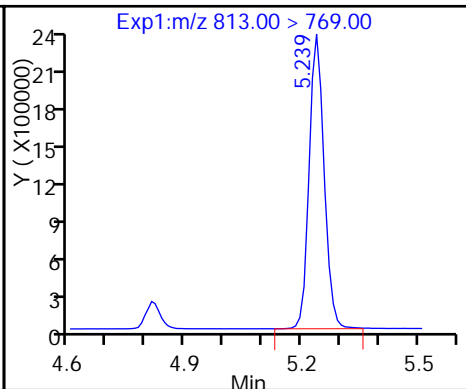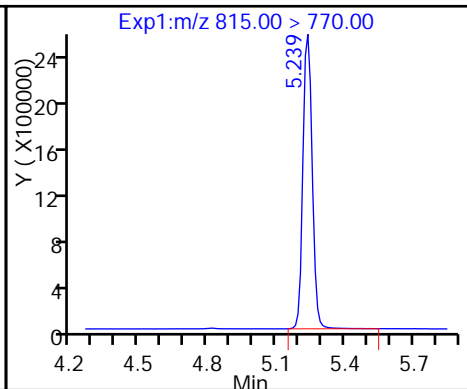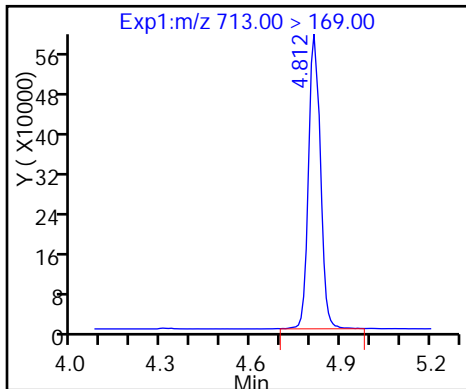

36 Perfluorooctadecanoic acid

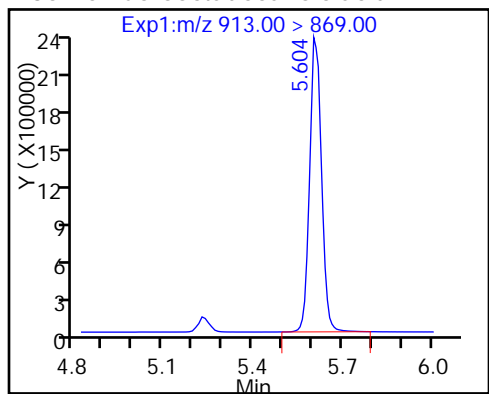

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Lab Sample ID: CCV 320-142602/1 Calibration Date: 12/16/2016 15:22
 Instrument ID: A8_N Calib Start Date: 12/15/2016 12:29
 GC Column: Acquity ID: 2.10 (mm) Calib End Date: 12/15/2016 14:18
 Lab File ID: 16DEC2016BB_001.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanoic acid (PFBA)	AveID	0.8537	0.9110		53.4	50.0	6.7	25.0
Perfluoropentanoic acid (PFPeA)	AveID	0.9868	1.029		52.2	50.0	4.3	25.0
Perfluorobutanesulfonic acid (PFBS)	AveID	1.417	1.616		50.4	44.2	14.0	25.0
Perfluorohexanoic acid (PFHxA)	AveID	0.9288	0.9260		49.8	50.0	-0.3	25.0
Perfluoroheptanoic acid (PFHpA)	AveID	0.9788	0.9710		49.6	50.0	-0.8	25.0
Perfluorohexanesulfonic acid (PFHxS)	AveID	1.030	1.049		46.4	45.5	1.9	25.0
Perfluoroheptanesulfonic Acid (PFHpS)	AveID	1.102	1.219		52.6	47.6	10.6	25.0
Perfluorooctanoic acid (PFOA)	AveID	1.003	1.034		51.5	50.0	3.1	25.0
Perfluorooctanesulfonic acid (PFOS)	AveID	0.9945	1.056		49.3	46.4	6.2	25.0
Perfluorononanoic acid (PFNA)	AveID	0.9518	0.9472		49.8	50.0	-0.5	25.0
Perfluorooctane Sulfonamide (FOSA)	AveID	0.9327	0.9278		49.7	50.0	-0.5	25.0
Perfluorodecanoic acid (PFDA)	AveID	0.9438	0.9428		49.9	50.0	-0.1	25.0
Perfluorodecanesulfonic acid (PFDS)	AveID	0.5840	0.6332		52.3	48.2	8.4	25.0
Perfluoroundecanoic acid (PFUnA)	AveID	0.9563	0.9772		51.1	50.0	2.2	25.0
Perfluorododecanoic acid (PFDoA)	AveID	0.9180	0.9524		51.9	50.0	3.8	25.0
Perfluorotridecanoic Acid (PFTriA)	AveID	0.9069	0.9246		51.0	50.0	2.0	25.0
Perfluorotetradecanoic acid (PFTeA)	AveID	1.585	1.661		52.4	50.0	4.8	25.0
Perfluoro-n-hexadecanoic acid (PFHxDA)	L1ID		0.8966		46.4	50.0	-7.3	25.0
Perfluoro-n-octadecanoic acid (PFODA)	AveID	1.030	0.9123		44.3	50.0	-11.5	25.0
13C4 PFBA	Ave	347743	321788		46.3	50.0	-7.5	50.0
13C5 PFPeA	Ave	266072	250320		47.0	50.0	-5.9	50.0
13C2 PFHxA	Ave	245110	227821		46.5	50.0	-7.1	50.0
13C4-PFHpA	Ave	226344	197190		43.6	50.0	-12.9	50.0
18O2 PFHxS	Ave	326976	294104		42.5	47.3	-10.1	50.0
13C4 PFOA	Ave	230362	201932		43.8	50.0	-12.3	50.0
13C4 PFOS	Ave	248847	223056		42.8	47.8	-10.4	50.0
13C5 PFNA	Ave	177687	155223		43.7	50.0	-12.6	50.0
13C8 FOSA	Ave	384141	363007		47.2	50.0	-5.5	50.0
13C2 PFDA	Ave	157302	136046		43.2	50.0	-13.5	50.0
13C2 PFUnA	Ave	117250	101045		43.1	50.0	-13.8	50.0
13C2 PFDoA	Ave	110957	98295		44.3	50.0	-11.4	50.0
13C2-PFTeA	Ave	227387	194368		42.7	50.0	-14.5	50.0
13C2-PFHxDA	Ave	124568	99924		40.1	50.0	-19.8	50.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161216-37940.b\16DEC2016BB_001.d
 Lims ID: CCV L5
 Client ID:
 Sample Type: CCV
 Inject. Date: 16-Dec-2016 15:22:43 ALS Bottle#: 41 Worklist Smp#: 1
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L5
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Sublist: chrom-A8_N*sub5
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161216-37940.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 16:15:23 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 16-Dec-2016 16:15:23

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.566	1.566	0.0	16089379	46.3		92.5	1252638	
1 Perfluorobutyric acid	212.90 > 169.00	1.574	1.574	0.0	14656578	53.4		107	132817	
D 4 13C5-PFPeA	267.90 > 223.00	1.849	1.849	0.0	12515997	47.0		94.1	1188584	
3 Perfluoropentanoic acid	262.90 > 219.00	1.849	1.849	0.0	12882163	52.2		104	126443	
5 Perfluorobutanesulfonic acid	298.90 > 80.00	1.887	1.887	0.0	21005446	50.4		114		
	298.90 > 99.00	1.887	1.887	0.0	9675408		2.17(0.00-0.00)			
7 Perfluorohexanoic acid	313.00 > 269.00	2.143	2.143	0.0	10548023	49.8		99.7	326206	
D 6 13C2 PFHxA	315.00 > 270.00	2.143	2.143	0.0	11391037	46.5		92.9	595461	
12 Perfluoroheptanoic acid	363.00 > 319.00	2.483	2.483	0.0	9573483	49.6		99.2	106730	
D 11 13C4-PFHpA	367.00 > 322.00	2.483	2.483	0.0	9859511	43.6		87.1	1148849	
D 10 18O2 PFHxS	403.00 > 84.00	2.490	2.490	0.0	13911132	42.5		89.9	971558	
9 Perfluorohexanesulfonic acid	399.00 > 80.00	2.498	2.498	0.0	14040380	46.4		102		
D 14 13C4 PFOA	417.00 > 372.00	2.837	2.837	0.0	10096596	43.8		87.7	423031	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
15 Perfluorooctanoic acid										
413.00 > 369.00	2.845	2.845	0.0	1.000	10438208	51.5		103	77318	
413.00 > 169.00	2.837	2.845	-0.008	0.997	6536148		1.60(0.90-1.10)		319161	
13 Perfluoroheptanesulfonic Acid										
449.00 > 80.00	2.845	2.845	0.0	1.000	12939672	52.6		111		
18 Perfluorooctane sulfonic acid										
499.00 > 80.00	3.101	3.101	0.0	1.000	10930998	49.3		106	77035	
499.00 > 99.00	3.207	3.101	0.106	1.034	2335098		4.68(0.90-1.10)		178880	
20 Perfluorononanoic acid										
463.00 > 419.00	3.207	3.207	0.0	1.000	7351277	49.8		99.5	101739	
D 17 13C4 PFOS										
503.00 > 80.00	3.207	3.207	0.0		10662055	42.8		89.6	219546	
D 19 13C5 PFNA										
468.00 > 423.00	3.216	3.216	0.0		7761170	43.7		87.4	497236	
D 21 13C8 FOSA										
506.00 > 78.00	3.539	3.539	0.0		18150358	47.2		94.5	629588	
22 Perfluorooctane Sulfonamide										
498.00 > 78.00	3.547	3.547	0.0	1.000	16840500	49.7		99.5	546550	
24 Perfluorodecanoic acid										
513.00 > 469.00	3.573	3.573	0.0	1.000	6413340	49.9		99.9	145910	
D 23 13C2 PFDA										
515.00 > 470.00	3.573	3.573	0.0		6802283	43.2		86.5	171352	
26 Perfluorodecane Sulfonic acid										
599.00 > 80.00	3.880	3.880	0.0	1.000	6808173	52.3		108		
28 Perfluoroundecanoic acid										
563.00 > 519.00	3.898	3.898	0.0	1.000	4936841	51.1		102	110564	
D 27 13C2 PFUnA										
565.00 > 520.00	3.898	3.898	0.0		5052226	43.1		86.2	342267	
D 30 13C2 PFDaA										
615.00 > 570.00	4.186	4.186	0.0		4914728	44.3		88.6	137561	
29 Perfluorododecanoic acid										
613.00 > 569.00	4.179	4.179	0.0	1.000	4680959	51.9		104	93837	
31 Perfluorotridecanoic acid										
663.00 > 619.00	4.455	4.455	0.0	1.000	4544252	51.0		102	89151	
D 32 13C2-PFTeDA										
715.00 > 670.00	4.696	4.696	0.0		9718424	42.7		85.5	1153883	
33 Perfluorotetradecanoic acid										
712.50 > 668.90	4.696	4.696	0.0	1.000	8161505	52.4		105	15487	
713.00 > 169.00	4.688	4.696	-0.008	0.998	1297089		6.29(0.00-0.00)		161331	
D 34 13C2-PFHxDA										
815.00 > 770.00	5.090	5.090	0.0		4996216	40.1		80.2	99927	
35 Perfluorohexadecanoic acid										
813.00 > 769.00	5.101	5.101	0.0	1.000	4406580	46.4		92.7	4620	
36 Perfluorooctadecanoic acid										
913.00 > 869.00	5.451	5.451	0.0	1.000	4483733	44.3		88.5	8077	

Reagents:

LCPFC-L5_00022

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161216-37940.b\16DEC2016BB_001.d

Injection Date: 16-Dec-2016 15:22:43

Instrument ID: A8_N

Lims ID: CCV L5

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 41

Worklist Smp#: 1

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: A8_N

Limit Group: LC PFC_DOD ICAL

D 2 13C4 PFBA

1 Perfluorobutyric acid




D 4 13C5-PFPeA

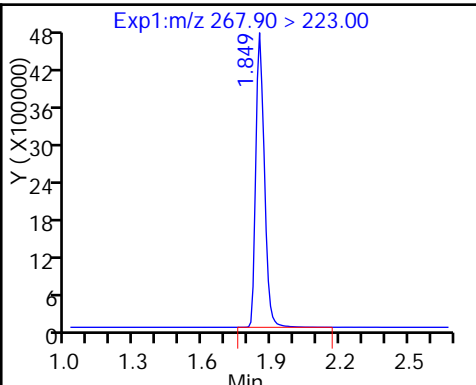

3 Perfluoropentanoic acid

5 Perfluorobutanesulfonic acid




5 Perfluorobutanesulfonic acid

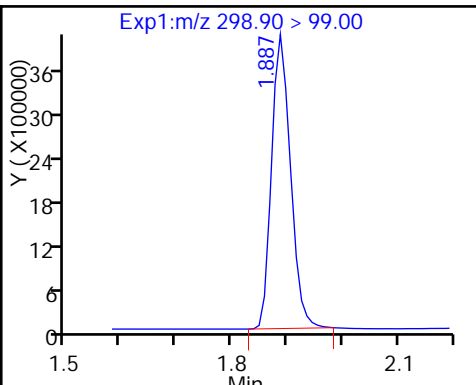

7 Perfluorohexanoic acid

D 6 13C2 PFHxA




12 Perfluoroheptanoic acid

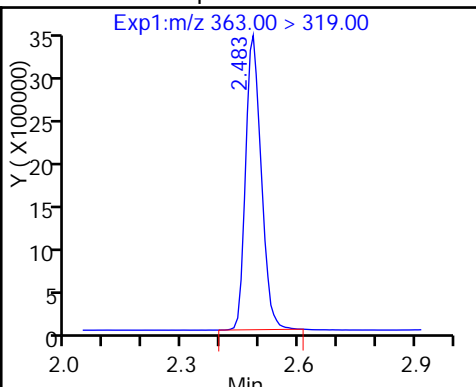


D 11 13C4-PFHpA

D 10 18O2 PFHxS


9 Perfluorohexanesulfonic acid

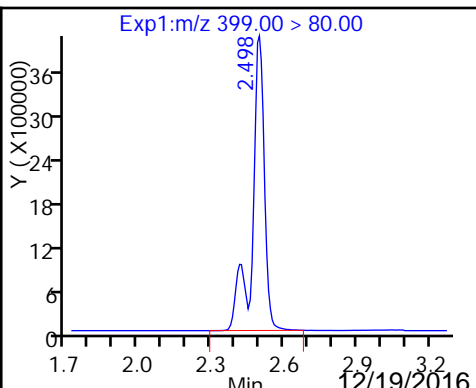


D 14 13C4 PFOA




15 Perfluorooctanoic acid

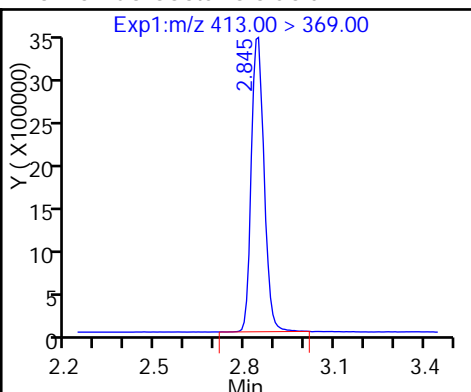


15 Perfluorooctanoic acid

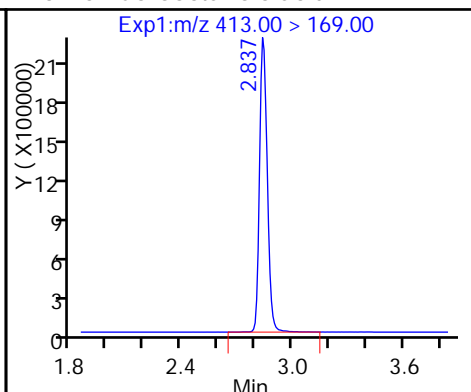


13 Perfluoroheptanesulfonic Acid




18 Perfluorooctane sulfonic acid




18 Perfluorooctane sulfonic acid




20 Perfluorononanoic acid




D 17 13C4 PFOS




D 19 13C5 PFNA




D 21 13C8 FOSA



22 Perfluorooctane Sulfonamide






24 Perfluorodecanoic acid



D 23 13C2 PFDA

26 Perfluorodecane Sulfonic acid




28 Perfluoroundecanoic acid



D 27 13C2 PFUa

D 30 13C2 PFDa




29 Perfluorododecanoic acid



31 Perfluorotridecanoic acid

D 32 13C2-PFTeDA




33 Perfluorotetradecanoic acid




33 Perfluorotetradecanoic acid

D 34 13C2-PFHxDA

35 Perfluorohexadecanoic acid



36 Perfluorooctadecanoic acid

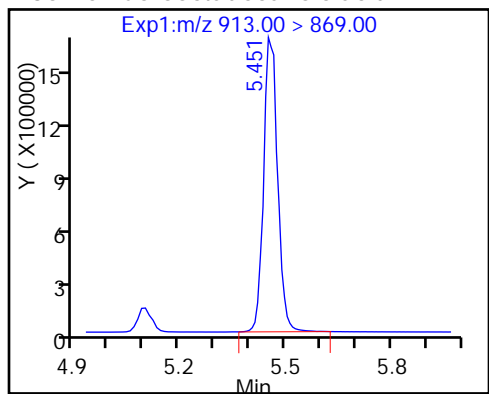

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Lab Sample ID: CCV 320-142602/4 Calibration Date: 12/16/2016 15:45
 Instrument ID: A8_N Calib Start Date: 12/15/2016 12:29
 GC Column: Acquity ID: 2.10 (mm) Calib End Date: 12/15/2016 14:18
 Lab File ID: 16DEC2016BB_004.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanoic acid (PFBA)	AveID	0.8537	0.9621		22.5	20.0	12.7	25.0
Perfluoropentanoic acid (PFPeA)	AveID	0.9868	1.054		21.4	20.0	6.8	25.0
Perfluorobutanesulfonic acid (PFBS)	AveID	1.417	1.747		21.8	17.7	23.3	25.0
Perfluorohexanoic acid (PFHxA)	AveID	0.9288	0.9754		21.0	20.0	5.0	25.0
Perfluoroheptanoic acid (PFHpA)	AveID	0.9788	1.013		20.7	20.0	3.5	25.0
Perfluorohexanesulfonic acid (PFHxS)	AveID	1.030	1.076		19.0	18.2	4.4	25.0
Perfluorooctanoic acid (PFOA)	AveID	1.003	1.063		21.2	20.0	5.9	25.0
Perfluoroheptanesulfonic Acid (PFHpS)	AveID	1.102	1.179		20.4	19.0	7.0	25.0
Perfluorooctanesulfonic acid (PFOS)	AveID	0.9945	1.047		19.5	18.6	5.3	25.0
Perfluorononanoic acid (PFNA)	AveID	0.9518	0.9693		20.4	20.0	1.8	25.0
Perfluorooctane Sulfonamide (FOSA)	AveID	0.9327	1.012		21.7	20.0	8.5	25.0
Perfluorodecanoic acid (PFDA)	AveID	0.9438	0.9752		20.7	20.0	3.3	25.0
Perfluorodecanesulfonic acid (PFDS)	AveID	0.5840	0.6179		20.4	19.3	5.8	25.0
Perfluoroundecanoic acid (PFUnA)	AveID	0.9563	0.9442		19.7	20.0	-1.3	25.0
Perfluorododecanoic acid (PFDoA)	AveID	0.9180	0.9660		21.0	20.0	5.2	25.0
Perfluorotridecanoic Acid (PFTriA)	AveID	0.9069	0.8928		19.7	20.0	-1.6	25.0
Perfluorotetradecanoic acid (PFTeA)	AveID	1.585	1.637		20.7	20.0	3.3	25.0
Perfluoro-n-hexadecanoic acid (PFHxDA)	L1ID		0.8735		17.7	20.0	-11.5	25.0
Perfluoro-n-octadecanoic acid (PFODA)	AveID	1.030	0.8600		16.7	20.0	-16.5	25.0
13C4 PFBA	Ave	347743	350232		50.4	50.0	0.7	50.0
13C5 PFPeA	Ave	266072	282590		53.1	50.0	6.2	50.0
13C2 PFHxA	Ave	245110	259592		53.0	50.0	5.9	50.0
13C4-PFHpA	Ave	226344	229042		50.6	50.0	1.2	50.0
18O2 PFHxS	Ave	326976	326785		47.3	47.3	-0.0	50.0
13C4 PFOA	Ave	230362	243980		53.0	50.0	5.9	50.0
13C4 PFOS	Ave	248847	259142		49.8	47.8	4.1	50.0
13C5 PFNA	Ave	177687	177969		50.1	50.0	0.2	50.0
13C8 FOSA	Ave	384141	408714		53.2	50.0	6.4	50.0
13C2 PFDA	Ave	157302	160670		51.1	50.0	2.1	50.0
13C2 PFUnA	Ave	117250	124676		53.2	50.0	6.3	50.0
13C2 PFDoA	Ave	110957	116786		52.6	50.0	5.3	50.0
13C2-PFTeDA	Ave	227387	211625		46.5	50.0	-6.9	50.0
13C2-PFHxDA	Ave	124568	114360		45.9	50.0	-8.2	50.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161216-37940.b\16DEC2016BB_004.d
 Lims ID: CCV L4
 Client ID:
 Sample Type: CCV
 Inject. Date: 16-Dec-2016 15:45:11 ALS Bottle#: 40 Worklist Smp#: 4
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L4
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Sublist: chrom-A8_N*sub5
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161216-37940.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 16:14:13 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 16-Dec-2016 16:05:51

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.574	1.574	0.0	17511596	50.4		101	1313684	
1 Perfluorobutyric acid	212.90 > 169.00	1.574	1.574	0.0	1.000	6738882	22.5	113	63028	
D 4 13C5-PFPeA	267.90 > 223.00	1.848	1.848	0.0	14129491	53.1		106	1218720	
3 Perfluoropentanoic acid	262.90 > 219.00	1.858	1.858	0.0	1.000	5954557	21.4	107	52431	
5 Perfluorobutanesulfonic acid	298.90 > 80.00	1.897	1.897	0.0	1.000	10095087	21.8	123		
	298.90 > 99.00	1.897	1.897	0.0	1.000	4304708	2.35(0.00-0.00)			
7 Perfluorohexanoic acid	313.00 > 269.00	2.150	2.150	0.0	1.000	5064211	21.0	105	203726	
D 6 13C2 PFHxA	315.00 > 270.00	2.150	2.150	0.0	12979576	53.0		106	934428	
12 Perfluoroheptanoic acid	363.00 > 319.00	2.483	2.483	0.0	1.000	4642643	20.7	104	53942	
D 11 13C4-PFHpA	367.00 > 322.00	2.483	2.483	0.0	11452095	50.6		101	988197	
D 10 18O2 PFHxS	403.00 > 84.00	2.499	2.499	0.0	15456926	47.3		99.9	773345	
9 Perfluorohexanesulfonic acid	399.00 > 80.00	2.499	2.499	0.0	1.000	6398159	19.0	104		
D 14 13C4 PFOA	417.00 > 372.00	2.846	2.846	0.0	12199024	53.0		106	673451	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
15 Perfluorooctanoic acid										
413.00 > 369.00	2.846	2.846	0.0	1.000	5185952	21.2		106	42392	
413.00 > 169.00	2.846	2.846	0.0	1.000	3087598		1.68(0.90-1.10)		149989	
13 Perfluoroheptanesulfonic Acid										
449.00 > 80.00	2.854	2.854	0.0	1.000	5817809	20.4		107		
18 Perfluorooctane sulfonic acid										
499.00 > 80.00	3.111	3.111	0.0	1.000	5038074	19.5		105	60962	
499.00 > 99.00	3.217	3.111	0.106	1.034	1084727		4.64(0.90-1.10)		56661	
20 Perfluorononanoic acid										
463.00 > 419.00	3.217	3.217	0.0	1.000	3450095	20.4		102	52750	
D 17 13C4 PFOS										
503.00 > 80.00	3.217	3.217	0.0		12387008	49.8		104	476291	
D 19 13C5 PFNA										
468.00 > 423.00	3.217	3.217	0.0		8898451	50.1		100	604703	
D 21 13C8 FOSA										
506.00 > 78.00	3.548	3.548	0.0		20435699	53.2		106	785114	
22 Perfluorooctane Sulfonamide										
498.00 > 78.00	3.557	3.557	0.0	1.000	8273176	21.7		109	301125	
24 Perfluorodecanoic acid										
513.00 > 469.00	3.573	3.573	0.0	1.000	3133761	20.7		103	109860	
D 23 13C2 PFDA										
515.00 > 470.00	3.573	3.573	0.0		8033517	51.1		102	390544	
26 Perfluorodecane Sulfonic acid										
599.00 > 80.00	3.881	3.881	0.0	1.000	3087305	20.4		106		
28 Perfluoroundecanoic acid										
563.00 > 519.00	3.898	3.898	0.0	1.000	2354363	19.7		98.7	46168	
D 27 13C2 PFUnA										
565.00 > 520.00	3.898	3.898	0.0		6233775	53.2		106	321916	
29 Perfluorododecanoic acid										
613.00 > 569.00	4.199	4.199	0.0	1.000	2256266	21.0		105	38821	
D 30 13C2 PFDoA										
615.00 > 570.00	4.193	4.193	0.0		5839295	52.6		105	149836	
31 Perfluorotridecanoic acid										
663.00 > 619.00	4.452	4.452	0.0	1.000	2085289	19.7		98.4	42105	
D 32 13C2-PFTeDA										
715.00 > 670.00	4.693	4.693	0.0		10581271	46.5		93.1	938559	
33 Perfluorotetradecanoic acid										
712.50 > 668.90	4.702	4.702	0.0	1.000	3824158	20.7		103	3601	
713.00 > 169.00	4.693	4.702	-0.009	0.998	590785		6.47(0.00-0.00)		75168	
D 34 13C2-PFHxDA										
815.00 > 770.00	5.110	5.110	0.0		5718024	45.9		91.8	99823	
35 Perfluorohexadecanoic acid										
813.00 > 769.00	5.110	5.110	0.0	1.000	2040330	17.7		88.5	2416	
36 Perfluorooctadecanoic acid										
913.00 > 869.00	5.459	5.459	0.0	1.000	2008770	16.7		83.5	3127	

Reagents:

LCPFC-L4_00024

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161216-37940.b\16DEC2016BB_004.d

Injection Date: 16-Dec-2016 15:45:11

Instrument ID: A8_N

Lims ID: CCV L4

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 40

Worklist Smp#: 4

Injection Vol: 2.0 ul

Dil. Factor: 1.0000













Method: A8_N

Limit Group: LC PFC_DOD ICAL


D 2 13C4 PFBA

1 Perfluorobutyric acid


D 4 13C5-PFPeA

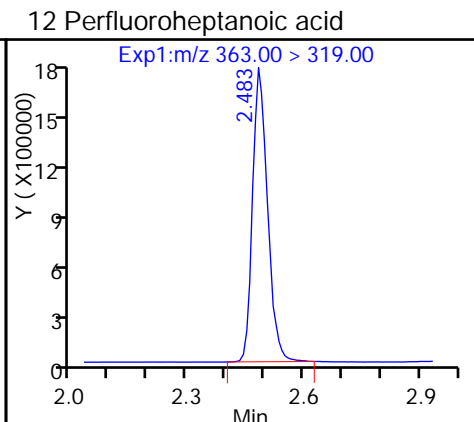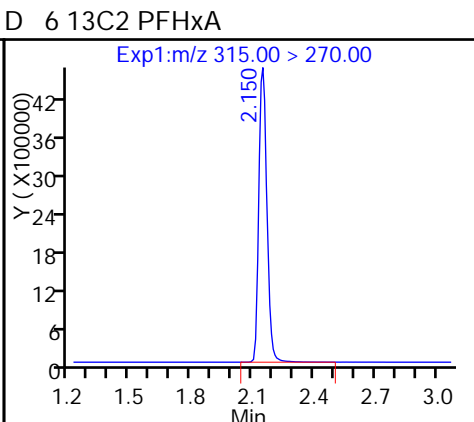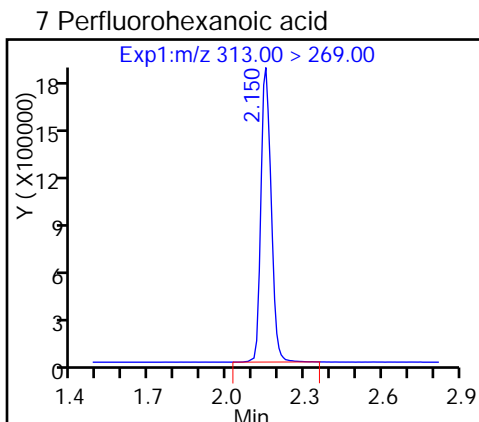


D 14 13C4 PFOA




15 Perfluorooctanoic acid

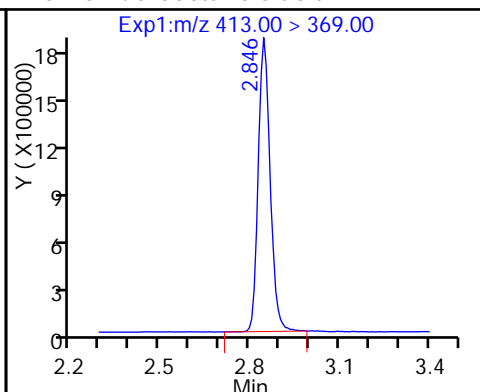


15 Perfluorooctanoic acid




13 Perfluoroheptanesulfonic Acid




18 Perfluorooctane sulfonic acid




18 Perfluorooctane sulfonic acid




20 Perfluorononanoic acid




D 17 13C4 PFOS




D 19 13C5 PFNA




D 21 13C8 FOSA




22 Perfluorooctane Sulfonamide




24 Perfluorodecanoic acid




D 23 13C2 PFDA




26 Perfluorodecane Sulfonic acid




28 Perfluoroundecanoic acid

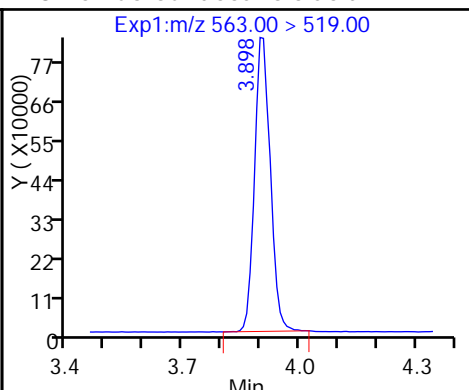


D 27 13C2 PFUa




29 Perfluorododecanoic acid




D 30 13C2 PFDa




31 Perfluorotridecanoic acid




D 32 13C2-PFTeDA




33 Perfluorotetradecanoic acid

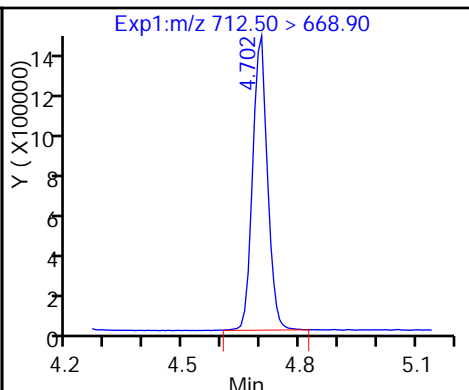


33 Perfluorotetradecanoic acid




D 34 13C2-PFHxDA



35 Perfluorohexadecanoic acid



36 Perfluorooctadecanoic acid

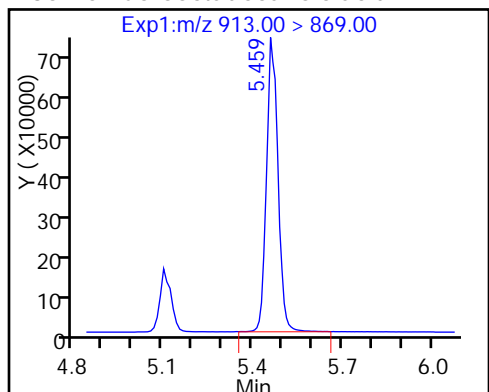

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: MB 320-142235/1-A
 Matrix: Water Lab File ID: 15DEC2016B_029.d
 Analysis Method: 537 (Modified) Date Collected: _____
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 250 (mL) Date Analyzed: 12/15/2016 16:24
 Con. Extract Vol.: 0.5 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: Acquity ID: 2.1 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142379 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
375-22-4	Perfluorobutanoic acid (PFBA)	1.0	U	2.5	1.0	0.46
2706-90-3	Perfluoropentanoic acid (PFPeA)	2.0	U	2.5	2.0	0.99
307-24-4	Perfluorohexanoic acid (PFHxA)	2.0	U	2.5	2.0	0.79
375-85-9	Perfluoroheptanoic acid (PFHpA)	2.0	U	2.5	2.0	0.80
335-67-1	Perfluorooctanoic acid (PFOA)	2.0	U	2.5	2.0	0.75
375-95-1	Perfluorononanoic acid (PFNA)	2.0	U	2.5	2.0	0.65
335-76-2	Perfluorodecanoic acid (PFDA)	1.0	U	2.5	1.0	0.44
2058-94-8	Perfluoroundecanoic acid (PFUnA)	2.0	U	2.5	2.0	0.75
307-55-1	Perfluorododecanoic acid (PFDoA)	2.0	U	2.5	2.0	0.58
72629-94-8	Perfluorotridecanoic Acid (PFTriA)	2.0	U	2.5	2.0	0.55
376-06-7	Perfluorotetradecanoic acid (PFTeA)	0.559	J	2.5	1.0	0.40
375-73-5	Perfluorobutanesulfonic acid (PFBS)	2.0	U	2.5	2.0	0.92
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	2.0	U	2.5	2.0	0.87
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	3.0	U	4.0	3.0	1.3
335-77-3	Perfluorodecanesulfonic acid (PFDS)	3.0	U	4.0	3.0	1.2
754-91-6	Perfluorooctane Sulfonamide (FOSA)	2.0	U	2.5	2.0	0.64

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: MB 320-142235/1-A
 Matrix: Water Lab File ID: 15DEC2016B_029.d
 Analysis Method: 537 (Modified) Date Collected: _____
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 250 (mL) Date Analyzed: 12/15/2016 16:24
 Con. Extract Vol.: 0.5 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: Acquity ID: 2.1 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142379 Units: ng/L

CAS NO.	ISOTOPE DILUTION	%REC	Q	LIMITS
STL01056	13C8 FOSA	39		25-150
STL00992	13C4 PFBA	118		25-150
STL00993	13C2 PFHxA	118		25-150
STL00990	13C4 PFOA	128		25-150
STL00995	13C5 PFNA	125		25-150
STL00996	13C2 PFDA	136		25-150
STL00997	13C2 PFUnA	135		25-150
STL00998	13C2 PFDoA	129		25-150
STL00994	18O2 PFHxS	111		25-150
STL00991	13C4 PFOS	115		25-150
STL01892	13C4-PFHpA	127		25-150
STL01893	13C5 PFPeA	126		25-150

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_029.d
 Lims ID: MB 320-142235/1-A
 Client ID:
 Sample Type: MB
 Inject. Date: 15-Dec-2016 16:24:17 ALS Bottle#: 37 Worklist Smp#: 29
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: mb 320-142235/1-a
 Misc. Info.: Plate: 1 Rack: 5
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 15:30:05 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 16-Dec-2016 09:36:47

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.638	1.534	0.104	20598687	59.2		118	1865470	
1 Perfluorobutyric acid	212.90 > 169.00	1.662	1.535	0.127	49942	0.1420			294	
D 4 13C5-PFPeA	267.90 > 223.00	1.925	1.810	0.115	16778664	63.1		126	1032310	
3 Perfluoropentanoic acid	262.90 > 219.00	1.925	1.810	0.115	30961	0.0935			212	
7 Perfluorohexanoic acid	313.00 > 269.00	2.234	2.096	0.138	11872	0.0440			293	
D 6 13C2 PFHxA	315.00 > 270.00	2.234	2.097	0.137	14510716	59.2		118	916569	
D 11 13C4-PFHpA	367.00 > 322.00	2.583	2.426	0.157	14391711	63.6		127	875115	
D 10 18O2 PFHxS	403.00 > 84.00	2.598	2.446	0.152	17112184	52.3		111	2637190	
D 47 M2-6:2FTS	429.00 > 409.00	2.914	2.767	0.147	2254	0.0193		0.0		
48 Sodium 1H,1H,2H,2H-perfluorooctane	427.00 > 407.00	2.922	2.768	0.154	26222	NR				
D 14 13C4 PFOA	417.00 > 372.00	2.946	2.783	0.163	14728125	63.9		128	492862	
D 17 13C4 PFOS	503.00 > 80.00	3.323	3.151	0.172	13670077	54.9		115	725392	
D 19 13C5 PFNA	468.00 > 423.00	3.331	3.153	0.178	11076729	62.3		125	1104643	
D 21 13C8 FOSA	506.00 > 78.00	3.646	3.488	0.158	7421393	19.3		38.6	223585	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
24 Perfluorodecanoic acid	513.00	> 469.00	3.453	3.510	-0.057	1.000	1381	0.006857		41.2
43 Sodium 1H,1H,2H,2H-perfluorooctane	527.00	> 507.00	3.665	3.511	0.154	1.005	557	NR		
D 23 13C2 PFDA	515.00	> 470.00	3.684	3.513	0.171		10669712	67.8	136	252461
D 42 M2-8:2FTS	529.00	> 509.00	3.646	3.513	0.133		1672	0.0156	0.0	
D 45 d3-NMeFOSAA	573.00	> 419.00	3.714	3.676	0.038		277	0.003677	0.0	
26 Perfluorodecane Sulfonic acid	599.00	> 80.00	3.994	3.822	0.172	1.000	1500	0.008982		
28 Perfluoroundecanoic acid	563.00	> 519.00	4.003	3.839	0.164	1.000	14815	0.0982		449
D 27 13C2 PFUnA	565.00	> 520.00	4.003	3.842	0.161		7886494	67.3	135	307591
D 46 d5-NEtFOSAA	589.00	> 419.00	3.813	3.842	-0.029		1856	0.0237	0.0	
49 N-ethyl perfluorooctane sulfonamid	584.00	> 419.00	3.994	3.854	0.140	1.047	2938	NR		
D 52 d-N-MeFOSA-M	515.00	> 169.00	4.021	3.992	0.029		499	0.005249	0.0	
D 30 13C2 PFDoA	615.00	> 570.00	4.296	4.132	0.164		7165157	64.6	129	208244
D 51 d-N-EtFOSA-M	531.00	> 169.00	4.315	4.180	0.135		3524	0.0411	0.0	
D 32 13C2-PFTeDA	715.00	> 670.00	4.799	4.641	0.158		18623446	81.9	164	1508251
33 Perfluorotetradecanoic acid	712.50	> 668.90	4.799	4.642	0.157	1.000	63486	0.2795		31.2
	713.00	> 169.00	4.799	4.642	0.157	1.000	7812	8.13(0.00-0.00)		694
D 34 13C2-PFHxDA	815.00	> 770.00	5.208	5.057	0.151		7506550	60.3	121	242967
35 Perfluorohexadecanoic acid	813.00	> 769.00	5.034	5.059	-0.025	1.000	2379	-0.5252		4.1
36 Perfluorooctadecanoic acid	913.00	> 869.00	5.440	5.414	0.026	1.000	2122	0.0144		3.4

QC Flag Legend

Processing Flags

NR - Missing Quant Standard

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_029.d

Injection Date: 15-Dec-2016 16:24:17

Instrument ID: A8_N

Lims ID: MB 320-142235/1-A

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 37

Worklist Smp#: 29

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: A8_N

Limit Group: LC PFC_DOD ICAL

D 2 13C4 PFBA

1 Perfluorobutyric acid




D 4 13C5-PFPeA



3 Perfluoropentanoic acid

5 Perfluorobutanesulfonic acid (ND)




5 Perfluorobutanesulfonic acid (ND)



7 Perfluorohexanoic acid

D 6 13C2 PFHxA




D 11 13C4-PFHpA

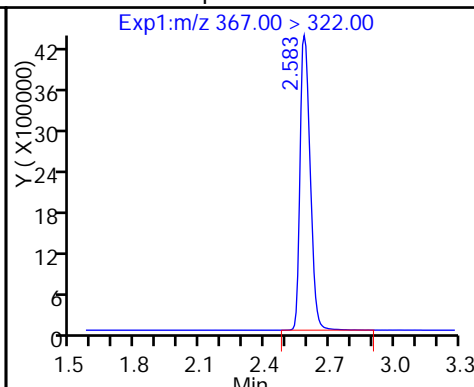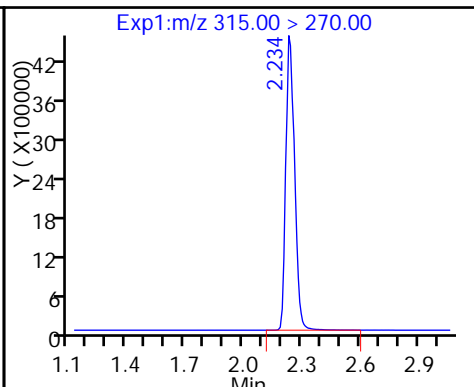

12 Perfluoroheptanoic acid (ND)

9 Perfluorohexanesulfonic acid (ND)


D 10 18O2 PFHxS

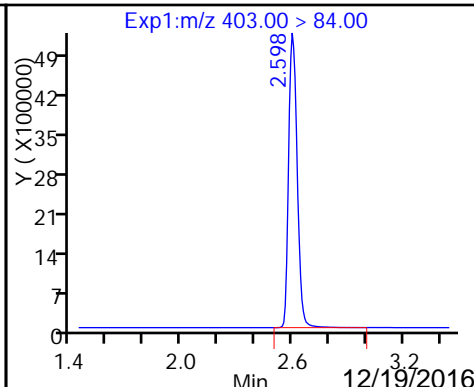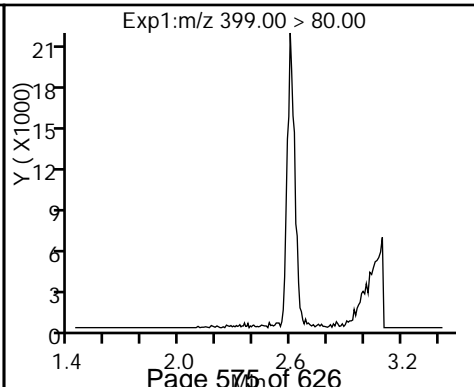

D 47 M2-6:2FTS

48 Sodium 1H,1H,2H,2H-perfluorooctanoate


D 14 13C4 PFOA

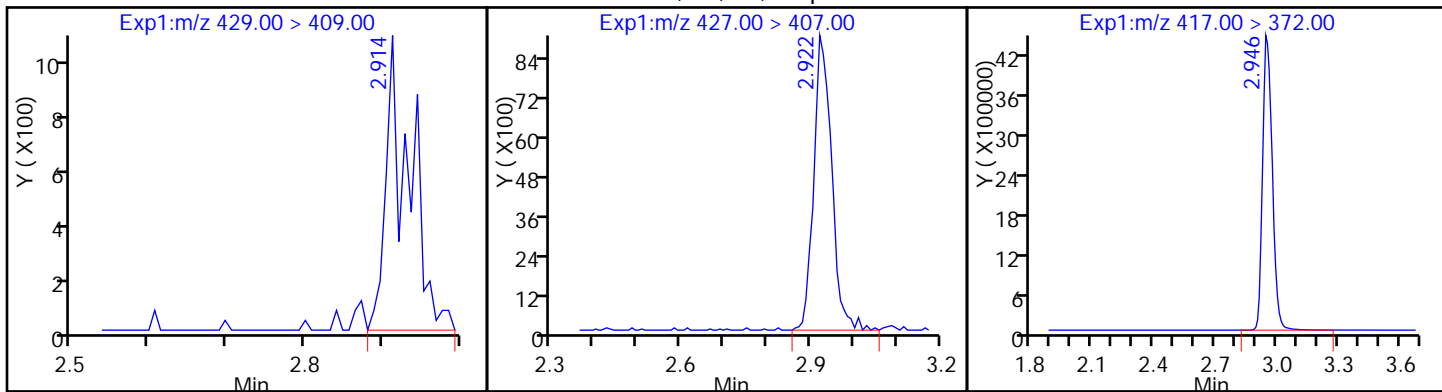

15 Perfluorooctanoic acid (ND)

15 Perfluorooctanoic acid (ND)


13 Perfluoroheptanesulfonic Acid (ND)

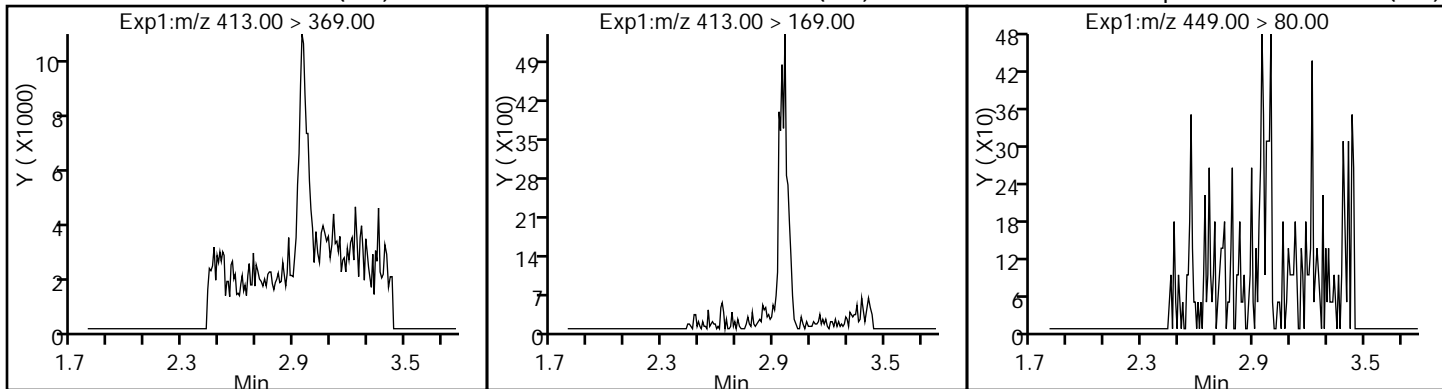

18 Perfluorooctane sulfonic acid (ND)

18 Perfluorooctane sulfonic acid (ND)


D 17 13C4 PFOS

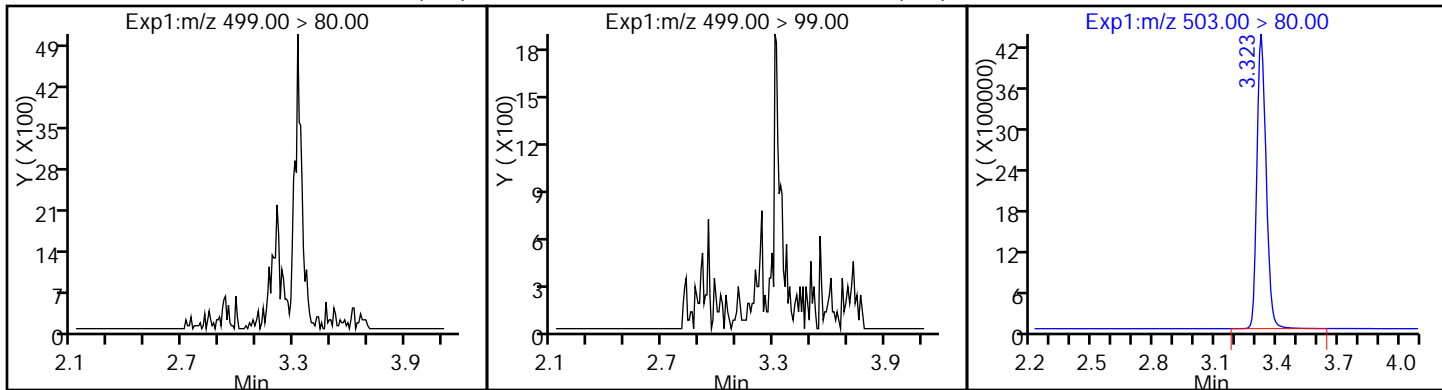

D 19 13C5 PFNA

20 Perfluorononanoic acid (ND)




D 21 13C8 FOSA

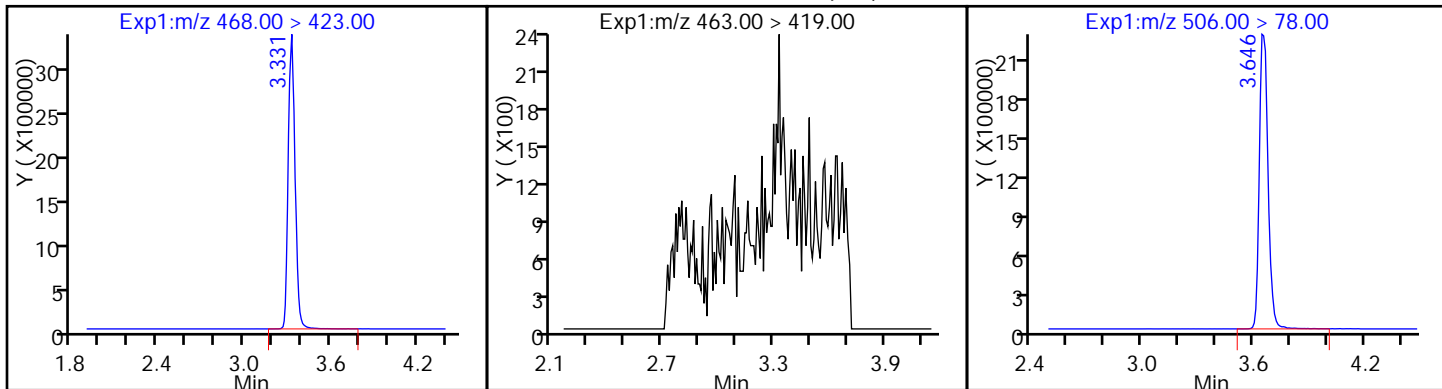

22 Perfluorooctane Sulfonamide (ND)

24 Perfluorodecanoic acid




43 Sodium 1H,1H,2H,2H-perfluorooctane

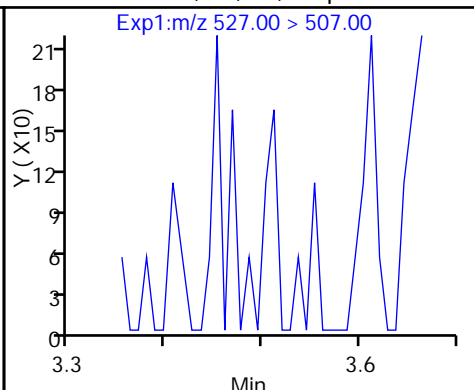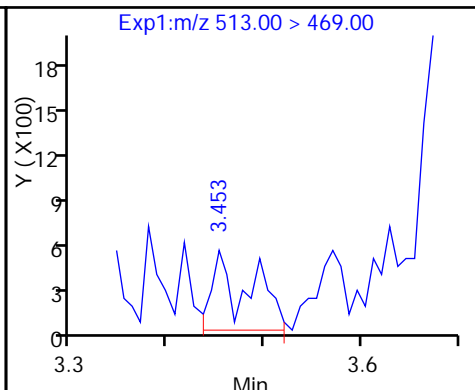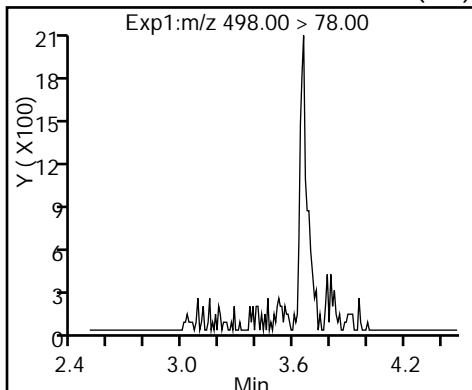

D 23 13C2 PFDA

D 42 M2-8:2FTS




D 45 d3-NMeFOSAA

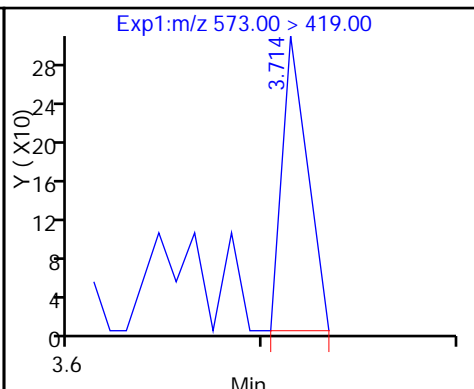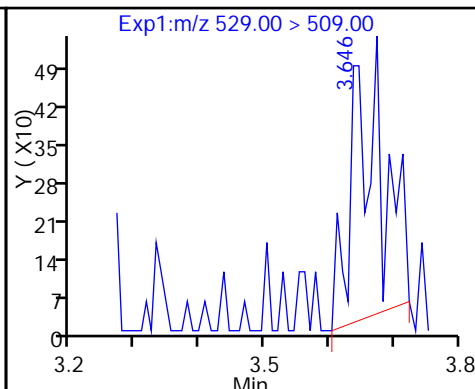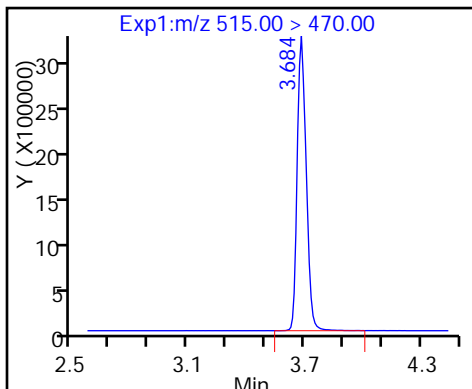

44 N-methyl perfluorooctane sulfonami

26 Perfluorodecanoic Sulfonic acid




28 Perfluoroundecanoic acid

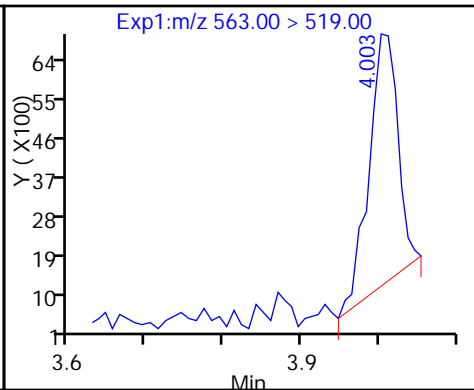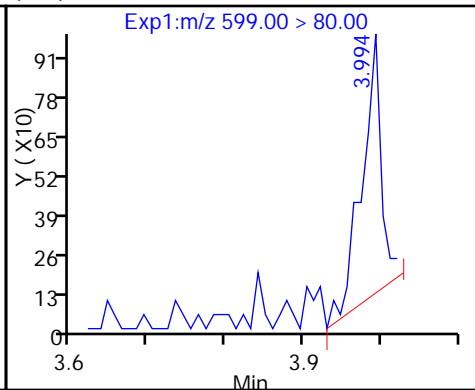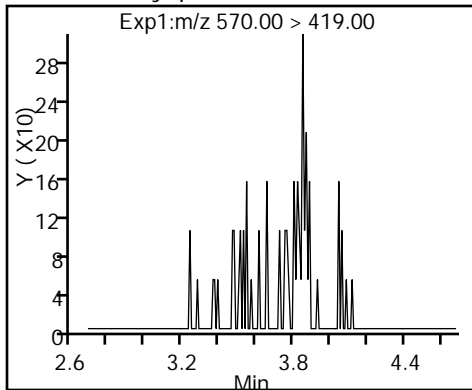

D 27 13C2 PFUnA

D 46 d5-NEtFOSAA




49 N-ethyl perfluorooctane sulfonamid

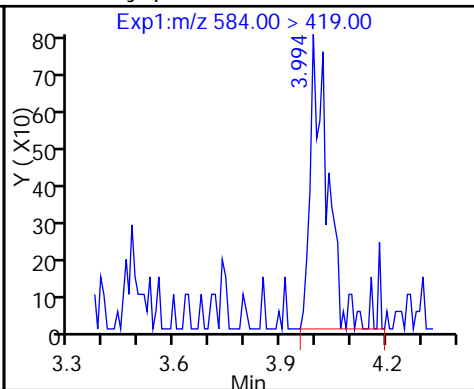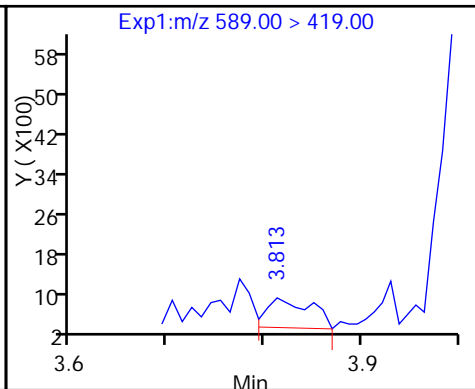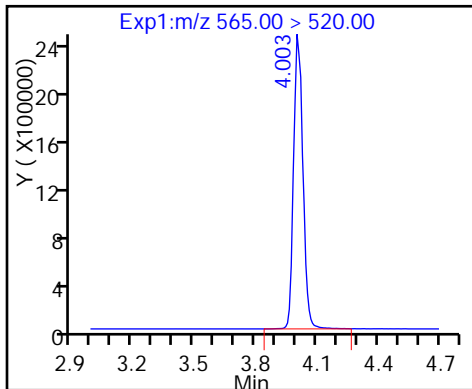

D 52 d-N-MeFOSA-M

54 MeFOSA (ND)




D 30 13C2 PFDoA

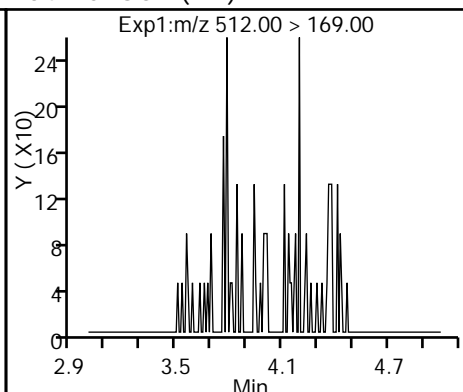

29 Perfluorododecanoic acid (ND)

D 51 d-N-EtFOSA-M




53 N-ethylperfluoro-1-octanesulfonami (ND)

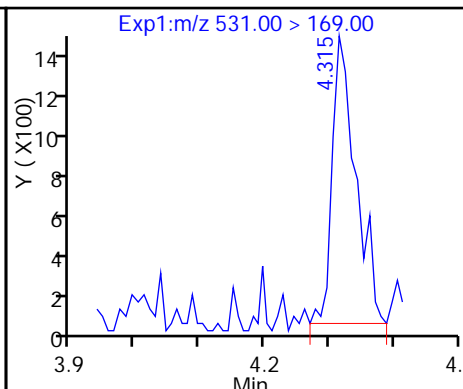

31 Perfluorotridecanoic acid (ND)

D 32 13C2-PFTeDA




33 Perfluorotetradecanoic acid




33 Perfluorotetradecanoic acid

D 34 13C2-PFHxDA

35 Perfluorohexadecanoic acid

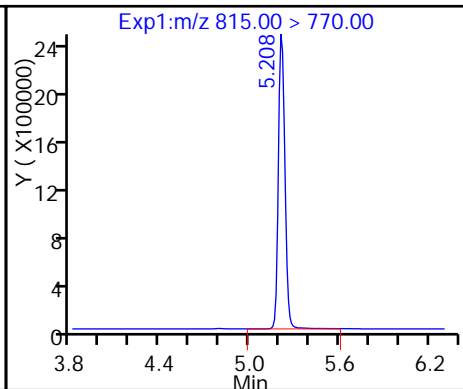

36 Perfluorooctadecanoic acid

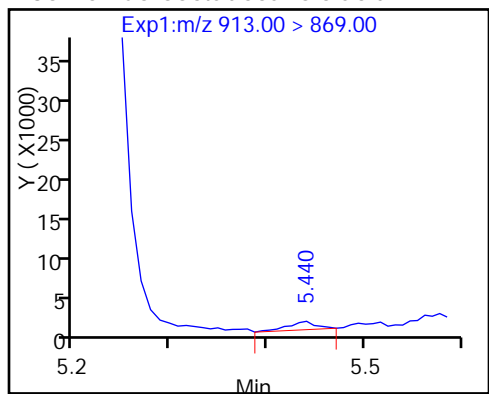

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: LCS 320-142235/2-A
 Matrix: Water Lab File ID: 15DEC2016B_030.d
 Analysis Method: 537 (Modified) Date Collected: _____
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 250 (mL) Date Analyzed: 12/15/2016 16:31
 Con. Extract Vol.: 0.5 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: Acquity ID: 2.1 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142379 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
375-22-4	Perfluorobutanoic acid (PFBA)	41.3		2.5	1.0	0.46
2706-90-3	Perfluoropentanoic acid (PFPeA)	40.6		2.5	2.0	0.99
307-24-4	Perfluorohexanoic acid (PFHxA)	38.6		2.5	2.0	0.79
375-85-9	Perfluoroheptanoic acid (PFHpA)	37.8		2.5	2.0	0.80
335-67-1	Perfluorooctanoic acid (PFOA)	39.8		2.5	2.0	0.75
375-95-1	Perfluorononanoic acid (PFNA)	38.5	M	2.5	2.0	0.65
335-76-2	Perfluorodecanoic acid (PFDA)	37.7		2.5	1.0	0.44
2058-94-8	Perfluoroundecanoic acid (PFUnA)	38.1		2.5	2.0	0.75
307-55-1	Perfluorododecanoic acid (PFDoA)	38.5		2.5	2.0	0.58
72629-94-8	Perfluorotridecanoic Acid (PFTriA)	41.4		2.5	2.0	0.55
376-06-7	Perfluorotetradecanoic acid (PFTeA)	43.7		2.5	1.0	0.40
375-73-5	Perfluorobutanesulfonic acid (PFBS)	39.8		2.5	2.0	0.92
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	34.7		2.5	2.0	0.87
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	37.5		4.0	3.0	1.3
335-77-3	Perfluorodecanesulfonic acid (PFDS)	38.2		4.0	3.0	1.2
754-91-6	Perfluorooctane Sulfonamide (FOSA)	38.3		2.5	2.0	0.64

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: LCS 320-142235/2-A
 Matrix: Water Lab File ID: 15DEC2016B_030.d
 Analysis Method: 537 (Modified) Date Collected: _____
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 250 (mL) Date Analyzed: 12/15/2016 16:31
 Con. Extract Vol.: 0.5 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: Acquity ID: 2.1 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142379 Units: ng/L

CAS NO.	ISOTOPE DILUTION	%REC	Q	LIMITS
STL01056	13C8 FOSA	13	Q	25-150
STL00992	13C4 PFBA	105		25-150
STL00993	13C2 PFHxA	103		25-150
STL00990	13C4 PFOA	110		25-150
STL00995	13C5 PFNA	111		25-150
STL00996	13C2 PFDA	122		25-150
STL00997	13C2 PFUnA	116		25-150
STL00998	13C2 PFDoA	112		25-150
STL00994	18O2 PFHxS	100		25-150
STL00991	13C4 PFOS	101		25-150
STL01892	13C4-PFHpA	110		25-150
STL01893	13C5 PFPeA	107		25-150

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_030.d
 Lims ID: LCS 320-142235/2-A
 Client ID:
 Sample Type: LCS
 Inject. Date: 15-Dec-2016 16:31:49 ALS Bottle#: 38 Worklist Smp#: 30
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: lcs 320-142235/2-a
 Misc. Info.: Plate: 1 Rack: 5
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 15:30:05 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 16-Dec-2016 09:38:15

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.630	1.534	0.096	18191322	52.3		105	1604384	
1 Perfluorobutyric acid	212.90 > 169.00	1.630	1.535	0.095	6419259	20.7		103	44385	
D 4 13C5-PFPeA	267.90 > 223.00	1.916	1.810	0.106	14216005	53.4		107	2214644	
3 Perfluoropentanoic acid	262.90 > 219.00	1.916	1.810	0.106	5690233	20.3		101	38700	
5 Perfluorobutanesulfonic acid	298.90 > 80.00	1.955	1.848	0.107	9209546	19.9		113		
	298.90 > 99.00	1.955	1.848	0.107	3906521		2.36(0.00-0.00)			
7 Perfluorohexanoic acid	313.00 > 269.00	2.222	2.096	0.126	4549209	19.3		96.6	109234	
D 6 13C2 PFHxA	315.00 > 270.00	2.231	2.097	0.134	12680151	51.7		103	638466	
D 11 13C4-PFHpA	367.00 > 322.00	2.576	2.426	0.150	12416361	54.9		110	1261192	
12 Perfluoroheptanoic acid	363.00 > 319.00	2.576	2.428	0.148	4595914	18.9		94.5	49499	
9 Perfluorohexanesulfonic acid	399.00 > 80.00	2.591	2.431	0.160	5828948	17.3		95.2		
D 10 18O2 PFHxS	403.00 > 84.00	2.591	2.446	0.145	15450301	47.3		99.9	2382881	
D 14 13C4 PFOA	417.00 > 372.00	2.938	2.783	0.155	12723737	55.2		110	770784	
15 Perfluorooctanoic acid	413.00 > 369.00	2.946	2.783	0.163	5079169	19.9		99.5	51309	
	413.00 > 169.00	2.938	2.783	0.155	2947621		1.72(0.90-1.10)		176408	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
13 Perfluoroheptanesulfonic Acid	449.00 > 80.00	2.954	2.790	0.164	1.000	5507681	19.8	104		
18 Perfluorooctane sulfonic acid	499.00 > 80.00	3.294	3.118	0.176	1.000	4706307	18.8	101	221474	
	499.00 > 99.00	3.317	3.118	0.199	1.007	998693		4.71(0.90-1.10)	66990	
D 17 13C4 PFOS	503.00 > 80.00	3.317	3.151	0.166		12057881	48.5	101	292378	
D 19 13C5 PFNA	468.00 > 423.00	3.317	3.153	0.164		9840334	55.4	111	332485	
20 Perfluorononanoic acid	463.00 > 419.00	3.309	3.155	0.154	1.000	3604467	19.2	96.2	51205	M
D 21 13C8 FOSA	506.00 > 78.00	3.641	3.488	0.153		2495483	6.50	13.0	99813	
22 Perfluorooctane Sulfonamide	498.00 > 78.00	3.641	3.491	0.150	1.000	891236	19.1	95.7	75304	
24 Perfluorodecanoic acid	513.00 > 469.00	3.669	3.510	0.159	1.000	3418934	18.9	94.3	65129	
D 23 13C2 PFDA	515.00 > 470.00	3.669	3.513	0.156		9600381	61.0	122	203535	
26 Perfluorodecane Sulfonic acid	599.00 > 80.00	3.976	3.822	0.154	1.000	2817140	19.1	99.2		
28 Perfluoroundecanoic acid	563.00 > 519.00	3.995	3.839	0.156	1.000	2472320	19.0	95.2	62630	
D 27 13C2 PFUnA	565.00 > 520.00	3.995	3.842	0.153		6792624	57.9	116	161681	
D 30 13C2 PFDoA	615.00 > 570.00	4.284	4.132	0.152		6237089	56.2	112	179080	
29 Perfluorododecanoic acid	613.00 > 569.00	4.294	4.136	0.158	1.000	2205977	19.3	96.3	8038	
31 Perfluorotridecanoic acid	663.00 > 619.00	4.547	4.400	0.147	1.000	2340490	20.7	103	2895	
D 32 13C2-PFTeDA	715.00 > 670.00	4.786	4.641	0.145		15218546	66.9	134	1723623	
33 Perfluorotetradecanoic acid	712.50 > 668.90	4.786	4.642	0.144	1.000	4317631	21.8	109	2510	
	713.00 > 169.00	4.786	4.642	0.144	1.000	746644		5.78(0.00-0.00)	60978	
D 34 13C2-PFHxDA	815.00 > 770.00	5.199	5.057	0.142		6406998	51.4	103	211048	
35 Perfluorohexadecanoic acid	813.00 > 769.00	5.199	5.059	0.140	1.000	2081300	16.9	84.6	3872	
36 Perfluorooctadecanoic acid	913.00 > 869.00	5.569	5.414	0.155	1.000	2323407	18.1	90.4	2756	

QC Flag Legend

Review Flags

M - Manually Integrated

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_030.d

Injection Date: 15-Dec-2016 16:31:49

Instrument ID: A8_N

Lims ID: LCS 320-142235/2-A

Client ID:

Operator ID: A8-PC\A8

ALS Bottle#: 38

Worklist Smp#: 30

Injection Vol: 2.0 ul

Dil. Factor: 1.0000













Method: A8_N

Limit Group: LC PFC_DOD ICAL


D 2 13C4 PFBA

1 Perfluorobutyric acid


D 4 13C5-PFPeA

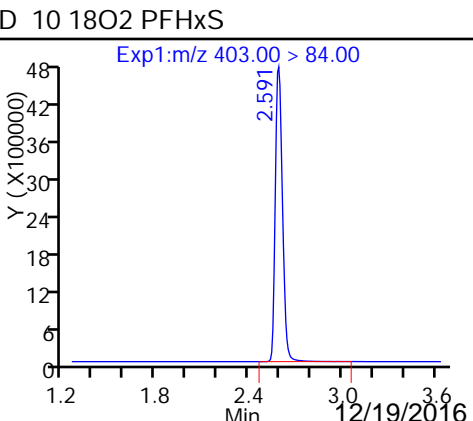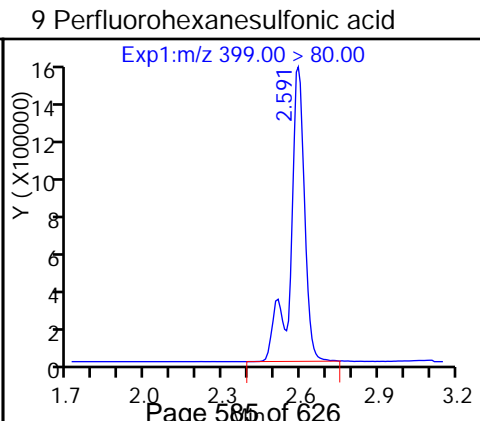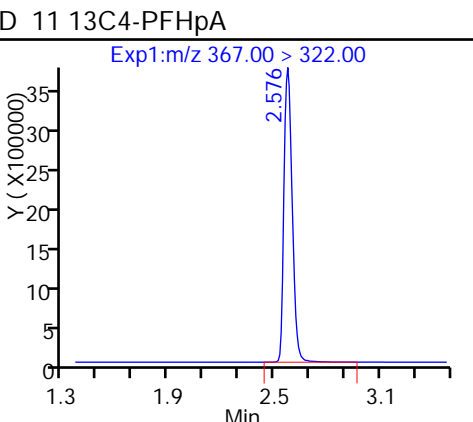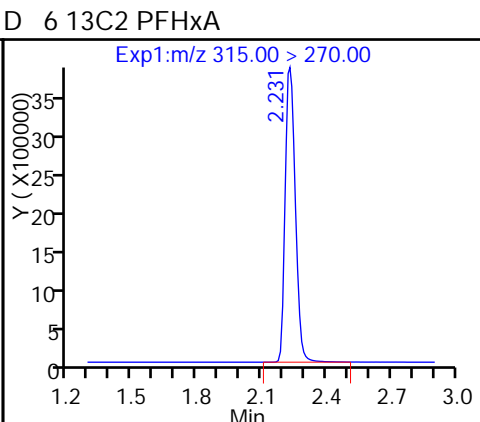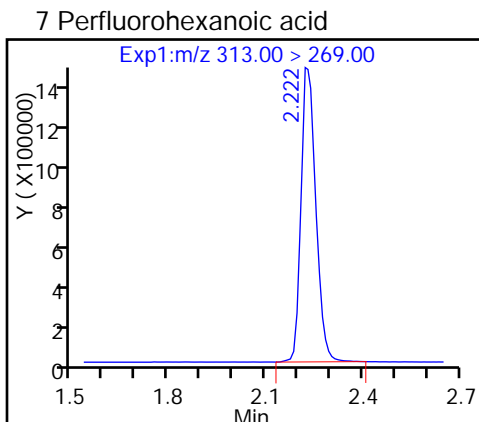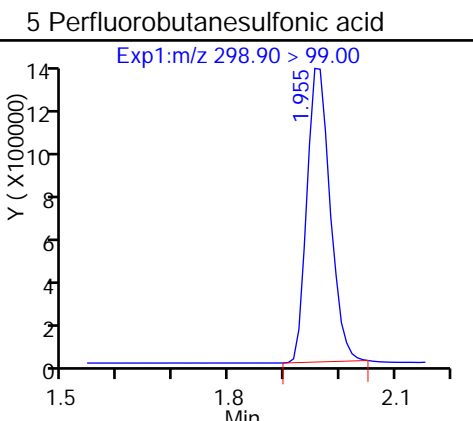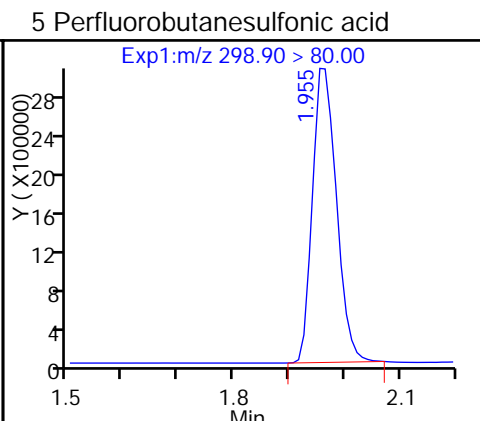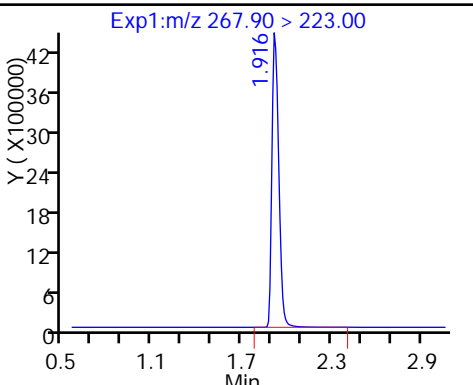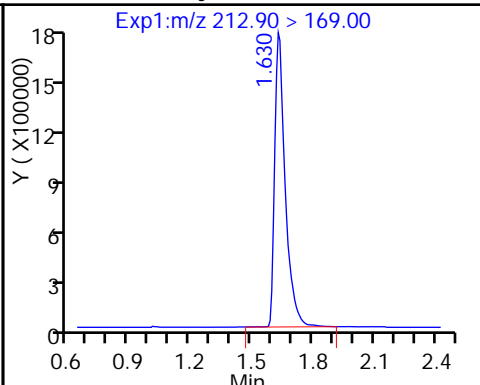


D 14 13C4 PFOA




15 Perfluorooctanoic acid




15 Perfluorooctanoic acid

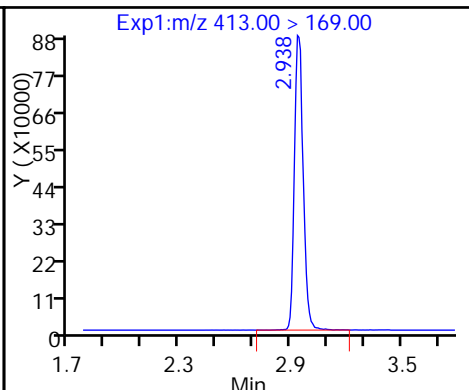


13 Perfluoroheptanesulfonic Acid




18 Perfluorooctane sulfonic acid




18 Perfluorooctane sulfonic acid




D 17 13C4 PFOS




D 19 13C5 PFNA




20 Perfluorononanoic acid (M)

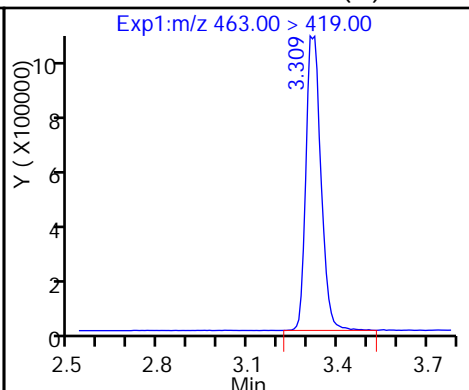


D 21 13C8 FOSA




22 Perfluorooctane Sulfonamide




24 Perfluorodecanoic acid




D 23 13C2 PFDA

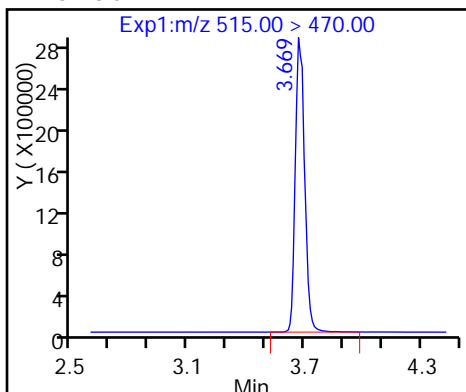


26 Perfluorodecane Sulfonic acid

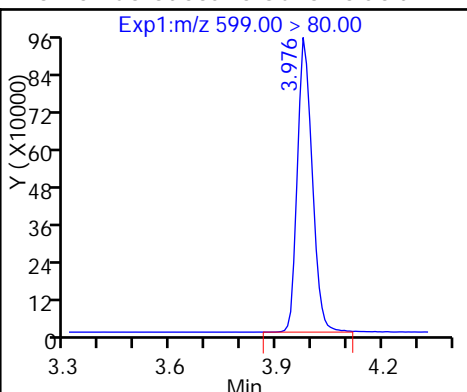


28 Perfluoroundecanoic acid

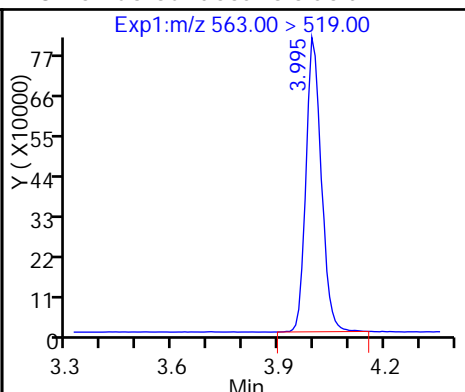


D 27 13C2 PFUa

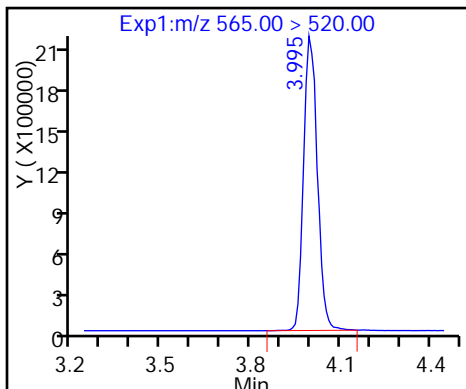


D 30 13C2 PFDa

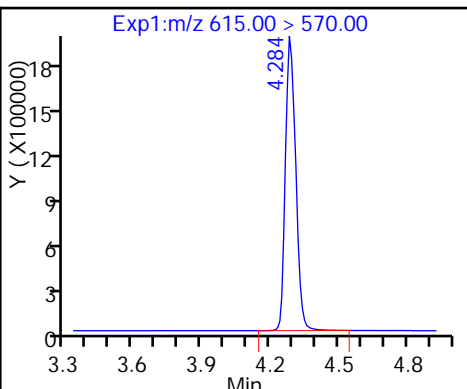


29 Perfluorododecanoic acid

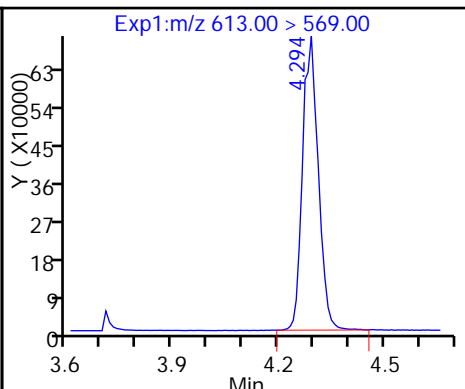


31 Perfluorotridecanoic acid

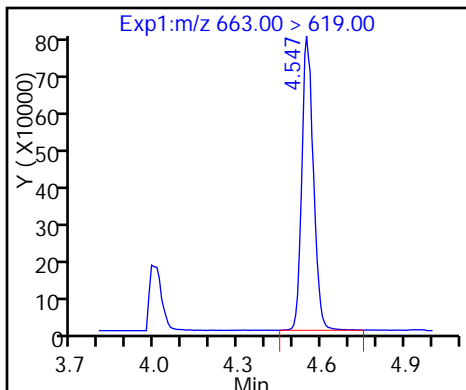


D 32 13C2-PFTeDA

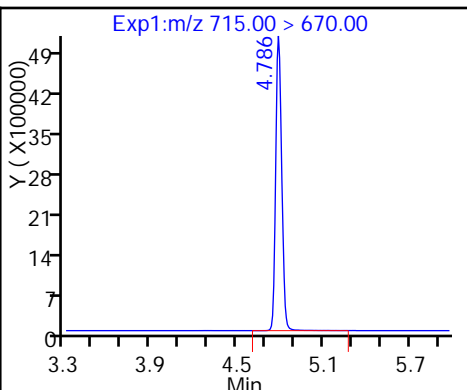


33 Perfluorotetradecanoic acid

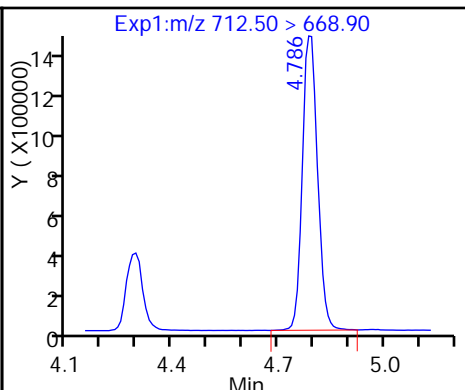


33 Perfluorotetradecanoic acid

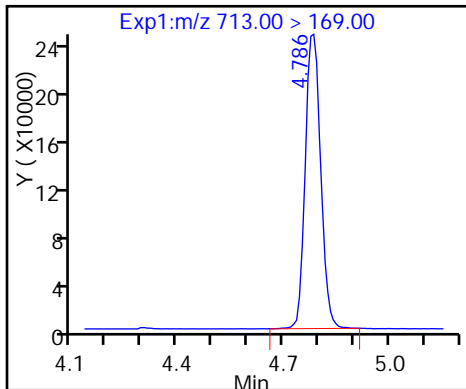


D 34 13C2-PFHxDA

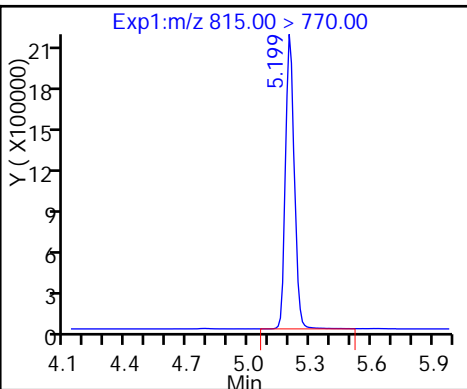

35 Perfluorohexadecanoic acid

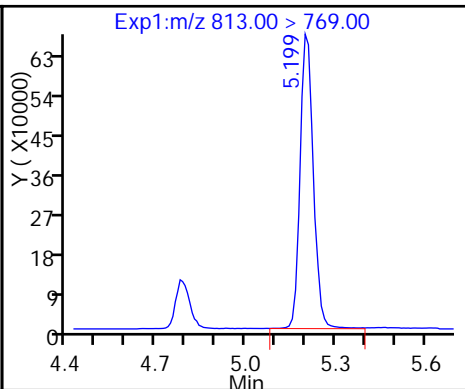

36 Perfluorooctadecanoic acid

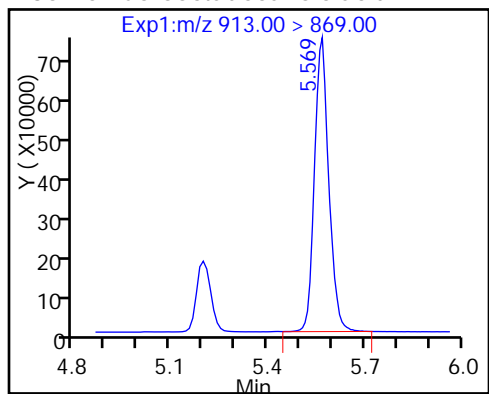

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_030.d
Injection Date: 15-Dec-2016 16:31:49 Instrument ID: A8_N
Lims ID: LCS 320-142235/2-A
Client ID:
Operator ID: A8-PC\A8 ALS Bottle#: 38 Worklist Smp#: 30
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: A8_N Limit Group: LC PFC_DOD ICAL
Column: Detector EXP1

20 Perfluorononanoic acid, CAS: 375-95-1

Signal: 1


RT: 3.31
Area: 2796058
Amount: 14.926260
Amount Units: ng/ml

Processing Integration Results

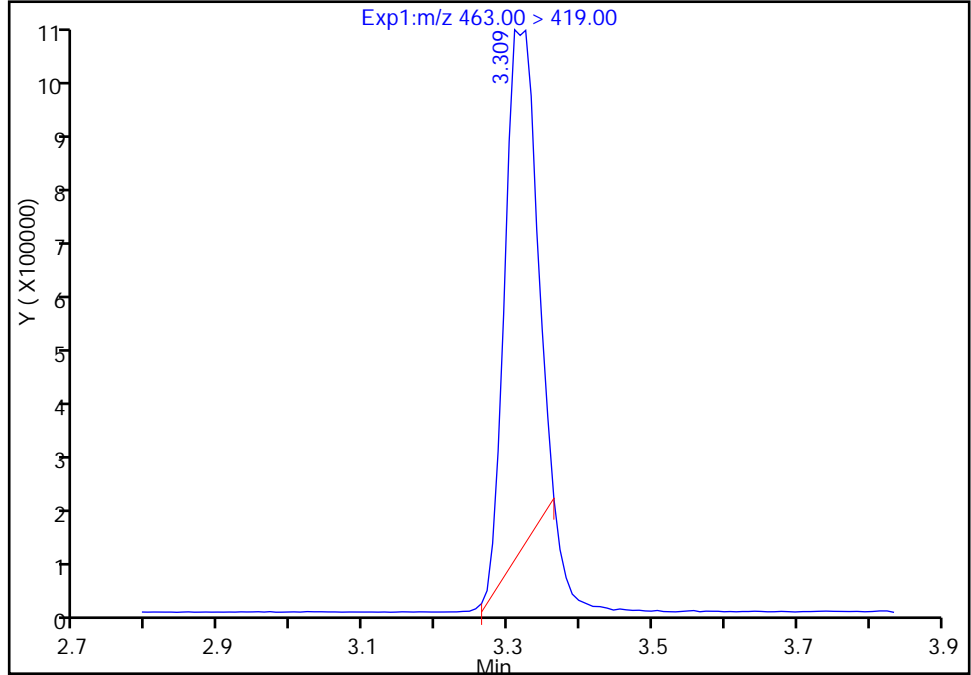

RT: 3.31
Area: 3604467
Amount: 19.241809
Amount Units: ng/ml

Manual Integration Results

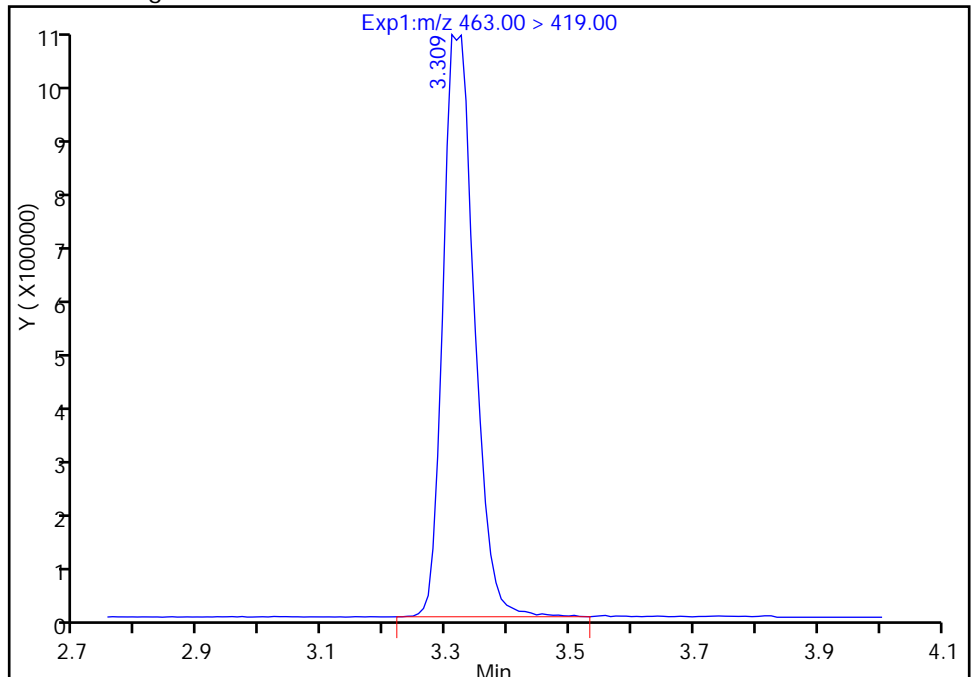

Reviewer: chandrasenas, 16-Dec-2016 09:38:15
Audit Action: Manually Integrated

Audit Reason: Incomplete Integration

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: CS-1 MS Lab Sample ID: 320-24118-6 MS
 Matrix: Water Lab File ID: 15DEC2016B_037.d
 Analysis Method: 537 (Modified) Date Collected: 12/06/2016 09:17
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 260.8 (mL) Date Analyzed: 12/15/2016 17:24
 Con. Extract Vol.: 0.5 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: Acquity ID: 2.1 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142379 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
375-22-4	Perfluorobutanoic acid (PFBA)	40.3		2.4	0.96	0.44
2706-90-3	Perfluoropentanoic acid (PFPeA)	38.5		2.4	1.9	0.95
307-24-4	Perfluorohexanoic acid (PFHxA)	37.3		2.4	1.9	0.75
375-85-9	Perfluoroheptanoic acid (PFHpA)	37.4		2.4	1.9	0.77
335-67-1	Perfluorooctanoic acid (PFOA)	38.1		2.4	1.9	0.72
375-95-1	Perfluorononanoic acid (PFNA)	37.4		2.4	1.9	0.63
335-76-2	Perfluorodecanoic acid (PFDA)	36.8		2.4	0.96	0.42
2058-94-8	Perfluoroundecanoic acid (PFUnA)	37.7		2.4	1.9	0.72
307-55-1	Perfluorododecanoic acid (PFDoA)	37.6		2.4	1.9	0.56
72629-94-8	Perfluorotridecanoic Acid (PFTriA)	52.7		2.4	1.9	0.53
376-06-7	Perfluorotetradecanoic acid (PFTeA)	58.5	J	2.4	0.96	0.38
375-73-5	Perfluorobutanesulfonic acid (PFBS)	39.2		2.4	1.9	0.88
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	34.1		2.4	1.9	0.83
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	37.8		3.8	2.9	1.2
335-77-3	Perfluorodecanesulfonic acid (PFDS)	37.7		3.8	2.9	1.2
754-91-6	Perfluorooctane Sulfonamide (FOSA)	37.6		2.4	1.9	0.61

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: <u>TestAmerica Sacramento</u>	Job No.: <u>320-24118-1</u>
SDG No.: _____	
Client Sample ID: <u>CS-1 MS</u>	Lab Sample ID: <u>320-24118-6 MS</u>
Matrix: <u>Water</u>	Lab File ID: <u>15DEC2016B_037.d</u>
Analysis Method: <u>537 (Modified)</u>	Date Collected: <u>12/06/2016 09:17</u>
Extraction Method: <u>3535</u>	Date Extracted: <u>12/14/2016 18:18</u>
Sample wt/vol: <u>260.8 (mL)</u>	Date Analyzed: <u>12/15/2016 17:24</u>
Con. Extract Vol.: <u>0.5 (mL)</u>	Dilution Factor: <u>1</u>
Injection Volume: <u>2 (uL)</u>	GC Column: <u>Acquity</u> ID: <u>2.1 (mm)</u>
% Moisture: _____	GPC Cleanup: (Y/N) <u>N</u>
Analysis Batch No.: <u>142379</u>	Units: <u>ng/L</u>

CAS NO.	ISOTOPE DILUTION	%REC	Q	LIMITS
STL01056	13C8 FOSA	6	Q	25-150
STL00992	13C4 PFBA	93		25-150
STL00993	13C2 PFHxA	102		25-150
STL00990	13C4 PFOA	101		25-150
STL00995	13C5 PFNA	82		25-150
STL00996	13C2 PFDA	82		25-150
STL00997	13C2 PFUnA	92		25-150
STL00998	13C2 PFDoA	110		25-150
STL00994	18O2 PFHxS	123		25-150
STL00991	13C4 PFOS	125		25-150
STL01892	13C4-PFHpA	107		25-150
STL01893	13C5 PFPeA	117		25-150

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_037.d
 Lims ID: 320-24118-B-6-B MS
 Client ID: CS-1
 Sample Type: MS
 Inject. Date: 15-Dec-2016 17:24:19 ALS Bottle#: 45 Worklist Smp#: 37
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-24118-b-6-b ms
 Misc. Info.: Plate: 1 Rack: 5
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 15:30:05 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 16-Dec-2016 15:28:51

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.705	1.534	0.171	16181658	46.5		93.1	812703	
1 Perfluorobutyric acid	212.90 > 169.00	1.705	1.535	0.170	5802787	21.0		105	29890	
D 4 13C5-PFPeA	267.90 > 223.00	2.005	1.810	0.195	15616198	58.7		117	1554359	
3 Perfluoropentanoic acid	262.90 > 219.00	2.005	1.810	0.195	6186158	20.1		100	52637	
5 Perfluorobutanesulfonic acid	298.90 > 80.00	2.044	1.848	0.196	11653029	20.5		116		
	298.90 > 99.00	2.044	1.848	0.196	4931116		2.36(0.00-0.00)			
7 Perfluorohexanoic acid	313.00 > 269.00	2.330	2.096	0.234	4507901	19.4		97.2	77183	
D 6 13C2 PFHxA	315.00 > 270.00	2.320	2.097	0.223	12481400	50.9		102	636085	
D 11 13C4-PFHpA	367.00 > 322.00	2.681	2.426	0.255	12164170	53.7		107	893473	
12 Perfluoroheptanoic acid	363.00 > 319.00	2.673	2.428	0.245	4650793	19.5		97.7	37452	
9 Perfluorohexanesulfonic acid	399.00 > 80.00	2.688	2.431	0.257	7367757	17.8		97.8		
D 10 18O2 PFHxS	403.00 > 84.00	2.688	2.446	0.242	19006327	58.1		123	1823134	
D 14 13C4 PFOA	417.00 > 372.00	3.048	2.783	0.265	11681140	50.7		101	1127614	
15 Perfluorooctanoic acid	413.00 > 369.00	3.048	2.783	0.265	4655925	19.9		99.3	36143	
	413.00 > 169.00	3.048	2.783	0.265	2724722		1.71(0.90-1.10)		194597	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
13 Perfluoroheptanesulfonic Acid	449.00 > 80.00	3.058	2.790	0.268	1.000	7226846	21.0	110		
18 Perfluorooctane sulfonic acid	499.00 > 80.00	3.305	3.118	0.187	1.000	6107430	19.7	106	57903	
	499.00 > 99.00	3.424	3.118	0.306	1.036	1277606	4.78(0.90-1.10)		65911	
D 17 13C4 PFOS	503.00 > 80.00	3.424	3.151	0.273		14905185	59.9	125	398684	
D 19 13C5 PFNA	468.00 > 423.00	3.424	3.153	0.271		7254517	40.8	81.7	662107	
20 Perfluorononanoic acid	463.00 > 419.00	3.424	3.155	0.269	1.000	2695597	19.5	97.6	38874	
D 21 13C8 FOSA	506.00 > 78.00	3.744	3.488	0.256		1082943	2.82	5.6	83058	
22 Perfluorooctane Sulfonamide	498.00 > 78.00	3.755	3.491	0.264	1.000	396061	19.6	98.0	31903	
24 Perfluorodecanoic acid	513.00 > 469.00	3.775	3.510	0.265	1.000	2349937	19.2	96.1	56109	
D 23 13C2 PFDA	515.00 > 470.00	3.775	3.513	0.262		6477275	41.2	82.4	93837	
D 42 M2-8:2FTS	529.00 > 509.00	3.620	3.513	0.107		401	0.003732	0.0		
D 45 d3-NMeFOSAA	573.00 > 419.00	3.460	3.676	-0.216		565	0.007501	0.0		
26 Perfluorodecane Sulfonic acid	599.00 > 80.00	4.075	3.822	0.253	1.000	3578170	19.7	102		
28 Perfluoroundecanoic acid	563.00 > 519.00	4.097	3.839	0.258	1.000	2026698	19.7	98.3	56028	
D 27 13C2 PFUnA	565.00 > 520.00	4.097	3.842	0.255		5387549	45.9	91.9	205833	
D 46 d5-NEtFOSAA	589.00 > 419.00	3.816	3.842	-0.026		2533	0.0323	0.0		
D 52 d-N-MeFOSA-M	515.00 > 169.00	3.775	3.992	-0.217		543256	5.71	0.0		
D 30 13C2 PFDaA	615.00 > 570.00	4.390	4.132	0.258		6102520	55.0	110	179434	
29 Perfluorododecanoic acid	613.00 > 569.00	4.390	4.136	0.254	1.000	2197146	19.6	98.1	4134	
D 51 d-N-EtFOSA-M	531.00 > 169.00	4.217	4.180	0.037		222	0.002588	0.0		
53 N-ethylperfluoro-1-octanesulfonami	526.00 > 169.00	4.195	4.187	0.008	1.000	248	NR	0.0		
31 Perfluorotridecanoic acid	663.00 > 619.00	4.642	4.400	0.242	1.000	3044576	27.5	138	4550	
D 32 13C2-PFTeDA	715.00 > 670.00	4.884	4.641	0.243		19500525	85.8	172	895209	

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
33 Perfluorotetradecanoic acid										
712.50 > 668.90	4.884	4.642	0.242	1.000	5900470	30.5		153	4041	
713.00 > 169.00	4.876	4.642	0.234	0.998	1017964		5.80(0.00-0.00)		84909	
D 34 13C2-PFHxDA										
815.00 > 770.00	5.296	5.057	0.239		7555753	60.7		121	198612	
35 Perfluorohexadecanoic acid										
813.00 > 769.00	5.296	5.059	0.237	1.000	2598687	21.7		109	4676	
36 Perfluorooctadecanoic acid										
913.00 > 869.00	5.650	5.414	0.236	1.000	2610316	20.8		104	3865	

QC Flag Legend

Processing Flags

NR - Missing Quant Standard

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_037.d

Injection Date: 15-Dec-2016 17:24:19

Instrument ID: A8_N

Lims ID: 320-24118-B-6-B MS

Client ID: CS-1

Operator ID: A8-PC\A8

ALS Bottle#: 45

Worklist Smp#: 37

Injection Vol: 2.0 ul

Dil. Factor: 1.0000













Method: A8_N

Limit Group: LC PFC_DOD ICAL

D 2 13C4 PFBA


1 Perfluorobutyric acid

D 4 13C5-PFPeA

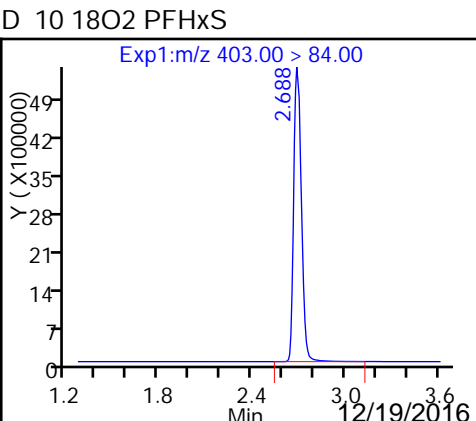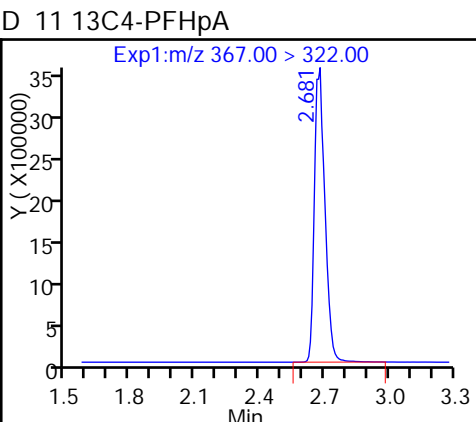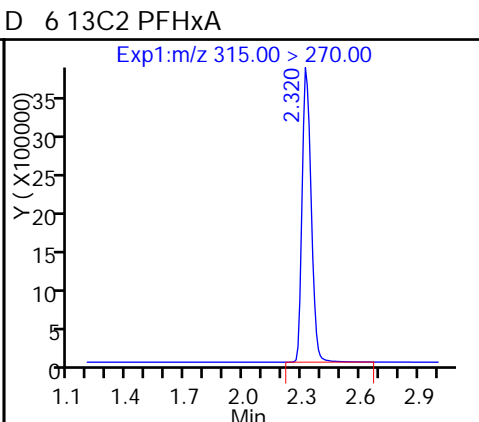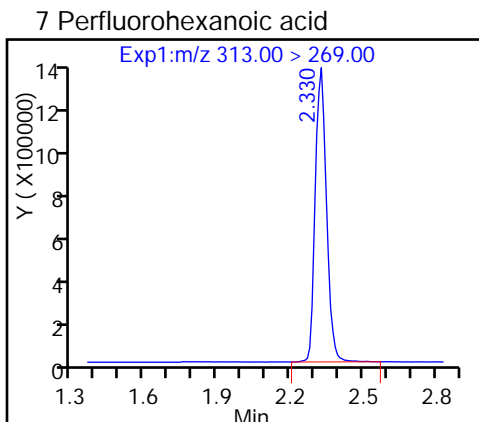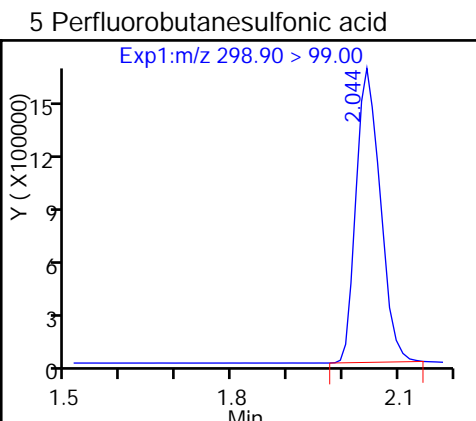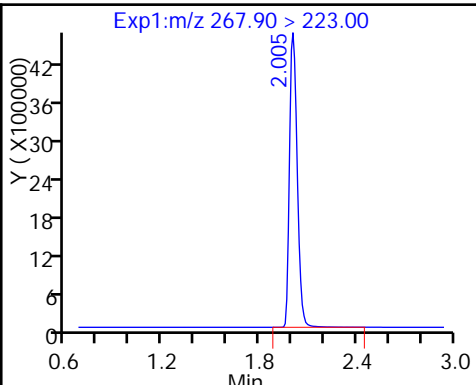

D 47 M2-6:2FTS (ND)


48 Sodium 1H,1H,2H,2H-perfluorooctadecanoate (MD) 3C4 PFOA

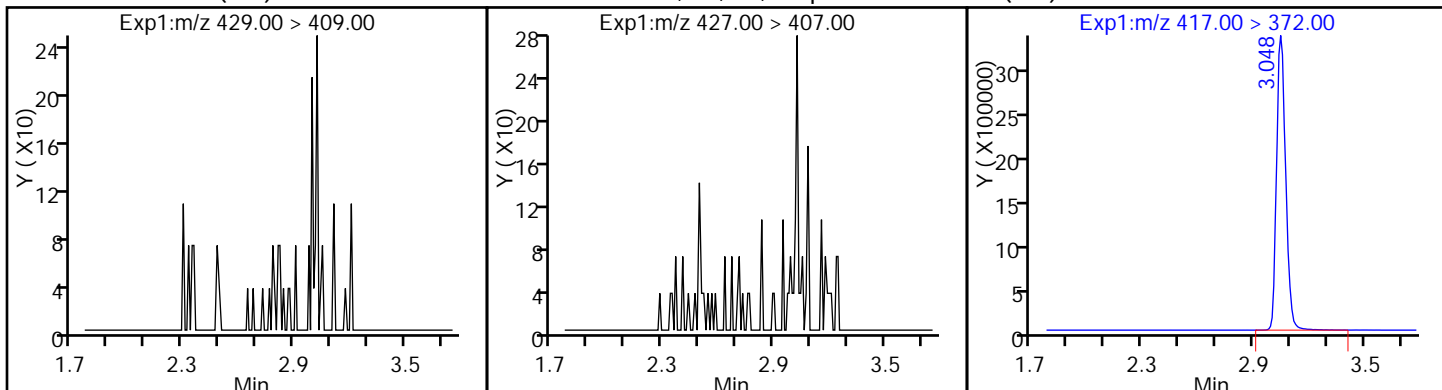

15 Perfluorooctanoic acid

15 Perfluorooctanoic acid


13 Perfluoroheptanesulfonic Acid

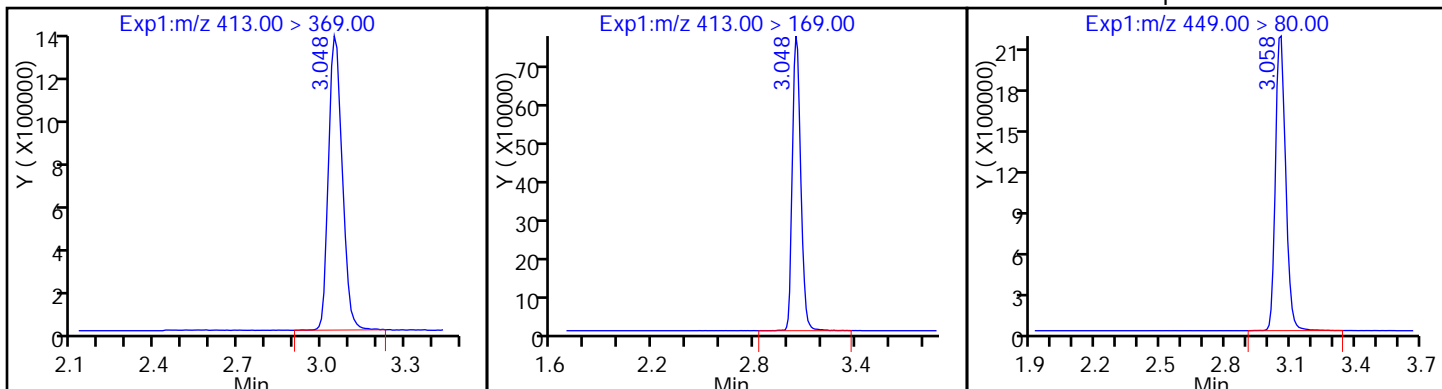

18 Perfluorooctane sulfonic acid

18 Perfluorooctane sulfonic acid


D 17 13C4 PFOS

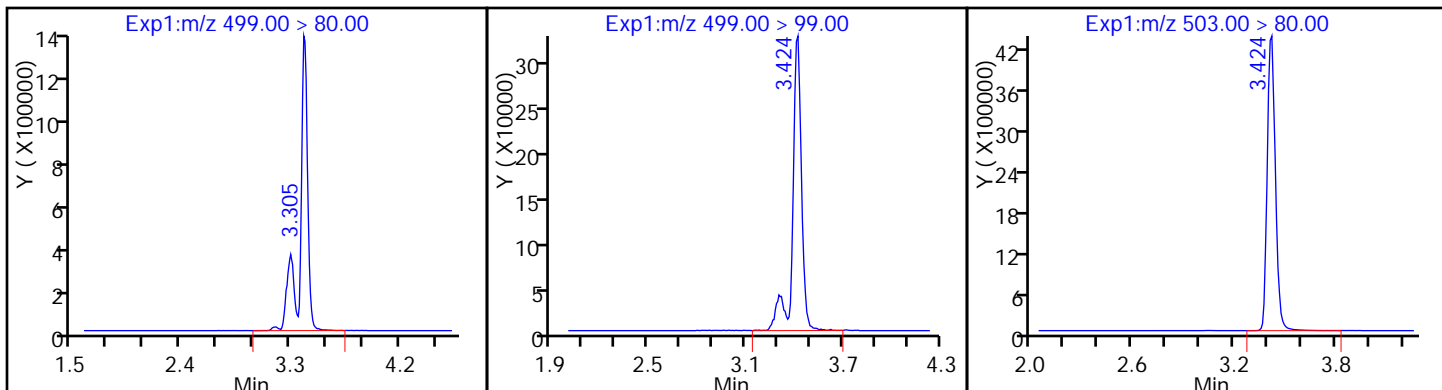


D 19 13C5 PFNA

20 Perfluorononanoic acid


D 21 13C8 FOSA

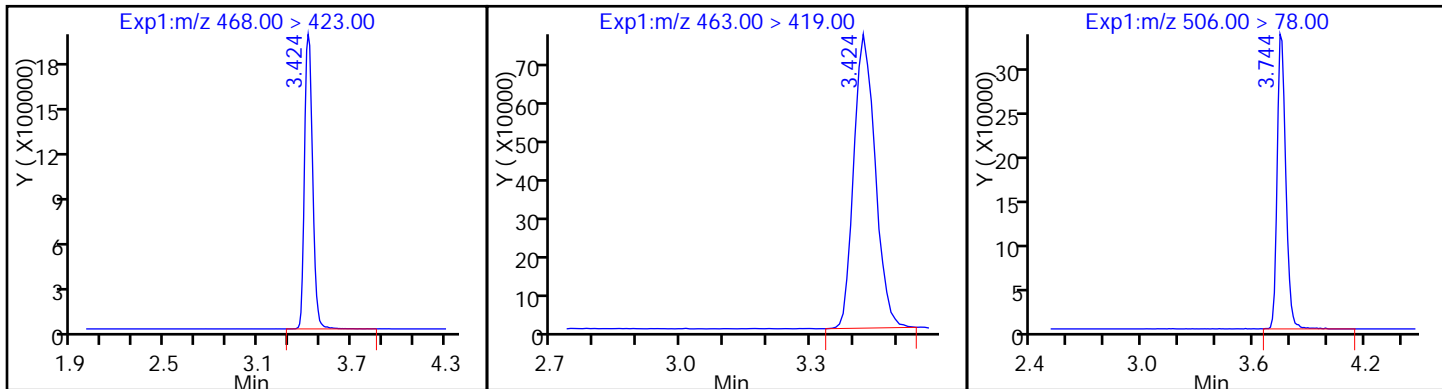


22 Perfluorooctane Sulfonamide




24 Perfluorodecanoic acid

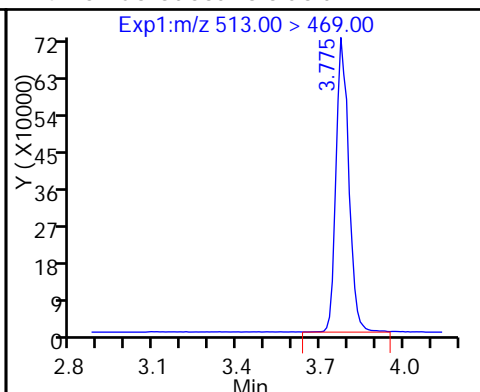


43 Sodium 1H,1H,2H,2H-perfluorooctane (ND)




D 23 13C2 PFDA

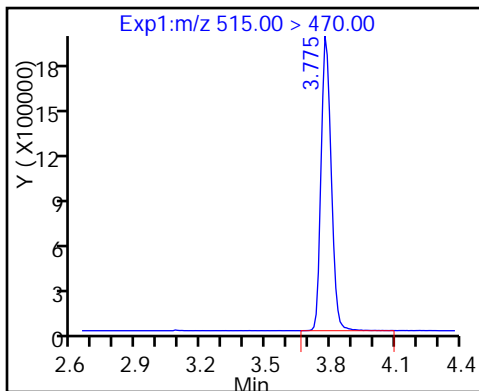


D 42 M2-8:2FTS

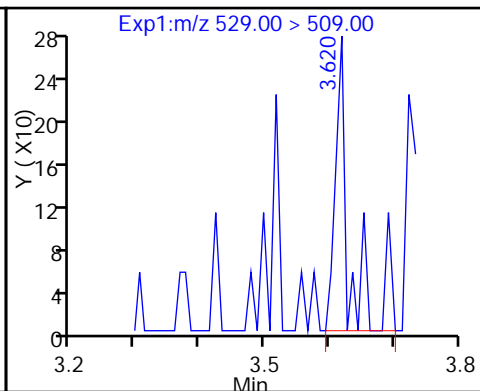


D 45 d3-NMeFOSAA

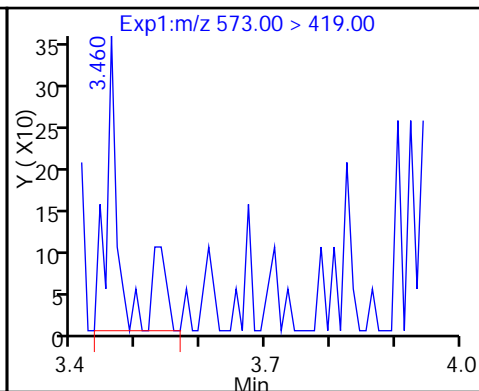


44 N-methyl perfluorooctane sulfonamide (ND)




26 Perfluorodecanoic Sulfonic acid

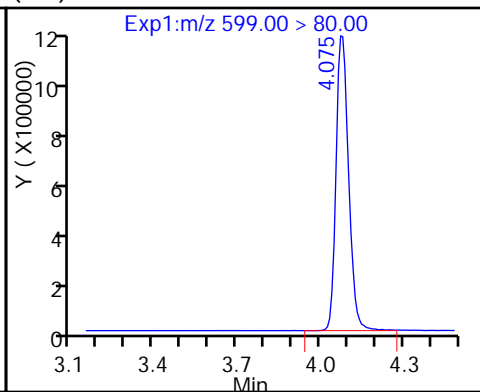


28 Perfluoroundecanoic acid




D 27 13C2 PFUnA

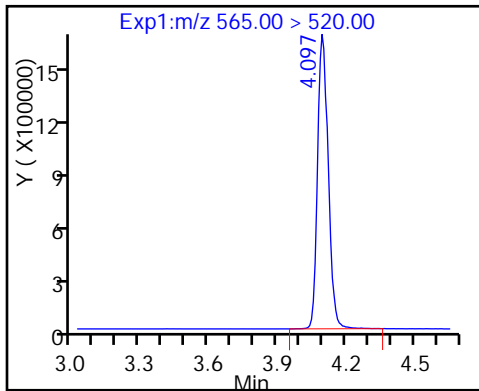

D 46 d5-NEtFOSAA

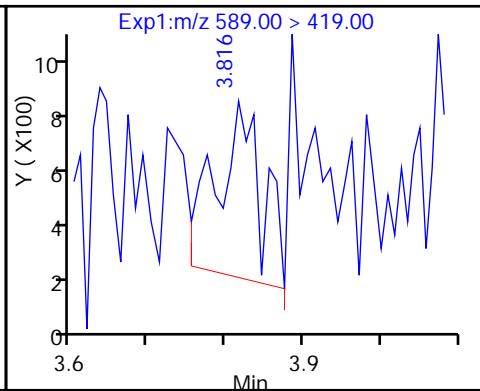




49 N-ethyl perfluorooctane sulfonamid (ND)

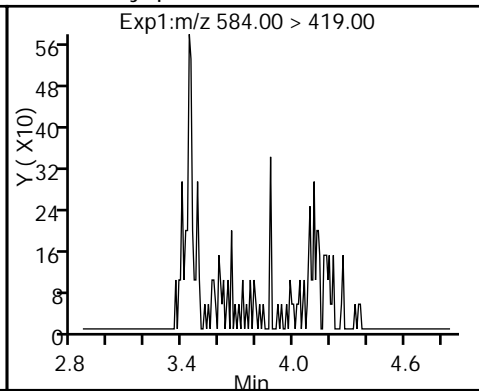

D 52 d-N-MeFOSA-M

54 MeFOSA (ND)




D 30 13C2 PFDaA



29 Perfluorododecanoic acid

D 51 d-N-EtFOSA-M




53 N-ethylperfluoro-1-octanesulfonami



31 Perfluorotridecanoic acid

D 32 13C2-PFTeDA




33 Perfluorotetradecanoic acid




33 Perfluorotetradecanoic acid

D 34 13C2-PFHxDA

35 Perfluorohexadecanoic acid



36 Perfluorooctadecanoic acid

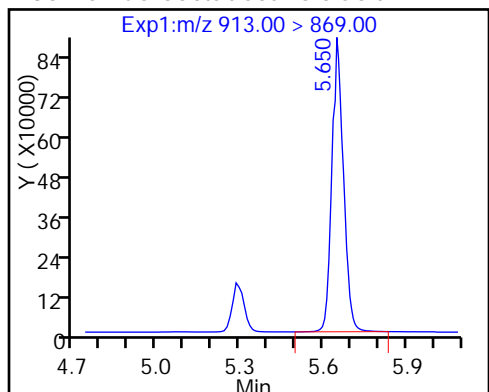

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1
 SDG No.: _____
 Client Sample ID: CS-1 MSD Lab Sample ID: 320-24118-6 MSD
 Matrix: Water Lab File ID: 16DEC2016BB_003.d
 Analysis Method: 537 (Modified) Date Collected: 12/06/2016 09:17
 Extraction Method: 3535 Date Extracted: 12/14/2016 18:18
 Sample wt/vol: 255.7 (mL) Date Analyzed: 12/16/2016 15:37
 Con. Extract Vol.: 0.5 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: Acquity ID: 2.1 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 142602 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
375-22-4	Perfluorobutanoic acid (PFBA)	41.1		2.4	0.98	0.45
2706-90-3	Perfluoropentanoic acid (PFPeA)	39.3		2.4	2.0	0.97
307-24-4	Perfluorohexanoic acid (PFHxA)	38.1		2.4	2.0	0.77
375-85-9	Perfluoroheptanoic acid (PFHpA)	38.2		2.4	2.0	0.78
335-67-1	Perfluorooctanoic acid (PFOA)	39.0		2.4	2.0	0.73
375-95-1	Perfluorononanoic acid (PFNA)	37.6		2.4	2.0	0.64
335-76-2	Perfluorodecanoic acid (PFDA)	36.4		2.4	0.98	0.43
2058-94-8	Perfluoroundecanoic acid (PFUnA)	38.3		2.4	2.0	0.73
307-55-1	Perfluorododecanoic acid (PFDoA)	38.8		2.4	2.0	0.57
72629-94-8	Perfluorotridecanoic Acid (PFTriA)	51.3		2.4	2.0	0.54
376-06-7	Perfluorotetradecanoic acid (PFTeA)	68.0	J	2.4	0.98	0.39
375-73-5	Perfluorobutanesulfonic acid (PFBS)	42.3		2.4	2.0	0.90
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	35.7		2.4	2.0	0.85
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	37.1		3.9	2.9	1.2
335-77-3	Perfluorodecanesulfonic acid (PFDS)	37.2		3.9	2.9	1.2
754-91-6	Perfluorooctane Sulfonamide (FOSA)	36.9		2.4	2.0	0.62

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: <u>TestAmerica Sacramento</u>	Job No.: <u>320-24118-1</u>
SDG No.: _____	
Client Sample ID: <u>CS-1 MSD</u>	Lab Sample ID: <u>320-24118-6 MSD</u>
Matrix: <u>Water</u>	Lab File ID: <u>16DEC2016BB_003.d</u>
Analysis Method: <u>537 (Modified)</u>	Date Collected: <u>12/06/2016 09:17</u>
Extraction Method: <u>3535</u>	Date Extracted: <u>12/14/2016 18:18</u>
Sample wt/vol: <u>255.7 (mL)</u>	Date Analyzed: <u>12/16/2016 15:37</u>
Con. Extract Vol.: <u>0.5 (mL)</u>	Dilution Factor: <u>1</u>
Injection Volume: <u>2 (uL)</u>	GC Column: <u>Acquity</u> ID: <u>2.1 (mm)</u>
% Moisture: _____	GPC Cleanup: (Y/N) <u>N</u>
Analysis Batch No.: <u>142602</u>	Units: <u>ng/L</u>

CAS NO.	ISOTOPE DILUTION	%REC	Q	LIMITS
STL01056	13C8 FOSA	4	Q	25-150
STL00992	13C4 PFBA	95		25-150
STL00993	13C2 PFHxA	101		25-150
STL00990	13C4 PFOA	97		25-150
STL00995	13C5 PFNA	76		25-150
STL00996	13C2 PFDA	83		25-150
STL00997	13C2 PFUnA	87		25-150
STL00998	13C2 PFDoA	99		25-150
STL00994	18O2 PFHxS	118		25-150
STL00991	13C4 PFOS	125		25-150
STL01892	13C4-PFHpA	105		25-150
STL01893	13C5 PFPeA	115		25-150

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161216-37940.b\16DEC2016BB_003.d
 Lims ID: 320-24118-B-6-C MSD
 Client ID: CS-1
 Sample Type: MSD
 Inject. Date: 16-Dec-2016 15:37:42 ALS Bottle#: 46 Worklist Smp#: 3
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-24118-b-6-c msd
 Misc. Info.: Plate: 1 Rack: 5
 Operator ID: A8-PC\A8 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20161216-37940.b\A8_N.m
 Limit Group: LC PFC_DOD ICAL
 Last Update: 16-Dec-2016 16:14:08 Calib Date: 15-Dec-2016 14:18:33
 Integrator: Picker
 Quant Method: Isotopic Dilution Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20161215-37881.b\15DEC2016B_018.d
 Column 1 : Det: EXP1
 Process Host: XAWRK007

First Level Reviewer: chandrasenas Date: 16-Dec-2016 16:12:23

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
D 2 13C4 PFBA	217.00 > 172.00	1.566	1.566	0.0	16497607	47.4		94.9	1698459	
1 Perfluorobutyric acid	212.90 > 169.00	1.566	1.574	-0.008	5917947	21.0		105	46659	
D 4 13C5-PFPeA	267.90 > 223.00	1.849	1.849	0.0	15343359	57.7		115	1139945	
3 Perfluoropentanoic acid	262.90 > 219.00	1.849	1.849	0.0	6090857	20.1		101	79565	
5 Perfluorobutanesulfonic acid	298.90 > 80.00	1.887	1.887	0.0	11821479	21.7		122		
	298.90 > 99.00	1.887	1.887	0.0	5047721		2.34(0.00-0.00)			
7 Perfluorohexanoic acid	313.00 > 269.00	2.141	2.143	-0.002	4491500	19.5		97.3	114973	
D 6 13C2 PFHxA	315.00 > 270.00	2.141	2.143	-0.002	12422368	50.7		101	788538	
12 Perfluoroheptanoic acid	363.00 > 319.00	2.479	2.483	-0.004	4532494	19.5		97.6	45589	
D 11 13C4-PFHpA	367.00 > 322.00	2.479	2.483	-0.004	11855838	52.4		105	868546	
D 10 18O2 PFHxS	403.00 > 84.00	2.494	2.490	0.004	18223229	55.7		118	928688	
9 Perfluorohexanesulfonic acid	399.00 > 80.00	2.494	2.498	-0.004	7246803	18.3		100		
D 47 M2-6:2FTS	429.00 > 409.00	2.826	2.821	0.005	2113	0.0181		0.0		
48 Sodium 1H,1H,2H,2H-perfluorooctane	427.00 > 407.00	2.826	2.821	0.005	15085	NR		0.0		
D 14 13C4 PFOA	417.00 > 372.00	2.842	2.837	0.005	11126088	48.3		96.6	479209	12/19/2016

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
15 Perfluorooctanoic acid										
413.00 > 369.00	2.842	2.845	-0.003	1.000	4448396	19.9		99.6	38077	
413.00 > 169.00	2.842	2.845	-0.003	1.000	2675271		1.66(0.90-1.10)		158164	
13 Perfluoroheptanesulfonic Acid										
449.00 > 80.00	2.842	2.845	-0.003	1.000	6804471	19.9		104		
18 Perfluorooctane sulfonic acid										
499.00 > 80.00	3.107	3.101	0.006	1.000	5868940	19.0		102	43319	
499.00 > 99.00	3.213	3.101	0.112	1.034	1286715		4.56(0.90-1.10)		127323	
20 Perfluorononanoic acid										
463.00 > 419.00	3.213	3.207	0.006	1.000	2464689	19.2		96.2	36448	
D 17 13C4 PFOS										
503.00 > 80.00	3.213	3.207	0.006		14848581	59.7		125	569591	
D 19 13C5 PFNA										
468.00 > 423.00	3.213	3.216	-0.003		6728239	37.9		75.7	700163	
D 21 13C8 FOSA										
506.00 > 78.00	3.545	3.539	0.006		826966	2.15		4.3	44700	
22 Perfluorooctane Sulfonamide										
498.00 > 78.00	3.553	3.547	0.006	1.000	291324	18.9		94.4	26026	
D 42 M2-8:2FTS										
529.00 > 509.00	3.562	3.570	-0.008		1134	0.0106		0.0		
43 Sodium 1H,1H,2H,2H-perfluorooctane										
527.00 > 507.00	3.537	3.570	-0.033	0.993	1319	NR		0.0		
24 Perfluorodecanoic acid										
513.00 > 469.00	3.570	3.573	-0.003	1.000	2291336	18.6		93.0	66978	
D 23 13C2 PFDA										
515.00 > 470.00	3.570	3.573	-0.003		6522870	41.5		82.9	206976	
D 45 d3-NMeFOSAA										
573.00 > 419.00	3.735	3.732	0.003		8357	0.1109		0.0		
44 N-methyl perfluorooctane sulfonami										
570.00 > 419.00	3.715	3.732	-0.017	0.995	1135	NR		0.0		
26 Perfluorodecane Sulfonic acid										
599.00 > 80.00	3.886	3.880	0.006	1.000	3446862	19.0		98.6		
28 Perfluoroundecanoic acid										
563.00 > 519.00	3.894	3.898	-0.004	1.000	1913491	19.6		98.0	59990	
D 27 13C2 PFUnA										
565.00 > 520.00	3.903	3.898	0.005		5106085	43.5		87.1	361563	
49 N-ethyl perfluorooctane sulfonamid										
584.00 > 419.00	3.912	3.899	0.013	1.007	2295	NR		0.0		
D 46 d5-NEtFOSAA										
589.00 > 419.00	3.886	3.899	-0.013		10686	0.1364		0.0		
D 52 d-N-MeFOSA-M										
515.00 > 169.00	4.028	4.051	-0.023		2311	0.0243		0.0		
29 Perfluorododecanoic acid										
613.00 > 569.00	4.184	4.179	0.005	1.000	1999373	19.8		99.1	45026	
D 30 13C2 PFDoA										
615.00 > 570.00	4.184	4.186	-0.002		5495278	49.5		99.1	166361	
D 51 d-N-EtFOSA-M										
531.00 > 169.00	4.211	4.232	-0.021		4063	0.0474		0.0		

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	%Rec	S/N	Flags
53 N-ethylperfluoro-1-octanesulfonami	526.00 > 169.00	4.428	4.241	0.187	1.000	485	NR	0.0		
31 Perfluorotridecanoic acid	663.00 > 619.00	4.457	4.455	0.002	1.000	2615687	26.2	131	52003	
D 32 13C2-PFTeDA	715.00 > 670.00	4.698	4.696	0.002		18160167	79.9	160	810013	
33 Perfluorotetradecanoic acid	712.50 > 668.90	4.698	4.696	0.002	1.000	6055744	34.8	174	10125	
	713.00 > 169.00	4.690	4.696	-0.006	0.998	948399	6.39(0.00-0.00)	88853		
D 34 13C2-PFHxDA	815.00 > 770.00	5.103	5.090	0.013		7054388	56.6	113	294904	
35 Perfluorohexadecanoic acid	813.00 > 769.00	5.103	5.101	0.002	1.000	2243148	20.8	104	4979	M
36 Perfluorooctadecanoic acid	913.00 > 869.00	5.462	5.451	0.011	1.000	2247446	19.8	99.2	3800	M

QC Flag Legend

Processing Flags

NR - Missing Quant Standard

Review Flags

M - Manually Integrated

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20161216-37940.b\16DEC2016BB_003.d

Injection Date: 16-Dec-2016 15:37:42 Instrument ID: A8_N

Lims ID: 320-24118-B-6-C MSD

Client ID: CS-1

Operator ID: A8-PC\A8

ALS Bottle#: 46 Worklist Smp#: 3

Injection Vol: 2.0 ul

Dil. Factor: 1.0000













Method: A8_N

Limit Group: LC PFC_DOD ICAL

D 2 13C4 PFBA

1 Perfluorobutyric acid


D 4 13C5-PFPeA

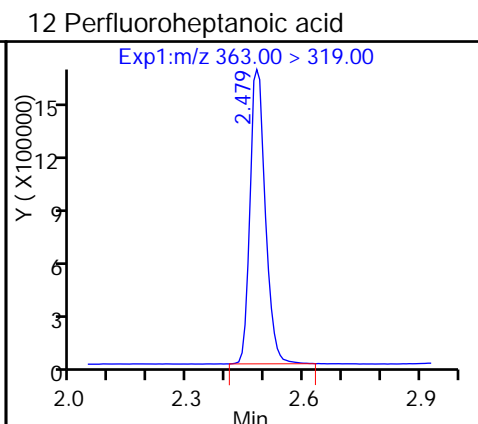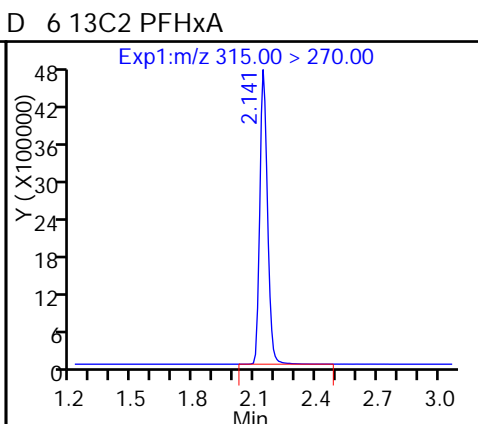

D 47 M2-6:2FTS

48 Sodium 1H,1H,2H,2H-perfluorooctanoate


D 14 13C4 PFOA

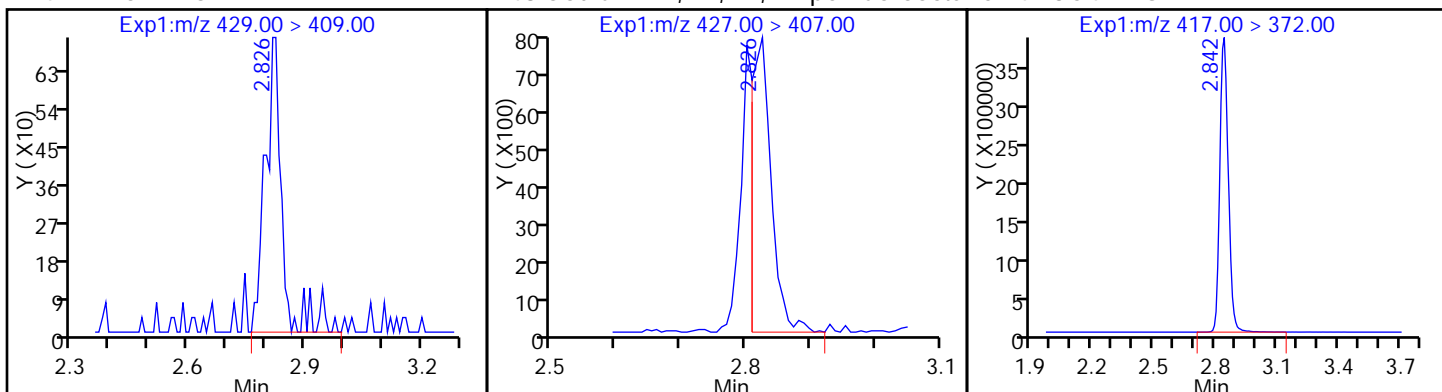

15 Perfluorooctanoic acid

15 Perfluorooctanoic acid


13 Perfluoroheptanesulfonic Acid

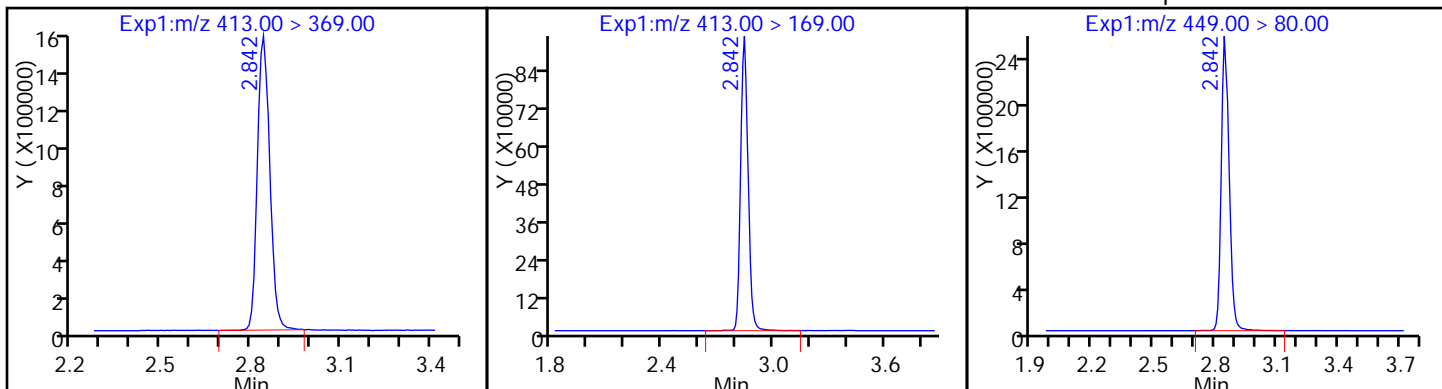

18 Perfluorooctane sulfonic acid

18 Perfluorooctane sulfonic acid


20 Perfluorononanoic acid

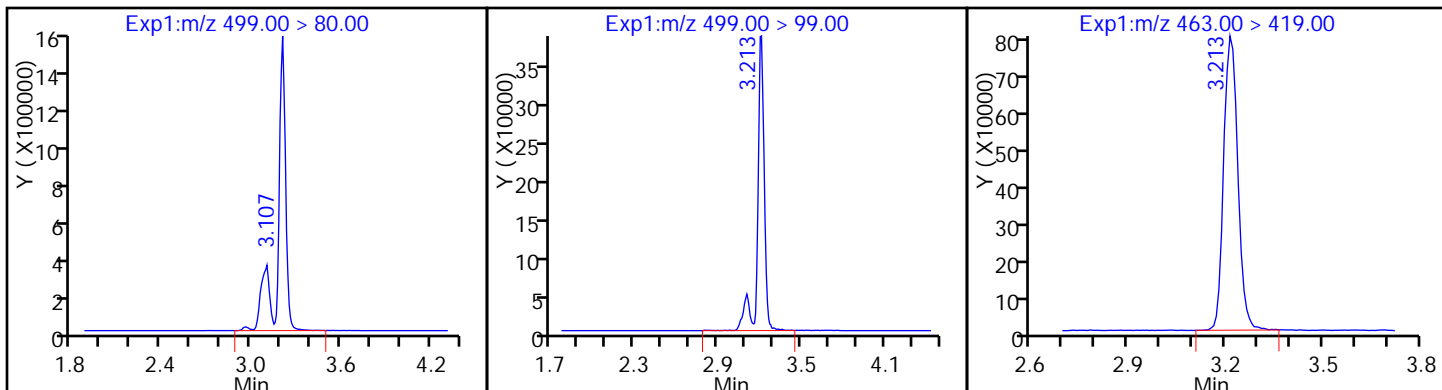

D 17 13C4 PFOS

D 19 13C5 PFNA




D 21 13C8 FOSA

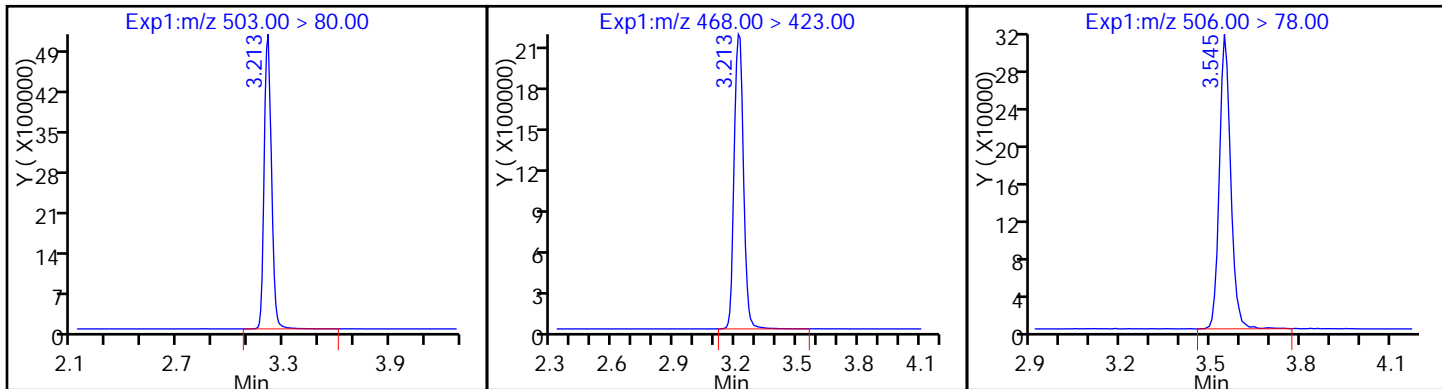

22 Perfluorooctane Sulfonamide

D 42 M2-8:2FTS




43 Sodium 1H,1H,2H,2H-perfluorooctane

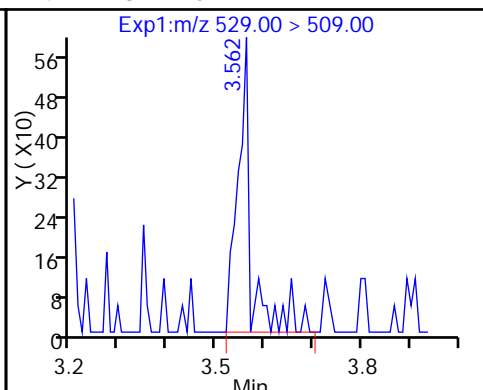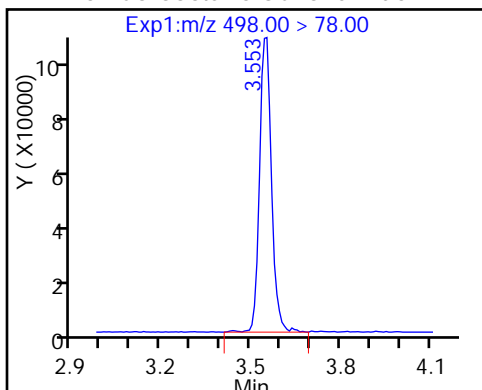

24 Perfluorodecanoic acid

D 23 13C2 PFDA




D 45 d3-NMeFOSAA

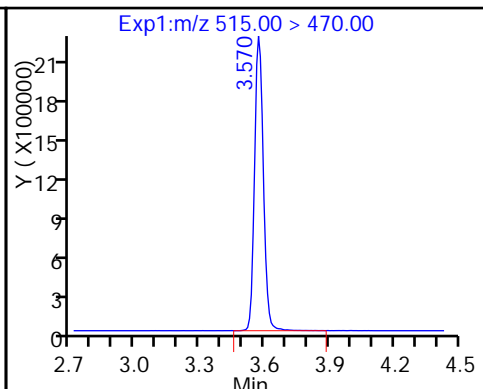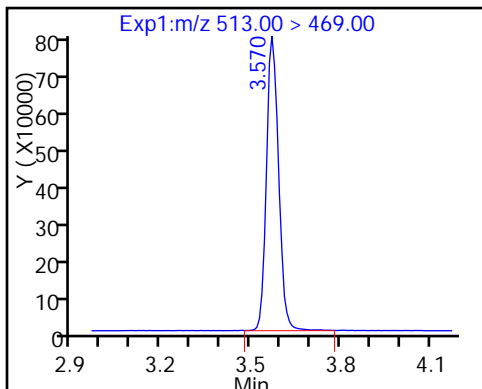

44 N-methyl perfluorooctane sulfonamid

26 Perfluorodecane Sulfonic acid




28 Perfluoroundecanoic acid

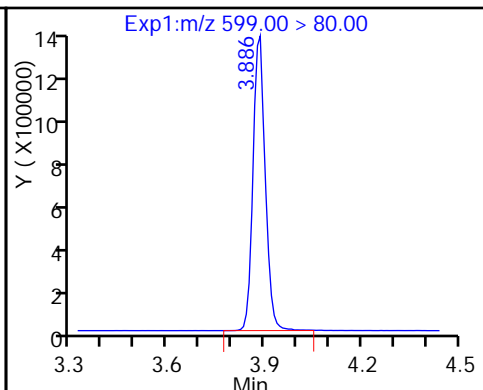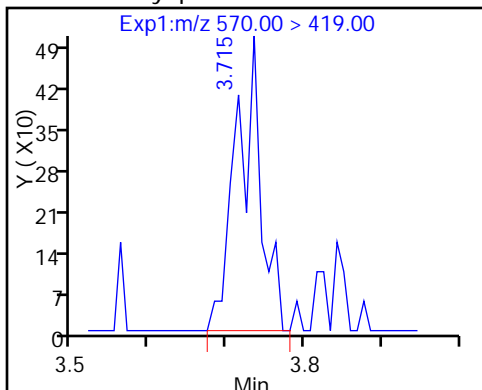


D 27 13C2 PFUnA


49 N-ethyl perfluorooctane sulfonamid

D 46 d5-NEtFOSAA

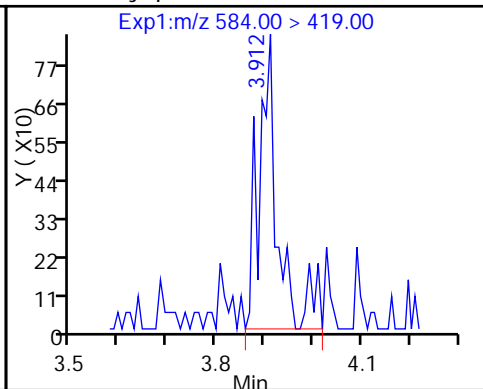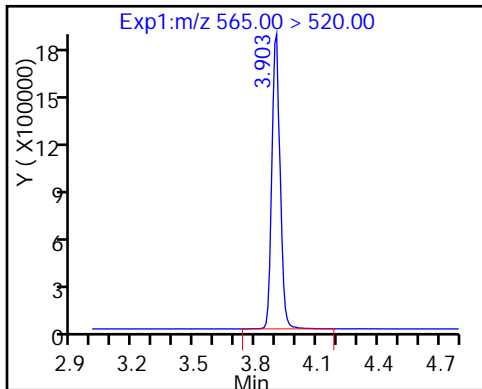

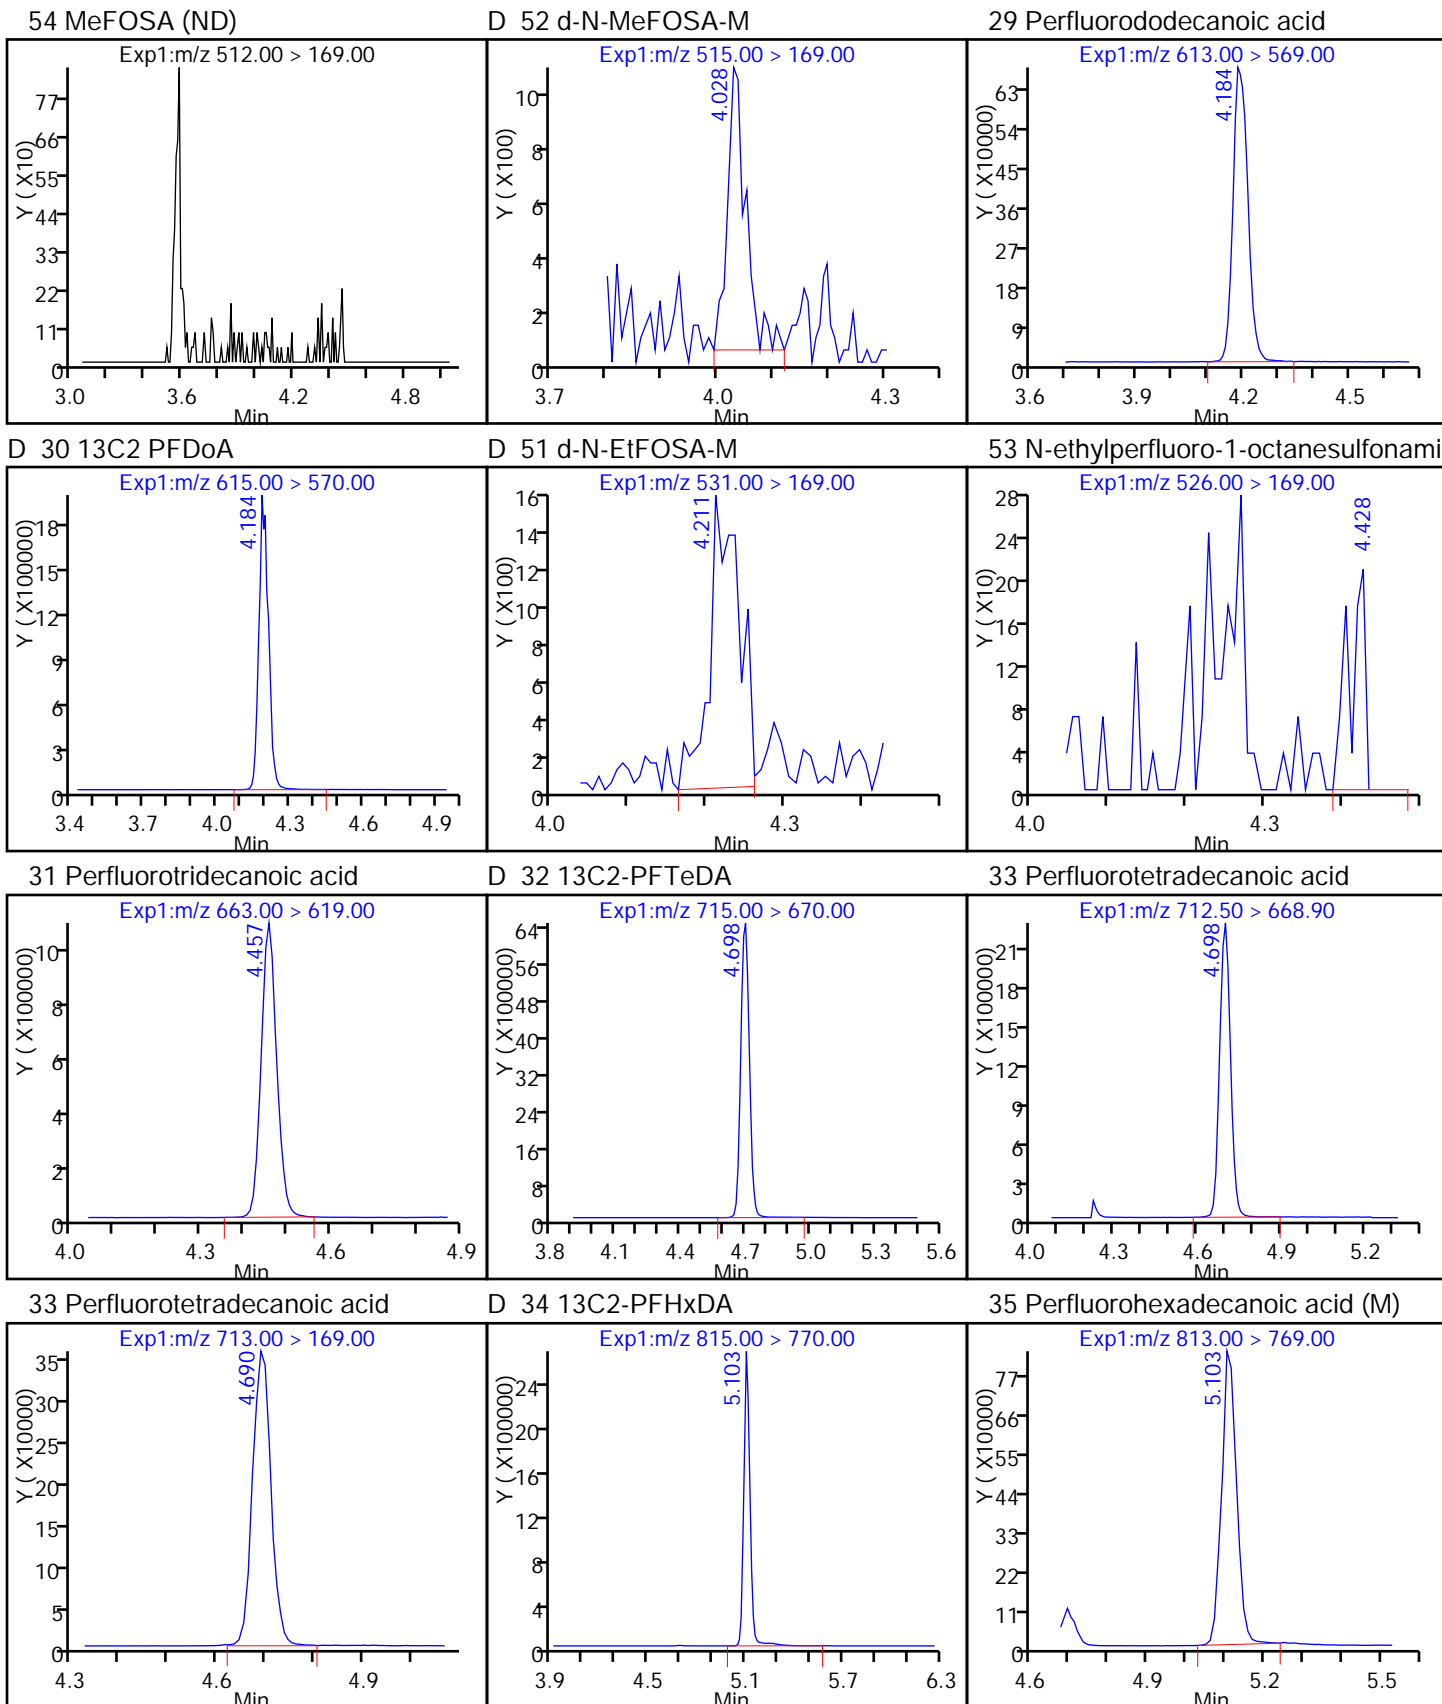

36 Perfluorooctadecanoic acid (M)

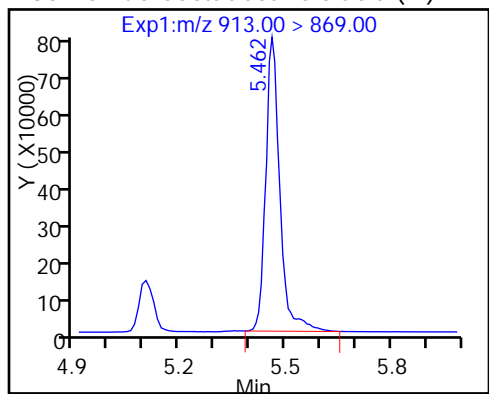

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1

SDG No.: _____

Instrument ID: A8_N Start Date: 12/15/2016 12:06

Analysis Batch Number: 142379 End Date: 12/15/2016 19:54

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
RB 320-142379/1 CCB		12/15/2016 12:06	1		Acquity 2.1(mm)
RB 320-142379/2 CCB		12/15/2016 12:14	1		Acquity 2.1(mm)
RB 320-142379/3 CCB		12/15/2016 12:21	1		Acquity 2.1(mm)
IC 320-142379/4		12/15/2016 12:29	1	15DEC2016B_004.d	Acquity 2.1(mm)
IC 320-142379/5		12/15/2016 12:36	1	15DEC2016B_005.d	Acquity 2.1(mm)
IC 320-142379/6		12/15/2016 12:44	1	15DEC2016B_006.d	Acquity 2.1(mm)
IC 320-142379/7		12/15/2016 12:51	1	15DEC2016B_007.d	Acquity 2.1(mm)
IC 320-142379/8		12/15/2016 12:59	1	15DEC2016B_008.d	Acquity 2.1(mm)
IC 320-142379/9		12/15/2016 13:06	1	15DEC2016B_009.d	Acquity 2.1(mm)
ICB 320-142379/10		12/15/2016 13:14	1		Acquity 2.1(mm)
ICV 320-142379/11		12/15/2016 13:21	1	15DEC2016B_011.d	Acquity 2.1(mm)
IC 320-142379/13		12/15/2016 13:41	1	15DEC2016BB_013.d	Acquity 2.1(mm)
IC 320-142379/14		12/15/2016 13:48	1	15DEC2016B_014.d	Acquity 2.1(mm)
IC 320-142379/15		12/15/2016 13:56	1	15DEC2016B_015.d	Acquity 2.1(mm)
IC 320-142379/16		12/15/2016 14:03	1	15DEC2016B_016.d	Acquity 2.1(mm)
IC 320-142379/17		12/15/2016 14:11	1	15DEC2016B_017.d	Acquity 2.1(mm)
IC 320-142379/18		12/15/2016 14:18	1	15DEC2016B_018.d	Acquity 2.1(mm)
ICB 320-142379/19		12/15/2016 14:26	1		Acquity 2.1(mm)
ICV 320-142379/20		12/15/2016 14:33	1		Acquity 2.1(mm)
RB 320-142379/21 CCB		12/15/2016 14:41	1		Acquity 2.1(mm)
CCV 320-142379/24		12/15/2016 15:46	1		Acquity 2.1(mm)
RB 320-142379/25 CCB		12/15/2016 15:54	1		Acquity 2.1(mm)
ZZZZZ		12/15/2016 16:01	1		Acquity 2.1(mm)
CCV 320-142379/27		12/15/2016 16:09	1	15DEC2016B_027.d	Acquity 2.1(mm)
RB 320-142379/28 CCB		12/15/2016 16:16	1		Acquity 2.1(mm)
MB 320-142235/1-A		12/15/2016 16:24	1	15DEC2016B_029.d	Acquity 2.1(mm)
LCS 320-142235/2-A		12/15/2016 16:31	1	15DEC2016B_030.d	Acquity 2.1(mm)
320-24118-1		12/15/2016 16:39	1	15DEC2016B_031.d	Acquity 2.1(mm)
320-24118-2		12/15/2016 16:46	1	15DEC2016B_032.d	Acquity 2.1(mm)
320-24118-3		12/15/2016 16:54	1	15DEC2016B_033.d	Acquity 2.1(mm)
320-24118-4		12/15/2016 17:01	1	15DEC2016B_034.d	Acquity 2.1(mm)
320-24118-5		12/15/2016 17:09	1	15DEC2016B_035.d	Acquity 2.1(mm)
320-24118-6		12/15/2016 17:16	1	15DEC2016B_036.d	Acquity 2.1(mm)
320-24118-6 MS		12/15/2016 17:24	1	15DEC2016B_037.d	Acquity 2.1(mm)
RB 320-142379/44 CCB		12/15/2016 19:47	1		Acquity 2.1(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1

SDG No.: _____

Instrument ID: A8_N Start Date: 12/15/2016 12:06

Analysis Batch Number: 142379 End Date: 12/15/2016 19:54

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-142379/42		12/15/2016 19:54	1	15DEC2016BB_039.d	Acquity 2.1(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1

SDG No.: _____

Instrument ID: A8_N Start Date: 12/16/2016 15:22

Analysis Batch Number: 142602 End Date: 12/16/2016 15:52

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-142602/1		12/16/2016 15:22	1	16DEC2016BB_001.d	Acquity 2.1(mm)
RB 320-142602/2 CCB		12/16/2016 15:30	1		Acquity 2.1(mm)
320-24118-6 MSD		12/16/2016 15:37	1	16DEC2016BB_003.d	Acquity 2.1(mm)
CCV 320-142602/4		12/16/2016 15:45	1	16DEC2016BB_004.d	Acquity 2.1(mm)
RB 320-142602/5 CCB		12/16/2016 15:52	1		Acquity 2.1(mm)

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1

SDG No.: _____

Batch Number: 142235 Batch Start Date: 12/14/16 18:18 Batch Analyst: Marchenko, Veronika P

Batch Method: 3535 Batch End Date: 12/15/16 10:10

Lab Sample ID	Client Sample ID	Method Chain	Basis	GrossWeight	TareWeight	InitialAmount	FinalAmount	LCMPFCSU 00047	LCPFCSP 00075
MB 320-142235/1		3535, 537 (Modified)				250 mL	0.5 mL	25 uL	
LCS 320-142235/2		3535, 537 (Modified)				250 mL	0.5 mL	25 uL	20 uL
320-24118-B-1	TB-1	3535, 537 (Modified)	T	270.14 g	26.51 g	243.6 mL	0.5 mL	25 uL	
320-24118-B-2	FB-1	3535, 537 (Modified)	T	288.15 g	26.63 g	261.5 mL	0.5 mL	25 uL	
320-24118-B-3	CS-10	3535, 537 (Modified)	T	285.57 g	25.85 g	259.7 mL	0.5 mL	25 uL	
320-24118-B-4	CS-41	3535, 537 (Modified)	T	273.01 g	26.43 g	246.6 mL	0.5 mL	25 uL	
320-24118-B-5	CS-12	3535, 537 (Modified)	T	288.32 g	26.75 g	261.6 mL	0.5 mL	25 uL	
320-24118-B-6	CS-1	3535, 537 (Modified)	T	276.88 g	26.73 g	250.2 mL	0.5 mL	25 uL	
320-24118-B-6 MS	CS-1	3535, 537 (Modified)	T	287.52 g	26.70 g	260.8 mL	0.5 mL	25 uL	20 uL
320-24118-B-6 MSD	CS-1	3535, 537 (Modified)	T	282.42 g	26.69 g	255.7 mL	0.5 mL	25 uL	20 uL

Batch Notes	
Balance ID	QA-070
H2O ID	12-14-16
Hexane ID	0000146278
Manifold ID	7
Methanol ID	807186
Pipette ID	BJ15128
Analyst ID - Reagent Drop	NSH
Analyst ID - SU Reagent Drop	NSH
Analyst ID - SU Reagent Drop Witness	JER
Solvent Lot #	800652
Solvent Name	3% NH4OH/MeOH
SOP Number	WS-LC-0025
SPE Cartridge Type	500 mg wax
Solid Phase Extraction Disk ID	002836112A

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-24118-1

SDG No.: _____

Batch Number: 142235 Batch Start Date: 12/14/16 18:18 Batch Analyst: Marchenko, Veronika P

Batch Method: 3535 Batch End Date: 12/15/16 10:10

Basis	Basis Description
T	Total/NA

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

HPLC/LCMS Data Review Checklist

Job Number(s): 24118

Work List ID(s): 37881; 37940

Extraction Batch: 142235

Analysis Batch(es): 142379; 142602; 141670

Delivery Rank: 2

Due Date: 12/13/16

A. Calibration/Instrument Run QC	1 st Level	2 nd Level	N/A
1. ICAL locked in Chrom and TALS? ICAL Batch# <u>142379</u>	✓	✓	
2. ICAL, CCV Frequency & Criteria met.	✓	✓	
• RF _{average} criteria appropriate for the method.	✓	✓	
• Linear Regression criteria appropriate if required ($r \geq 0.995$).	✓	✓	
• Quadratic fit criteria appropriate if required ($r^2 \geq 0.990$).			✓
• For Linear Regression and Quadratic fit – Does the y-intercept support ½ the reporting limit as described in CA-Q-S-005?	✓	✓	
• All curve points show calculated concentrations.	✓	✓	
3. Peaks correctly ID'd by data system.	✓	✓	
5. Tune check frequency & criteria met and Tune check report attached.	✓	✓	
B. QA/QC			
1. Are all QC samples properly linked in TALS?	✓	✓	
2. Method blank, LCS/LCSD and MS/SD frequencies met.	✓	✓	
3. LCS/LCSD and MB data are within control limits. If not, NCM is present.	✓	✓	
4. Are MS/MSD recoveries and RPD within control limits?	✓	✓	
5. Holding Times were met for prep and analytical.	✓	✓	
6. IS/Surrogate recoveries meet criteria or properly noted.	✓	✓	
C. Sample Analysis			
1. Was correct analysis performed and were project instructions followed?	✓	✓	
2. If required, are compounds within RT windows?	✓	✓	
3. If required, are positive hits confirmed and >40% RPD flagged?			✓
4. Manual Integrations reviewed and appropriate.	✓	✓	
5. All analytes correctly reported. (Primary, secondary, acceptable status)	✓	✓	
6. Correct reporting limits used. (based on client request, prep factors, and dilutions)	✓	✓	
D. Documentation			
1. Are all non-conformances documented/attached? NCM#	✓	✓	
2. Do results make sense (e.g. dilutions, etc.)?	✓	✓	
3. Have all flags been reviewed for appropriateness?	✓	✓	
4. For level 3 and 4 reports, have forms and raw data been reviewed?		✓	
5. Was QC Checker run for this job?	✓	✓	

*Upon completion of this checklist, the reviewer must scan and attach the checklist to the TALS job.

1st Level (Analyst): [Signature]

Date: 12/16/16

2nd Level Reviewer: [Signature]

Date: 12/19/2016

NCMS: 73213; 73211; 73212; 73210

TestAmerica Laboratories
Worklist QC Batch Report

Worklist Name: 15DEC2016B_PFC Worklist Number: 37881
 Instrument Name: A8_N Chrom Method: A8_N
 Data Directory: \\ChromNa\Sacramento\ChromData\A8_N\20161215-37881.b
 QC Batching: Disabled Limit Group Batching: Enabled

QC Batch: 1	LC PFC_DOD ICAL Raw Batch: 142379	LC PFC ICAL Raw Batch: 142380	LC PFAS ICAL Raw Batch: 142381
# 1 RB	# 1 RB		
# 2 RB	# 2 RB		
# 3 RB	# 3 RB		
# 4 IC L1	# 4 IC L1	# 4 IC L1	# 4 IC L1
# 5 IC L2	# 5 IC L2	# 5 IC L2	# 5 IC L2
# 6 IC L3	# 6 IC L3	# 6 IC L3	# 6 IC L3
# 7 IC L4	# 7 IC L4	# 7 IC L4	# 7 IC L4
# 8 IC L5	# 8 IC L5	# 8 IC L5	# 8 IC L5
# 9 IC L6	# 9 IC L6	# 9 IC L6	# 9 IC L6
#10 ICB	#10 ICB	#10 ICB	#10 ICB
#11 ICV	#11 ICV	#11 ICV	
#12 RB	#12 RB	#12 RB	#12 RB
#13 IC L1 Add-on	#13 IC L1 Add-on	#13 IC L1 Add-on	#13 IC L1 Add-on
#14 IC L2 Add-on	#14 IC L2 Add-on	#14 IC L2 Add-on	#14 IC L2 Add-on
#15 IC L3 Add-on	#15 IC L3 Add-on	#15 IC L3 Add-on	#15 IC L3 Add-on
#16 IC L4 Add-on	#16 IC L4 Add-on	#16 IC L4 Add-on	#16 IC L4 Add-on
#17 IC L5 Add-on	#17 IC L5 Add-on	#17 IC L5 Add-on	#17 IC L5 Add-on
#18 IC L6 Add-on	#18 IC L6 Add-on	#18 IC L6 Add-on	#18 IC L6 Add-on
#19 ICB	#19 ICB	#19 ICB	#19 ICB
#20 ICV Add-on	#20 ICV Add-on	#20 ICV Add-on	
#21 RB	#21 RB	#21 RB	#21 RB
#22 MB 320-142235/1-A	#22 MB 320-142235/1-A		
#23 RB	#23 RB	#23 RB	#23 RB
#24 CCV L5	#24 CCV L5	#24 CCV L5	#24 CCV L5
#25 RB	#25 RB	#25 RB	#25 RB
#26 LCSD 320-139585/3-A		#26 LCSD 320-139585/3-A	#26 LCSD 320-139585/3-A
#27 CCV L4	#27 CCV L4	#27 CCV L4	#27 CCV L4
#28 RB	#28 RB	#28 RB	#28 RB
#29 MB 320-142235/1-A	#29 MB 320-142235/1-A		
#30 LCS 320-142235/2-A	#30 LCS 320-142235/2-A		
#31 320-24118-B-1-A	#31 320-24118-B-1-A		
#32 320-24118-B-2-A	#32 320-24118-B-2-A		
#33 320-24118-B-3-A	#33 320-24118-B-3-A		
#34 320-24118-B-4-A	#34 320-24118-B-4-A		
#35 320-24118-B-5-A	#35 320-24118-B-5-A		
#36 320-24118-B-6-A	#36 320-24118-B-6-A		
#37 320-24118-B-6-B MS	#37 320-24118-B-6-B MS		
#44 RB	#44 RB	#44 RB	#44 RB
#42 CCV L5	#42 CCV L5	#42 CCV L5	#42 CCV L5
#45 RB	#45 RB	#45 RB	#45 RB
#43 CCV L5	#43 CCV L5	#43 CCV L5	#43 CCV L5
#46 RB	#46 RB	#46 RB	#46 RB
#38 320-24118-B-6-C MSD	#38 320-24118-B-6-C MSD		
#39 RB	#39 RB	#39 RB	#39 RB
#40 CCV L5	#40 CCV L5	#40 CCV L5	#40 CCV L5
#41 RB	#41 RB	#41 RB	#41 RB

*TUNE
NCM
73213*

*FOSA
IDA low 73211
IDA high 73212
MS/MSD PFTeDA I.R, LCS pass NCM
73210*

TestAmerica Laboratories
Worklist QC Batch Report

Worklist Name: 16DEC2016BB_PFC Worklist Number: 37940
 Instrument Name: A8_N Chrom Method: A8_N
 Data Directory: \\ChromNa\Sacramento\ChromData\A8_N\20161216-37940.b
 QC Batching: Disabled Limit Group Batching: Enabled

QC Batch: 1	LC PFC_DGD ICAL Raw Batch: 142602	LC PFC ICAL Raw Batch: 142603	LC PFAS ICAL Raw Batch: 142604
# 1 CCV L5	# 1 CCV L5	# 1 CCV L5	# 1 CCV L5
# 2 RB	# 2 RB	# 2 RB	# 2 RB
# 3 320-24118-B-6-C MSD	# 3 320-24118-B-6-C MSD 73210		
# 4 CCV L4	# 4 CCV L4	# 4 CCV L4	# 4 CCV L4
# 5 RB	# 5 RB	# 5 RB	# 5 RB

ICV 142379

CCV L2 142571

REWORK

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-142235

Analyst: Marchenko, Veronika P

Method Code: 320-3535_IVWT-320

AG 12/15/16

Batch Open: 12/14/2016 6:18:00PM

Batch End: 12/15/16 10:10

12/16/16

Solid-Phase Extraction (SPE)

Input Sample Lab ID (Analytical Method)	SDG (Job #)	GrossWt TareWt	InitAmt FinAmt	PHs		Due Date	Analytical TAT	Div Rank	Comments	Output Sample Lab ID
				Rcvd	Adj1 Adj2					
1 M/B-320-142235/1 N/A	N/A		250 mL 0.5 mL			N/A	N/A	N/A		M B 3 2 0 - 1 4 2 2 3 5 1 - A
2 LCS-320-142235/2 N/A	N/A		250 mL 0.5 mL			N/A	N/A	N/A		L C S 3 2 0 - 1 4 2 2 3 5 1 - A
3 320-24118-B-1 (PFC_IDA_DOD5)	N/A (320-24118-1)	270.14 g 26.51 g	243.6 mL 0.5 mL			12/13/16	4_Day_RUSH	2		3 2 0 - 2 4 1 1 8 - B - 1 - A
4 320-24118-B-2 (PFC_IDA_DOD5)	N/A (320-24118-1)	288.15 g 26.63 g	261.5 mL 0.5 mL			12/13/16	4_Day_RUSH	2		3 2 0 - 2 4 1 1 8 - B - 2 - A
5 320-24118-B-3 (PFC_IDA_DOD5)	N/A (320-24118-1)	285.57 g 25.85 g	259.7 mL 0.5 mL			12/13/16	4_Day_RUSH	2		3 2 0 - 2 4 1 1 8 - B - 3 - A
6 320-24118-B-4 (PFC_IDA_DOD5)	N/A (320-24118-1)	273.01 g 26.43 g	246.6 mL 0.5 mL			12/13/16	4_Day_RUSH	2		3 2 0 - 2 4 1 1 8 - B - 4 - A
7 320-24118-B-5 (PFC_IDA_DOD5)	N/A (320-24118-1)	288.32 g 26.75 g	261.6 mL 0.5 mL			12/13/16	4_Day_RUSH	2		3 2 0 - 2 4 1 1 8 - B - 5 - A
8 320-24118-B-6 (PFC_IDA_DOD5)	N/A (320-24118-1)	276.88 g 26.73 g	250.2 mL 0.5 mL			12/13/16	4_Day_RUSH	2		3 2 0 - 2 4 1 1 8 - B - 6 - A
9 320-24118-B-6-MS (PFC_IDA_DOD5)	N/A (320-24118-1)	287.52 g 26.70 g	260.8 mL 0.5 mL			12/13/16	4_Day_RUSH	2		3 2 0 - 2 4 1 1 8 - B - 6 - M S
10 320-24118-B-6-MSD (PFC_IDA_DOD5)	N/A (320-24118-1)	282.42 g 26.69 g	255.7 mL 0.5 mL			12/13/16	4_Day_RUSH	2		3 2 0 - 2 4 1 1 8 - B - 6 - C M S D

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-142235

Batch Open: 12/14/2016 6:18:00PM

Analyst: Marchenko, Veronika P

Method Code: 320-3535_IVWT-320

Batch End:

	Batch Notes
Manifold ID	7
Methanol ID	807186
Hexane ID	0000140278
Sodium Hypochlorite ID	NA
First Start time	NA
First End time	NA
Balance ID	QA-070
SPE Cartridge Type	500 mg wax
Solid Phase Extraction Disk ID	002836112A
H2O ID	12-14-16
Pipette ID	B515128
Solvent Name	3% NH4OH/MeOH
Solvent Lot #	800652
Analyst ID - Reagent Drop	NSH
Analyst ID - SU Reagent Drop	NSH
Analyst ID - SU Reagent Drop Witness	JER
Acid Name	NA
Acid ID	NA
Reagent ID	NA
Reagent Lot Number	NA
NaCl ID	NA

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-142235

Analyst: Marchenko, Veronika P

Batch Open: 12/14/2016 6:18:00PM

Method Code: 320-3535_IVWT-320

Batch End:

SOP Number WS-LC-0025

Batch Comment

Comments

320-24118-B-1	Method Comments: No AFFF at site Rework Comments: Surrogate was concentrated. Please re-extract with newest surrogate and spike.
320-24118-B-2	Method Comments: No AFFF at site Rework Comments: Surrogate was concentrated. Please re-extract with newest surrogate and spike.
320-24118-B-3	Method Comments: No AFFF at site Rework Comments: Surrogate was concentrated. Please re-extract with newest surrogate and spike.
320-24118-B-4	Method Comments: No AFFF at site Rework Comments: Surrogate was concentrated. Please re-extract with newest surrogate and spike.
320-24118-B-5	Method Comments: No AFFF at site Rework Comments: Surrogate was concentrated. Please re-extract with newest surrogate and spike.
320-24118-B-6	Method Comments: No AFFF at site Rework Comments: Surrogate was concentrated. Please re-extract with newest surrogate and spike.
320-24118-B-6~MS	Method Comments: No AFFF at site Rework Comments: Surrogate was concentrated. Please re-extract with newest surrogate and spike.
320-24118-B-6~MSD	Method Comments: No AFFF at site Rework Comments: Surrogate was concentrated. Please re-extract with newest surrogate and spike.

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-142235

Analyst: Marchenko, Veronika P

Batch Open: 12/14/2016 6:18:00PM

Method Code: 320-3535_IVWT-320

Batch End:

Reagent Additions Worksheet

Lab ID	Reagent Code	Amount Added	Final Amount	By	Witness
MB 320-142235/1	LCMPFCSU_00047	25 uL	0.5 mL	NSH 12-14-16	[Signature]
LCS 320-142235/2	LCMPFCSU_00047	25 uL	0.5 mL		
LCS 320-142235/2	LCPFCSP_00075	20 uL	0.5 mL		
320-24118-B-1	LCMPFCSU_00047	25 uL	0.5 mL		
320-24118-B-2	LCMPFCSU_00047	25 uL	0.5 mL		
320-24118-B-3	LCMPFCSU_00047	25 uL	0.5 mL		
320-24118-B-4	LCMPFCSU_00047	25 uL	0.5 mL		
320-24118-B-5	LCMPFCSU_00047	25 uL	0.5 mL		
320-24118-B-6	LCMPFCSU_00047	25 uL	0.5 mL		
320-24118-B-6 MS	LCMPFCSU_00047	25 uL	0.5 mL		
320-24118-B-6 MS	LCPFCSP_00075	20 uL	0.5 mL	[Signature]	
320-24118-B-6 MSD	LCMPFCSU_00047	25 uL	0.5 mL		
320-24118-B-6 MSD	LCPFCSP_00075	20 uL	0.5 mL		

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-142235

Analyst: Marchenko, Veronika P

Batch Open: 12/14/2016 6:18:00PM

Method Code: 320-3535_IVWT-320

Batch End:

Reagent	Other Reagents:	Amount/Units	Lot#:

Preparation Batch Number(s): 142235 Test: PFC(1)A.0005 Reworks

Earliest Holding Time: 12/13/14 (under the 3535-IVNT but under 3535-PFC not out of hold).

Sample List Tab		1 st Level Reviewer	2 nd Level Reviewer
Samples identified to the correct method		/	/
All necessary NCMs filed (including holding time)		NA	NA
Method/sample/login/QAS checked and correct		/	/
Worksheet Tab		1 st Level Reviewer	2 nd Level Reviewer
All samples properly preserved		NA	NA
Weights in anticipated range and not targeted		/	/
All additional test requirements performed, documented, and uploaded to TALS correctly (e.g. final amount, initial amount, turbidity, and CI Check)		/	/
The pH is transcribed correctly in TALS		NA	NA
All additional information transcribed into TALS is correct and raw data is attached		/	/
Comments are transcribed correctly in TALS		/	/
Reagents Tab		1 st Level Reviewer	2 nd Level Reviewer
All necessary reagents not expired and entered into TALS		/	/
All spike amounts correct and added to necessary samples and QC		/	/
Batch Information		1 st Level Reviewer	2 nd Level Reviewer
Date and time accurate and entered into TALS correctly		/	/
All necessary 'batch information' complete and entered into TALS correctly		/	/

1st Level Reviewer: VPM Date: 12/15/14
 2nd Level Reviewer: NSH Date: 12-15-16
 Comments: _____


Shipping and Receiving Documents

Chain of Custody Record

167027

West Sacramento, CA 95605
 Phone: 916.373.5600 Fax:

Regulatory Program: DW NPDES RCRA Other:

Client Contact		Project Manager: <u>Tammy Chang</u>		Date: <u>12/6/16</u>		COC No: <u>1</u> of <u>1</u> COCs	
Company Name: <u>Parsons LCS&A</u>		Tel/Fax: <u>512-719-6092</u>		Carrier: <u>Fed Ex</u>		Sampler: <u>SE + 80</u>	
Address: <u>8000 Centre Park Dr.</u>		Analysis Turnaround Time		For Lab Use Only:		Walk-in Client:	
City/State/Zip: <u>Austin, TX</u>		<input checked="" type="checkbox"/> CALENDAR DAYS <input type="checkbox"/> WORKING DAYS		Lab Sampling:		Job / SDG No.:	
Phone: <u>512-719-6000</u>		TAT if different from Below		Job / SDG No.:		Sample Specific Notes:	
Fax:		<input type="checkbox"/> 2 weeks		Job / SDG No.:			
Project Name: <u>Camp Stanley Storage Activity</u>		<input checked="" type="checkbox"/> 1 week		Job / SDG No.:			
Site: <u>PWS</u>		<input type="checkbox"/> 2 days		Job / SDG No.:			
PO # <u>110046 03000</u>		<input type="checkbox"/> 1 day		Job / SDG No.:			
Sample Identification	Sample Date	Sample Time	Sample Type (C=Comp, G=Grab)	Matrix	# of Cont.	Filtered Sample (Y/N)	Perform MS / MSD (Y/N)
T0-1	12/6/16	0800	NA	WQ	2	X	X
F0-1		0922	NA	WQ	2	X	X
C5-10		1046	G	WG	2	X	X
C5-41		0830	G	WG	2	X	X
C5-12		1000	G	WG	2	X	X
C5-1		0917	G	WG	6	X	X
 320-24118 Chain of Custody							
Preservation Used: 1 = Ice, 2 = HCl, 3 = H2SO4, 4 = HNO3, 5 = NaOH, 6 = Other							
Possible Hazard Identification: Please List any EPA Waste Codes for the sample in the Comments Section if the lab is to dispose of the sample.							
Special Instructions/QC Requirements & Comments:							
Custody Seal No.:		Cooler Temp. (°C):		Obs'd:		Therm ID No.:	
Company: <u>Parsons</u>		Company: <u>Thylo. Turpen</u>		Company: <u>AS</u>		Date/Time: <u>12/7/16 1030</u>	
Relinquished by: <u>B. D. Tit</u>		Received by: <u>Angela Jyn</u>		Company:		Date/Time:	
Relinquished by:		Received by:		Company:		Date/Time:	

Login Sample Receipt Checklist

Client: Parsons Corporation

Job Number: 320-24118-1

Login Number: 24118
List Number: 1
Creator: Edman, Connor M

List Source: TestAmerica Sacramento

Question	Answer	Comment
Radioactivity wasn't checked or is \leq background as measured by a survey meter.	True	
The cooler's custody seal, if present, is intact.	True	
Sample custody seals, if present, are intact.	N/A	
The cooler or samples do not appear to have been compromised or tampered with.	True	
Samples were received on ice.	True	
Cooler Temperature is acceptable.	True	
Cooler Temperature is recorded.	True	
COC is present.	True	
COC is filled out in ink and legible.	True	
COC is filled out with all pertinent information.	True	
Is the Field Sampler's name present on COC?	True	
There are no discrepancies between the containers received and the COC.	True	
Samples are received within Holding Time (excluding tests with immediate HTs)	True	
Sample containers have legible labels.	True	
Containers are not broken or leaking.	True	
Sample collection date/times are provided.	True	
Appropriate sample containers are used.	True	
Sample bottles are completely filled.	True	
Sample Preservation Verified.	N/A	
There is sufficient vol. for all requested analyses, incl. any requested MS/MSDs	True	
Containers requiring zero headspace have no headspace or bubble is $<6\text{mm}$ (1/4").	N/A	
Multiphasic samples are not present.	True	
Samples do not require splitting or compositing.	True	
Residual Chlorine Checked.	N/A	